

Data File : BN006405.D
Acq On : 19 Jun 2019 20:21
Operator : JU/SJ
Sample : K3224-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0C61

Quant Time: Jun 20 05:44:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 20 05:40:58 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	198209	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	947963	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.28	164	592593	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.04	188	1352519	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	1313955	20.00	ng/ul	0.00
85) Perylene-d12	23.48	264	1576089	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	9219	1.82	ng/uL	0.00
5) Phenol-d5	6.80	99	169821	8.05	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	463247	35.46	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	444083	28.54	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	301172	17.99	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	277758	36.59	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	313175	37.87	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	490680	30.88	ng/ul	0.00
29) 4-Chloroaniline-d4	10.58	131	4975	0.27	ng/ul	0.03
43) Dimethylphthalate-d6	13.70	166	2046923	39.41	ng/ul	0.00
46) Acenaphthylene-d8	13.97	160	2328688	36.58	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	49200	5.54	ng/ul	0.00
57) Fluorene-d10	15.28	176	1731808	39.20	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	286893	33.52	ng/ul	0.00
70) Anthracene-d10	17.14	188	2769573	40.67	ng/ul	0.00
78) Pyrene-d10	19.45	212	3090140	40.26	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.34	264	3647431	40.97	ng/ul	0.00


Target Compounds					Qvalue
45) 2,6-Dinitrotoluene	13.70	165	14238	1.526	ng/ul# 37


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN006405.D
Acq On : 19 Jun 2019 20:21
Operator : JU/SJ
Sample : K3224-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0C61

Quant Time: Jun 20 05:44:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 20 05:40:58 2019
Response via : Initial Calibration

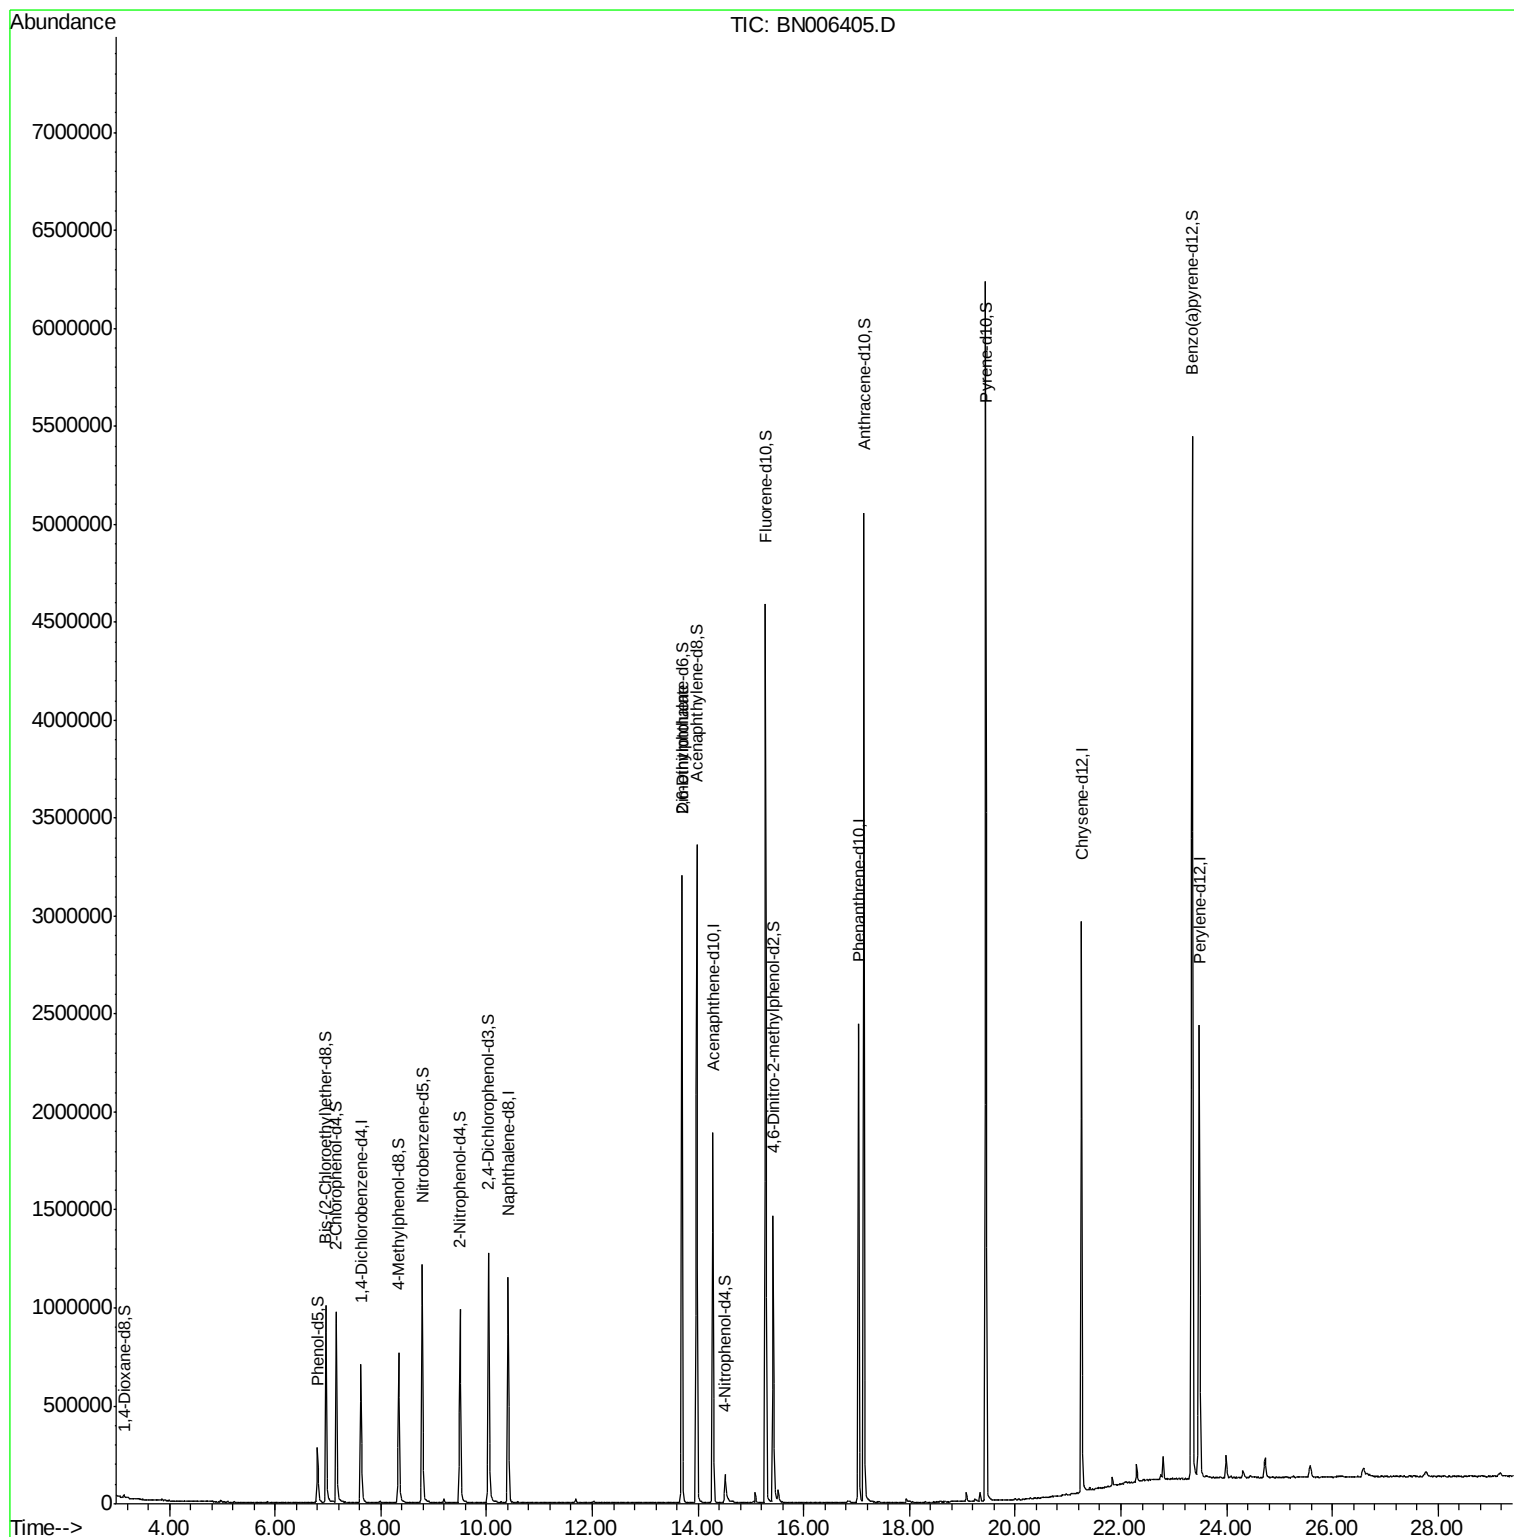

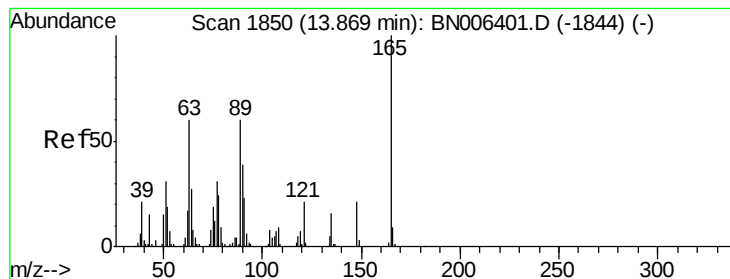

#45

2,6-Dinitrotoluene

Concen: 1.526 ng/ul

RT: 13.70 min Scan# 1821

Delta R.T. -0.17 min

Lab File: BN006405.D


Acq: 19 Jun 2019 20:21

Instrument :

BNA_N

ClientSampleId :

C0C61

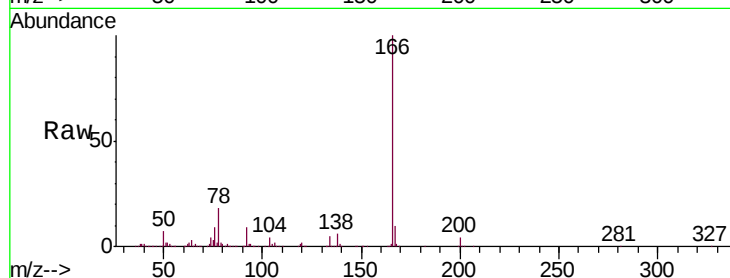

Tgt Ion:	165	Resp:	14238
Ion	Ratio	Lower	Upper
165	100		
89	0.0	48.6	72.8#
121	28.9	17.2	25.8#

