

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061919\
 Data File : BN006411.D
 Acq On : 19 Jun 2019 23:49
 Operator : JU/SJ
 Sample : K3335-10
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4237

Quant Time: Jun 20 05:44:43 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 20 05:40:58 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	235839	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	1090322	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.28	164	656655	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.03	188	1472657	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	1499458	20.00	ng/ul	0.00
85) Perylene-d12	23.48	264	1723641	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	21794	3.61	ng/uL	0.00
5) Phenol-d5	6.80	99	368892	14.69	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	277693	17.86	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	304903	16.47	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	192249	9.65	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	155619	17.82	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	159847	16.80	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	274457	15.02	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	264117	12.57	ng/ul	0.00
43) Dimethylphthalate-d6	13.69	166	1136793	19.75	ng/ul	0.00
46) Acenaphthylene-d8	13.97	160	1343800	19.05	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	65449	6.66	ng/ul	0.00
57) Fluorene-d10	15.28	176	993763	20.30	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	61511	6.60	ng/ul	0.00
70) Anthracene-d10	17.13	188	1402312	18.91	ng/ul	0.00
78) Pyrene-d10	19.45	212	1756103	20.05	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.34	264	1859197	19.10	ng/ul	0.00


Target Compounds					Ovalue
44) Dimethylphthalate	13.74	163	396725	7.477	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061919\
Data File : BN006411.D
Acq On : 19 Jun 2019 23:49
Operator : JU/SJ
Sample : K3335-10
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A4237

Quant Time: Jun 20 05:44:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 20 05:40:58 2019
Response via : Initial Calibration

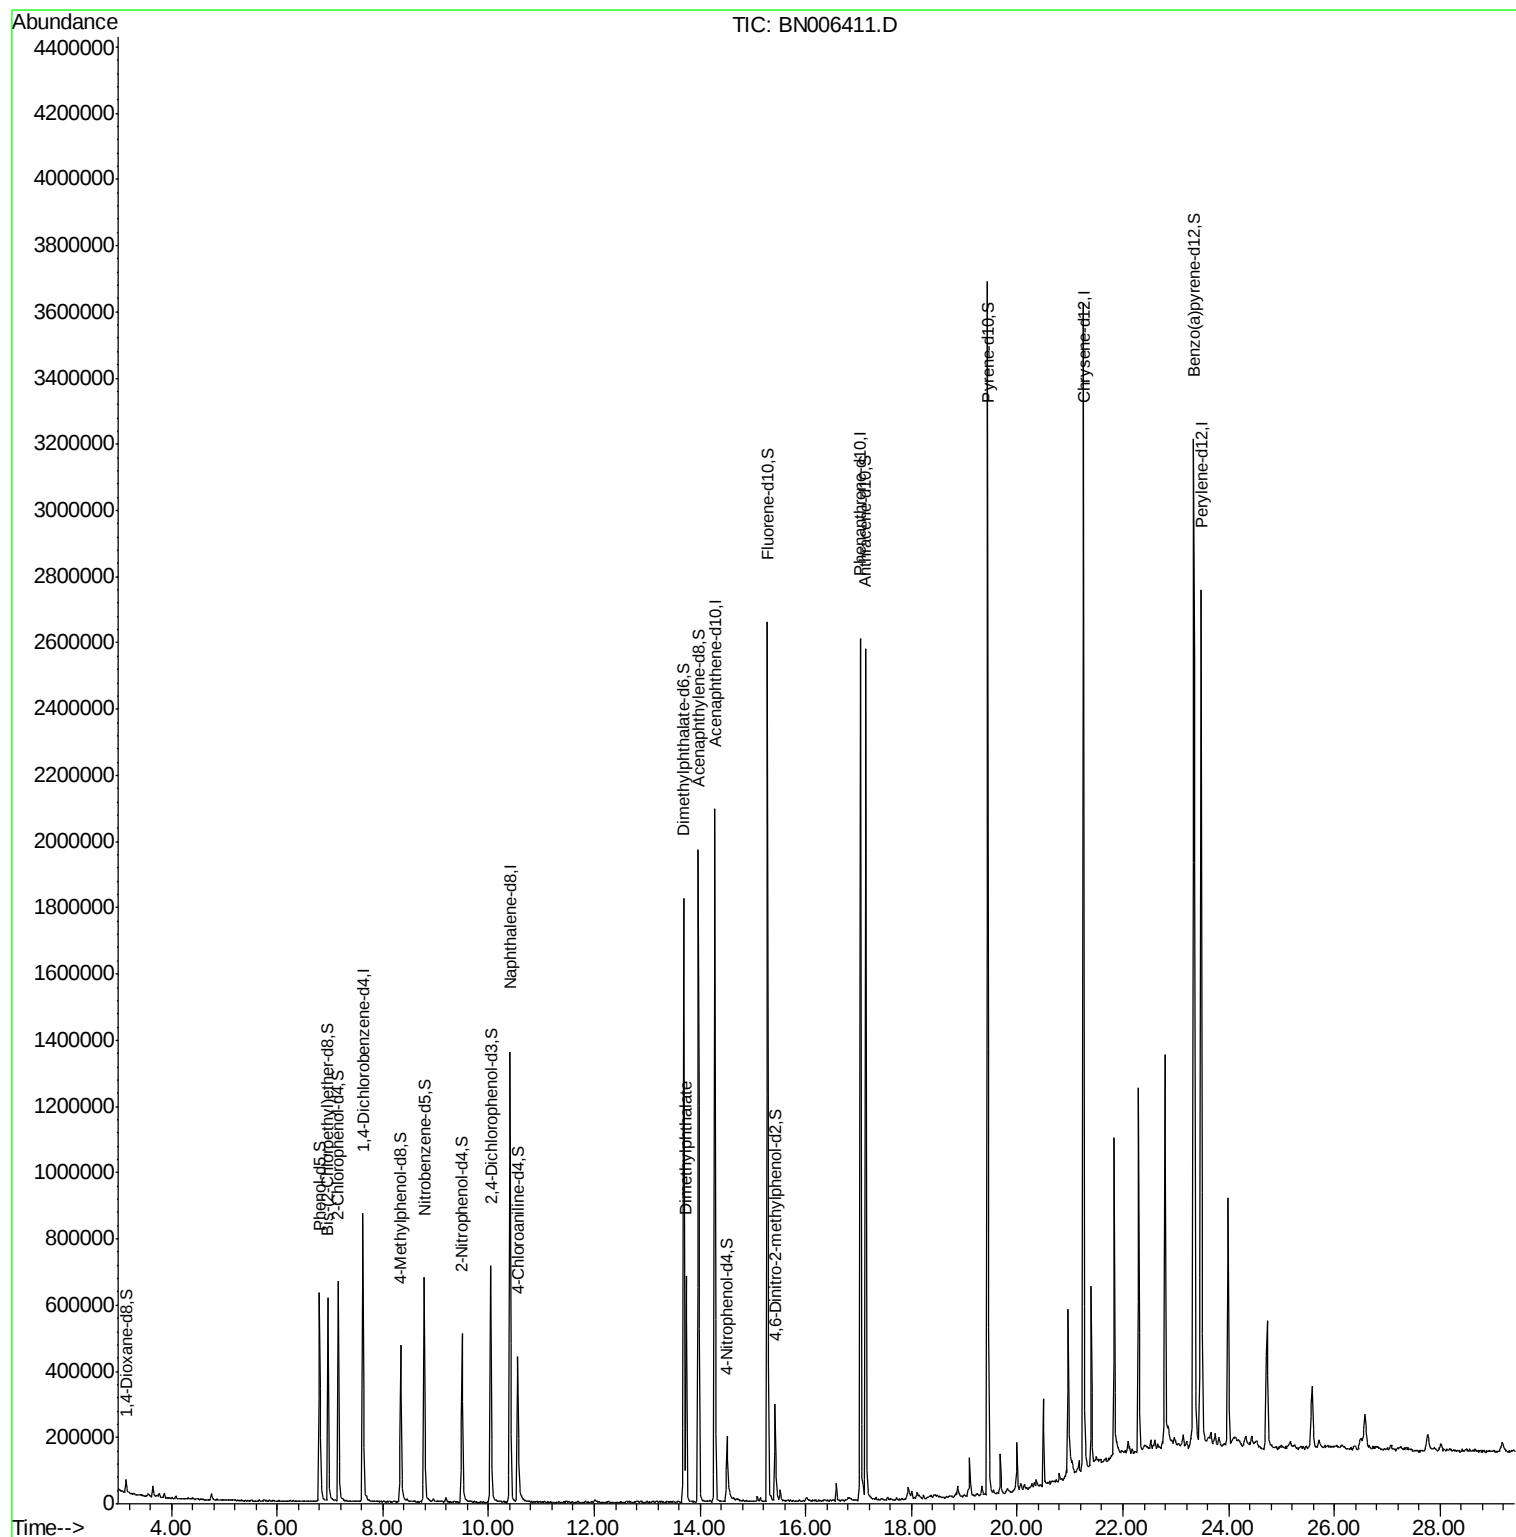

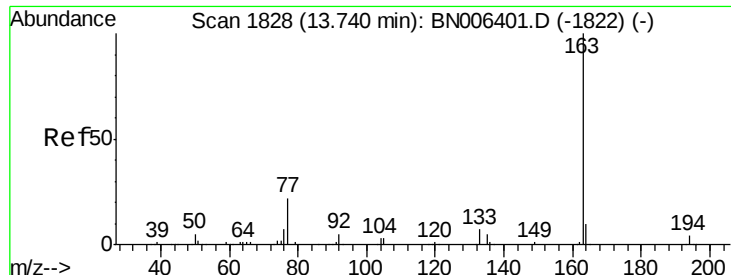

#44

Dimethylphthalate

Concen: 7.477 ng/ul

RT: 13.74 min Scan# 1828

Delta R.T. -0.00 min

Lab File: BN006411.D

Acq: 19 Jun 2019 23:49

Instrument :

BNA_N

ClientSampleId :

A4237


Tot Ion:163 Resp: 396725

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.0

164 10.1 8.0 12.0

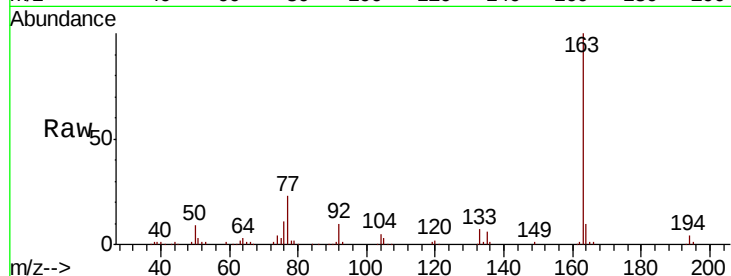

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

