

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061919\
 Data File : BN006417.D
 Acq On : 20 Jun 2019 04:25
 Operator : JU/SJ
 Sample : K3335-18
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4205

Quant Time: Jun 20 05:45:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 20 05:40:58 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	237869	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	1125355	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.28	164	704364	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.04	188	1632956	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	1646688	20.00	ng/ul	0.00
85) Perylene-d12	23.49	264	1937145	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.14	96	34257	5.63	ng/uL	0.00
5) Phenol-d5	6.80	99	638896	25.23	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	455453	29.05	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	503681	26.97	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	522195	25.99	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	261563	29.03	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	292985	29.84	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	488843	25.92	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	716425	33.03	ng/ul	0.00
43) Dimethylphthalate-d6	13.70	166	1951963	31.62	ng/ul	0.00
46) Acenaphthylene-d8	13.97	160	2196700	29.03	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	237844	22.55	ng/ul	0.00
57) Fluorene-d10	15.28	176	1621538	30.88	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	241309	23.35	ng/ul	0.00
70) Anthracene-d10	17.14	188	2515540	30.60	ng/ul	0.00
78) Pyrene-d10	19.45	212	2771903	28.82	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.35	264	3148689	28.78	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.74	163	642355	11.287	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061919\
Data File : BN006417.D
Acq On : 20 Jun 2019 04:25
Operator : JU/SJ
Sample : K3335-18
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4205

Quant Time: Jun 20 05:45:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 20 05:40:58 2019
Response via : Initial Calibration

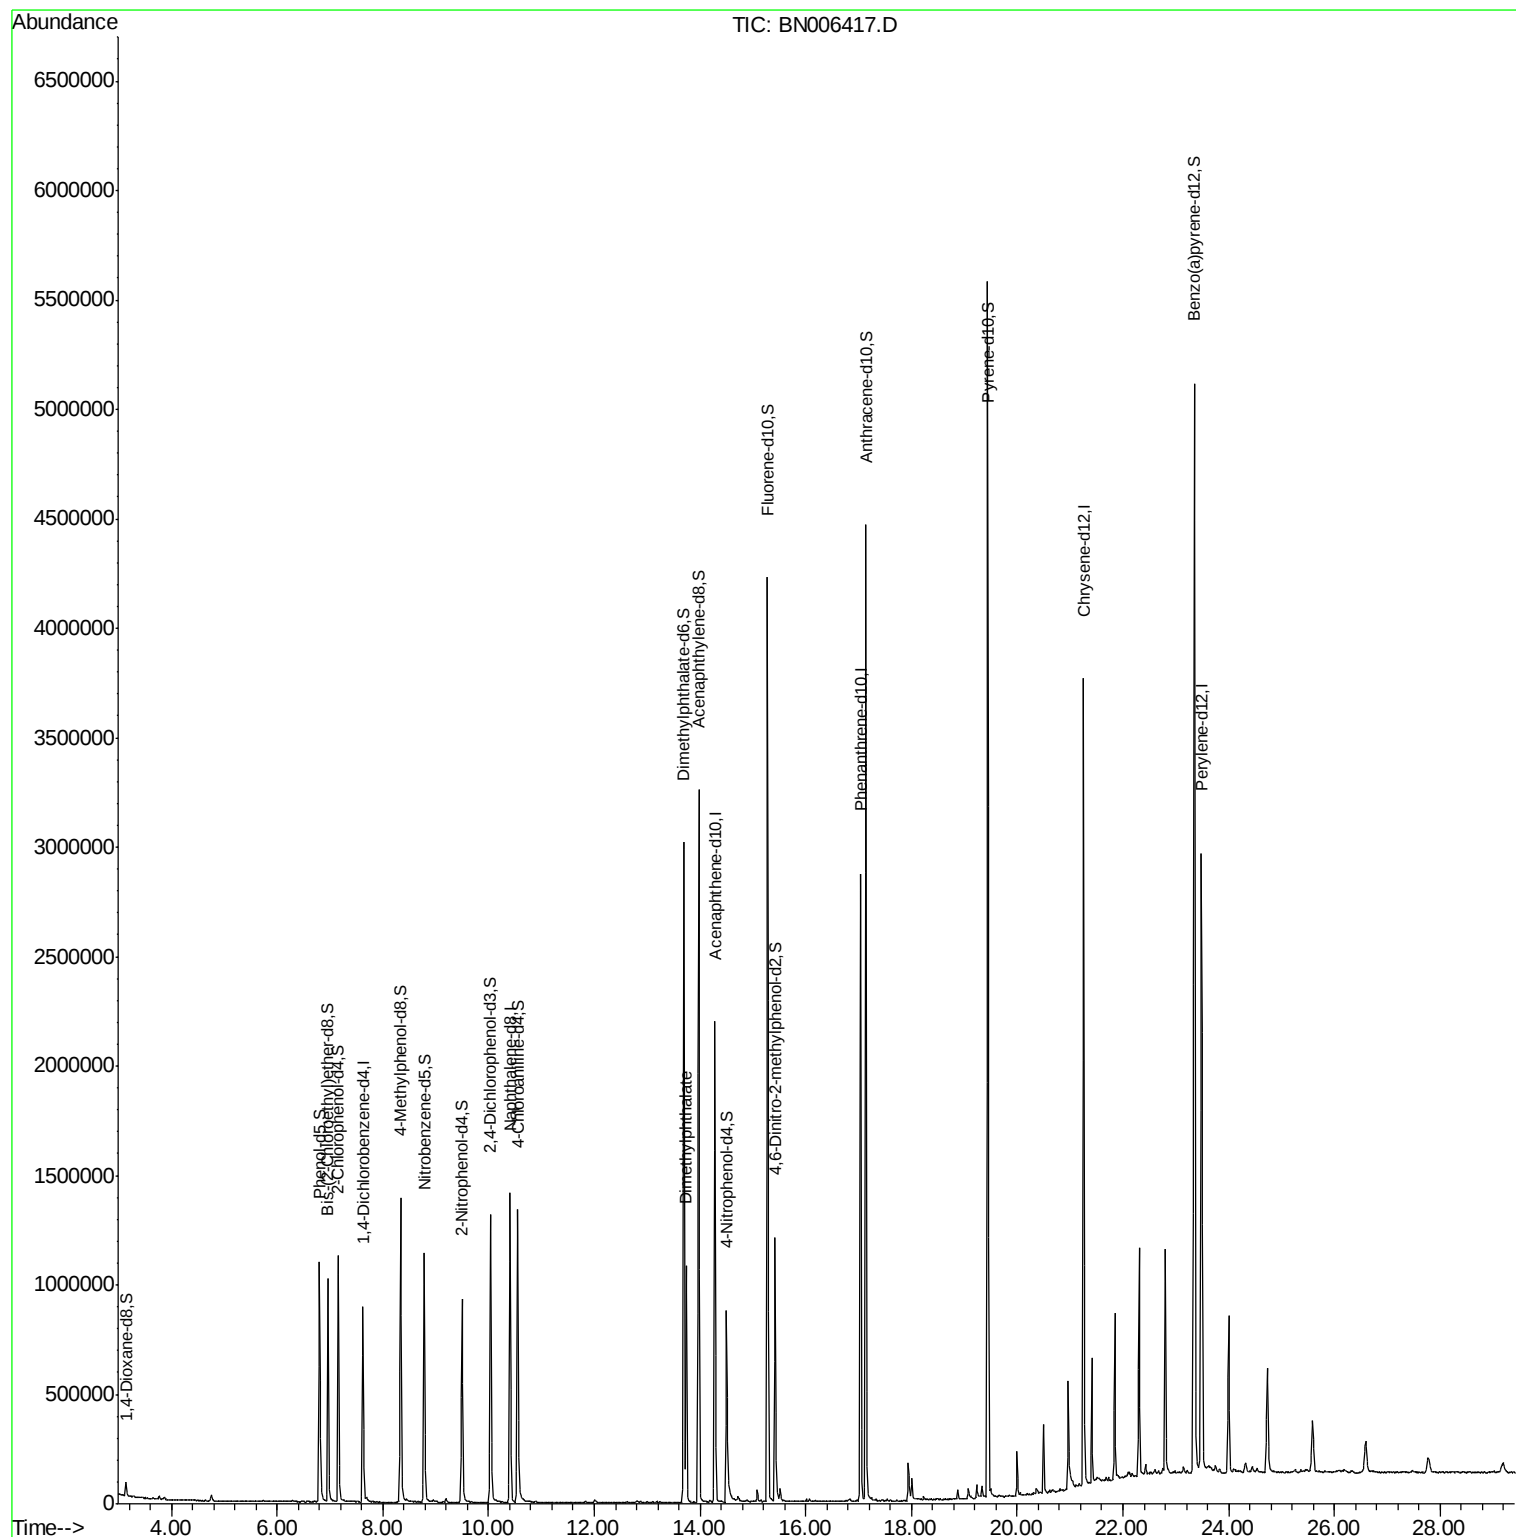

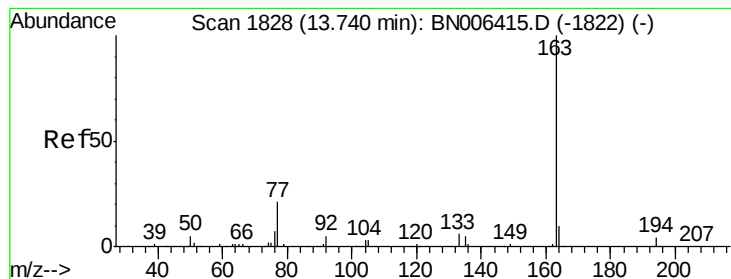

#44

Dimethylphthalate

Concen: 11.287 ng/ul

RT: 13.74 min Scan# 1828

Delta R.T. 0.00 min

Lab File: BN006417.D

Acq: 20 Jun 2019 04:25

Instrument :

BNA_N

ClientSampleId :

A4205


Tot Ion:163 Resp: 642355

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.0

164 10.1 8.0 12.0

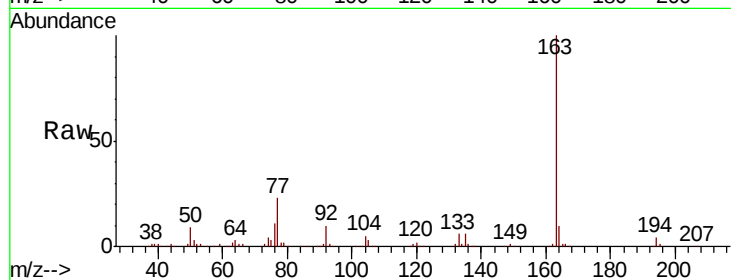

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

