

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061919\
 Data File : BN006418.D
 Acq On : 20 Jun 2019 04:59
 Operator : JU/SJ
 Sample : K3335-21
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A41X1

Quant Time: Jun 20 05:45:47 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 20 05:40:58 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	245190	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	1146283	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.28	164	721478	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.04	188	1629263	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	1645994	20.00	ng/ul	0.00
85) Perylene-d12	23.48	264	1866707	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	18097	2.88	ng/uL	0.00
5) Phenol-d5	6.80	99	338060	12.95	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	258023	15.97	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	269502	14.00	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	263946	12.75	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	141431	15.41	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	155129	15.51	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	260740	13.57	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	358107	16.21	ng/ul	0.00
43) Dimethylphthalate-d6	13.69	166	1107770	17.52	ng/ul	0.00
46) Acenaphthylene-d8	13.97	160	1201055	15.50	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	119717	11.08	ng/ul	0.00
57) Fluorene-d10	15.28	176	905700	16.84	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	115548	11.21	ng/ul	0.00
70) Anthracene-d10	17.13	188	1354851	16.52	ng/ul	0.00
78) Pyrene-d10	19.45	212	1557620	16.20	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.34	264	1711396	16.23	ng/ul	0.00

Target Compounds


				Ovalue	
44) Dimethylphthalate	13.74	163	935532	16.049	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061919\
Data File : BN006418.D
Acq On : 20 Jun 2019 04:59
Operator : JU/SJ
Sample : K3335-21
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41X1

Quant Time: Jun 20 05:45:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 20 05:40:58 2019
Response via : Initial Calibration

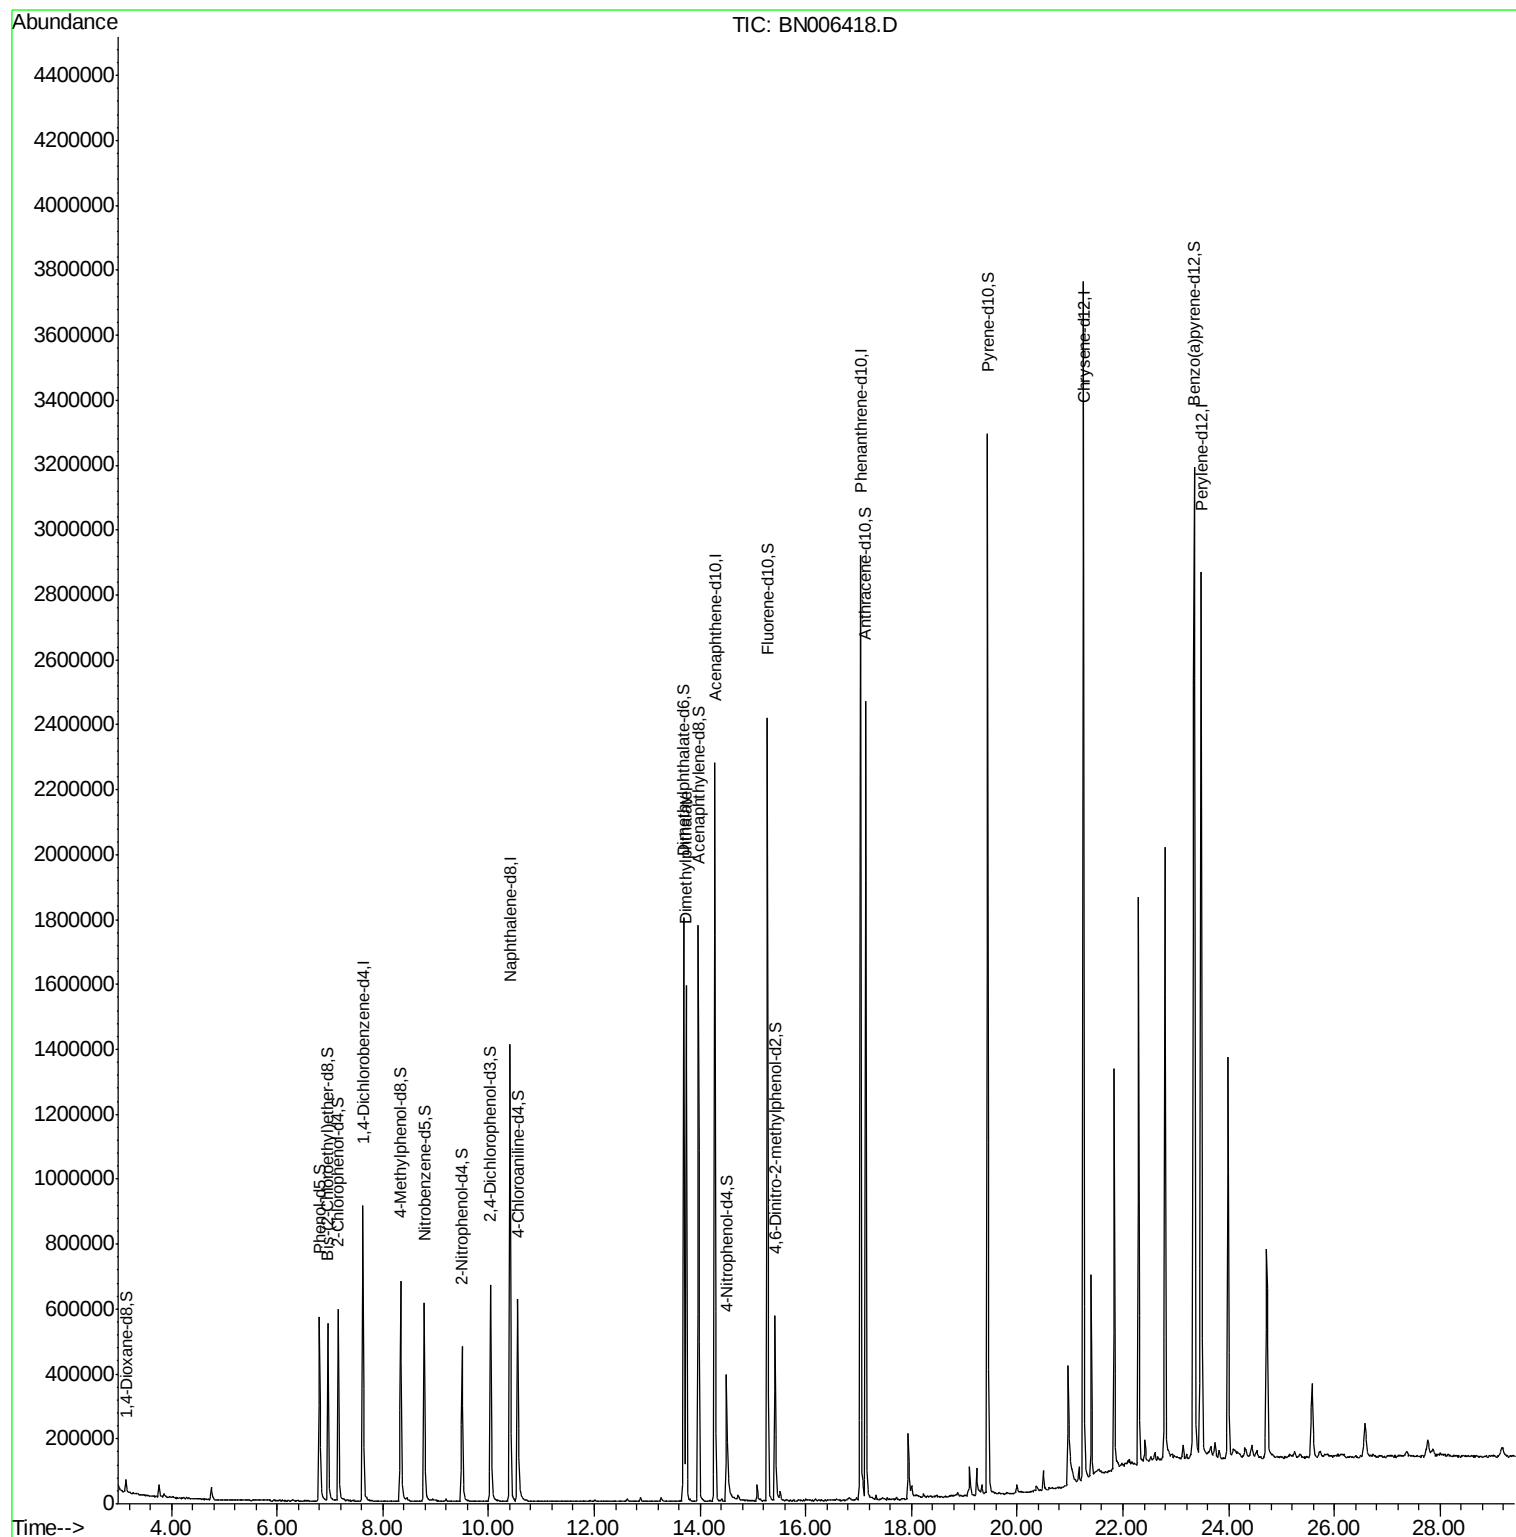

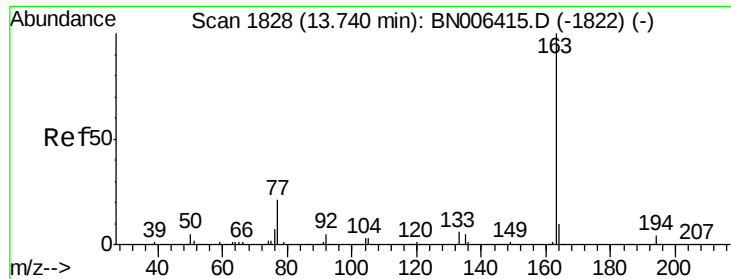

#44

Dimethylphthalate

Concen: 16.049 ng/ul

RT: 13.74 min Scan# 1828

Delta R.T. -0.00 min

Lab File: BN006418.D

Acq: 20 Jun 2019 04:59

Instrument :

BNA_N

ClientSampleId :

A41X1


Tot Ion:163 Resp: 935532

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.0

164 10.2 8.0 12.0

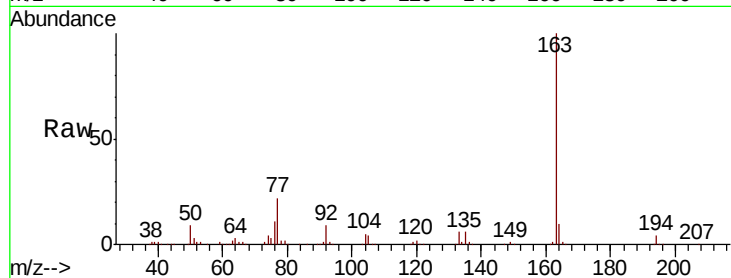

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

