

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061919\
 Data File : BN006422.D
 Acq On : 20 Jun 2019 07:17
 Operator : JU/SJ
 Sample : K3335-24
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4240

Quant Time: Jun 20 07:56:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 20 07:11:27 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	238429	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	1141563	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.28	164	724104	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.04	188	1649178	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	1630830	20.00	ng/ul	0.00
85) Perylene-d12	23.49	264	1955275	20.00	ng/ul	0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	10540	1.73	ng/uL	0.00
5) Phenol-d5	6.80	99	181637	7.16	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	483761	30.78	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	468476	25.03	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	332408	16.51	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	295863	32.37	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	326501	32.78	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	547744	28.63	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	2000	0.09	ng/ul	0.02
43) Dimethylphthalate-d6	13.69	166	2191058	34.52	ng/ul	0.00
46) Acenaphthylene-d8	13.97	160	2578541	33.15	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	61178	5.64	ng/ul	0.00
57) Fluorene-d10	15.28	176	1867770	34.60	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	318919	30.56	ng/ul	0.00
70) Anthracene-d10	17.14	188	2977773	35.86	ng/ul	0.00
78) Pyrene-d10	19.45	212	3310012	34.75	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.36	264	3843347	34.80	ng/ul	0.02

Target Compounds


				Ovalue	
33) 4-Chloro-3-methylphenol	11.72	107	57026	2.711	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061919\
Data File : BN006422.D
Acq On : 20 Jun 2019 07:17
Operator : JU/SJ
Sample : K3335-24
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4240

Quant Time: Jun 20 07:56:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 20 07:11:27 2019
Response via : Initial Calibration

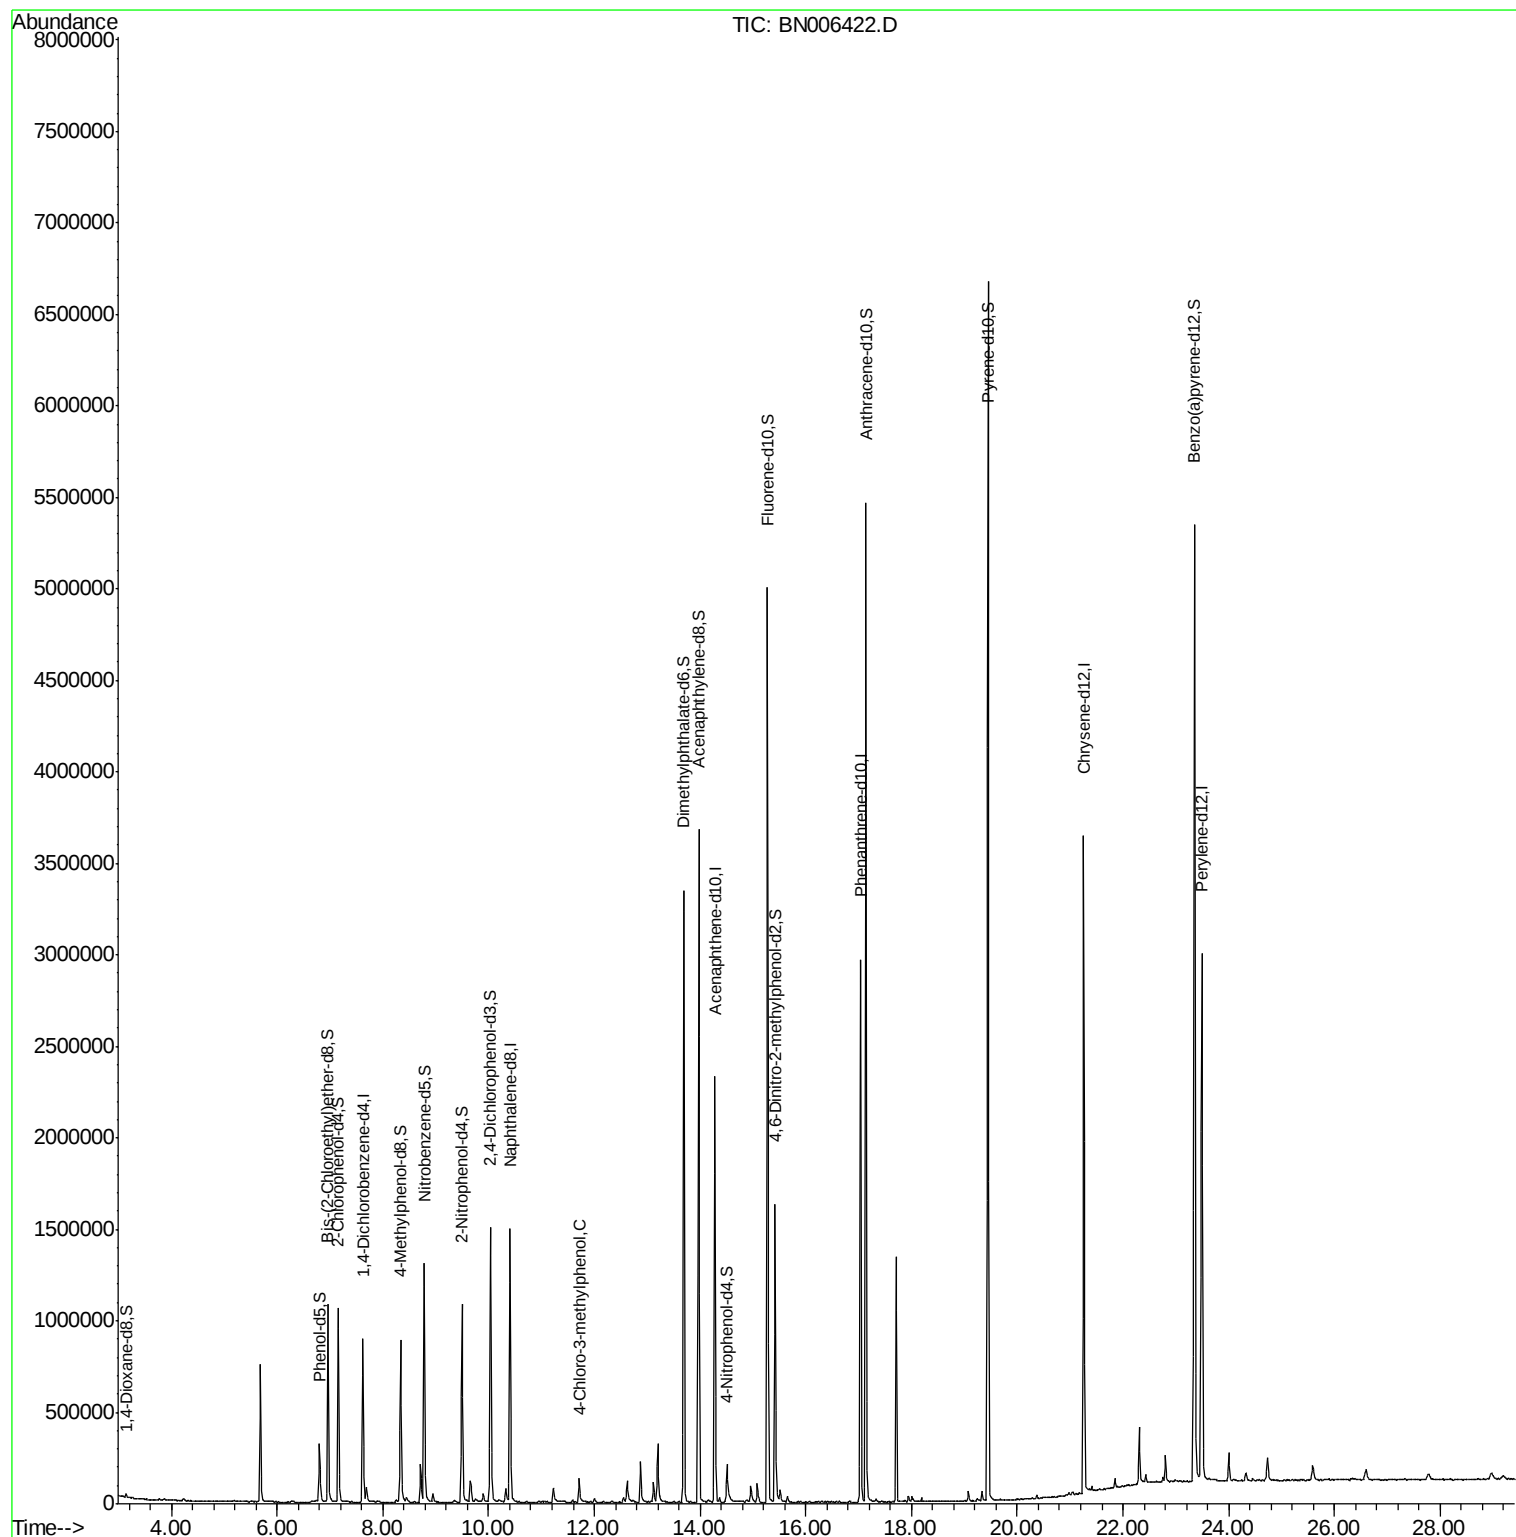


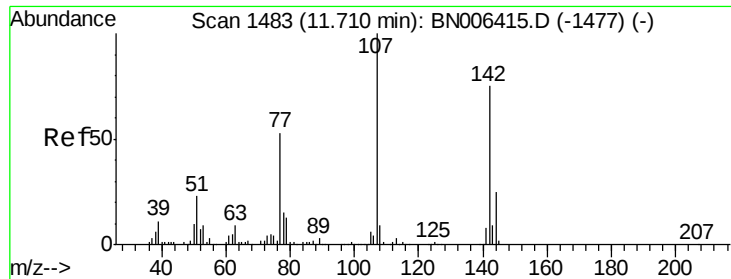

#33
 4-Chloro-3-methylphenol
 Concen: 2.711 ng/ul
 RT: 11.72 min Scan# 1484
 Delta R.T. 0.01 min
 Lab File: BN006422.D
 Acq: 20 Jun 2019 07:17

Instrument :
 BNA_N
 ClientSampleId :
 A4240

Tot Ion	Ratio	Lower	Upper
107	100		
144	23.6	20.7	31.1
142	76.3	60.8	91.2

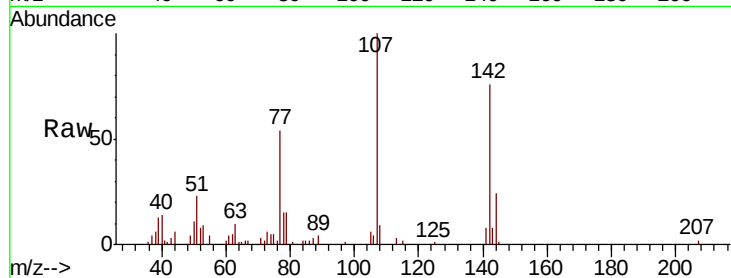

Abundance

Ion 107.00 (106.70 to 107.70): E

Ion 144.00 (143.70 to 144.70): E

Ion 142.00 (141.70 to 142.70): E

