

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061919\
 Data File : BN006430.D
 Acq On : 20 Jun 2019 15:21
 Operator : JU/SJ
 Sample : K3335-14
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A41Z6

Quant Time: Jun 20 16:14:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 20 07:11:27 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	232428	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1076214	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.29	164	670320	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.04	188	1523769	20.00	ng/ul	0.00
77) Chrysene-d12	21.28	240	1523893	20.00	ng/ul	0.03
85) Perylene-d12	23.53	264	1731878	20.00	ng/ul	0.05

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.14	96	17494	2.94	ng/uL	0.00
5) Phenol-d5	6.80	99	290338	11.73	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	215464	14.06	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	231659	12.69	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	237273	12.09	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	115390	13.39	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	121867	12.98	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	211171	11.71	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	314997	15.19	ng/ul	0.00
43) Dimethylphthalate-d6	13.70	166	921531	15.69	ng/ul	0.00
46) Acenaphthylene-d8	13.97	160	966994	13.43	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	86706	8.64	ng/ul	0.00
57) Fluorene-d10	15.28	176	726113	14.53	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	80654	8.36	ng/ul	0.00
70) Anthracene-d10	17.14	188	1105112	14.41	ng/ul	0.00
78) Pyrene-d10	19.45	212	1264606	14.21	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.39	264	1364333	13.95	ng/ul	0.05


Target Compounds					Ovalue	
44) Dimethylphthalate	13.75	163	296685	5.478	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061919\
Data File : BN006430.D
Acq On : 20 Jun 2019 15:21
Operator : JU/SJ
Sample : K3335-14
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41Z6

Quant Time: Jun 20 16:14:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 20 07:11:27 2019
Response via : Initial Calibration

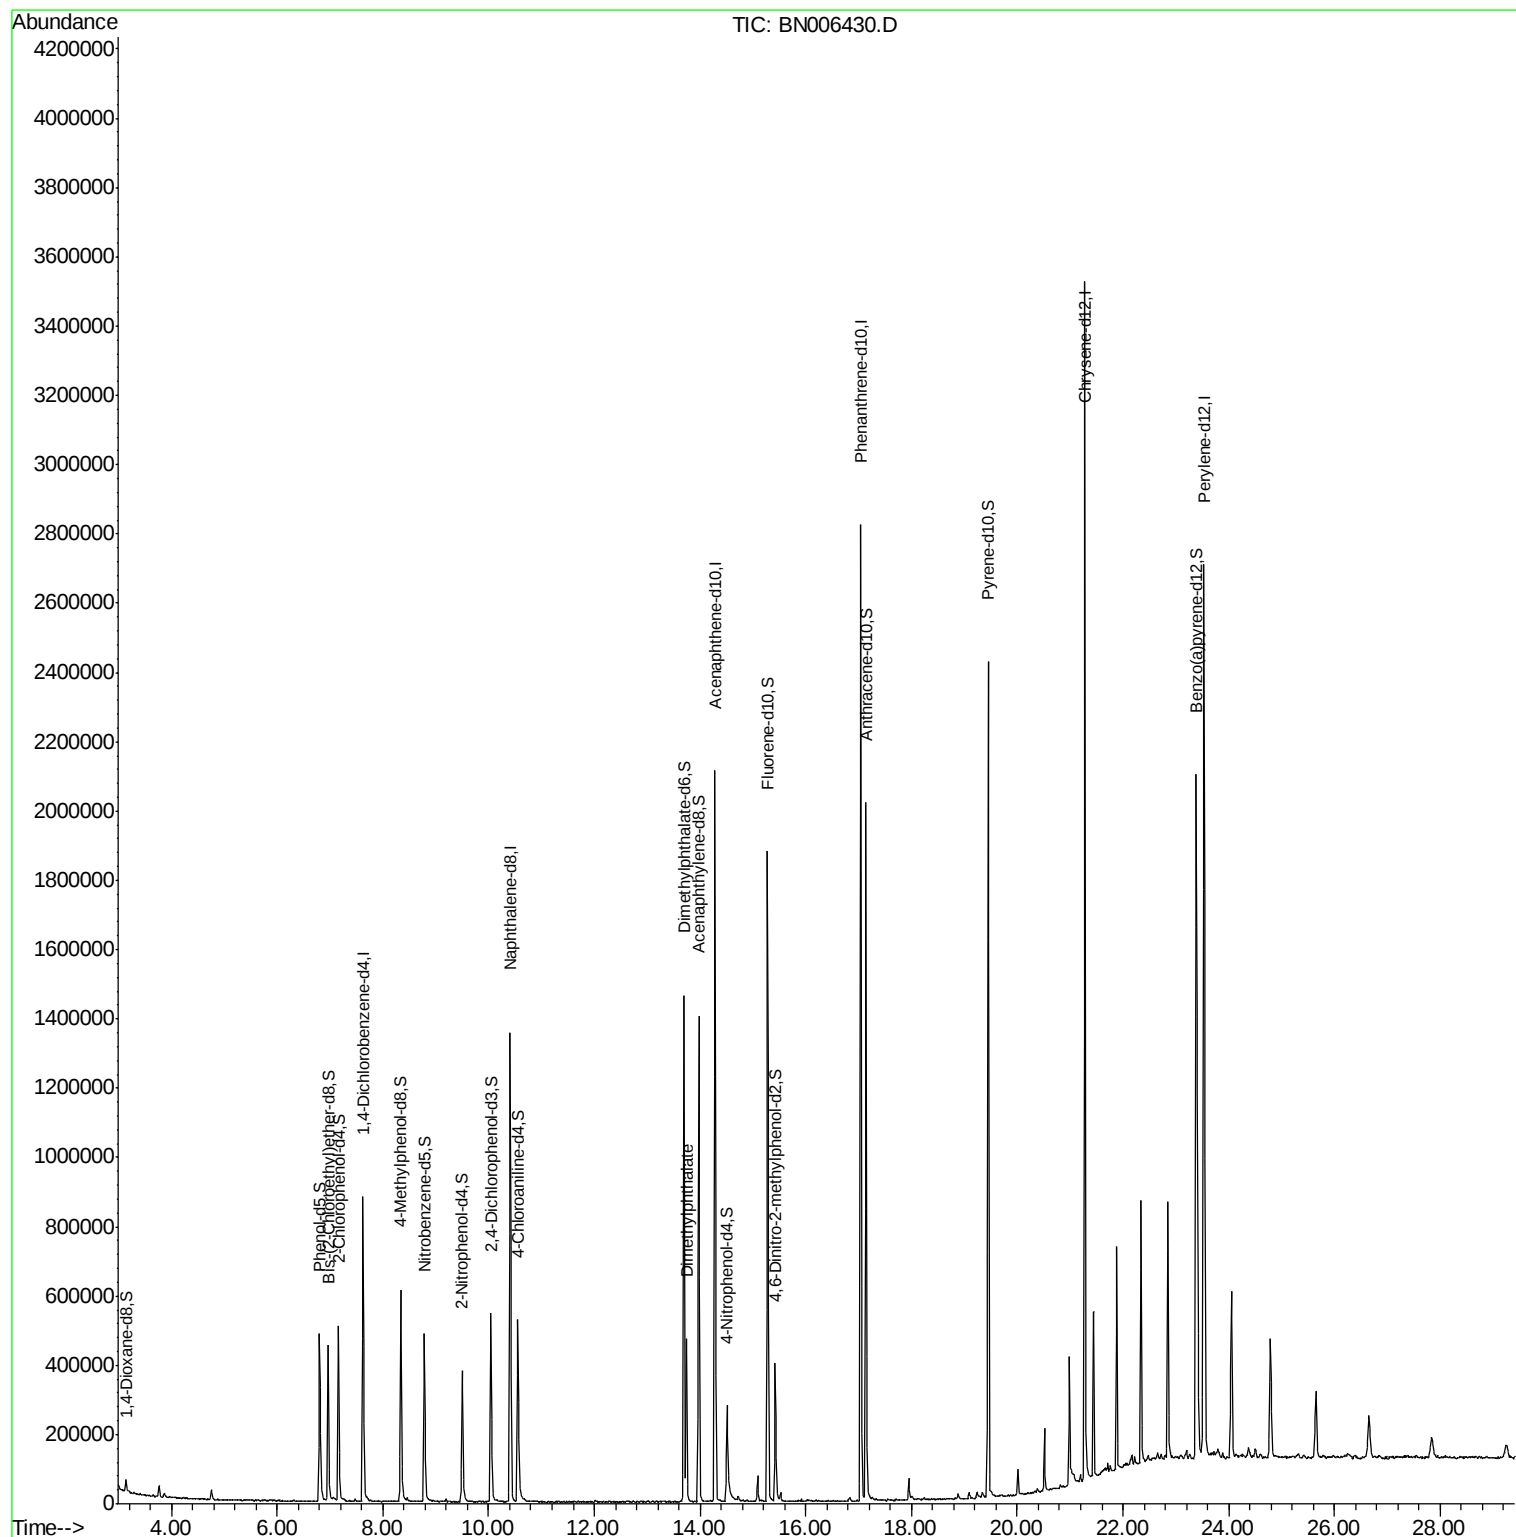

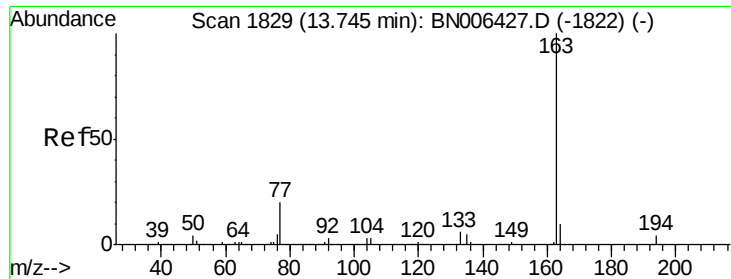

#44

Dimethylphthalate

Concen: 5.478 ng/ul

RT: 13.75 min Scan# 1829

Delta R.T. 0.01 min

Lab File: BN006430.D

Acq: 20 Jun 2019 15:21

Instrument :

BNA_N

ClientSampleId :

A41Z6


Tot Ion:163 Resp: 296685

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.0

164 9.9 8.0 12.0

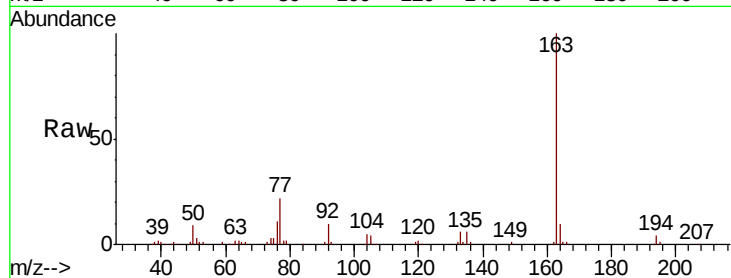

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

