

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061919\
 Data File : BN006445.D
 Acq On : 21 Jun 2019 01:10
 Operator : JU/SJ
 Sample : K3360-09
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A41Y9

Quant Time: Jun 21 04:56:51 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 21 04:51:38 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	205385	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	977826	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.28	164	607909	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.03	188	1405007	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	1425705	20.00	ng/ul	-0.02
85) Perylene-d12	23.48	264	1644725	20.00	ng/ul	-0.04

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	22474	4.27	ng/uL	0.00
5) Phenol-d5	6.80	99	400576	18.32	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	294376	21.74	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	328542	20.37	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	322354	18.58	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	167199	21.35	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	182560	21.40	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	311195	18.99	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	462564	24.54	ng/ul	0.00
43) Dimethylphthalate-d6	13.69	166	1206412	22.64	ng/ul	0.00
46) Acenaphthylene-d8	13.97	160	1390456	21.29	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	115915	12.73	ng/ul	0.00
57) Fluorene-d10	15.28	176	1025311	22.63	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	123571	13.90	ng/ul	0.00
70) Anthracene-d10	17.13	188	1618389	22.88	ng/ul	0.00
78) Pyrene-d10	19.45	212	1825604	21.92	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.34	264	2023538	21.78	ng/ul	-0.04

Target Compounds


				Ovalue	
6) Phenol	6.83	94	30277	1.436	ng/ul 91
44) Dimethylphthalate	13.74	163	197195	4.015	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061919\
Data File : BN006445.D
Acq On : 21 Jun 2019 01:10
Operator : JU/SJ
Sample : K3360-09
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41Y9

Quant Time: Jun 21 04:56:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 04:51:38 2019
Response via : Initial Calibration

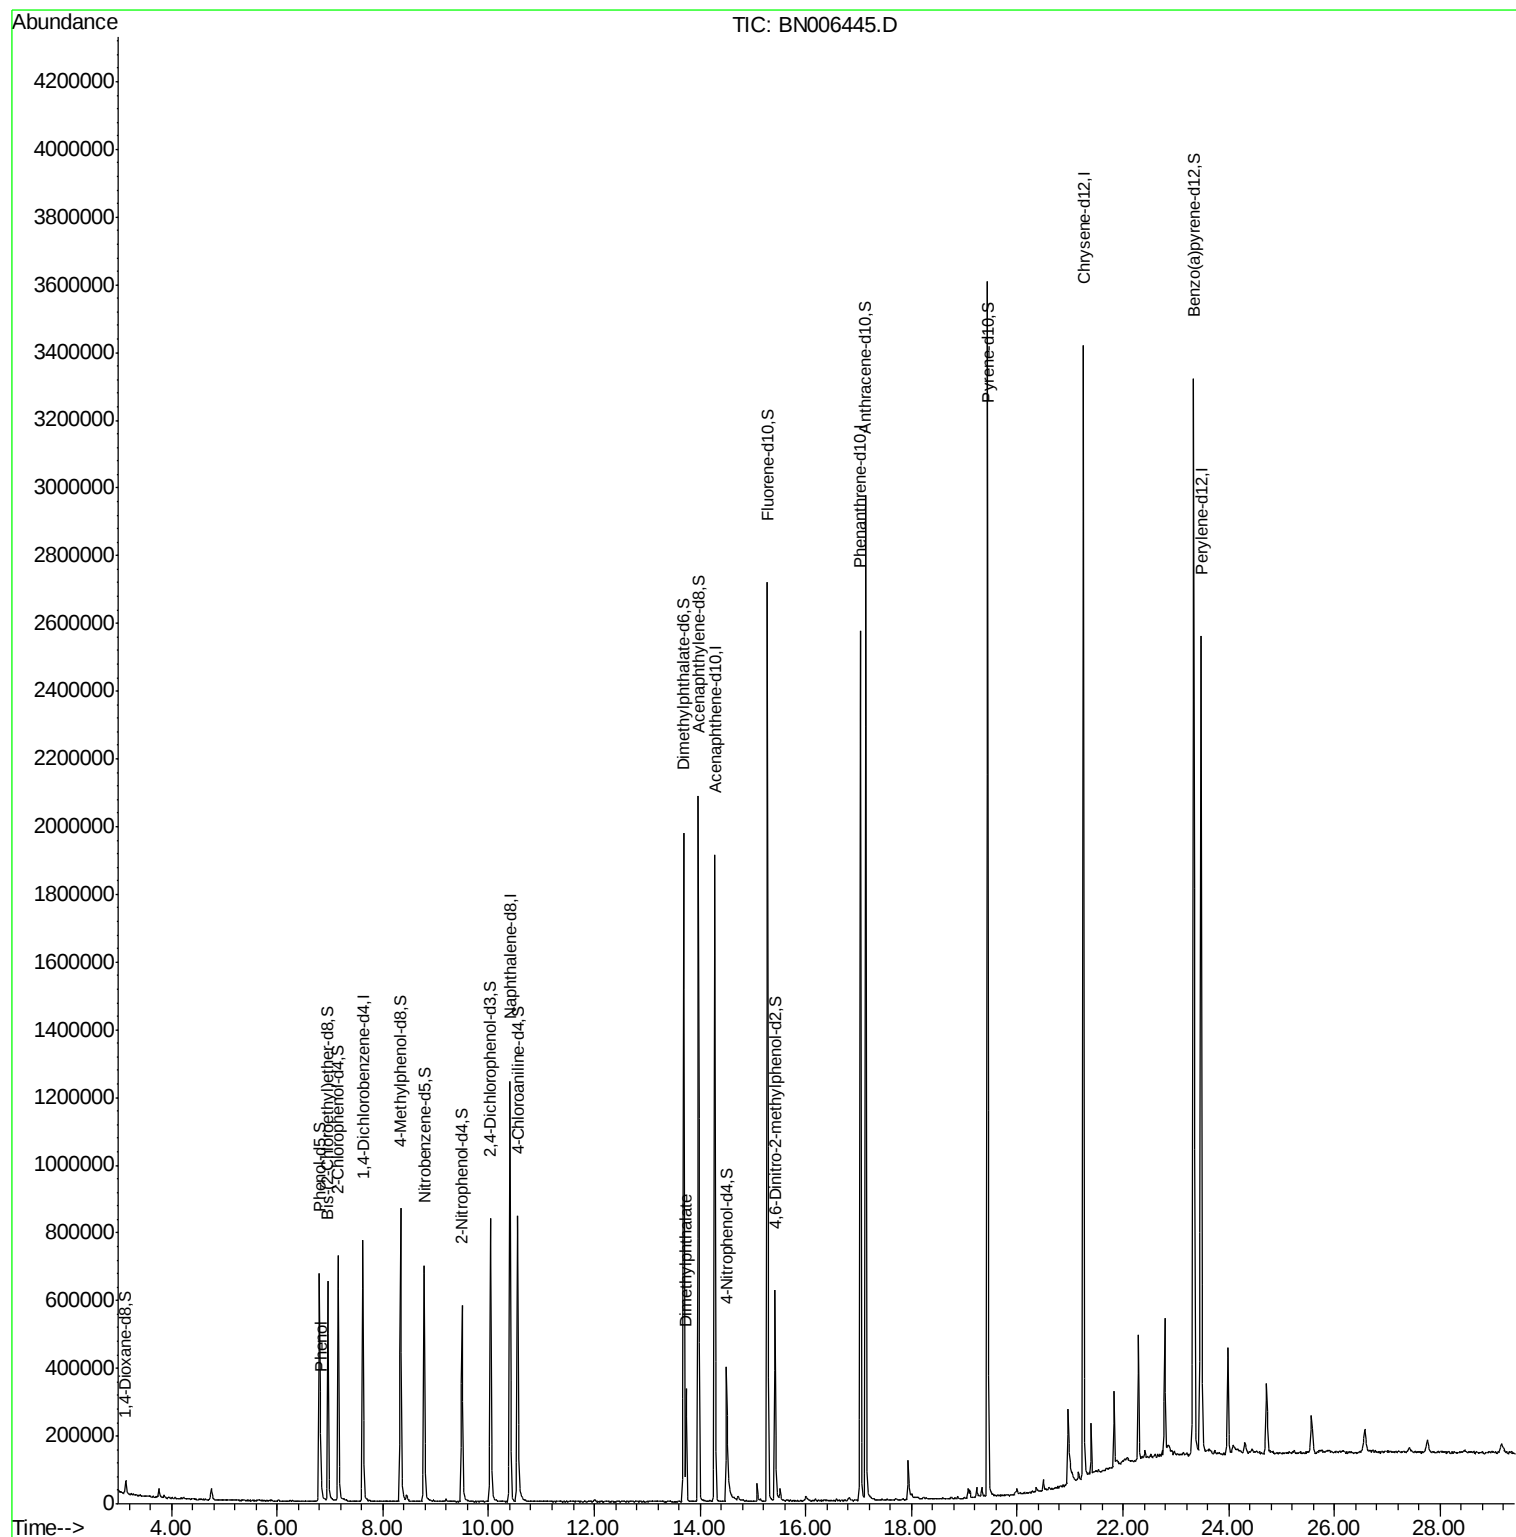

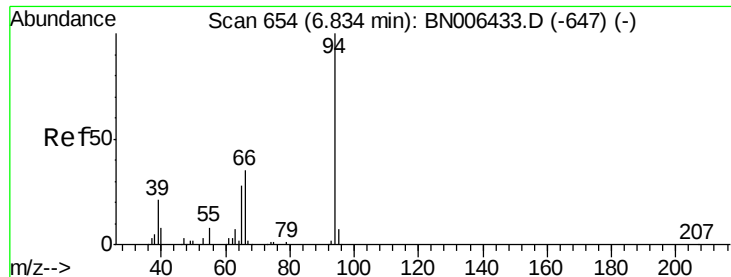





#6

Phenol

Concen: 1.436 ng/ul
 RT: 6.83 min Scan# 653
 Delta R.T. -0.01 min
 Lab File: BN006445.D
 Acq: 21 Jun 2019 01:10

Instrument :
 BNA_N
 ClientSampleId :
 A41Y9

Tot Ion	94	Resp	30277
Ion Ratio	Lower	Upper	
94	100		
65	30.9	22.5	33.7
66	44.1	29.5	44.3

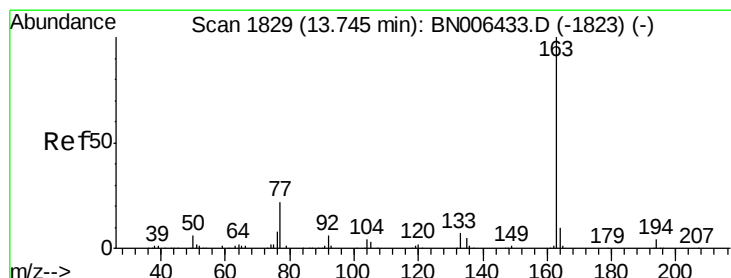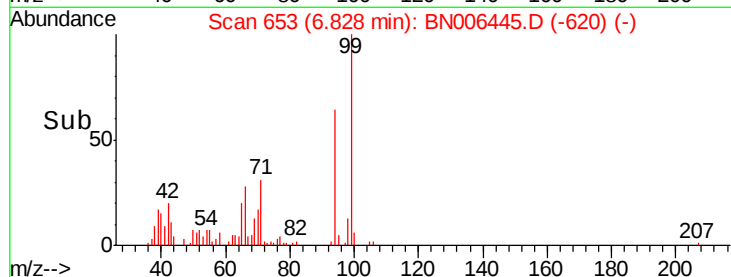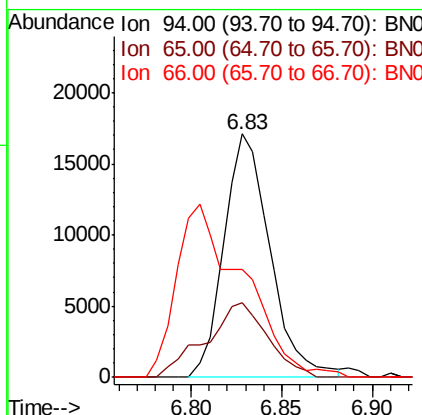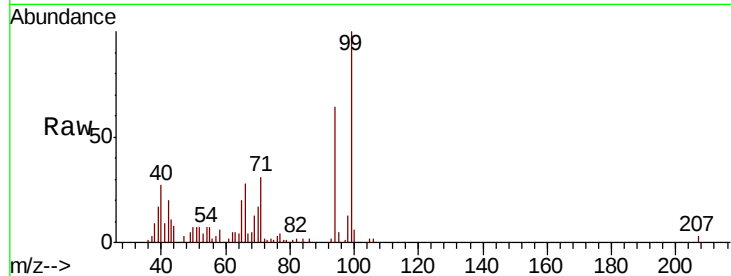

#44

Dimethylphthalate

Concen: 4.015 ng/ul
 RT: 13.74 min Scan# 1828
 Delta R.T. -0.01 min
 Lab File: BN006445.D
 Acq: 21 Jun 2019 01:10

Tgt Ion	163	Resp	197195
Ion Ratio	Lower	Upper	
163	100		
194	3.9	3.4	5.0
164	10.4	8.0	12.0

