

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061919\
 Data File : BN006456.D
 Acq On : 21 Jun 2019 08:04
 Operator : JU/SJ
 Sample : K3360-08
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A41Y8

Quant Time: Jun 21 12:07:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 21 06:31:50 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	239150	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	1114058	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.28	164	679636	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.03	188	1524037	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	1468625	20.00	ng/ul	0.00
85) Perylene-d12	23.49	264	1600628	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	23998	3.92	ng/uL	0.00
5) Phenol-d5	6.80	99	501170	19.68	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	318932	20.23	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	379773	20.23	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	355485	17.60	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	190254	21.33	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	210979	21.71	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	391502	20.97	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	455956	21.23	ng/ul	0.00
43) Dimethylphthalate-d6	13.69	166	1397681	23.46	ng/ul	0.00
46) Acenaphthylene-d8	13.97	160	1662277	22.77	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	171776	16.88	ng/ul	0.00
57) Fluorene-d10	15.28	176	1216996	24.02	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	145949	15.13	ng/ul	0.00
70) Anthracene-d10	17.13	188	1835473	23.92	ng/ul	0.00
78) Pyrene-d10	19.45	212	2057766	23.99	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.35	264	2107995	23.32	ng/ul	0.00

Target Compounds


					Ovalue
6) Phenol	6.83	94	28259	1.151 ng/ul	91
44) Dimethylphthalate	13.74	163	253977	4.625 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061919\
Data File : BN006456.D
Acq On : 21 Jun 2019 08:04
Operator : JU/SJ
Sample : K3360-08
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41Y8

Quant Time: Jun 21 12:07:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 06:31:50 2019
Response via : Initial Calibration

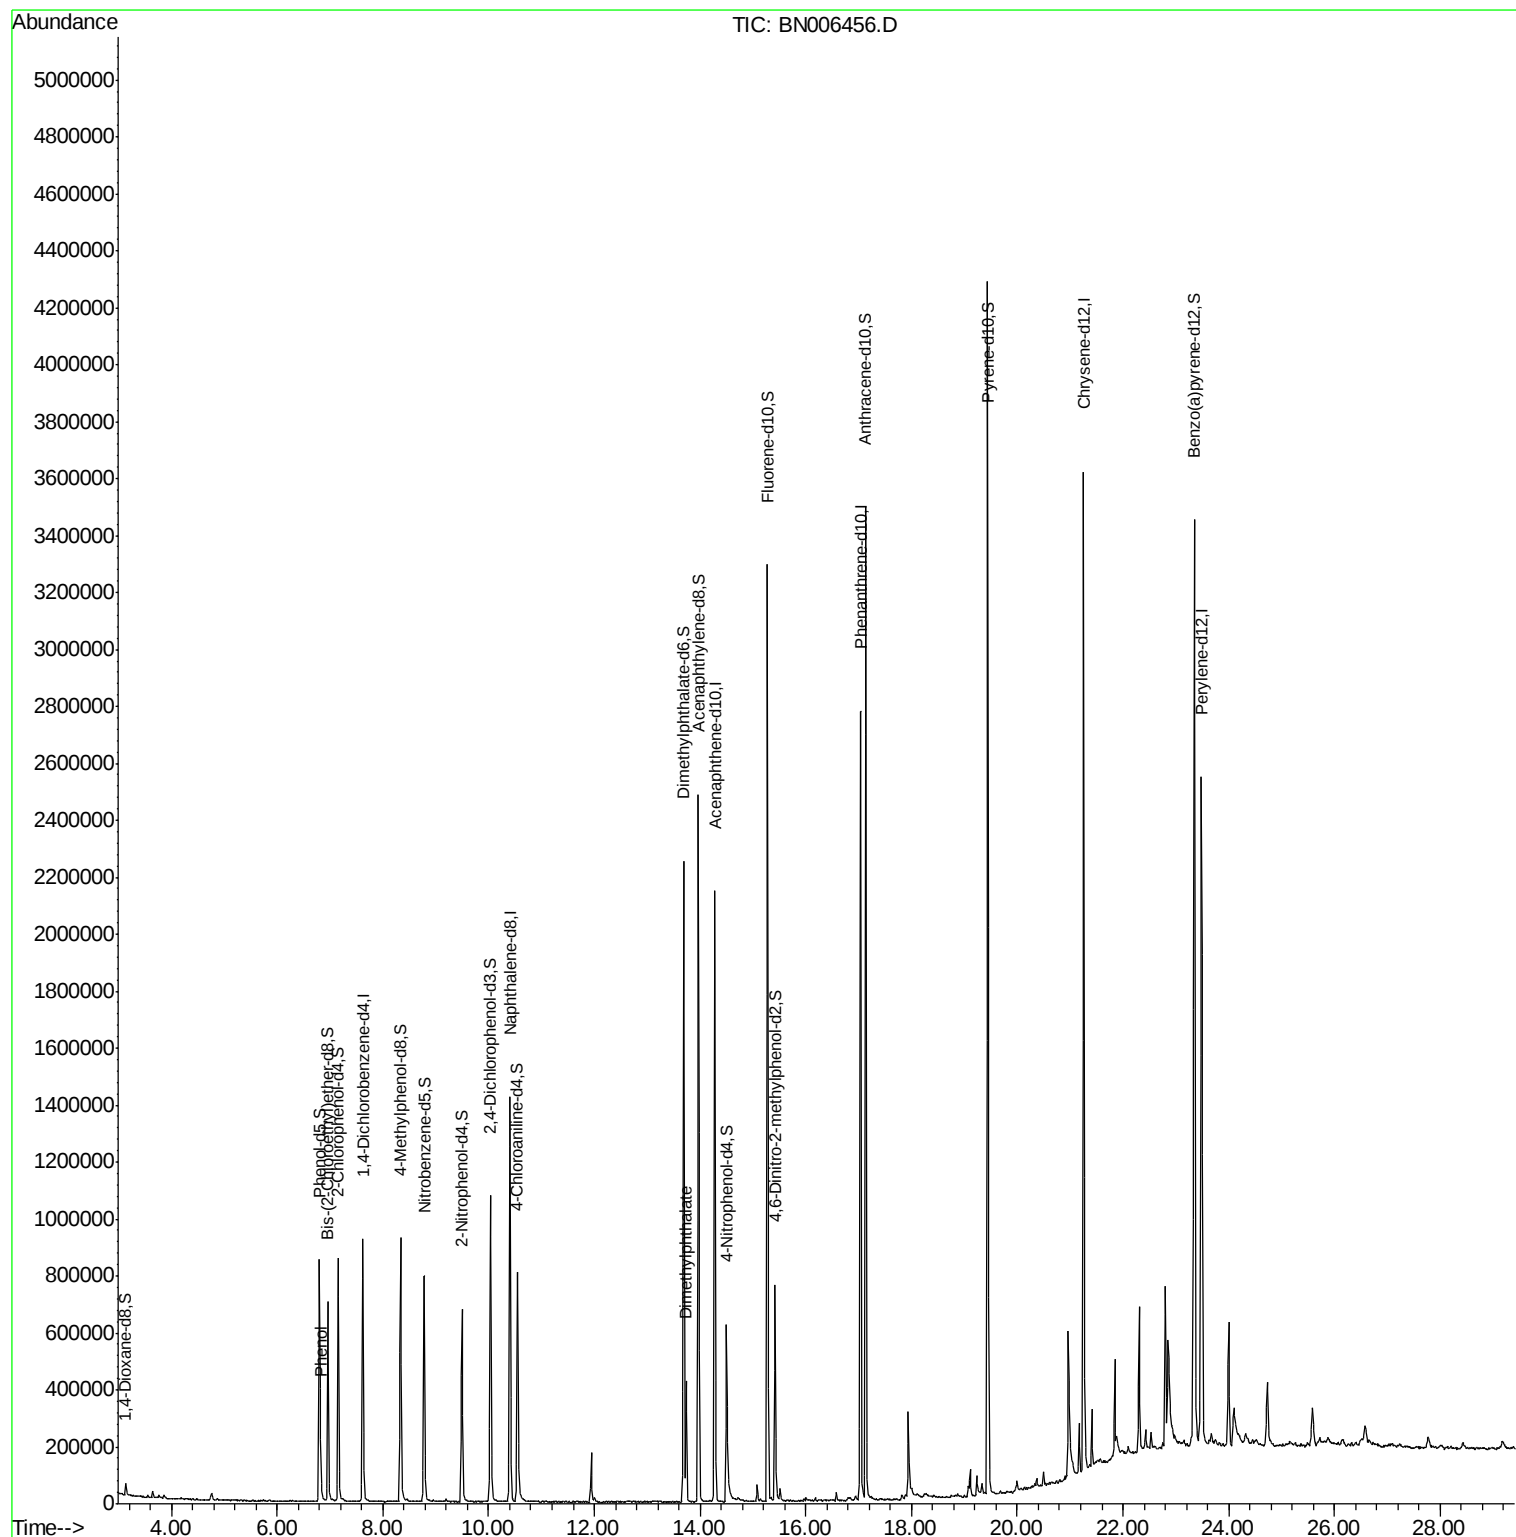

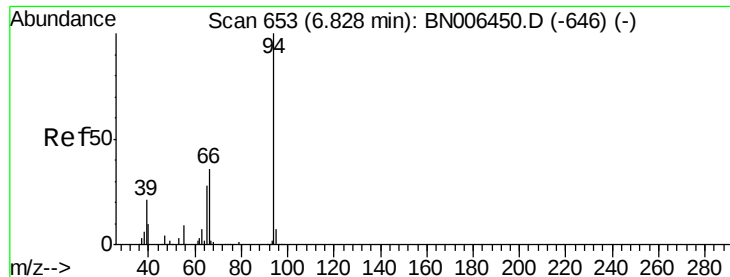

#6

Phenol

Concen: 1.151 ng/ul

RT: 6.83 min Scan# 653

Delta R.T. -0.00 min

Lab File: BN006456.D

Acq: 21 Jun 2019 08:04

Instrument :

BNA_N

ClientSampleId :

A41Y8





Tot Ion: 94 Resp: 28259

Ion Ratio Lower Upper

94 100

65 31.0 22.5 33.7

66 43.7 29.5 44.3

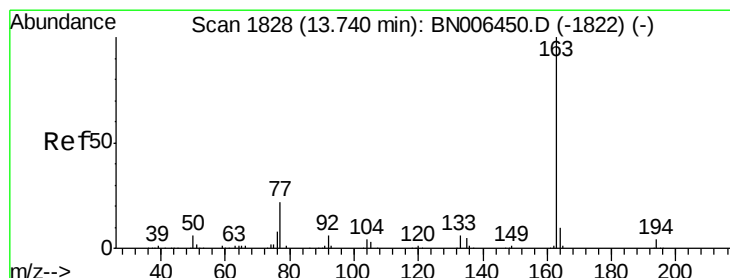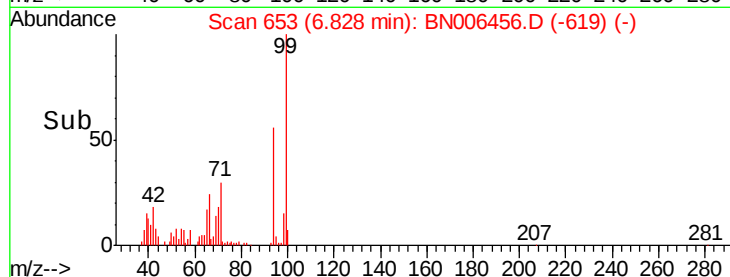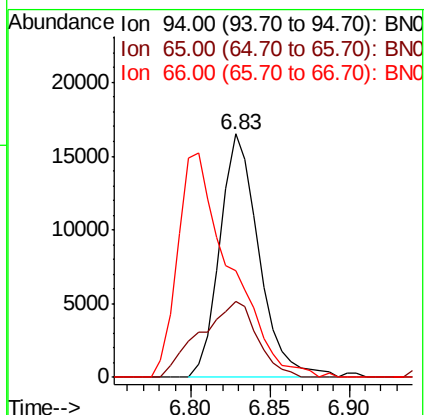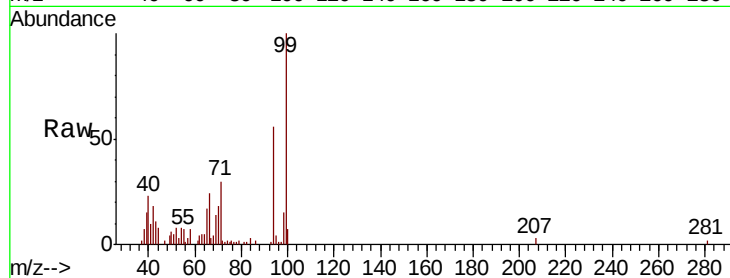

#44

Dimethylphthalate

Concen: 4.625 ng/ul

RT: 13.74 min Scan# 1828

Delta R.T. -0.00 min

Lab File: BN006456.D

Acq: 21 Jun 2019 08:04

Tgt Ion: 163 Resp: 253977

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.0

164 10.2 8.0 12.0

