

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061919\
 Data File : BN006406.D
 Acq On : 19 Jun 2019 20:55
 Operator : JU/SJ
 Sample : K3224-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0C62

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	23	26	31	rVB	23364	27643	0.29%	0.034%
2	3.764	129	132	137	rVB2	10452	13180	0.14%	0.016%
3	3.864	145	149	155	rVB2	9143	12079	0.13%	0.015%
4	4.293	219	222	225	rBV	8399	11315	0.12%	0.014%
5	4.975	334	338	343	rVB5	8815	14636	0.15%	0.018%
6	6.769	638	643	644	rBV	13809	16902	0.18%	0.021%
7	6.805	644	649	670	rVB	348559	566709	5.90%	0.696%
8	6.963	670	676	688	rBV	1258068	1905301	19.83%	2.341%
9	7.157	703	709	723	rBV	1240893	2020241	21.02%	2.483%
10	7.628	782	789	803	rBV	814905	1373391	14.29%	1.688%
11	7.987	845	850	854	rVB4	5618	9926	0.10%	0.012%
12	8.340	903	910	927	rBV	935714	1613467	16.79%	1.983%
13	8.781	978	985	1000	rBV	1479392	2447139	25.46%	3.007%
14	9.193	1049	1055	1061	rBV	34752	54480	0.57%	0.067%
15	9.498	1100	1107	1124	rBV	1208423	2032608	21.15%	2.498%
16	10.034	1191	1198	1218	rBV	1617766	2918859	30.37%	3.587%
17	10.410	1254	1262	1277	rBV	1263158	2129717	22.16%	2.617%
18	11.687	1474	1479	1485	rVB	30060	43538	0.45%	0.054%
19	12.016	1529	1535	1543	rBV2	12934	27912	0.29%	0.034%
20	13.698	1814	1821	1836	rBV	3675206	5097782	53.05%	6.264%
21	13.975	1861	1868	1890	rBV	4035755	5990213	62.33%	7.361%
22	14.281	1914	1920	1934	rBV2	2074111	3030602	31.54%	3.724%
23	14.510	1954	1959	1976	rBV	149670	341058	3.55%	0.419%
24	15.086	2053	2057	2064	rVB	44025	56519	0.59%	0.069%
25	15.281	2084	2090	2108	rBV	5254804	7448509	77.51%	9.153%
26	15.422	2108	2114	2127	rVV	1624774	2360912	24.57%	2.901%
27	15.522	2127	2131	2142	rVB	72014	120279	1.25%	0.148%
28	16.833	2349	2354	2355	rBV2	7719	9930	0.10%	0.012%
29	17.039	2382	2389	2399	rBV2	2532818	3685651	38.35%	4.529%
30	17.139	2399	2406	2425	rVV	5467331	8031811	83.58%	9.870%
31	17.939	2539	2542	2548	rBV4	12915	21388	0.22%	0.026%
32	19.080	2730	2736	2743	rBV	51978	80028	0.83%	0.098%
33	19.239	2758	2763	2766	rBV4	6846	11604	0.12%	0.014%
34	19.333	2775	2779	2789	rBV	50184	63238	0.66%	0.078%

LSC Area Percent Report

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061919\
Data File : BN006406.D
Acq On : 19 Jun 2019 20:55
Operator : JU/SJ
Sample : K3224-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0C62

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
Title : SVOA CALIBRATION

35	19.445	2792	2798	2813	rBV2	6510066	9236337	96.11%	11.350%
36	19.992	2887	2891	2896	rBV4	6925	11363	0.12%	0.014%
37	20.968	3055	3057	3065	rVB5	12913	21057	0.22%	0.026%
38	21.039	3065	3069	3073	rBV5	23575	38916	0.40%	0.048%
39	21.251	3100	3105	3119	rBV	2906377	4002616	41.65%	4.919%
40	21.410	3129	3132	3136	rVB2	23690	27301	0.28%	0.034%
41	21.839	3202	3205	3210	rBV	60604	71897	0.75%	0.088%
42	22.298	3279	3283	3288	rBV	100821	133282	1.39%	0.164%
43	22.798	3364	3368	3373	rVB	117797	156258	1.63%	0.192%
44	23.345	3453	3461	3475	rBV	5261802	9609936	100.00%	11.809%
45	23.480	3477	3484	3499	rVB	2246874	4158469	43.27%	5.110%
46	23.992	3566	3571	3578	rVB	99536	179037	1.86%	0.220%
47	24.721	3692	3695	3705	rVB2	72880	142565	1.48%	0.175%


Sum of corrected areas: 81377601

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061919\
Data File : BN006406.D
Acq On : 19 Jun 2019 20:55
Operator : JU/SJ
Sample : K3224-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0C62

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

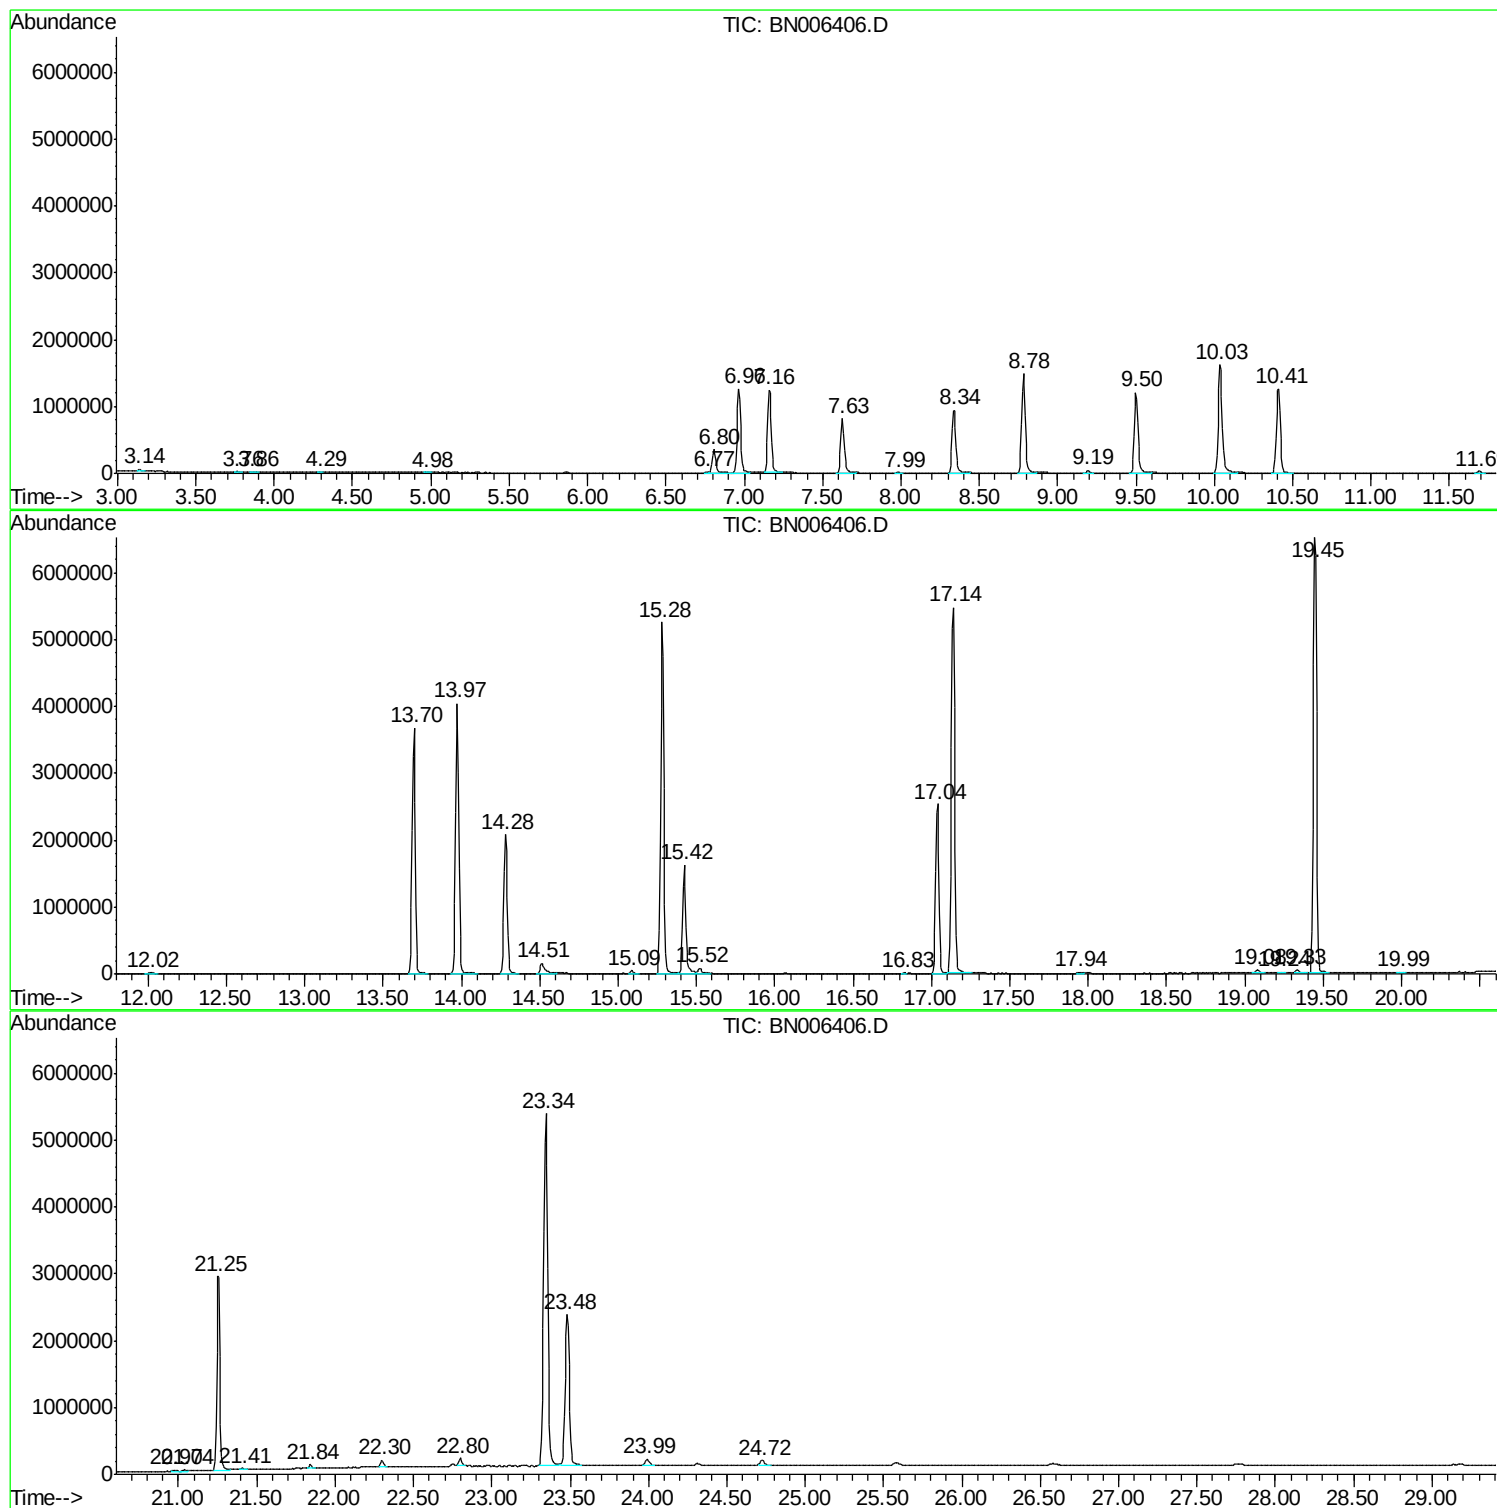

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061919\
Data File : BN006406.D
Acq On : 19 Jun 2019 20:55
Operator : JU/SJ
Sample : K3224-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0C62

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061919\
Data File : BN006406.D
Acq On : 19 Jun 2019 20:55
Operator : JU/SJ
Sample : K3224-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0C62

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc