
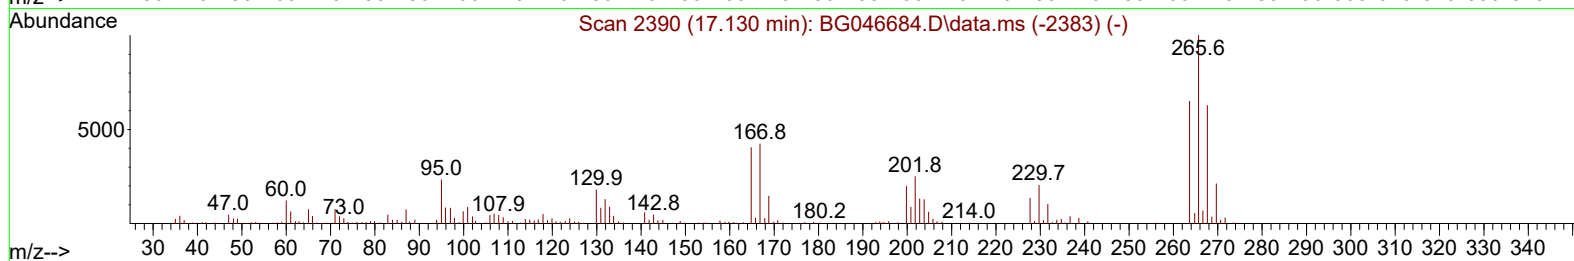
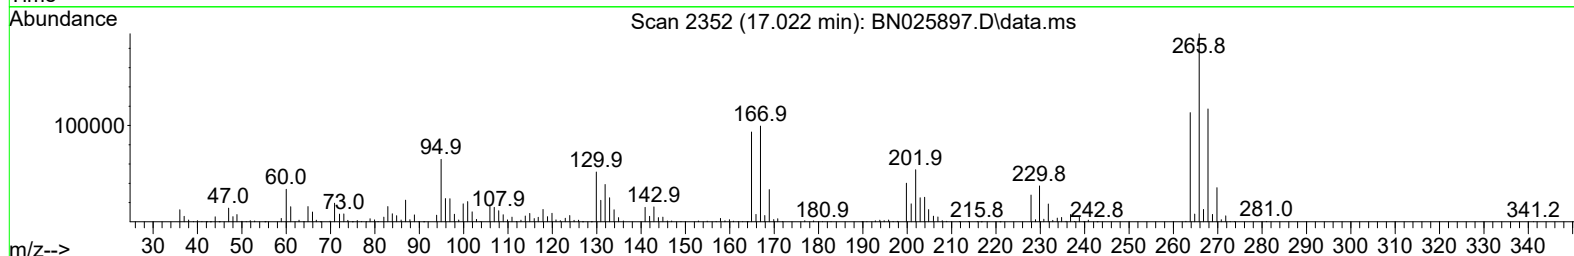


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061923\
 Data File : BN025897.D
 Acq On : 19 Jun 2023 13:01
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 20 05:21:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 05:20:59 2023
 Response via : Initial Calibration

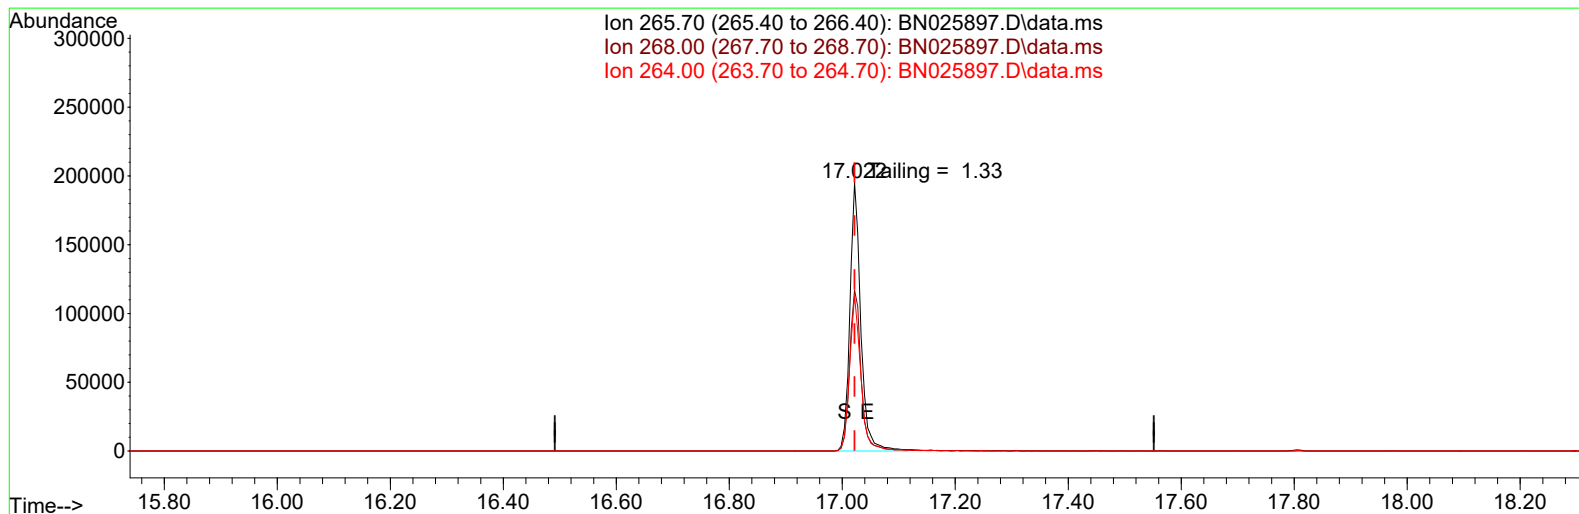

TIC: BN025897.D\data.ms

(70) Pentachlorophenol (C)




17.022min (0.000) 18822.02 ng

response 264254

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.00
264.00	61.60	58.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061923\
Data File : BN025897.D
Acq On : 19 Jun 2023 13:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 20 05:21:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 05:20:59 2023
Response via : Initial Calibration

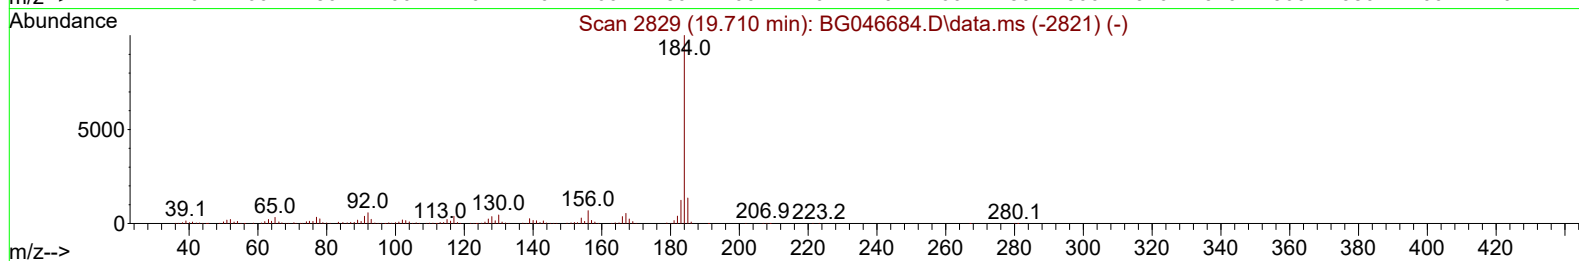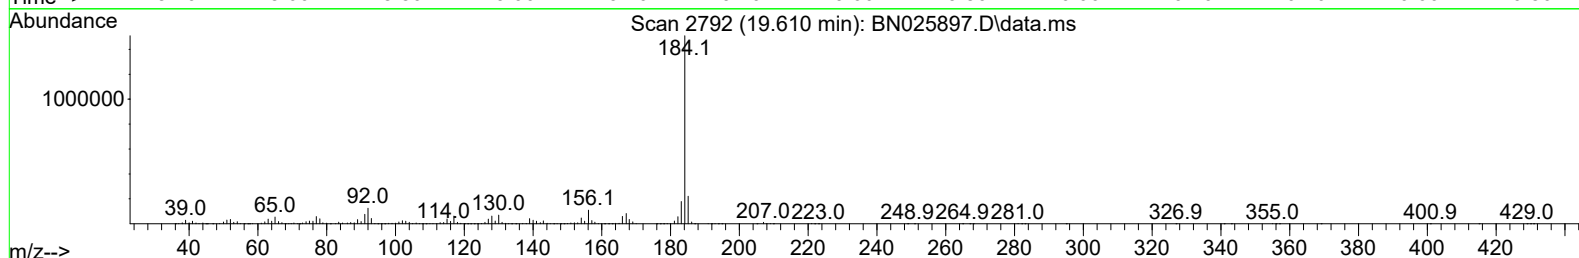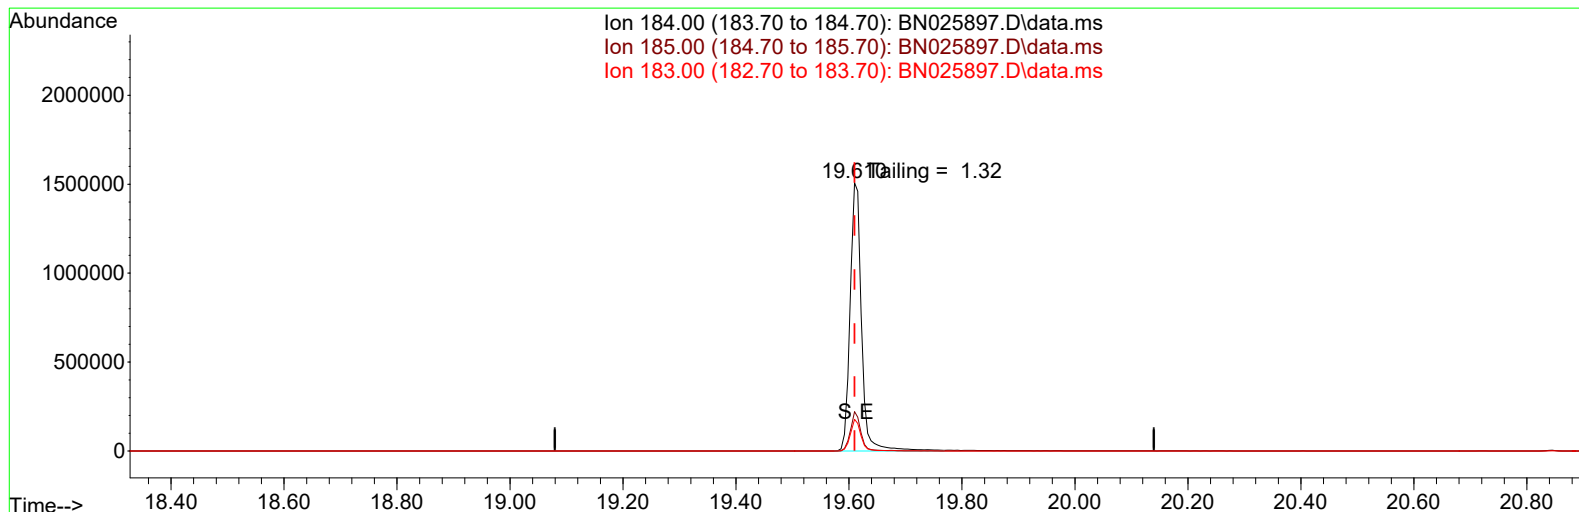

TIC: BN025897.D\data.ms

(77) Benzidine

19.610min (0.000) 0.00 ng

response 2126058

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.67
183.00	13.20	11.84
0.00	0.00	0.00