
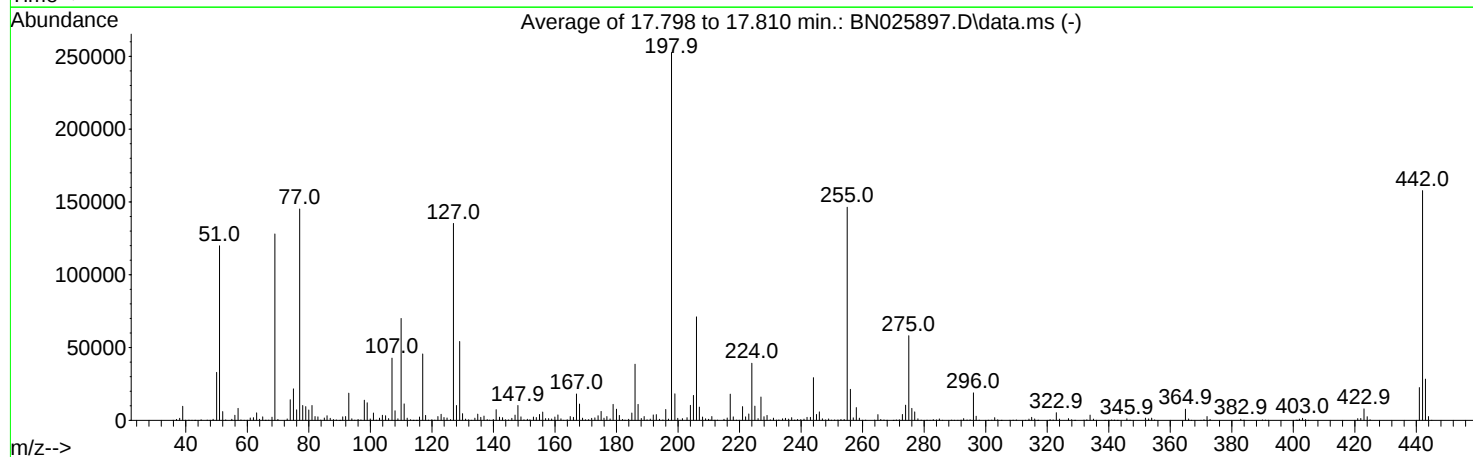


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061923\
Data File : BN025897.D
Acq On : 19 Jun 2023 13:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN053123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 16 14:10:48 2023

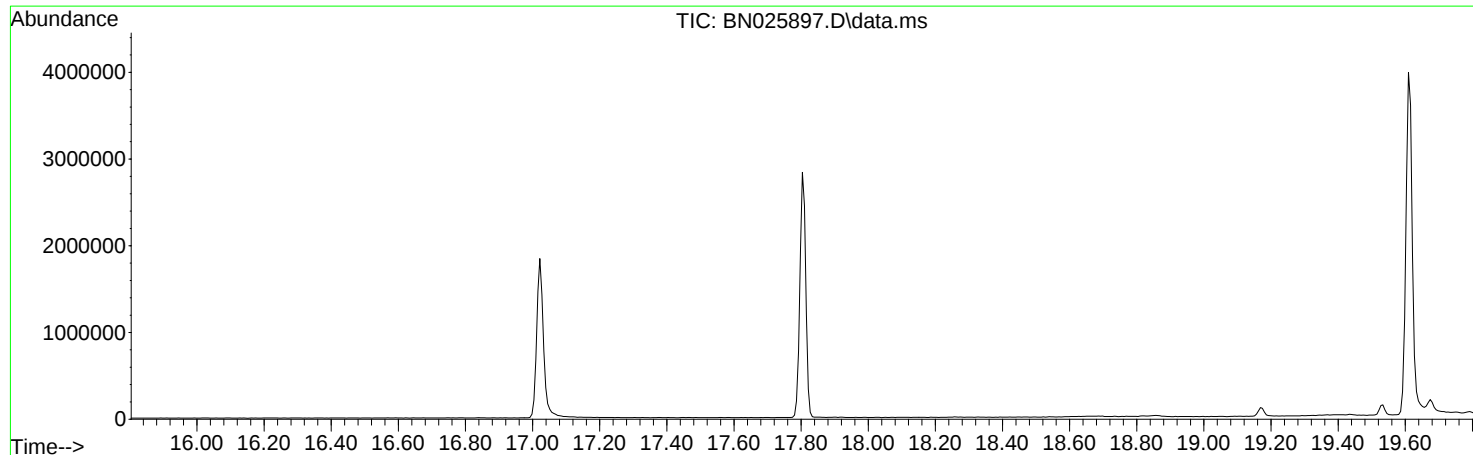

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.5	119932	PASS
68	69	0.00	2	1.7	2234	PASS
69	198	0.00	100	50.7	128061	PASS
70	69	0.00	2	0.5	635	PASS
127	198	10	80	53.5	135251	PASS
197	198	0.00	2	0.3	880	PASS
198	198	100	100	100.0	252651	PASS
199	198	5	9	7.2	18251	PASS
275	198	10	60	23.0	58131	PASS
365	198	1	100	3.0	7658	PASS
441	198	0.01	100	8.9	22539	PASS
442	442	50	100	100.0	157856	PASS
443	442	15	24	18.0	28384	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/19/2023	BNA_N	<u>BN025897.D</u>
Compound Name	Response	Retention Time
DDT	850356	20.845
DDD	21065	20.404
DDE	709	19.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21774	872130	2.50

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061923\
 Data File : BN025897.D
 Acq On : 19 Jun 2023 13:01
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jun 20 05:21:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 05:20:59 2023
 Response via : Initial Calibration

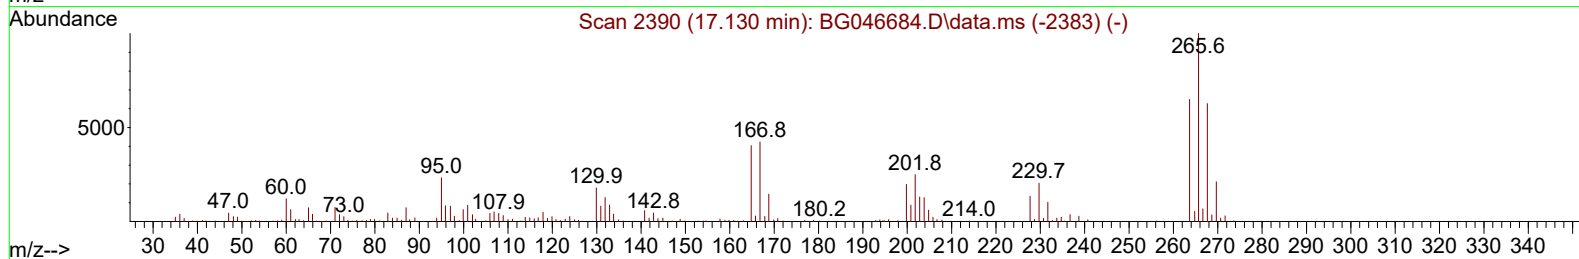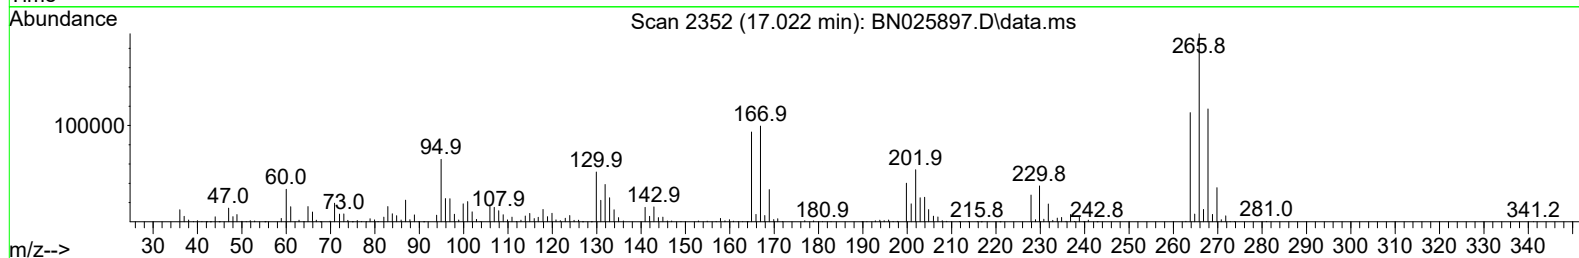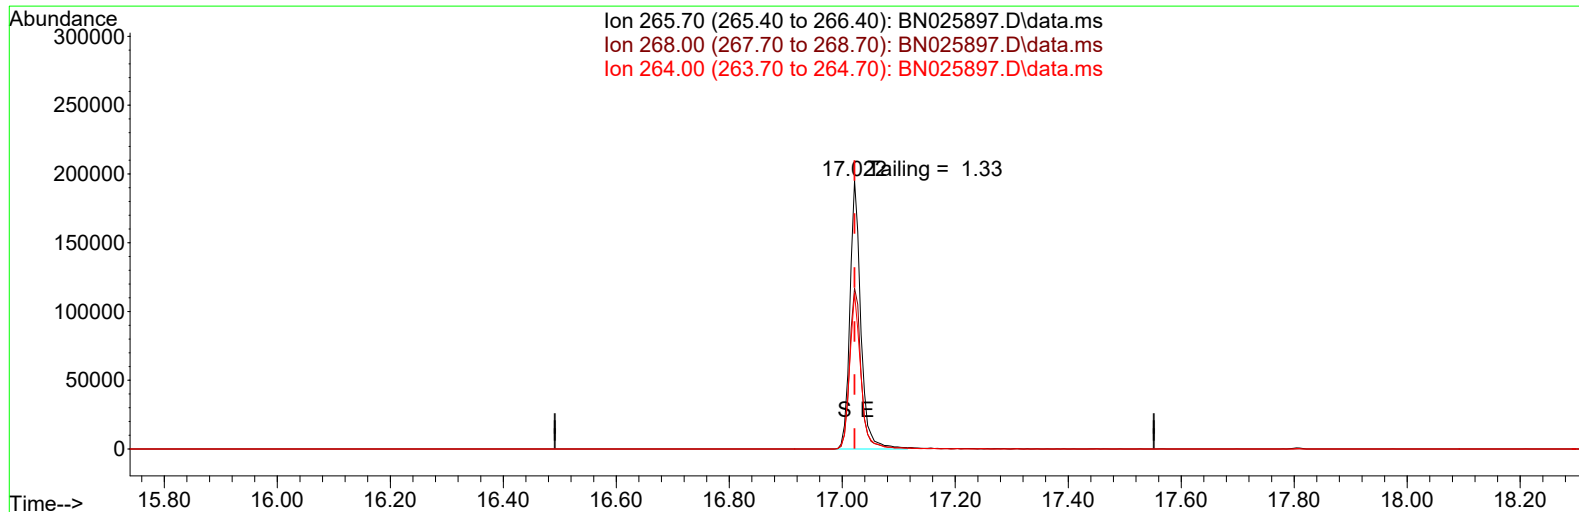

TIC: BN025897.D\data.ms

(70) Pentachlorophenol (C)

17.022min (0.000) 18822.02 ng




response 264254

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.00
264.00	61.60	58.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061923\
Data File : BN025897.D
Acq On : 19 Jun 2023 13:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 20 05:21:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 05:20:59 2023
Response via : Initial Calibration

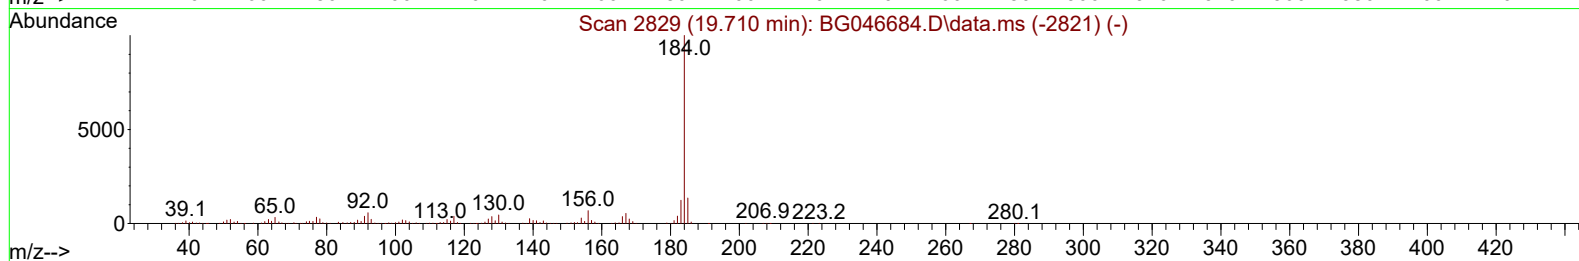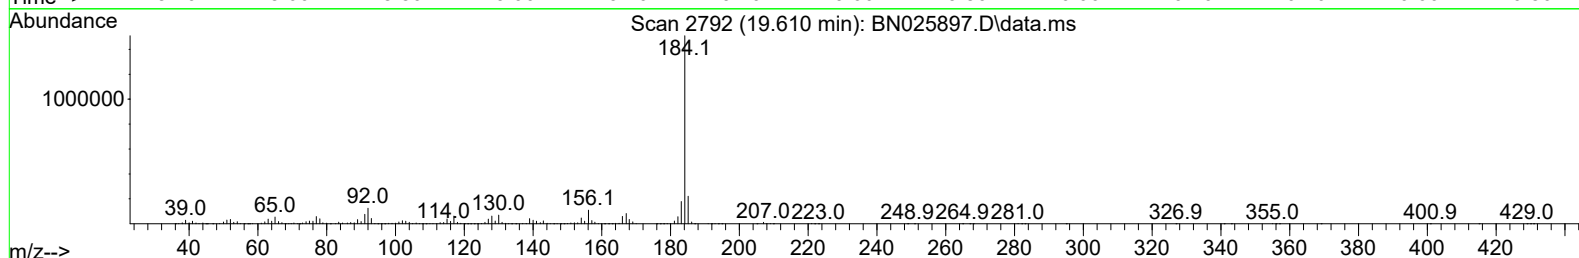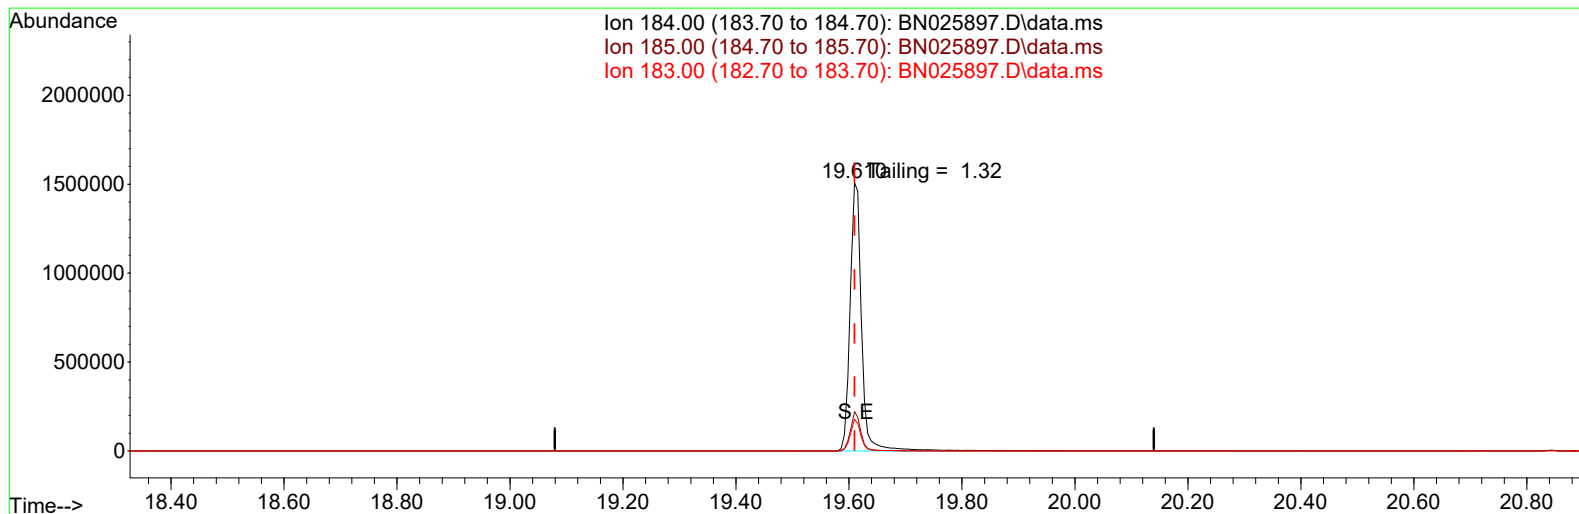

TIC: BN025897.D\data.ms

(77) Benzidine

19.610min (0.000) 0.00 ng

response 2126058

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.67
183.00	13.20	11.84
0.00	0.00	0.00