

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN062018\

Data File : BN001896.D

Acq On : 20 Jun 2018 20:54

Operator : JU/SJ

Sample : J3568-04

Misc :

ALS Vial : 19 Sample Multiplier: 1

Quant Time: Jun 21 03:27:51 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061918.M

Quant Title : SVOA CALIBRATION

QLast Update : Tue Jun 19 14:50:02 2018

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :


DAXP0

Manual Integrations

APPROVED

Sohil

6/21/2018 6:32:59 PM

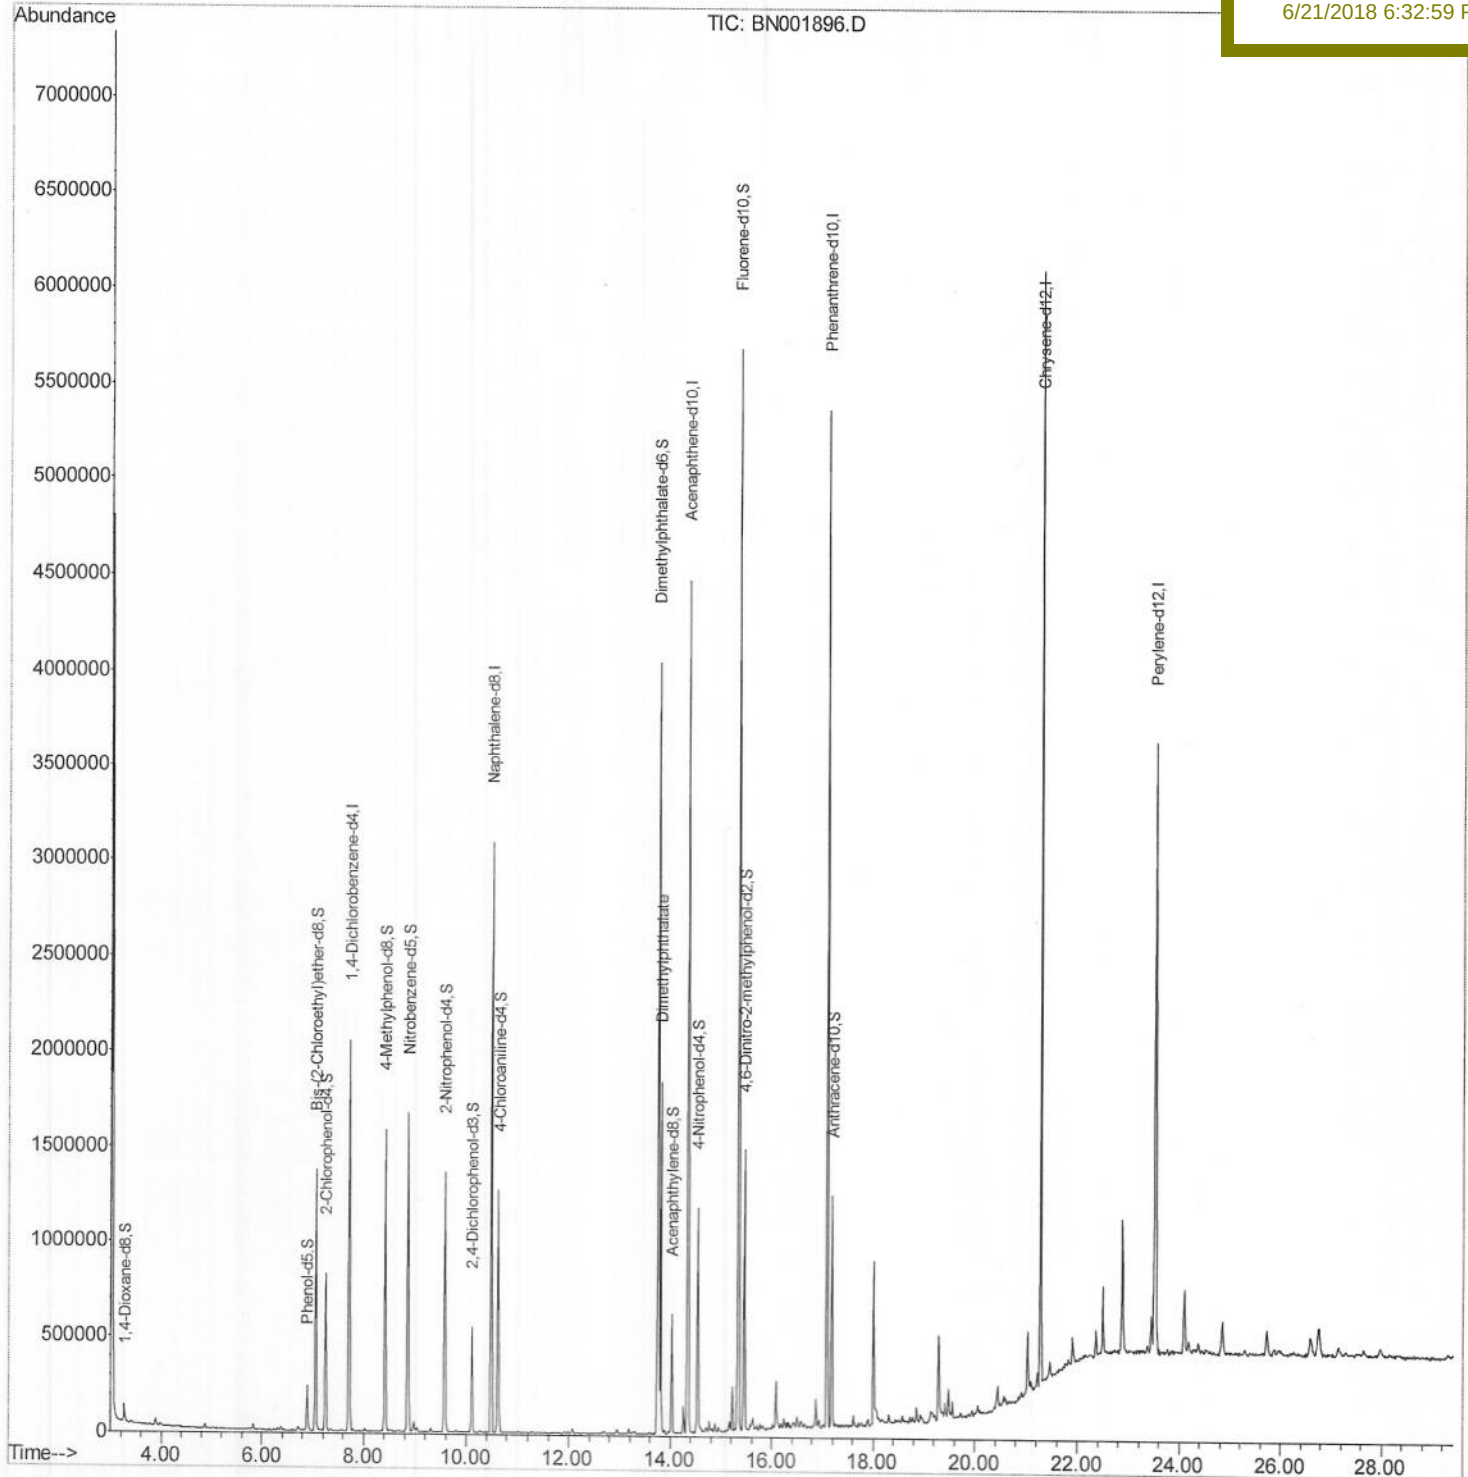

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062018\

Data File : BN001896.D

Acq On : 20 Jun 2018 20:54

Operator : JU/SJ

Sample : J3568-04

Misc :

ALS Vial : 19 Sample Multiplier: 1

Quant Time: Jun 21 01:12:06 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061918.M

Quant Title : SVOA CALIBRATION

QLast Update : Tue Jun 19 14:50:02 2018

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




DAXP0

Manual Integrations

APPROVED

Sohil

6/21/2018 6:32:59 PM

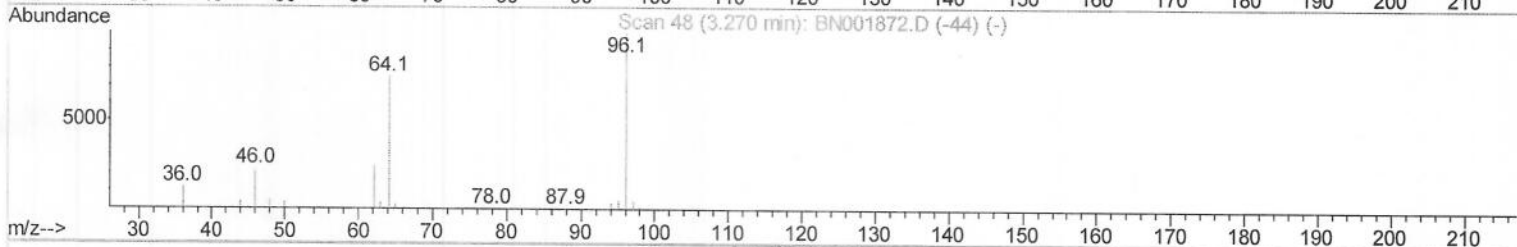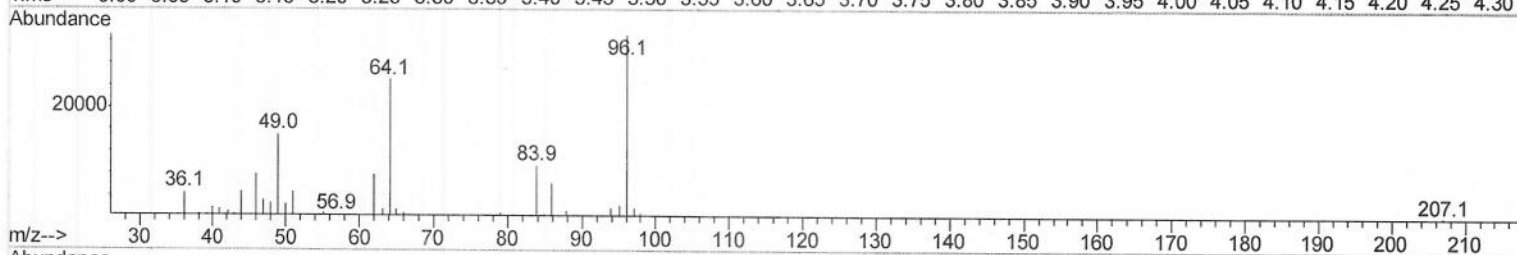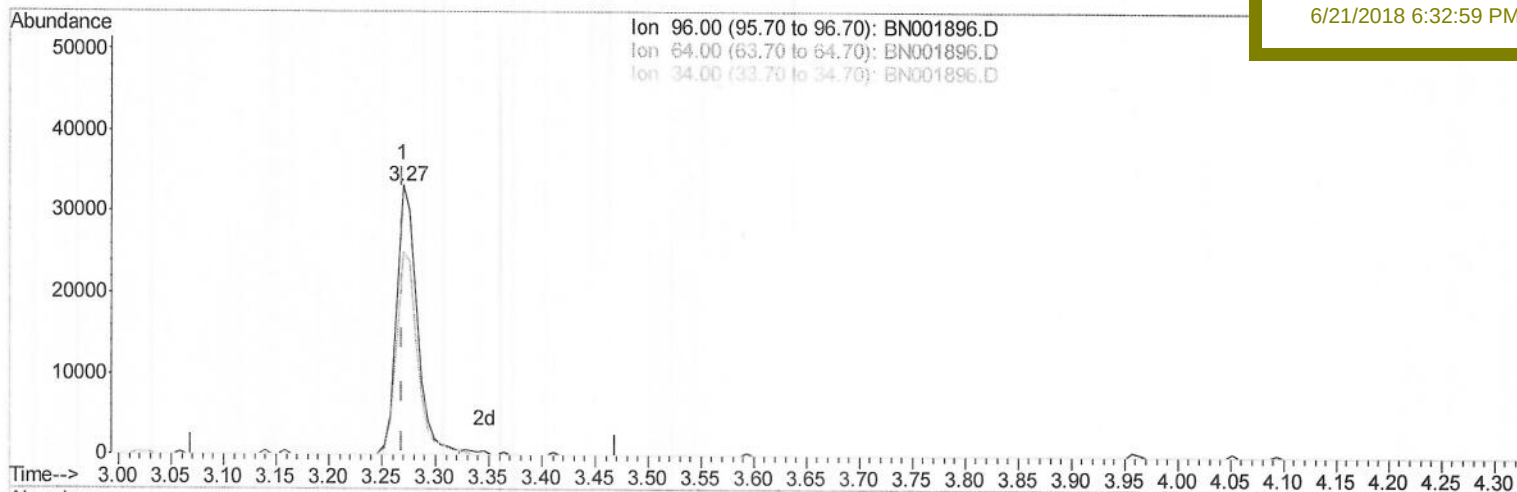

TIC: BN001896.D

(3) 1,4-Dioxane-d8 (S)

3.269min (-0.000) 3.48ng/uL

response 44620

Ion	Exp%	Act%
96.00	100	100
64.00	74.00	75.54
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062018\

Data File : BN001896.D

Acq On : 20 Jun 2018 20:54

Operator : JU/SJ

Sample : J3568-04

Misc :

ALS Vial : 19 Sample Multiplier: 1

Quant Time: Jun 21 01:12:06 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061918.M

Quant Title : SVOA CALIBRATION

QLast Update : Tue Jun 19 14:50:02 2018

Response via : Initial Calibration

Instrument :

BNA_N




ClientSampleId :

DAXP0

Manual Integrations
APPROVED

Sohil

6/21/2018 6:32:59 PM

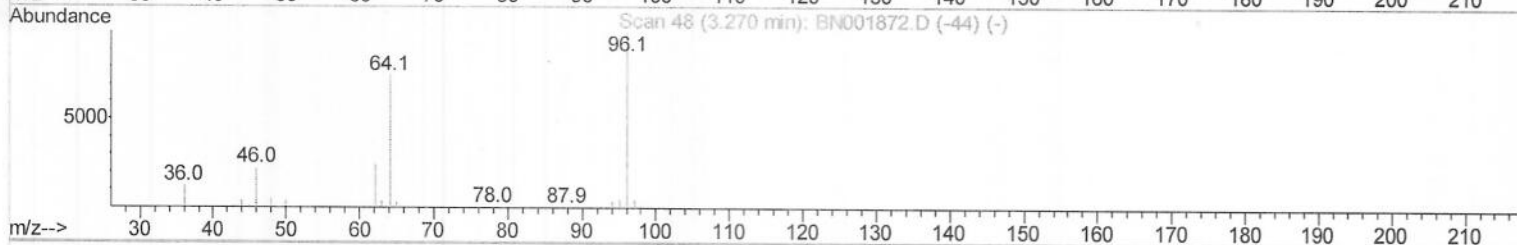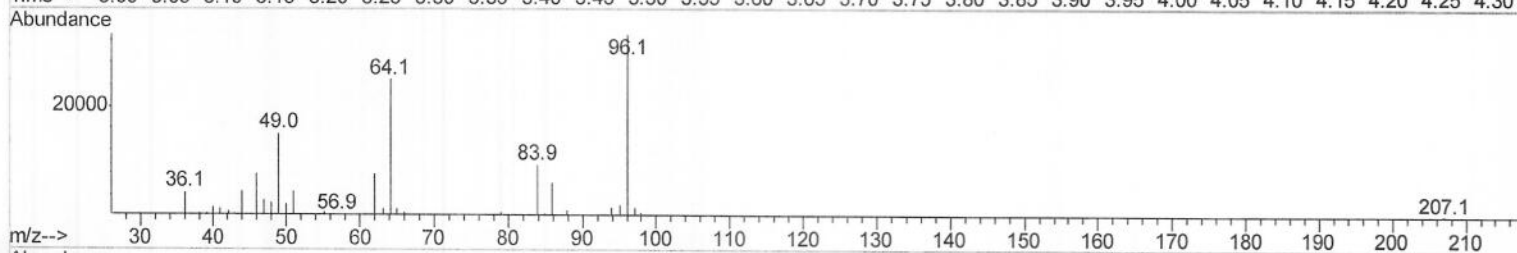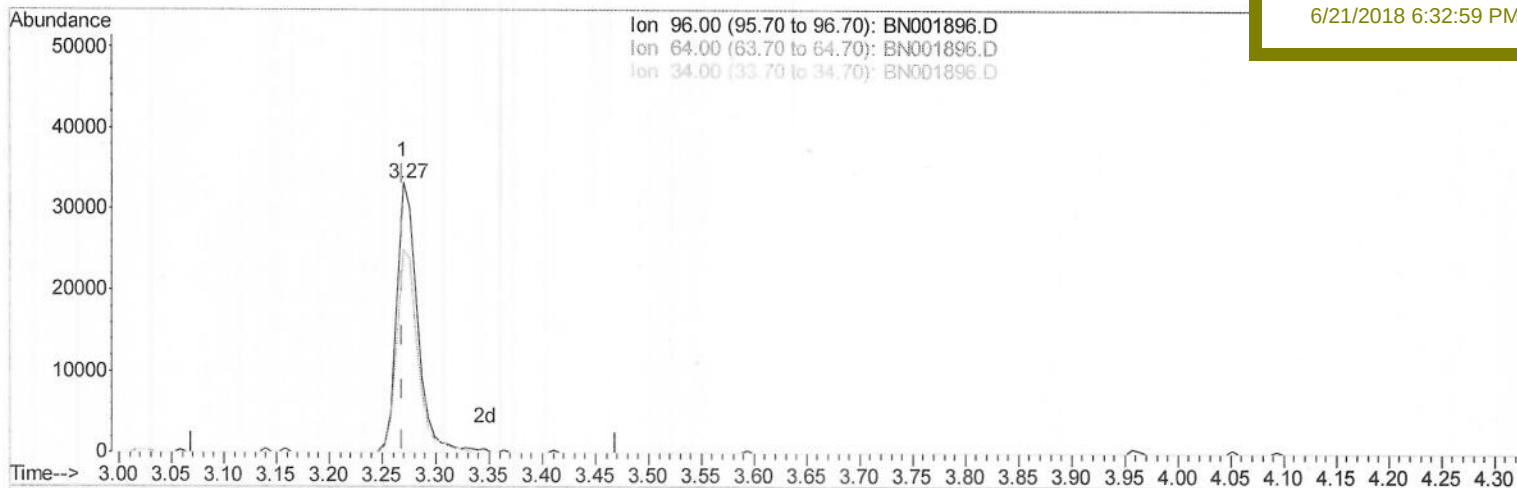

TIC: BN001896.D

(3) 1,4-Dioxane-d8 (S)

3.269min (-0.000) 3.53ng/uL m

response 45237

Ion	Exp%	Act%
96.00	100	100
64.00	74.00	75.54
34.00	0.00	0.00
0.00	0.00	0.00

57
07/03/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062018\
 Data File : BN001896.D
 Acq On : 20 Jun 2018 20:54
 Operator : JU/SJ
 Sample : J3568-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Quant Time: Jun 21 03:27:51 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 19 14:50:02 2018
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 DAXP0

Manual Integrations
 APPROVED

Sohil
 6/21/2018 6:32:59 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	556752	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	2513686	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.35	164	1484742	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.09	188	3184821	20.00	ng/ul	0.00
75) Chrysene-d12	21.29	240	2522395	20.00	ng/ul	0.00
83) Perylene-d12	23.52	264	2243767	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.27	96	45237m	3.53	ng/uL	0.00
5) Phenol-d5	6.89	99	135740	2.69	ng/ul	0.00
7) Bis-(2-Chloroethyl) ether-d	7.05	67	626893	20.16	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	379210	9.49	ng/ul	0.00
13) 4-Methylphenol-d8	8.41	113	592029	14.67	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	399811	21.42	ng/ul	0.00
22) 2-Nitrophenol-d4	9.58	143	435719	22.55	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.11	165	192596	4.67	ng/ul	0.00
29) 4-Chloroaniline-d4	10.62	131	672698	15.75	ng/ul	0.00
43) Dimethylphthalate-d6	13.76	166	2680501	21.38	ng/ul	0.00
46) Acenaphthylene-d8	14.03	160	439659	2.84	ng/ul	0.00
51) 4-Nitrophenol-d4	14.54	143	275728	11.94	ng/ul	0.00
57) Fluorene-d10	15.34	176	2187661	19.91	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.45	200	292799	16.88	ng/ul	0.00
70) Anthracene-d10	17.19	188	653843	4.25	ng/ul	0.00
76) Pyrene-d10	19.49	212	63178	0.50	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.37	264	26955	0.22	ng/ul	-0.01

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.80	163	1149657	9.329	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SJ
 07/03/18