

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN062018\
 Data File : BN001883.D
 Acq On : 20 Jun 2018 12:47
 Operator : JU/SJ
 Sample : J3568-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DAXN9

Quant Time: Jun 20 16:11:48 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 19 14:50:02 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	508003	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	2255704	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.35	164	1358395	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.09	188	2914368	20.00	ng/ul	0.00
75) Chrysene-d12	21.30	240	2306345	20.00	ng/ul	0.00
83) Perylene-d12	23.54	264	2095156	20.00	ng/ul	0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.28	96	41228	3.52	ng/uL	0.00
5) Phenol-d5	6.88	99	630	0.01	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	575164	20.27	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	1705	0.05	ng/ul	0.00
13) 4-Methylphenol-d8	8.41	113	4383	0.12	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	189656	11.32	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	150176	8.66	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	504	0.01	ng/ul	0.00
29) 4-Chloroaniline-d4	10.63	131	7061	0.18	ng/ul	0.00
43) Dimethylphthalate-d6	13.76	166	2385756	20.80	ng/ul	0.00
46) Acenaphthylene-d8	14.03	160	2998	0.02	ng/ul	0.00
51) 4-Nitrophenol-d4	14.55	143	1877	0.09	ng/ul	0.00
57) Fluorene-d10	15.34	176	62738	0.62	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.45	200	196997	12.41	ng/ul	0.00
70) Anthracene-d10	17.19	188	10844	0.08	ng/ul	0.00
76) Pyrene-d10	19.49	212	1216	0.01	ng/ul	0.00
87) Benzo(a)pyrene-d12	0.00	264	0d	0.00	ng/ul	


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.80	163	1098492	9.743	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062018\
Data File : BN001883.D
Acq On : 20 Jun 2018 12:47
Operator : JU/SJ
Sample : J3568-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DAXN9

Quant Time: Jun 20 16:11:48 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061918.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 19 14:50:02 2018
Response via : Initial Calibration

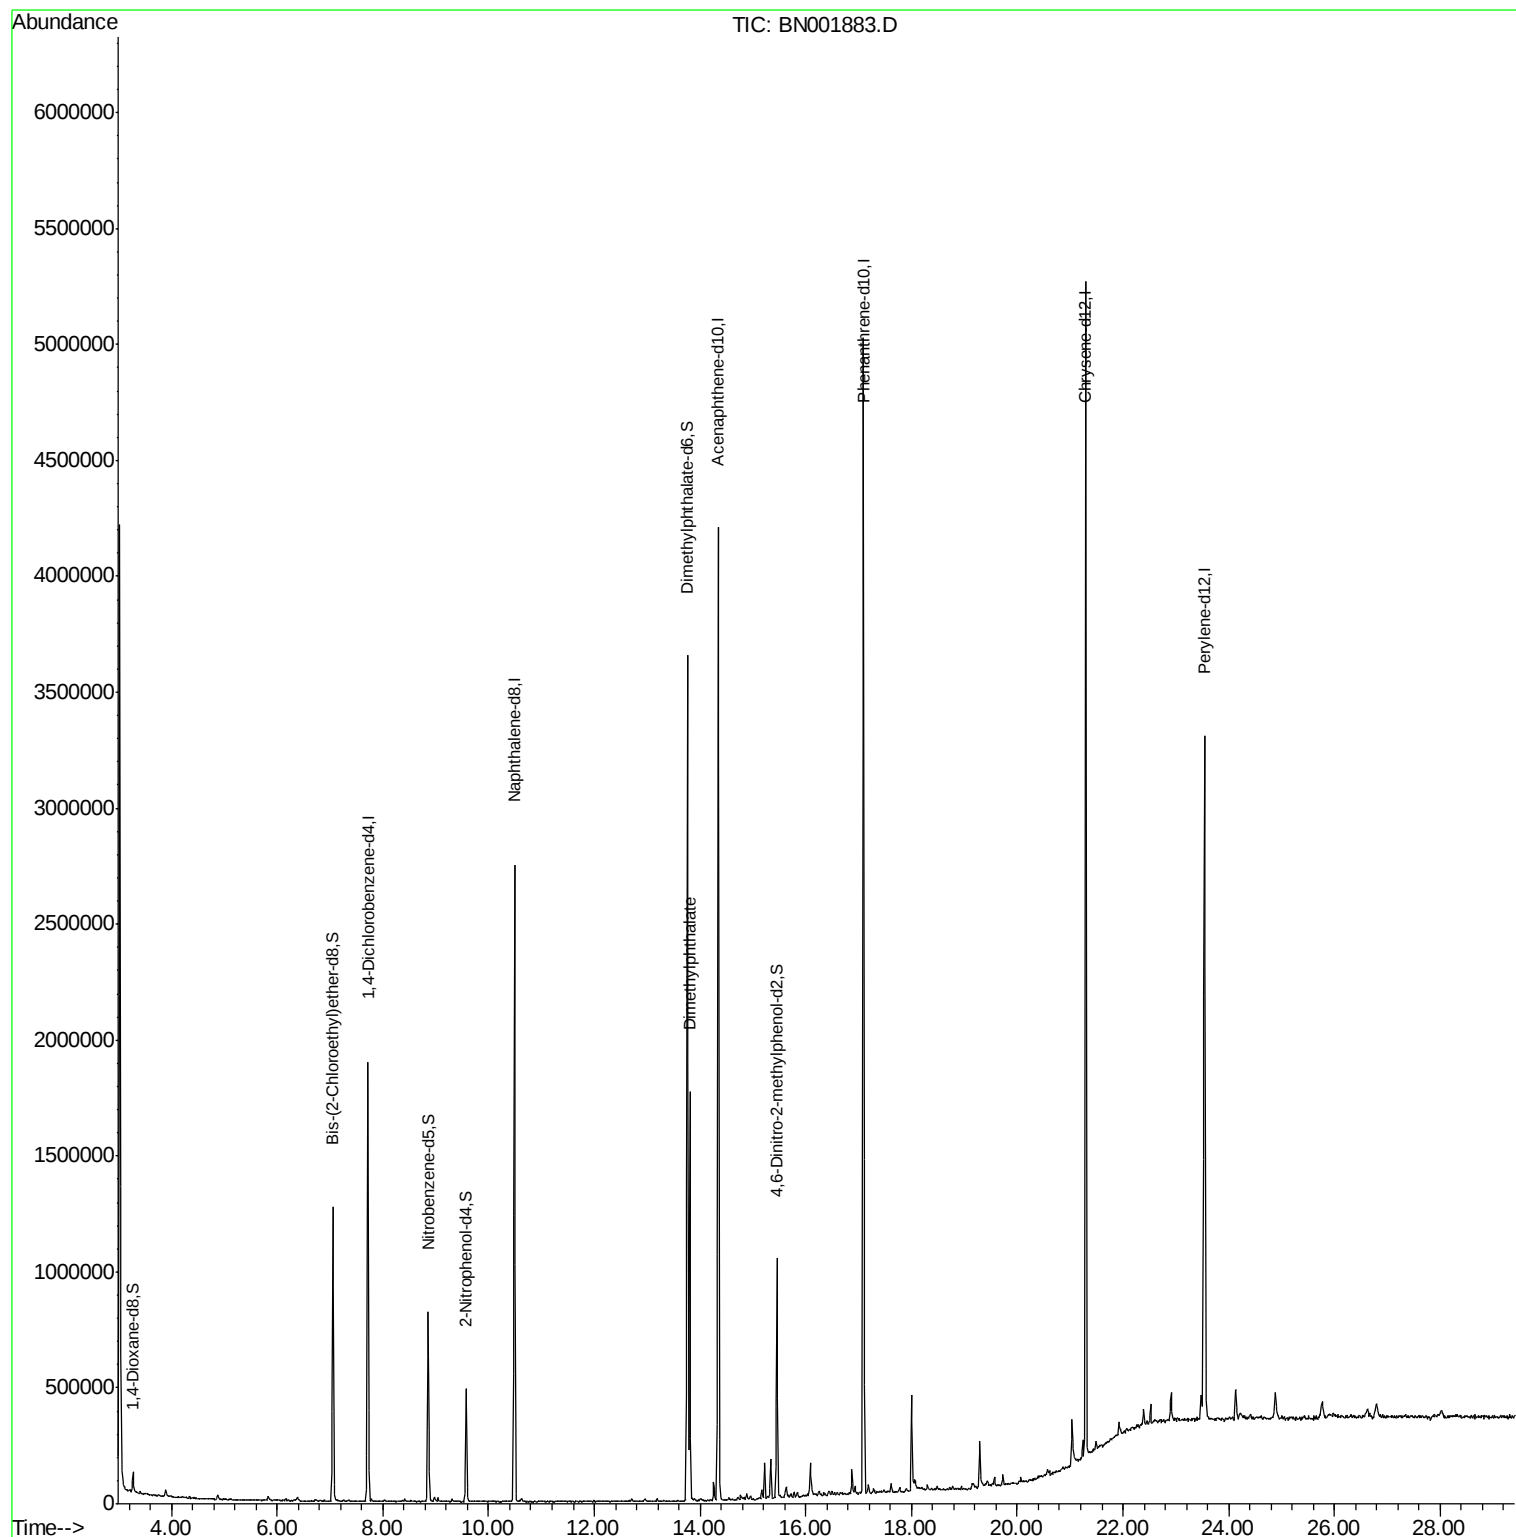

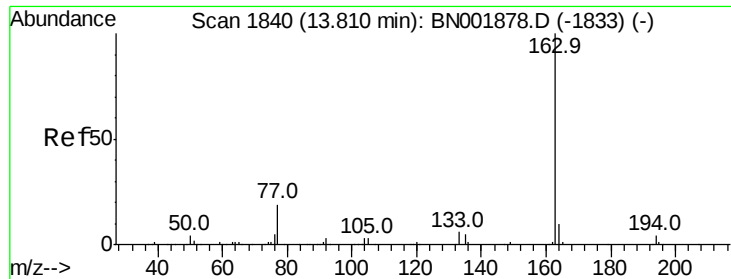

#44

Dimethylphthalate

Concen: 9.743 ng/ul

RT: 13.80 min Scan# 1839

Delta R.T. -0.01 min

Lab File: BN001883.D

Acq: 20 Jun 2018 12:47

Instrument :

BNA_N

ClientSampleId :

DAXN9


Tot Ion:163 Resp: 1098492

Ion Ratio Lower Upper

163 100

194 4.3 4.0 6.0

164 10.2 8.4 12.6

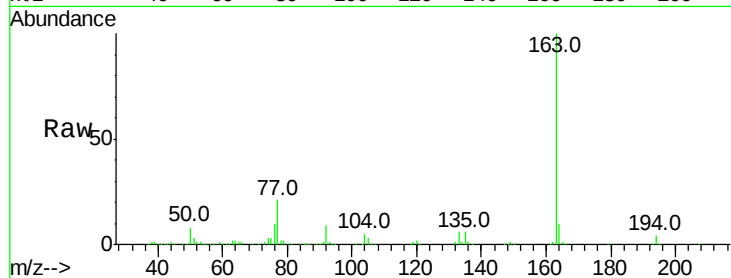

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

