

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062018\
 Data File : BN001884.D
 Acq On : 20 Jun 2018 13:22
 Operator : JU/SJ
 Sample : J3568-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DAXP1

Quant Time: Jun 20 16:14:30 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 19 14:50:02 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	525889	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	2334889	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.35	164	1430174	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.09	188	3232487	20.00	ng/ul	0.00
75) Chrysene-d12	21.29	240	2986174	20.00	ng/ul	0.00
83) Perylene-d12	23.53	264	2514038	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.28	96	36976	3.05	ng/uL	0.00
5) Phenol-d5	6.89	99	725	0.02	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	665799	22.67	ng/ul	0.00
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	1332	0.03	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	74048	4.27	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	47181	2.63	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	239	0.01	ng/ul	0.00
29) 4-Chloroaniline-d4	10.63	131	4120	0.10	ng/ul	0.00
43) Dimethylphthalate-d6	13.76	166	2816943	23.32	ng/ul	0.00
46) Acenaphthylene-d8	14.03	160	1491	0.01	ng/ul	0.00
51) 4-Nitrophenol-d4	14.55	143	715	0.03	ng/ul	0.00
57) Fluorene-d10	15.34	176	27049	0.26	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.45	200	249360	14.16	ng/ul	0.00
70) Anthracene-d10	17.19	188	7184	0.05	ng/ul	0.00
76) Pyrene-d10	19.49	212	981	0.01	ng/ul	0.00
87) Benzo(a)pyrene-d12	0.00	264	0d	0.00	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.80	163	1361197	11.467	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN062018\
Data File : BN001884.D
Acq On : 20 Jun 2018 13:22
Operator : JU/SJ
Sample : J3568-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DAXP1

Quant Time: Jun 20 16:14:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061918.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 19 14:50:02 2018
Response via : Initial Calibration

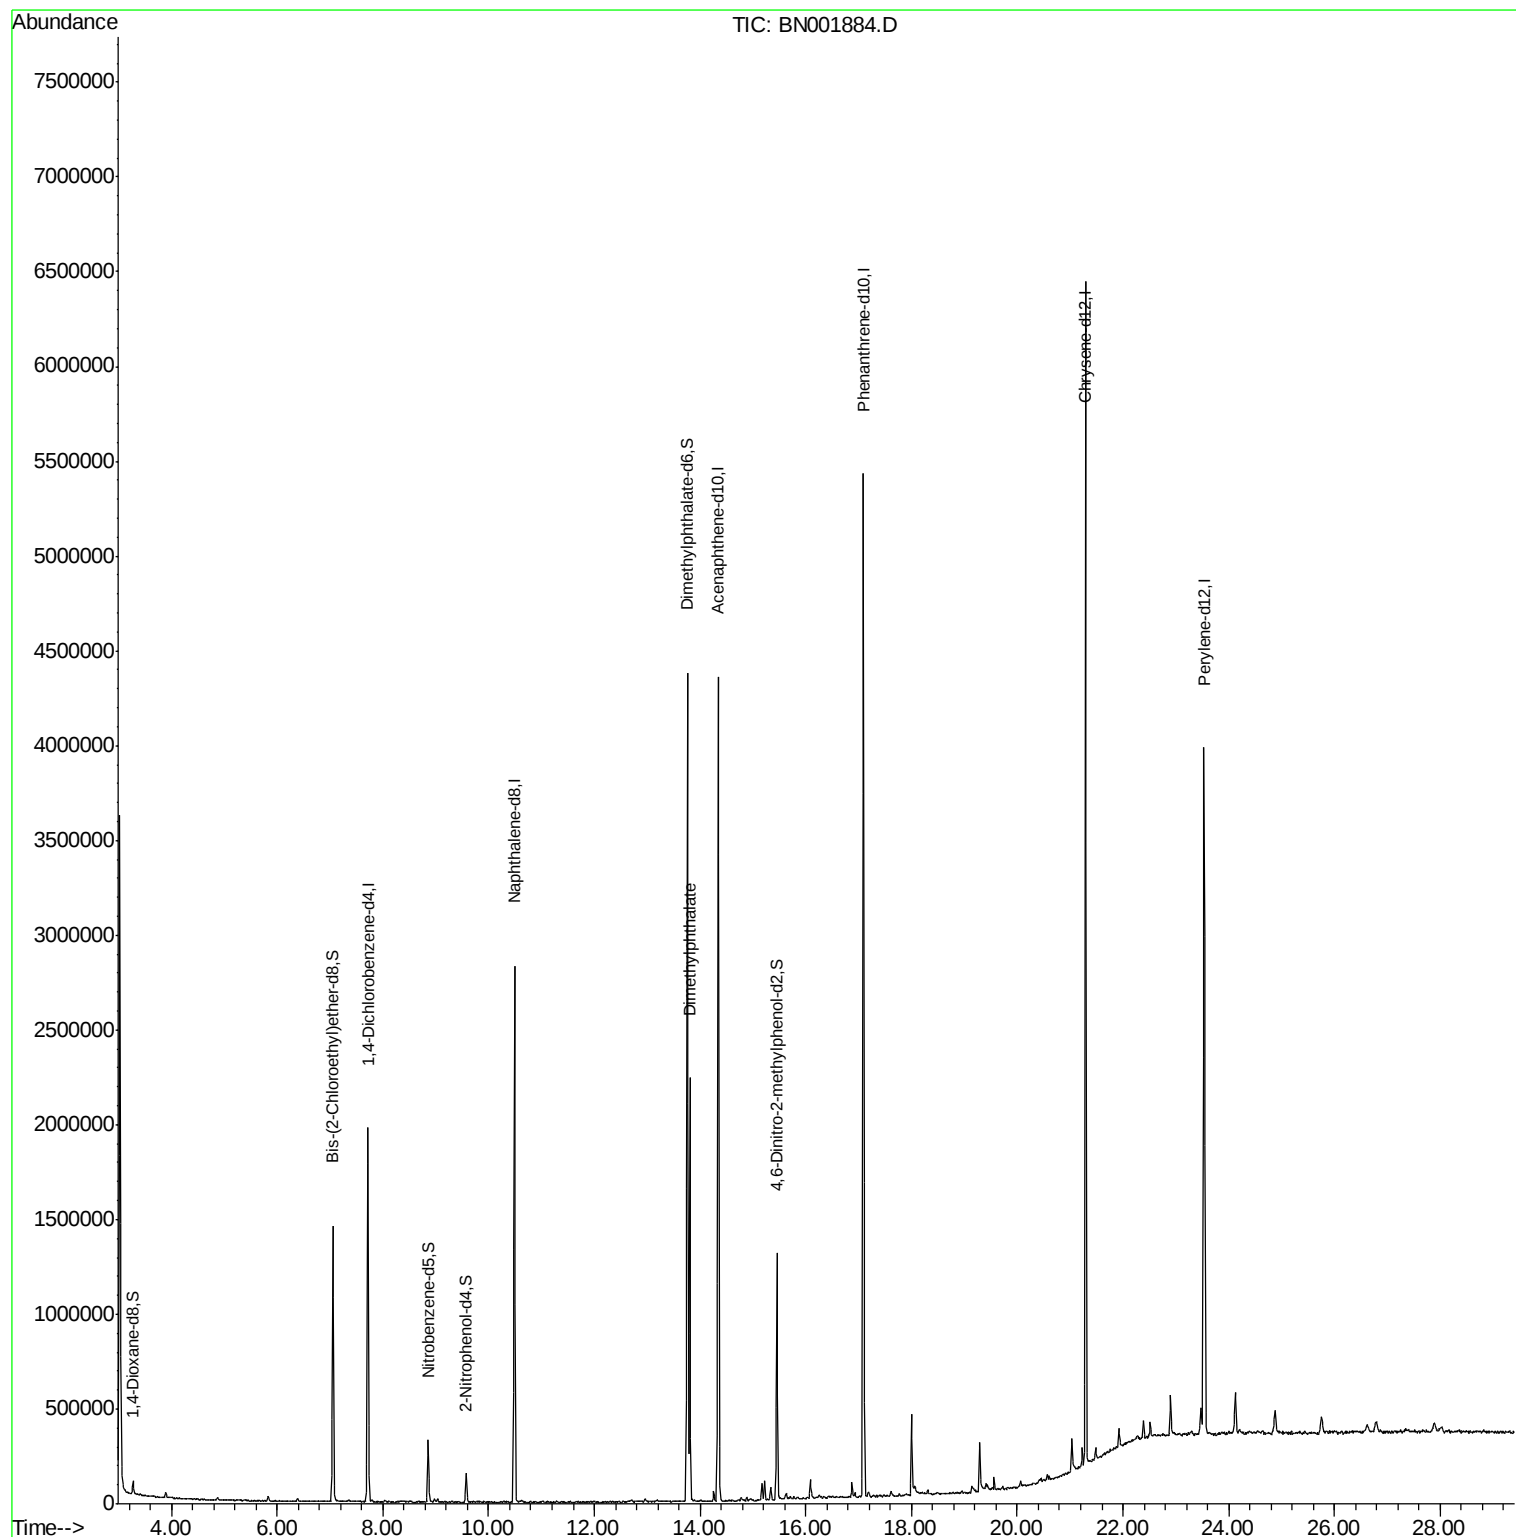

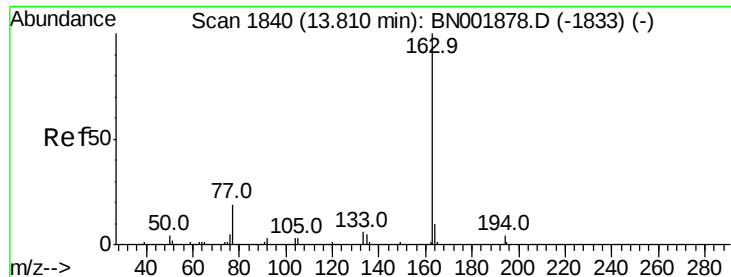

#44

Dimethylphthalate

Concen: 11.467 ng/ul

RT: 13.80 min Scan# 1839

Delta R.T. -0.01 min

Lab File: BN001884.D

Acq: 20 Jun 2018 13:22

Instrument :

BNA_N

ClientSampleId :

DAXP1


Tot Ion:163 Resp: 1361197

Ion Ratio Lower Upper

163 100

194 4.2 4.0 6.0

164 10.1 8.4 12.6

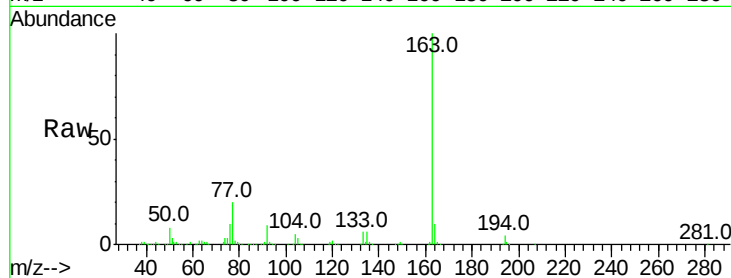

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

