
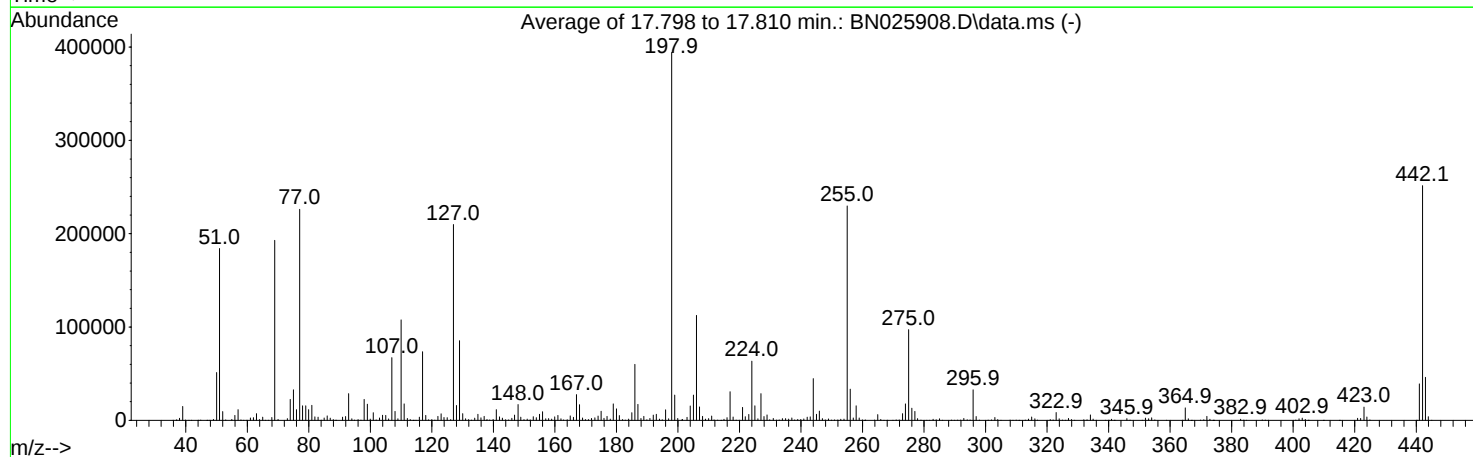


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062023\  
 Data File : BN025908.D  
 Acq On : 20 Jun 2023 07:59  
 Operator : MA/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN053123.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Jun 21 12:47:53 2023

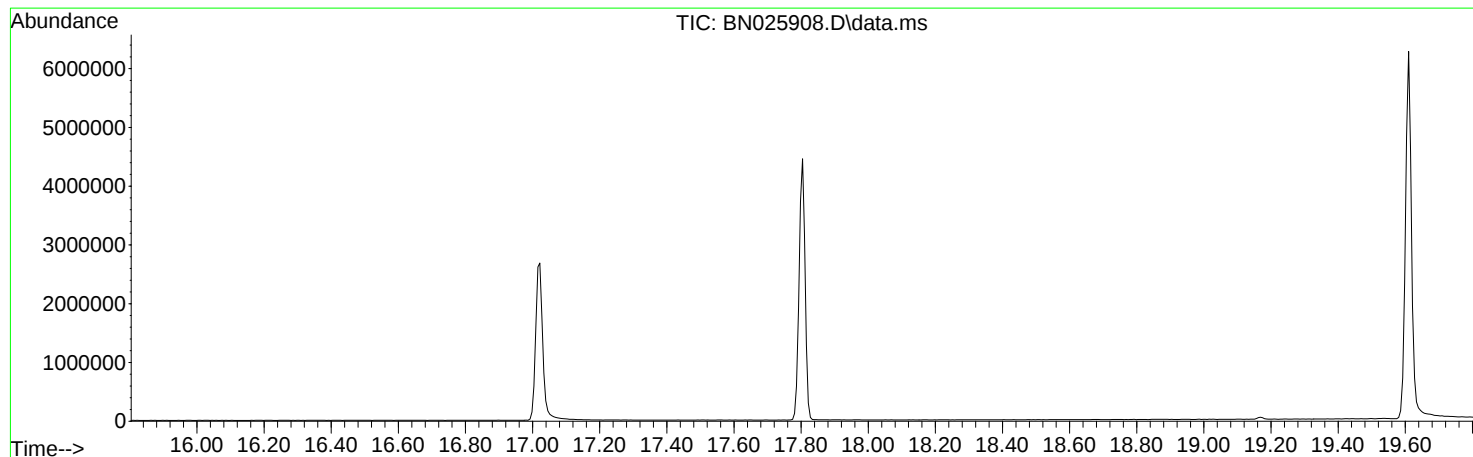

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 46.7         | 184104     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.6          | 3157       | PASS                |
| 69             | 198             | 0.00            | 100             | 48.9         | 192789     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 965        | PASS                |
| 127            | 198             | 10              | 80              | 53.2         | 209835     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.5          | 1776       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 394112     | PASS                |
| 199            | 198             | 5               | 9               | 6.9          | 27029      | PASS                |
| 275            | 198             | 10              | 60              | 24.7         | 97227      | PASS                |
| 365            | 198             | 1               | 100             | 3.4          | 13383      | PASS                |
| 441            | 198             | 0.01            | 100             | 9.9          | 39096      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 251413     | PASS                |
| 443            | 442             | 15              | 24              | 18.3         | 46123      | PASS                |

# DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 6/20/2023     | BNA_N            | <u>BN025908.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 1277680          | 20.839             |
| DDD           | 24307            | 20.398             |
| DDE           | 1389             | 19.892             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 25696         | 1303376          | 1.97               |
|               |                  |                    |

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062023\  
 Data File : BN025908.D  
 Acq On : 20 Jun 2023 07:59  
 Operator : MA/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Quant Time: Jun 20 08:56:52 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Jun 20 08:56:48 2023  
 Response via : Initial Calibration

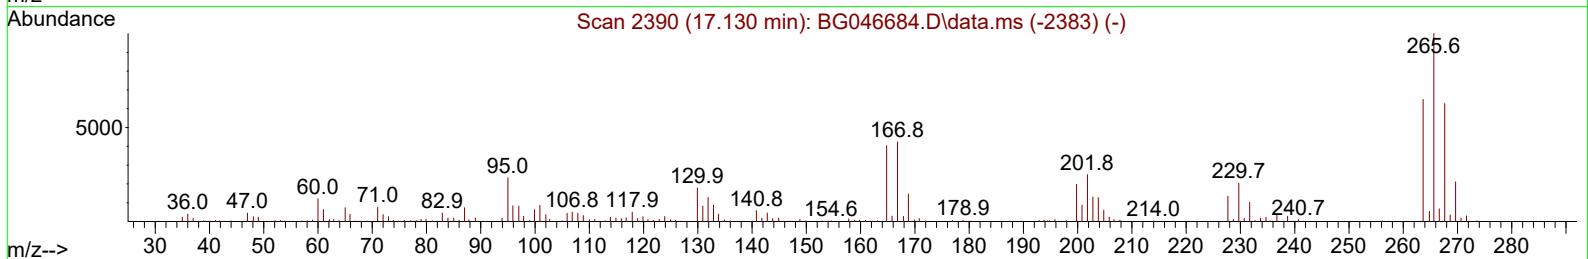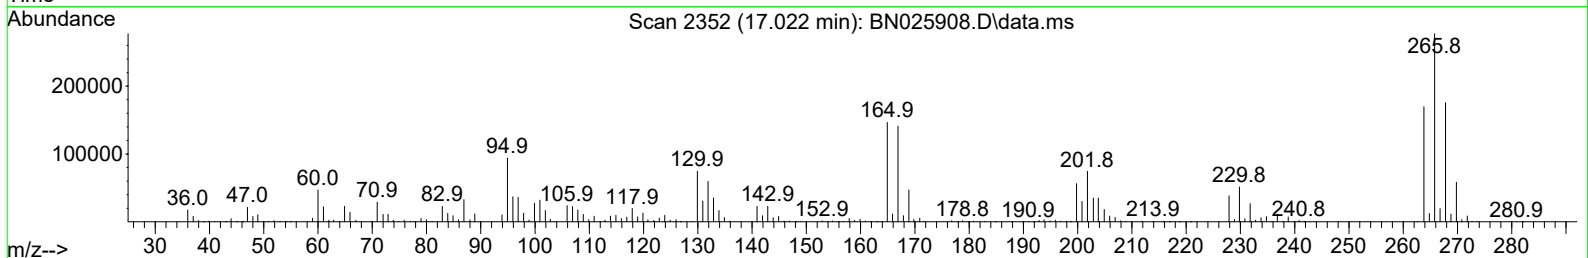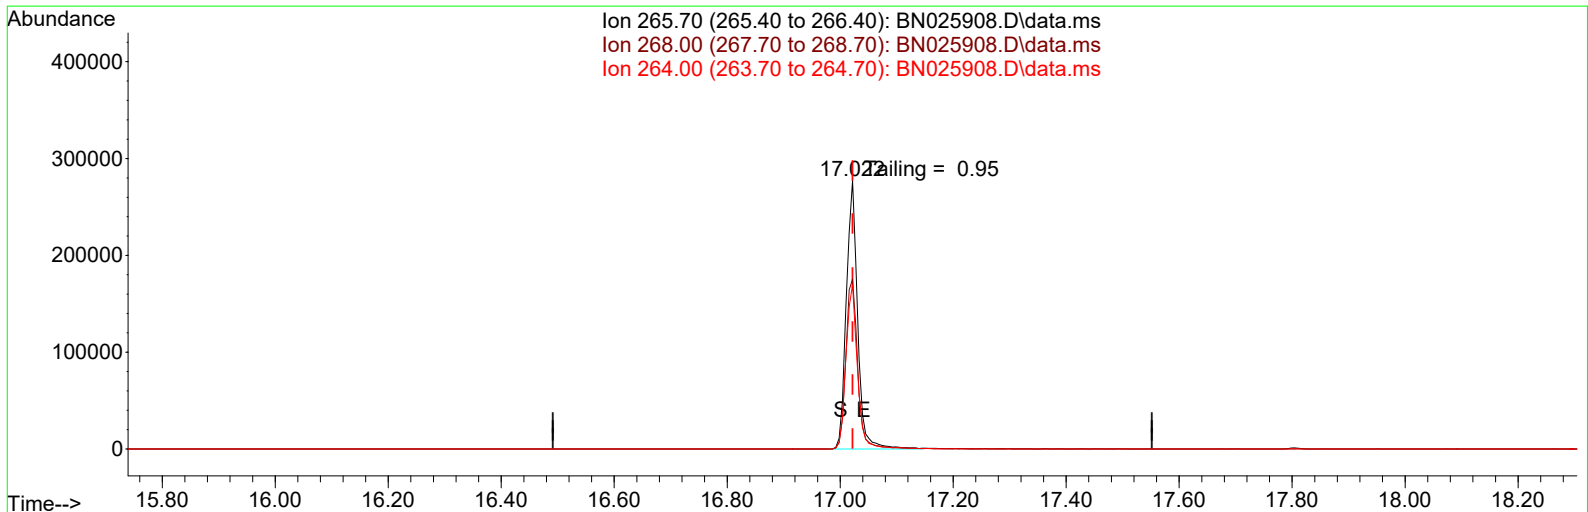

TIC: BN025908.D\data.ms

**(70) Pentachlorophenol (C)**

17.022min ( 0.000) 16362.82 ng




response 388059

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 63.31  |
| 264.00 | 61.60  | 61.21  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062023\  
 Data File : BN025908.D  
 Acq On : 20 Jun 2023 07:59  
 Operator : MA/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Quant Time: Jun 20 08:56:52 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Jun 20 08:56:48 2023  
 Response via : Initial Calibration

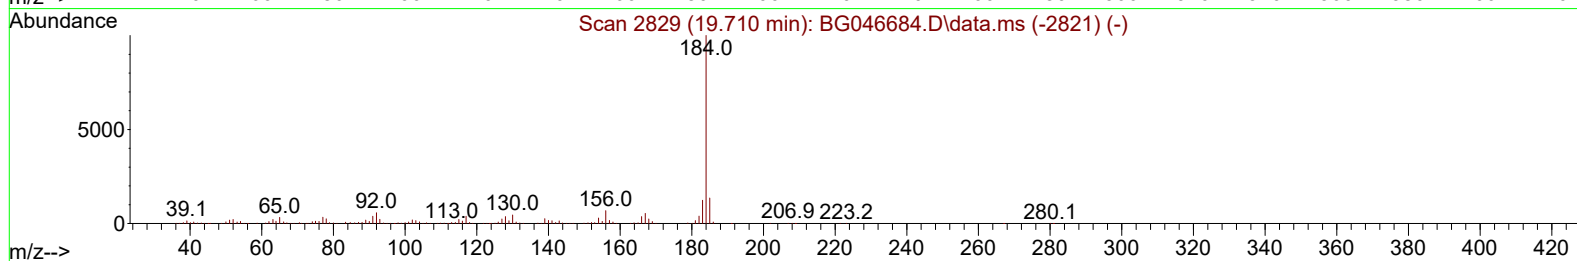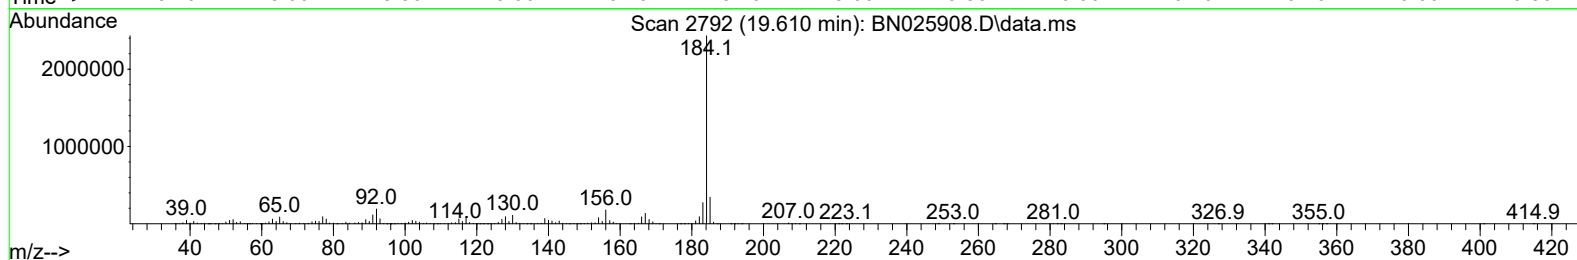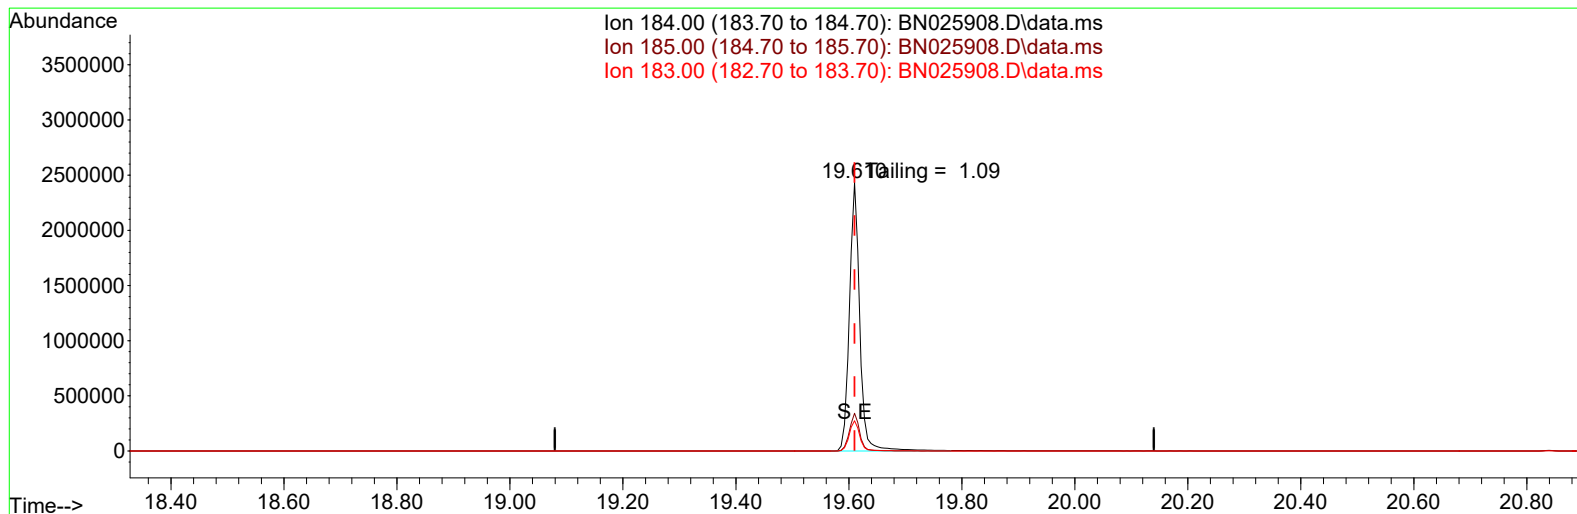

TIC: BN025908.D\data.ms

**(77) Benzidine**

19.610min ( 0.000) 0.00 ng

response 3104031

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 14.06  |
| 183.00 | 13.20  | 11.28  |
| 0.00   | 0.00   | 0.00   |