

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062024\
 Data File : BN032104.D
 Acq On : 20 Jun 2024 19:59
 Operator : MA/JU
 Sample : P2710-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4BM4

Quant Time: Jun 21 02:21:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 20 10:49:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.634	152	331919	20.000	ng/u1	0.00
20) Naphthalene-d8	10.416	136	1577759	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.281	164	1087703	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.028	188	2211004	20.000	ng/u1	0.00
79) Chrysene-d12	21.263	240	1534918	20.000	ng/u1	0.00
88) Perylene-d12	24.174	264	1410935	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	27789	3.464	ng/uL	0.00
4) Pyridine-d5	3.570	84	402877	17.838	ng/u1	0.00
7) Phenol-d5	6.816	99	606654	21.320	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.981	67	341386	20.511	ng/u1	0.00
11) 2-Chlorophenol-d4	7.169	132	524484	24.157	ng/u1	0.00
15) 4-Methylphenol-d8	8.346	113	546302	23.553	ng/u1	0.00
21) Nitrobenzene-d5	8.793	128	270877	22.454	ng/u1	0.00
24) 2-Nitrophenol-d4	9.510	143	299226	24.012	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.046	165	540895	23.250	ng/u1	0.00
31) 4-Chloroaniline-d4	10.563	131	764222	22.125	ng/u1	0.00
46) Dimethylphthalate-d6	13.698	166	1740182	22.965	ng/u1	0.00
49) Acenaphthylene-d8	13.975	160	1963893	22.540	ng/u1	0.00
54) 4-Nitrophenol-d4	14.504	143	279569	18.427	ng/u1	0.00
60) Fluorene-d10	15.275	176	1474773	23.002	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.410	200	208861	18.793	ng/u1	0.00
73) Anthracene-d10	17.128	188	2142487	22.634	ng/u1	0.00
81) Pyrene-d10	19.427	212	2259365	27.507	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.974	264	1554888	23.079	ng/u1	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.174	149	500267	7.215	ng/u1	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062024\
Data File : BN032104.D
Acq On : 20 Jun 2024 19:59
Operator : MA/JU
Sample : P2710-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BM4

Quant Time: Jun 21 02:21:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 20 10:49:40 2024
Response via : Initial Calibration

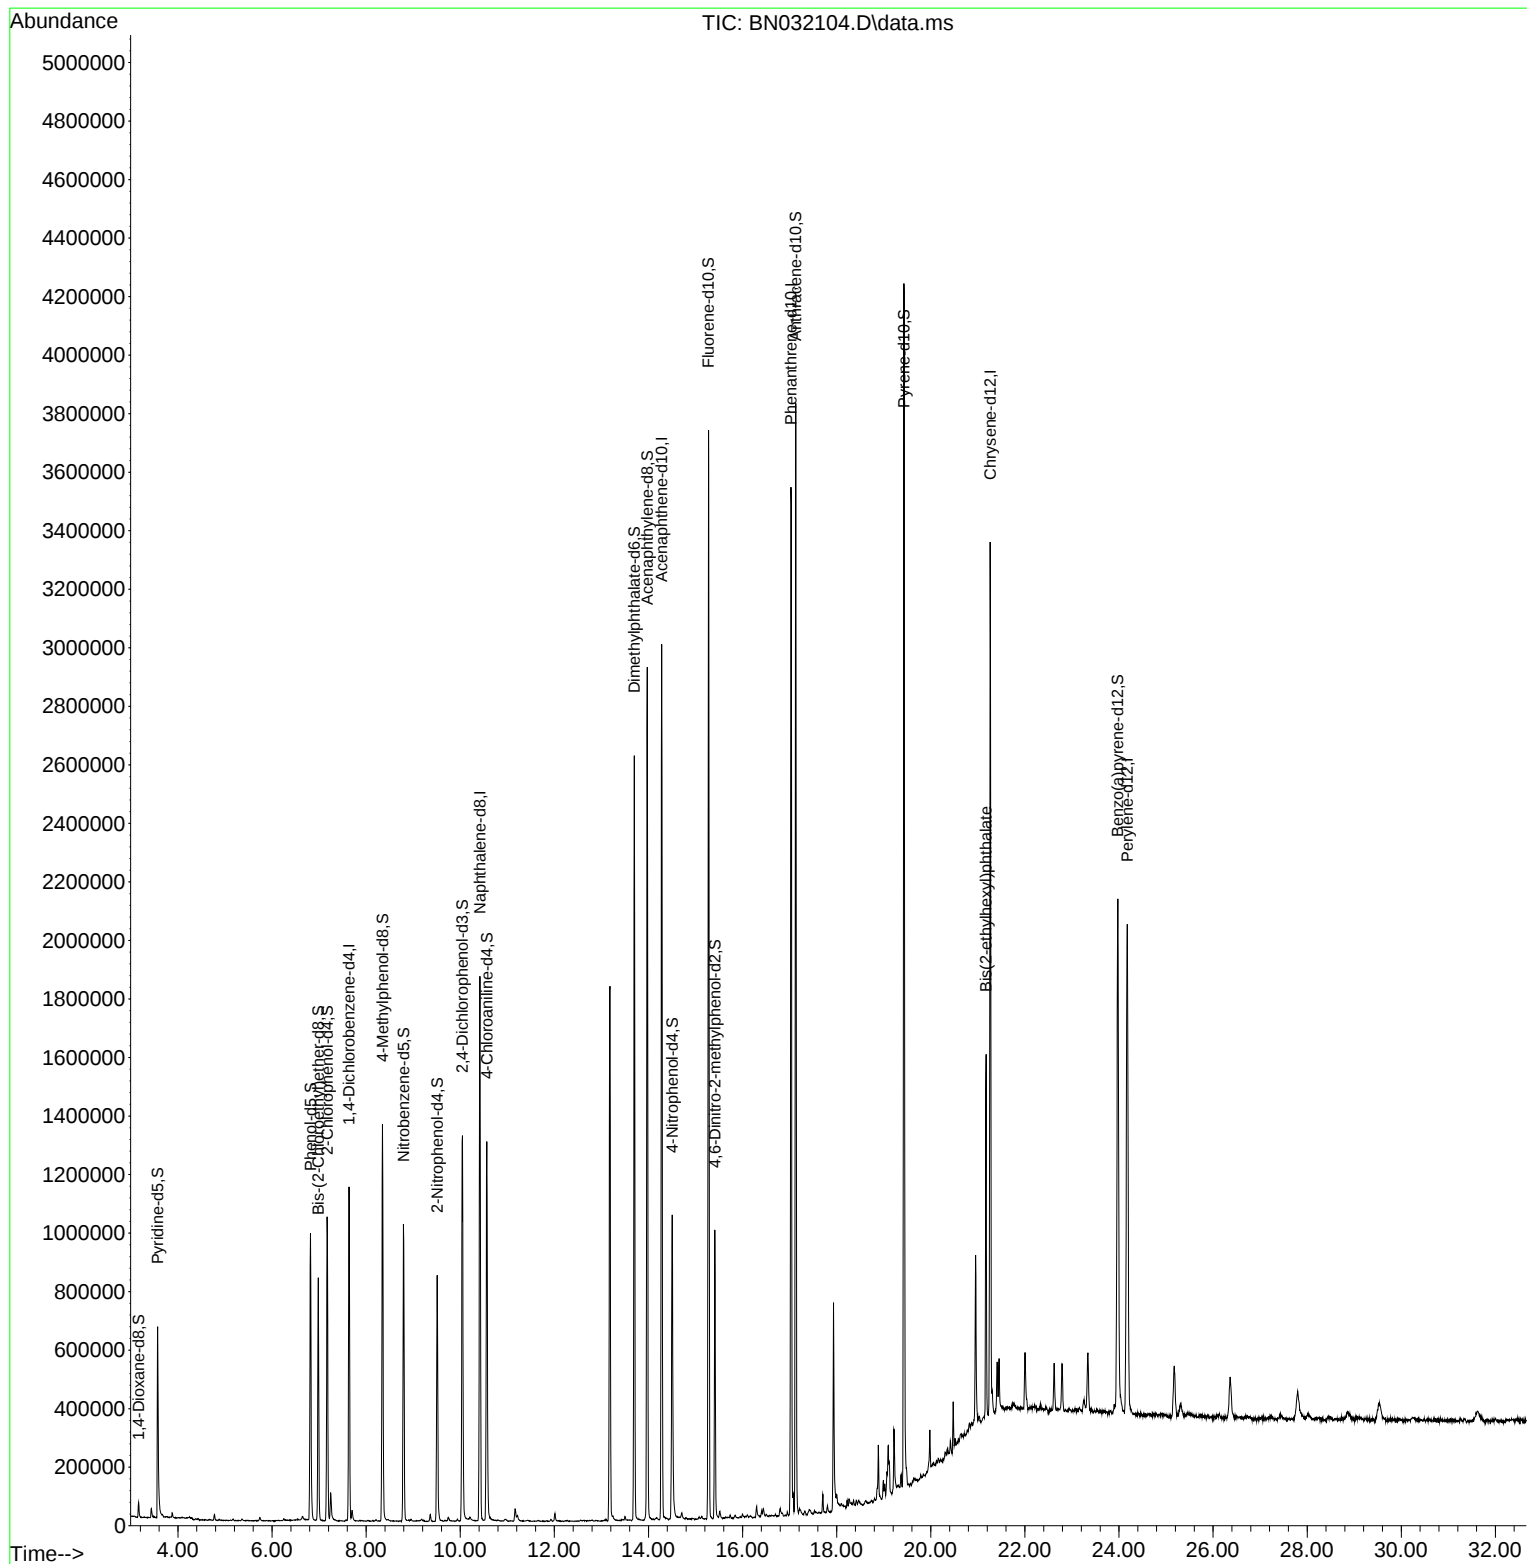

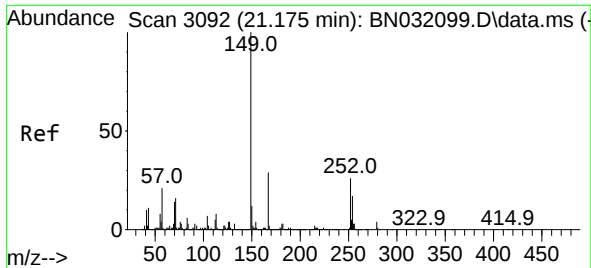

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 7.215 ng/ul
 RT: 21.174 min Scan# 3092
 Delta R.T. 0.000 min
 Lab File: BN032104.D
 Acq: 20 Jun 2024 19:59

Instrument :
 BNA_N
 ClientSampleId :
 A4BM4

Tgt Ion:149 Resp: 500267
 Ion Ratio Lower Upper
 149 100
 167 27.8 21.4 32.0
 279 4.2 3.3 4.9

