

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062024\
 Data File : BN032125.D
 Acq On : 21 Jun 2024 10:22
 Operator : MA/JU
 Sample : P2710-15
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4BM9

Quant Time: Jun 21 11:46:14 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 20 10:49:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.634	152	365248	20.000	ng/u1	0.00
20) Naphthalene-d8	10.416	136	1728131	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.281	164	1202727	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.034	188	2455275	20.000	ng/u1	0.00
79) Chrysene-d12	21.269	240	1807714	20.000	ng/u1	0.00
88) Perylene-d12	24.180	264	1693773	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	33734	3.821	ng/uL	0.00
4) Pyridine-d5	3.564	84	467711	18.819	ng/u1	0.00
7) Phenol-d5	6.817	99	731979	23.377	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.981	67	392264	21.417	ng/u1	0.00
11) 2-Chlorophenol-d4	7.169	132	643272	26.925	ng/u1	0.00
15) 4-Methylphenol-d8	8.346	113	637880	24.991	ng/u1	0.00
21) Nitrobenzene-d5	8.793	128	334651	25.327	ng/u1	0.00
24) 2-Nitrophenol-d4	9.510	143	374434	27.433	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.046	165	650679	25.535	ng/u1	0.00
31) 4-Chloroaniline-d4	10.563	131	898505	23.749	ng/u1	0.00
46) Dimethylphthalate-d6	13.698	166	2035774	24.296	ng/u1	0.00
49) Acenaphthylene-d8	13.975	160	2358286	24.478	ng/u1	0.00
54) 4-Nitrophenol-d4	14.510	143	332109	19.796	ng/u1	0.00
60) Fluorene-d10	15.275	176	1740087	24.544	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.416	200	192615	15.607	ng/u1	0.00
73) Anthracene-d10	17.134	188	2650052	25.211	ng/u1	0.00
81) Pyrene-d10	19.433	212	2759588	28.527	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.980	264	1995102	24.668	ng/u1	0.00
Target Compounds						
					Qvalue	
80) Fluoranthene	19.098	202	164711	1.425	ng/u1	99
82) Pyrene	19.463	202	154747	1.305	ng/u1	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062024\
Data File : BN032125.D
Acq On : 21 Jun 2024 10:22
Operator : MA/JU
Sample : P2710-15
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4BM9

Quant Time: Jun 21 11:46:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 20 10:49:40 2024
Response via : Initial Calibration




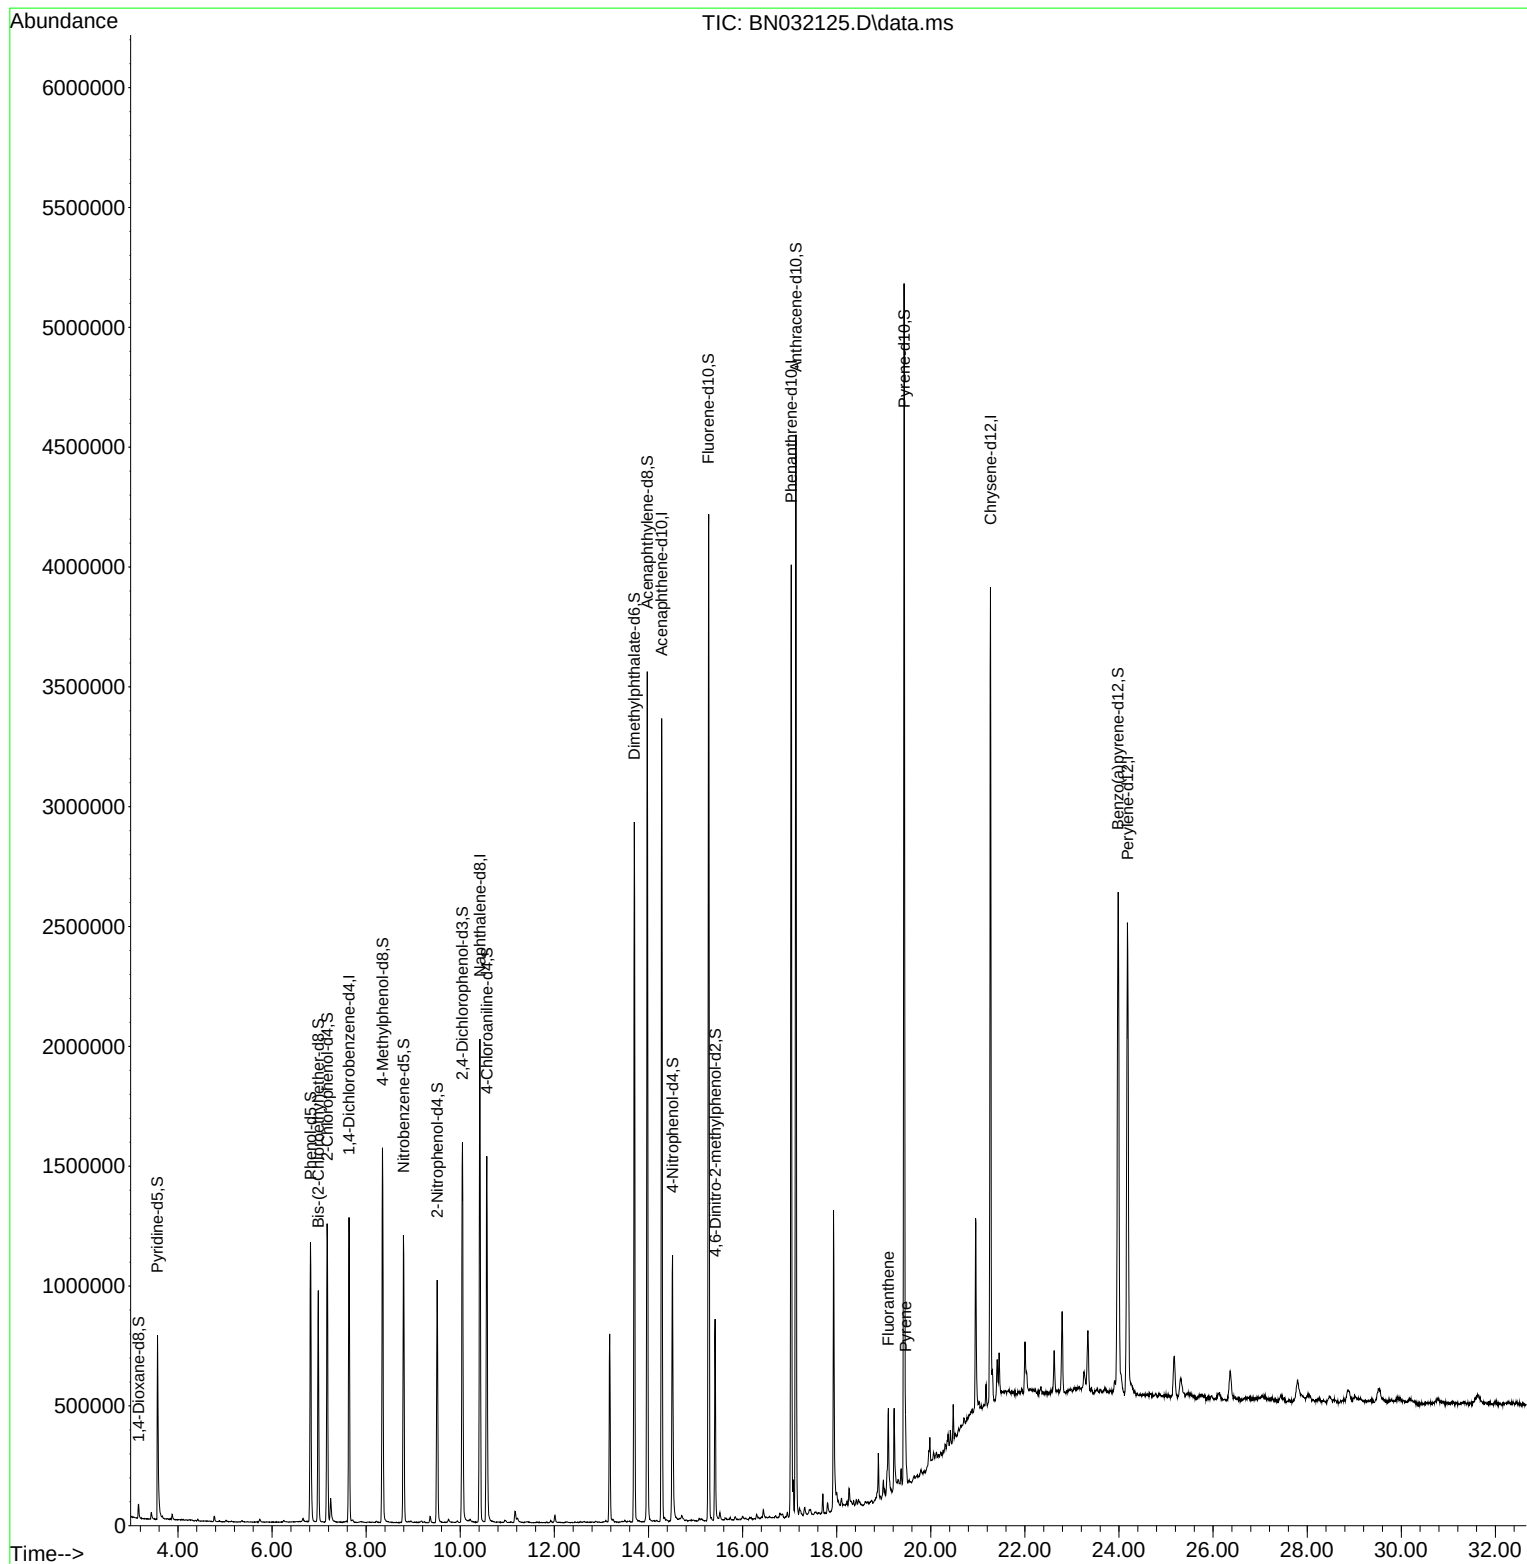


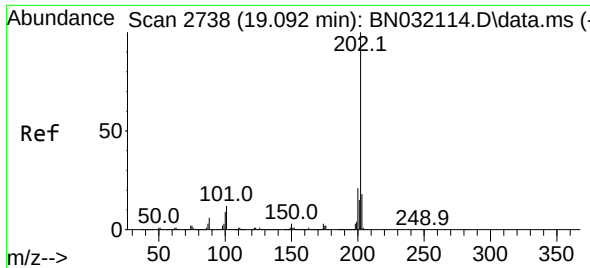

#80
Fluoranthene
Concen: 1.425 ng/ul
RT: 19.098 min Scan# 21
Delta R.T. 0.000 min
Lab File: BN032125.D
Acq: 21 Jun 2024 10:22

Instrument :
BNA_N
ClientSampleId :
A4BM9

Tgt Ion:202 Resp: 164711
Ion Ratio Lower Upper
202 100
101 12.6 10.3 15.5
100 9.4 8.0 12.0

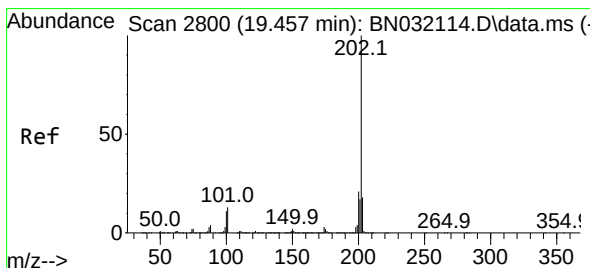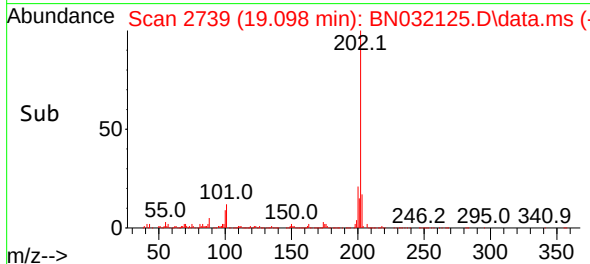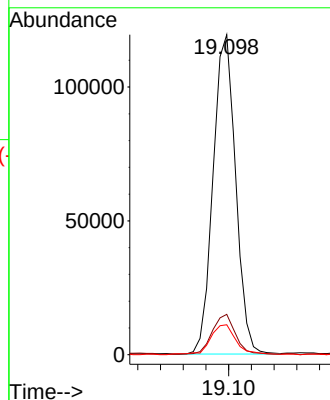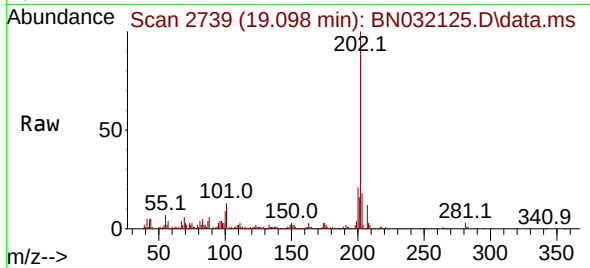

#82
Pyrene
Concen: 1.305 ng/ul
RT: 19.463 min Scan# 2801
Delta R.T. 0.000 min
Lab File: BN032125.D
Acq: 21 Jun 2024 10:22

Tgt Ion:202 Resp: 154747
Ion Ratio Lower Upper
202 100
101 12.8 12.6 18.8
100 11.4 10.2 15.2

