

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062024\
 Data File : BN032094.D
 Acq On : 20 Jun 2024 10:12
 Operator : MA/JU
 Sample : PB161544BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK544

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN032094.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	26	30	39	rVB	52352	75077	1.12%	0.116%
2	3.564	95	98	122	rBV	584579	1001940	15.00%	1.554%
3	3.875	148	151	155	rVB2	9612	13358	0.20%	0.021%
4	6.816	643	651	661	rBV	873941	1431483	21.43%	2.220%
5	6.981	672	679	688	rVB	754705	1188637	17.79%	1.843%
6	7.169	705	711	724	rBV	892717	1456623	21.80%	2.259%
7	7.634	783	790	807	rBV	716592	1193631	17.87%	1.851%
8	8.346	903	911	926	rBV	1184175	1973703	29.54%	3.060%
9	8.793	978	987	998	rBV	882317	1482979	22.20%	2.300%
10	9.510	1102	1109	1125	rBV	725889	1229435	18.40%	1.906%
11	10.046	1192	1200	1218	rBV	1144723	2077258	31.09%	3.221%
12	10.416	1254	1263	1274	rBV	1159125	1959443	29.33%	3.038%
13	10.563	1279	1288	1306	rBV	992644	1797699	26.91%	2.788%
14	12.022	1529	1536	1547	rVB2	15016	42832	0.64%	0.066%
15	13.251	1740	1745	1749	rVB7	4436	6844	0.10%	0.011%
16	13.698	1814	1821	1836	rBV	2413220	3394585	50.81%	5.264%
17	13.975	1861	1868	1879	rBV	2674854	4103909	61.43%	6.364%
18	14.281	1913	1920	1931	rBV	2044180	2987357	44.72%	4.632%
19	14.498	1951	1957	1978	rBV	949396	1611688	24.12%	2.499%
20	15.281	2082	2090	2102	rBV	3455701	5234470	78.35%	8.117%
21	15.410	2106	2112	2126	rBV	921105	1356150	20.30%	2.103%
22	15.516	2126	2130	2135	rVB2	18225	30293	0.45%	0.047%
23	15.786	2172	2176	2182	rBV5	6779	12920	0.19%	0.020%
24	16.063	2219	2223	2227	rVB3	11351	15318	0.23%	0.024%
25	16.704	2328	2332	2338	rBV7	5531	11174	0.17%	0.017%
26	16.816	2347	2351	2355	rBV2	7121	9721	0.15%	0.015%
27	17.028	2381	2387	2397	rBV	2526175	3669257	54.92%	5.690%
28	17.128	2398	2404	2418	rBV2	3856007	5799302	86.81%	8.992%
29	17.704	2498	2502	2508	rBV7	9038	17074	0.26%	0.026%
30	18.992	2716	2721	2725	rBV	52246	73987	1.11%	0.115%
31	19.063	2729	2733	2740	rVV	43405	63977	0.96%	0.099%
32	19.427	2789	2795	2807	rBV	4660775	6680661	100.00%	10.359%
33	21.263	3101	3107	3114	rBV	2559404	3719235	55.67%	5.767%
34	23.974	3559	3568	3582	rVB2	2267970	5458540	81.71%	8.464%
35	24.174	3593	3602	3613	rVB	1345920	3310392	49.55%	5.133%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062024\
Data File : BN032094.D
Acq On : 20 Jun 2024 10:12
Operator : MA/JU
Sample : PB161544BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK544

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 64490952

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062024\
Data File : BN032094.D
Acq On : 20 Jun 2024 10:12
Operator : MA/JU
Sample : PB161544BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK544

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

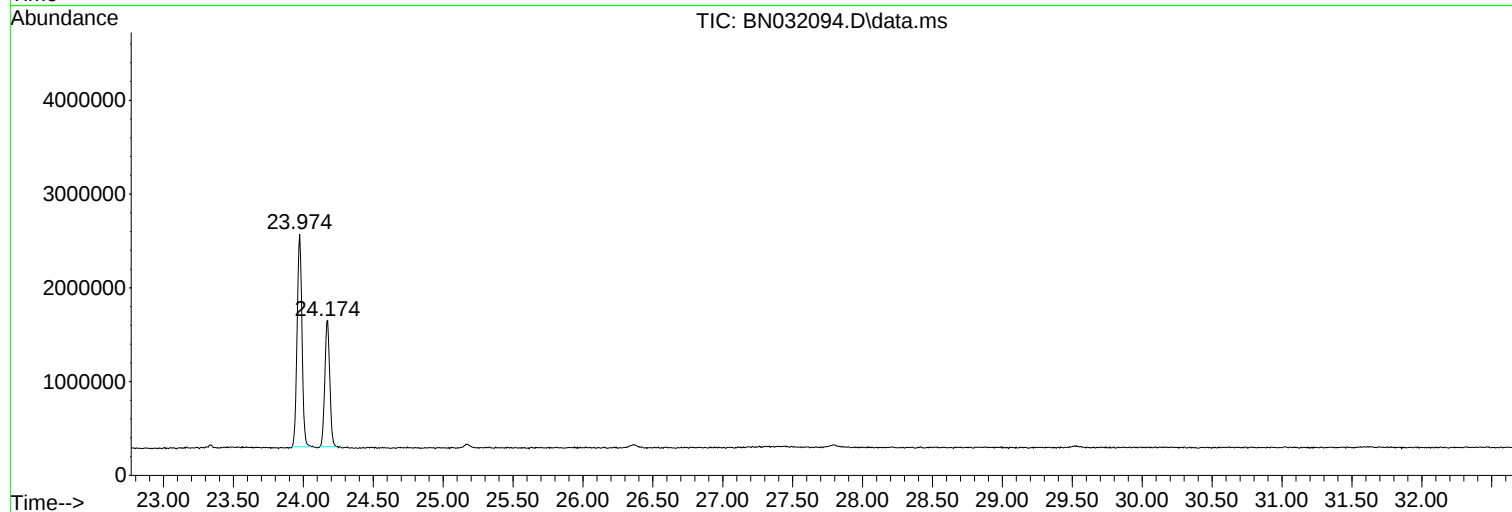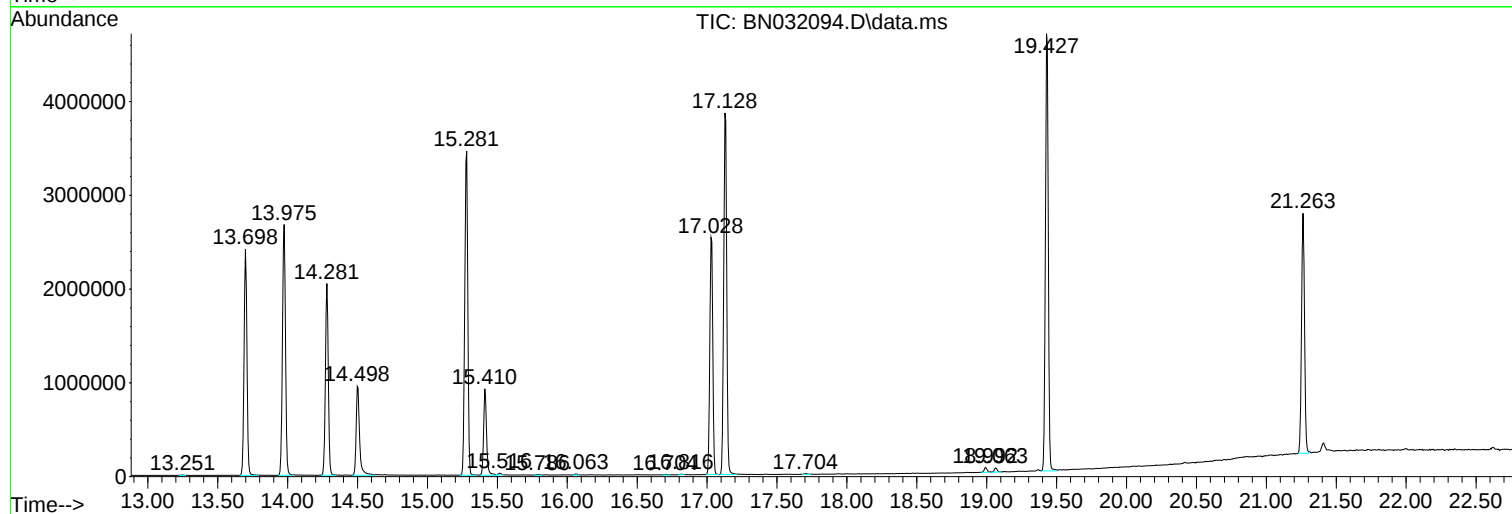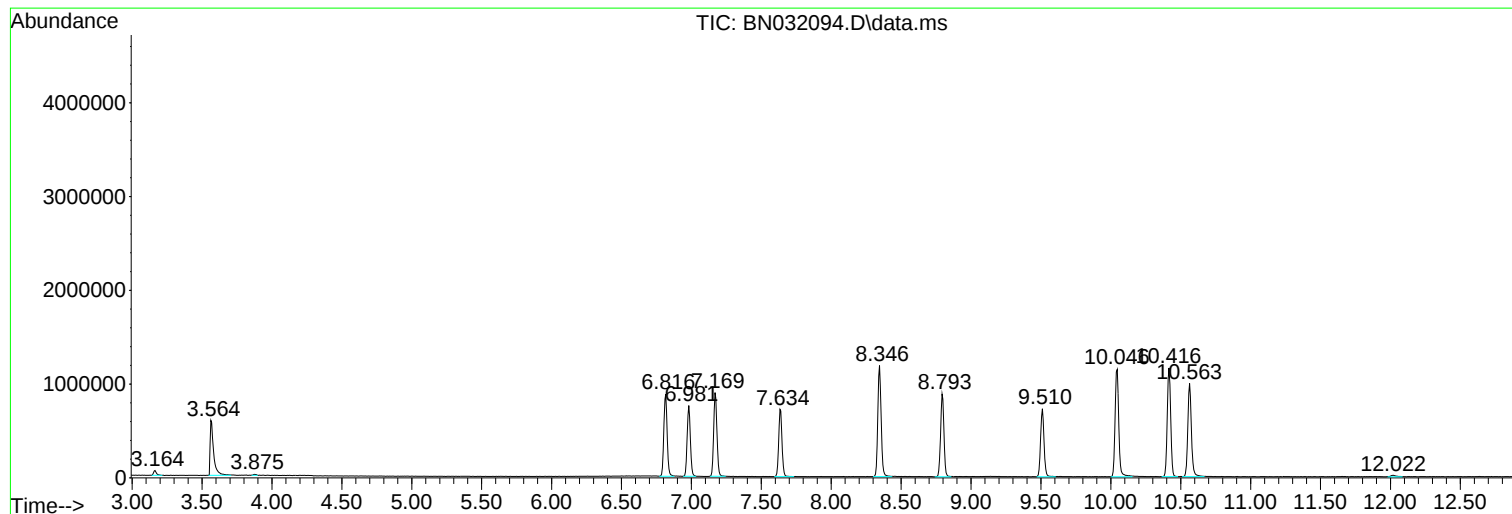

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062024\
Data File : BN032094.D
Acq On : 20 Jun 2024 10:12
Operator : MA/JU
Sample : PB161544BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK544

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062024\
Data File : BN032094.D
Acq On : 20 Jun 2024 10:12
Operator : MA/JU
Sample : PB161544BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK544

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------