

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062024\
 Data File : BN032100.D
 Acq On : 20 Jun 2024 17:21
 Operator : MA/JU
 Sample : PB161390BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK390

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN032100.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	26	30	35	rBV	64608	85639	1.13%	0.102%
2	3.564	95	98	116	rBV	824856	1305472	17.18%	1.551%
3	3.875	147	151	156	rBV2	14865	21102	0.28%	0.025%
4	6.816	643	651	668	rVV	1117358	1812848	23.86%	2.153%
5	6.981	672	679	691	rVB	957848	1483471	19.52%	1.762%
6	7.169	704	711	725	rBV	1170573	1921729	25.29%	2.283%
7	7.634	784	790	802	rVB	1138624	1889378	24.87%	2.244%
8	8.346	903	911	928	rBV	1508642	2515547	33.11%	2.988%
9	8.793	978	987	1001	rBV	1159679	1928901	25.39%	2.291%
10	9.510	1100	1109	1118	rBV	962514	1624419	21.38%	1.929%
11	10.046	1189	1200	1217	rBV	1463950	2653723	34.93%	3.152%
12	10.416	1255	1263	1271	rBV	1882582	3175167	41.79%	3.771%
13	10.563	1279	1288	1301	rBV	1600448	2796615	36.81%	3.322%
14	12.010	1528	1534	1544	rVB	25569	51035	0.67%	0.061%
15	13.245	1735	1744	1750	rBV7	6008	11822	0.16%	0.014%
16	13.698	1813	1821	1830	rBV	3060359	4288794	56.45%	5.094%
17	13.975	1859	1868	1886	rBV	3451668	5251289	69.11%	6.237%
18	14.281	1913	1920	1928	rBV	3263353	4830377	63.57%	5.737%
19	14.404	1937	1941	1947	rVB8	4745	8541	0.11%	0.010%
20	14.504	1950	1958	1978	rBV	1219427	2050607	26.99%	2.436%
21	15.281	2083	2090	2105	rVB	4290918	6399351	84.22%	7.601%
22	15.410	2105	2112	2126	rBV	1202099	1774435	23.35%	2.108%
23	15.516	2126	2130	2136	rVB3	25247	41342	0.54%	0.049%
24	16.710	2329	2333	2336	rVB4	8080	9064	0.12%	0.011%
25	16.822	2347	2352	2357	rBV3	9317	13586	0.18%	0.016%
26	17.034	2381	2388	2397	rBV	3887496	5752344	75.71%	6.832%
27	17.128	2397	2404	2421	rVV	4555171	6967802	91.71%	8.276%
28	17.704	2498	2502	2508	rBV7	8040	11631	0.15%	0.014%
29	17.933	2537	2541	2544	rBV6	6603	11050	0.15%	0.013%
30	18.992	2716	2721	2726	rBV2	66599	94765	1.25%	0.113%
31	19.063	2729	2733	2739	rVV	58531	82489	1.09%	0.098%
32	19.369	2782	2785	2788	rBV2	27781	31142	0.41%	0.037%
33	19.433	2789	2796	2807	rVV	5394361	7597954	100.00%	9.025%
34	21.263	3101	3107	3118	rBV2	3532964	5287131	69.59%	6.280%
35	21.410	3128	3132	3136	rBV	112205	172278	2.27%	0.205%
36	23.974	3560	3568	3581	rVB2	2283116	5584548	73.50%	6.633%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062024\
Data File : BN032100.D
Acq On : 20 Jun 2024 17:21
Operator : MA/JU
Sample : PB161390BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK390

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Title : SVOA CALIBRATION

37 24.174 3594 3602 3615 rVB 1892031 4653582 61.25% 5.527%




Sum of corrected areas: 84190970

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062024\
Data File : BN032100.D
Acq On : 20 Jun 2024 17:21
Operator : MA/JU
Sample : PB161390BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK390

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

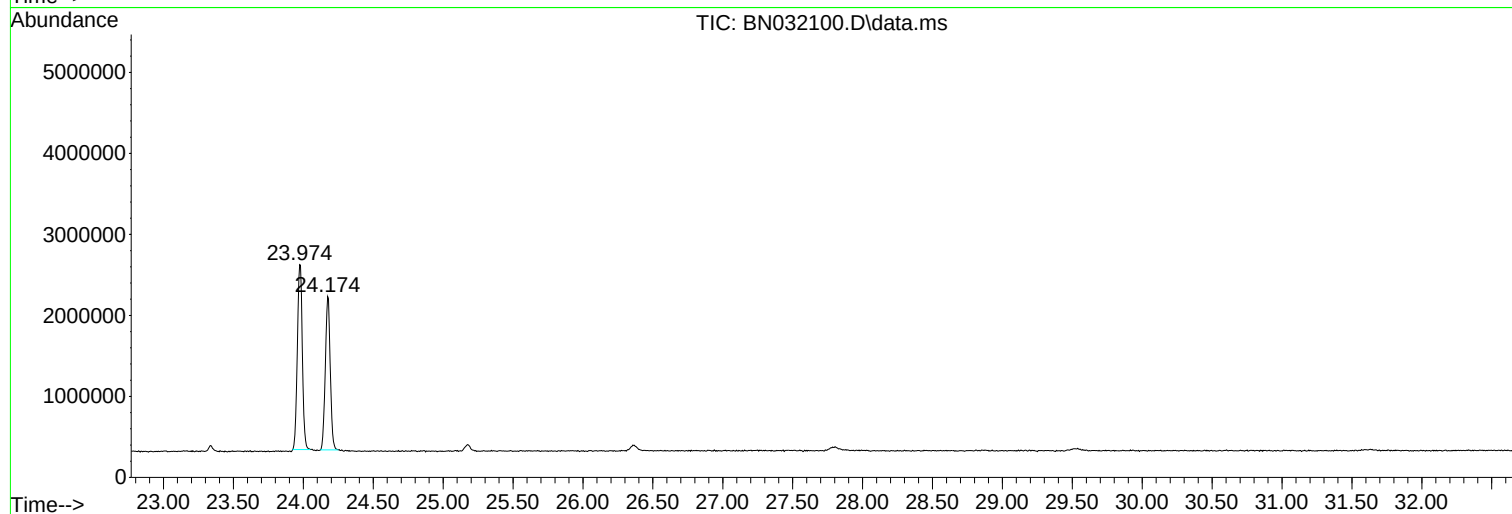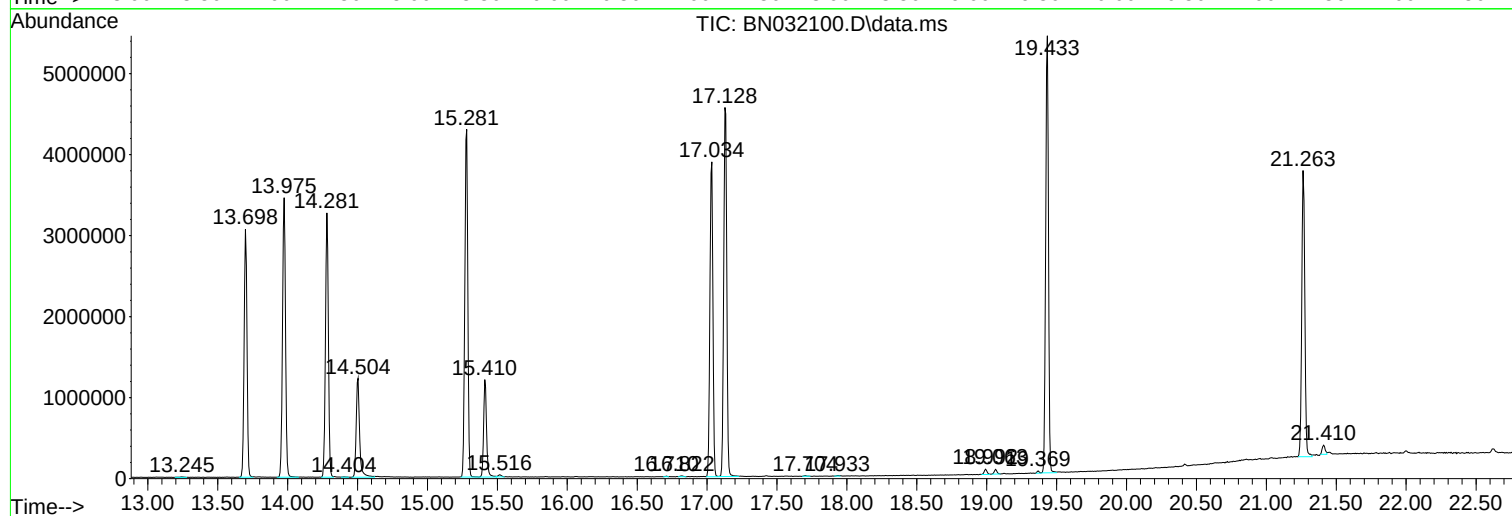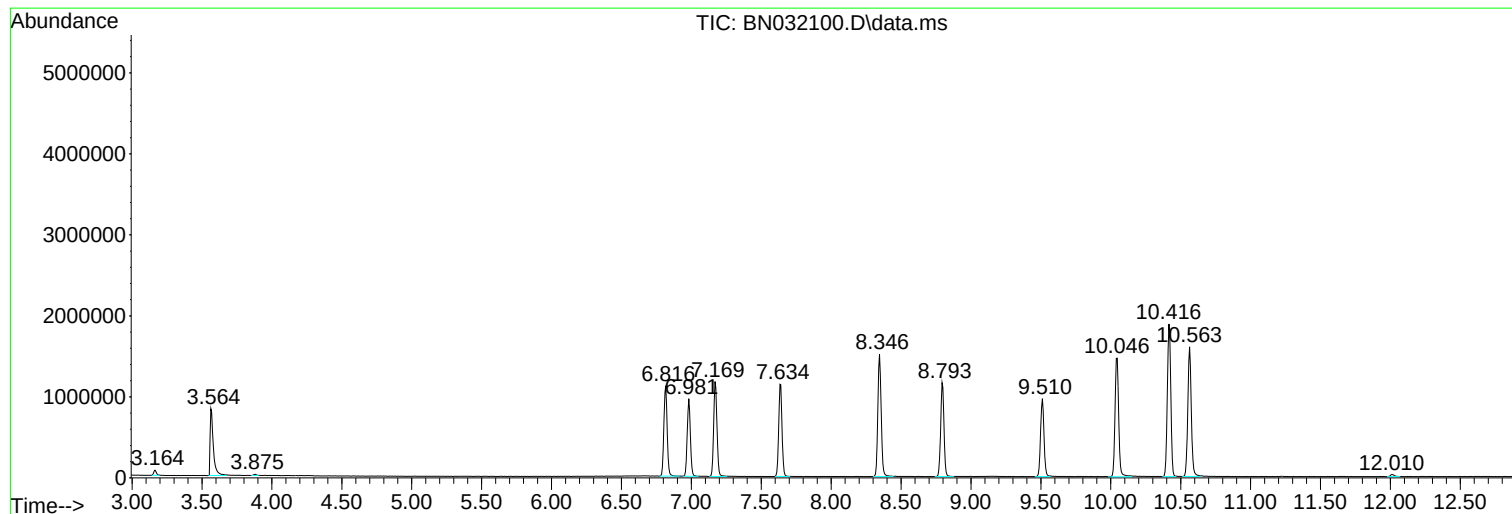

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062024\
Data File : BN032100.D
Acq On : 20 Jun 2024 17:21
Operator : MA/JU
Sample : PB161390BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK390

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062024\
Data File : BN032100.D
Acq On : 20 Jun 2024 17:21
Operator : MA/JU
Sample : PB161390BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK390

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc