

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062024\
 Data File : BN032115.D
 Acq On : 21 Jun 2024 03:51
 Operator : MA/JU
 Sample : PB161390BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK390

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN032115.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	25	30	42	rVB	70453	107789	1.23%	0.114%
2	3.564	95	98	122	rBV	948866	1501886	17.15%	1.587%
3	3.875	148	151	156	rVB	14460	20125	0.23%	0.021%
4	6.816	644	651	667	rVB	1301081	2122223	24.23%	2.243%
5	6.981	671	679	689	rVB	1086833	1712147	19.55%	1.810%
6	7.169	703	711	725	rBV	1400723	2264631	25.86%	2.394%
7	7.634	780	790	803	rBV	1268379	2019480	23.06%	2.135%
8	8.346	902	911	924	rBV	1776643	2960699	33.81%	3.129%
9	8.793	979	987	1001	rBV	1339505	2248406	25.67%	2.377%
10	9.510	1098	1109	1126	rBV	1119629	1928545	22.02%	2.038%
11	10.040	1191	1199	1214	rBV	1734857	3085891	35.24%	3.262%
12	10.416	1254	1263	1274	rBV	1957674	3353887	38.30%	3.545%
13	10.563	1278	1288	1307	rBV	1784117	3245896	37.06%	3.431%
14	12.010	1527	1534	1547	rVB2	29969	61685	0.70%	0.065%
15	13.245	1740	1744	1749	rVB6	6765	9504	0.11%	0.010%
16	13.698	1814	1821	1835	rBV	3413916	4896925	55.92%	5.176%
17	13.975	1860	1868	1880	rBV	3773081	5976932	68.25%	6.318%
18	14.281	1912	1920	1935	rBV	3292017	4968527	56.73%	5.252%
19	14.504	1951	1958	1976	rBV	1393685	2354986	26.89%	2.489%
20	14.639	1979	1981	1985	rVV5	7229	11350	0.13%	0.012%
21	14.692	1987	1990	1996	rVB6	6033	12716	0.15%	0.013%
22	15.275	2082	2089	2103	rBV	4888990	7317959	83.56%	7.735%
23	15.410	2106	2112	2125	rVV	1361183	1989539	22.72%	2.103%
24	15.516	2125	2130	2137	rVB2	27381	46577	0.53%	0.049%
25	16.063	2215	2223	2228	rBV8	5346	10242	0.12%	0.011%
26	16.704	2329	2332	2339	rVB5	6968	10183	0.12%	0.011%
27	16.816	2345	2351	2357	rBV2	10407	20127	0.23%	0.021%
28	17.028	2380	2387	2397	rBV	4007741	5950751	67.95%	6.290%
29	17.128	2397	2404	2419	rVV	5178184	7913403	90.36%	8.364%
30	17.328	2432	2438	2441	rBV6	7796	15718	0.18%	0.017%
31	17.416	2450	2453	2457	rBV2	7994	12528	0.14%	0.013%
32	18.992	2716	2721	2726	rBV2	79415	110216	1.26%	0.116%
33	19.063	2728	2733	2740	rVV	72219	108471	1.24%	0.115%
34	19.363	2781	2784	2789	rBV3	34467	46928	0.54%	0.050%
35	19.427	2789	2795	2809	rVV2	5900275	8757503	100.00%	9.257%
36	21.263	3101	3107	3118	rBV2	3809133	5468559	62.44%	5.780%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062024\
Data File : BN032115.D
Acq On : 21 Jun 2024 03:51
Operator : MA/JU
Sample : PB161390BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK390

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Title : SVOA CALIBRATION

37	23.974	3559	3568	3587	rVB2	2742126	6890921	78.69%	7.284%
38	24.174	3593	3602	3614	rVB	1981796	5074253	57.94%	5.363%




Sum of corrected areas: 94608108

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062024\
Data File : BN032115.D
Acq On : 21 Jun 2024 03:51
Operator : MA/JU
Sample : PB161390BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK390

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

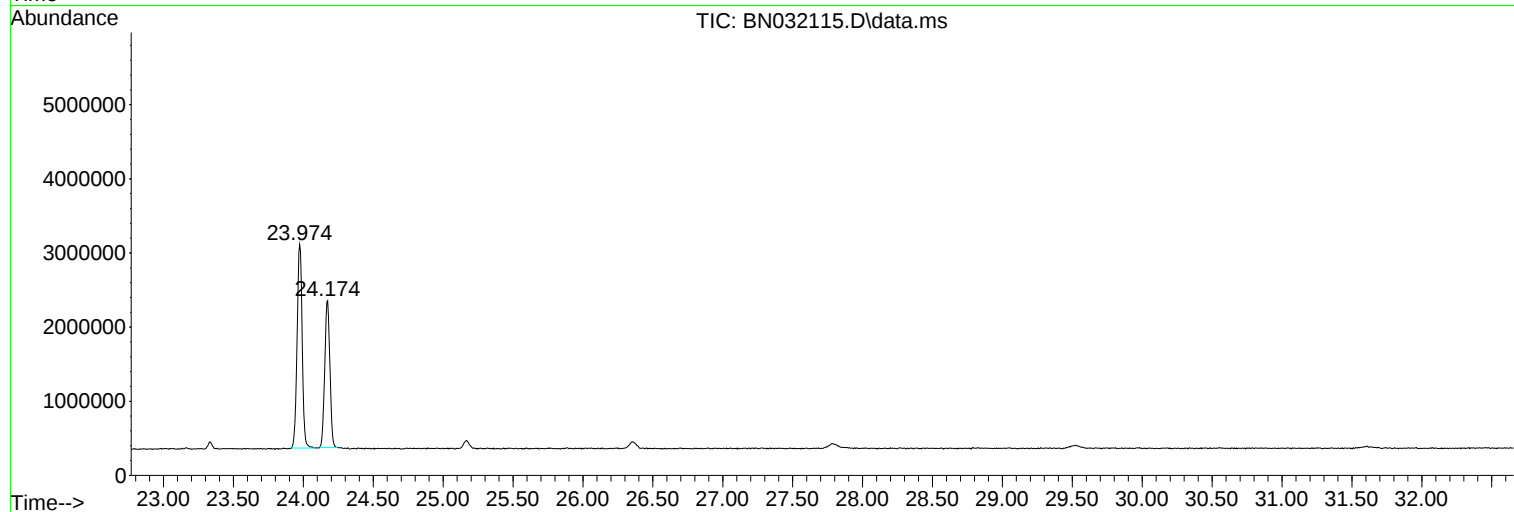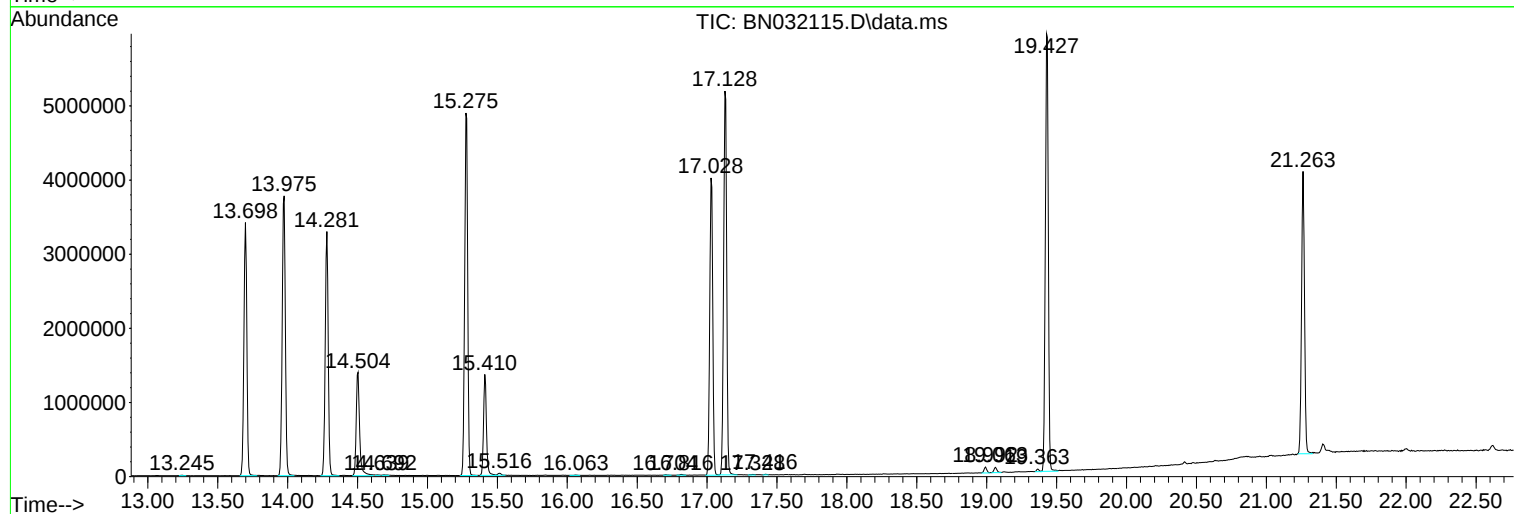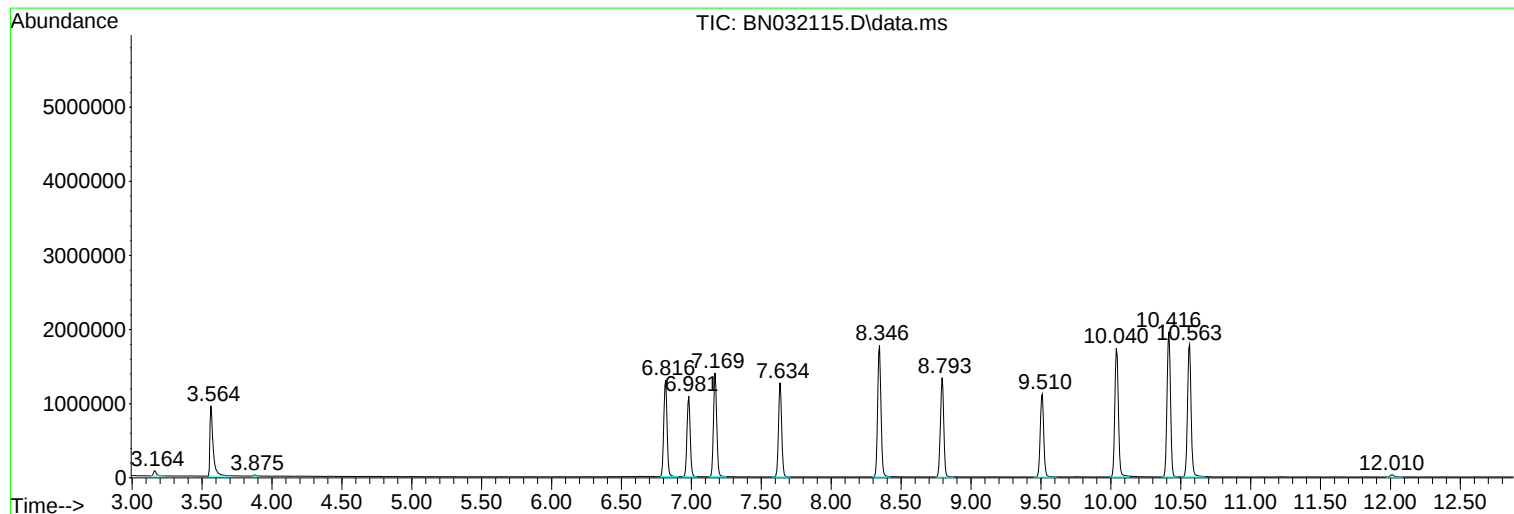

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062024\
Data File : BN032115.D
Acq On : 21 Jun 2024 03:51
Operator : MA/JU
Sample : PB161390BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK390

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062024\
Data File : BN032115.D
Acq On : 21 Jun 2024 03:51
Operator : MA/JU
Sample : PB161390BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK390

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------