

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062119\
 Data File : BN006477.D
 Acq On : 21 Jun 2019 22:15
 Operator : HP/JU
 Sample : K3335-22
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A41Y0

Quant Time: Jun 22 03:47:29 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 21 22:42:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	251159	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	1141279	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.28	164	657923	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.03	188	1429423	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	1133227	20.00	ng/ul	-0.01
85) Perylene-d12	23.48	264	1050572	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	25102	3.90	ng/uL	0.00
5) Phenol-d5	6.80	99	434887	16.26	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	318294	19.23	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	346482	17.57	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	302617	14.27	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	184015	20.14	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	193838	19.47	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	324966	16.99	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	426922	19.41	ng/ul	0.00
43) Dimethylphthalate-d6	13.69	166	1169681	20.28	ng/ul	0.00
46) Acenaphthylene-d8	13.97	160	1303439	18.44	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	131593	13.36	ng/ul	0.00
57) Fluorene-d10	15.28	176	961224	19.60	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	59718	6.60	ng/ul	0.00
70) Anthracene-d10	17.13	188	1357162	18.86	ng/ul	0.00
78) Pyrene-d10	19.45	212	1545214	23.34	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.34	264	1130361	19.05	ng/ul	-0.01

Target Compounds


					Qvalue
4) Benzaldehyde	6.78	77	25433	2.354 ng/ul	94
44) Dimethylphthalate	13.74	163	1172979	22.066 ng/ul	100
45) 2,6-Dinitrotoluene	13.74	165	12772	1.233 ng/ul#	51
49) Acenaphthene	14.35	153	51741	1.159 ng/ul	97
53) Dibenzofuran	14.68	168	63814	1.032 ng/ul	99
58) Fluorene	15.33	166	66600	1.332 ng/ul	99
69) Phenanthrene	17.08	178	876205	11.114 ng/ul	99
71) Anthracene	17.17	178	233631	2.919 ng/ul	99
74) Carbazole	17.45	167	81112	1.174 ng/ul	100
76) Fluoranthene	19.10	202	1002398	11.797 ng/ul	99
79) Pyrene	19.47	202	822176	10.656 ng/ul	98
82) Benzo(a)anthracene	21.23	228	364992	4.712 ng/ul	99
84) Chrysene	21.29	228	320905	4.353 ng/ul	98
87) Benzo(b)fluoranthene	22.82	252	306555	4.862 ng/ul	99
88) Benzo(k)fluoranthene	22.82	252	306555	5.087 ng/ul	99
90) Benzo(a)pyrene	23.38	252	206687	3.419 ng/ul	99
91) Indeno(1,2,3-cd)pyrene	25.70	276	112672	1.575 ng/ul	96
93) Benzo(g,h,i)perylene	26.39	276	87437	1.451 ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062119\
Data File : BN006477.D
Acq On : 21 Jun 2019 22:15
Operator : HP/JU
Sample : K3335-22
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41Y0

Quant Time: Jun 22 03:47:29 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 22:42:34 2019
Response via : Initial Calibration

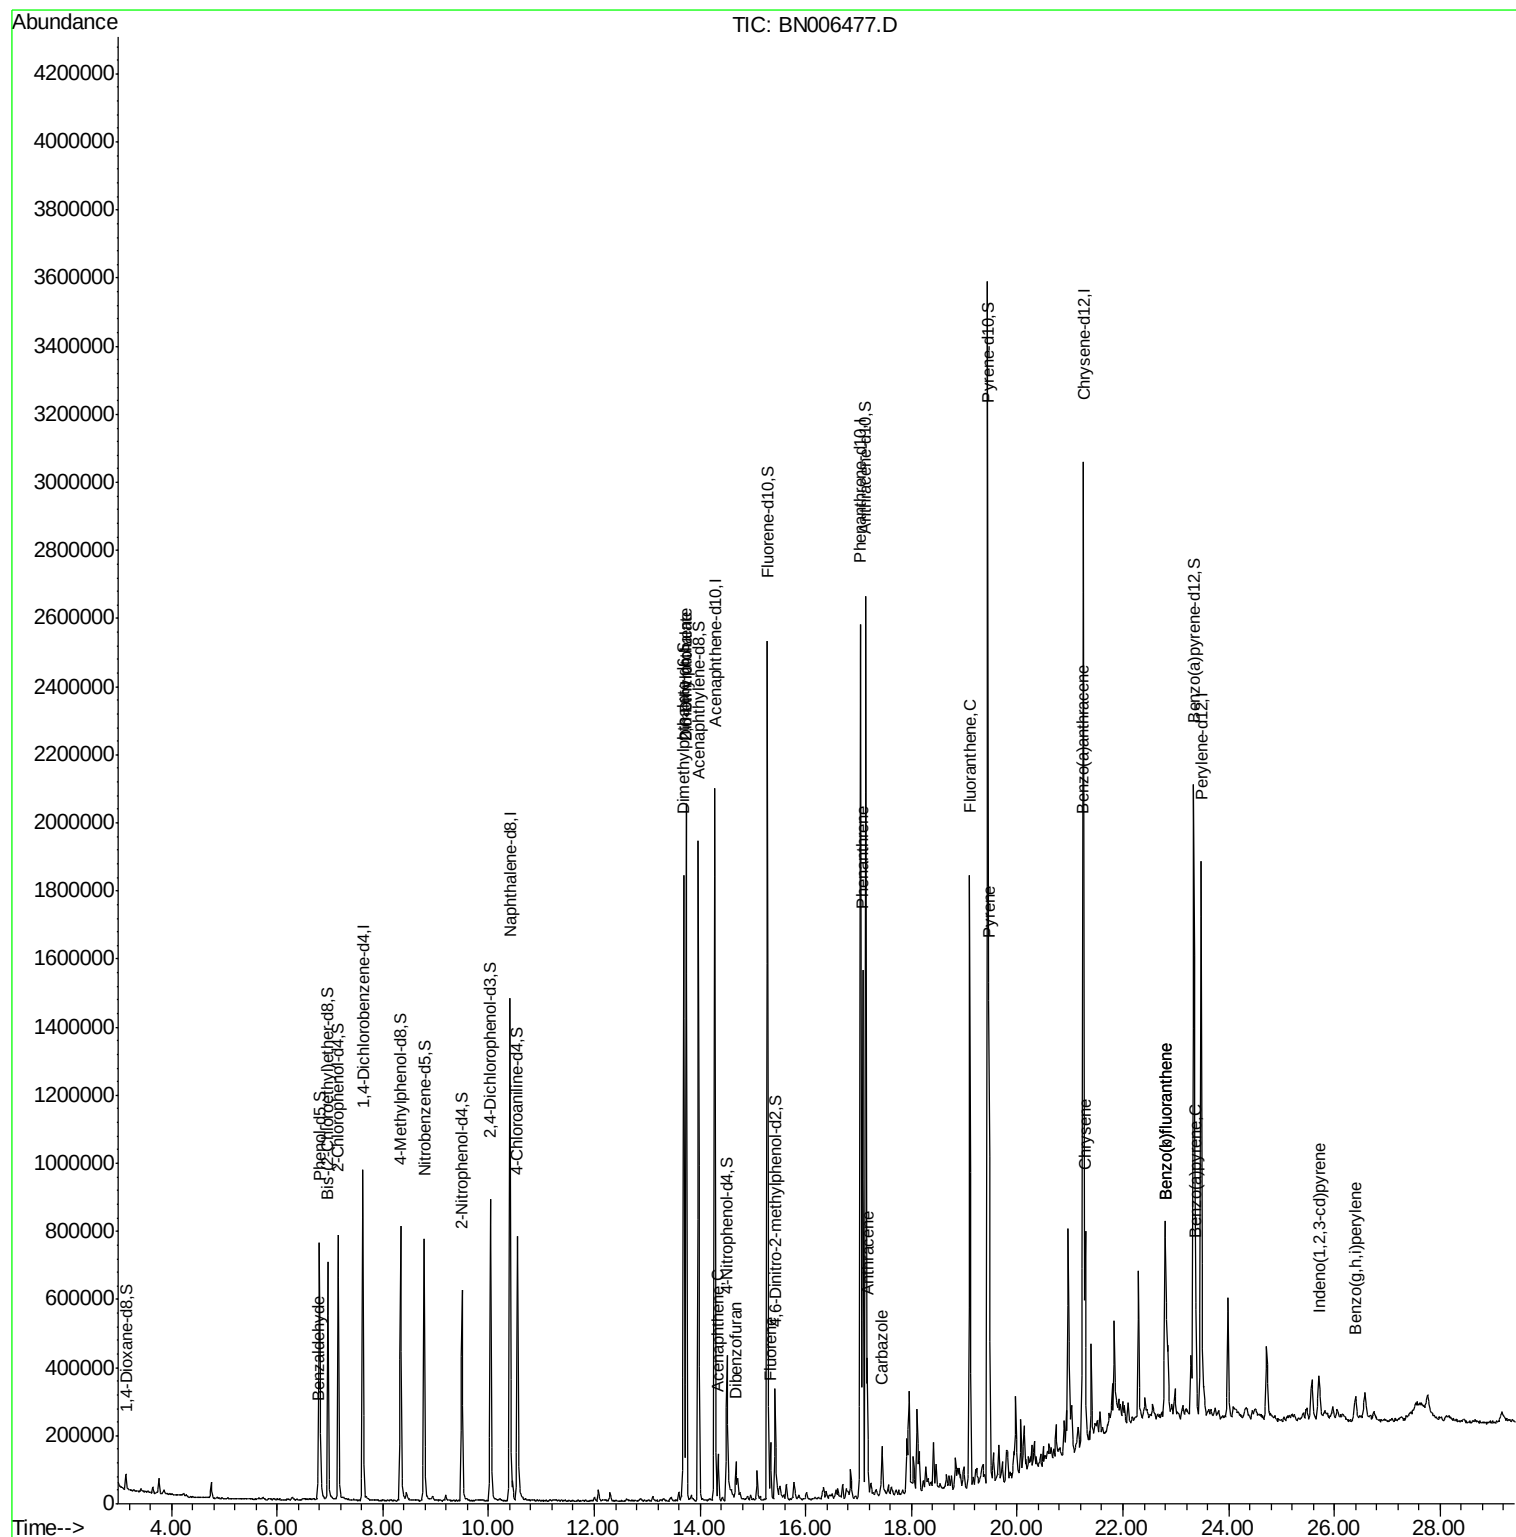



#4

Benzaldehyde

Concen: 2.354 ng/ul

RT: 6.78 min Scan# 644

Delta R.T. 0.00 min

Lab File: BN006477.D

Acq: 21 Jun 2019 22:15

Instrument :

BNA_N

ClientSampleId :

A41Y0


Tgt Ion: 77 Resp: 25433

Ion Ratio Lower Upper

77 100

105 100.0 74.1 111.1




106 94.2 72.7 109.1

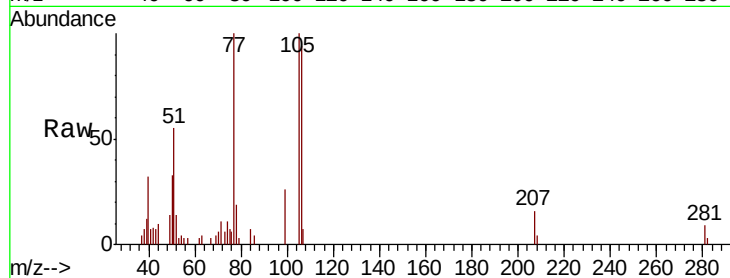

Abundance Ion 77.00 (76.70 to 77.70): BN006467.D (-637) (-)

Ion 105.00 (104.70 to 105.70): BN006467.D (-637) (-)

Ion 106.00 (105.70 to 106.70): BN006467.D (-637) (-)

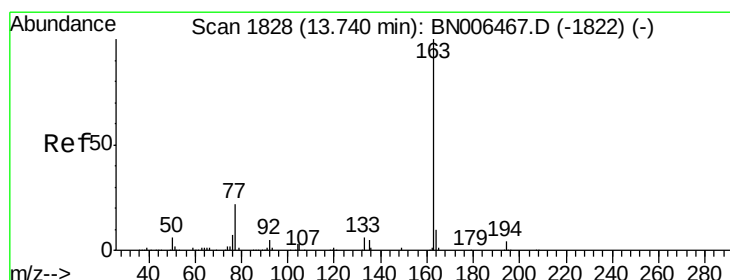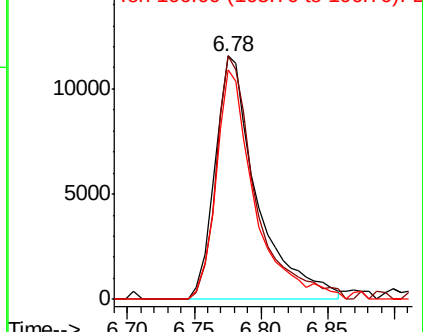

#44

Dimethylphthalate

Concen: 22.066 ng/ul

RT: 13.74 min Scan# 1828

Delta R.T. 0.00 min

Lab File: BN006477.D

Acq: 21 Jun 2019 22:15


Tgt Ion: 163 Resp: 1172979

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.0



164 10.1 8.0 12.0

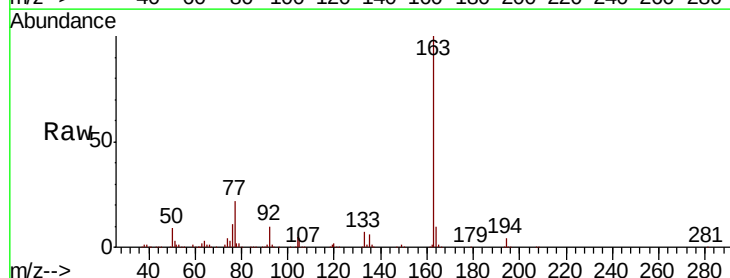


Abundance Ion 163.00 (162.70 to 163.70): BN006467.D (-1822) (-)

Ion 194.00 (193.70 to 194.70): BN006467.D (-1822) (-)

Ion 164.00 (163.70 to 164.70): BN006467.D (-1822) (-)

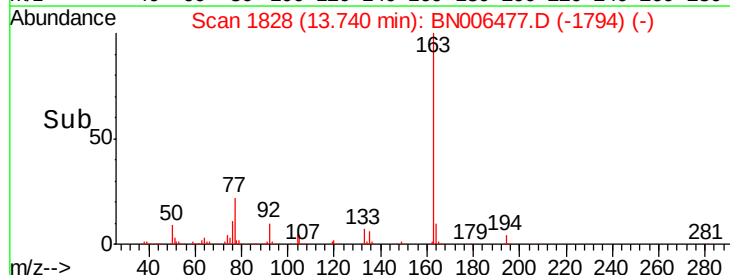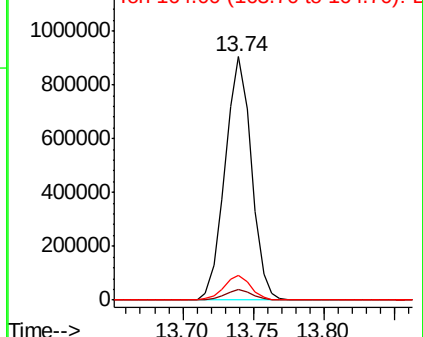







#45
 2,6-Dinitrotoluene
 Concen: 1.233 ng/ul
 RT: 13.74 min Scan# 1828
 Delta R.T. -0.13 min
 Lab File: BN006477.D
 Acq: 21 Jun 2019 22:15

Instrument :
 BNA_N
 ClientSampleId :
 A41Y0

Tgt Ion:165 Resp: 12772
 Ion Ratio Lower Upper
 165 100
 89 15.8 48.6 72.8#
 121 30.6 17.2 25.8#

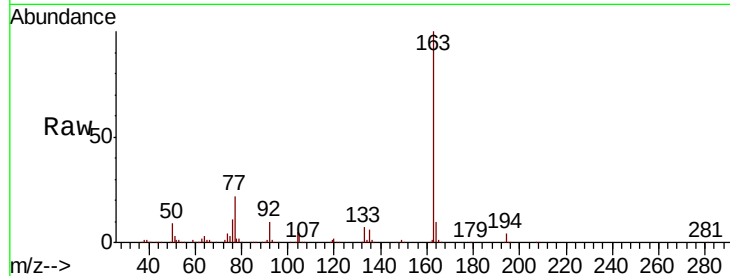


Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 89.00 (88.70 to 89.70): BNO
 Ion 121.00 (120.70 to 121.70): E

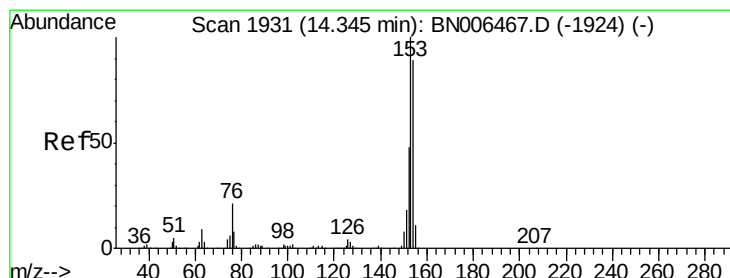
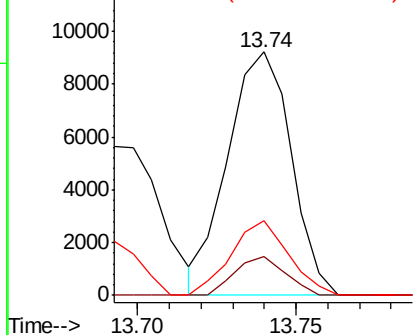



#49
 Acenaphthene
 Concen: 1.159 ng/ul
 RT: 14.35 min Scan# 1931
 Delta R.T. 0.00 min
 Lab File: BN006477.D
 Acq: 21 Jun 2019 22:15

Tgt Ion:153 Resp: 51741
 Ion Ratio Lower Upper
 153 100
 152 50.0 37.8 56.6
 154 87.4 71.2 106.8

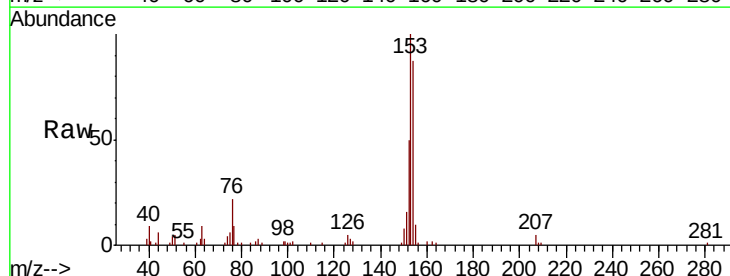

Abundance Ion 153.00 (152.70 to 153.70): E
 Ion 152.00 (151.70 to 152.70): E
 Ion 154.00 (153.70 to 154.70): E

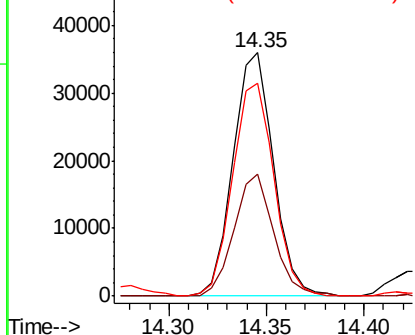

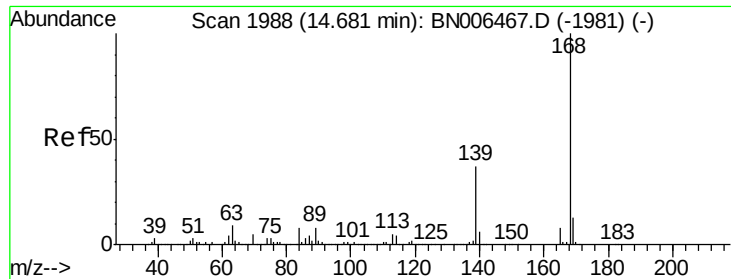

#53

Dibenzenofuran

Concen: 1.032 ng/ul

RT: 14.68 min Scan# 1988

Delta R.T. 0.00 min

Lab File: BN006477.D

Acq: 21 Jun 2019 22:15

Instrument :

BNA_N

ClientSampleId :


A41Y0

Tgt Ion:168 Resp: 63814

Ion Ratio Lower Upper




168 100

139 37.4 29.4 44.0



Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

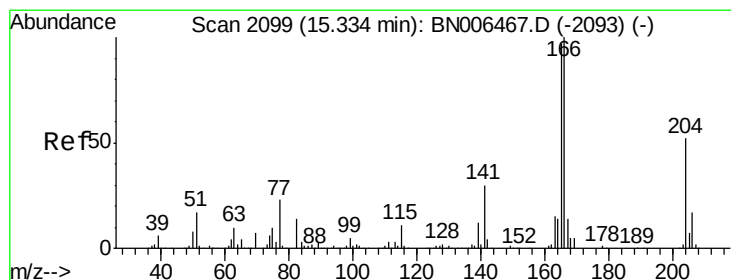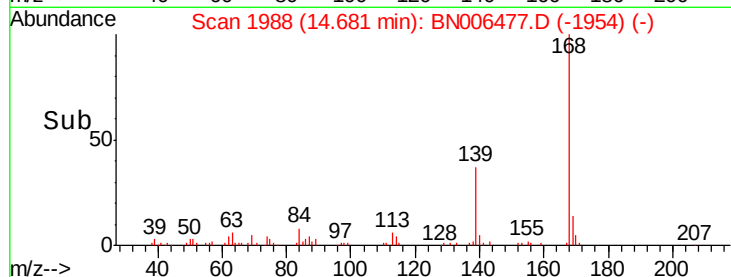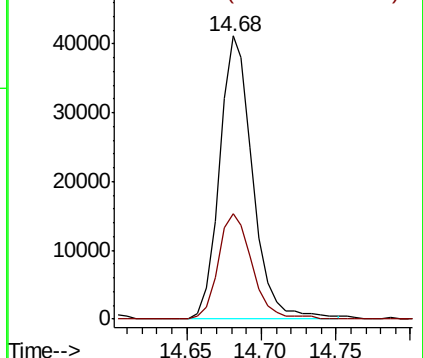

#58

Fluorene

Concen: 1.332 ng/ul

RT: 15.33 min Scan# 2099

Delta R.T. 0.00 min

Lab File: BN006477.D

Acq: 21 Jun 2019 22:15


Tgt Ion:166 Resp: 66600

Ion Ratio Lower Upper

166 100

165 97.6 77.5 116.3



167 14.6 10.7 16.1




Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

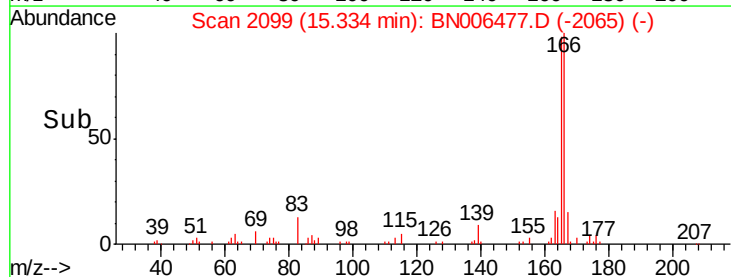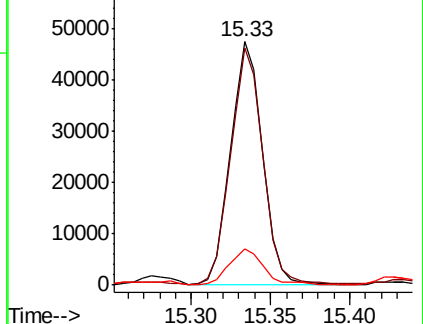



#69

Phenanthrene

Concen: 11.114 ng/ul

RT: 17.08 min Scan# 2396

Delta R.T. 0.00 min

Lab File: BN006477.D

Acq: 21 Jun 2019 22:15

Instrument :

BNA_N

ClientSampleId :

A41Y0


Tgt Ion:178 Resp: 876205

Ion Ratio Lower Upper

178 100

179 15.2 12.5 18.7




176 19.0 15.3 22.9

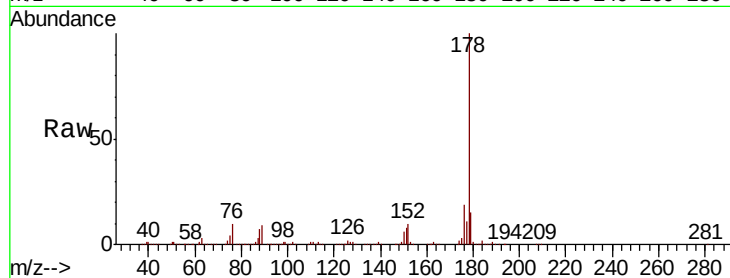

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

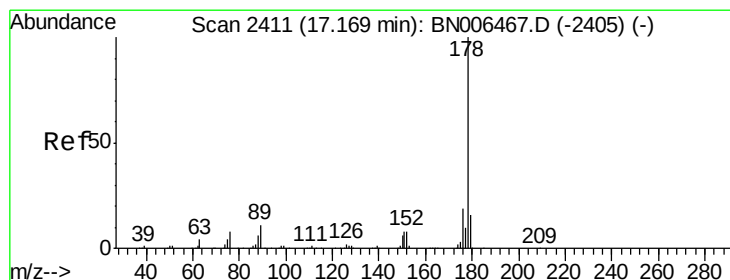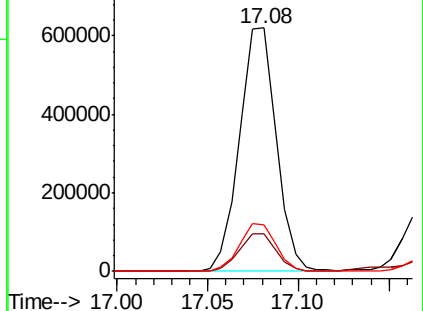

#71

Anthracene

Concen: 2.919 ng/ul

RT: 17.17 min Scan# 2411

Delta R.T. 0.00 min

Lab File: BN006477.D

Acq: 21 Jun 2019 22:15


Tgt Ion:178 Resp: 233631

Ion Ratio Lower Upper

178 100

179 15.9 12.3 18.5



176 18.5 14.7 22.1

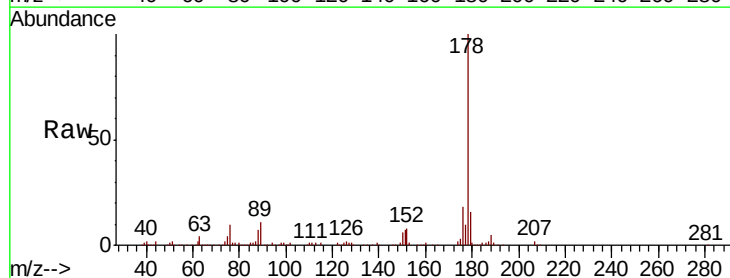


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

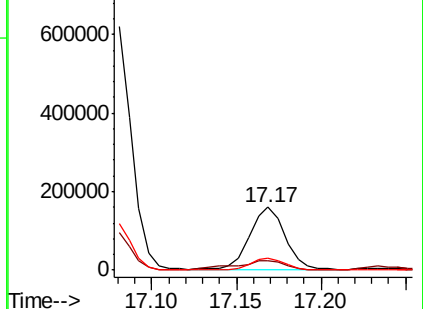



#74

Carbazole

Concen: 1.174 ng/ul

RT: 17.45 min Scan# 2458

Delta R.T. 0.00 min

Lab File: BN006477.D

Acq: 21 Jun 2019 22:15

Instrument :

BNA_N

ClientSampleId :

A41Y0


Tgt Ion:167 Resp: 81112

Ion Ratio Lower Upper

167 100

166 21.4 17.1 25.7




139 13.3 10.5 15.7

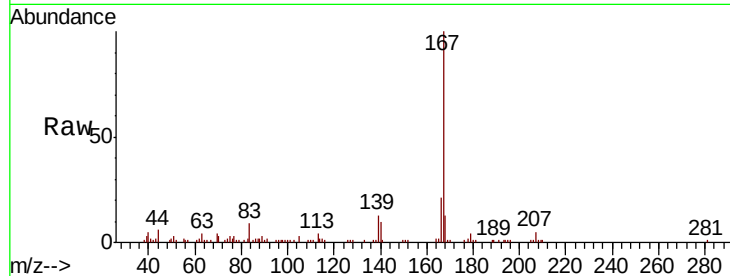

Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

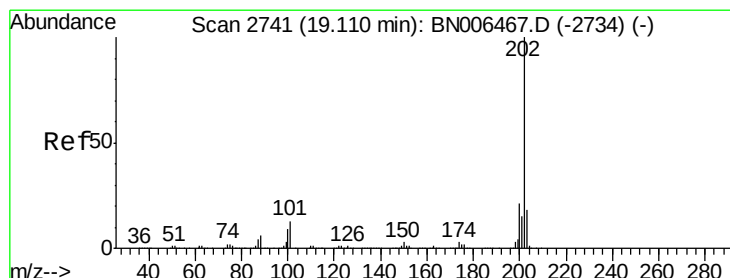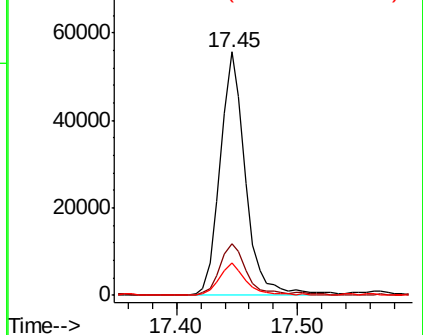

#76

Fluoranthene

Concen: 11.797 ng/ul

RT: 19.10 min Scan# 2740

Delta R.T. -0.01 min

Lab File: BN006477.D

Acq: 21 Jun 2019 22:15


Tgt Ion:202 Resp: 1002398

Ion Ratio Lower Upper

202 100

101 12.8 10.5 15.7



100 9.3 7.6 11.4

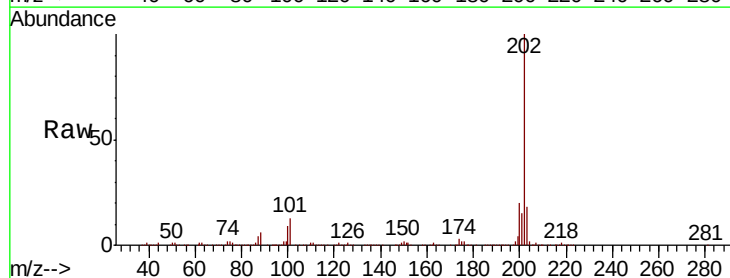


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E



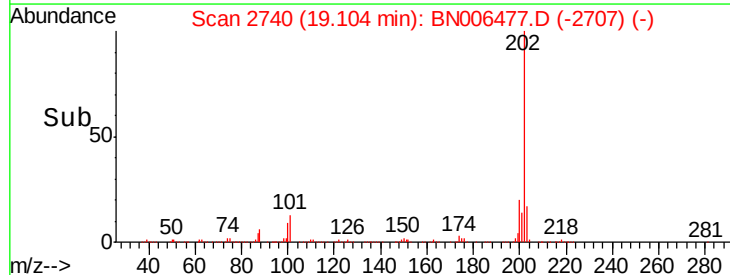
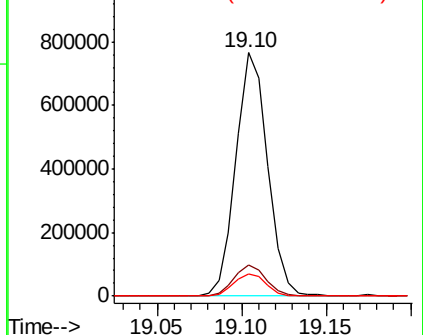


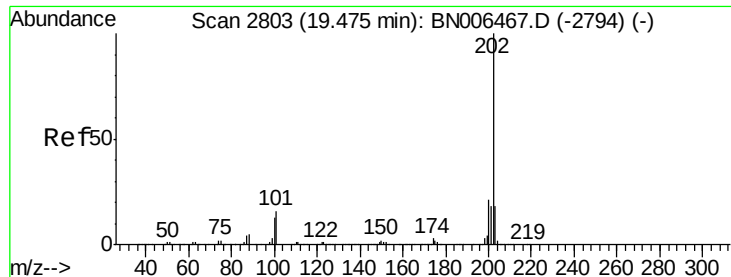

#79
 Pyrene
 Concen: 10.656 ng/ul
 RT: 19.47 min Scan# 2803
 Delta R.T. 0.00 min
 Lab File: BN006477.D
 Acq: 21 Jun 2019 22:15




Instrument :
 BNA_N
 ClientSampleId :
 A41Y0


Tgt Ion	Ratio	Lower	Upper
202	100		
101	14.3	12.2	18.4
100	11.3	9.8	14.6

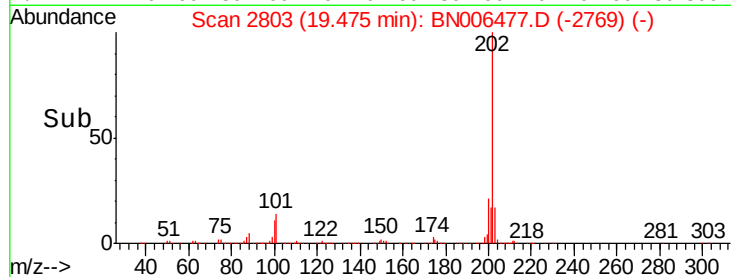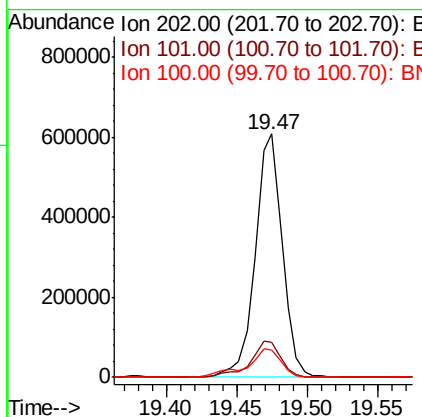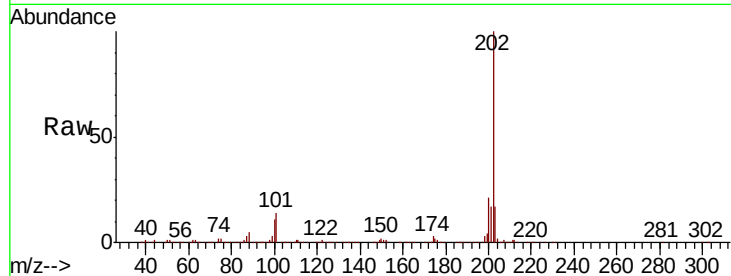

#82
 Benzo(a)anthracene
 Concen: 4.712 ng/ul
 RT: 21.23 min Scan# 3102
 Delta R.T. -0.01 min
 Lab File: BN006477.D
 Acq: 21 Jun 2019 22:15

Tgt Ion	Ratio	Lower	Upper
228	100		
229	20.6	15.6	23.4
226	26.9	21.5	32.3

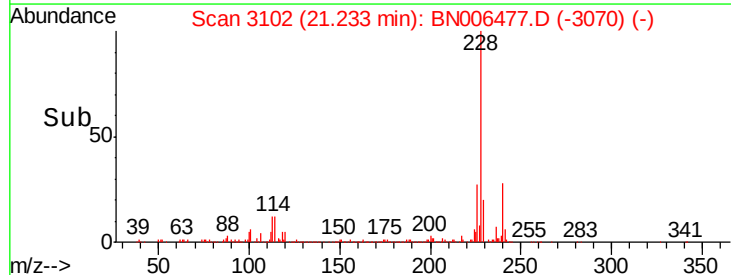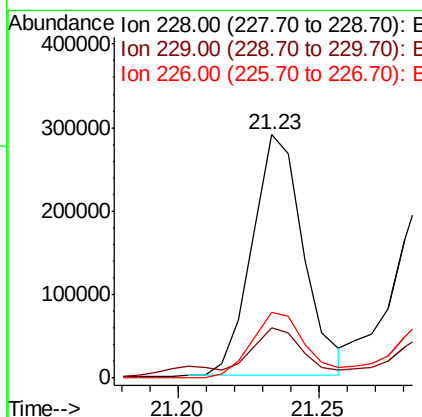

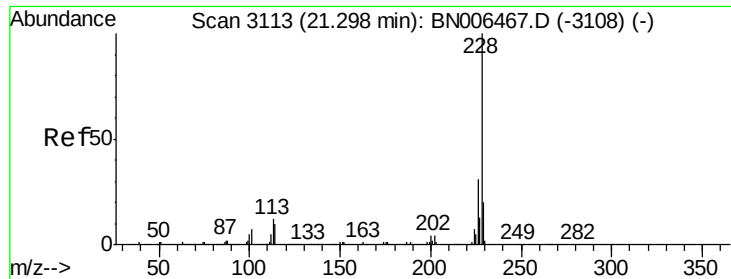

#84

Chrysene

Concen: 4.353 ng/ul

RT: 21.29 min Scan# 3111

Delta R.T. -0.01 min

Lab File: BN006477.D

Acq: 21 Jun 2019 22:15

Instrument :

BNA_N

ClientSampleId :

A41Y0


Tgt Ion:228 Resp: 320905

Ion Ratio Lower Upper

228 100

226 30.5 24.2 36.2

229 22.3 15.9 23.9






Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

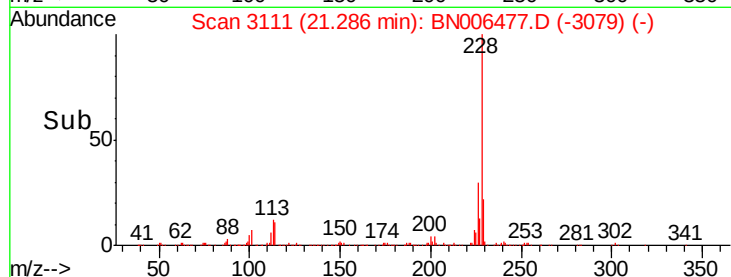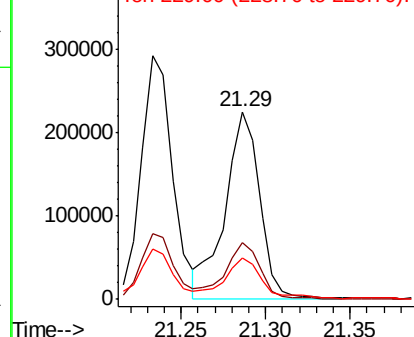

#87

Benzo(b)fluoranthene

Concen: 4.862 ng/ul

RT: 22.82 min Scan# 3371

Delta R.T. -0.01 min

Lab File: BN006477.D

Acq: 21 Jun 2019 22:15


Tgt Ion:252 Resp: 306555

Ion Ratio Lower Upper

252 100

253 22.4 17.7 26.5

125 11.8 9.0 13.6






Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E



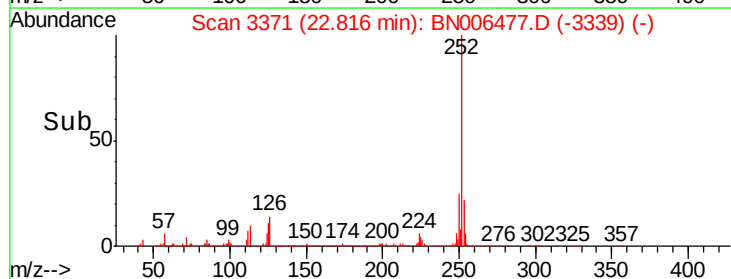
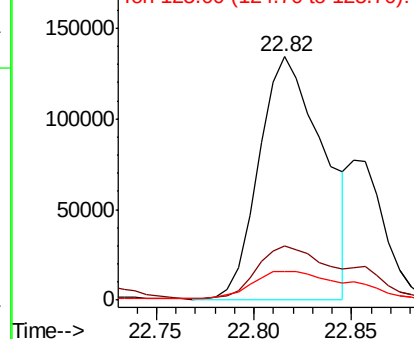


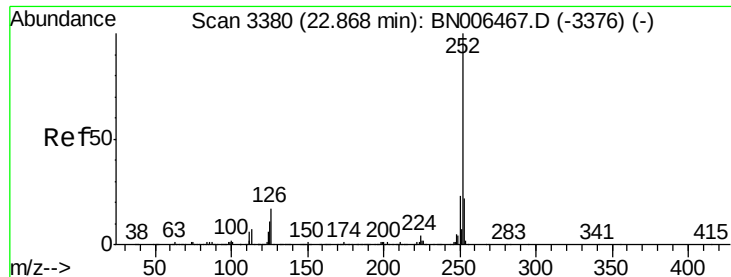

#88
Benzo(k)fluoranthene
Concen: 5.087 ng/ul
RT: 22.82 min Scan# 3371
Delta R.T. -0.05 min
Lab File: BN006477.D
Acq: 21 Jun 2019 22:15




Instrument :
BNA_N
ClientSampleId :
A41Y0


Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.4	17.4	26.0
125	11.8	9.1	13.7

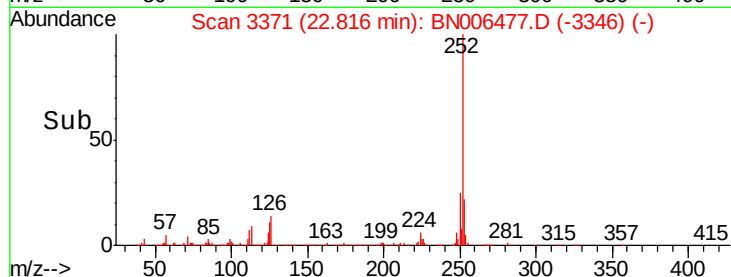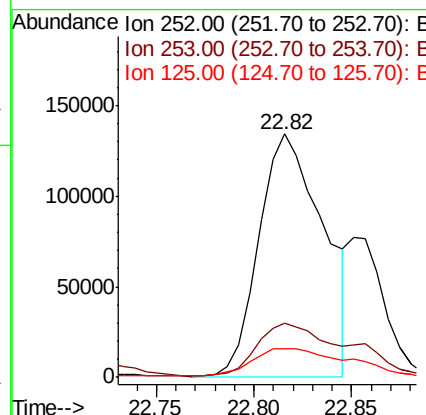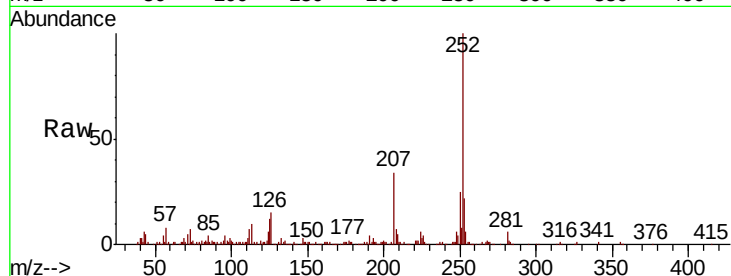

#90
Benzo(a)pyrene
Concen: 3.419 ng/ul
RT: 23.38 min Scan# 3467
Delta R.T. -0.02 min
Lab File: BN006477.D
Acq: 21 Jun 2019 22:15

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.8	17.7	26.5
125	12.6	10.0	15.0

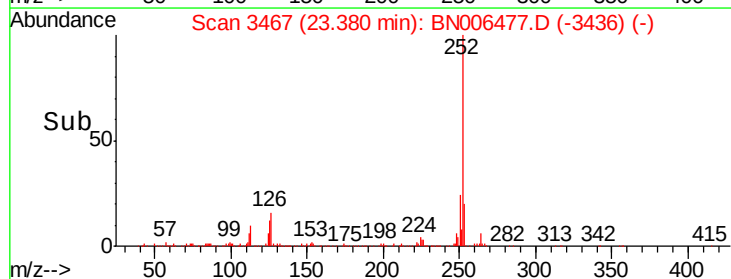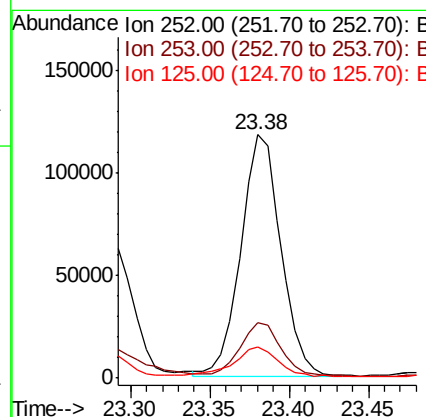

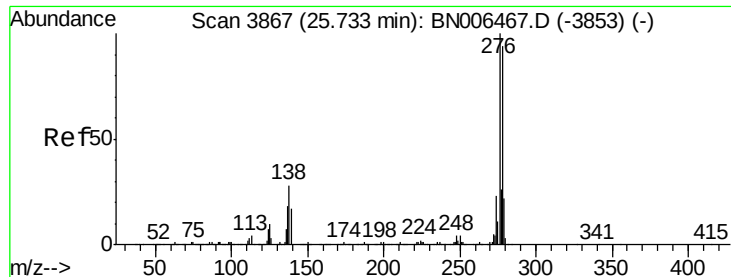

#91

Indeno(1,2,3-cd)pyrene

Concen: 1.575 ng/ul

RT: 25.70 min Scan# 3862

Delta R.T. -0.03 min

Lab File: BN006477.D

Acq: 21 Jun 2019 22:15

Instrument :

BNA_N

ClientSampled :

A41Y0


Tgt Ion:276 Resp: 112672

Ion Ratio Lower Upper

276 100

138 24.7 22.2 33.4




277 24.3 20.2 30.4

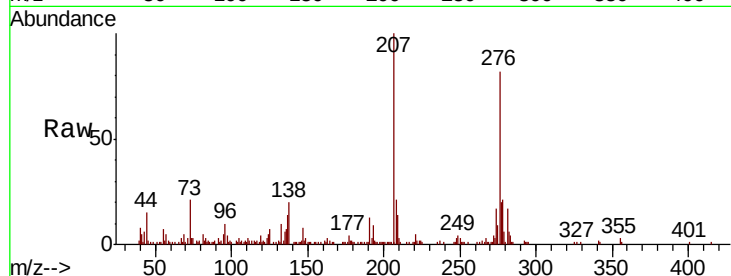

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

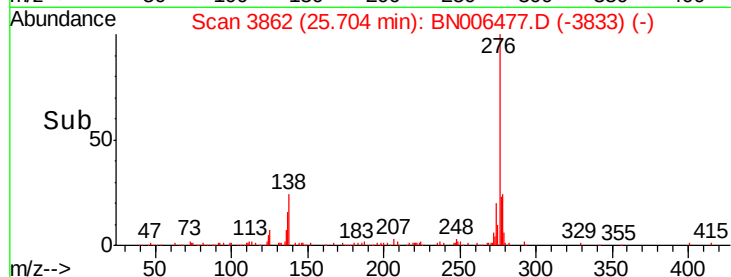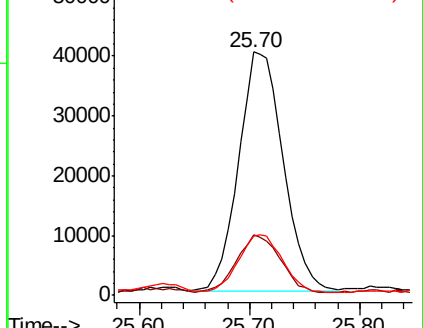

#93

Benzo(g,h,i)perylene

Concen: 1.451 ng/ul

RT: 26.39 min Scan# 3979

Delta R.T. -0.02 min

Lab File: BN006477.D

Acq: 21 Jun 2019 22:15


Tgt Ion:276 Resp: 87437

Ion Ratio Lower Upper

276 100

138 21.8 19.1 28.7

277 23.9 19.4 29.0



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

