

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062119\
 Data File : BN006479.D
 Acq On : 21 Jun 2019 23:24
 Operator : HP/JU
 Sample : K3362-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A41T7

Quant Time: Jun 22 03:47:46 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 21 22:42:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	266622	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	1221010	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.28	164	725125	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.03	188	1579662	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	1255307	20.00	ng/ul	-0.02
85) Perylene-d12	23.47	264	1121027	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	38115	5.58	ng/uL	0.00
5) Phenol-d5	6.80	99	839238	29.56	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	532313	30.29	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	642420	30.69	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	667791	29.65	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	323387	33.08	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	358336	33.64	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	640806	31.31	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	877605	37.29	ng/ul	0.00
43) Dimethylphthalate-d6	13.69	166	2041994	32.13	ng/ul	0.00
46) Acenaphthylene-d8	13.97	160	2461673	31.60	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	266322	24.53	ng/ul	0.00
57) Fluorene-d10	15.28	176	1754415	32.46	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	150440	15.05	ng/ul	0.00
70) Anthracene-d10	17.13	188	2672574	33.61	ng/ul	0.00
78) Pyrene-d10	19.45	212	2800904	38.20	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.33	264	2065633	32.62	ng/ul	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.74	163	684288	11.680	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062119\
Data File : BN006479.D
Acq On : 21 Jun 2019 23:24
Operator : HP/JU
Sample : K3362-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41T7

Quant Time: Jun 22 03:47:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 22:42:34 2019
Response via : Initial Calibration

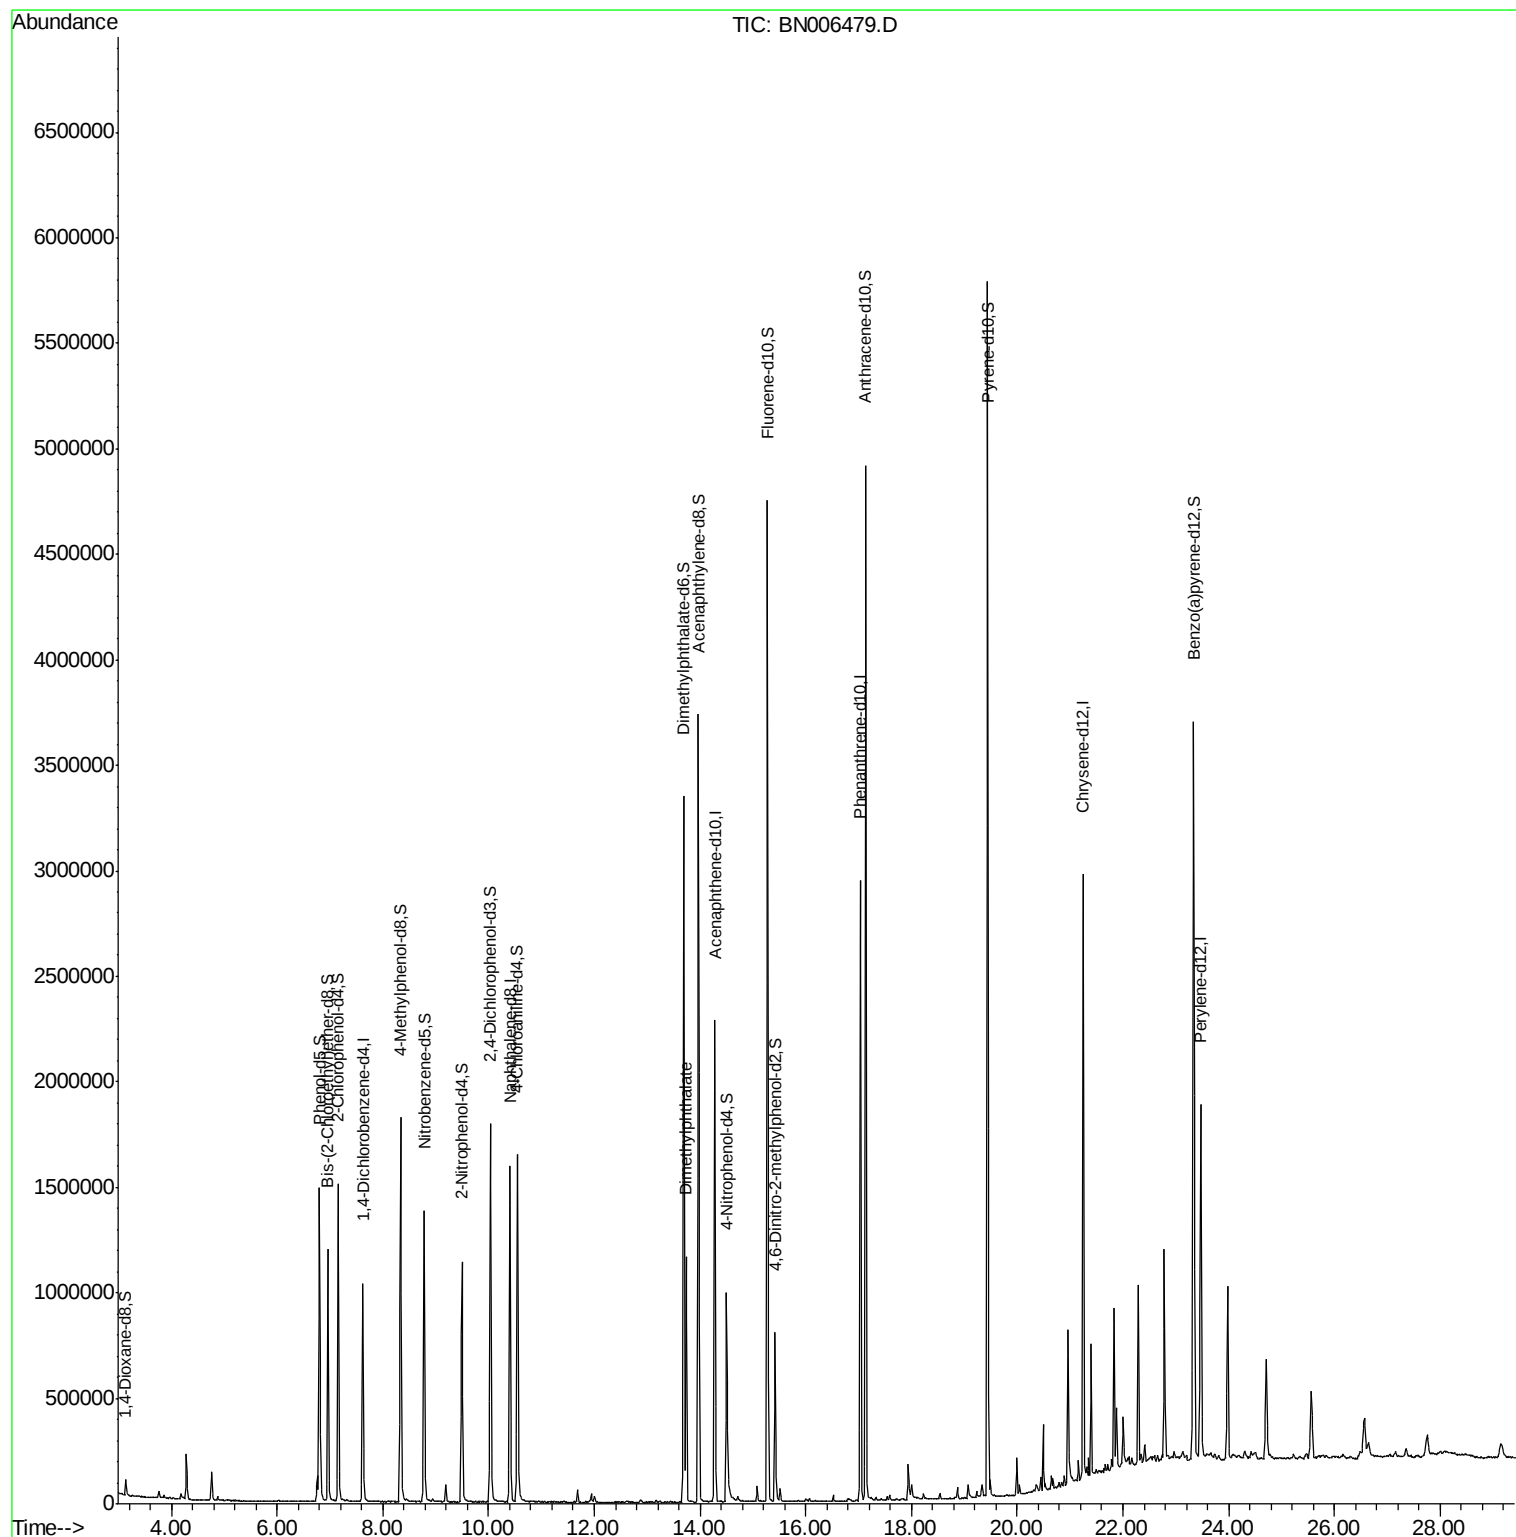

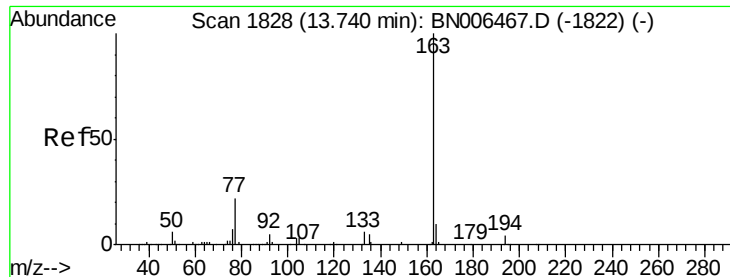

#44

Dimethylphthalate

Concen: 11.680 ng/ul

RT: 13.74 min Scan# 1828

Delta R.T. 0.00 min

Lab File: BN006479.D

Acq: 21 Jun 2019 23:24

Instrument :

BNA_N

ClientSampleId :

A41T7


Tgt Ion:163 Resp: 684288

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.0

164 10.2 8.0 12.0

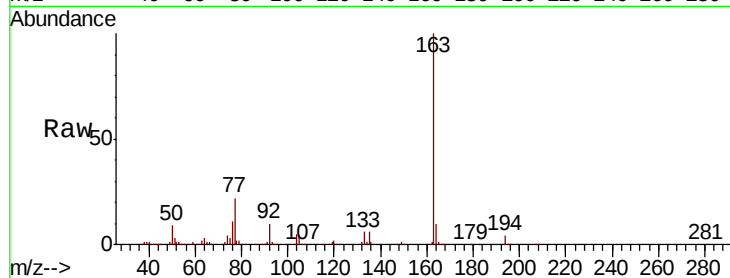

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

