

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062119\
 Data File : BN006481.D
 Acq On : 22 Jun 2019 00:33
 Operator : HP/JU
 Sample : PB120644BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 ABLK44

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.017	3	5	8	rVV4	12952	10451	0.13%	0.014%
2	3.052	8	11	21	rVV	321596	397246	4.86%	0.532%
3	3.123	21	23	28	rVB3	15247	18346	0.22%	0.025%
4	3.381	64	67	74	rVB	20043	28658	0.35%	0.038%
5	6.799	642	648	666	rBV	809862	1326008	16.23%	1.777%
6	6.958	669	675	688	rVV	807951	1224724	14.99%	1.641%
7	7.152	701	708	721	rBV	1013671	1651714	20.22%	2.213%
8	7.622	781	788	803	rBV	828946	1354567	16.58%	1.815%
9	8.334	900	909	931	rBV	1213855	2059356	25.21%	2.759%
10	8.775	977	984	1001	rBV	994264	1663440	20.37%	2.229%
11	9.493	1098	1106	1121	rBV	830778	1430689	17.52%	1.917%
12	10.034	1191	1198	1218	rBV	1349821	2365201	28.96%	3.169%
13	10.405	1253	1261	1274	rBV	1279081	2114379	25.89%	2.833%
14	10.546	1278	1285	1304	rBV	1393090	2383358	29.18%	3.193%
15	12.004	1529	1533	1539	rBV2	14132	26075	0.32%	0.035%
16	13.693	1813	1820	1833	rBV	2928652	3900358	47.75%	5.226%
17	13.969	1860	1867	1882	rBV	3360783	4742296	58.06%	6.354%
18	14.281	1913	1920	1930	rBV2	2151209	3170618	38.82%	4.248%
19	14.504	1952	1958	1984	rBV	1084618	1932431	23.66%	2.589%
20	15.087	2052	2057	2063	rBV	13647	18742	0.23%	0.025%
21	15.281	2083	2090	2108	rBV	4254600	6017531	73.67%	8.062%
22	15.422	2108	2114	2126	rVV	868552	1267351	15.52%	1.698%
23	15.516	2126	2130	2136	rVB	54574	79508	0.97%	0.107%
24	16.822	2348	2352	2359	rVB	9124	13790	0.17%	0.018%
25	17.034	2382	2388	2398	rBV2	2905051	4026794	49.30%	5.395%
26	17.134	2398	2405	2428	rVB2	5050604	7044729	86.25%	9.439%
27	19.075	2730	2735	2742	rVV	46700	65093	0.80%	0.087%
28	19.328	2773	2778	2784	rBV	44896	61807	0.76%	0.083%
29	19.445	2791	2798	2813	rBV	5958271	8167944	100.00%	10.944%
30	20.357	2950	2953	2957	rBV5	14979	16699	0.20%	0.022%
31	21.245	3099	3104	3117	rBV2	3206789	4307315	52.73%	5.771%
32	21.398	3127	3130	3134	rVB	34140	31534	0.39%	0.042%
33	21.827	3200	3203	3208	rBV	73094	94701	1.16%	0.127%
34	22.286	3278	3281	3287	rVB	138534	173831	2.13%	0.233%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062119\
Data File : BN006481.D
Acq On : 22 Jun 2019 00:33
Operator : HP/JU
Sample : PB120644BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
ABLK44

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
Title : SVOA CALIBRATION

35	22.786	3362	3366	3371	rVB	161109	226923	2.78%	0.304%
36	23.333	3451	3459	3474	rBV	3682928	6971235	85.35%	9.340%
37	23.474	3476	3483	3492	rVB2	1993172	3615887	44.27%	4.845%
38	23.980	3564	3569	3576	rVB	173268	313343	3.84%	0.420%
39	24.710	3688	3693	3702	rVB2	147561	322721	3.95%	0.432%


Sum of corrected areas: 74637393

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062119\
Data File : BN006481.D
Acq On : 22 Jun 2019 00:33
Operator : HP/JU
Sample : PB120644BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
ABLK44

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

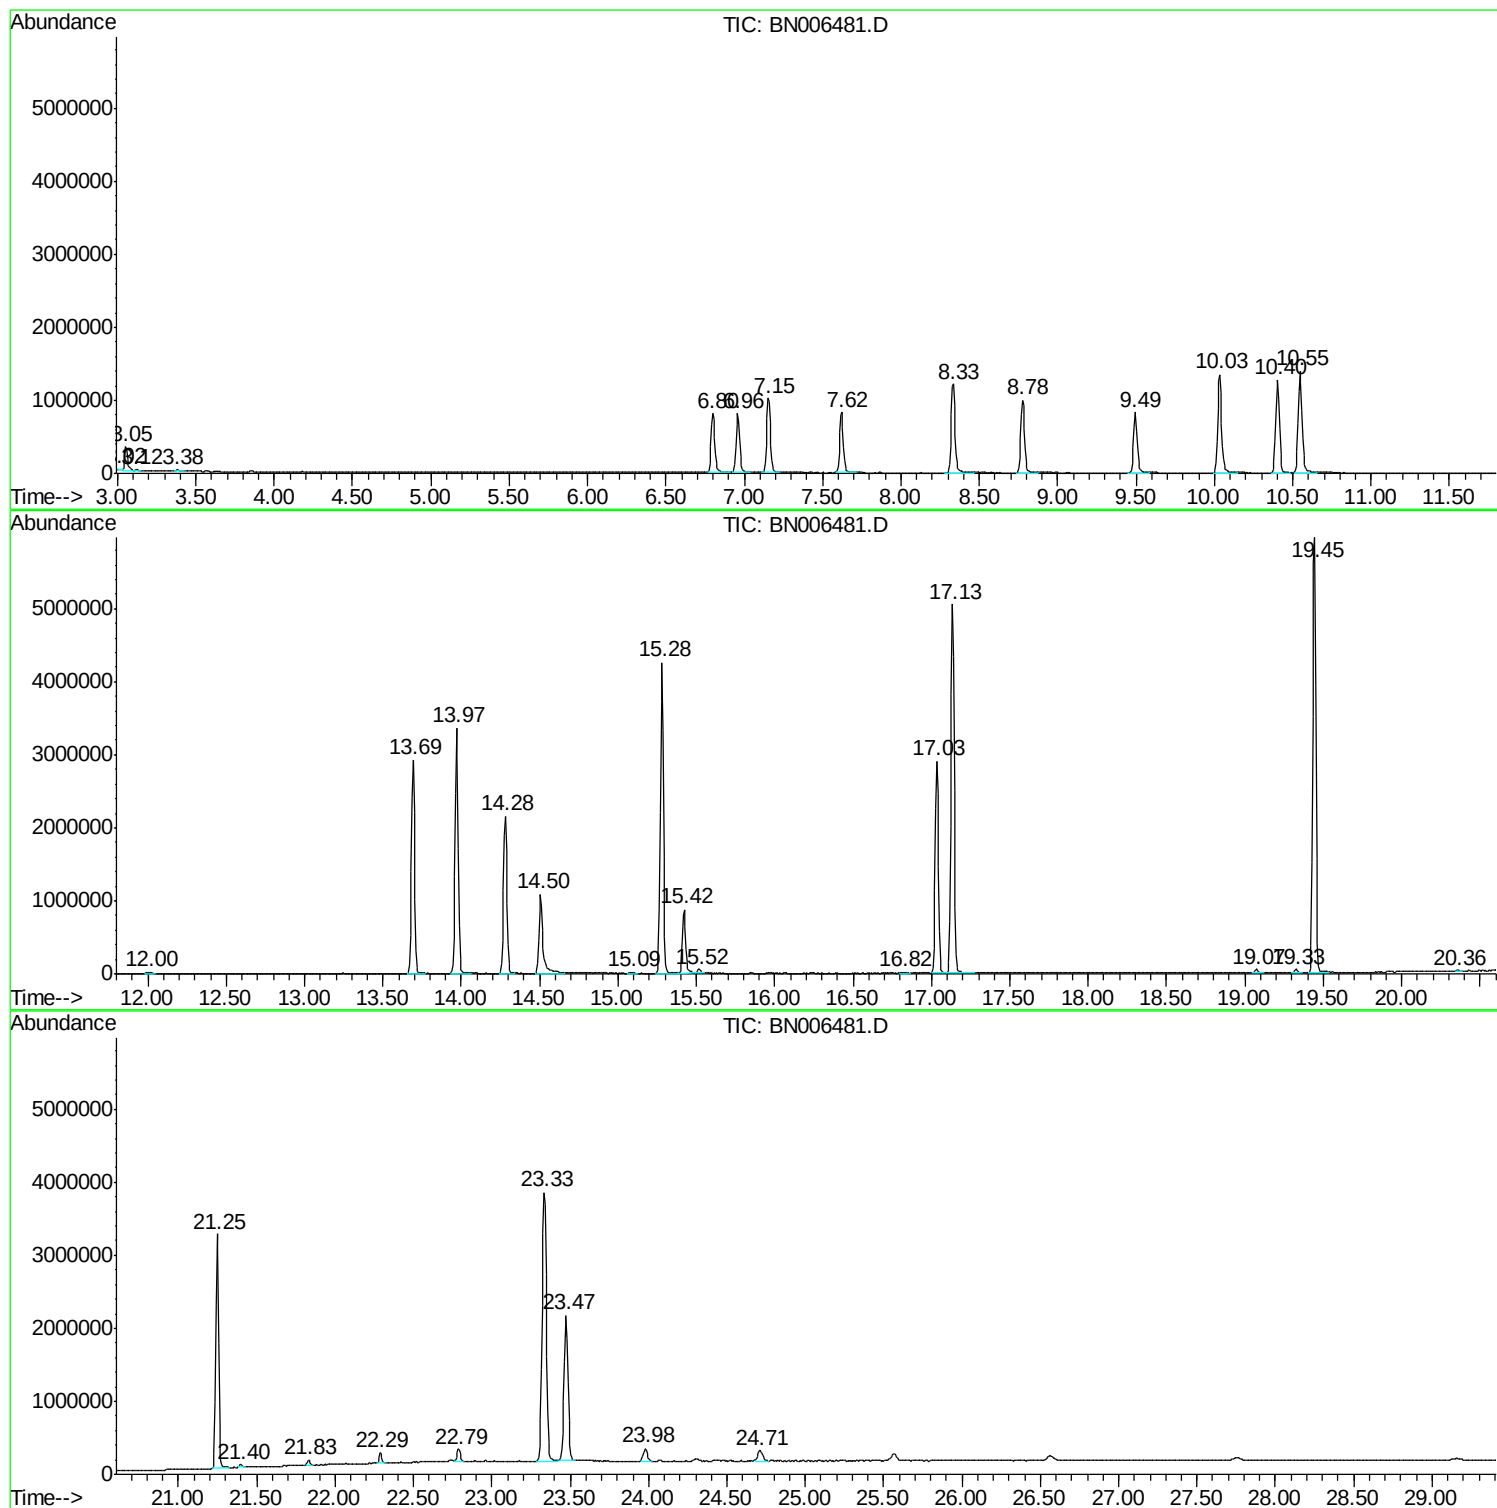

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062119\
Data File : BN006481.D
Acq On : 22 Jun 2019 00:33
Operator : HP/JU
Sample : PB120644BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
ABLK44










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.05	5.87 ng/ul	397246	1,4-Dichlorobenzene-d4	7.62

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Heptane	100	C7H16	000142-82-5	95
2		Heptane	100	C7H16	000142-82-5	94
3		Heptane	100	C7H16	000142-82-5	91
4		Heptane	100	C7H16	000142-82-5	87
5		Oxalic acid, isobutyl pentyl ester	216	C11H20O4	1000309-37-0	59

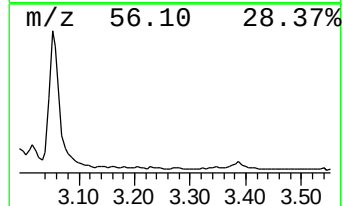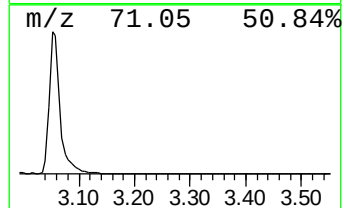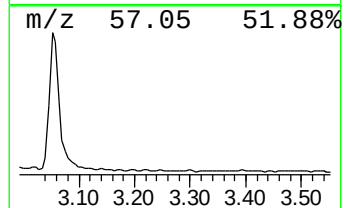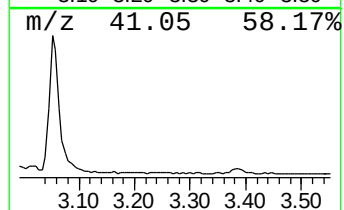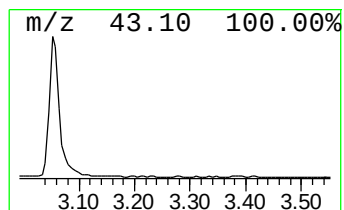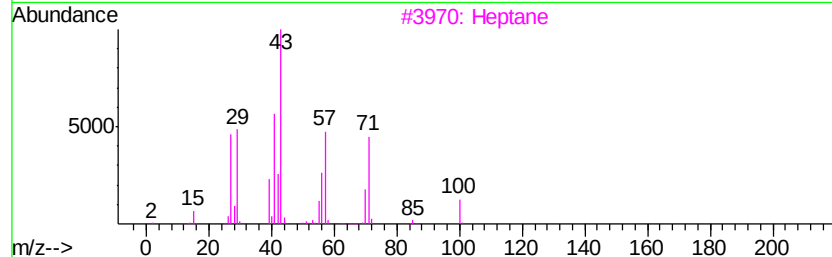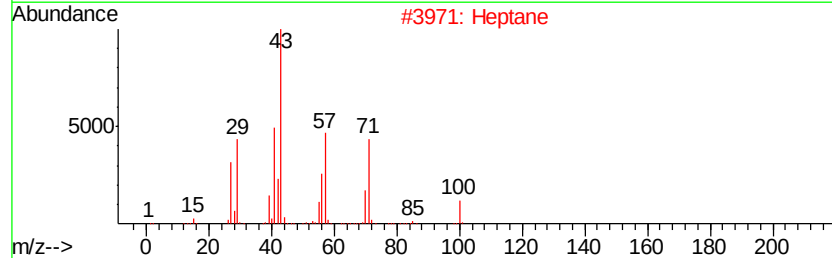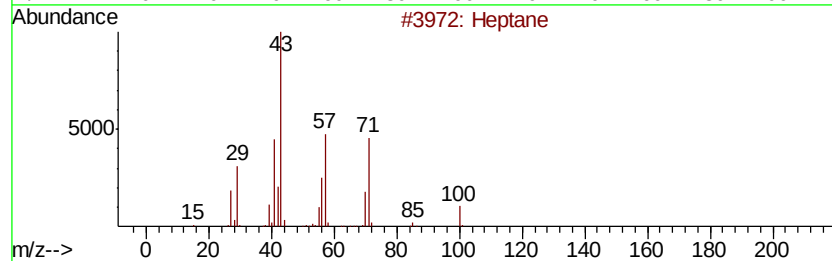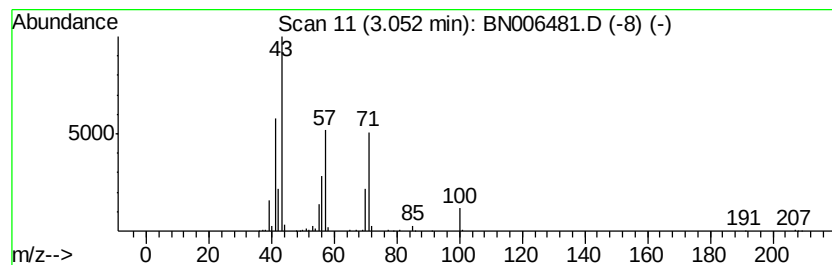

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062119\
Data File : BN006481.D
Acq On : 22 Jun 2019 00:33
Operator : HP/JU
Sample : PB120644BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
ABLK44

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: Str...	3.05	5.9	ng/ul	397246	1	7.62	1354570	20.0