
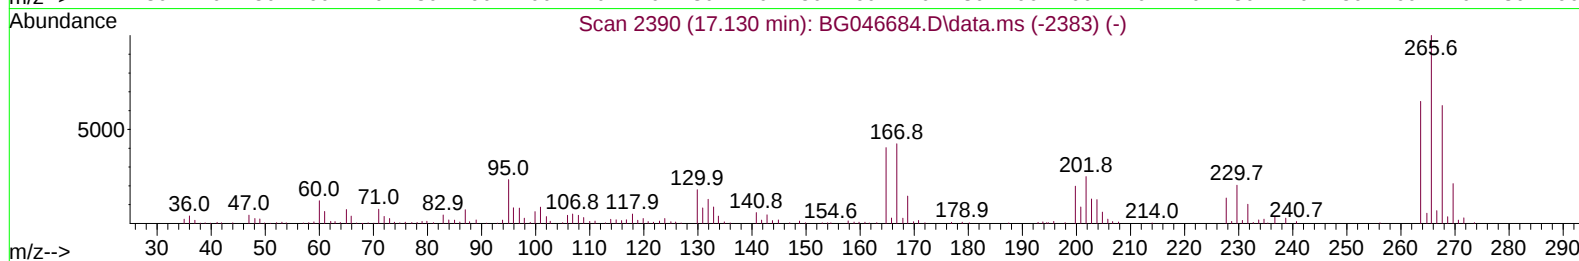
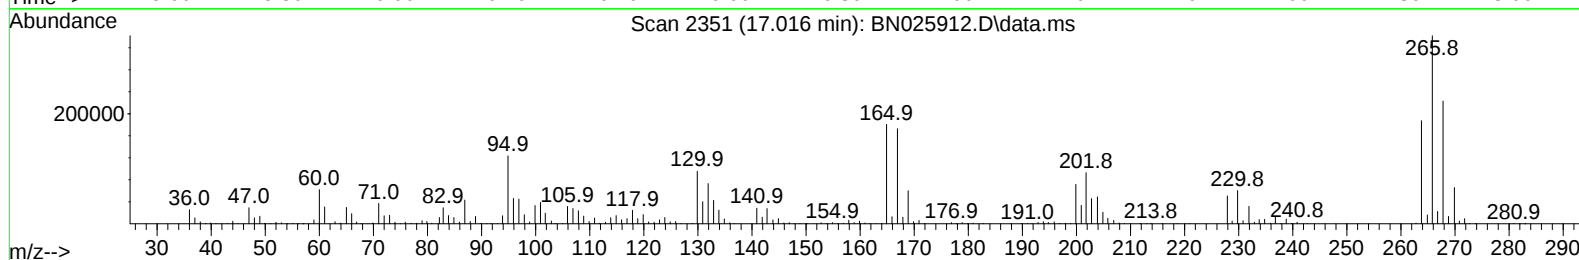


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062123\
 Data File : BN025912.D
 Acq On : 21 Jun 2023 10:57
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 05:47:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 08:56:48 2023
 Response via : Initial Calibration

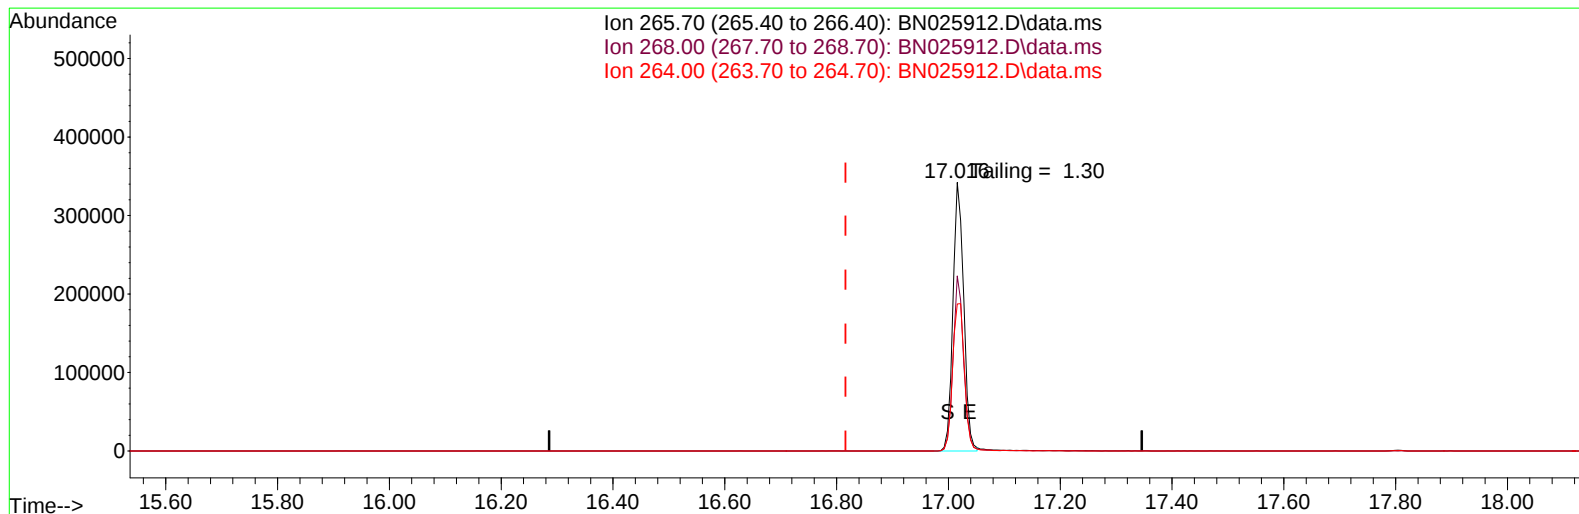

TIC: BN025912.D\data.ms

(70) Pentachlorophenol (C)




17.016min (+ 0.200) 20417.34 ng

response 462264

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.21
264.00	61.60	54.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062123\
Data File : BN025912.D
Acq On : 21 Jun 2023 10:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 05:47:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 08:56:48 2023
Response via : Initial Calibration

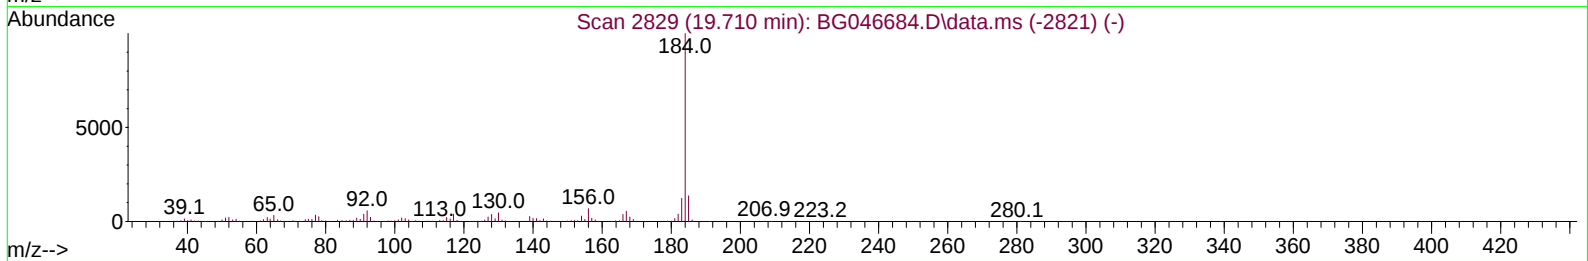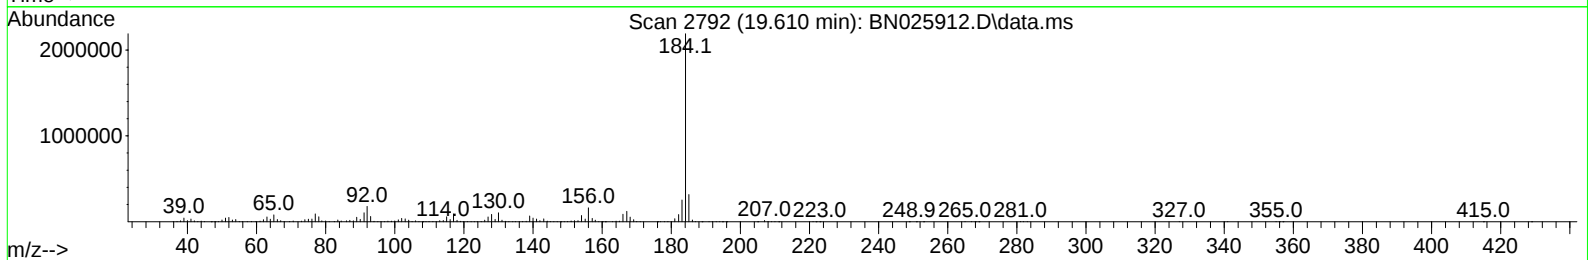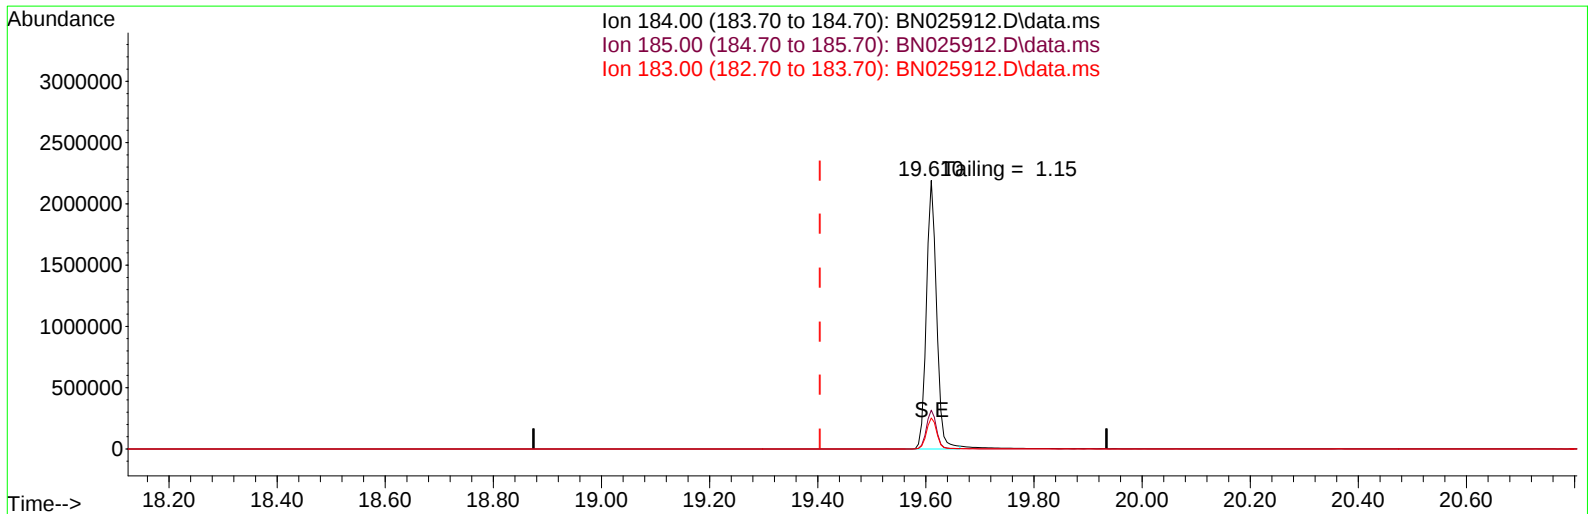

TIC: BN025912.D\data.ms

(77) Benzidine**19.610min (+ 0.206) 0.00 ng****response 2916349**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.45
183.00	13.20	11.54
0.00	0.00	0.00