


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062123\
Data File : BN025912.D
Acq On : 21 Jun 2023 10:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\BNDDTBREAKDOWN-8270.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 01 16:14:27 2010

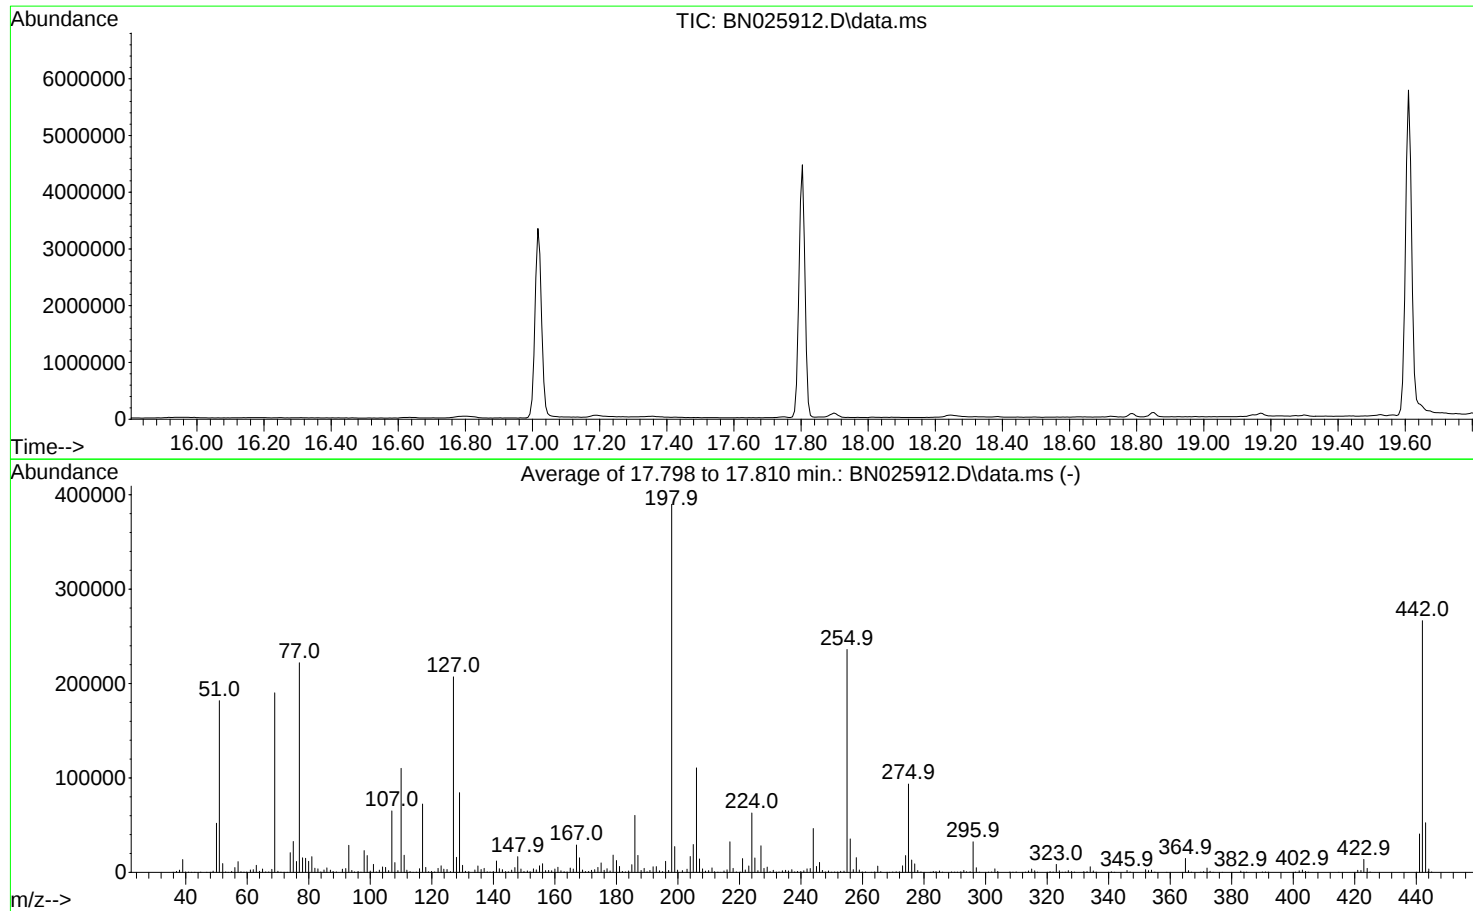




AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.7	181894	PASS
68	69	0.00	2	1.7	3220	PASS
69	198	0.00	100	48.8	190206	PASS
70	69	0.00	2	0.6	1193	PASS
127	198	10	80	53.1	207125	PASS
197	198	0.00	2	0.5	1947	PASS
198	198	100	100	100.0	389717	PASS
199	198	5	9	7.0	27267	PASS
275	198	10	60	24.0	93432	PASS
365	198	1	100	3.8	14699	PASS
441	442	0.01	24	15.2	40640	PASS
442	198	50	100	68.4	266603	PASS
443	442	15	24	19.7	52443	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062123\
Data File : BN025912.D
Acq On : 21 Jun 2023 10:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 22 05:47:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 08:56:48 2023
Response via : Initial Calibration

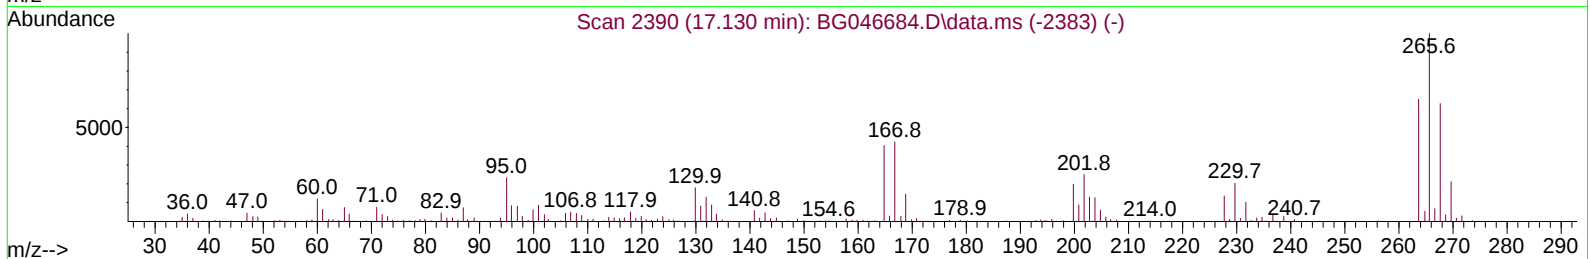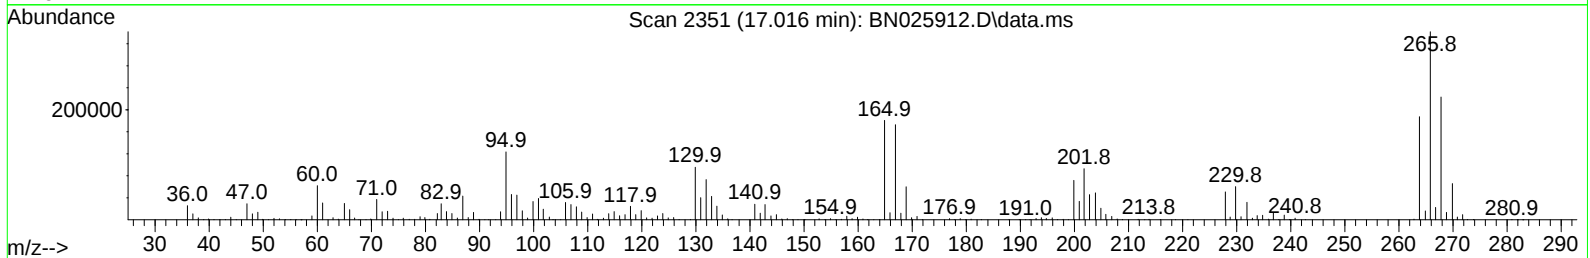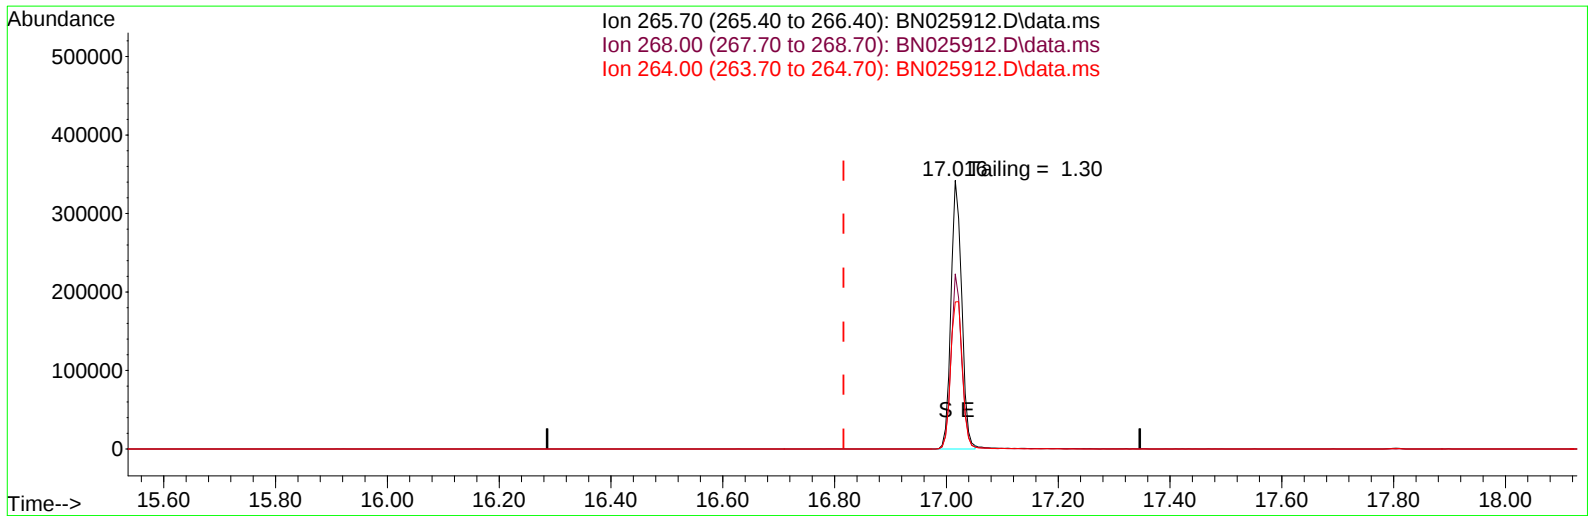

TIC: BN025912.D\data.ms

(70) Pentachlorophenol (C)

17.016min (+ 0.200) 20417.34 ng




response 462264

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.21
264.00	61.60	54.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062123\
Data File : BN025912.D
Acq On : 21 Jun 2023 10:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 22 05:47:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 08:56:48 2023
Response via : Initial Calibration

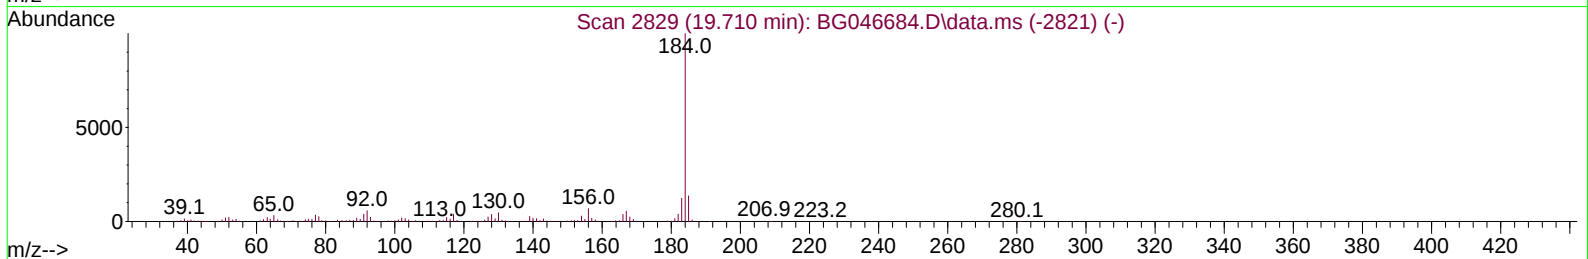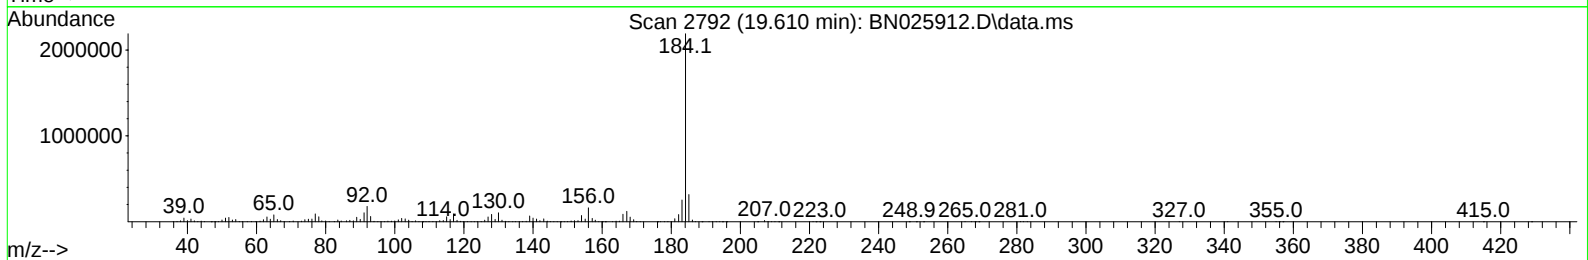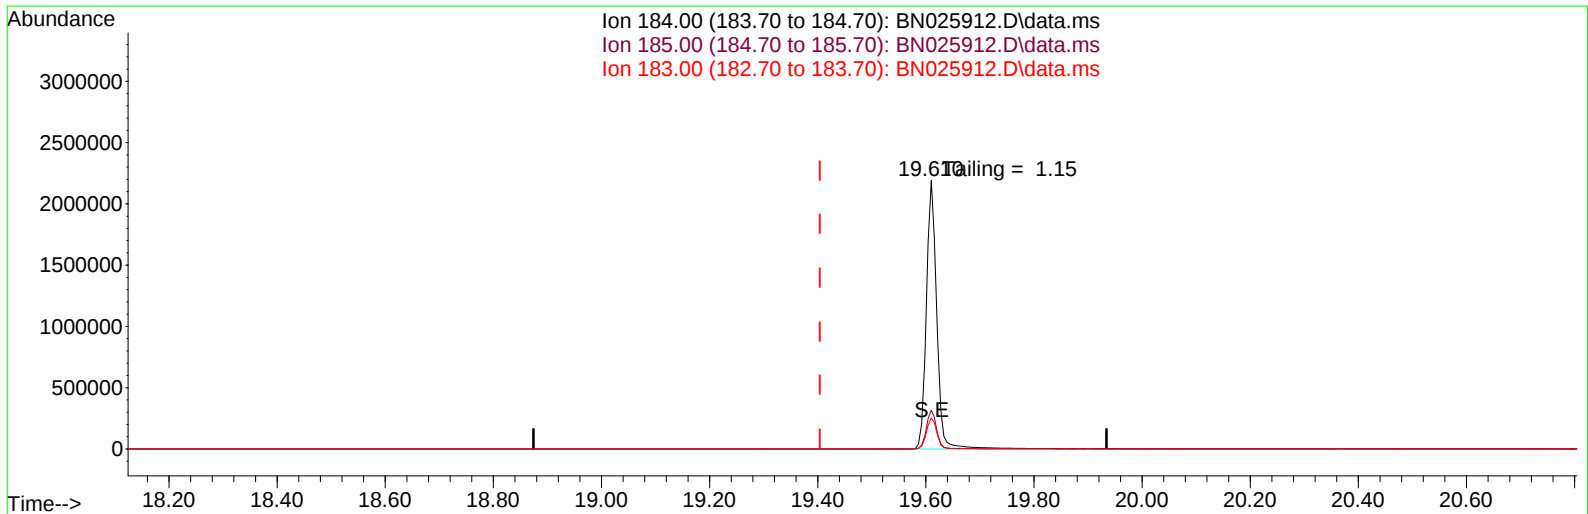

TIC: BN025912.D\data.ms

(77) Benzidine

19.610min (+ 0.206) 0.00 ng

response 2916349

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.45
183.00	13.20	11.54
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/21/2023	BNA_N	<u>BN025912.D</u>
Compound Name	Response	Retention Time
DDT	1291226	20.845
DDD	42986	20.586
DDE	1821	19.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
44807	1336033	3.35

Instrument :
BNA_N
ClientSampleId :
DFTPP