

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062219\
 Data File : BN006492.D
 Acq On : 22 Jun 2019 16:57
 Operator : HP/JU
 Sample : PB120667BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK67

Quant Time: Jun 24 04:05:57 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 21 22:42:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	279756	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	1271712	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.28	164	748235	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.03	188	1596928	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	1213358	20.00	ng/ul	0.00
85) Perylene-d12	23.49	264	1155358	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	54069	7.55	ng/uL	0.00
5) Phenol-d5	6.80	99	937984	31.49	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	591577	32.08	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	724860	33.00	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	741587	31.38	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	362495	35.60	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	403718	36.39	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	689331	32.34	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	1026551	41.88	ng/ul	0.00
43) Dimethylphthalate-d6	13.69	166	2137285	32.59	ng/ul	0.00
46) Acenaphthylene-d8	13.97	160	2731707	33.98	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	318619	28.44	ng/ul	0.00
57) Fluorene-d10	15.28	176	1815751	32.55	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	243055	24.05	ng/ul	0.00
70) Anthracene-d10	17.13	188	2703868	33.63	ng/ul	0.00
78) Pyrene-d10	19.45	212	2782027	39.25	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.36	264	2074847	31.79	ng/ul	0.00


Target Compounds					Qvalue
45) 2,6-Dinitrotoluene	13.69	165	15816	1.342	ng/ul# 37


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062219\
Data File : BN006492.D
Acq On : 22 Jun 2019 16:57
Operator : HP/JU
Sample : PB120667BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK67

Quant Time: Jun 24 04:05:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 21 22:42:34 2019
Response via : Initial Calibration

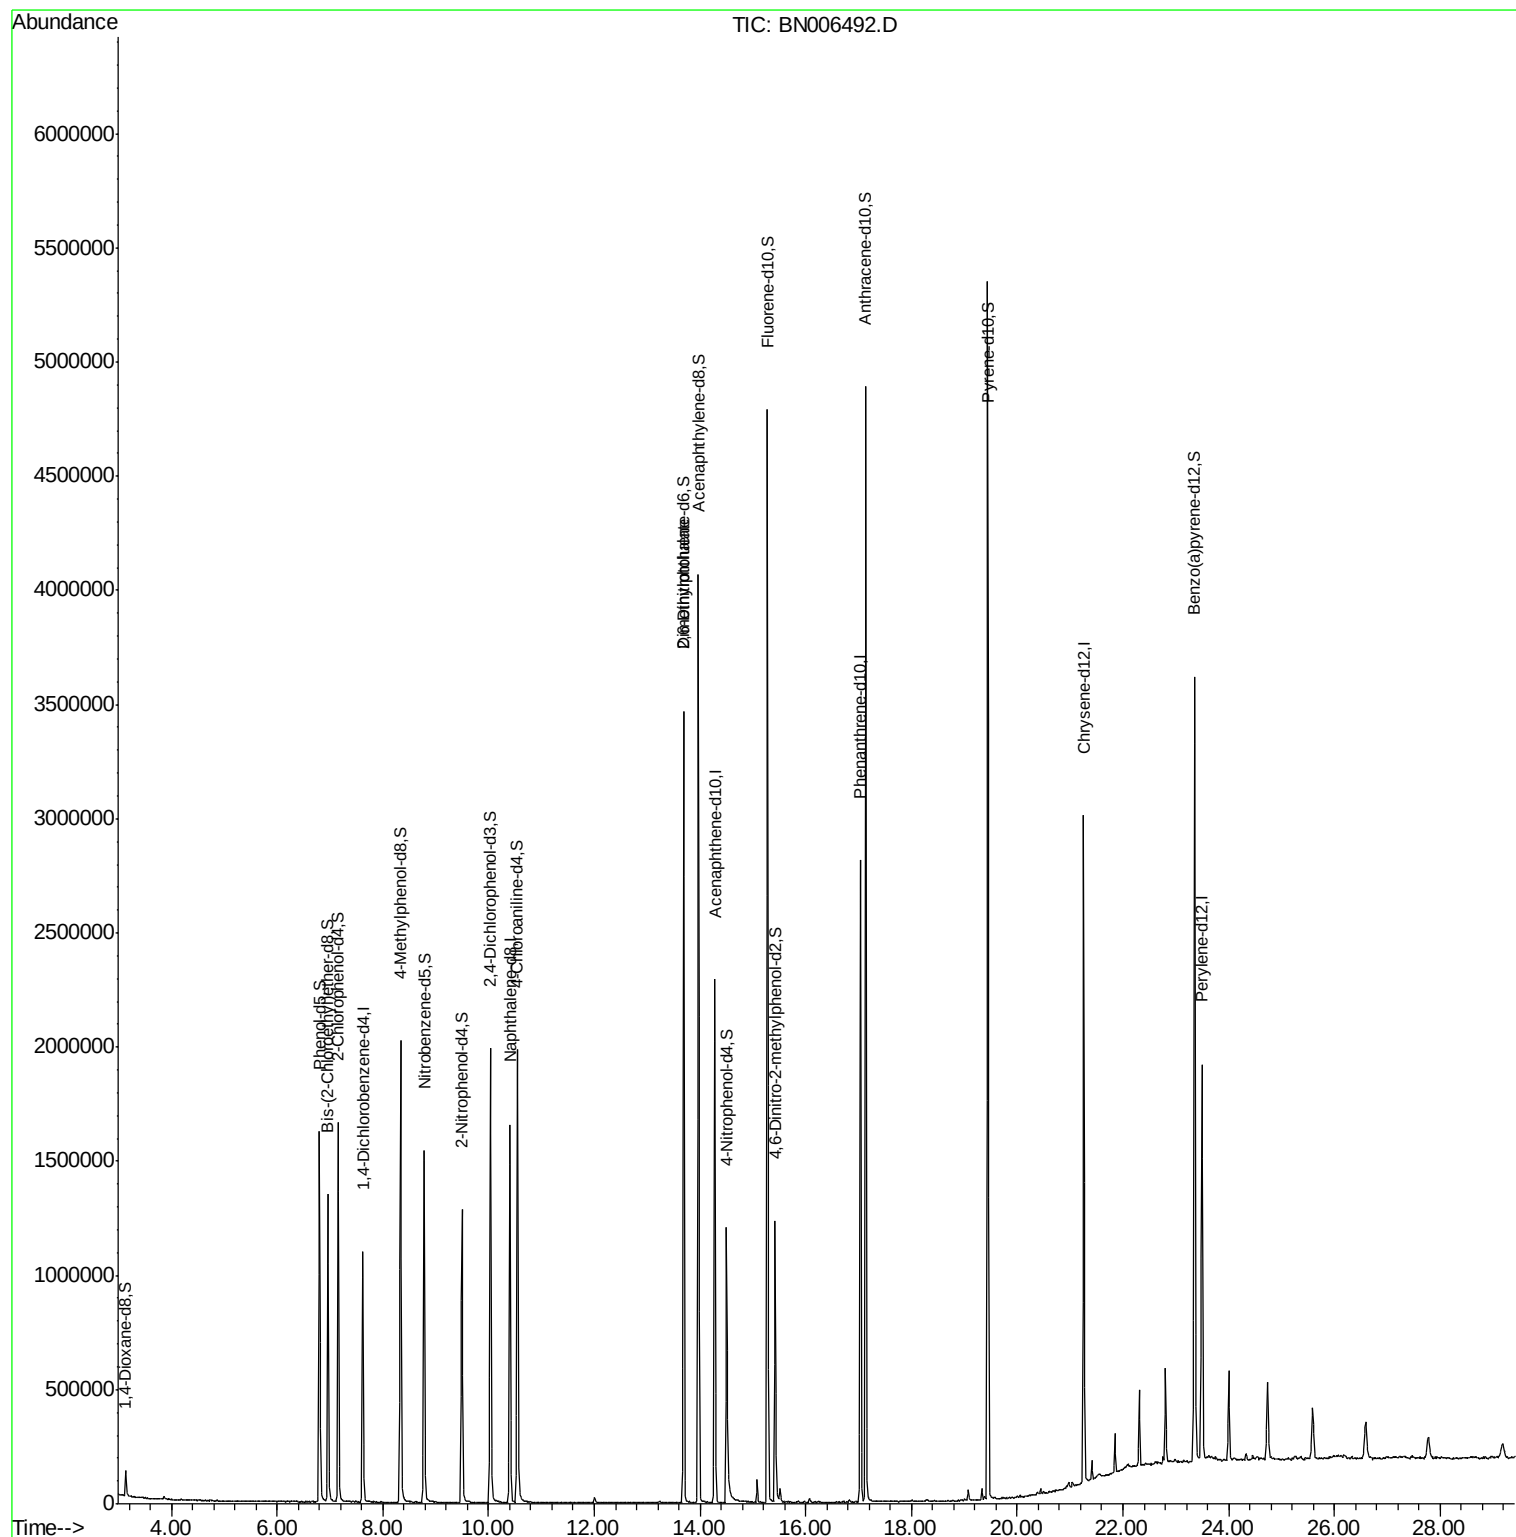


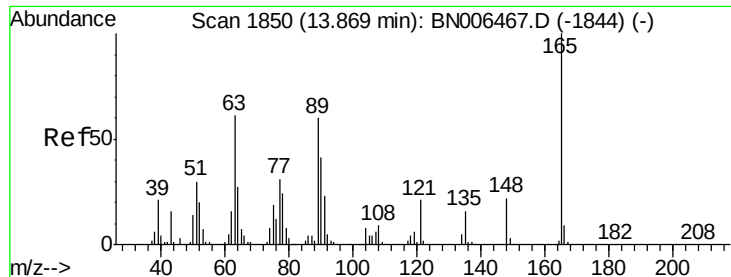

#45
 2,6-Dinitrotoluene
 Concen: 1.342 ng/ul
 RT: 13.69 min Scan# 1820
 Delta R.T. -0.18 min
 Lab File: BN006492.D
 Acq: 22 Jun 2019 16:57

Instrument :
 BNA_N
 ClientSampleId :
 SBLK67

Tgt Ion	Ratio	Lower	Upper
165	100		
89	0.0	48.6	72.8#
121	28.9	17.2	25.8#

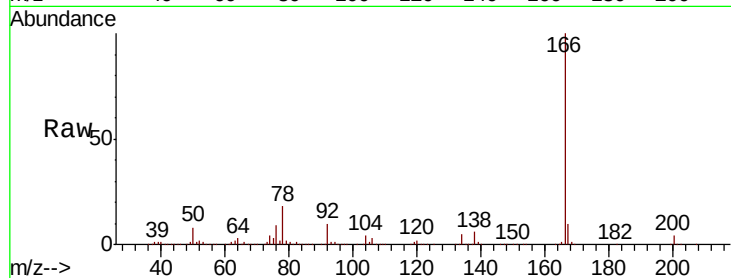

Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 89.00 (88.70 to 89.70): BNC
 Ion 121.00 (120.70 to 121.70): E

