


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062219\
Data File : BN006504.D
Acq On : 22 Jun 2019 23:51
Operator : HP/JU
Sample : K3360-10
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jun 24 09:21:28 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

Instrument :
BNA_N
Client Sample ID :
A41Z0

Manual Integrations
APPROVED

mohammad
6/25/2019 8:44:56 AM

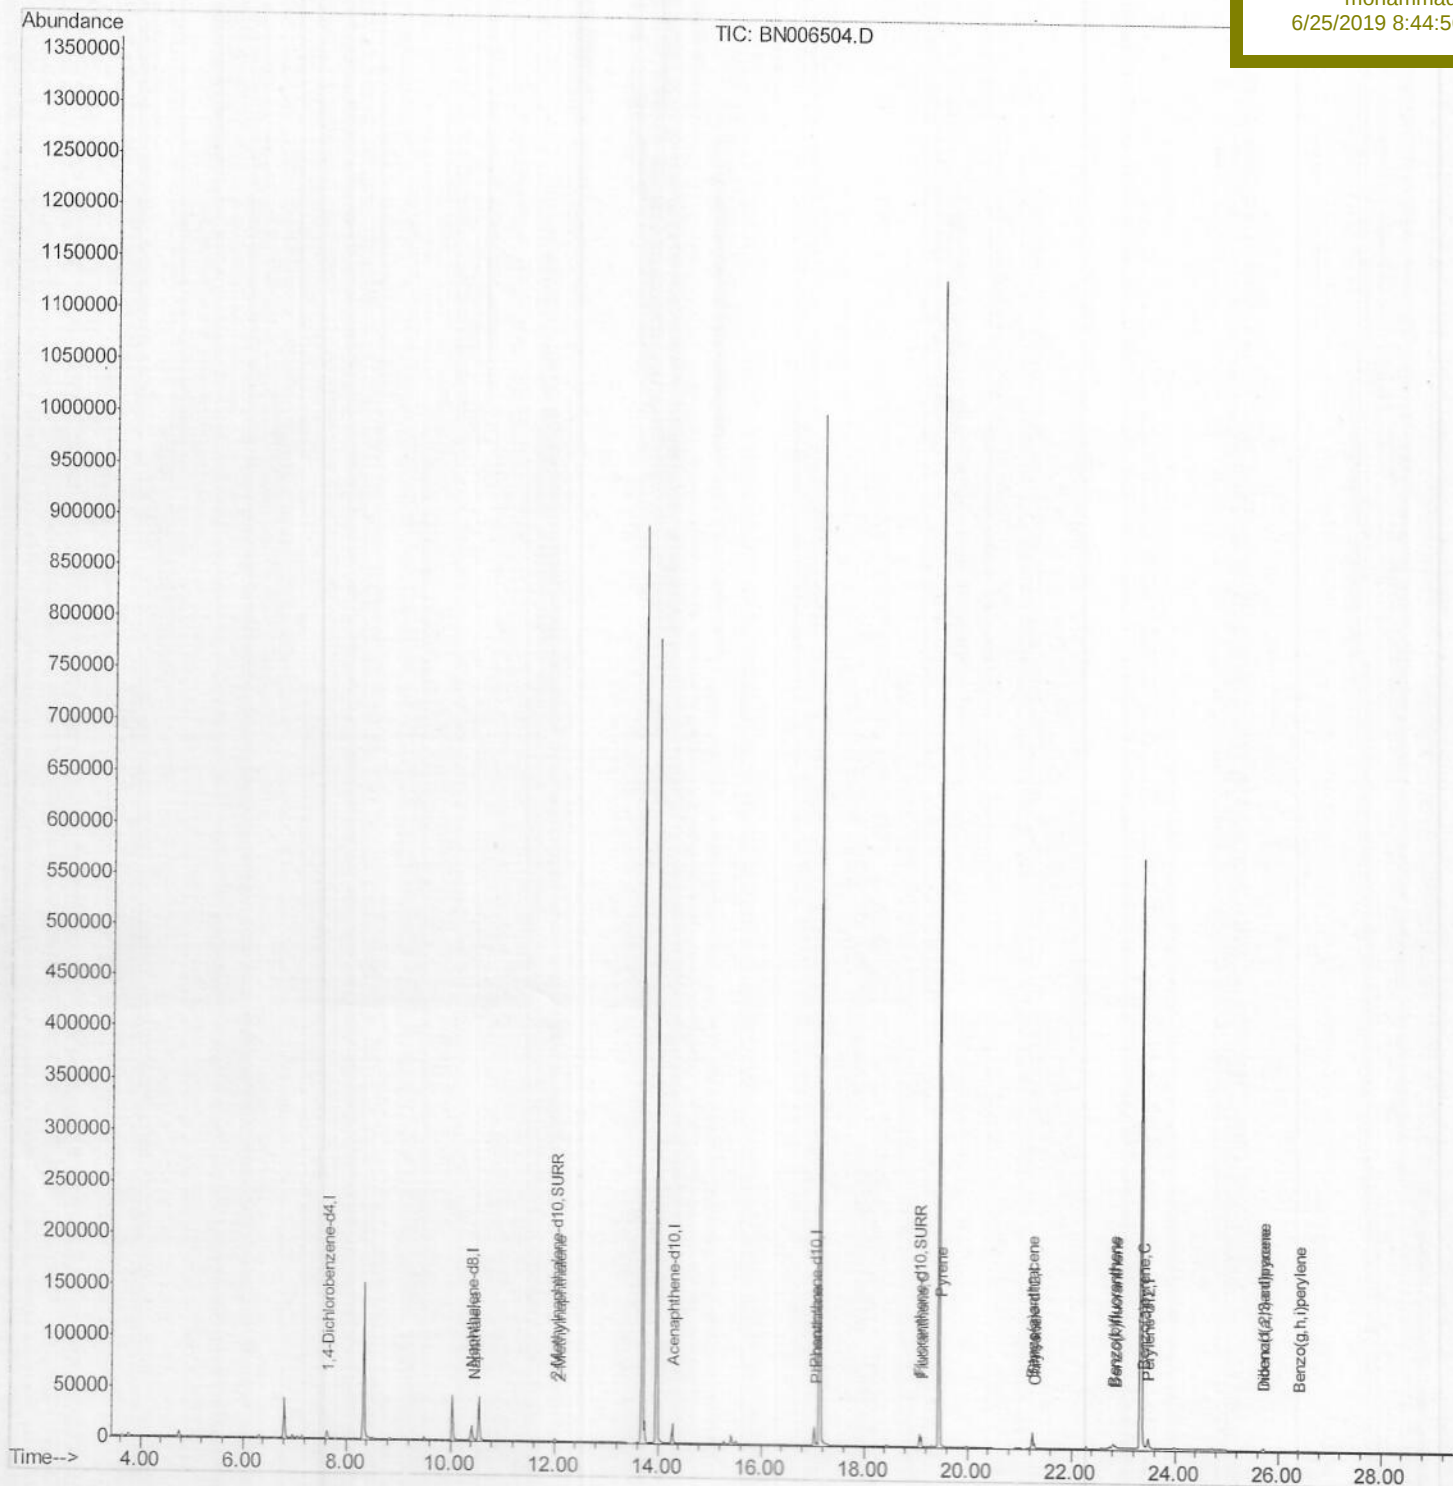

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062219\

Data File : BN006504.D

Acq On : 22 Jun 2019 23:51

Operator : HP/JU

Sample : K3360-10

Misc :

ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jun 24 09:14:46 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N


ClientSampleId :

A41Z0

Manual Integrations
APPROVED

mohammad

6/25/2019 8:44:56 AM

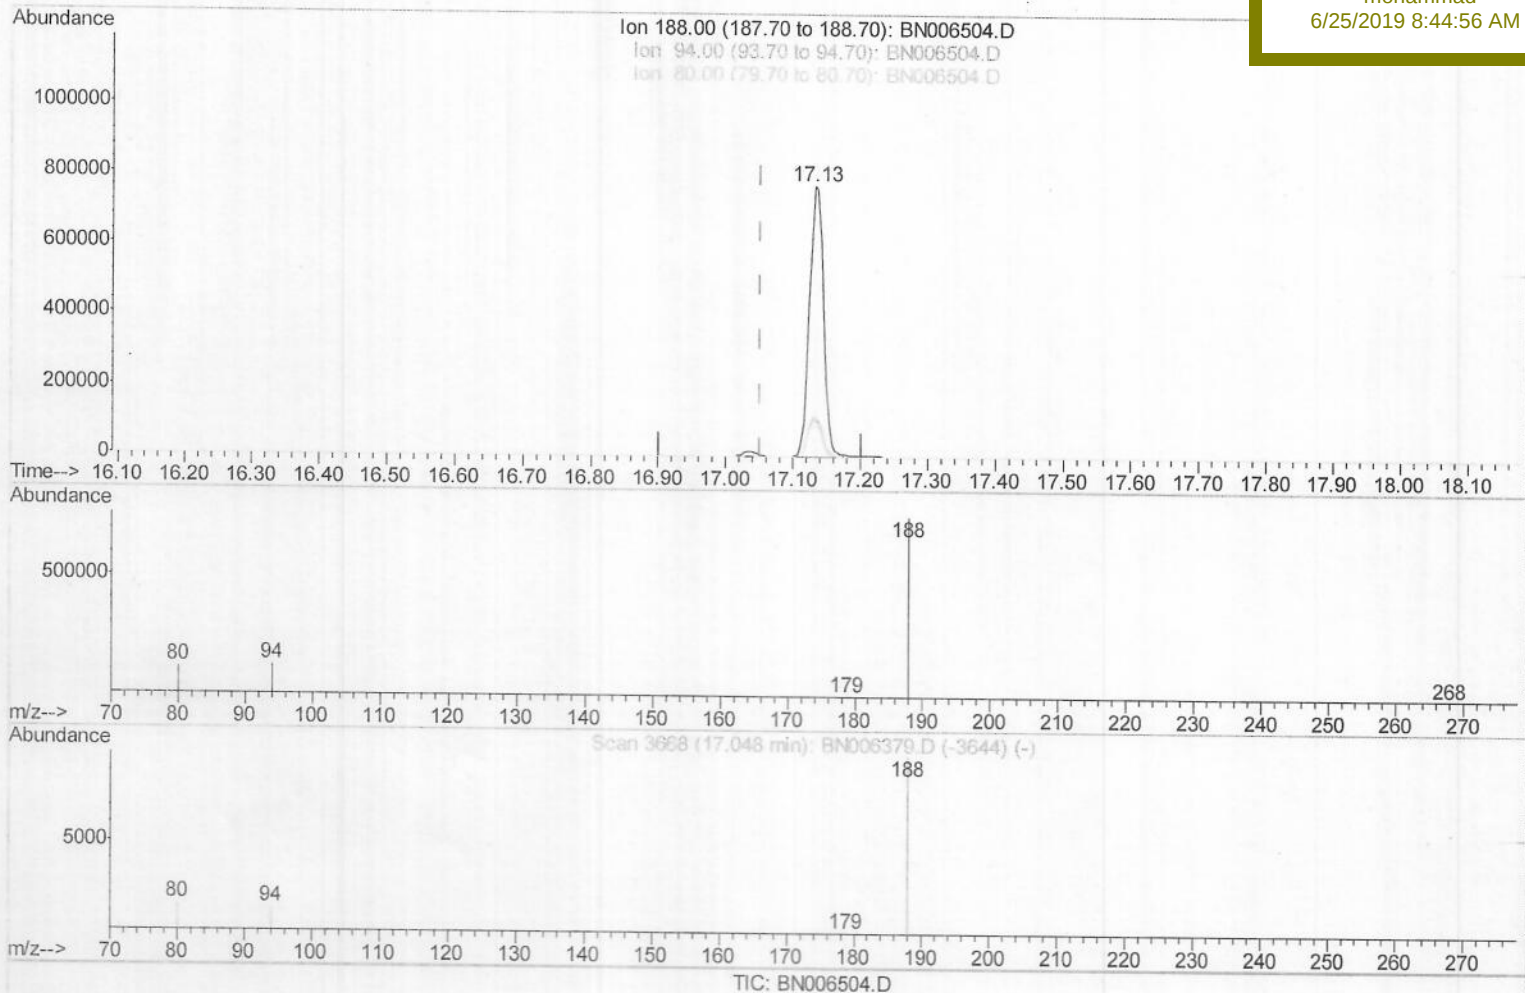

(10) Phenanthrene-d10 (I)

17.133min (+0.080) 0.40ng/ul

response 1108397

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	15.97#
80.00	13.60	14.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062219\

Data File : BN006504.D

Acq On : 22 Jun 2019 23:51

Operator : HP/JU

Sample : K3360-10

Misc :

ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jun 24 09:14:46 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019



Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A41Z0

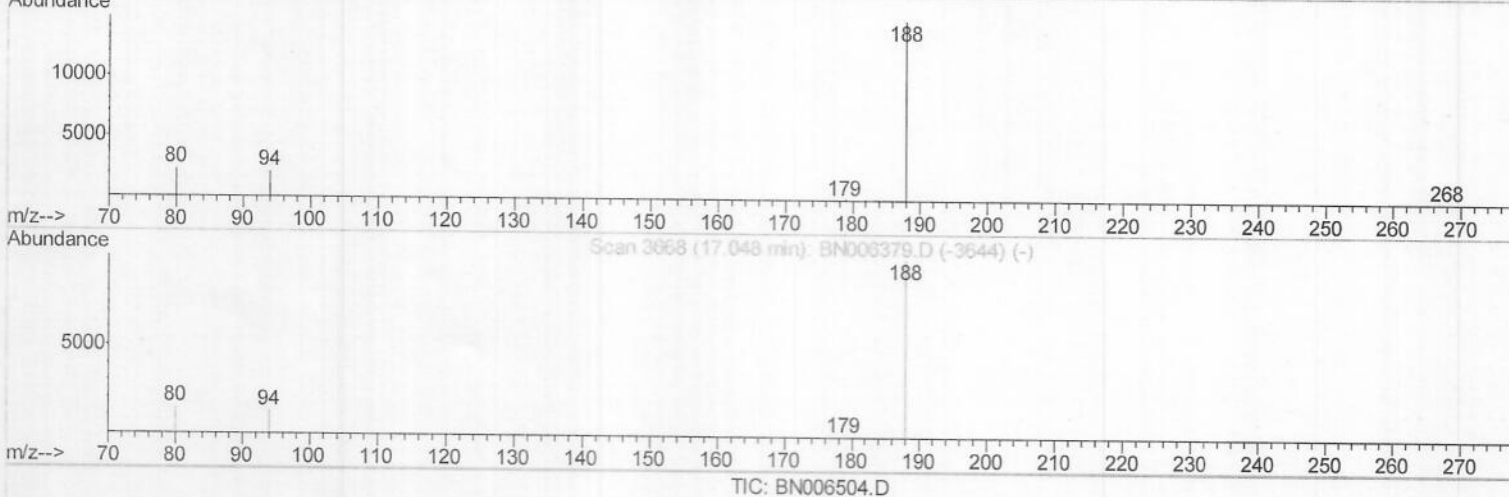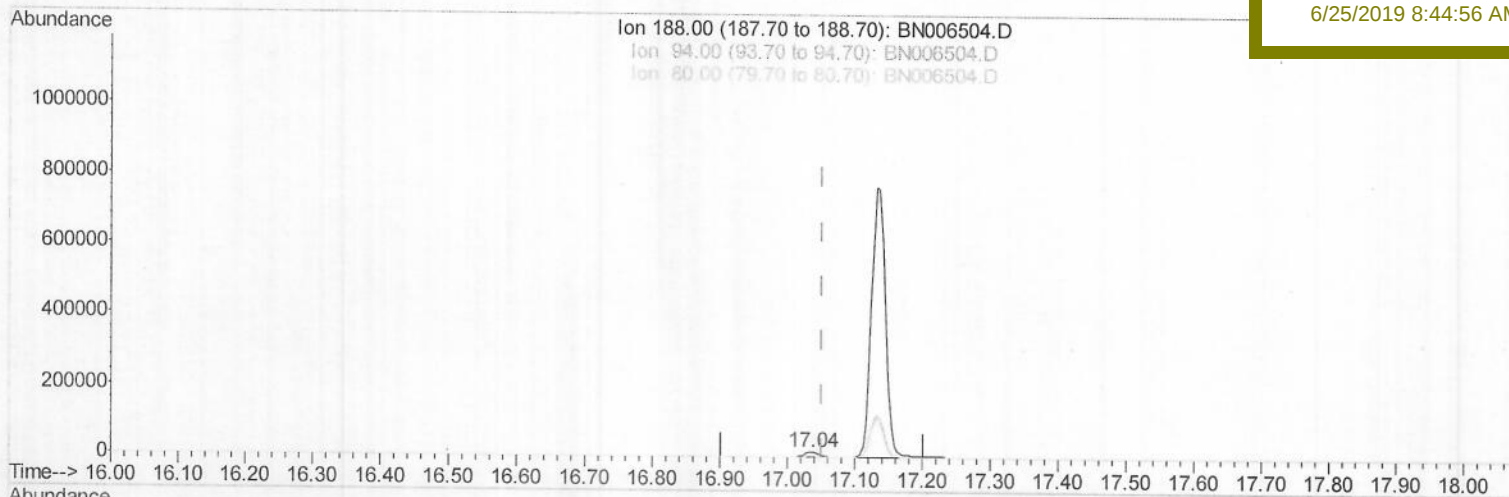Manual Integrations
APPROVEDmohammad
6/25/2019 8:44:56 AM

(10) Phenanthrene-d10 (I)

17.035min (-0.017) 0.40ng/ul m

response 22483

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	14.02
80.00	13.60	15.68
0.00	0.00	0.00

> JU 06126119

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062219\

Data File : BN006504.D

Acq On : 22 Jun 2019 23:51

Operator : HP/JU

Sample : K3360-10

Misc :

ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jun 24 09:16:42 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019




Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A41Z0

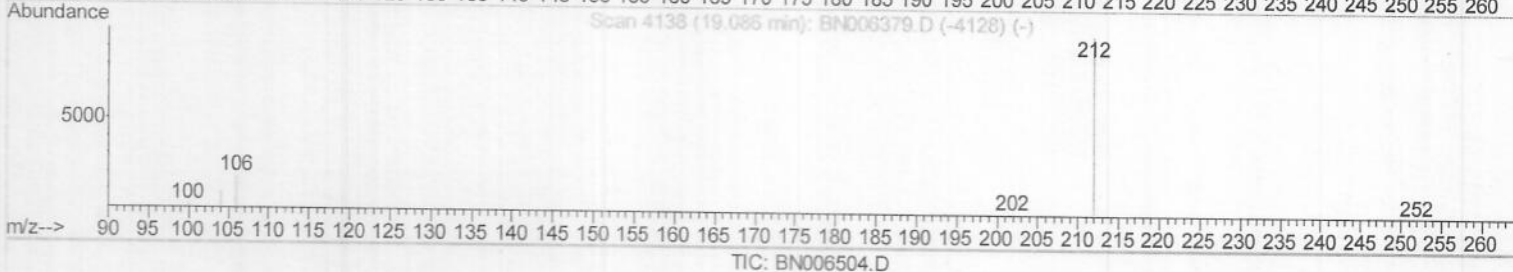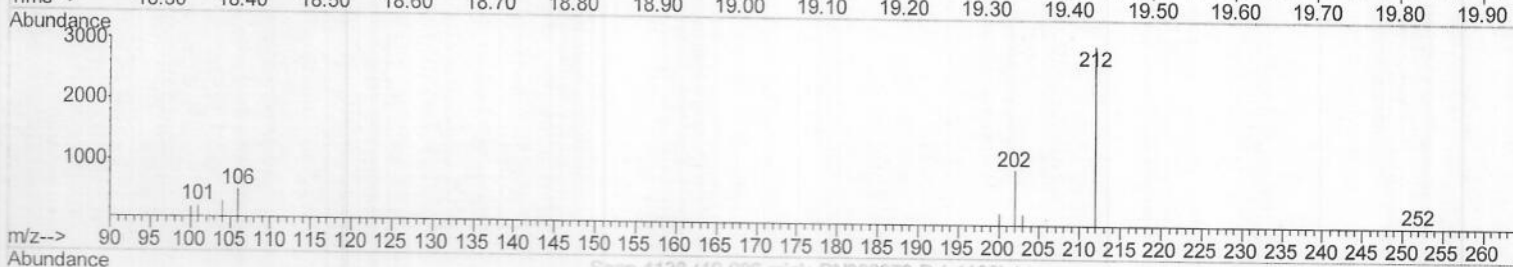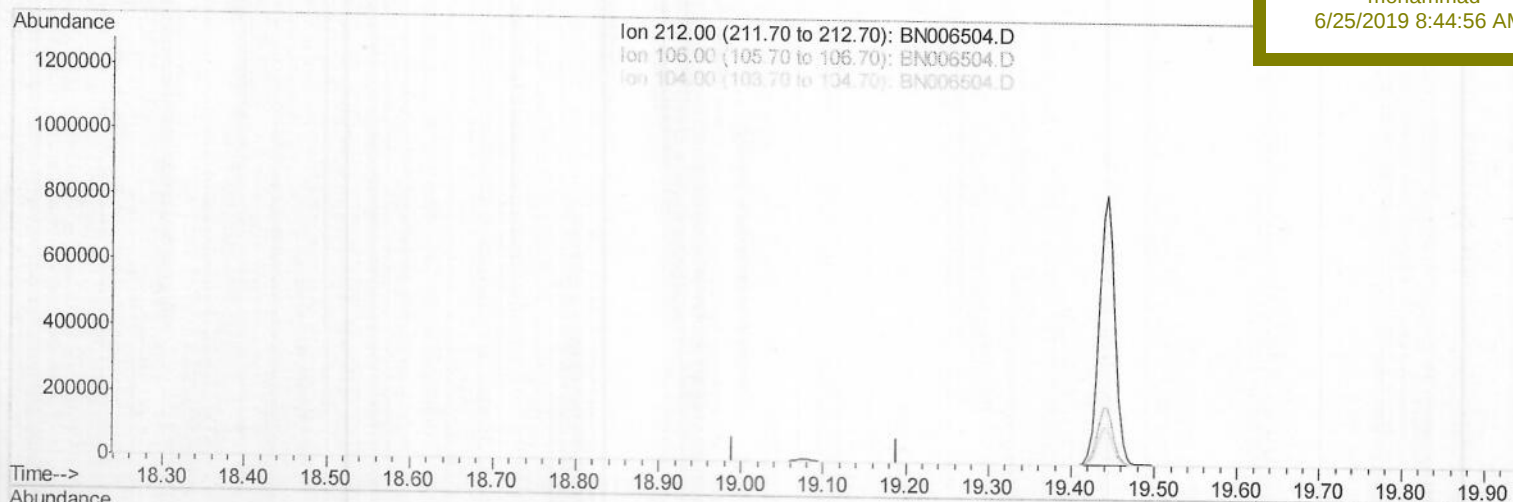Manual Integrations
APPROVEDmohammad
6/25/2019 8:44:56 AM

(14) Fluoranthene-d10 (SURR)

19.090min (-19.090) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062219\
 Data File : BN006504.D
 Acq On : 22 Jun 2019 23:51
 Operator : HP/JU
 Sample : K3360-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A41Z0

Manual Integrations
 APPROVED

mohammad
 6/25/2019 8:44:56 AM

Quant Time: Jun 24 09:16:42 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

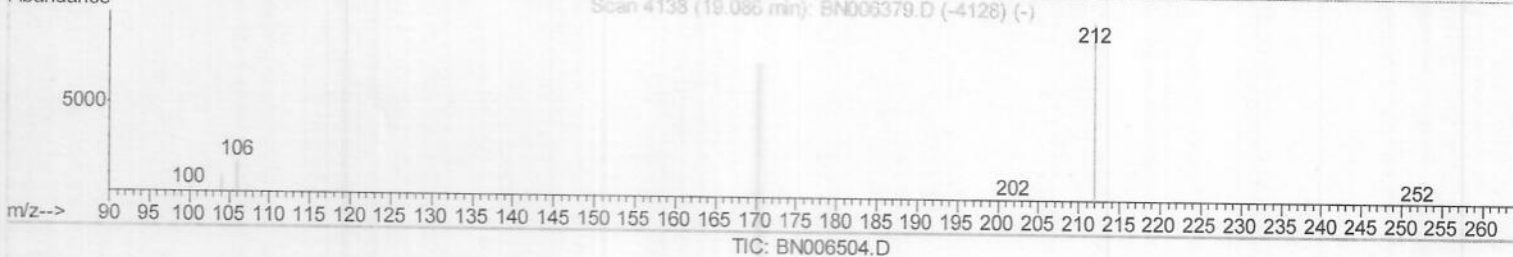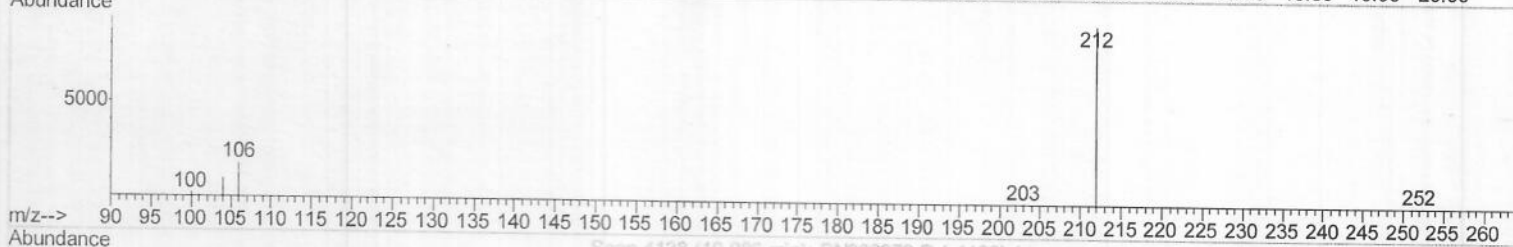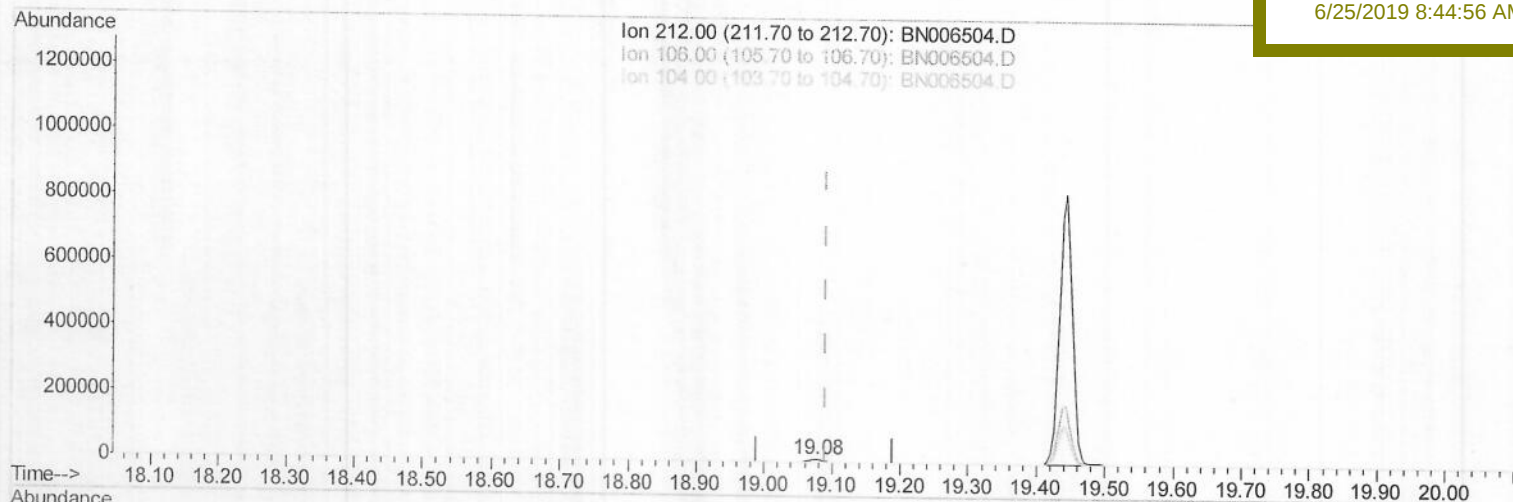

(14) Fluoranthene-d10 (SURR)

19.076min (-0.014) 0.22ng/ul m

JU 06/26/19

response 13086

Ion	Exp%	Act%
212.00	100	100
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062219\

Data File : BN006504.D

Acq On : 22 Jun 2019 23:51

Operator : HP/JU

Sample : K3360-10

Misc :

ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jun 24 09:16:42 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A41Z0

Manual Integrations

APPROVED

mohammad

6/25/2019 8:44:56 AM

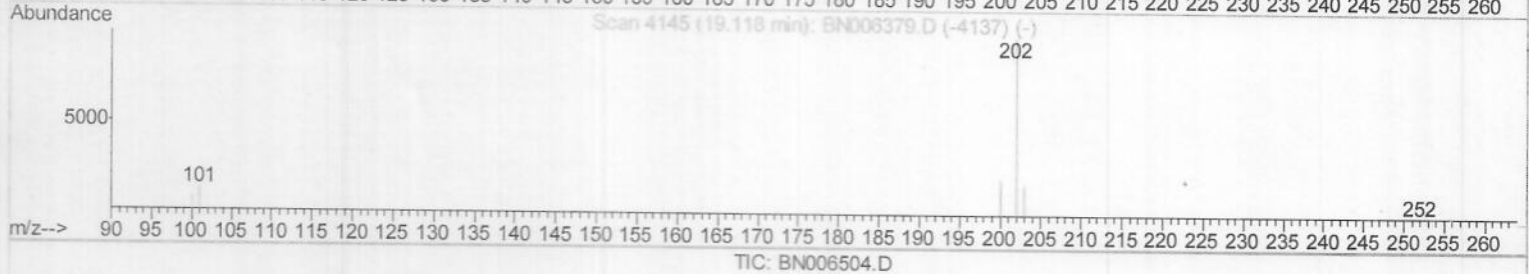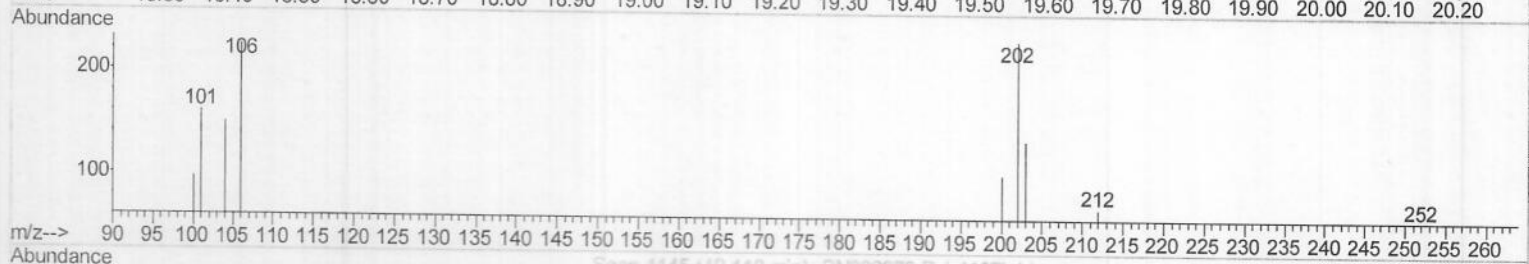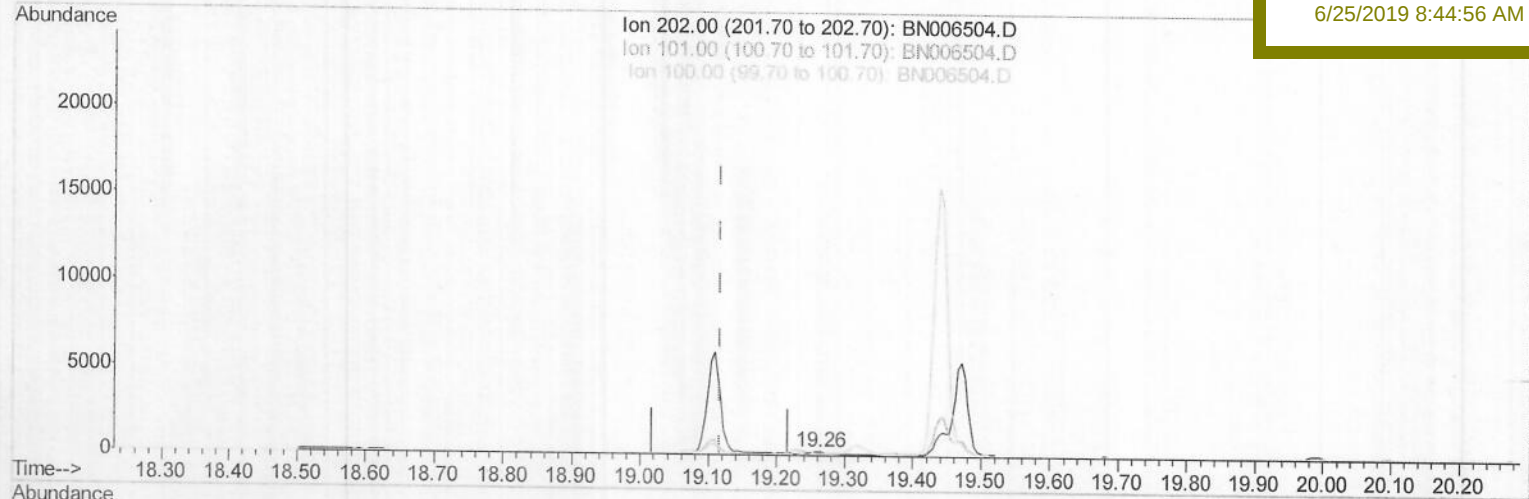

(15) Fluoranthene (C)

19.262min (+0.144) 0.00ng/ul

response 176

Ion	Exp%	Act%
202.00	100	100
101.00	12.10	68.97#
100.00	8.70	41.81#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062219\

Data File : BN006504.D

Acq On : 22 Jun 2019 23:51

Operator : HP/JU

Sample : K3360-10

Misc :

ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jun 24 09:16:42 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A41Z0

Manual Integrations

APPROVED

mohammad

6/25/2019 8:44:56 AM

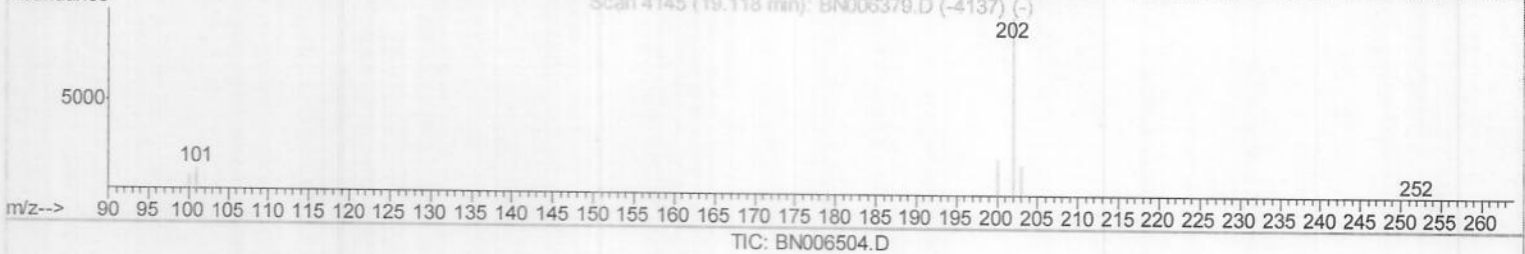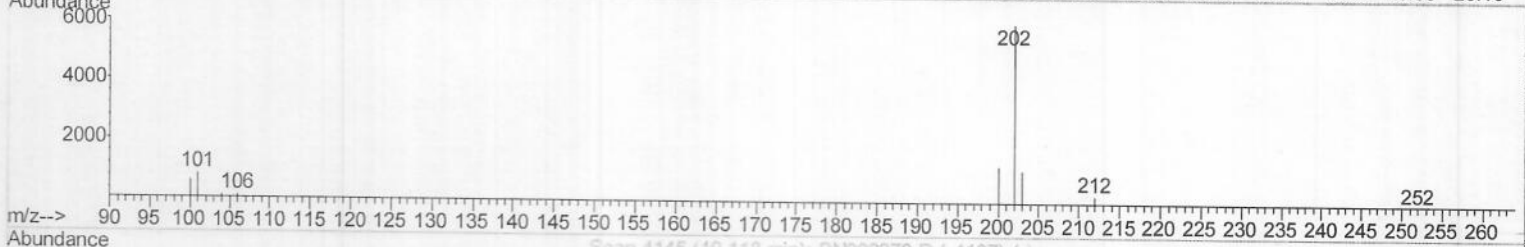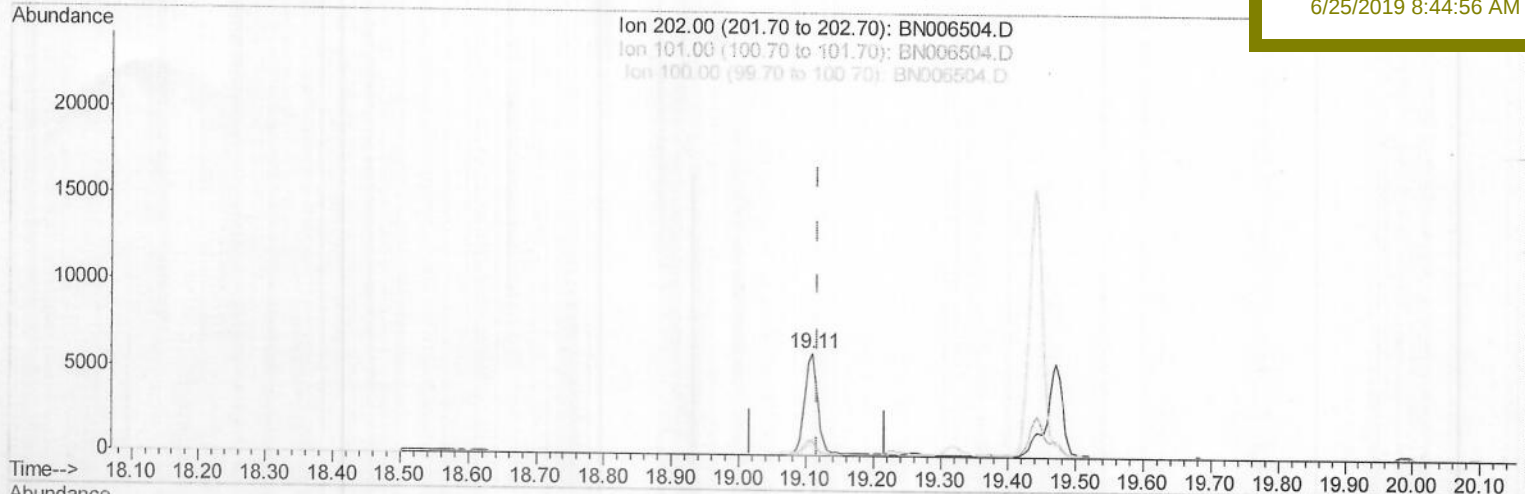

(15) Fluoranthene (C)

19.109min (-0.009) 0.11ng/ul m > JU 06/26/19

response 8487

Ion	Exp%	Act%
202.00	100	100
101.00	12.10	13.96
100.00	8.70	10.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062219\

Data File : BN006504.D

Acq On : 22 Jun 2019 23:51

Operator : HP/JU

Sample : K3360-10

Misc :

ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jun 24 09:16:42 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019




Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A41Z0

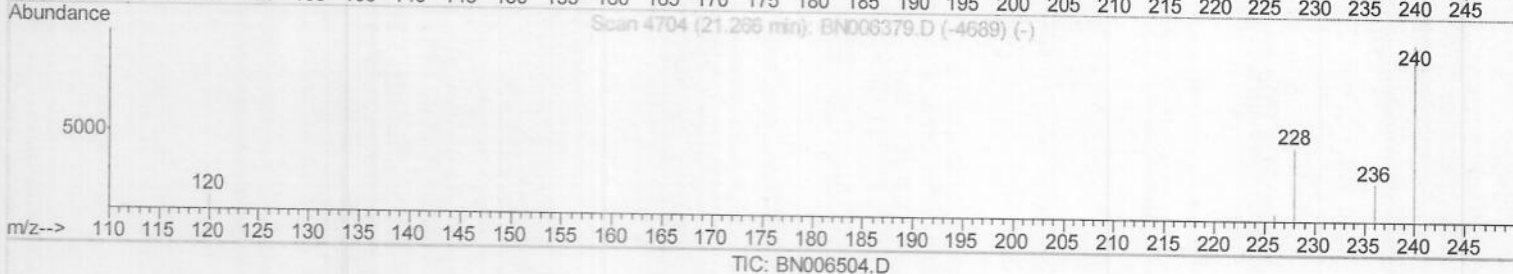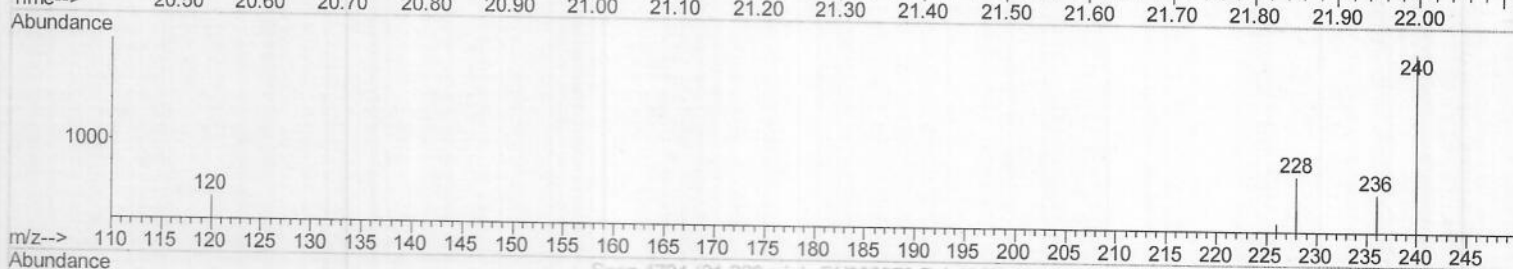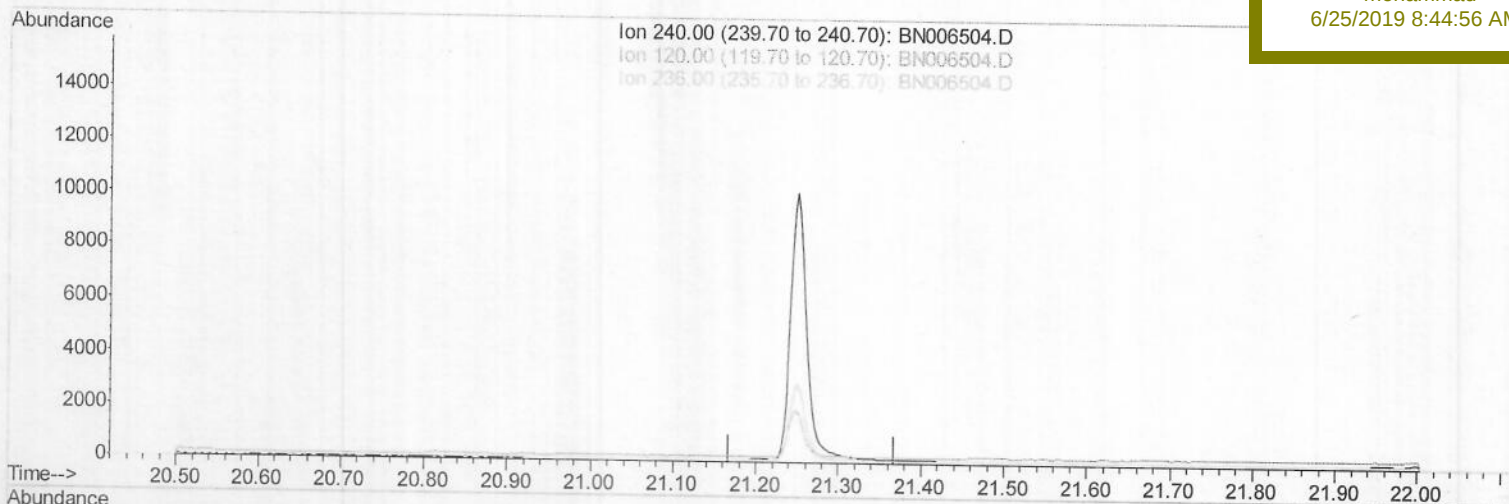Manual Integrations
APPROVEDmohammad
6/25/2019 8:44:56 AM

(16) Chrysene-d12 (I)

21.268min (-21.268) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	20.10	0.00#
236.00	30.10	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062219\

Data File : BN006504.D

Acq On : 22 Jun 2019 23:51

Operator : HP/JU

Sample : K3360-10

Misc :

ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jun 24 09:16:42 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A41Z0

Manual Integrations

APPROVED

mohammad

6/25/2019 8:44:56 AM

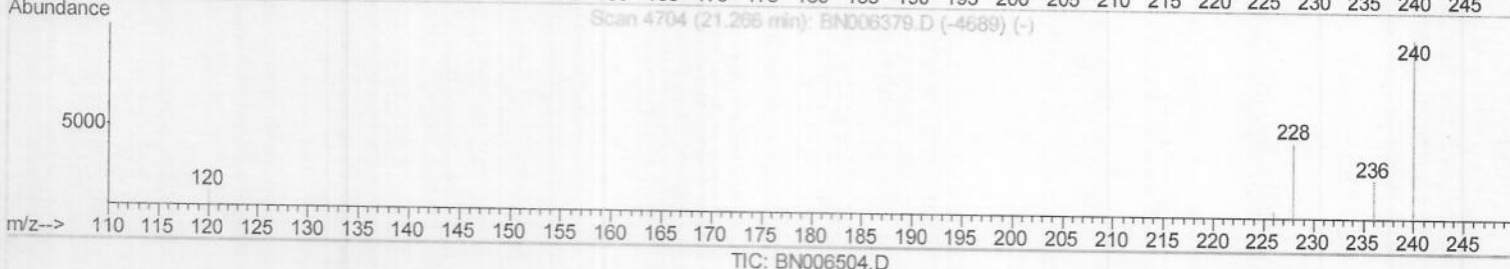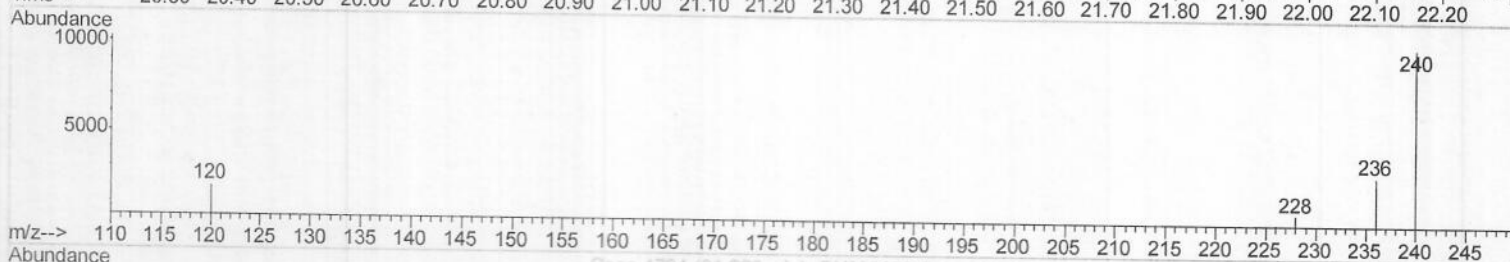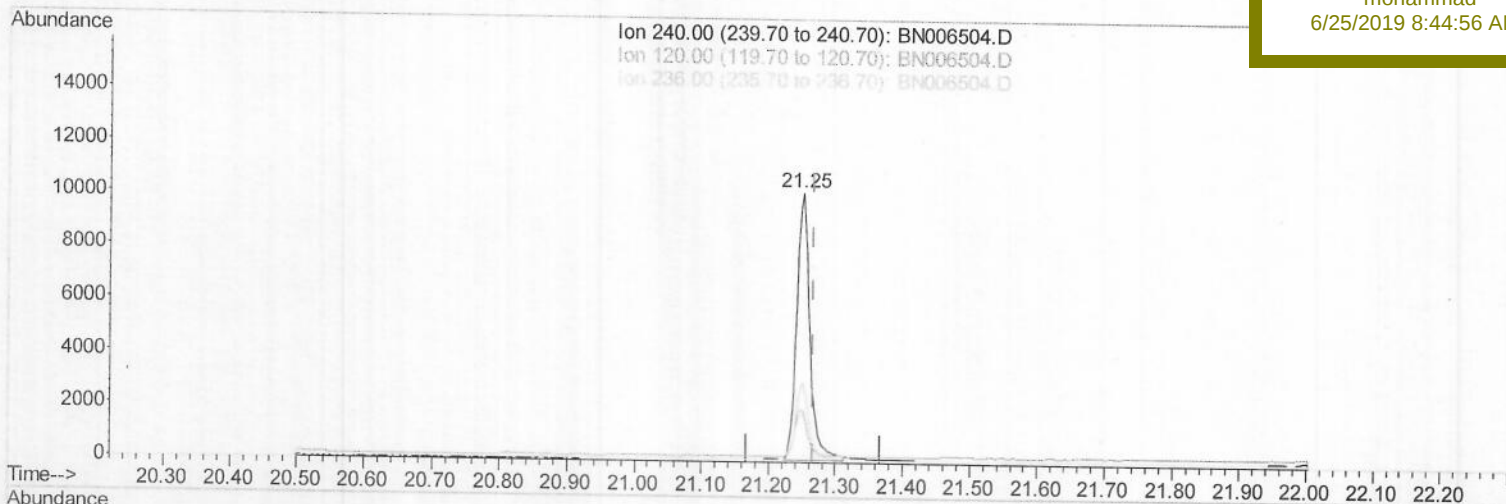

TIC: BN006504.D

(16) Chrysene-d12 (I)

21.251min (-0.017) 0.40ng/ul m

response 14021

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	18.98
236.00	30.10	29.73
0.00	0.00	0.00

> JU 06/26/19

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062219\
 Data File : BN006504.D
 Acq On : 22 Jun 2019 23:51
 Operator : HP/JU
 Sample : K3360-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jun 24 09:18:36 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 A41Z0

Manual Integrations
 APPROVED

mohammad
 6/25/2019 8:44:56 AM

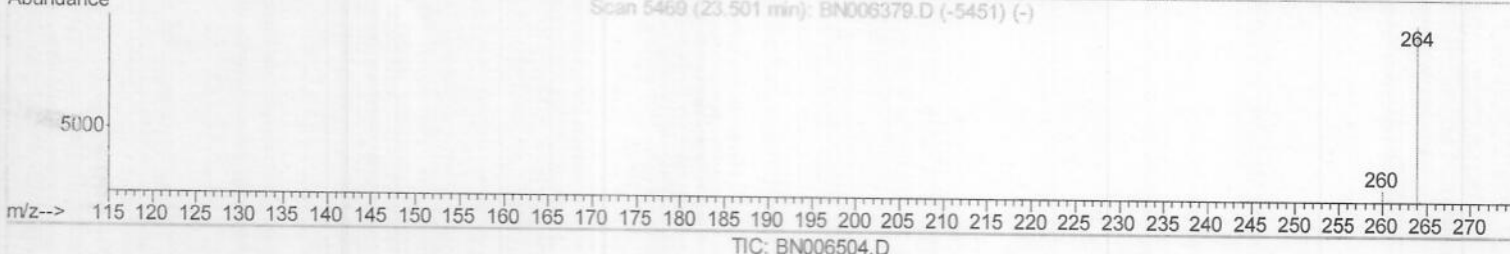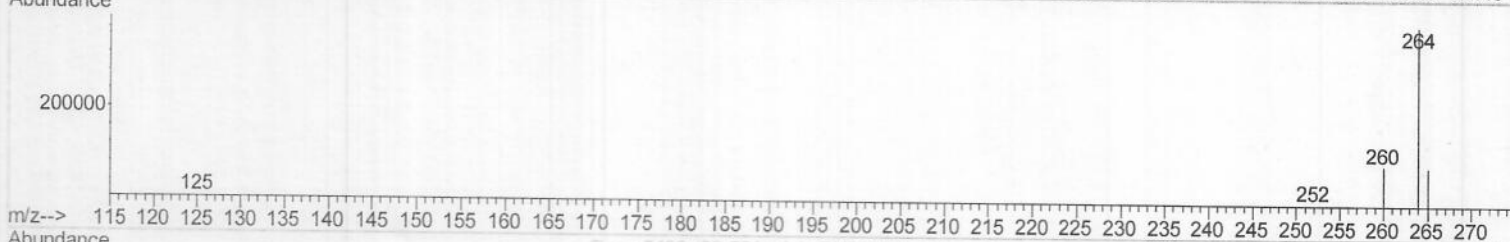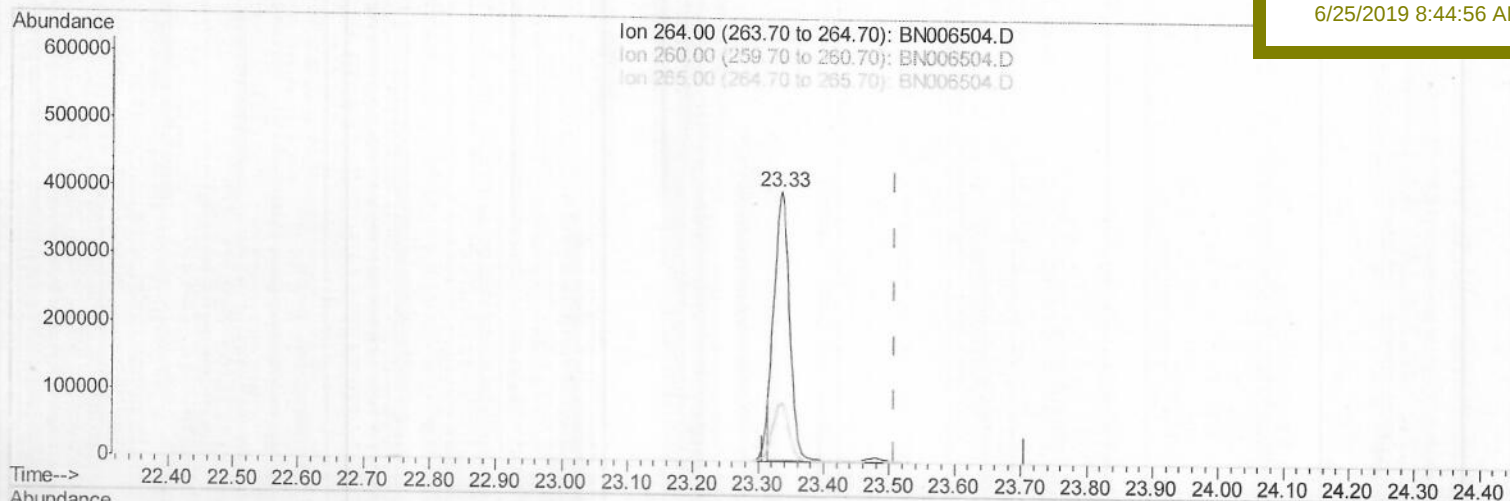

(20) Perylene-d12 (I)

23.335min (-0.172) 0.40ng/ul

response 663613

Ion	Exp%	Act%
264.00	100	100
260.00	29.20	22.05#
265.00	44.70	21.56#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062219\

Data File : BN006504.D

Acq On : 22 Jun 2019 23:51

Operator : HP/JU

Sample : K3360-10

Misc :

ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jun 24 09:18:36 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019




Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A41Z0

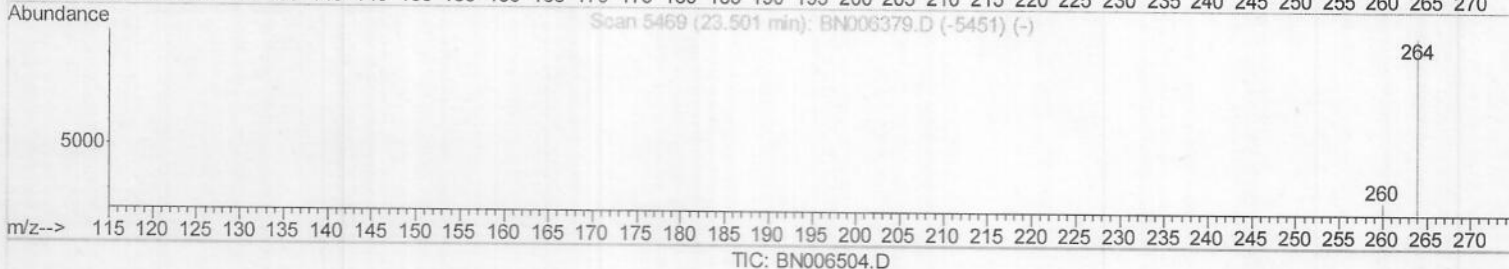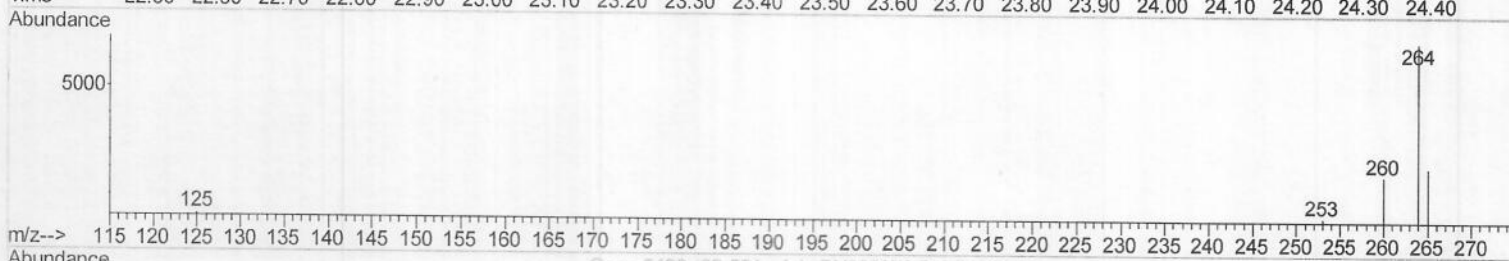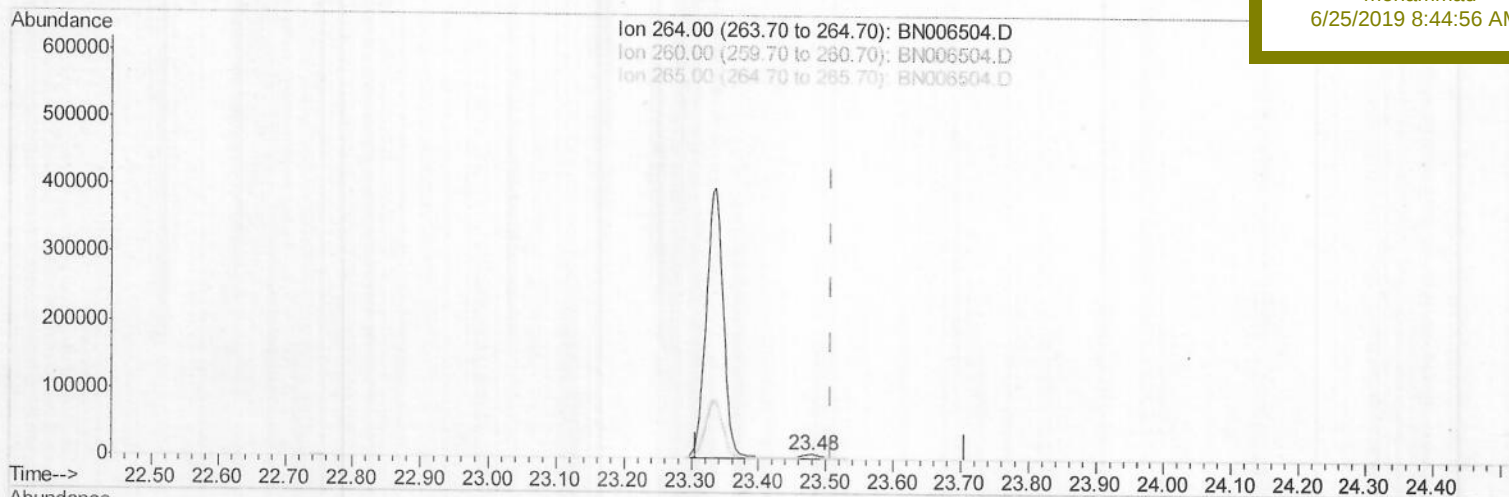Manual Integrations
APPROVEDmohammad
6/25/2019 8:44:56 AM

(20) Perylene-d12 (I)

23.478min (-0.029) 0.40ng/ul m

> JU 06/26/19

response 10949

Ion	Exp%	Act%
264.00	100	100
260.00	29.20	27.64
265.00	44.70	32.84#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062219\

Data File : BN006504.D

Acq On : 22 Jun 2019 23:51

Operator : HP/JU

Sample : K3360-10

Misc :

ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jun 24 09:19:08 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019




Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A41Z0

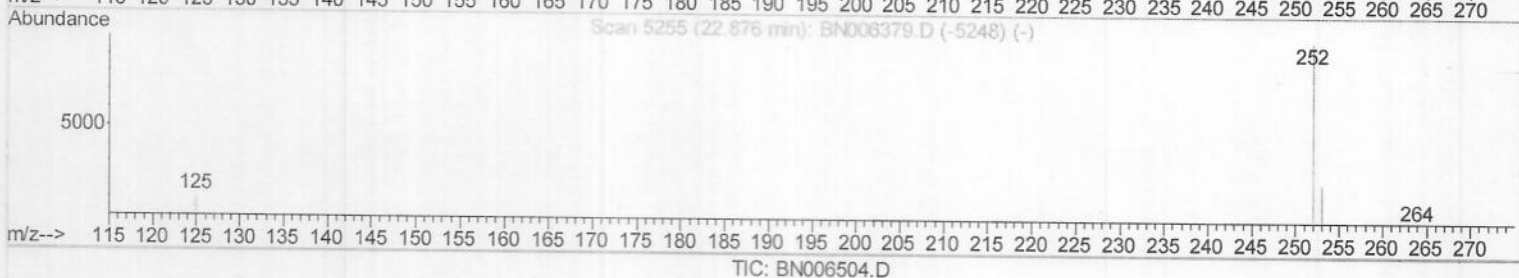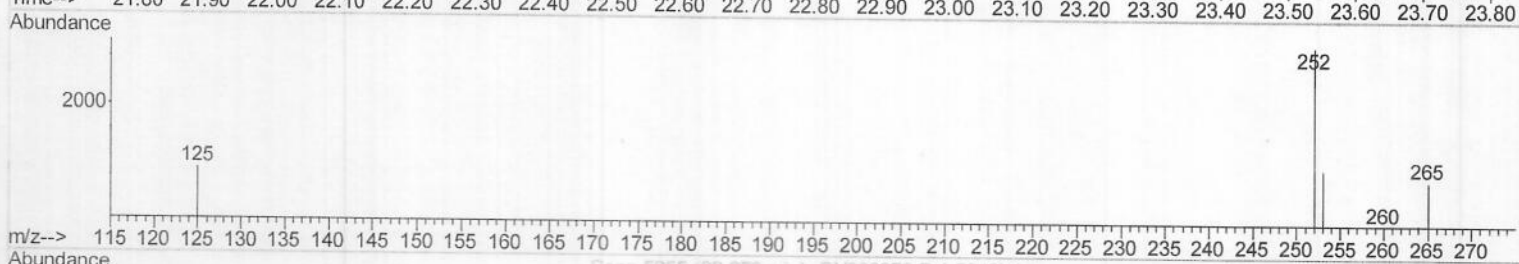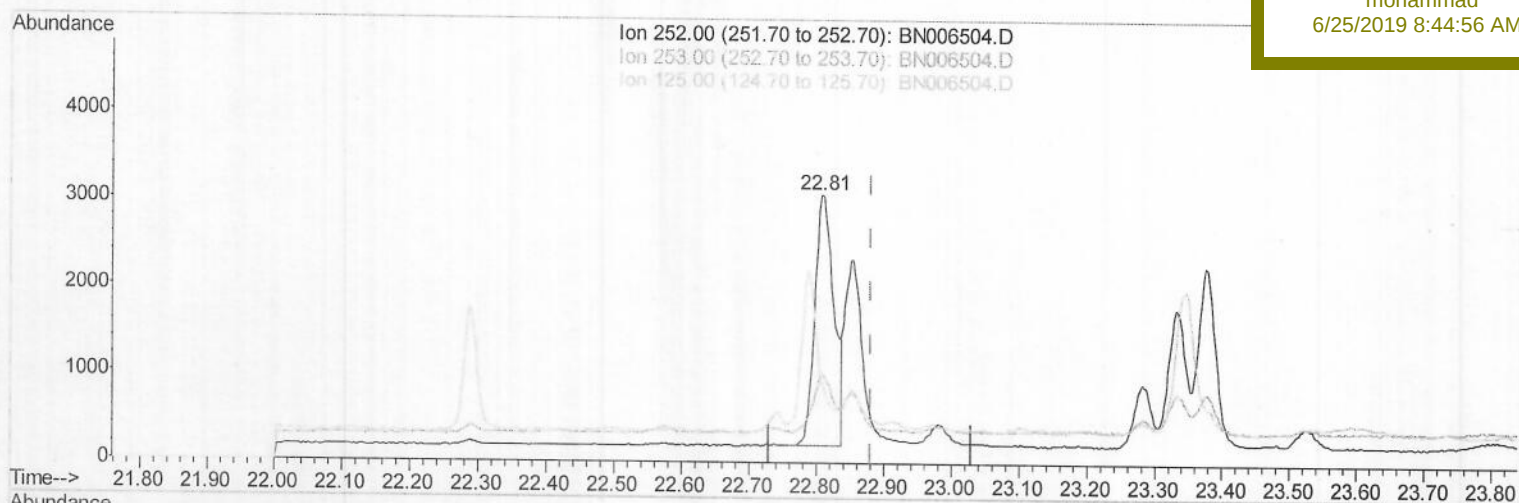Manual Integrations
APPROVEDmohammad
6/25/2019 8:44:56 AM

(22) Benzo(k)fluoranthene

22.808min (-0.073) 0.13ng/ul

response 5620

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	32.72#
125.00	17.90	30.21#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062219\
 Data File : BN006504.D
 Acq On : 22 Jun 2019 23:51
 Operator : HP/JU
 Sample : K3360-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jun 24 09:19:08 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 A41Z0

Manual Integrations
 APPROVED

mohammad
 6/25/2019 8:44:56 AM

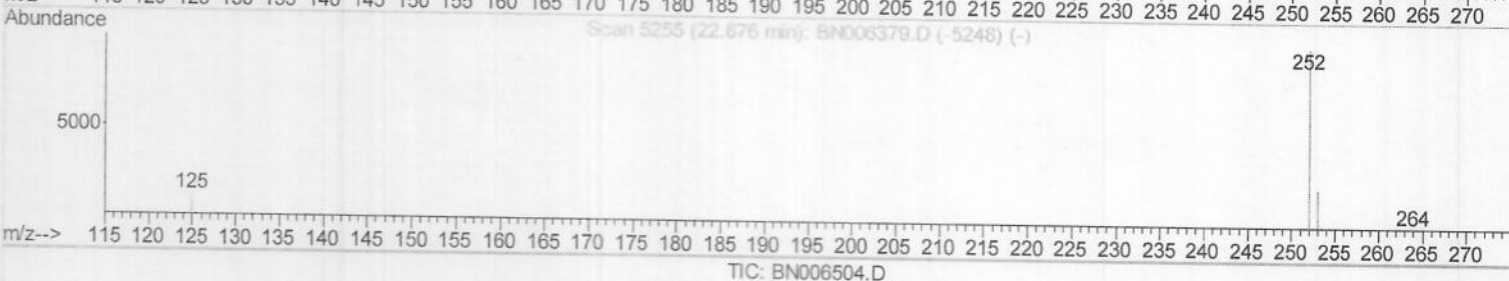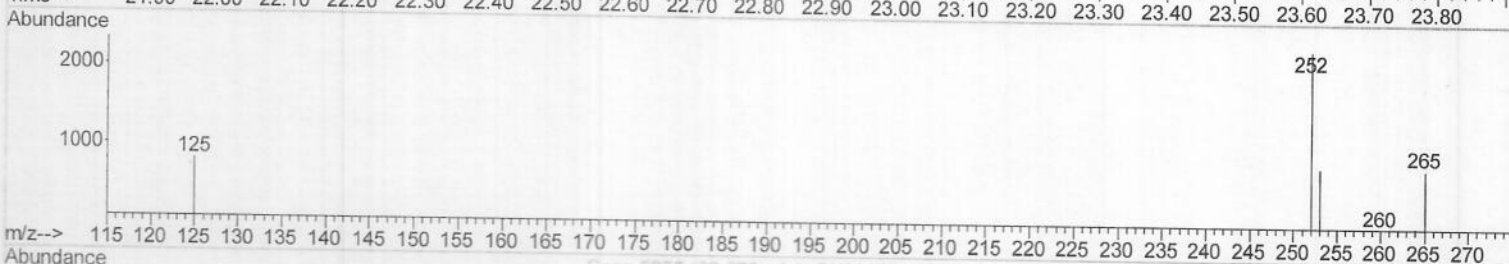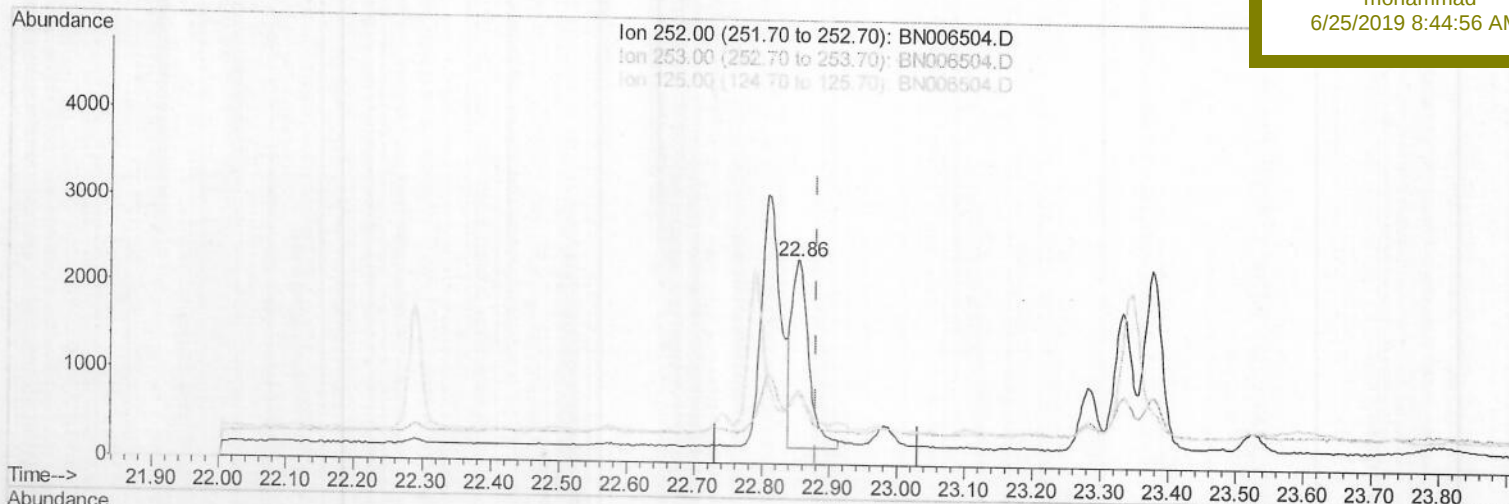

(22) Benzo(k)fluoranthene

22.855min (-0.026) 0.09ng/ul m

> JU 06/26/19

response 3871

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	35.55#
125.00	17.90	34.69#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062219\

Data File : BN006504.D

Acq On : 22 Jun 2019 23:51

Operator : HP/JU

Sample : K3360-10

Misc :

ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jun 24 09:19:08 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A41Z0

Manual Integrations

APPROVED

mohammad

6/25/2019 8:44:56 AM

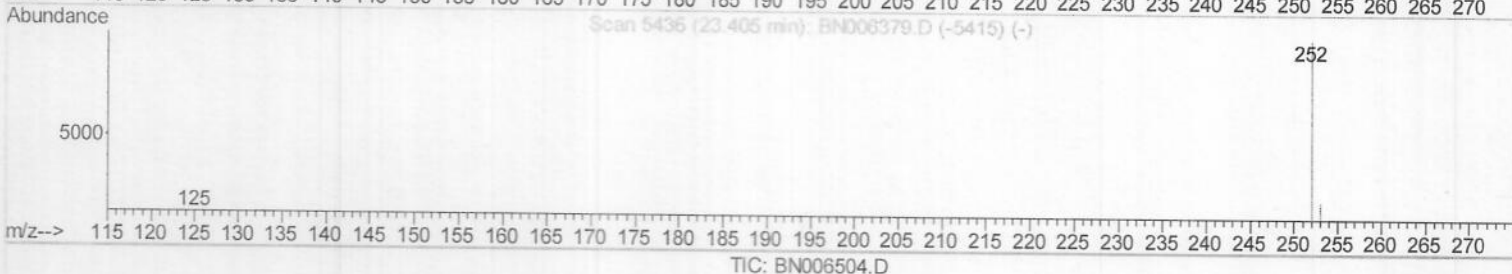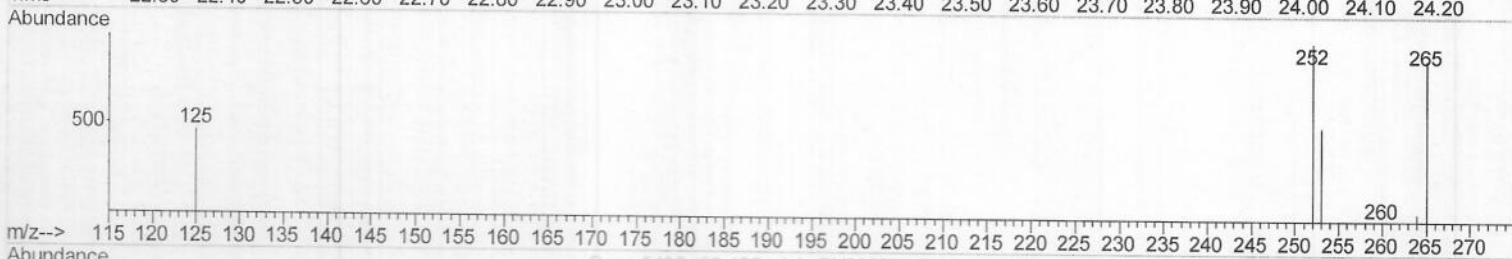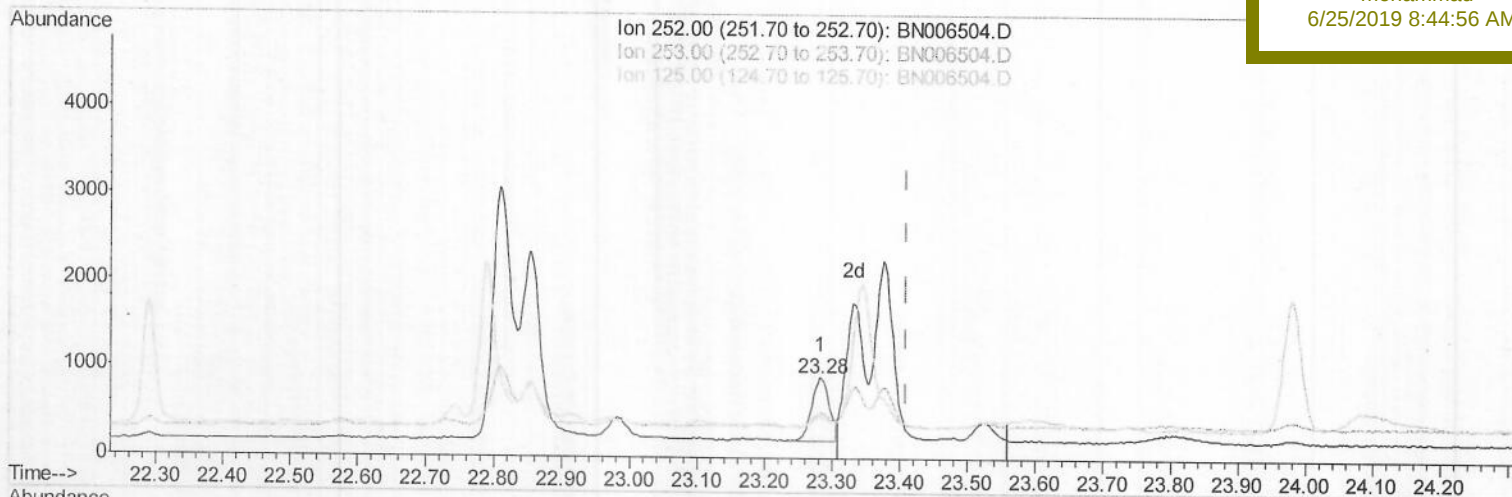

(23) Benzo(a)pyrene (C)

23.282min (-0.129) 0.03ng/ul

response 1255

Ion	Exp%	Act%
252.00	100	100
253.00	26.40	57.03#
125.00	25.40	51.94#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062219\

Data File : BN006504.D

Acq On : 22 Jun 2019 23:51

Operator : HP/JU

Sample : K3360-10

Misc :

ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jun 24 09:19:08 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A41Z0

Manual Integrations

APPROVED

mohammad

6/25/2019 8:44:56 AM

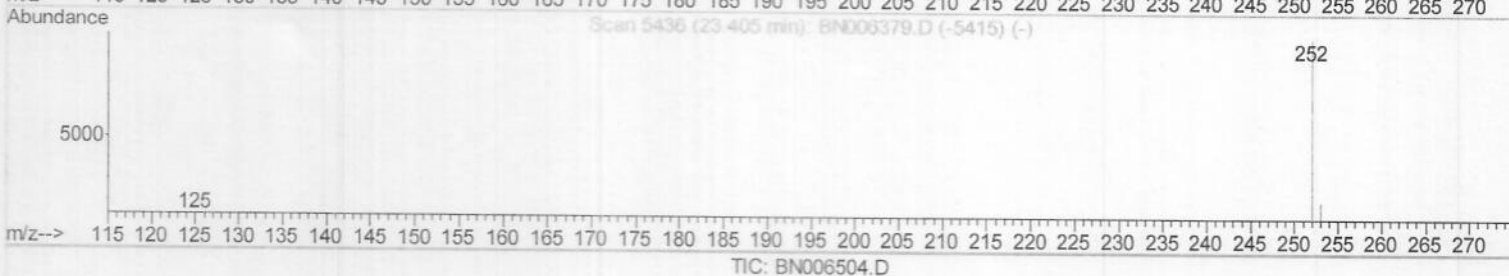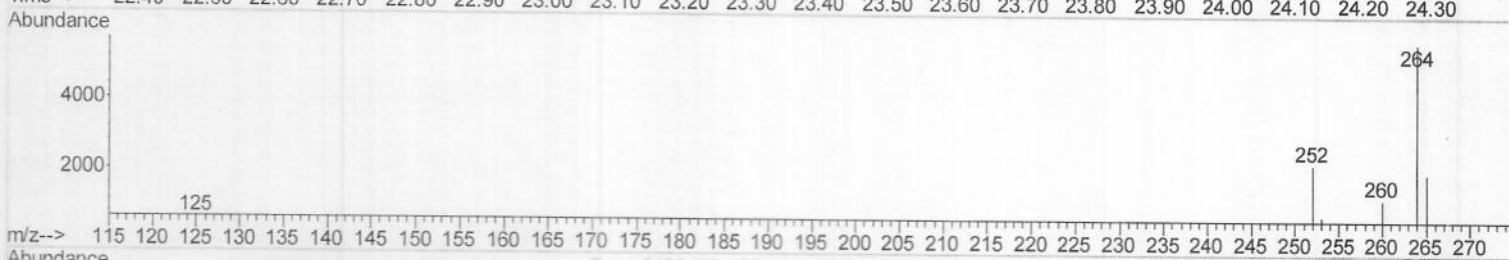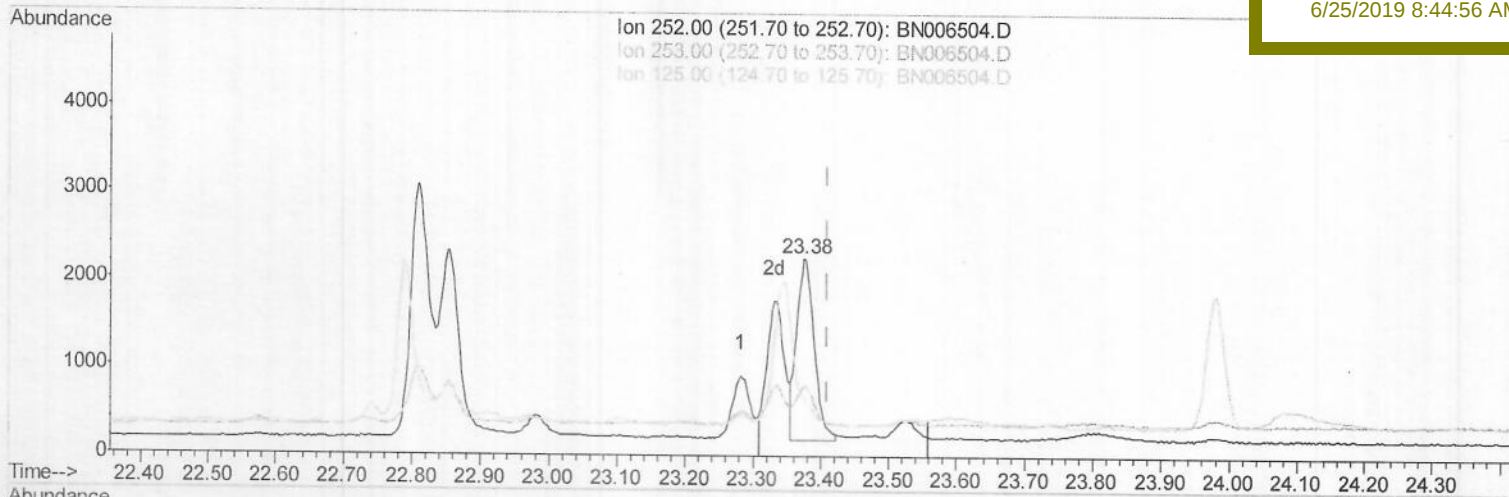

(23) Benzo(a)pyrene (C)

23.375min (-0.035) 0.09ng/ul m > JU 06/26/19

response 3722

Ion	Exp%	Act%
252.00	100	100
253.00	26.40	35.49#
125.00	25.40	29.77
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062219\

Data File : BN006504.D

Acq On : 22 Jun 2019 23:51

Operator : HP/JU

Sample : K3360-10

Misc :

ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jun 24 09:19:08 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A41Z0

Manual Integrations

APPROVED

mohammad

6/25/2019 8:44:56 AM

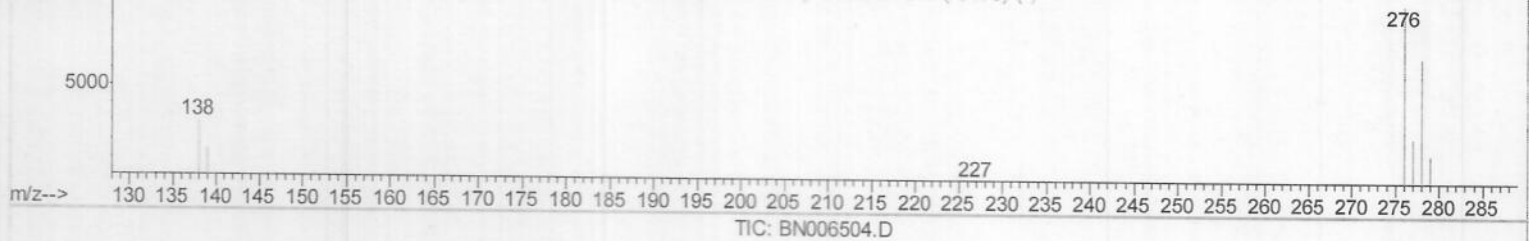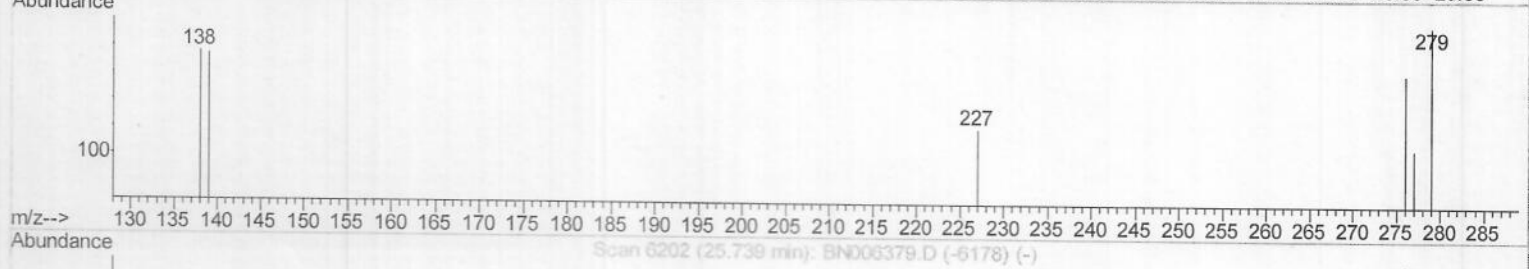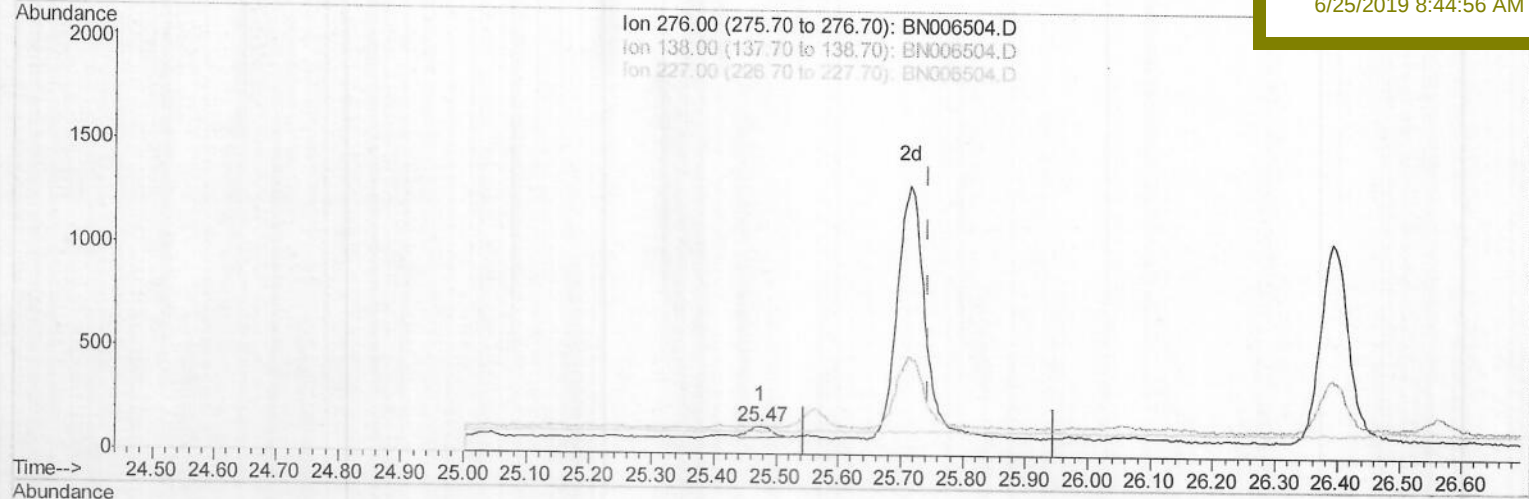

(24) Indeno(1,2,3-cd)pyrene

25.474min (-0.272) 0.00ng/ul

response 142

Ion	Exp%	Act%
276.00	100	100
138.00	32.00	0.00#
227.00	0.40	4.93#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062219\

Data File : BN006504.D

Acq On : 22 Jun 2019 23:51

Operator : HP/JU

Sample : K3360-10

Misc :

ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jun 24 09:19:08 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A41Z0

Manual Integrations

APPROVED

mohammad

6/25/2019 8:44:56 AM

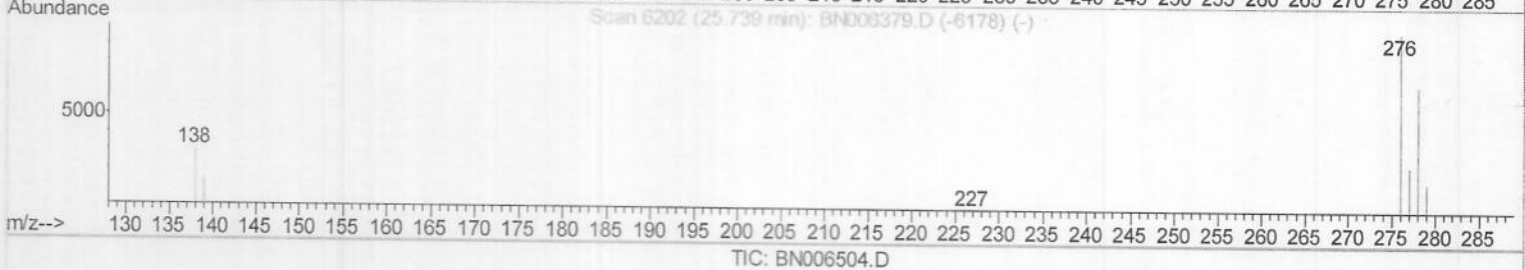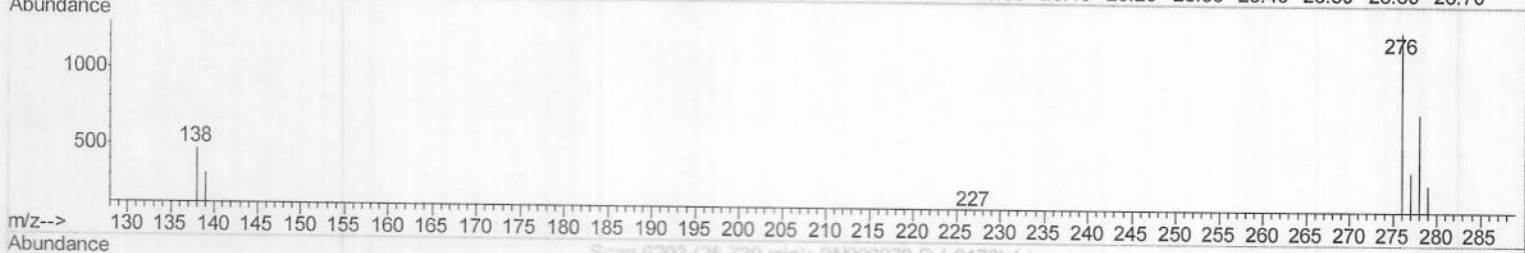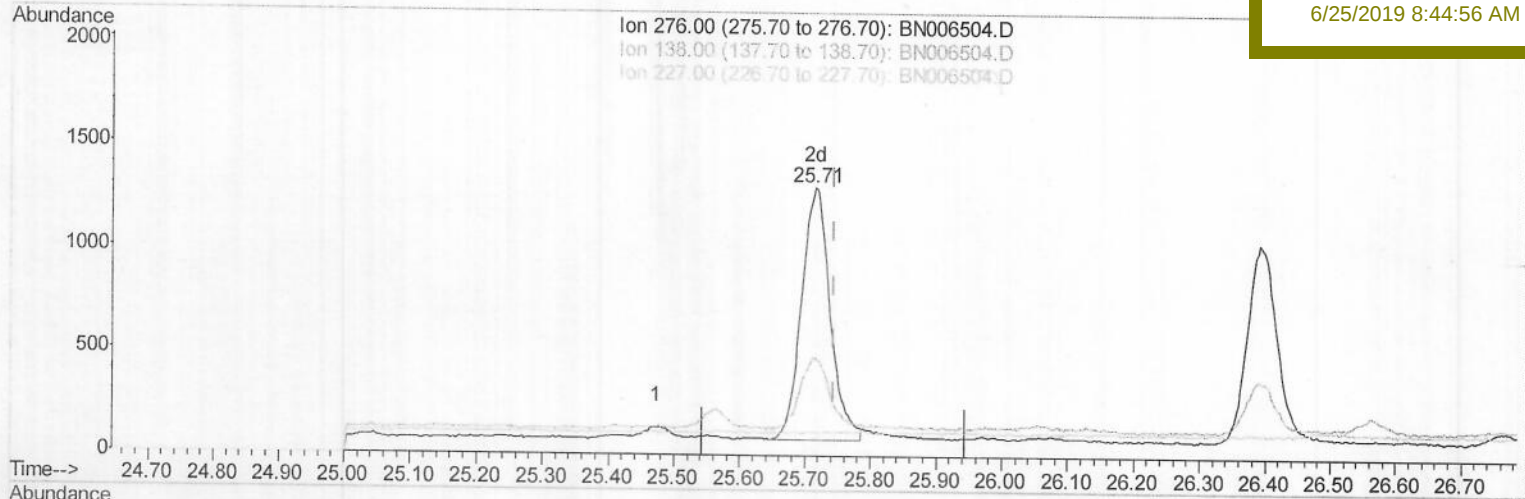

(24) Indeno(1,2,3-cd)pyrene

25.715min (-0.030) 0.08ng/ul m

JU 06/26/19

response 3733

Ion	Exp%	Act%
276.00	100	100
138.00	32.00	0.00#
227.00	0.40	0.19#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062219\
 Data File : BN006504.D
 Acq On : 22 Jun 2019 23:51
 Operator : HP/JU
 Sample : K3360-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jun 24 09:19:08 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 A41Z0

Manual Integrations
 APPROVED

mohammad
 6/25/2019 8:44:56 AM

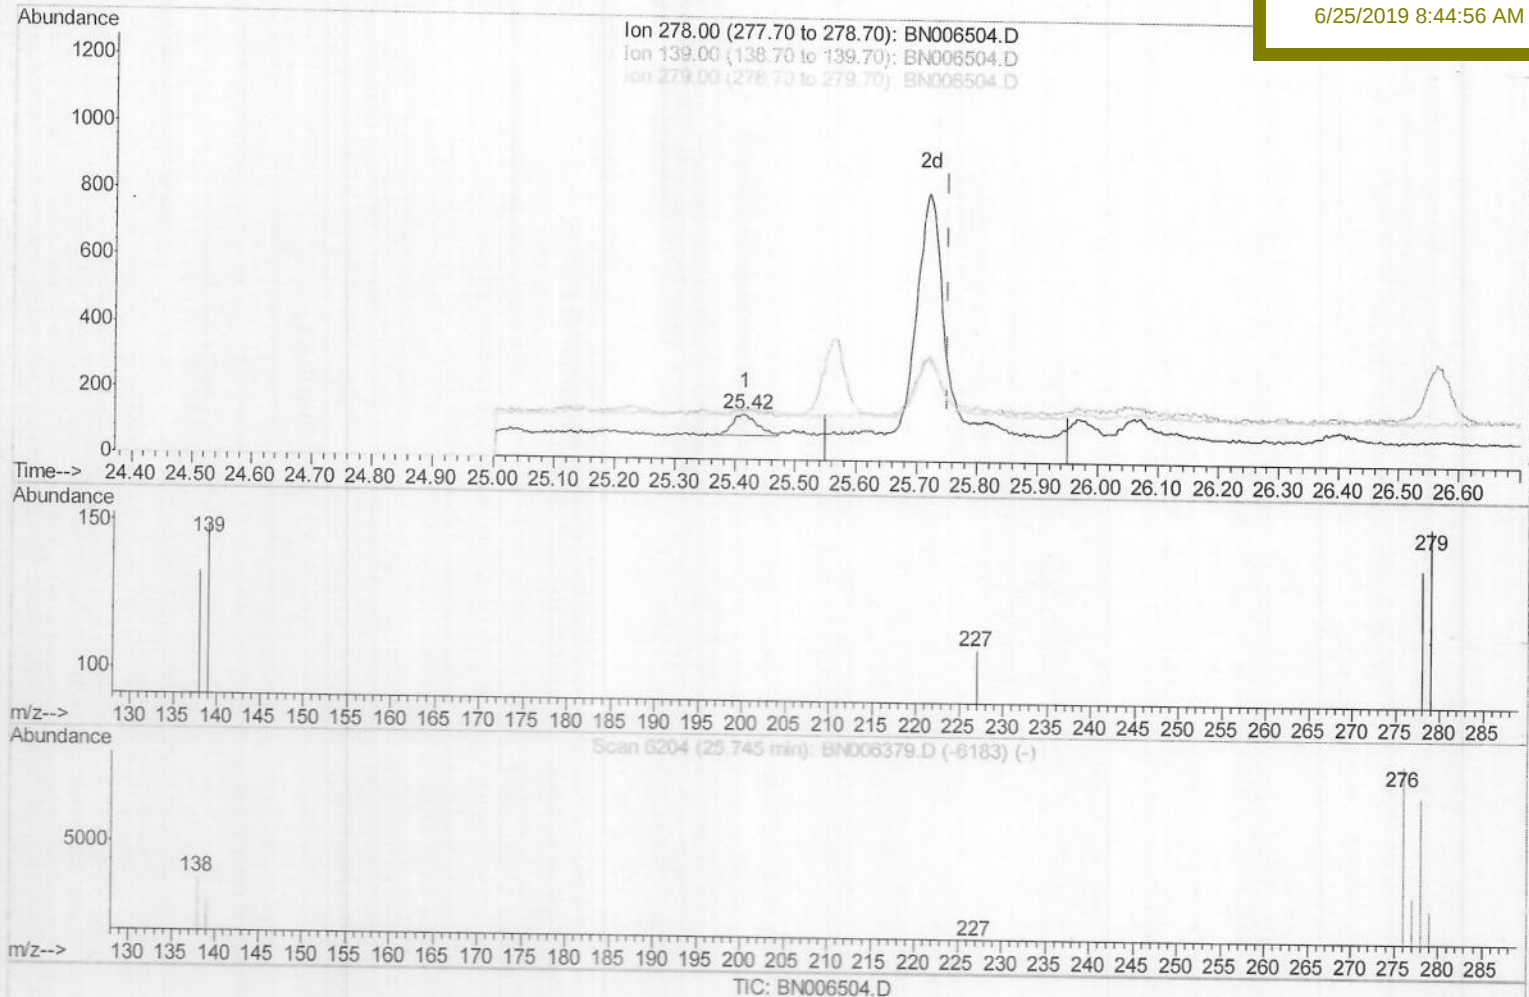

(25) Dibenzo(a,h)anthracene

25.416min (-0.335) 0.00ng/ul

response 175

Ion	Exp%	Act%
278.00	100	100
139.00	26.50	107.25#
279.00	28.20	110.14#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062219\

Data File : BN006504.D

Acq On : 22 Jun 2019 23:51

Operator : HP/JU

Sample : K3360-10

Misc :

ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jun 24 09:19:08 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :


A41Z0

Manual Integrations

APPROVED

mohammad

6/25/2019 8:44:56 AM

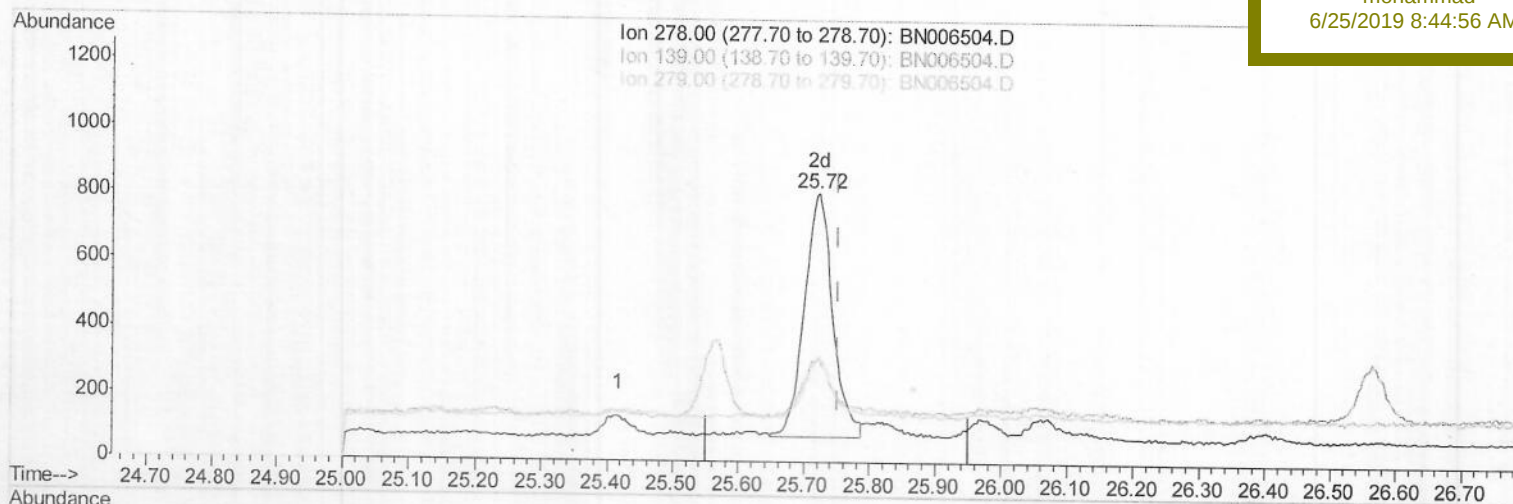

(25) Dibenzo(a,h)anthracene

25.722min (-0.030) 0.06ng/ul m > JU 06/26/19

response 2220

Ion	Exp%	Act%
278.00	100	100
139.00	26.50	40.20#
279.00	28.20	39.33#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062219\
 Data File : BN006504.D
 Acq On : 22 Jun 2019 23:51
 Operator : HP/JU
 Sample : K3360-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jun 24 09:19:08 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 A41Z0

Manual Integrations
 APPROVED

mohammad
 6/25/2019 8:44:56 AM

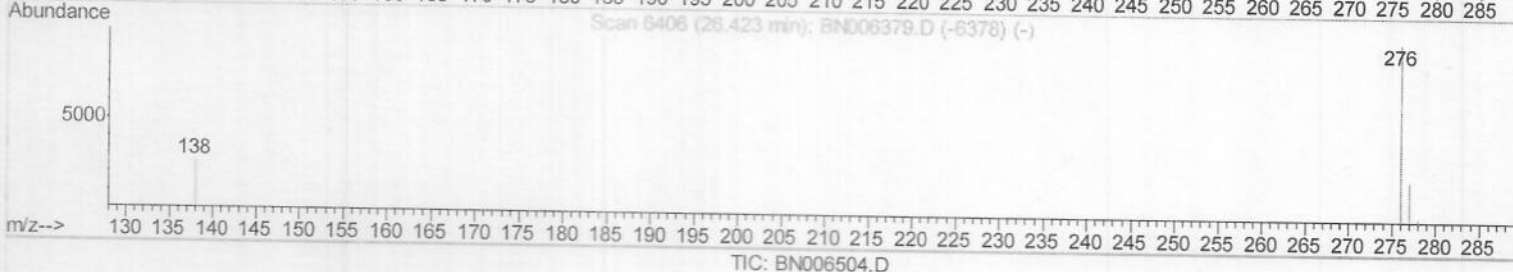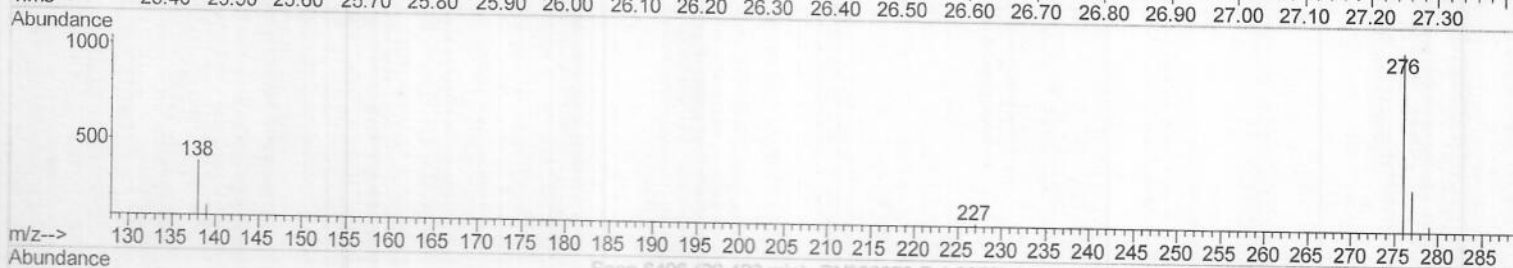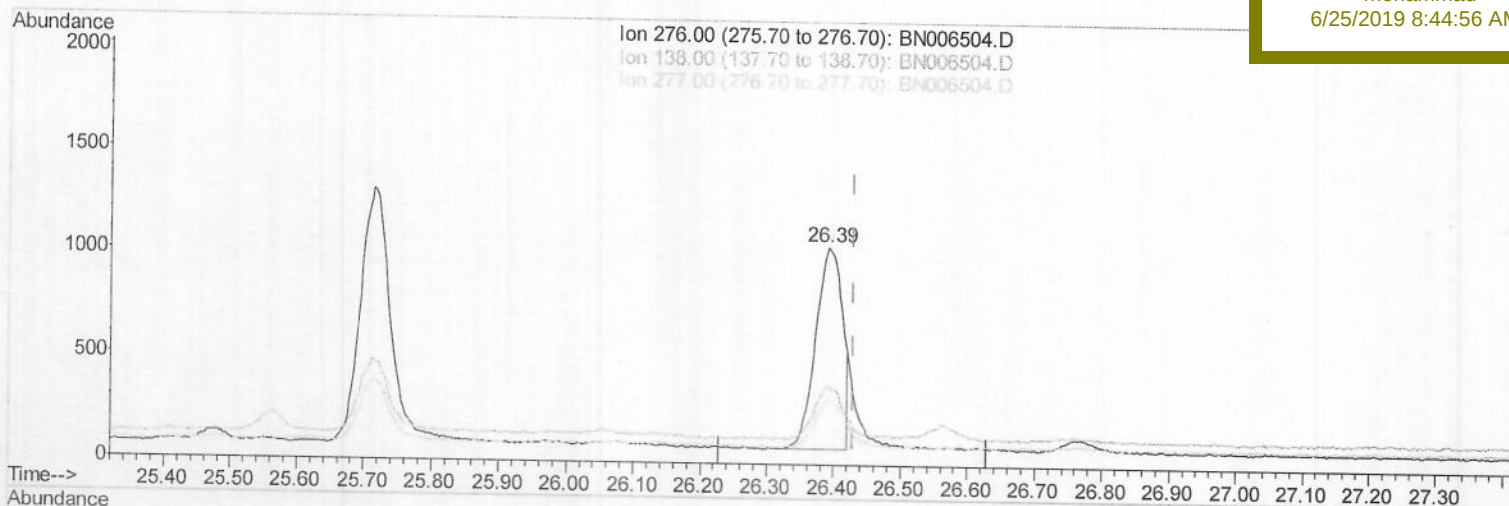

(26) Benzo(g,h,i)perylene
 26.392min (-0.037) 0.07ng/ul
 response 2658

Ion	Exp%	Act%
276.00	100	100
138.00	30.30	36.57#
277.00	26.90	30.51
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062219\

Data File : BN006504.D

Acq On : 22 Jun 2019 23:51

Operator : HP/JU

Sample : K3360-10

Misc :

ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jun 24 09:19:08 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A41Z0

Manual Integrations

APPROVED

mohammad

6/25/2019 8:44:56 AM

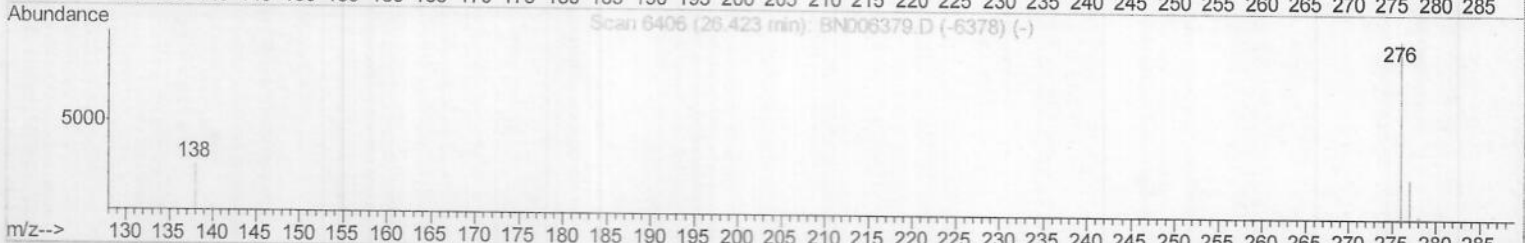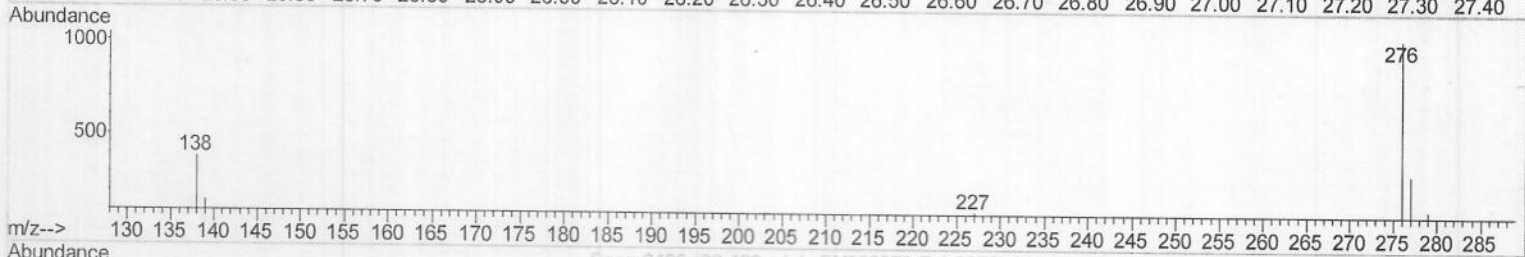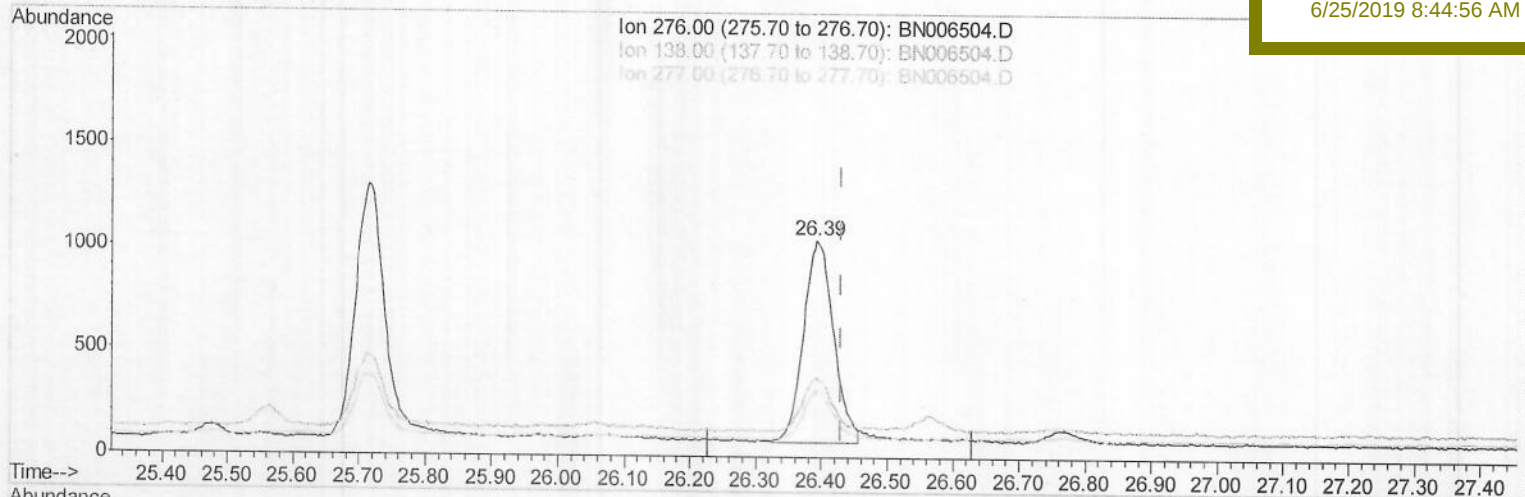

(26) Benzo(g,h,i)perylene

26.392min (-0.037) 0.08ng/ul m

> JU 06/26/19

response 3063

Ion	Exp%	Act%
276.00	100	100
138.00	30.30	36.57#
277.00	26.90	30.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062219\
 Data File : BN006504.D
 Acq On : 22 Jun 2019 23:51
 Operator : HP/JU
 Sample : K3360-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 Client Sampled :
 A41Z0

Quant Time: Jun 24 09:21:28 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 6/25/2019 8:44:56 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	5007	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.41	136	19849	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.28	164	10957	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	22483m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.25	240	14021m	0.40	ng/ul	-0.02
20) Perylene-d12	23.48	264	10949m	0.40	ng/ul	-0.03
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.01	152	5565	0.18	ng/ul	-0.01
14) Fluoranthene-d10	19.08	212	13086m	0.22	ng/ul	-0.01
Target Compounds						
3) Naphthalene	10.46	128	2345	0.043	ng/ul	# 89
5) 2-Methylnaphthalene	12.08	142	771	0.020	ng/ul	92
12) Phenanthrene	17.08	178	3246	0.045	ng/ul	93
15) Fluoranthene	19.11	202	8487m	0.106	ng/ul	
17) Pyrene	19.47	202	8903	0.121	ng/ul	96
18) Benzo(a)anthracene	21.23	228	4373	0.071	ng/ul	96
19) Chrysene	21.29	228	5206	0.089	ng/ul	97
21) Benzo(b)fluoranthene	22.81	252	5620	0.123	ng/ul	83
22) Benzo(k)fluoranthene	22.86	252	3871m	0.087	ng/ul	
23) Benzo(a)pyrene	23.38	252	3722m	0.088	ng/ul	
24) Indeno(1,2,3-cd)pyrene	25.71	276	3733m	0.081	ng/ul	
25) Dibenzo(a,h)anthracene	25.72	278	2220m	0.060	ng/ul	
26) Benzo(g,h,i)perylene	26.39	276	3063m	0.079	ng/ul	

JU
 06/26/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed