

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN062219\

Data File : BN006516.D

Acq On : 23 Jun 2019 08:28

Operator : HP/JU

Sample : K3360-07

Misc :

ALS Vial : 32 Sample Multiplier: 1

Quant Time: Jun 24 08:57:48 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :


A41Y7

Manual Integrations

APPROVED

mohammad

6/25/2019 8:45:34 AM

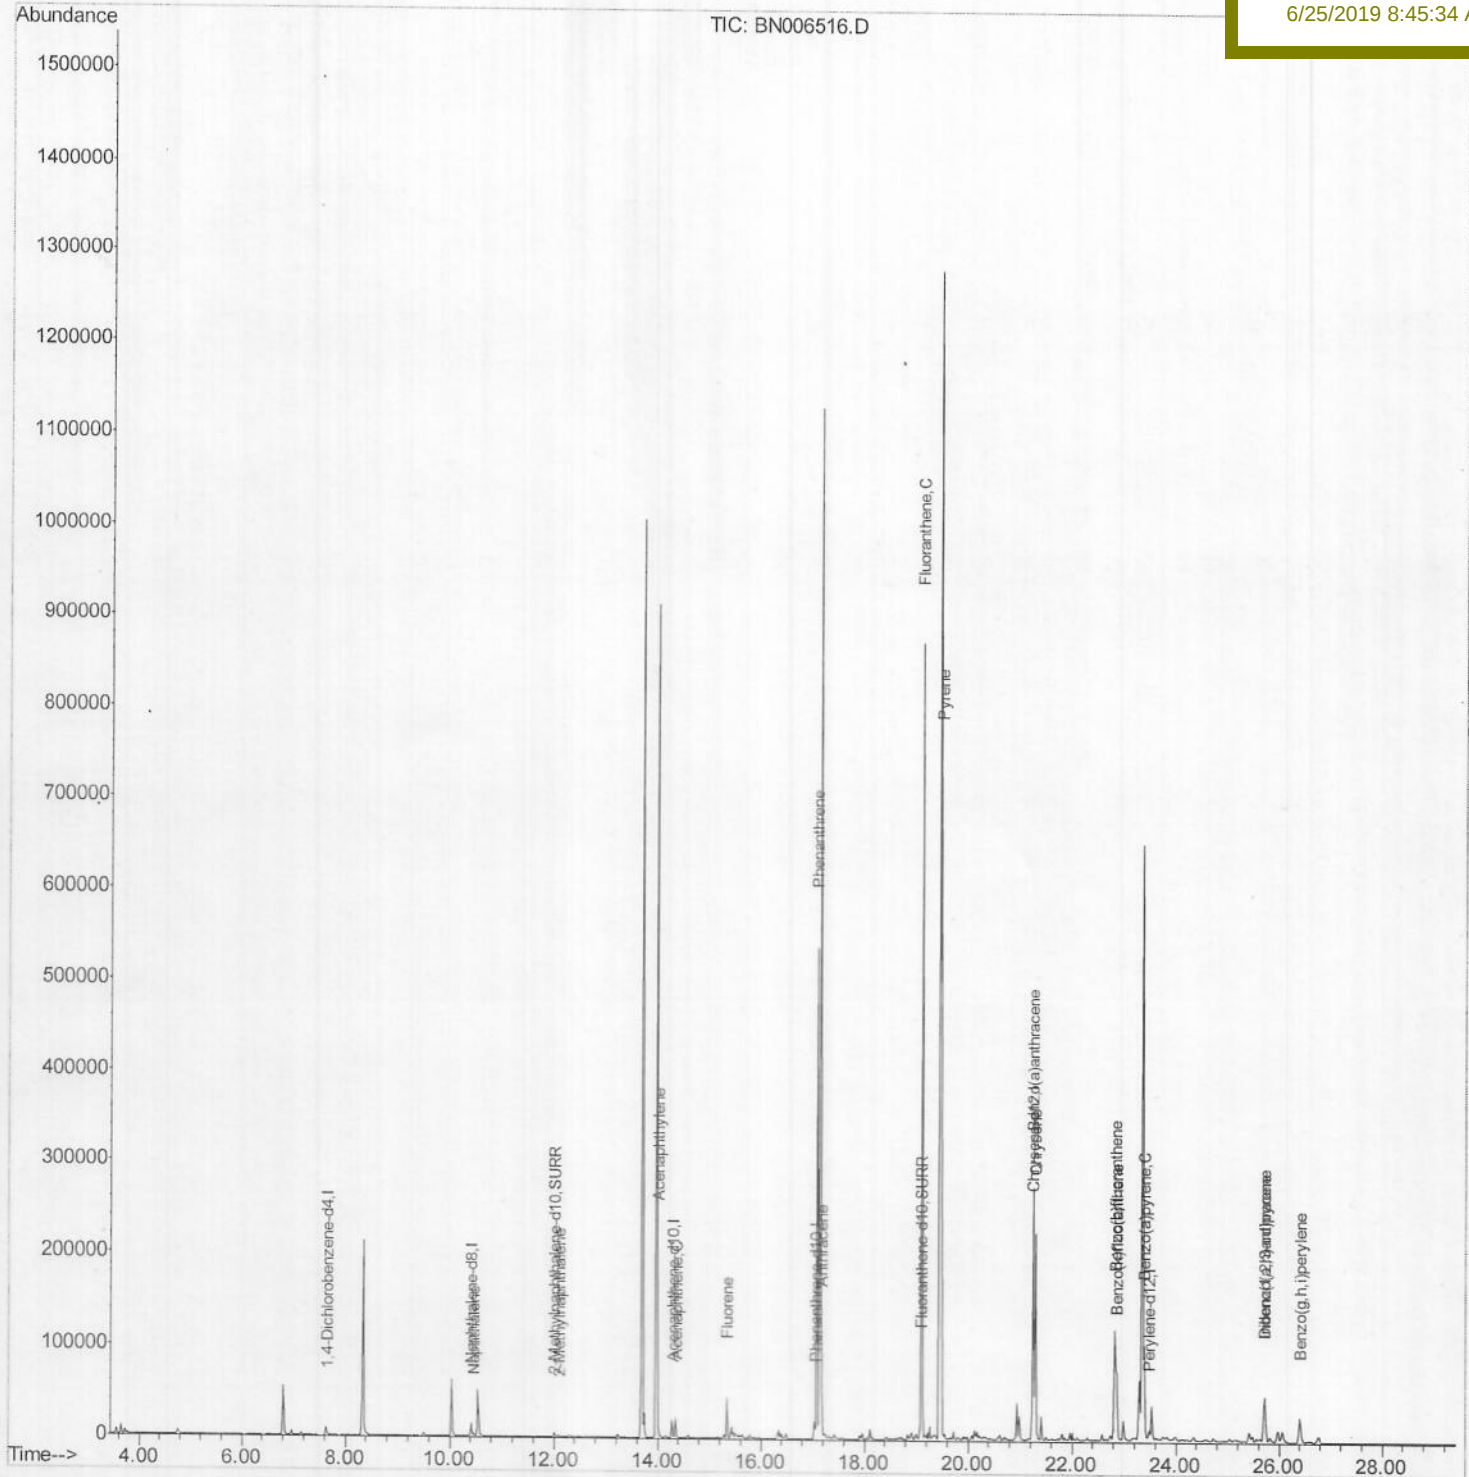

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN062219\
 Data File : BN006516.D
 Acq On : 23 Jun 2019 08:28
 Operator : HP/JU
 Sample : K3360-07
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Quant Time: Jun 24 08:53:33 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
ClientSampleId :
 A41Y7

Manual Integrations
APPROVED

mohammad
 6/25/2019 8:45:34 AM

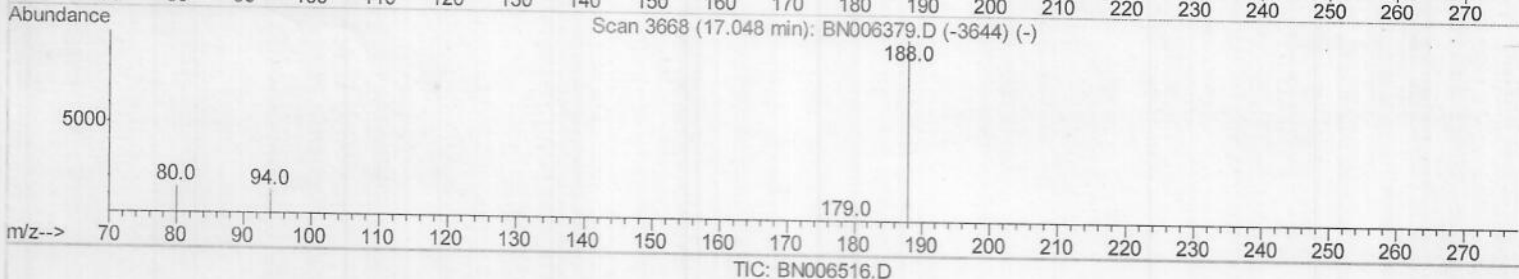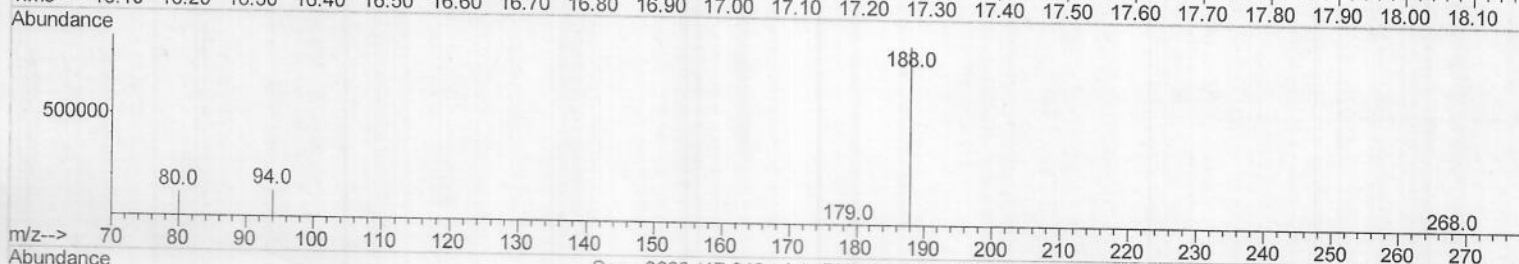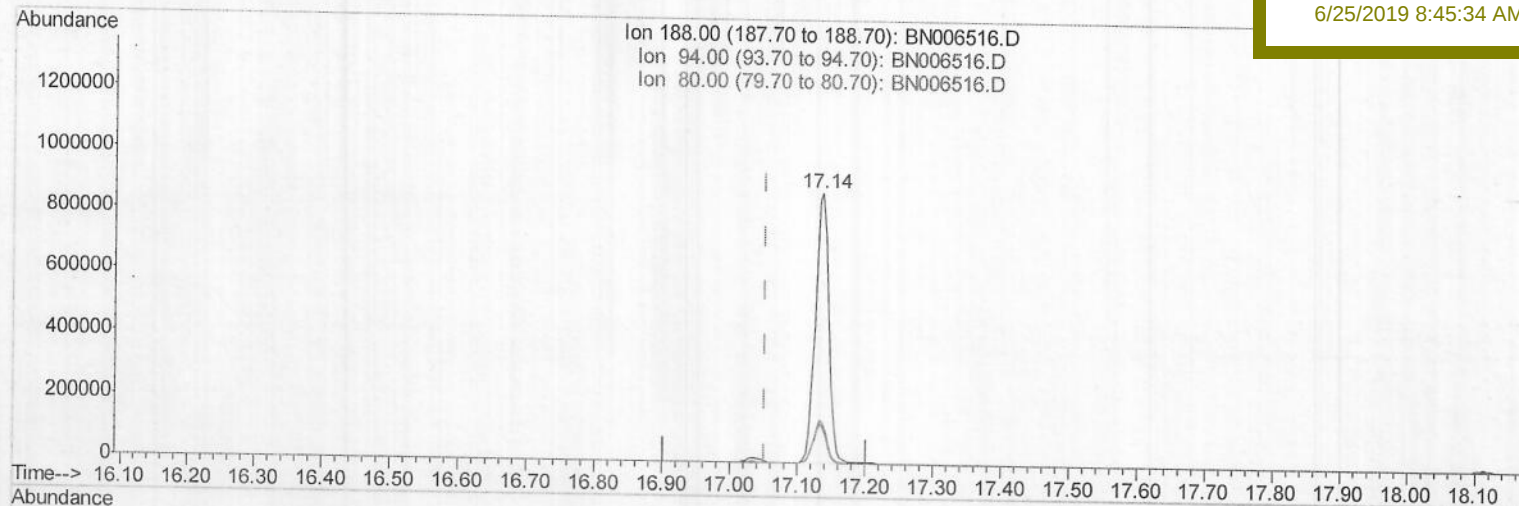

TIC: BN006516.D

(10) Phenanthrene-d10 (I)
 17.137min (+0.085) 0.40ng/ul
 response 1228088

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	15.19
80.00	13.60	13.74
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN062219\

Data File : BN006516.D

Acq On : 23 Jun 2019 08:28

Operator : HP/JU

Sample : K3360-07

Misc :

ALS Vial : 32 Sample Multiplier: 1

Quant Time: Jun 24 08:53:33 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A41Y7

Manual Integrations

APPROVED

mohammad

6/25/2019 8:45:34 AM

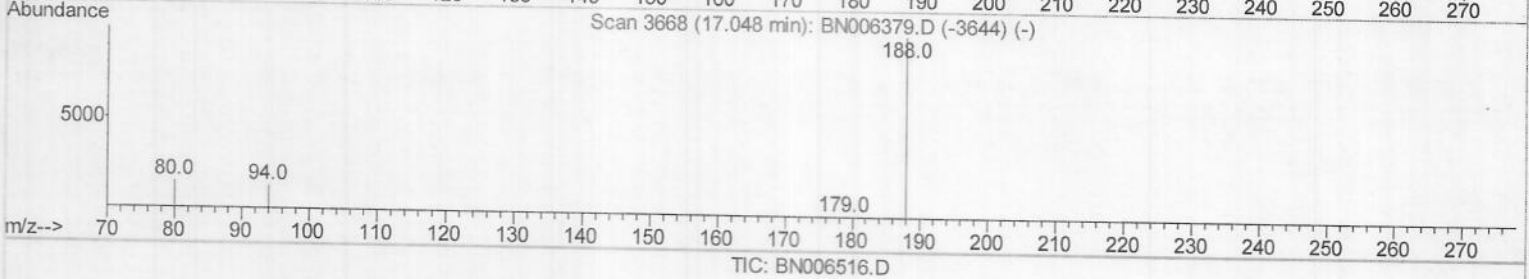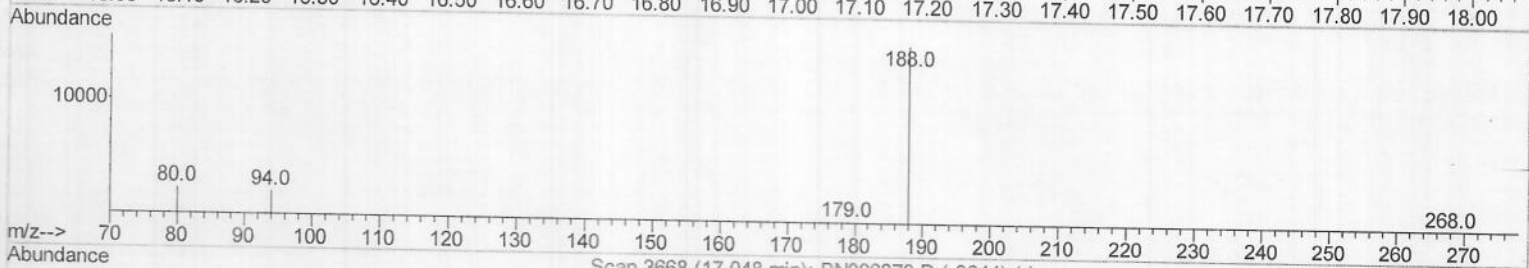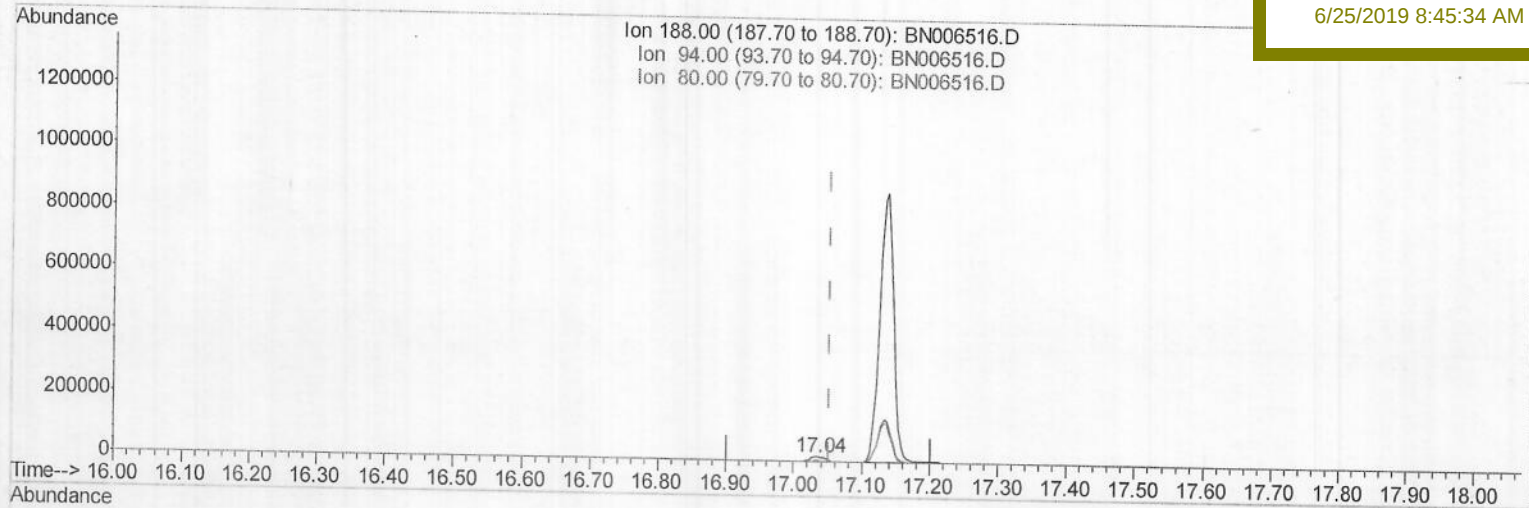

(10) Phenanthrene-d10 (I)

17.036min (-0.017) 0.40ng/ul m

JU 06/26/19

response 21608

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	13.44
80.00	13.60	14.70
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN062219\

Data File : BN006516.D

Acq On : 23 Jun 2019 08:28

Operator : HP/JU

Sample : K3360-07

Misc :

ALS Vial : 32 Sample Multiplier: 1

Quant Time: Jun 24 08:54:22 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A41Y7

Manual Integrations

APPROVED

mohammad

6/25/2019 8:45:34 AM

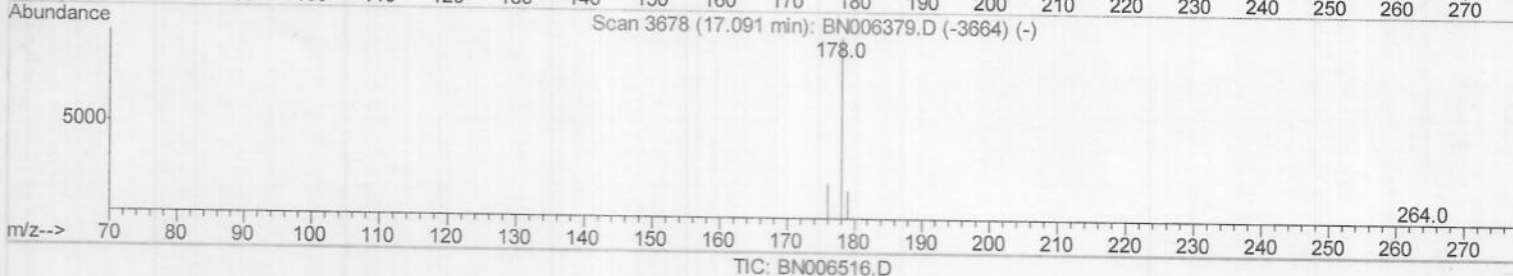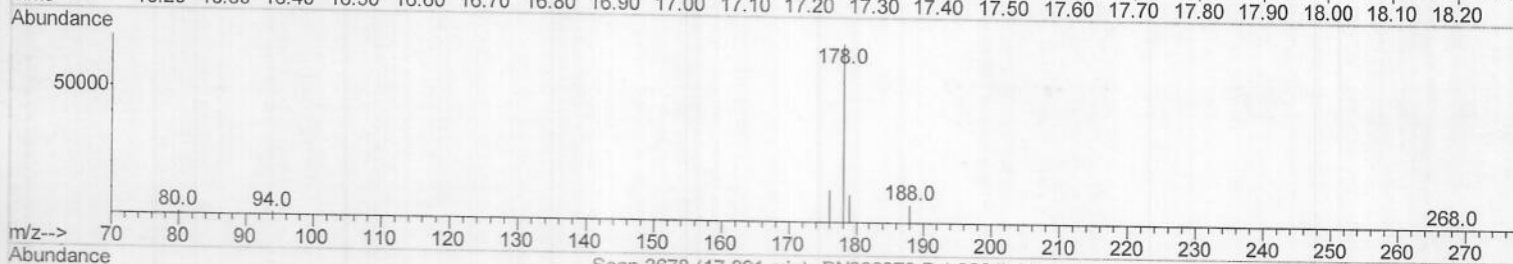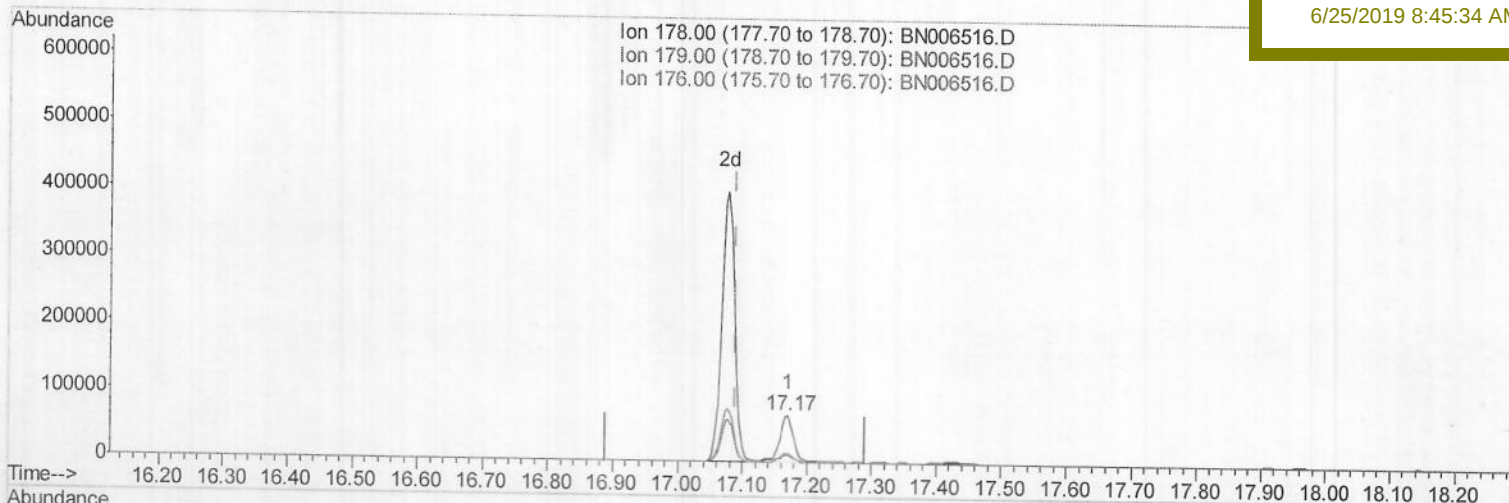

(12) Phenanthrene

17.171min (+0.080) 1.49ng/ul

response 103445

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	15.69
176.00	19.10	18.76
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN062219\

Data File : BN006516.D

Acq On : 23 Jun 2019 08:28

Operator : HP/JU

Sample : K3360-07

Misc :

ALS Vial : 32 Sample Multiplier: 1

Quant Time: Jun 24 08:54:22 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A41Y7

Manual Integrations

APPROVED

mohammad

6/25/2019 8:45:34 AM

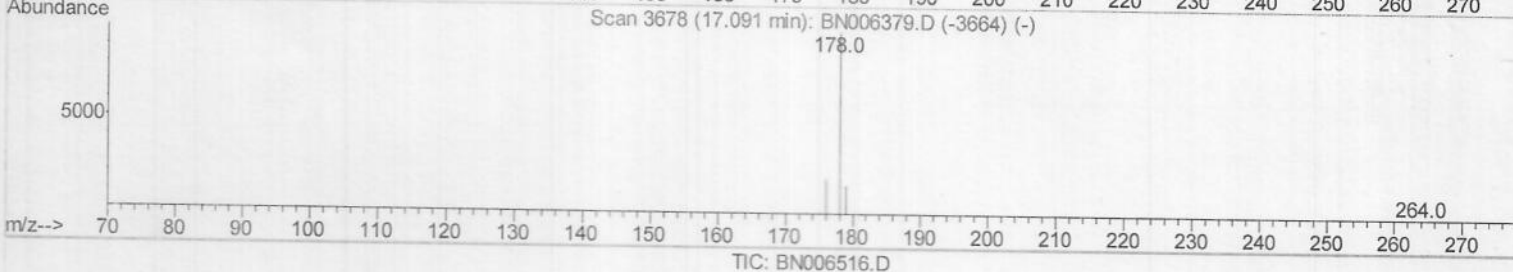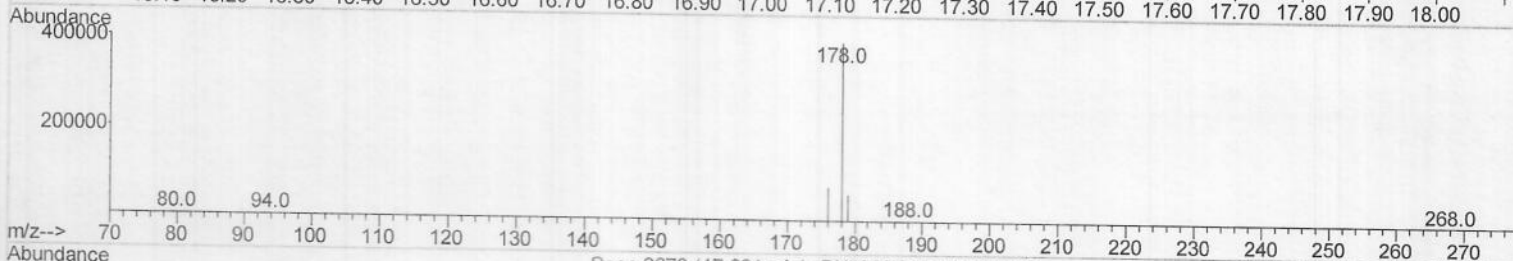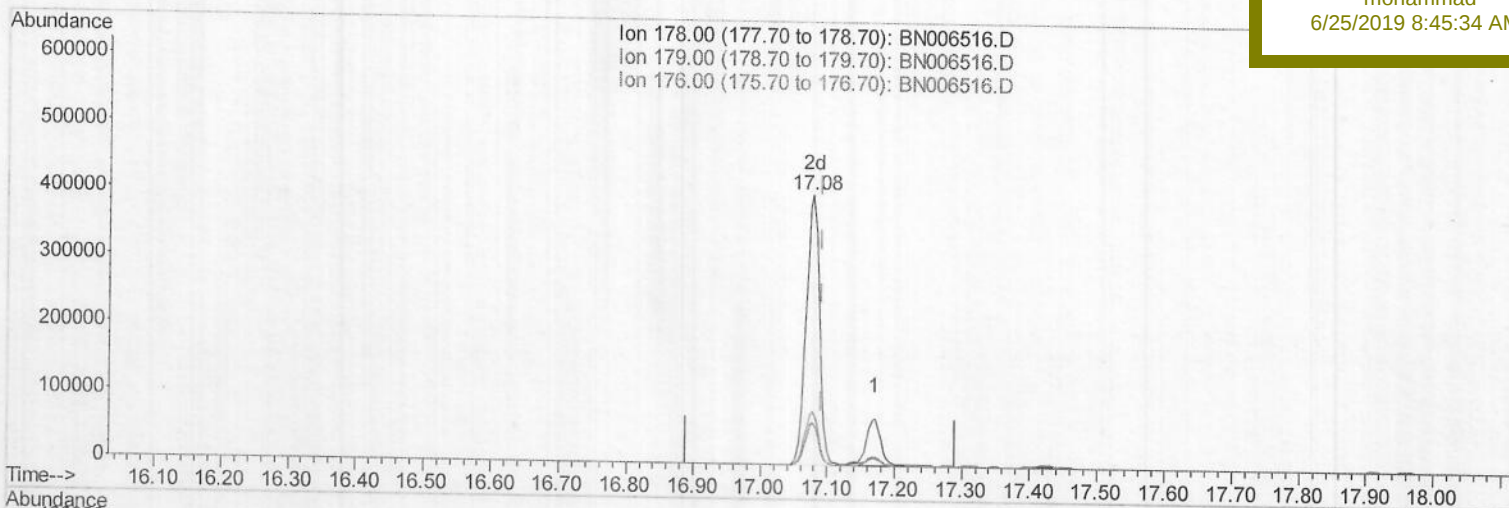

(12) Phenanthrene

17.078min (-0.013) 7.99ng/ul m

> JU 06/26/19

response 554100

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	15.29
176.00	19.10	19.42
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN062219\

Data File : BN006516.D

Acq On : 23 Jun 2019 08:28

Operator : HP/JU

Sample : K3360-07

Misc :

ALS Vial : 32 Sample Multiplier: 1

Quant Time: Jun 24 08:54:22 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A41Y7

Manual Integrations

APPROVED

mohammad

6/25/2019 8:45:34 AM

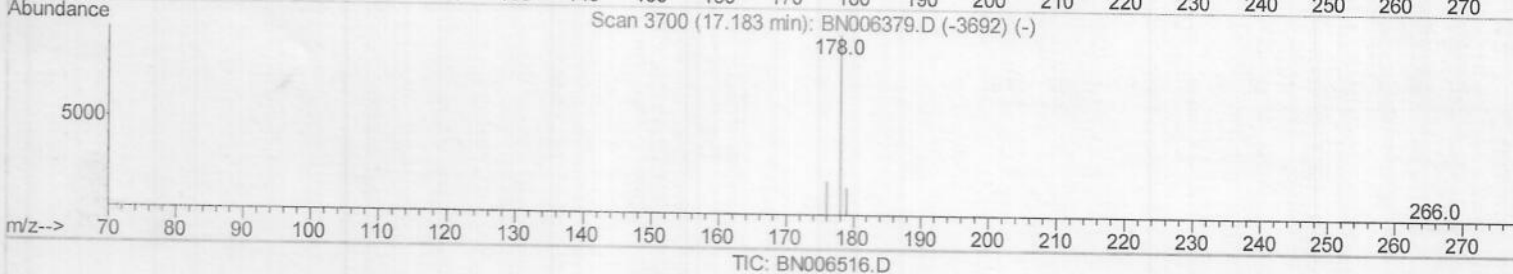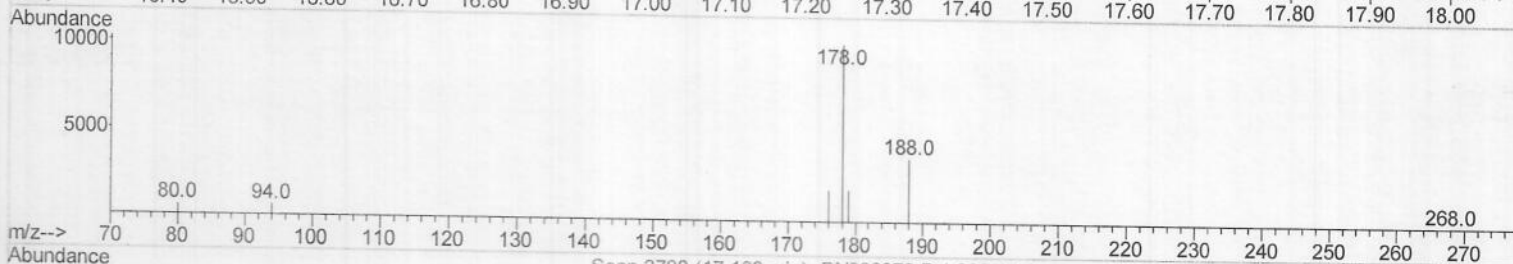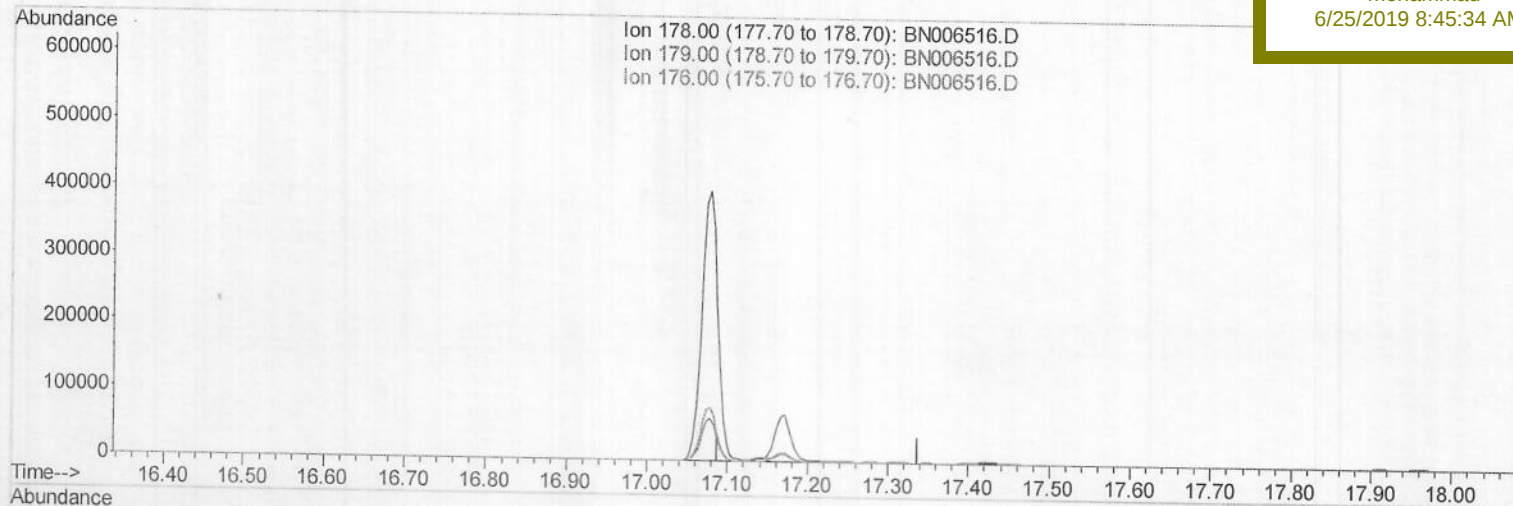

(13) Anthracene

17.187min (-17.187) 0.00ng/ul

response 0

Ion	Exp%	Act%
178.00	100	0.00
179.00	15.30	0.00#
176.00	18.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN062219\

Data File : BN006516.D

Acq On : 23 Jun 2019 08:28

Operator : HP/JU

Sample : K3360-07

Misc :

ALS Vial : 32 Sample Multiplier: 1

Quant Time: Jun 24 08:54:22 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A41Y7

Manual Integrations

APPROVED

mohammad

6/25/2019 8:45:34 AM

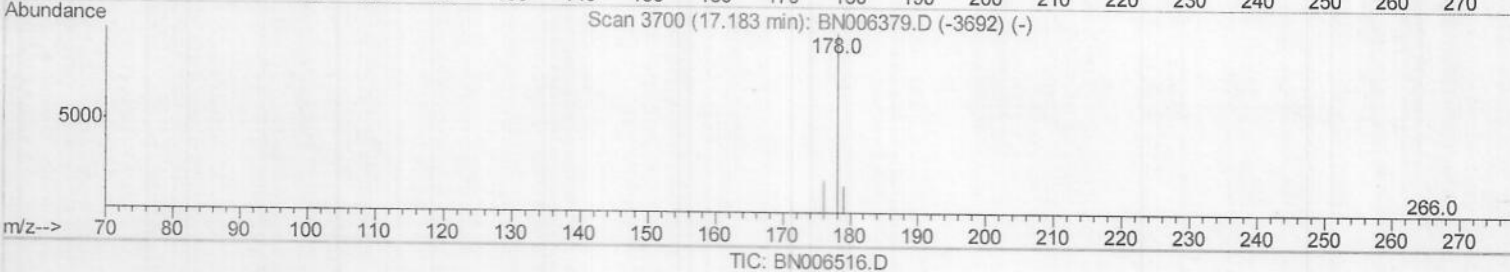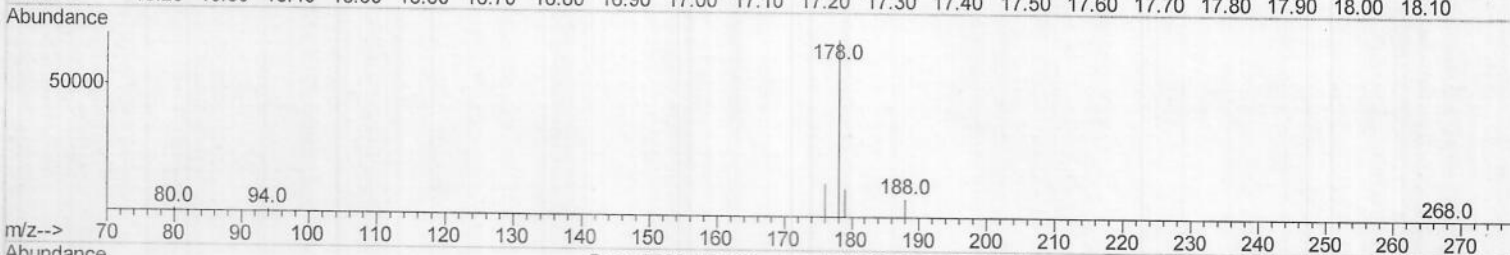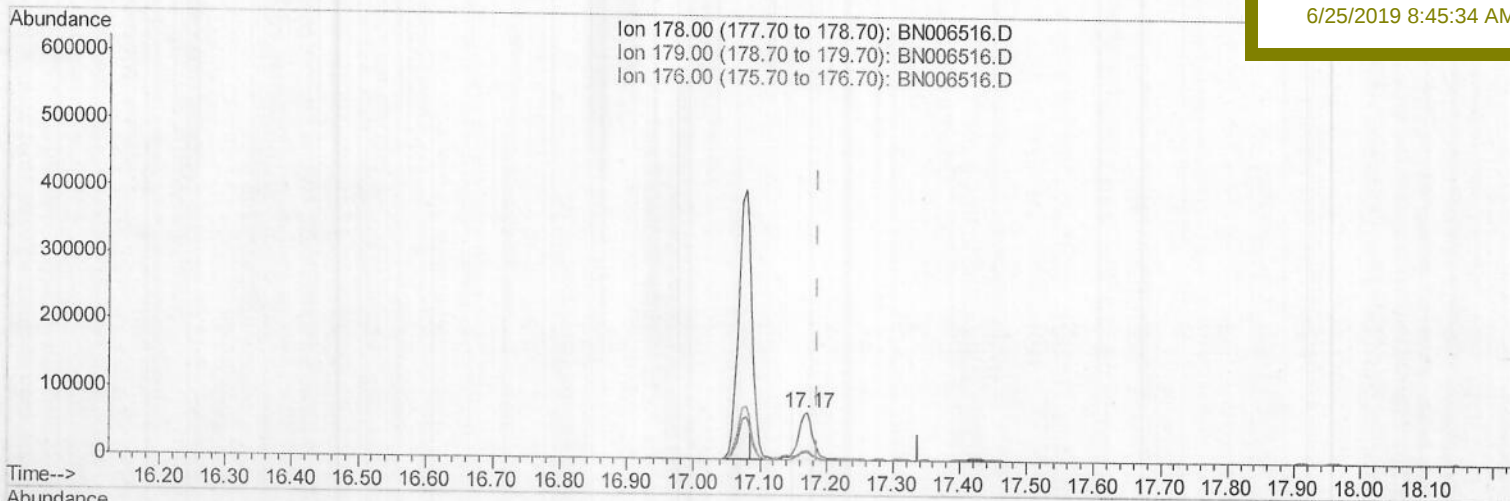

TIC: BN006516.D

(13) Anthracene

17.171min (-0.017) 1.59ng/ul m

> JU 06/26/19

response 105039

Ion	Exp%	Act%
178.00	100	100
179.00	15.30	15.69
176.00	18.90	18.76
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN062219\

Data File : BN006516.D

Acq On : 23 Jun 2019 08:28

Operator : HP/JU

Sample : K3360-07

Misc :

ALS Vial : 32 Sample Multiplier: 1

Quant Time: Jun 24 08:54:22 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019




Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A41Y7

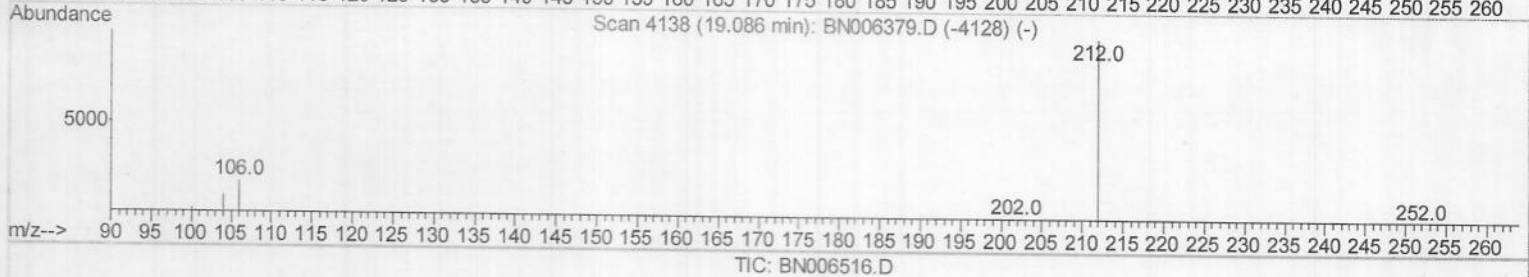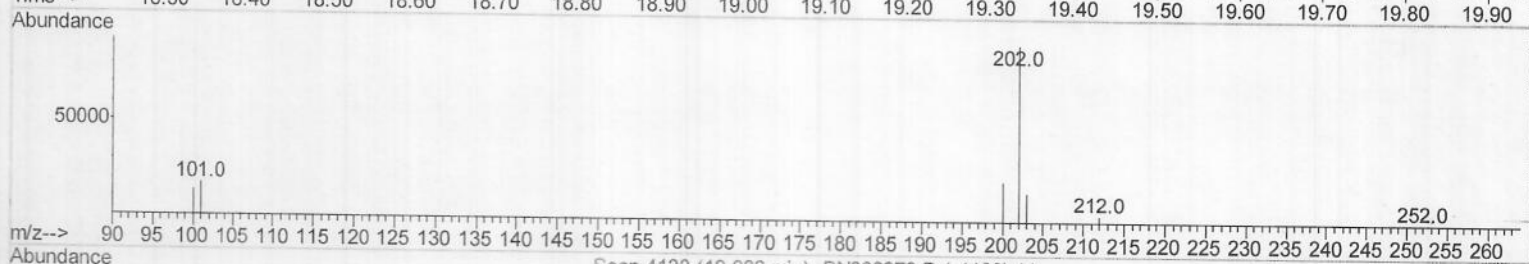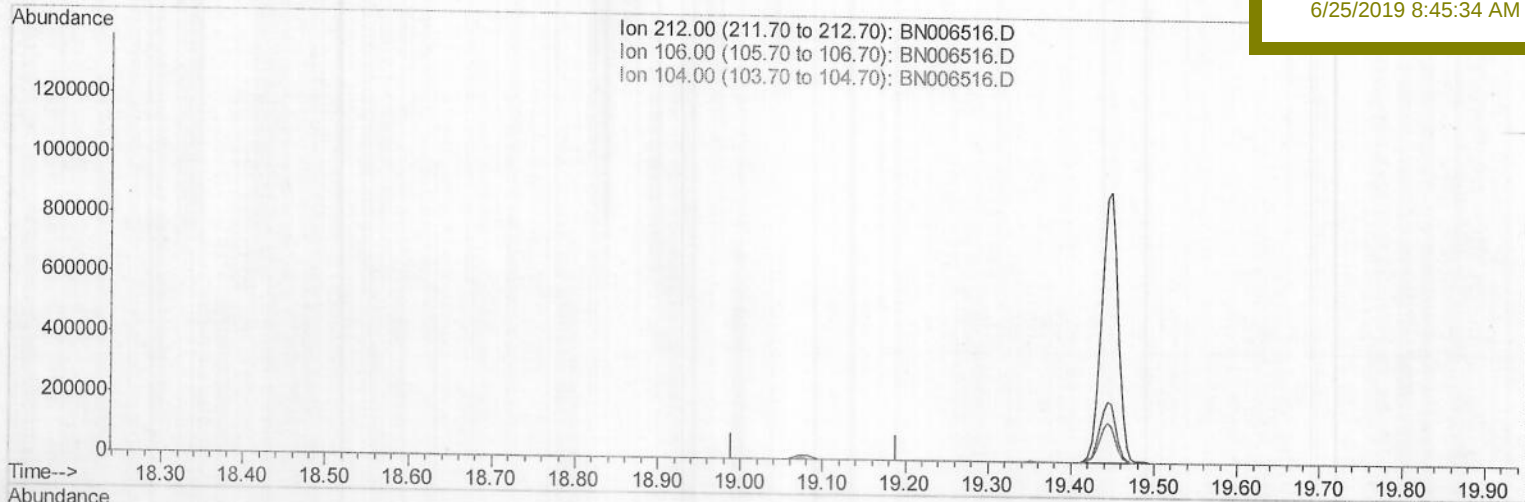Manual Integrations
APPROVEDmohammad
6/25/2019 8:45:34 AM

(14) Fluoranthene-d10 (SURR)

19.090min (-19.090) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN062219\

Data File : BN006516.D

Acq On : 23 Jun 2019 08:28

Operator : HP/JU

Sample : K3360-07

Misc :

ALS Vial : 32 Sample Multiplier: 1

Quant Time: Jun 24 08:54:22 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019



Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A41Y7

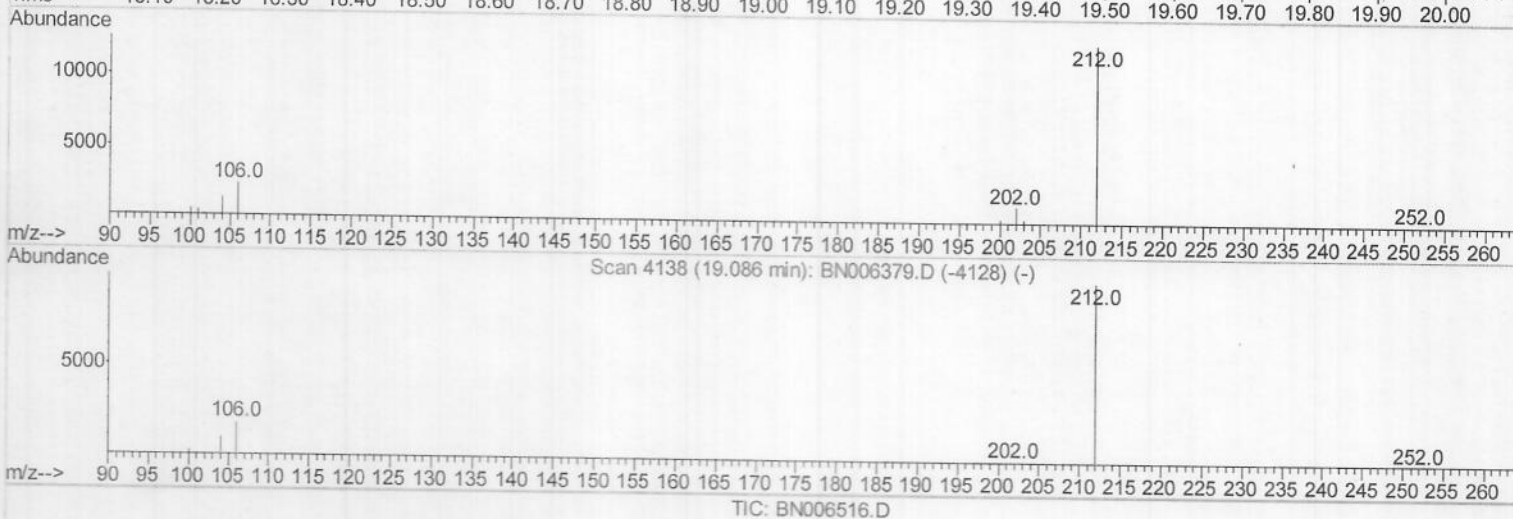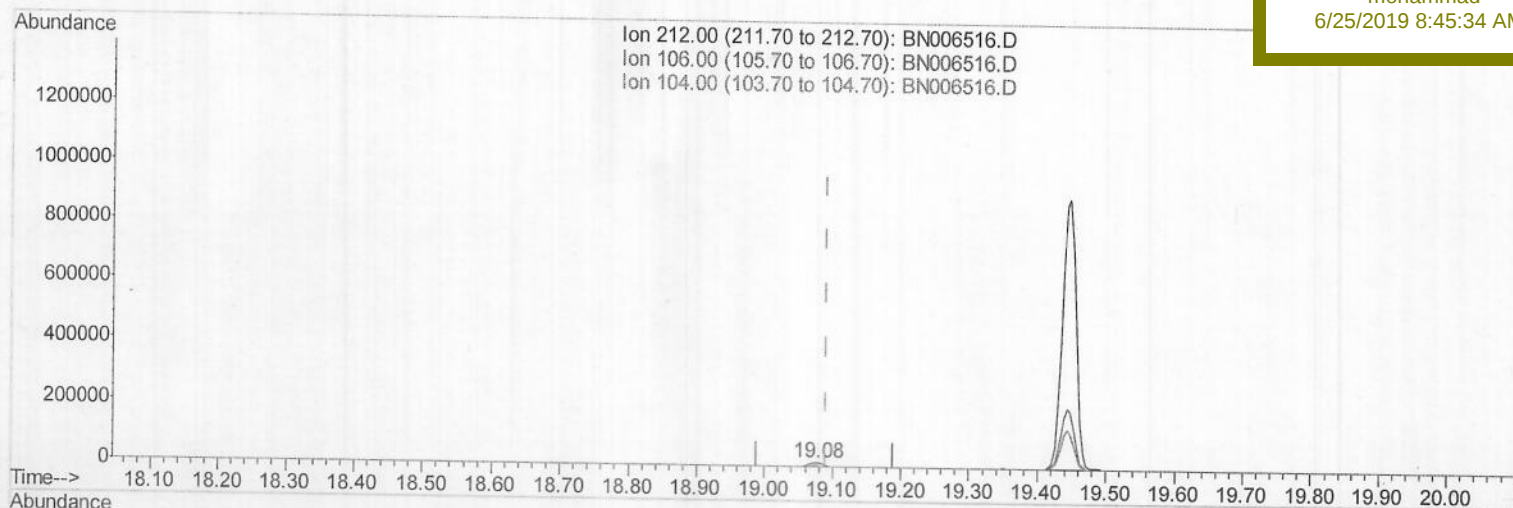Manual Integrations
APPROVEDmohammad
6/25/2019 8:45:34 AM

(14) Fluoranthene-d10 (SURR)

19.076min (-0.014) 0.28ng/ul m

> JU 06/26/19

response 16369

Ion	Exp%	Act%
212.00	100	100
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN062219\
 Data File : BN006516.D
 Acq On : 23 Jun 2019 08:28
 Operator : HP/JU
 Sample : K3360-07
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Quant Time: Jun 24 08:54:22 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 A41Y7

Manual Integrations
 APPROVED

mohammad
 6/25/2019 8:45:34 AM

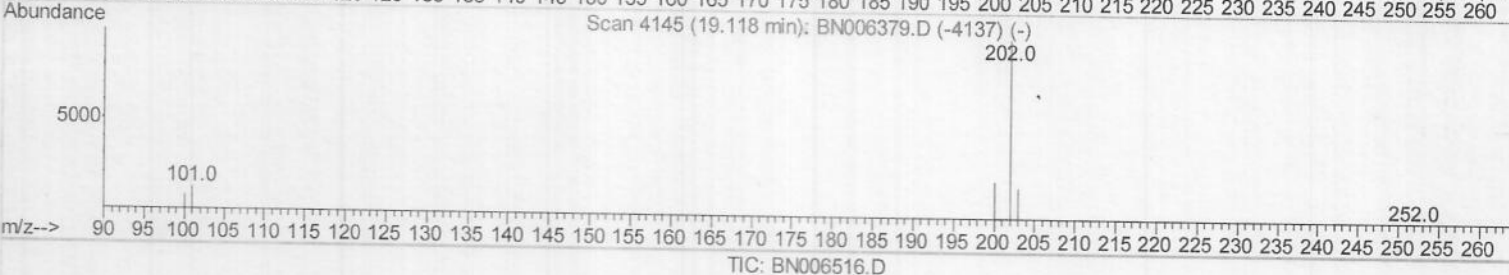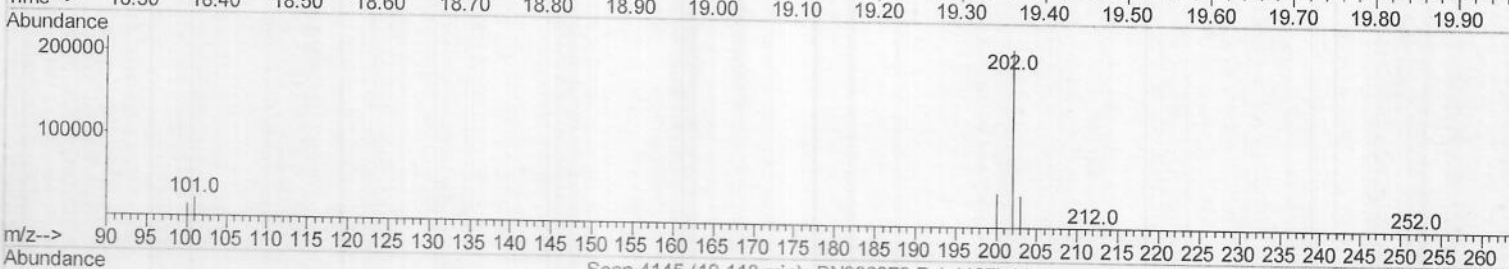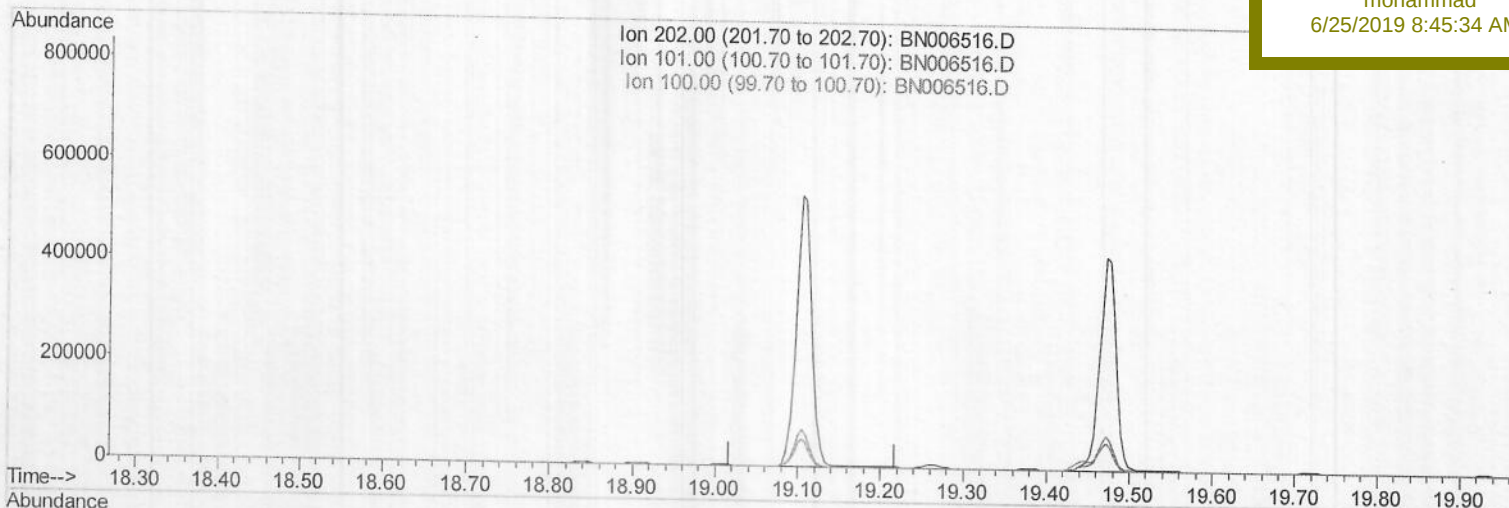

(15) Fluoranthene (C)

19.118min (-19.118) 0.00ng/ul

response 0

Ion	Exp%	Act%
202.00	100	0.00
101.00	12.10	0.00
100.00	8.70	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN062219\

Data File : BN006516.D

Acq On : 23 Jun 2019 08:28

Operator : HP/JU

Sample : K3360-07

Misc :

ALS Vial : 32 Sample Multiplier: 1

Quant Time: Jun 24 08:54:22 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019




Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A41Y7

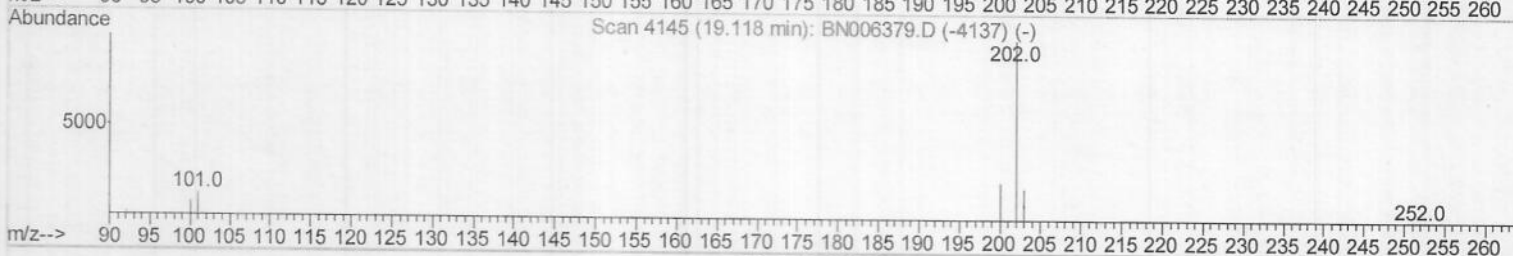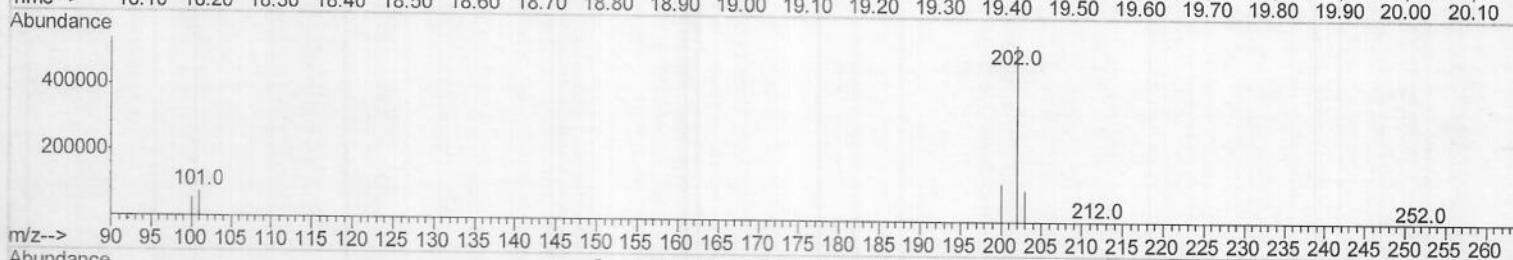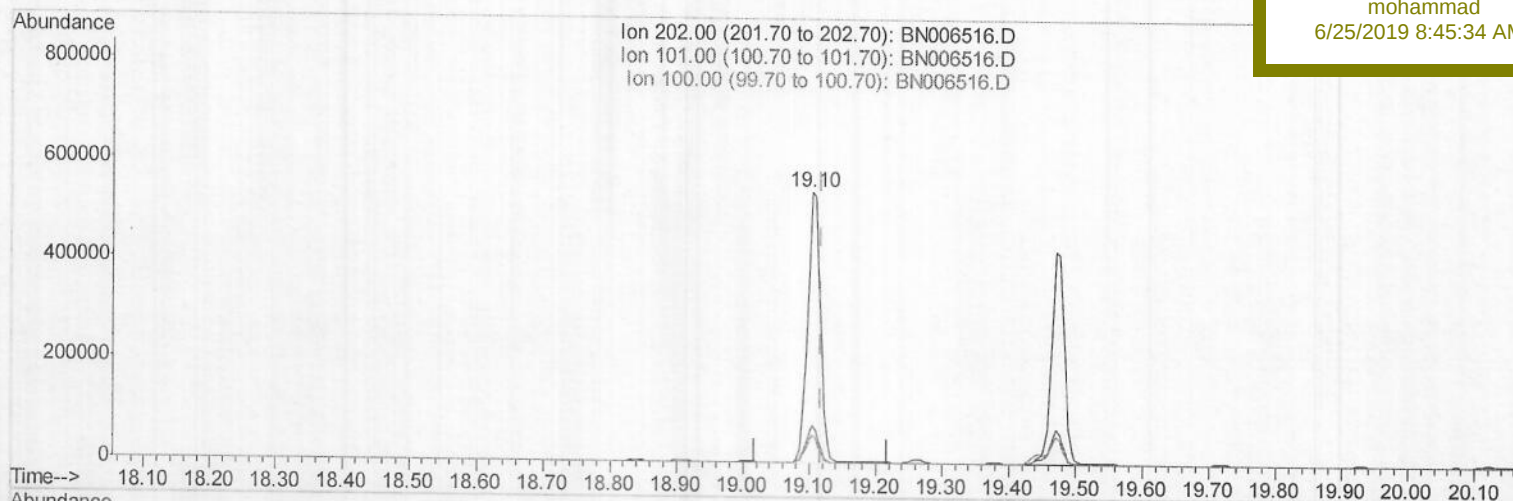Manual Integrations
APPROVEDmohammad
6/25/2019 8:45:34 AM

TIC: BN006516.D

(15) Fluoranthene (C)

19.104min (-0.014) 9.29ng/ul m > JU 06/26/19

response 711512

Ion	Exp%	Act%
202.00	100	100
101.00	12.10	13.74
100.00	8.70	10.10
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN062219\

Data File : BN006516.D

Acq On : 23 Jun 2019 08:28

Operator : HP/JU

Sample : K3360-07

Misc :

ALS Vial : 32 Sample Multiplier: 1

Quant Time: Jun 24 08:54:22 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A41Y7

Manual Integrations

APPROVED

mohammad

6/25/2019 8:45:34 AM

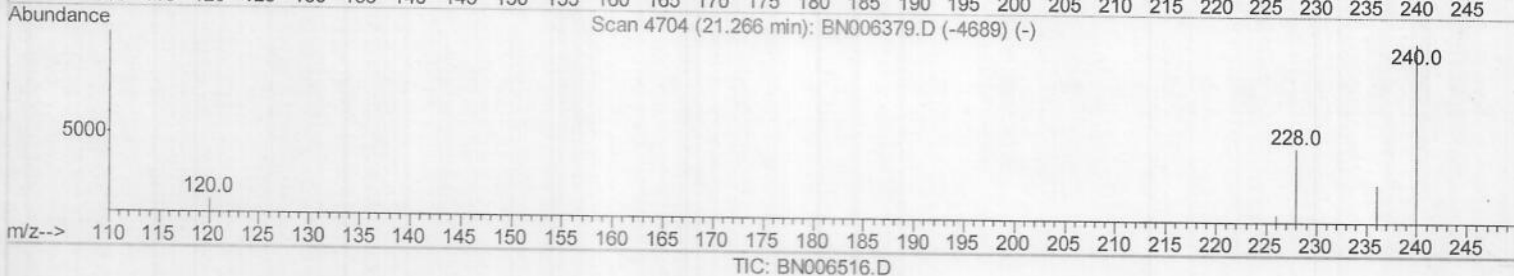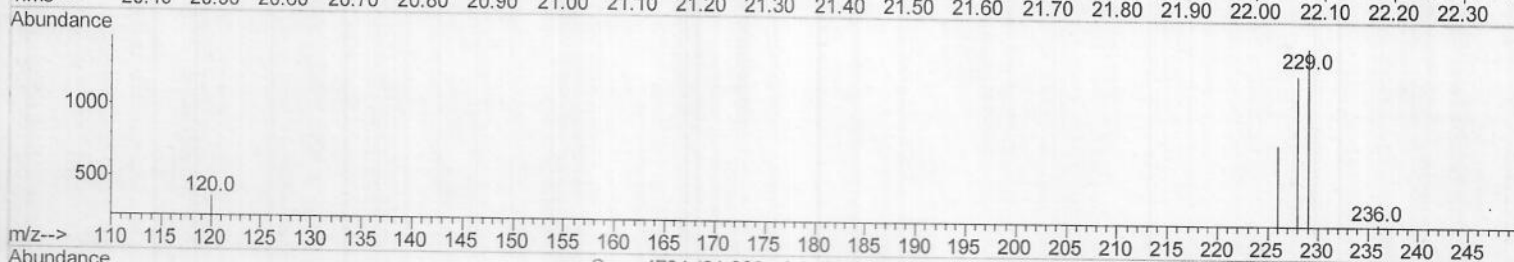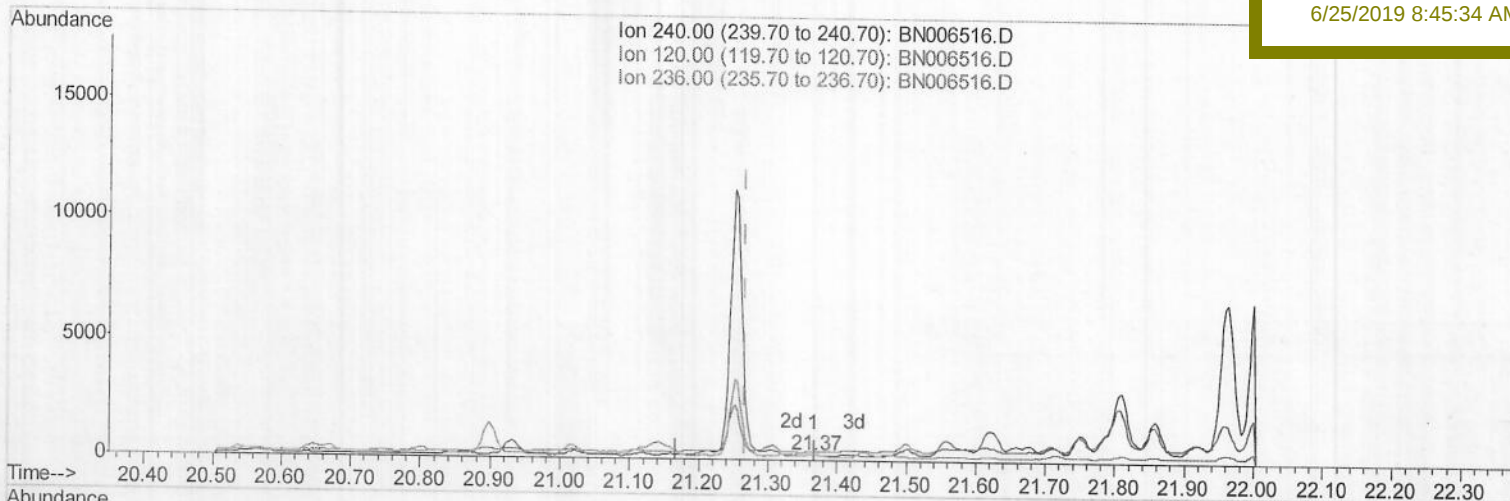

(16) Chrysene-d12 (I)

21.366min (+0.098) 0.40ng/ul

response 43

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	162.10#
236.00	30.10	108.68#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN062219\

Data File : BN006516.D

Acq On : 23 Jun 2019 08:28

Operator : HP/JU

Sample : K3360-07

Misc :

ALS Vial : 32 Sample Multiplier: 1

Quant Time: Jun 24 08:54:22 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

Client Sampled :




A41Y7

Manual Integrations

APPROVED

mohammad

6/25/2019 8:45:34 AM

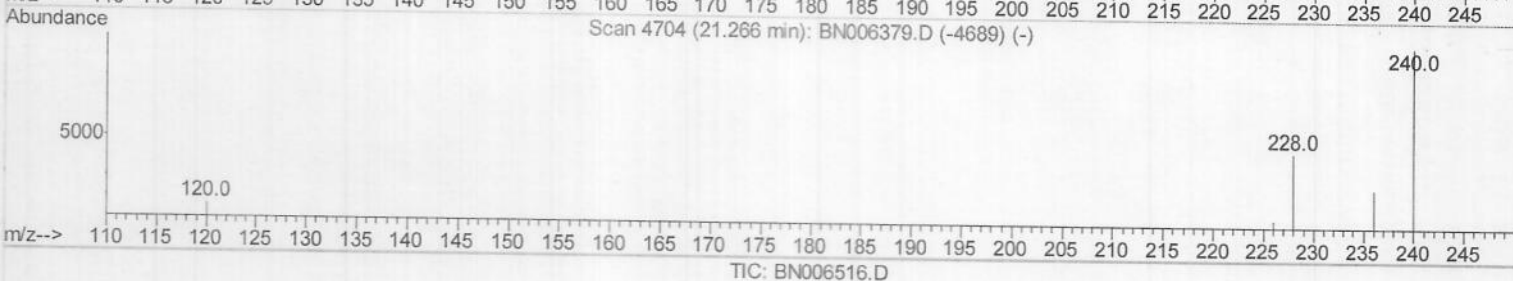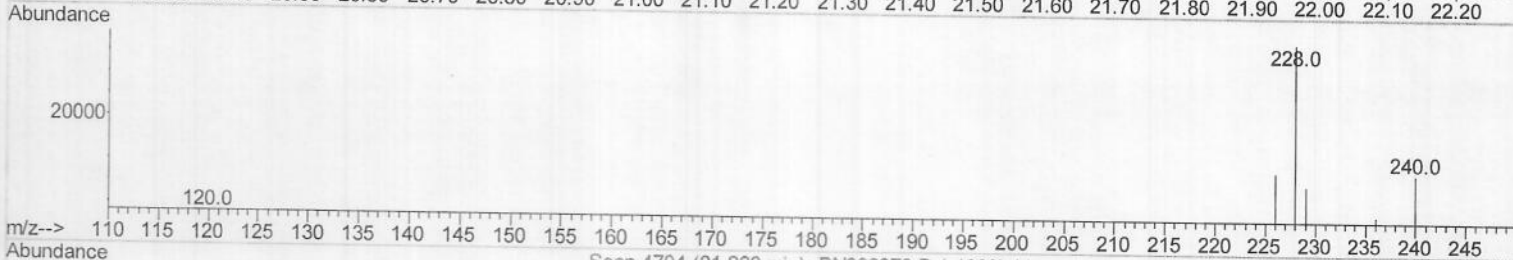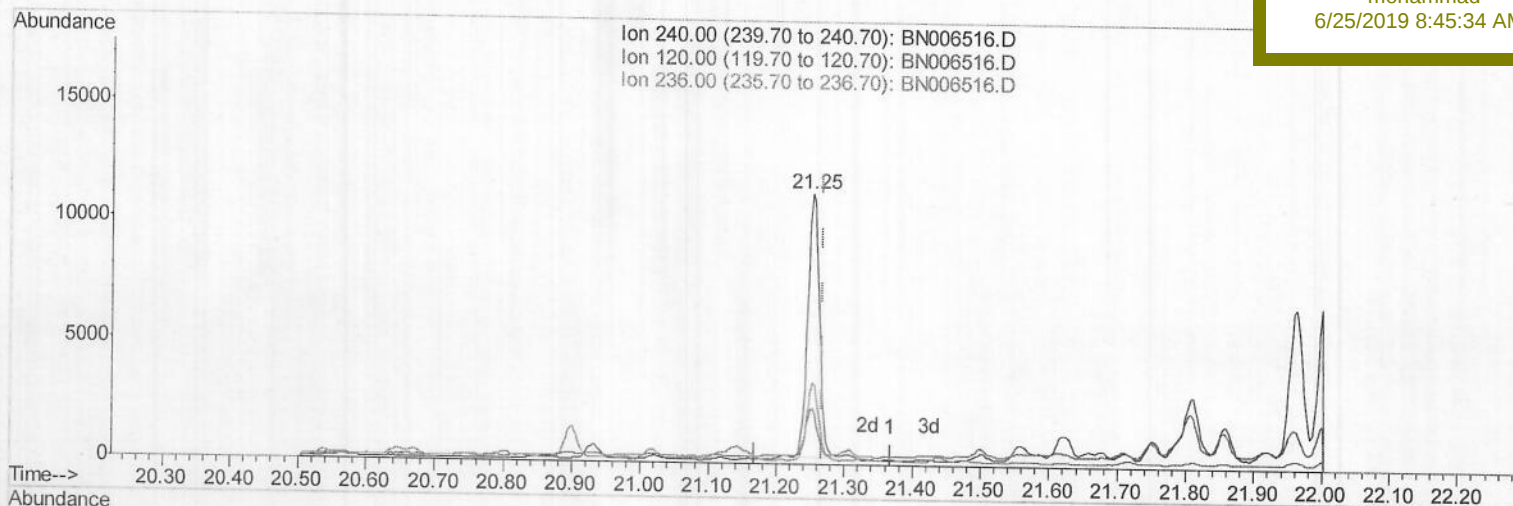

(16) Chrysene-d12 (I)

21.253min (-0.016) 0.40ng/ul m

> JU 06/26/19

response 13016

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	20.52
236.00	30.10	29.92
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN062219\

Data File : BN006516.D

Acq On : 23 Jun 2019 08:28

Operator : HP/JU

Sample : K3360-07

Misc :

ALS Vial : 32 Sample Multiplier: 1

Quant Time: Jun 24 08:56:09 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A41Y7

Manual Integrations

APPROVED

mohammad

6/25/2019 8:45:34 AM

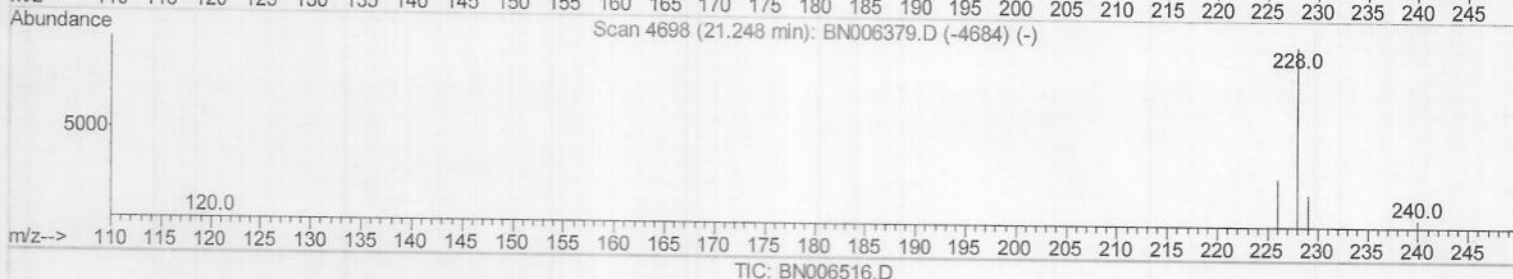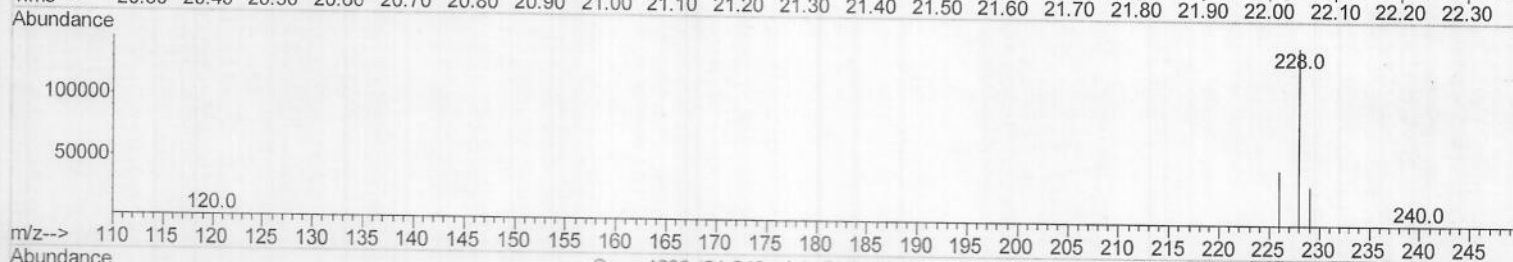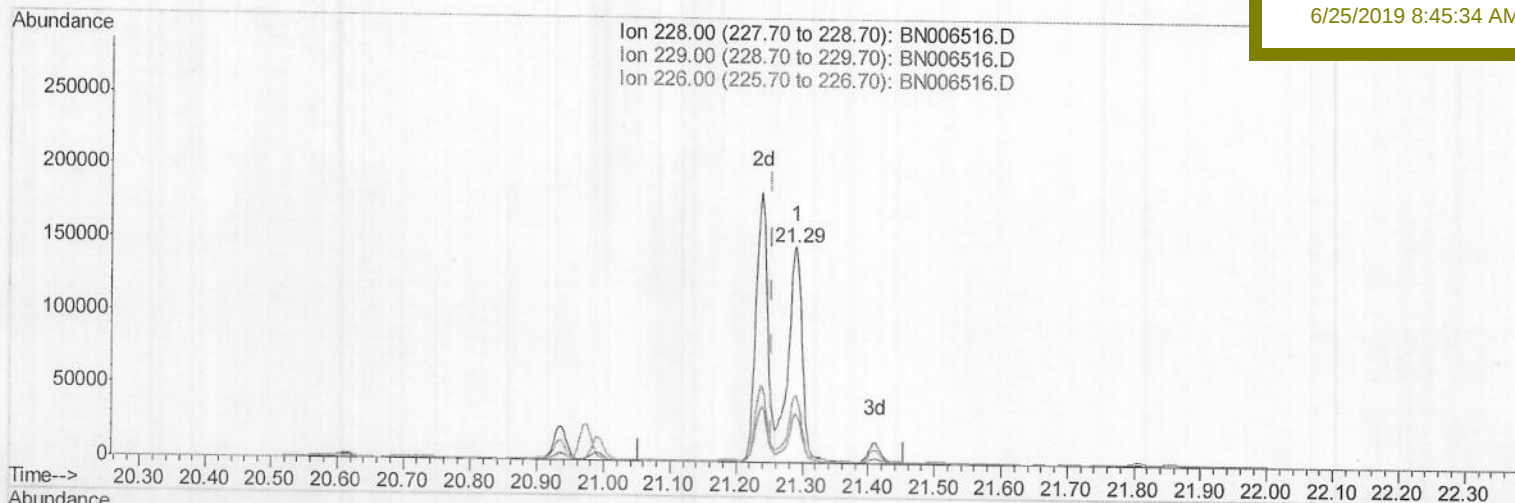

(18) Benzo(a)anthracene

21.291min (+0.037) 3.79ng/ul

response 217991

Ion	Exp%	Act%
228.00	100	100
229.00	20.60	22.15
226.00	28.50	30.93
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN062219\

Data File : BN006516.D

Acq On : 23 Jun 2019 08:28

Operator : HP/JU

Sample : K3360-07

Misc :

ALS Vial : 32 Sample Multiplier: 1

Quant Time: Jun 24 08:56:09 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A41Y7

Manual Integrations

APPROVED

mohammad

6/25/2019 8:45:34 AM

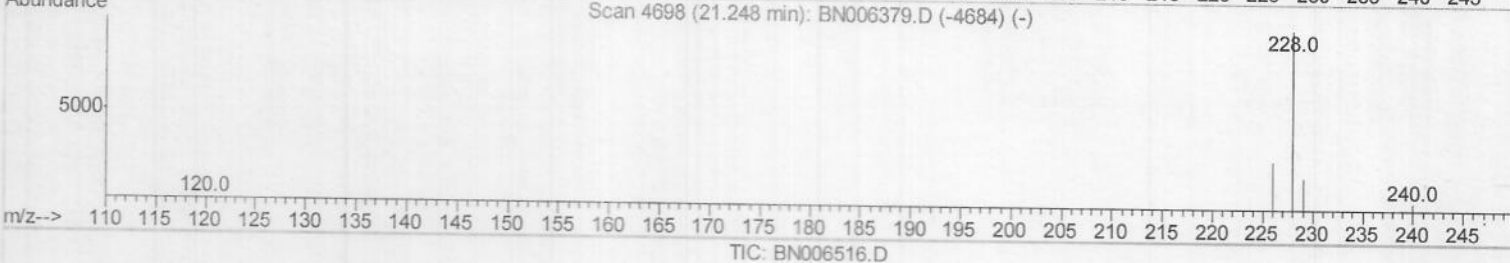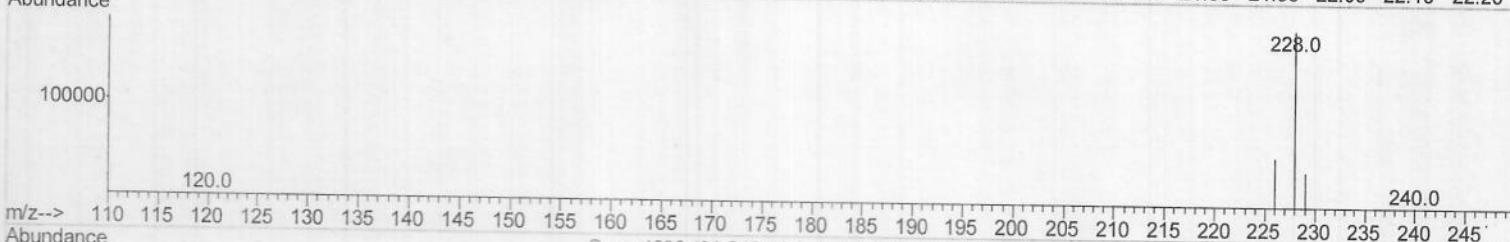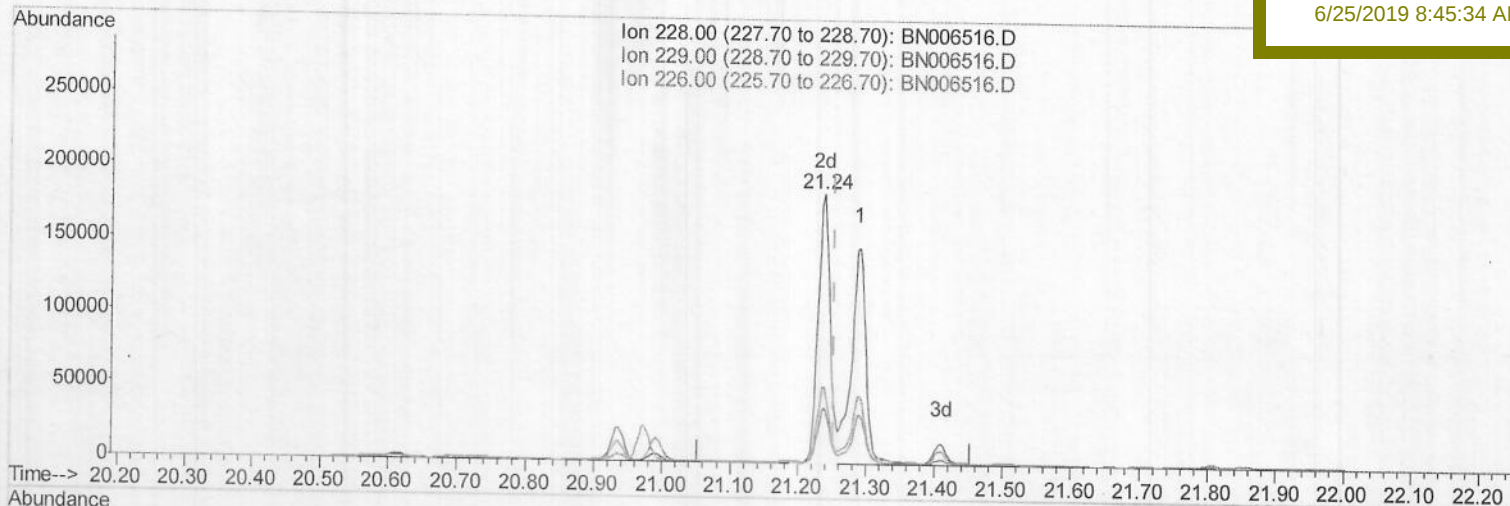

(18) Benzo(a)anthracene

21.238min (-0.016) 3.97ng/ul m

response 228500

Ion	Exp%	Act%
228.00	100	100
229.00	20.60	20.28
226.00	28.50	28.23
0.00	0.00	0.00

> JU 06/26/19

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN062219\

Data File : BN006516.D

Acq On : 23 Jun 2019 08:28

Operator : HP/JU

Sample : K3360-07

Misc :

ALS Vial : 32 Sample Multiplier: 1

Quant Time: Jun 24 08:56:09 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019




Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A41Y7

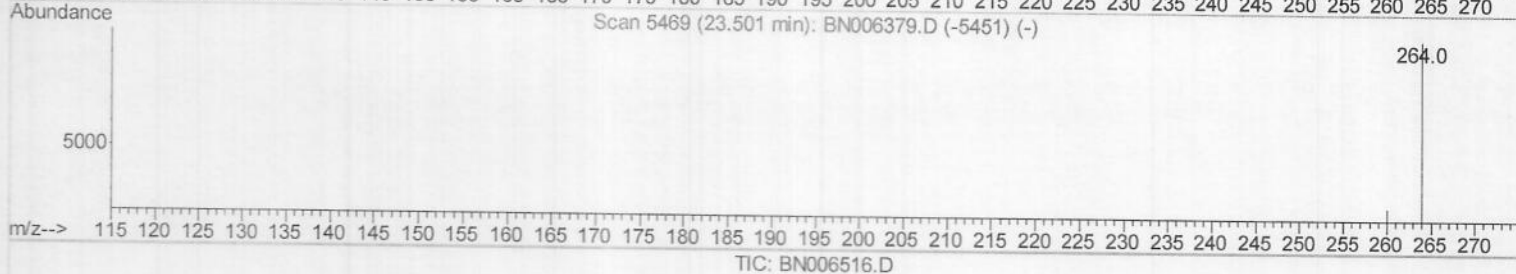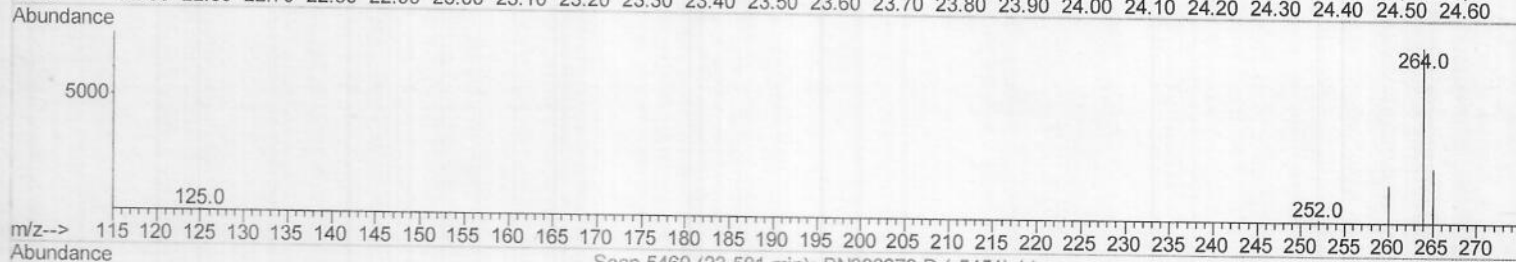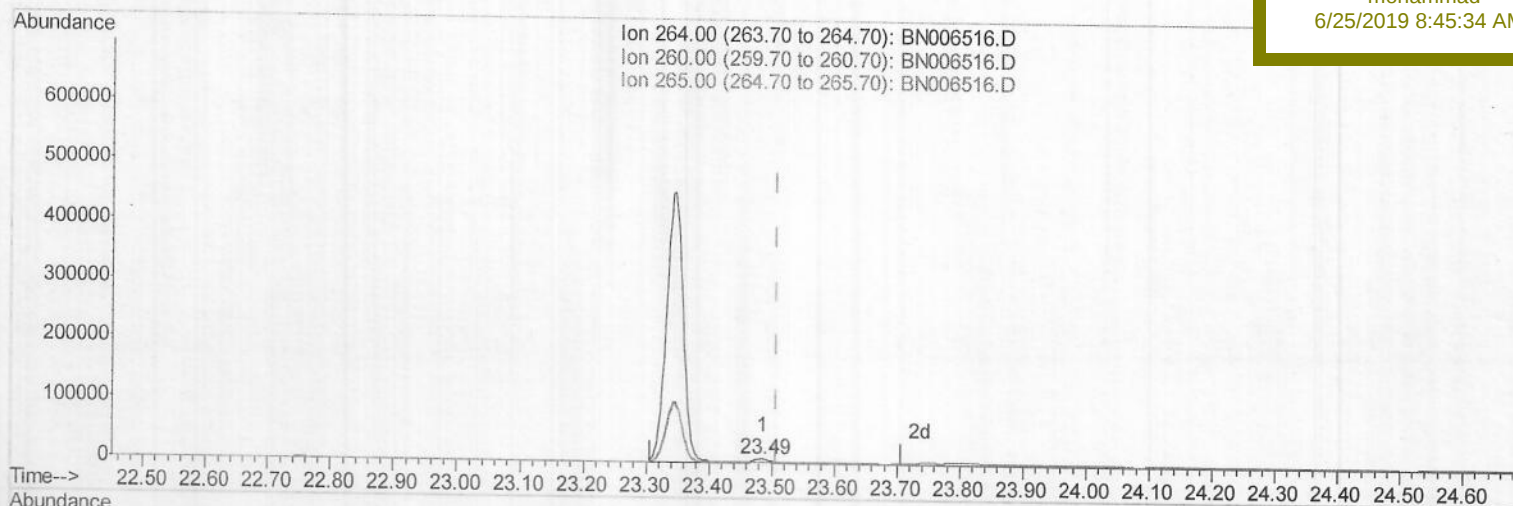Manual Integrations
APPROVEDmohammad
6/25/2019 8:45:34 AM

(20) Perylene-d12 (I)

23.485min (-0.022) 0.40ng/ul

response 16940

Ion	Exp%	Act%
264.00	100	100
260.00	29.20	27.65
265.00	44.70	36.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN062219\

Data File : BN006516.D

Acq On : 23 Jun 2019 08:28

Operator : HP/JU

Sample : K3360-07

Misc :

ALS Vial : 32 Sample Multiplier: 1

Quant Time: Jun 24 08:56:09 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019




Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A41Y7

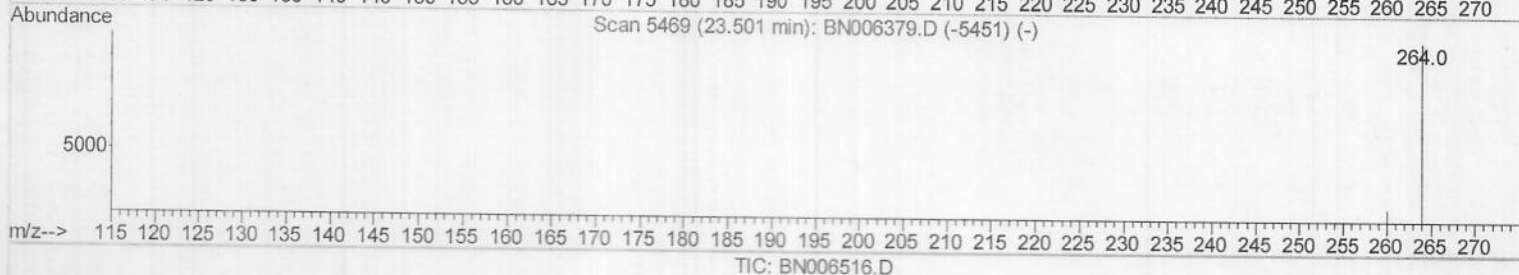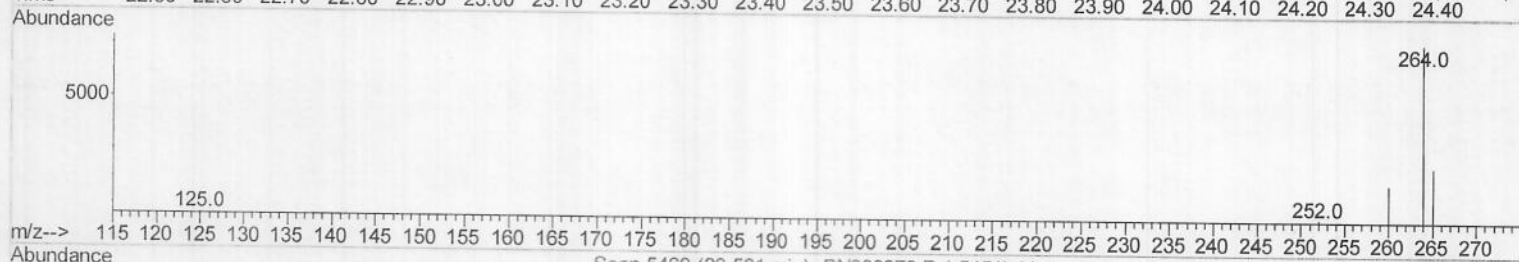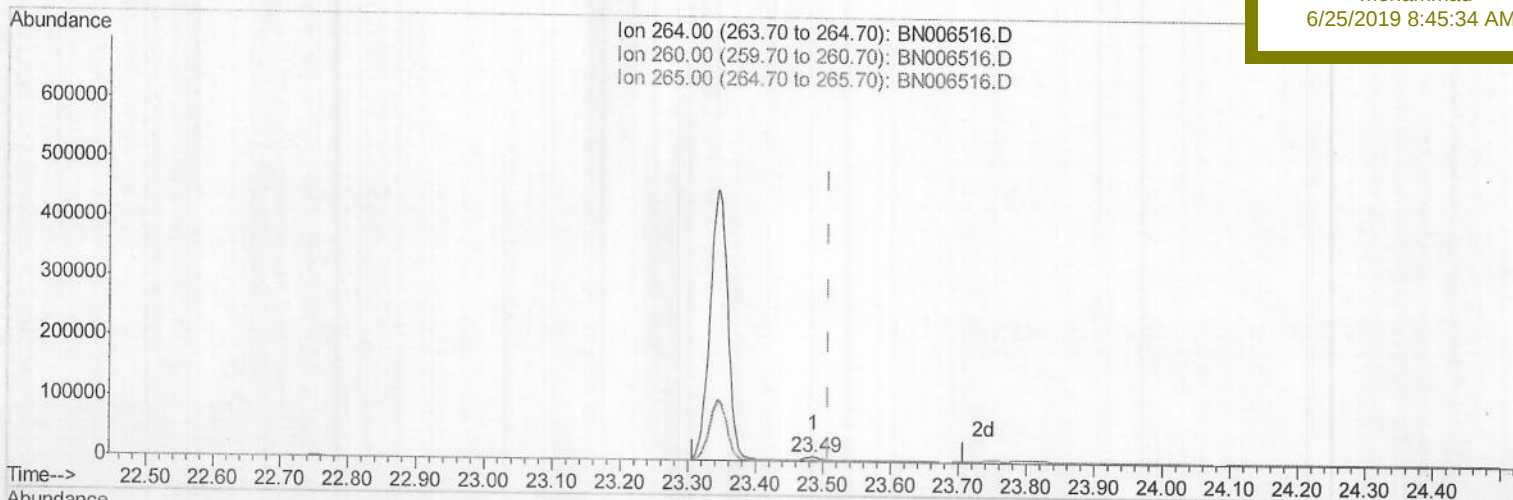Manual Integrations
APPROVEDmohammad
6/25/2019 8:45:34 AM

(20) Perylene-d12 (I)

23.485min (-0.022) 0.40ng/ul m

> JU 06/26/19

response 11017

Ion	Exp%	Act%
264.00	100	100
260.00	29.20	27.65
265.00	44.70	36.50
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN062219\

Data File : BN006516.D

Acq On : 23 Jun 2019 08:28

Operator : HP/JU

Sample : K3360-07

Misc :

ALS Vial : 32 Sample Multiplier: 1

Quant Time: Jun 24 08:57:05 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A41Y7

Manual Integrations

APPROVED

mohammad

6/25/2019 8:45:34 AM

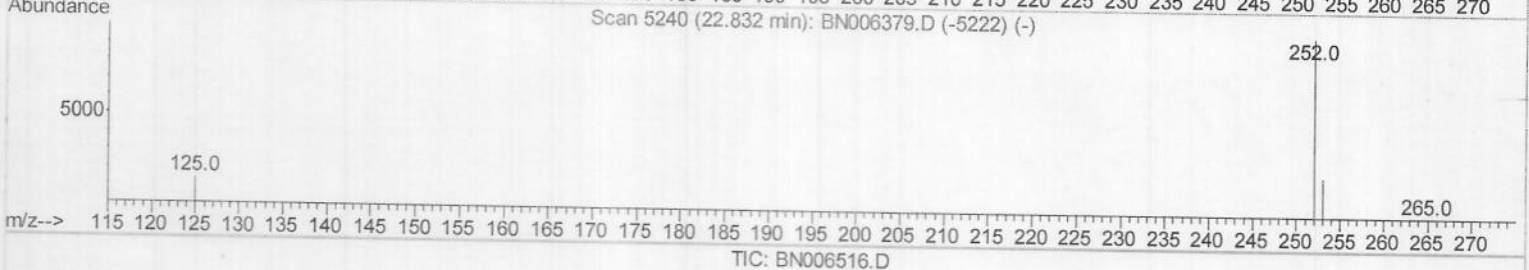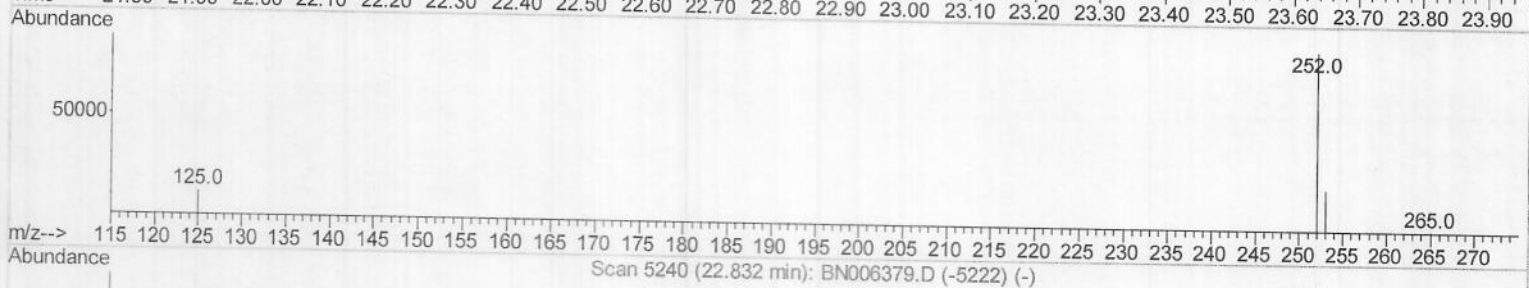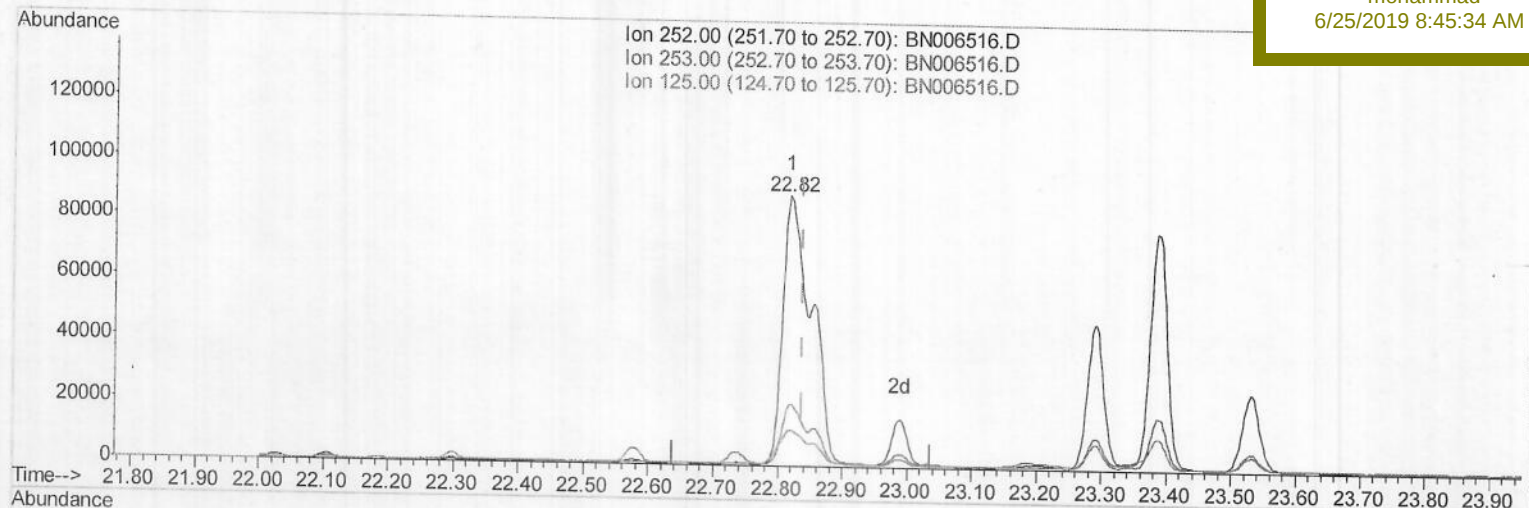

(21) Benzo(b)fluoranthene

22.819min (-0.019) 5.92ng/ul

response 271757

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	22.88
125.00	20.50	13.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN062219\
Data File : BN006516.D
Acq On : 23 Jun 2019 08:28
Operator : HP/JU
Sample : K3360-07
Misc :
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Jun 24 08:57:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

Instrument :




BNA_N

ClientSampleId :

A41Y7

Manual Integrations
APPROVED

mohammad
6/25/2019 8:45:34 AM

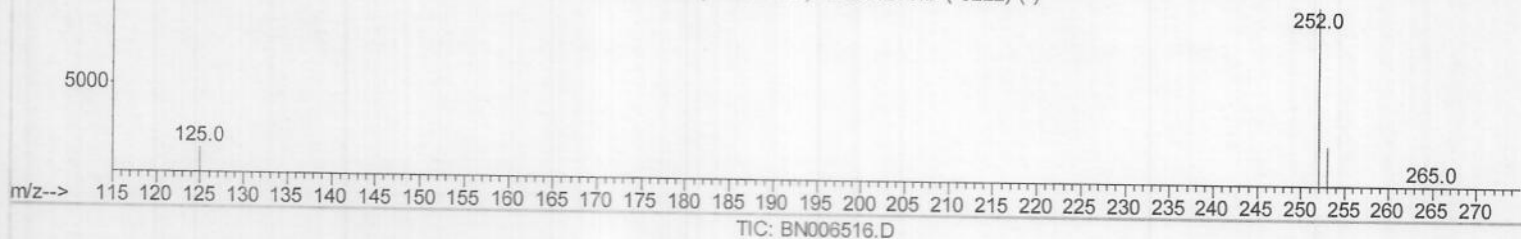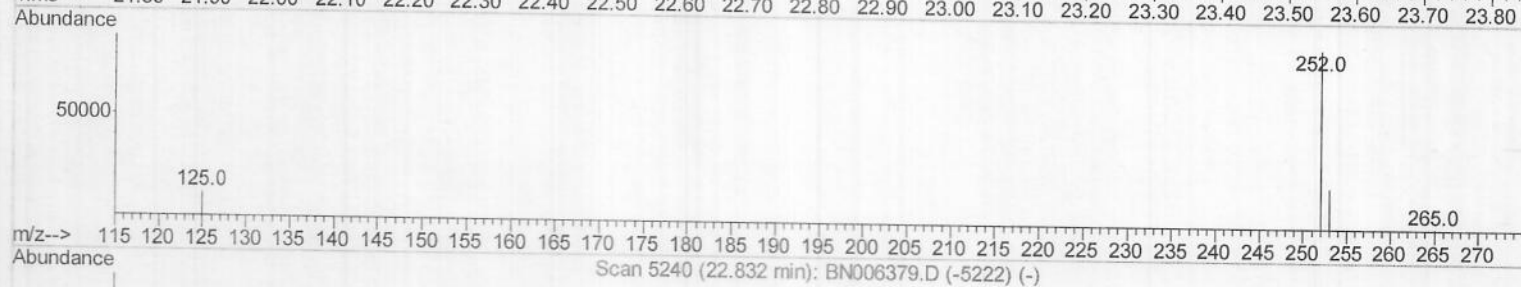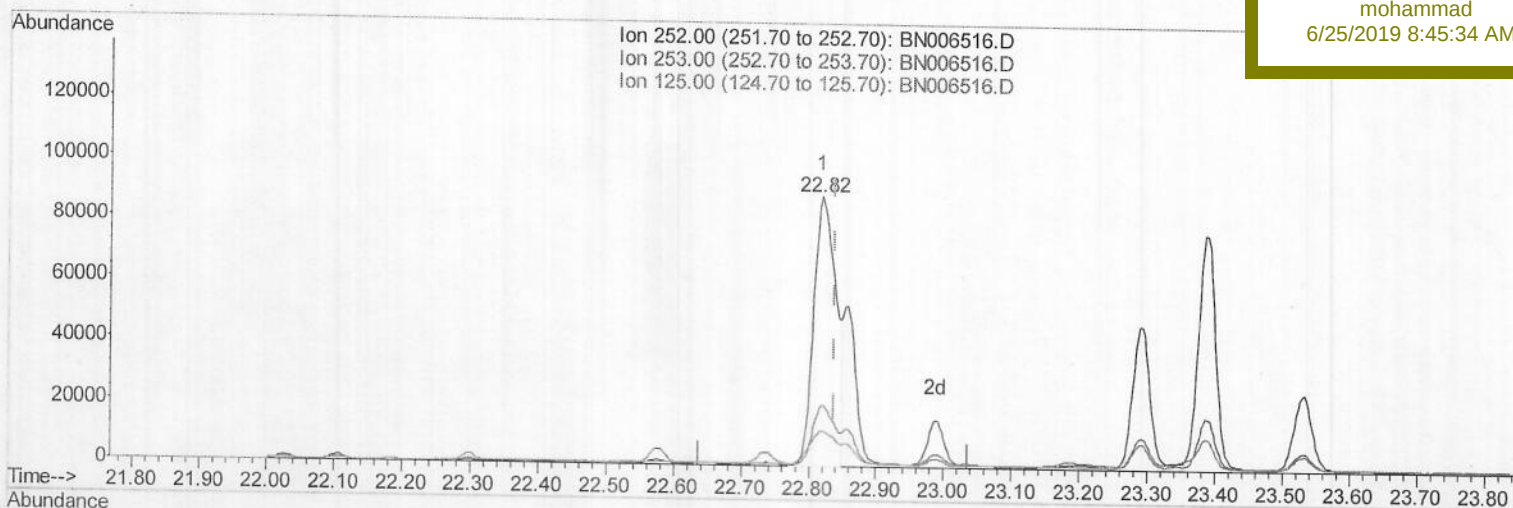

(21) Benzo(b)fluoranthene

22.819min (-0.019) 4.40ng/ul m

> JU 06/26/19

response 202289

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	22.88
125.00	20.50	13.36
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN062219\

Data File : BN006516.D

Acq On : 23 Jun 2019 08:28

Operator : HP/JU

Sample : K3360-07

Misc :

ALS Vial : 32 Sample Multiplier: 1

Quant Time: Jun 24 08:57:05 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A41Y7

Manual Integrations

APPROVED

mohammad

6/25/2019 8:45:34 AM

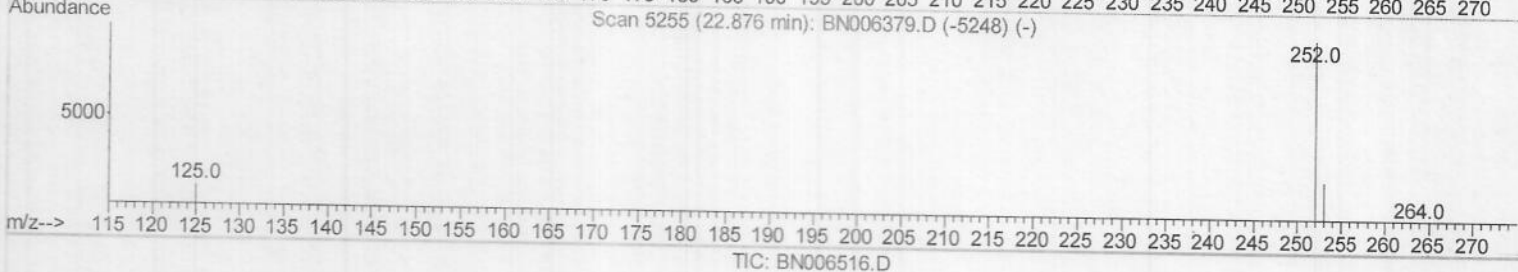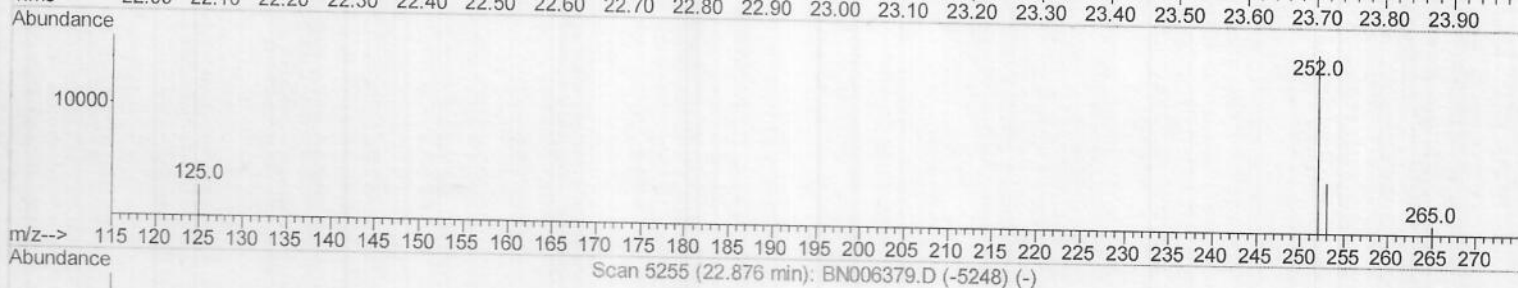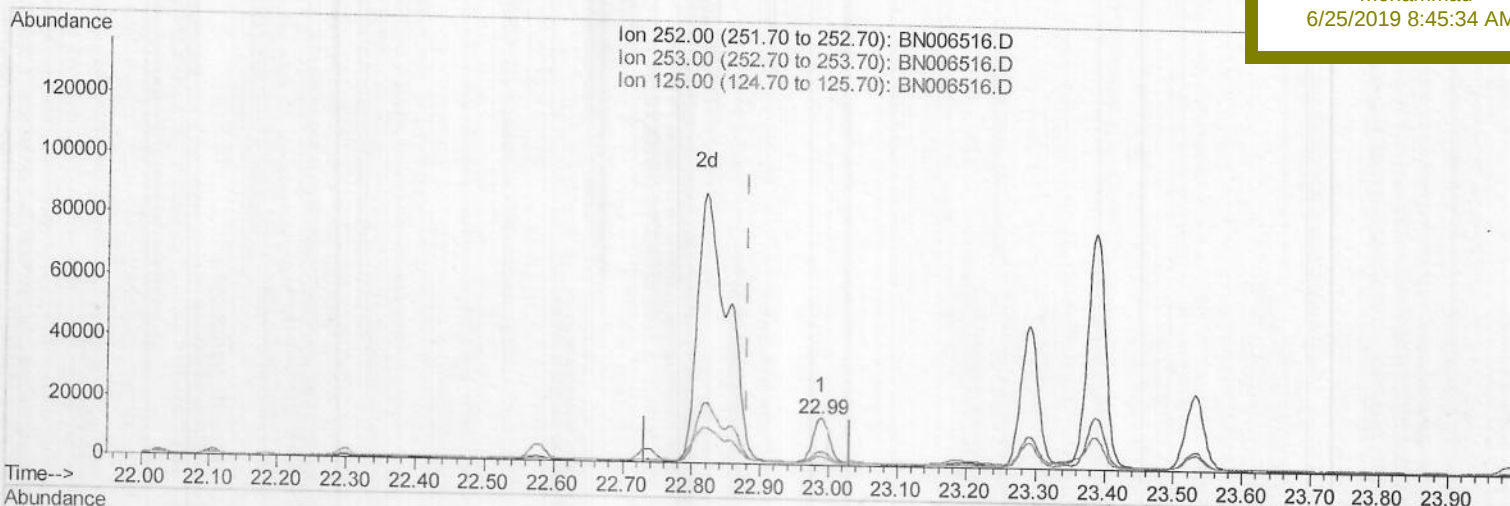

(22) Benzo(k)fluoranthene

22.988min (+0.107) 0.45ng/ul

response 19984

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	29.31
125.00	17.90	18.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN062219\
Data File : BN006516.D
Acq On : 23 Jun 2019 08:28
Operator : HP/JU
Sample : K3360-07
Misc :
ALS Vial : 32 Sample Multiplier: 1




Quant Time: Jun 24 08:57:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

Instrument :

BNA_N

ClientSampled :

A41Y7

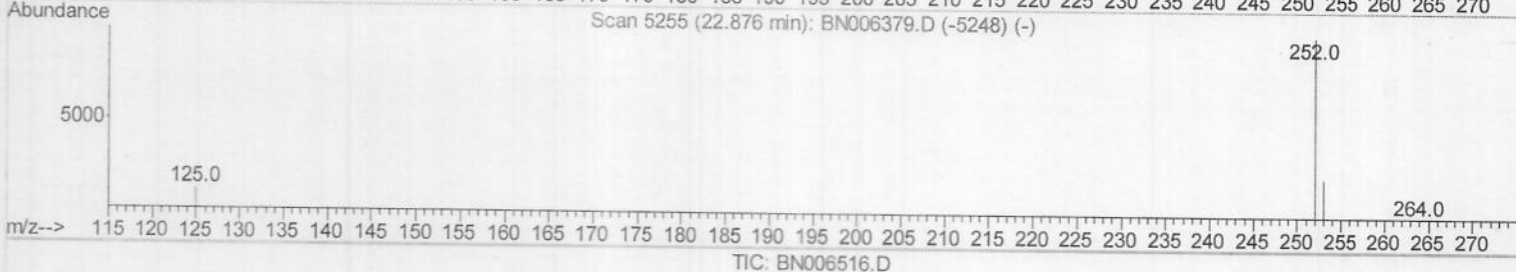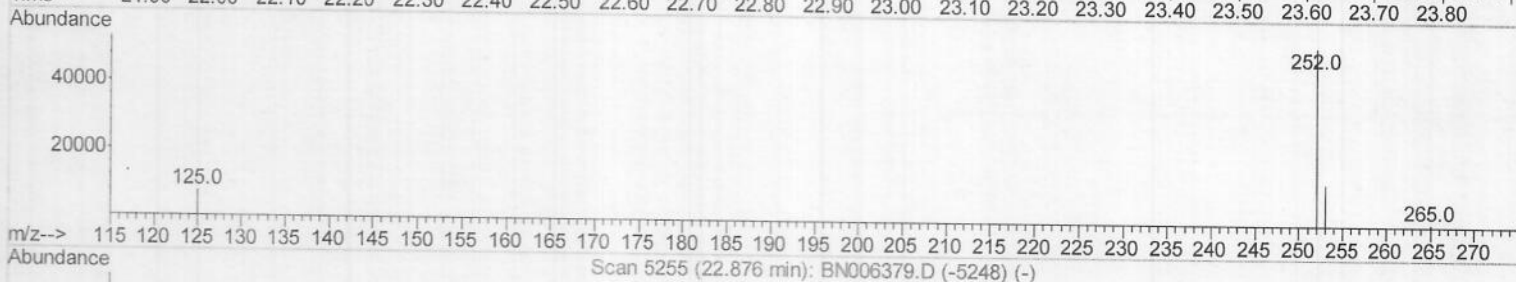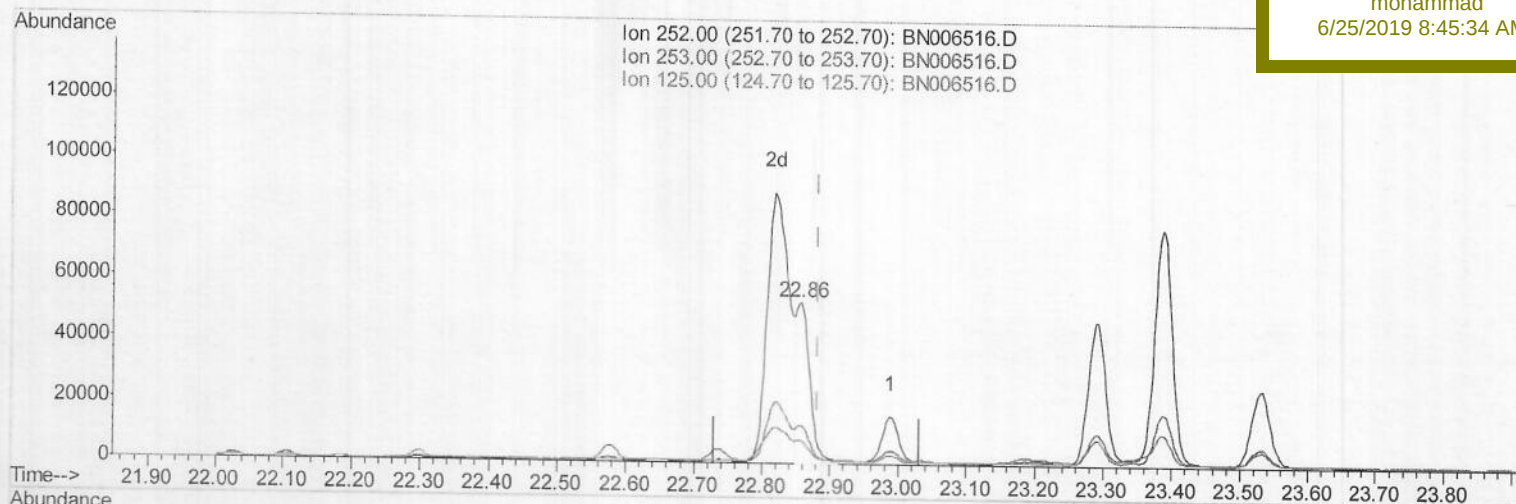Manual Integrations
APPROVEDmohammad
6/25/2019 8:45:34 AM

(22) Benzo(k)fluoranthene

22.857min (-0.024) 1.63ng/ul m

y JU 06/26/19

response 72738

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	23.48
125.00	17.90	14.20#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN062219\

Data File : BN006516.D

Acq On : 23 Jun 2019 08:28

Operator : HP/JU

Sample : K3360-07

Misc :

ALS Vial : 32 Sample Multiplier: 1

Quant Time: Jun 24 08:57:48 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A41Y7

Manual Integrations
APPROVEDmohammad
6/25/2019 8:45:34 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	4946	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.41	136	18834	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.28	164	10301	0.40	ng/ul	-0.01
10) Phenanthrene-d10	17.04	188	21608m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.25	240	13016m	0.40	ng/ul	-0.02
20) Perylene-d12	23.49	264	11017m	0.40	ng/ul	-0.02

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.01	152	7143	0.25	ng/ul	-0.02
14) Fluoranthene-d10	19.08	212	16369m	0.28	ng/ul	-0.01

Target Compounds

	R.T.	QIon	Response	Conc	Units	Dev(Min)	Ovalue
3) Naphthalene	10.46	128	3055	0.059	ng/ul#		92
5) 2-Methylnaphthalene	12.08	142	1223	0.034	ng/ul		98
7) Acenaphthylene	14.00	152	16514	0.288	ng/ul		99
8) Acenaphthene	14.34	153	12567	0.316	ng/ul		100
9) Fluorene	15.34	166	27844	0.599	ng/ul		99
12) Phenanthrene	17.08	178	554100m	7.989	ng/ul		
13) Anthracene	17.17	178	105039m	1.586	ng/ul		
15) Fluoranthene	19.10	202	711512m	9.290	ng/ul		
17) Pyrene	19.47	202	573724	8.368	ng/ul		99
18) Benzo(a)anthracene	21.24	228	228500m	3.969	ng/ul		
19) Chrysene	21.29	228	217329	4.021	ng/ul		98
21) Benzo(b)fluoranthene	22.82	252	202289m	4.404	ng/ul		
22) Benzo(k)fluoranthene	22.86	252	72738m	1.626	ng/ul		
23) Benzo(a)pyrene	23.39	252	139283	3.255	ng/ul#		84
24) Indeno(1,2,3-cd)pyrene	25.71	276	73991	1.598	ng/ul#		89
25) Dibenzo(a,h)anthracene	25.72	278	20933	0.565	ng/ul		97
26) Benzo(a,h,i)perylene	26.40	276	52714	1.359	ng/ul		95

(#) = qualifier out of range (m) = manual integration (+) = signals summed