

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062219\
 Data File : BN006501.D
 Acq On : 22 Jun 2019 22:08
 Operator : HP/JU
 Sample : K3360-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A41Y5

Manual Integrations
 APPROVED

mohammad
 6/25/2019 8:44:44 AM

Quant Time: Jun 24 09:02:57 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	4752	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.41	136	18674	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.28	164	10490	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	20989m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.25	240	12782m	0.40	ng/ul	-0.02
20) Perylene-d12	23.47	264	9761m	0.40	ng/ul	-0.03
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.01	152	7792	0.27	ng/ul	-0.01
14) Fluoranthene-d10	19.08	212	18123m	0.32	ng/ul	-0.01
Target Compounds						
19) Chrysene	21.29	228	1355m	0.026	ng/ul	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062219\
Data File : BN006501.D
Acq On : 22 Jun 2019 22:08
Operator : HP/JU
Sample : K3360-04
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
A41Y5

Manual Integrations
APPROVED

mohammad
6/25/2019 8:44:44 AM

Quant Time: Jun 24 09:02:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

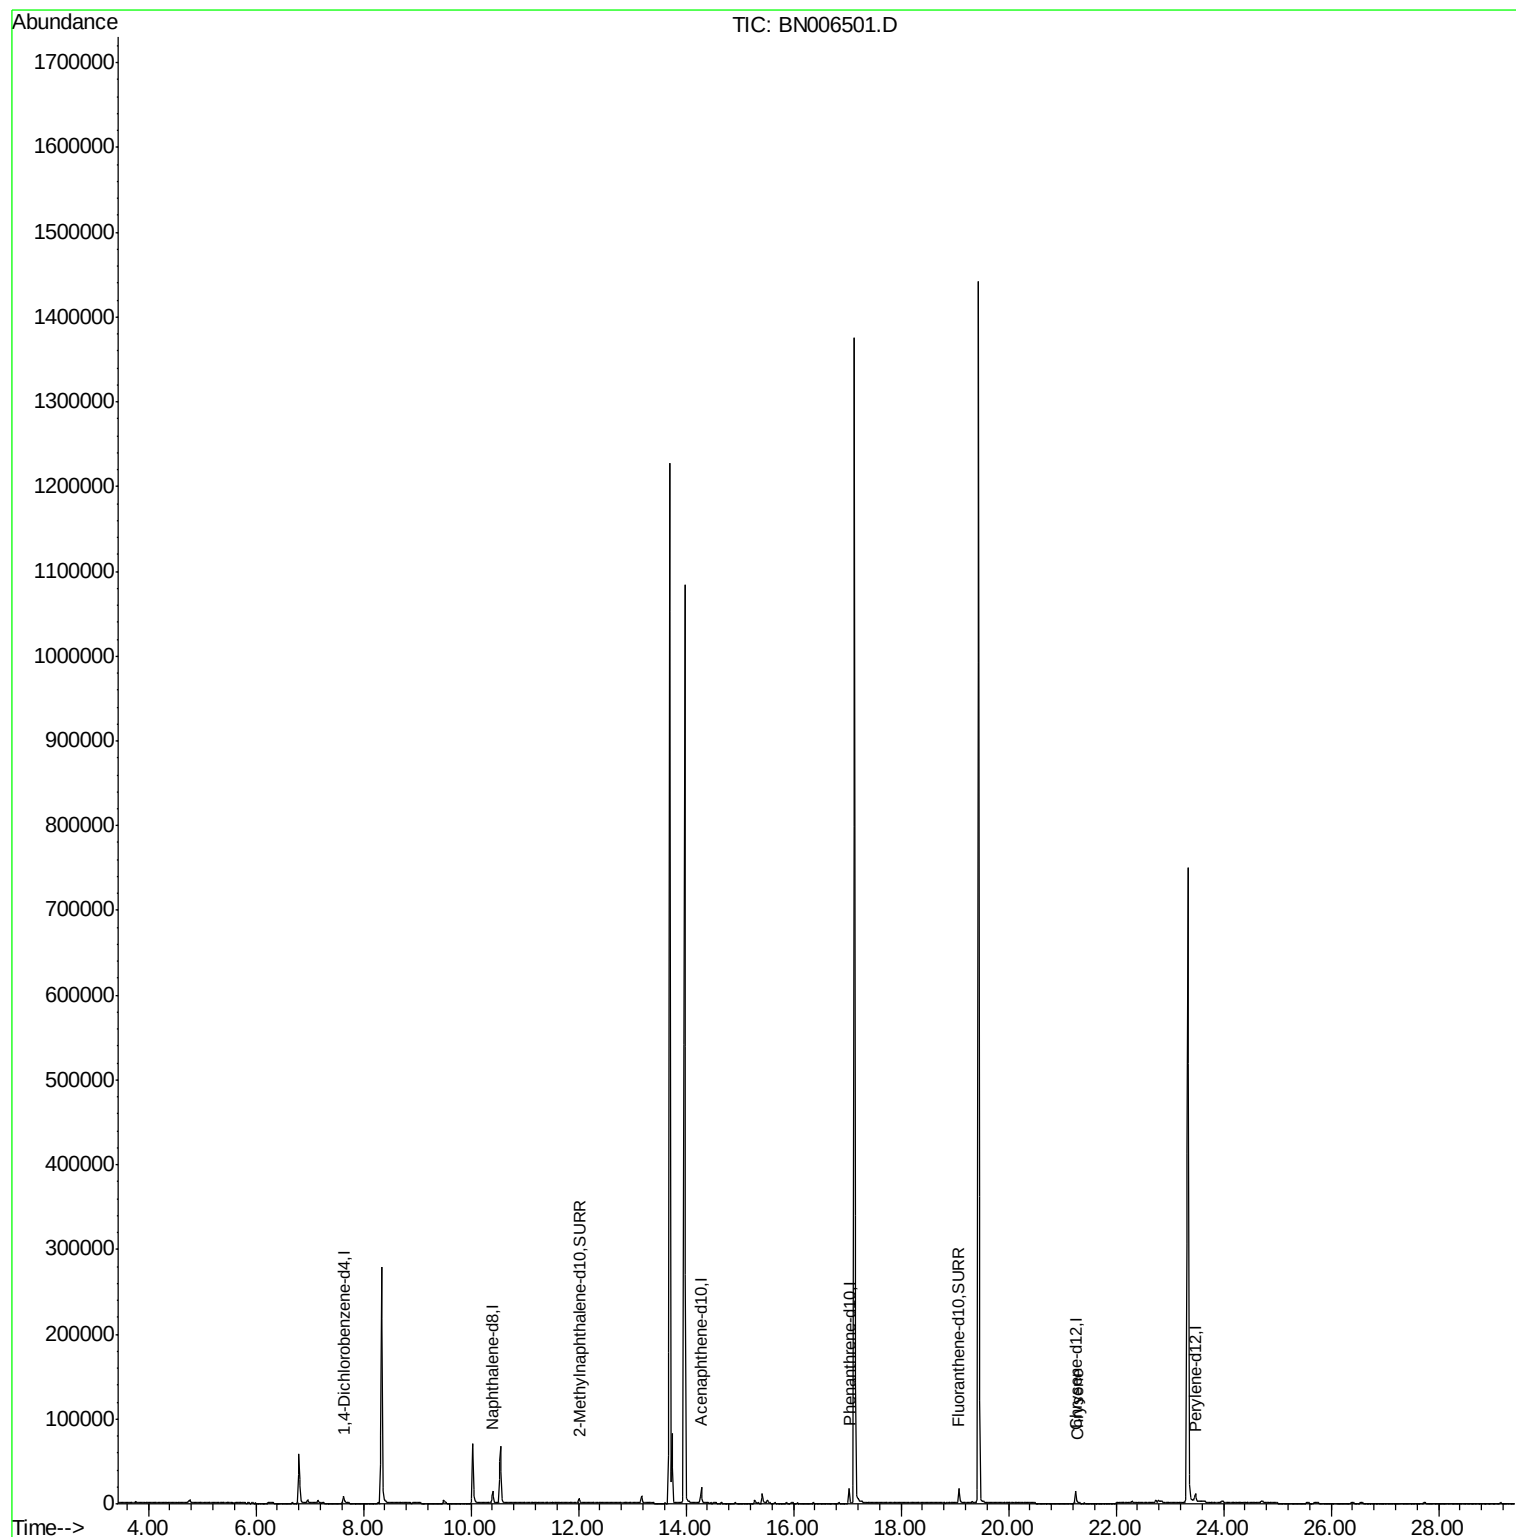

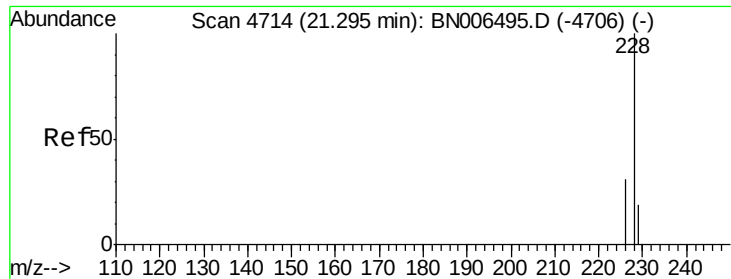

#19

Chrysene

Concen: 0.026 ng/ul m

RT: 21.29 min Scan# 4711

Delta R.T. -0.02 min

Lab File: BN006501.D


Acq: 22 Jun 2019 22:08

Instrument :

BNA_N

ClientSampleId :

A41Y5

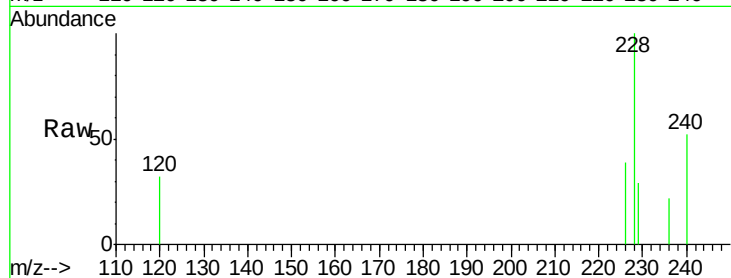

Tgt	Ion:228	Resp:	1355
Ion	Ratio	Lower	Upper
228	100		
226	38.8	25.0	37.6#
229	29.4	16.3	24.5#

Manual Integrations
APPROVED

mohammad
6/25/2019 8:44:44 AM

