

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062219\
 Data File : BN006517.D
 Acq On : 23 Jun 2019 09:02
 Operator : HP/JU
 Sample : K3360-17
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A41X2

Manual Integrations
 APPROVED

mohammad
 6/25/2019 8:45:37 AM

Quant Time: Jun 24 08:52:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	5316	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.41	136	20010	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.28	164	10222	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	17422m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.26	240	11507m	0.40	ng/ul	-0.01
20) Perylene-d12	23.49	264	11105m	0.40	ng/ul	-0.02
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.01	152	10347	0.34	ng/ul	-0.02
14) Fluoranthene-d10	19.08	212	16717m	0.36	ng/ul	-0.01
Target Compounds						
21) Benzo(b)fluoranthene	22.82	252	1581m	0.034	ng/ul	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062219\
Data File : BN006517.D
Acq On : 23 Jun 2019 09:02
Operator : HP/JU
Sample : K3360-17
Misc :
ALS Vial : 33 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
A41X2

Manual Integrations
APPROVED

mohammad
6/25/2019 8:45:37 AM

Quant Time: Jun 24 08:52:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

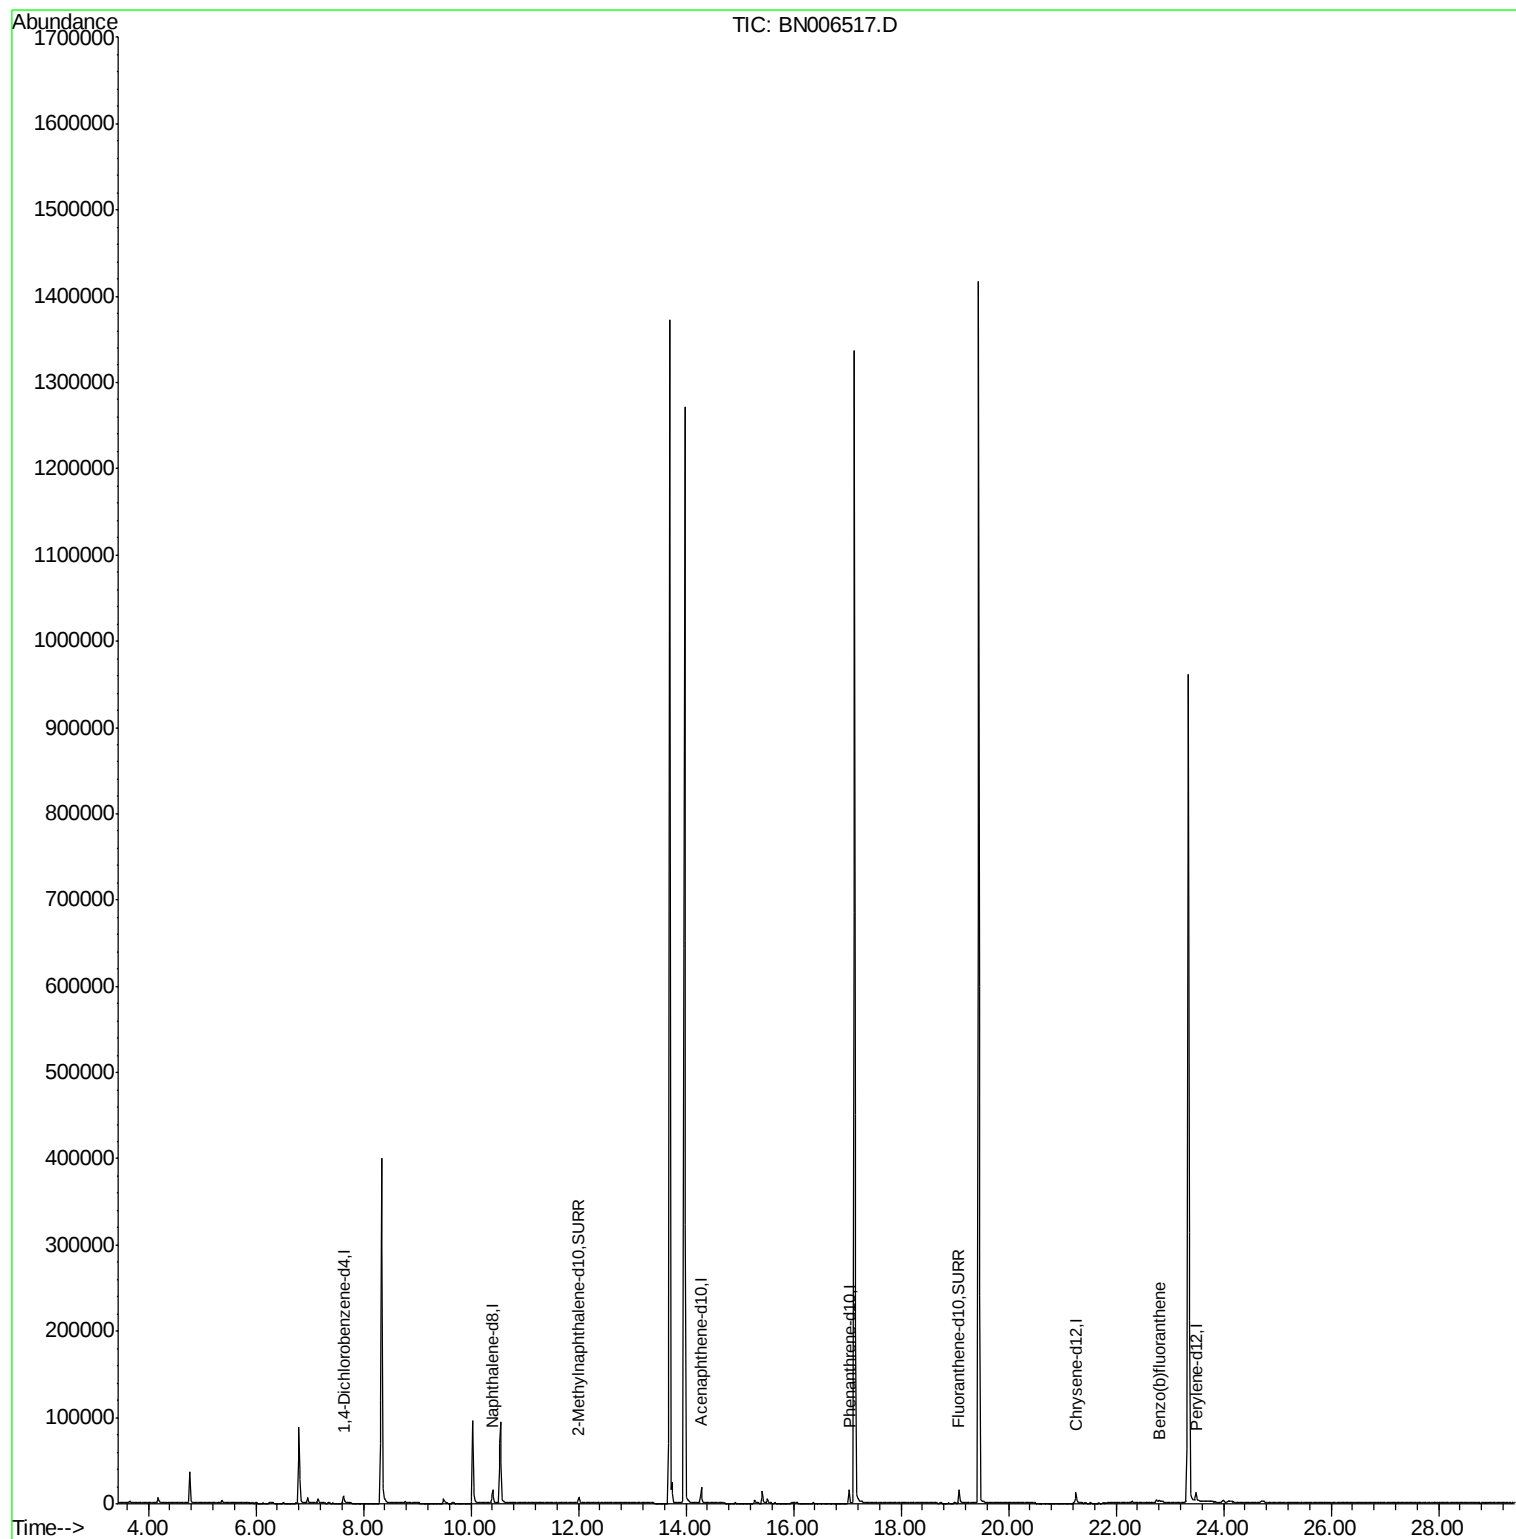

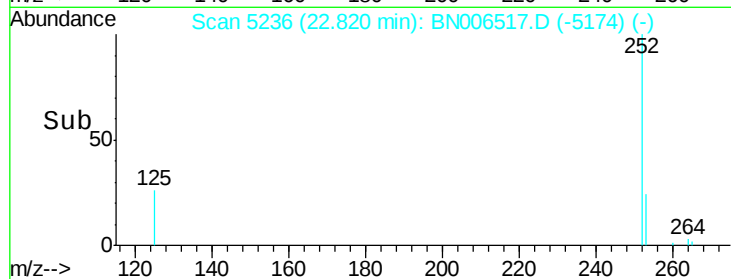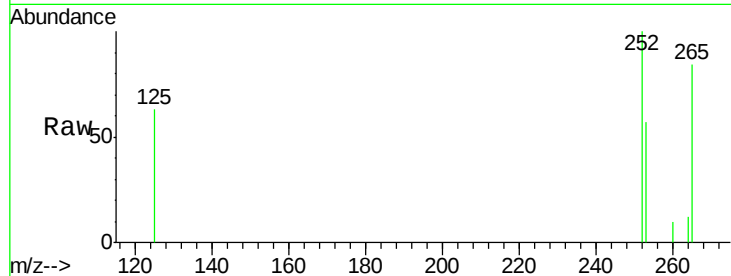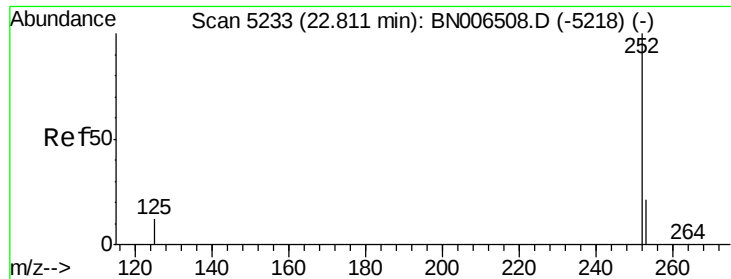

#21

Benzo(b)fluoranthene

Concen: 0.034 ng/ul m

RT: 22.82 min Scan# 5236

Delta R.T. -0.02 min

Lab File: BN006517.D

Acq: 23 Jun 2019 09:02

Instrument :

BNA_N

ClientSampleId :

A41X2

Tgt	Ion	Ratio	Lower	Upper
252	100			
253	56.7	0.0	51.4#	
125	62.7	0.0	41.0#	

Manual Integrations
APPROVED

mohammad
6/25/2019 8:45:37 AM

