


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062222\
 Data File : BN020335.D
 Acq On : 22 Jun 2022 09:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 22 15:57:15 2022

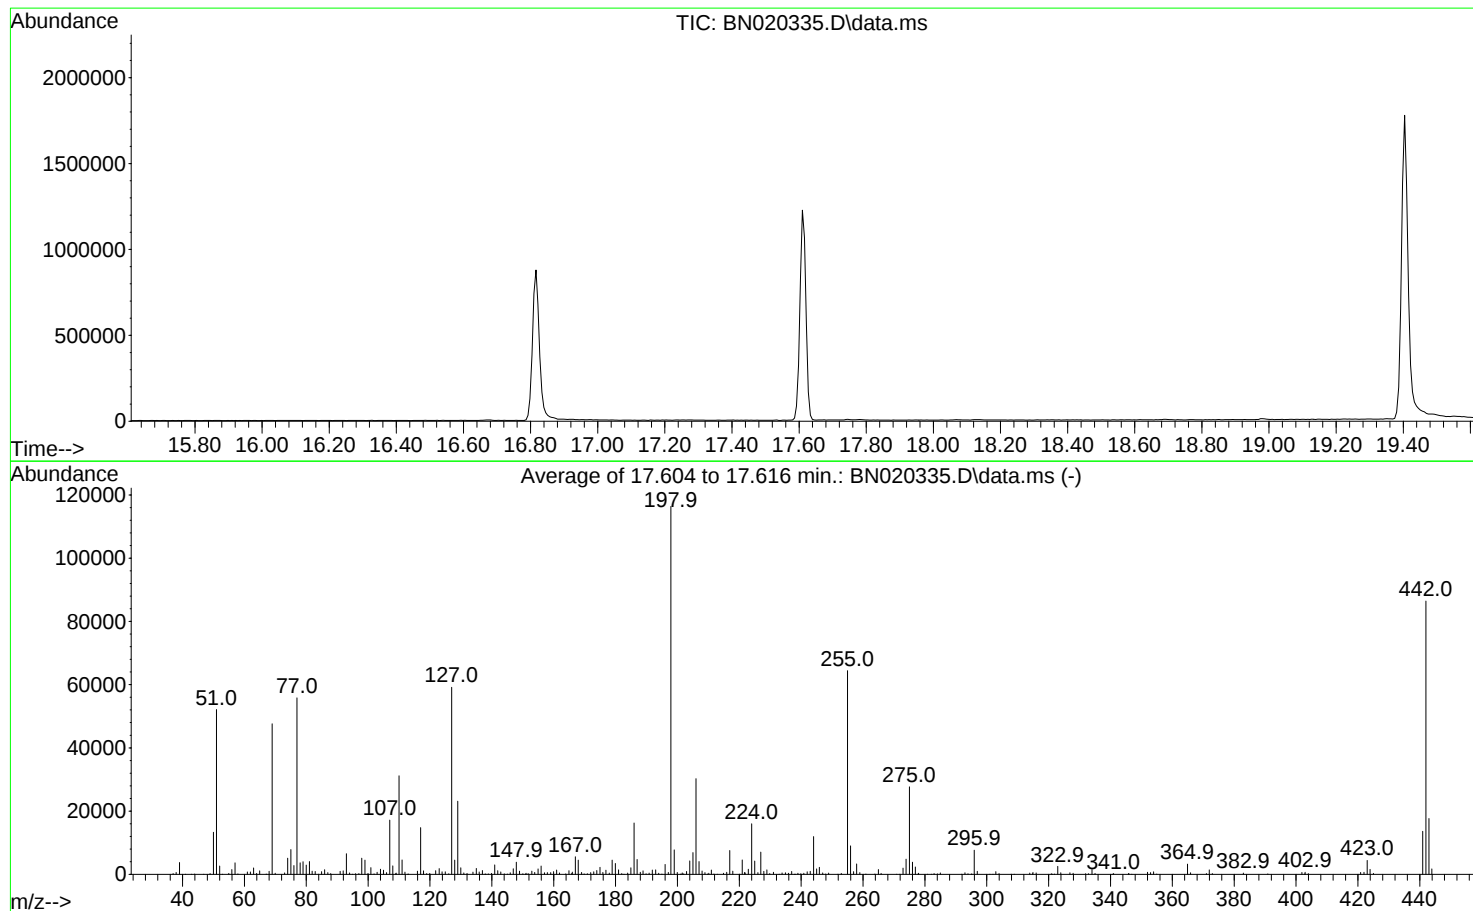




AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.8	52103	PASS
68	69	0.00	2	2.0	941	PASS
69	198	0.00	100	40.9	47616	PASS
70	69	0.00	2	0.7	332	PASS
127	198	10	80	50.9	59163	PASS
197	198	0.00	2	0.5	610	PASS
198	198	100	100	100.0	116341	PASS
199	198	5	9	6.7	7754	PASS
275	198	10	60	23.8	27677	PASS
365	198	1	100	2.8	3227	PASS
441	198	0.01	100	11.7	13613	PASS
442	442	50	100	100.0	86445	PASS
443	442	15	24	20.4	17645	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062222\
Data File : BN020335.D
Acq On : 22 Jun 2022 09:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 22 12:58:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 22 12:57:57 2022
Response via : Initial Calibration

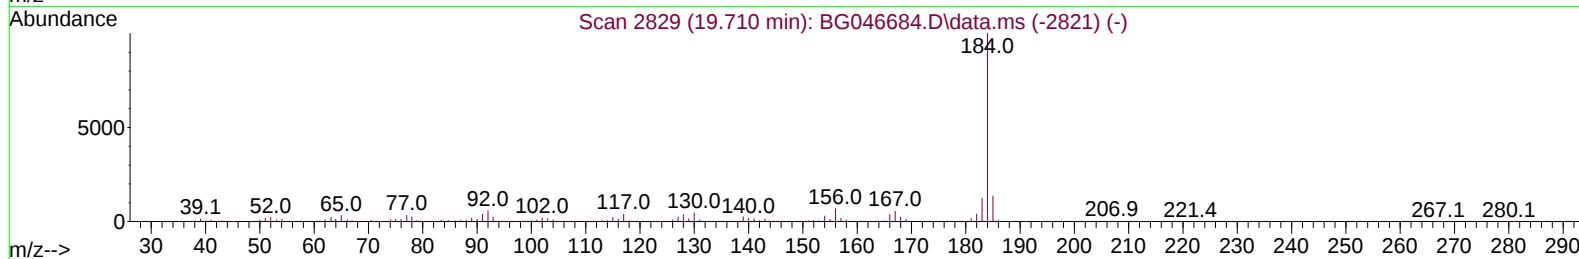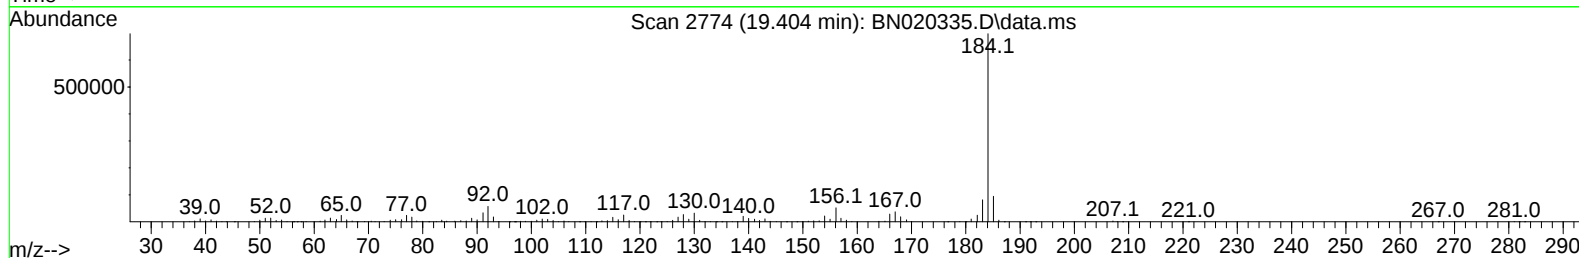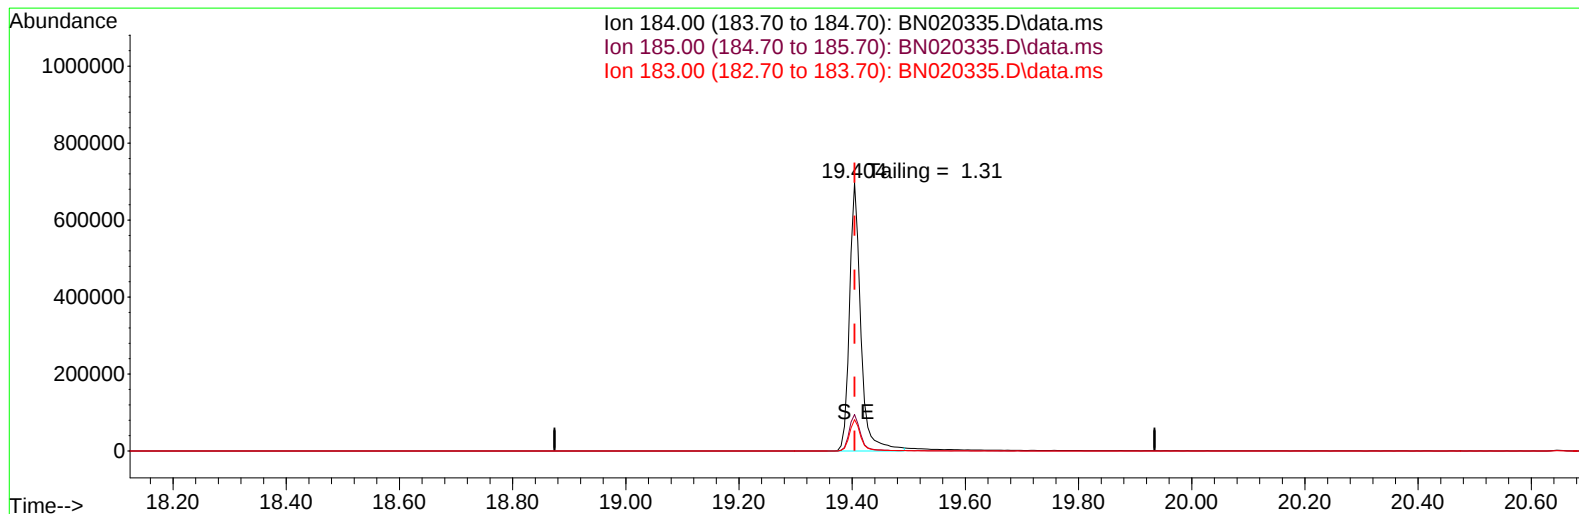

TIC: BN020335.D\data.ms

(77) Benzidine

19.404min (0.000) 0.00 ng

response 1007154

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.58
183.00	13.20	11.68
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/22/2022	BNA_N	<u>BN020335.D</u>
Compound Name	Response	Retention Time
DDT	492658	20.64
DDD	10589	20.21
DDE	778	19.69
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11367	504025	2.26

Instrument :
BNA_N
ClientSampleId :
DFTPP