

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062223\
 Data File : BN025929.D
 Acq On : 22 Jun 2023 10:11
 Operator : MA/JU
 Sample : PB153403BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK403

Quant Time: Jun 23 01:01:59 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 22 01:27:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.980	152	8633	0.400	ng/ul	0.00
4) Naphthalene-d8	10.792	136	26522	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.616	164	16634	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.364	188	35335	0.400	ng/ul	0.00
17) Chrysene-d12	21.552	240	24183	0.400	ng/ul	0.00
23) Perylene-d12	24.005	264	30206	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.335	96	59487	6.119	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.381	152	13360	0.328	ng/ul	0.00
18) Fluoranthene-d10	19.391	212	29509	0.321	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.606	166	5410	0.074	ng/ul#	13
20) Pyrene	19.754	202	4814	0.036	ng/ul#	1
26) Benzo(a)pyrene	23.847	252	10603	0.095	ng/ul#	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062223\
Data File : BN025929.D
Acq On : 22 Jun 2023 10:11
Operator : MA/JU
Sample : PB153403BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK403

Quant Time: Jun 23 01:01:59 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 22 01:27:41 2023
Response via : Initial Calibration




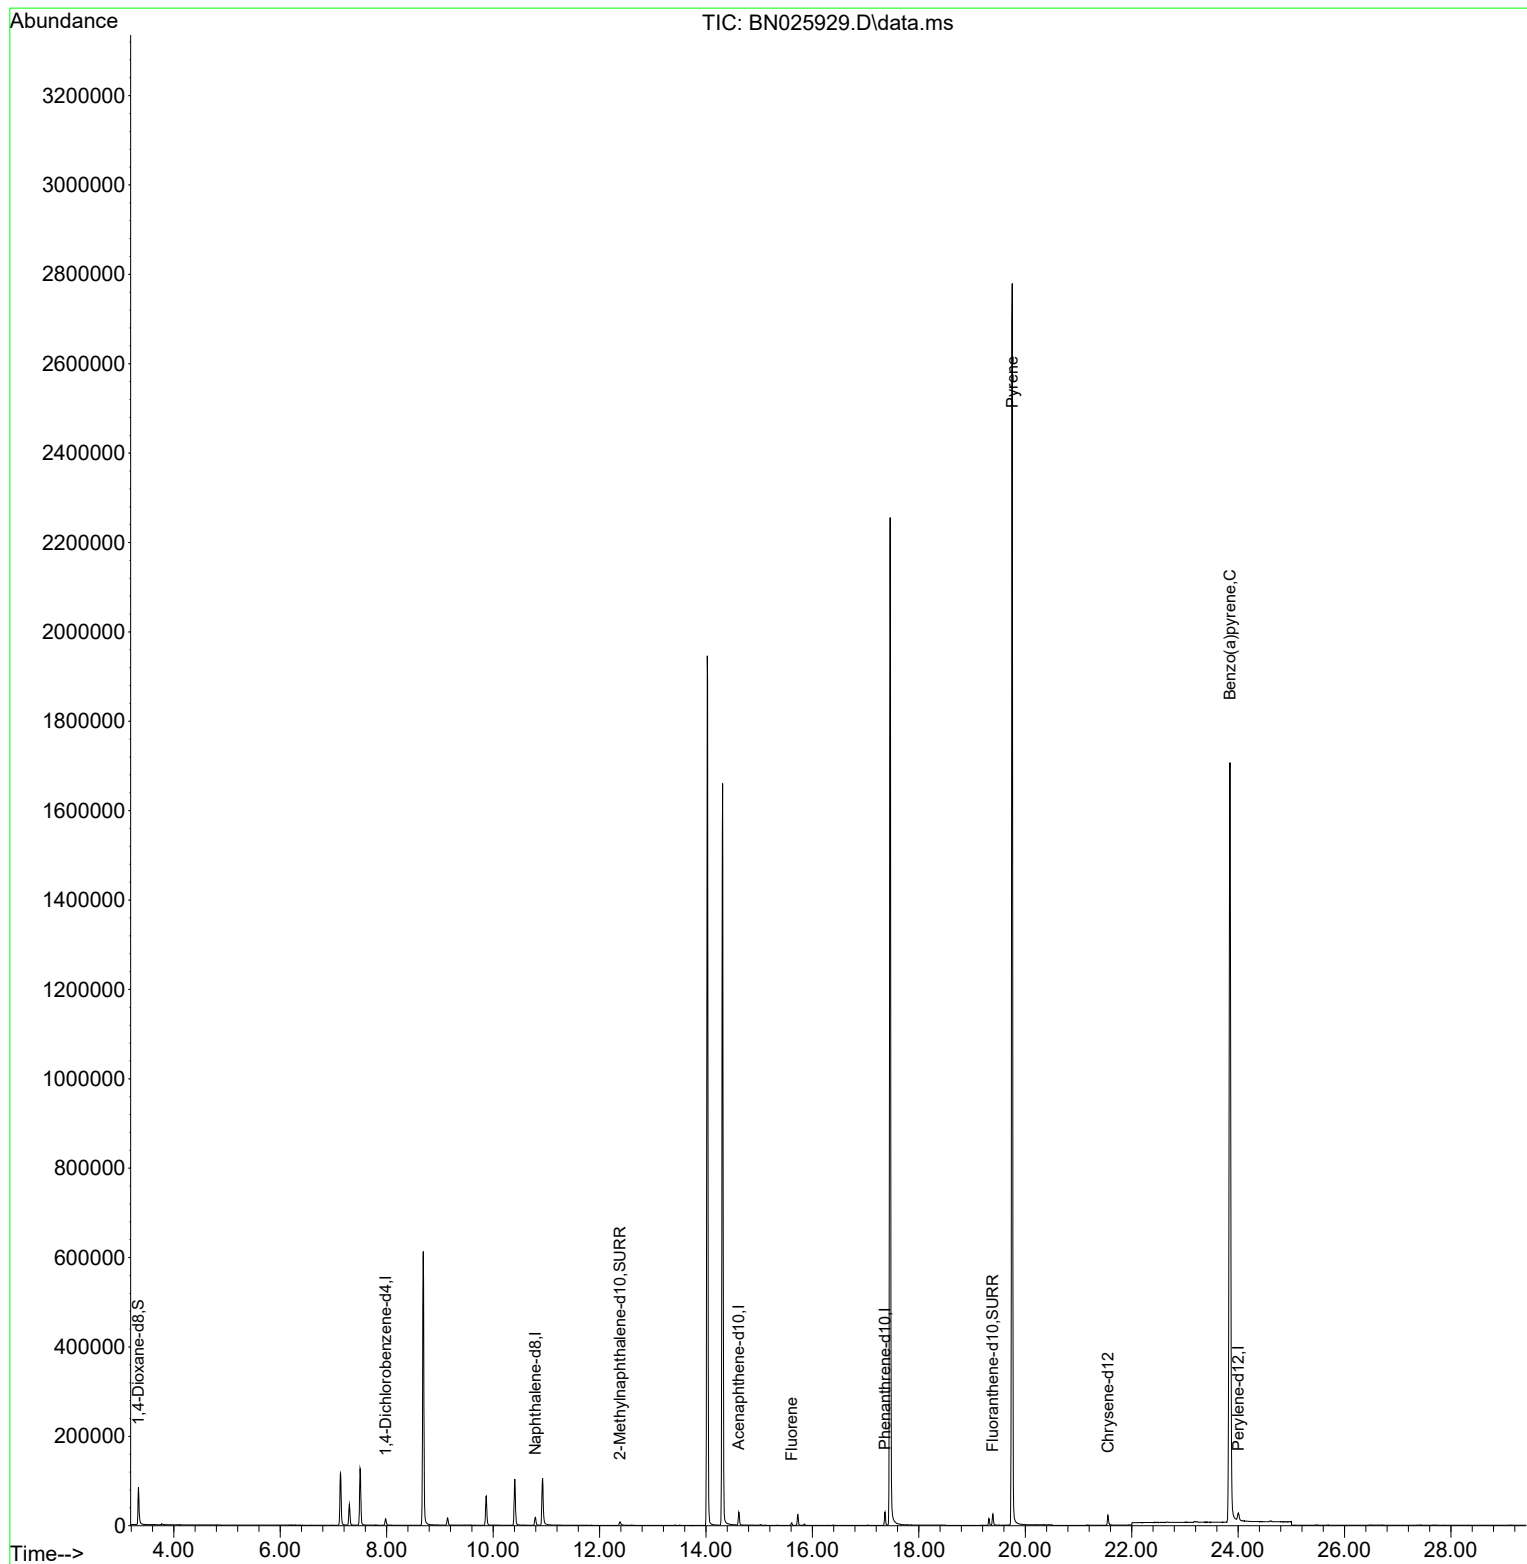


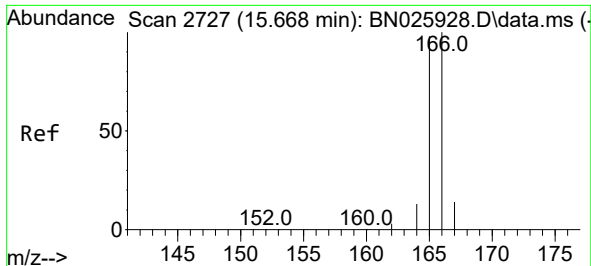

#12
Fluorene
Concen: 0.074 ng/ul
RT: 15.606 min Scan# 21
Delta R.T. -0.060 min
Lab File: BN025929.D
Acq: 22 Jun 2023 10:11




Instrument :
BNA_N
ClientSampleId :
SBLK403


Tgt Ion:166 Resp: 5410
Ion Ratio Lower Upper
166 100
165 6.5 79.9 119.9#
167 30.3 10.8 16.2#

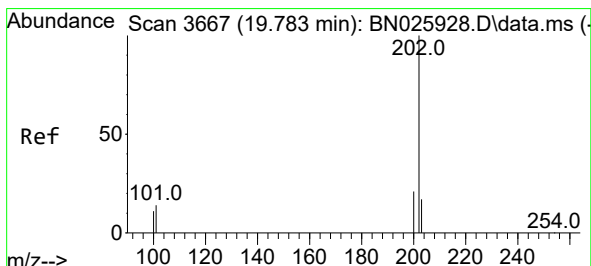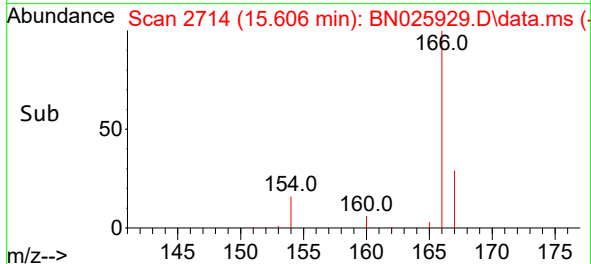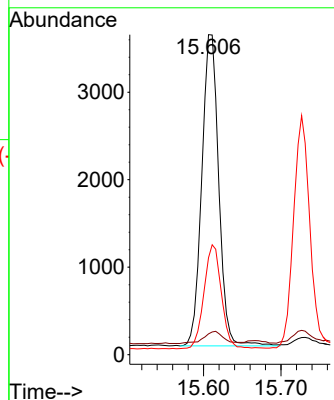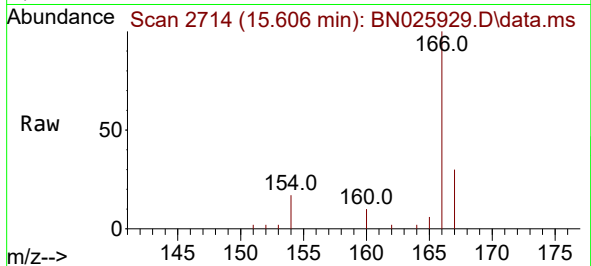

#20
Pyrene
Concen: 0.036 ng/ul
RT: 19.754 min Scan# 3661
Delta R.T. -0.028 min
Lab File: BN025929.D
Acq: 22 Jun 2023 10:11


Tgt Ion:202 Resp: 4814
Ion Ratio Lower Upper
202 100
101 178.8 11.4 17.0#
100 1341.9 9.1 13.7#

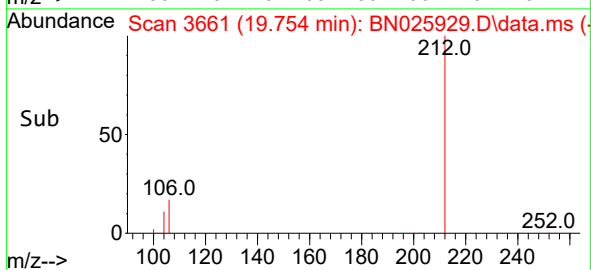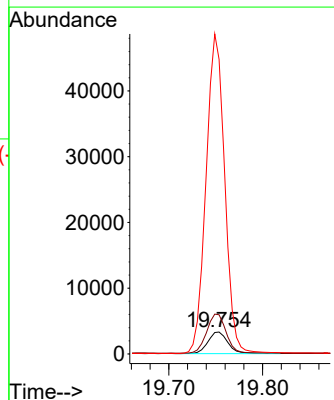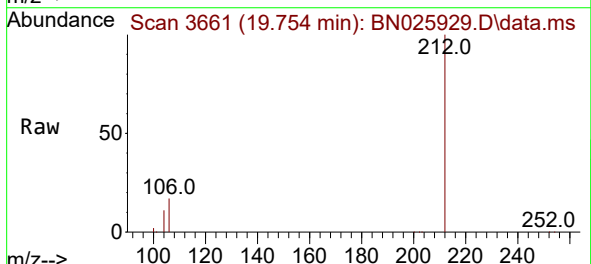

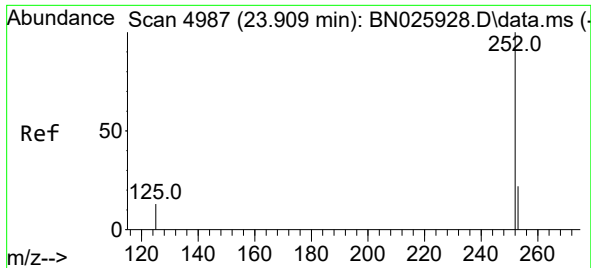

#26
 Benzo(a)pyrene
 Concen: 0.095 ng/ul
 RT: 23.847 min Scan# 4966
 Delta R.T. -0.062 min
 Lab File: BN025929.D
 Acq: 22 Jun 2023 10:11

Instrument :
 BNA_N
 ClientSampleId :
 SBLK403

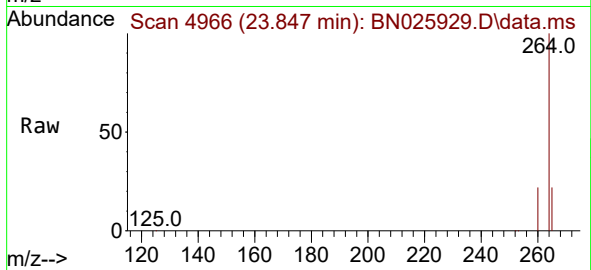

Tgt Ion:252 Resp: 10603
 Ion Ratio Lower Upper
 252 100
 253 50.6 26.0 39.0#
 125 44.7 17.3 25.9#

