

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062223\
 Data File : BN025945.D
 Acq On : 22 Jun 2023 19:47
 Operator : MA/JU
 Sample : PB153403BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK403

Quant Time: Jun 23 01:04:40 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 22 01:27:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.980	152	7996	0.400	ng/ul	0.00
4) Naphthalene-d8	10.792	136	25561	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.616	164	16079	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.364	188	33466	0.400	ng/ul	0.00
17) Chrysene-d12	21.552	240	19323	0.400	ng/ul	0.00
23) Perylene-d12	24.019	264	18510	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.331	96	50001	5.553	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.381	152	13058	0.332	ng/ul	0.00
18) Fluoranthene-d10	19.391	212	28256	0.384	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.611	166	4837	0.068	ng/ul#	13
20) Pyrene	19.754	202	4206	0.039	ng/ul#	1
26) Benzo(a)pyrene	23.867	252	6058	0.088	ng/ul#	41


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062223\
Data File : BN025945.D
Acq On : 22 Jun 2023 19:47
Operator : MA/JU
Sample : PB153403BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK403

Quant Time: Jun 23 01:04:40 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 22 01:27:41 2023
Response via : Initial Calibration




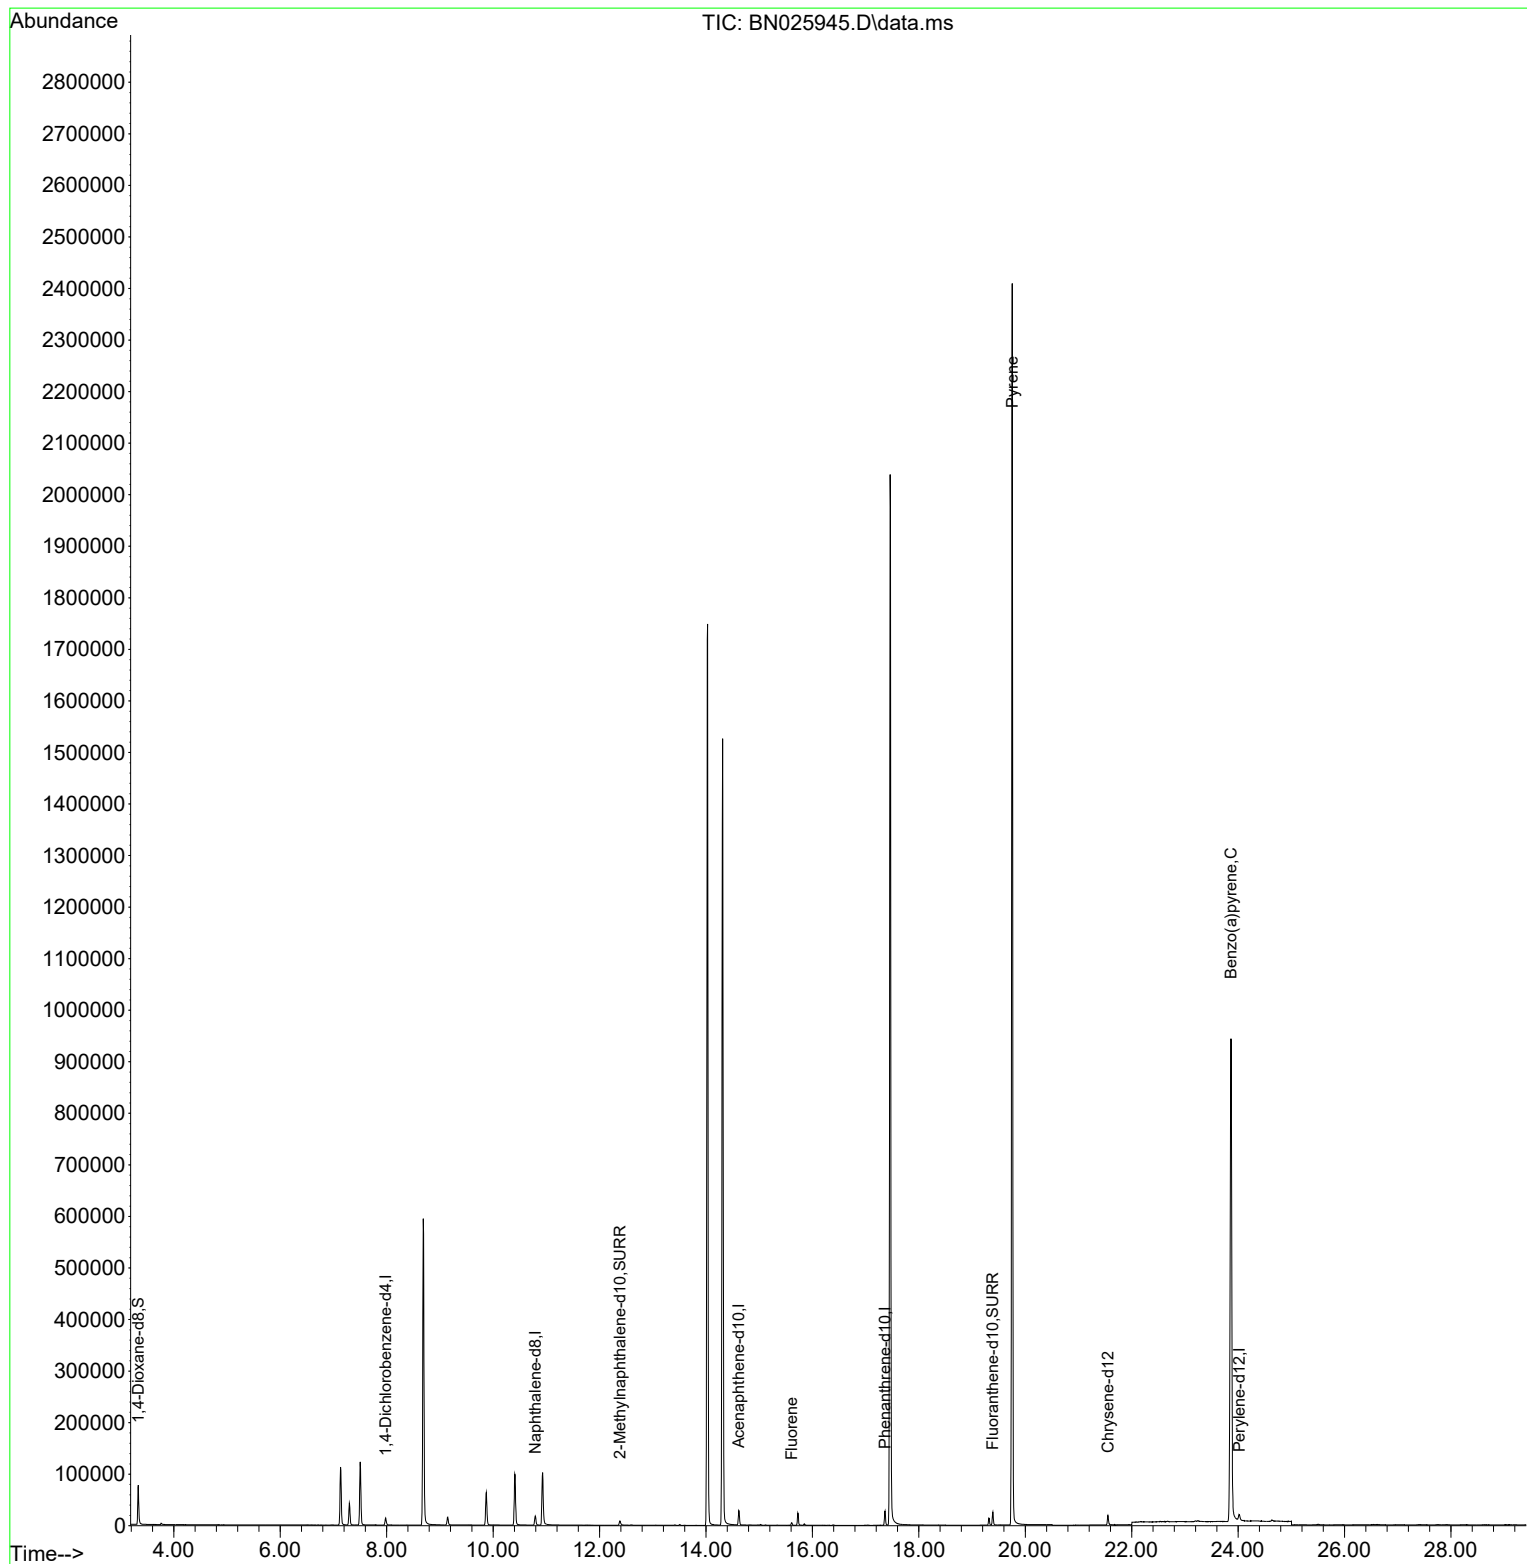


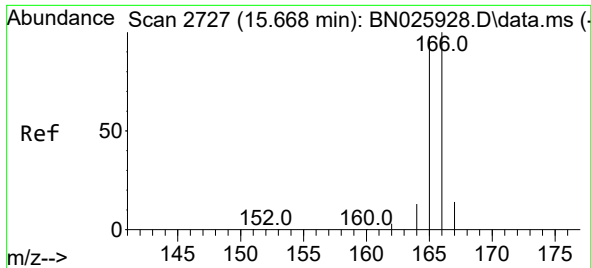

#12
Fluorene
Concen: 0.068 ng/ul
RT: 15.611 min Scan# 21
Delta R.T. -0.056 min
Lab File: BN025945.D
Acq: 22 Jun 2023 19:47




Instrument :
BNA_N
ClientSampleId :
SBLK403


Tgt Ion:166 Resp: 4837
Ion Ratio Lower Upper
166 100
165 7.6 79.9 119.9#
167 33.3 10.8 16.2#

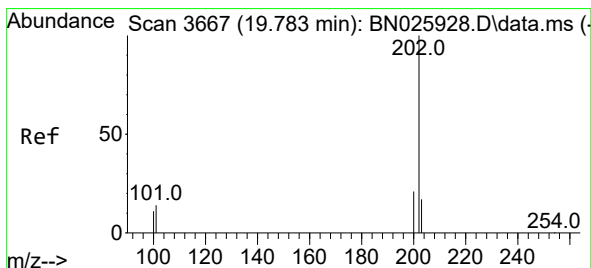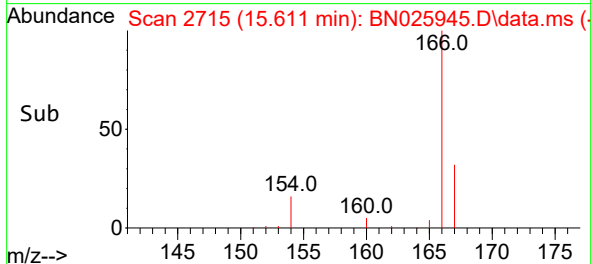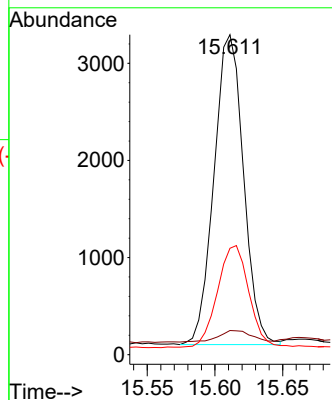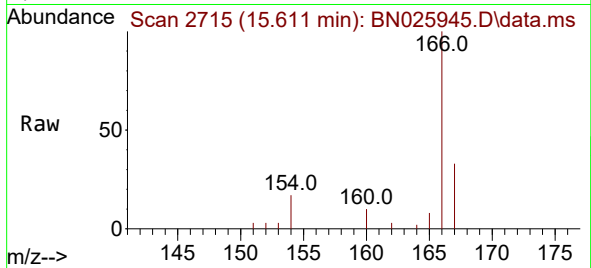

#20
Pyrene
Concen: 0.039 ng/ul
RT: 19.754 min Scan# 3661
Delta R.T. -0.028 min
Lab File: BN025945.D
Acq: 22 Jun 2023 19:47


Tgt Ion:202 Resp: 4206
Ion Ratio Lower Upper
202 100
101 171.4 11.4 17.0#
100 1306.1 9.1 13.7#

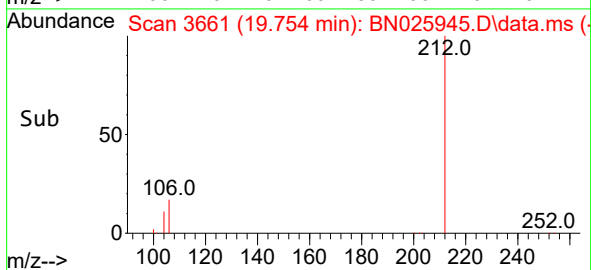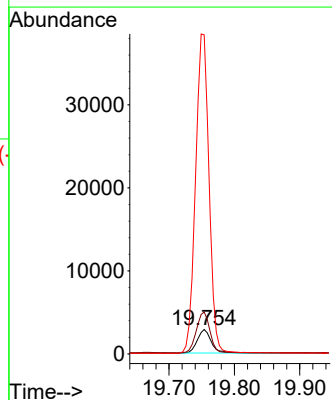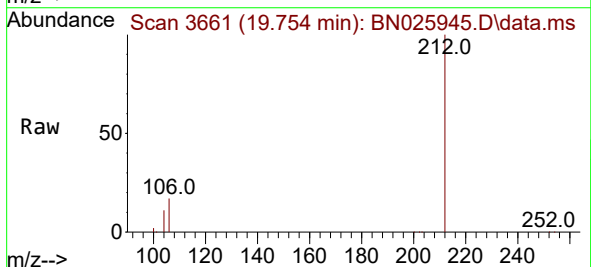

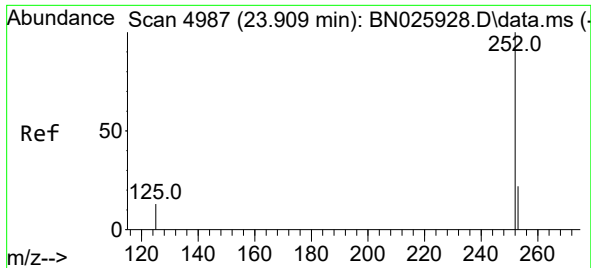

#26
Benzo(a)pyrene
Concen: 0.088 ng/ul
RT: 23.867 min Scan# 4973
Delta R.T. -0.041 min
Lab File: BN025945.D
Acq: 22 Jun 2023 19:47

Instrument :
BNA_N
ClientSampleId :
SBLK403

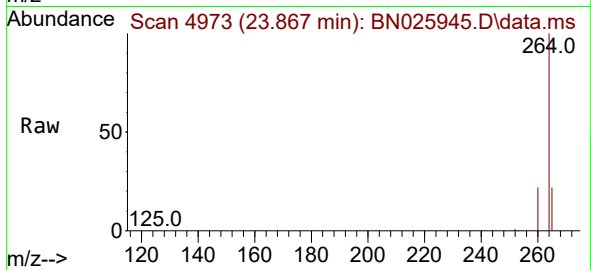

Tgt Ion:252 Resp: 6058
Ion Ratio Lower Upper
252 100
253 60.5 26.0 39.0#
125 56.3 17.3 25.9#

