
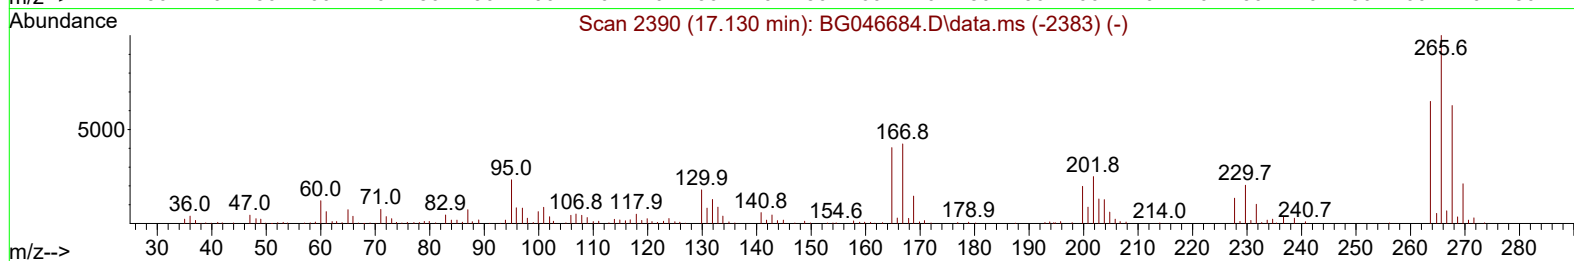
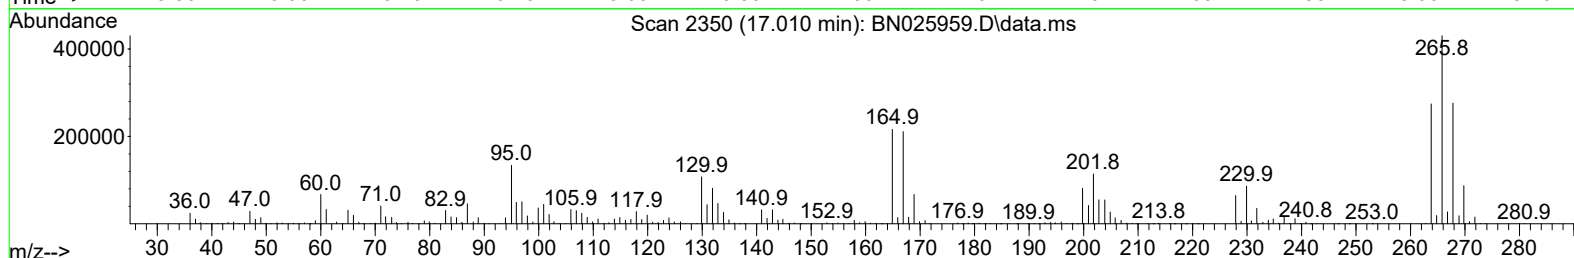


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062323\
 Data File : BN025959.D
 Acq On : 23 Jun 2023 09:05
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 07:09:38 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jun 24 07:09:34 2023
 Response via : Initial Calibration

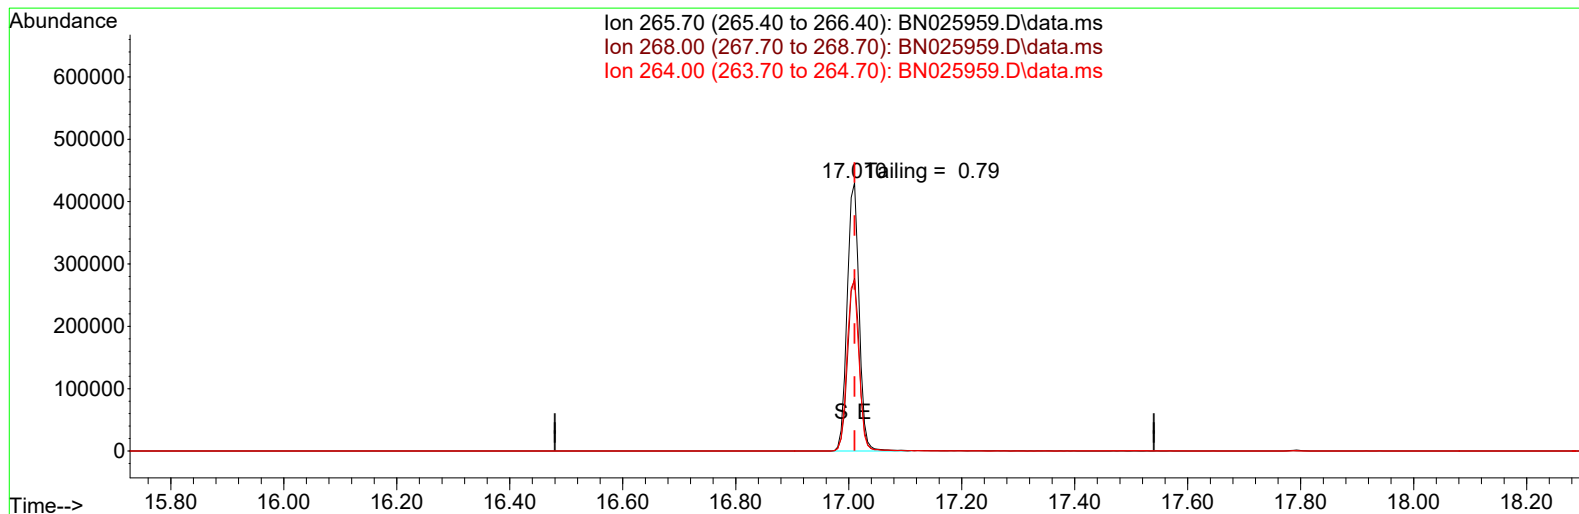

TIC: BN025959.D\data.ms

(70) Pentachlorophenol (C)




17.010min (0.000) 23744.44 ng

response 633371

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.20
264.00	61.60	63.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062323\
Data File : BN025959.D
Acq On : 23 Jun 2023 09:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 07:09:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 24 07:09:34 2023
Response via : Initial Calibration

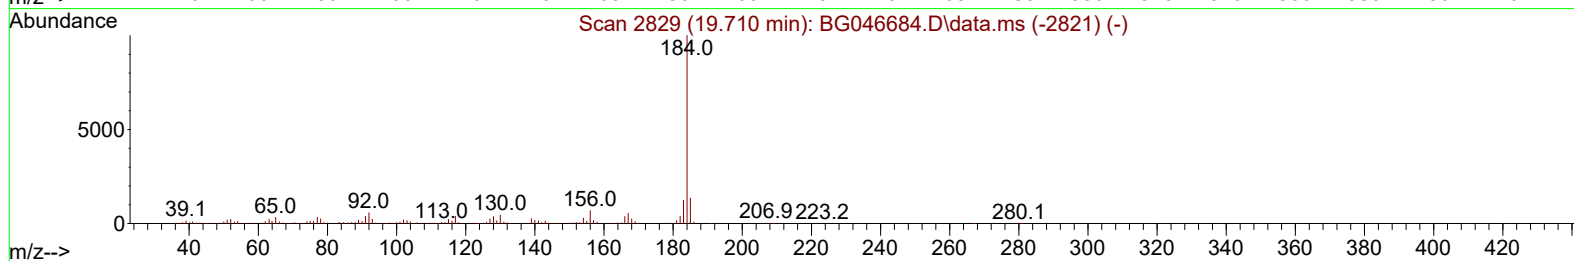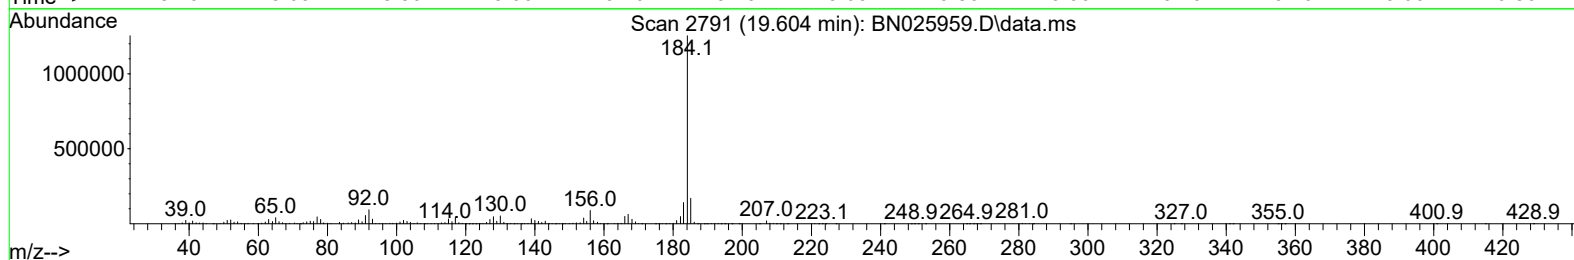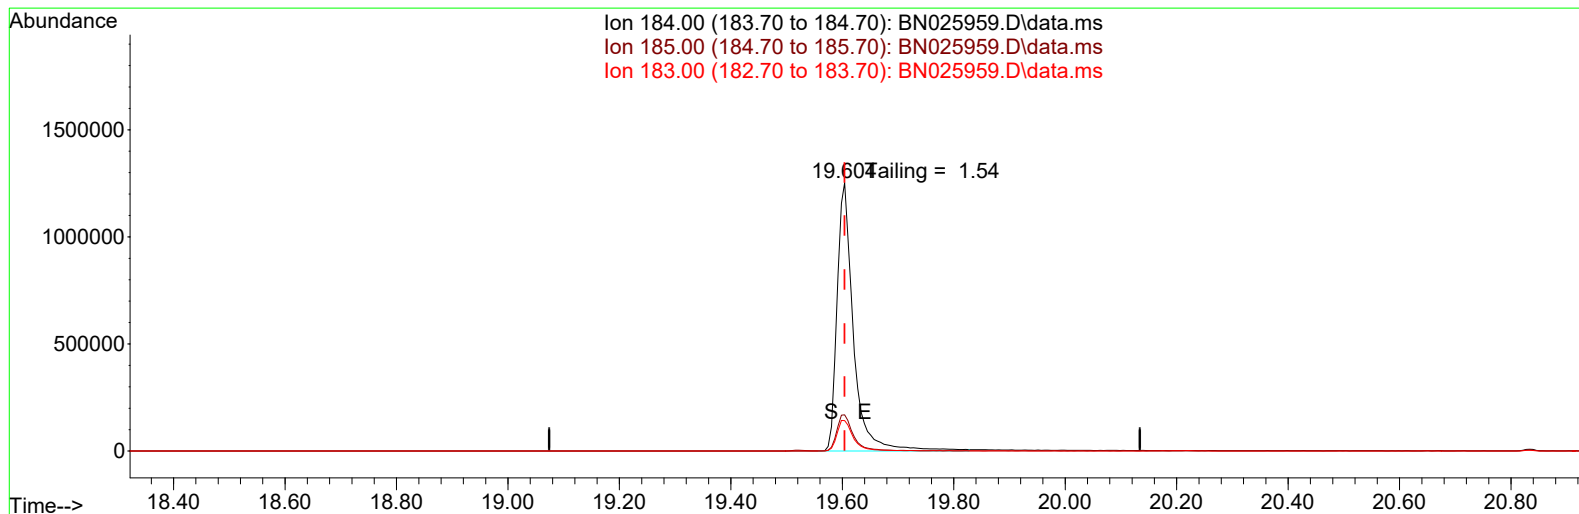

TIC: BN025959.D\data.ms

(77) Benzidine**19.604min (0.000) 1316165.19 ng****response 2596562**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.52
183.00	13.20	11.34
0.00	0.00	0.00