


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062323\
Data File : BN025959.D
Acq On : 23 Jun 2023 09:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN053123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 23 17:48:31 2023

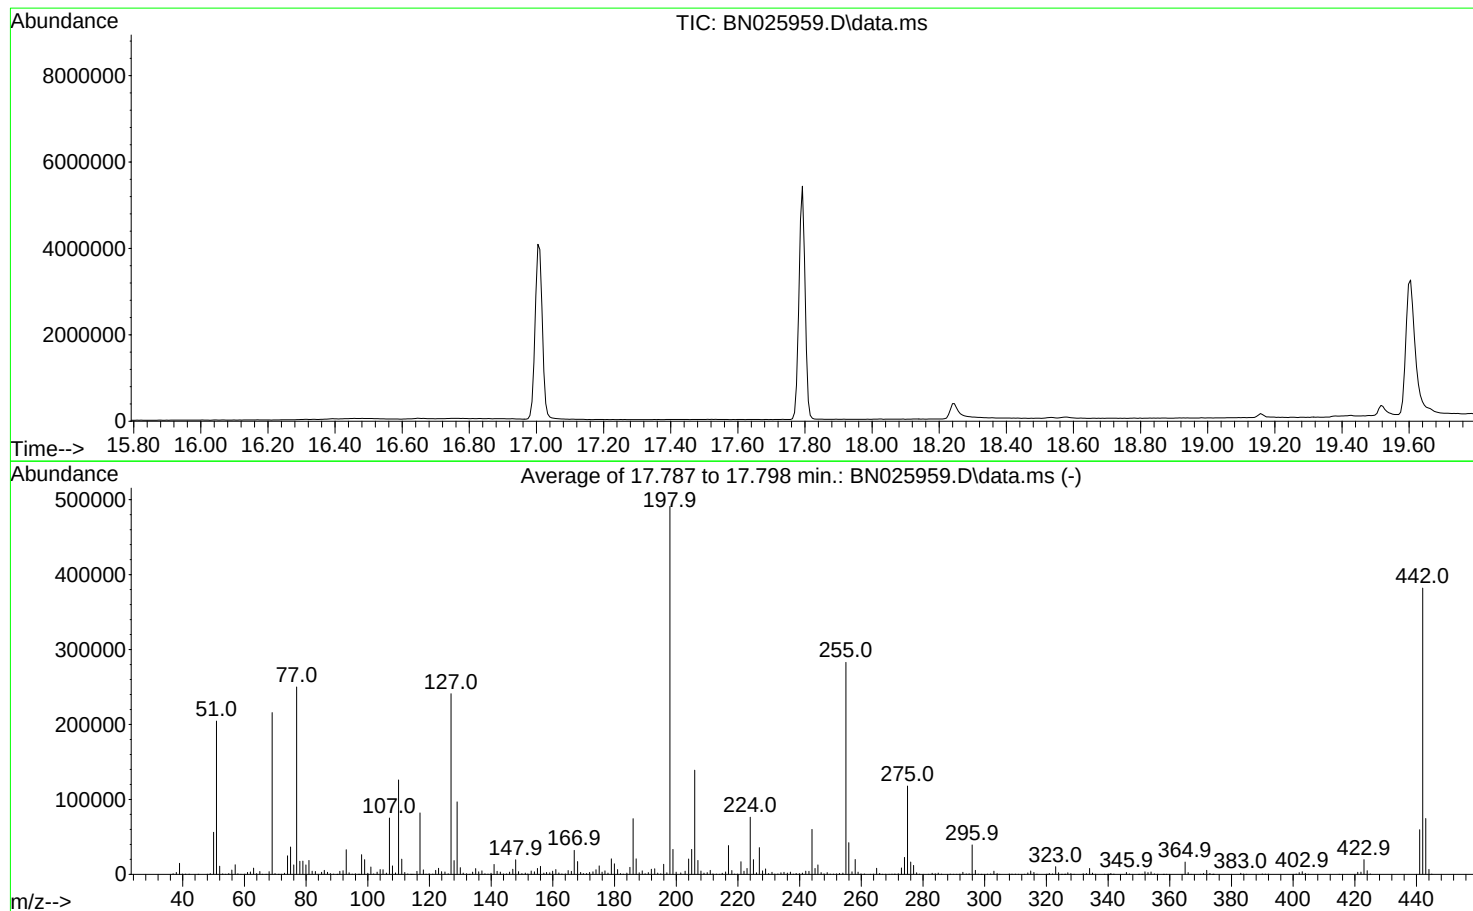

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	41.7	204628	PASS
68	69	0.00	2	1.7	3647	PASS
69	198	0.00	100	44.0	215981	PASS
70	69	0.00	2	0.5	1149	PASS
127	198	10	80	49.1	241152	PASS
197	198	0.00	2	0.4	2054	PASS
198	198	100	100	100.0	490901	PASS
199	198	5	9	6.8	33264	PASS
275	198	10	60	24.0	117824	PASS
365	198	1	100	3.4	16529	PASS
441	198	0.01	100	12.1	59547	PASS
442	442	50	100	100.0	382016	PASS
443	442	15	24	19.5	74624	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/23/2023	BNA_N	<u>BN025959.D</u>
Compound Name	Response	Retention Time
DDT	1837750	20.833
DDD	37132	20.392
DDE	1333	19.881
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
38465	1876215	2.05

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062323\
 Data File : BN025959.D
 Acq On : 23 Jun 2023 09:05
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jun 24 07:09:38 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jun 24 07:09:34 2023
 Response via : Initial Calibration

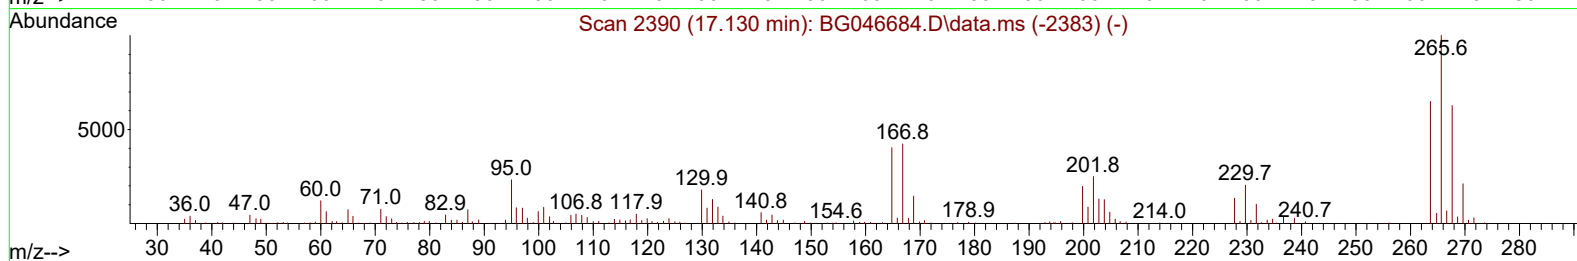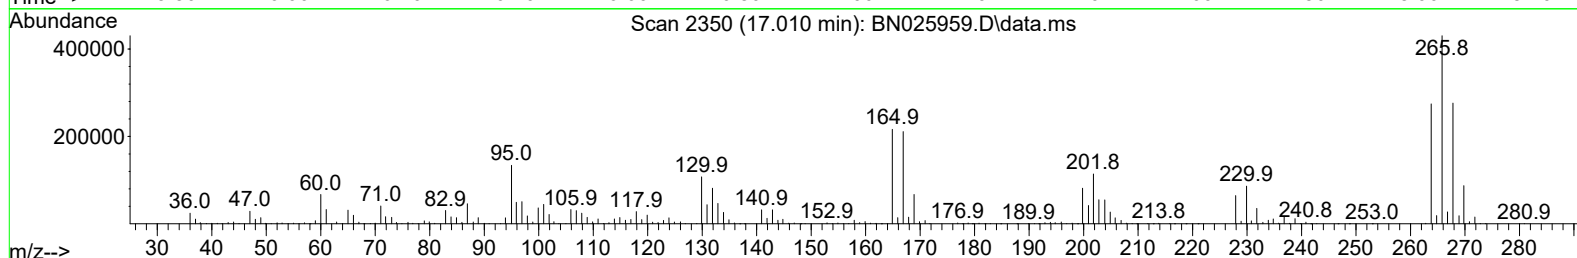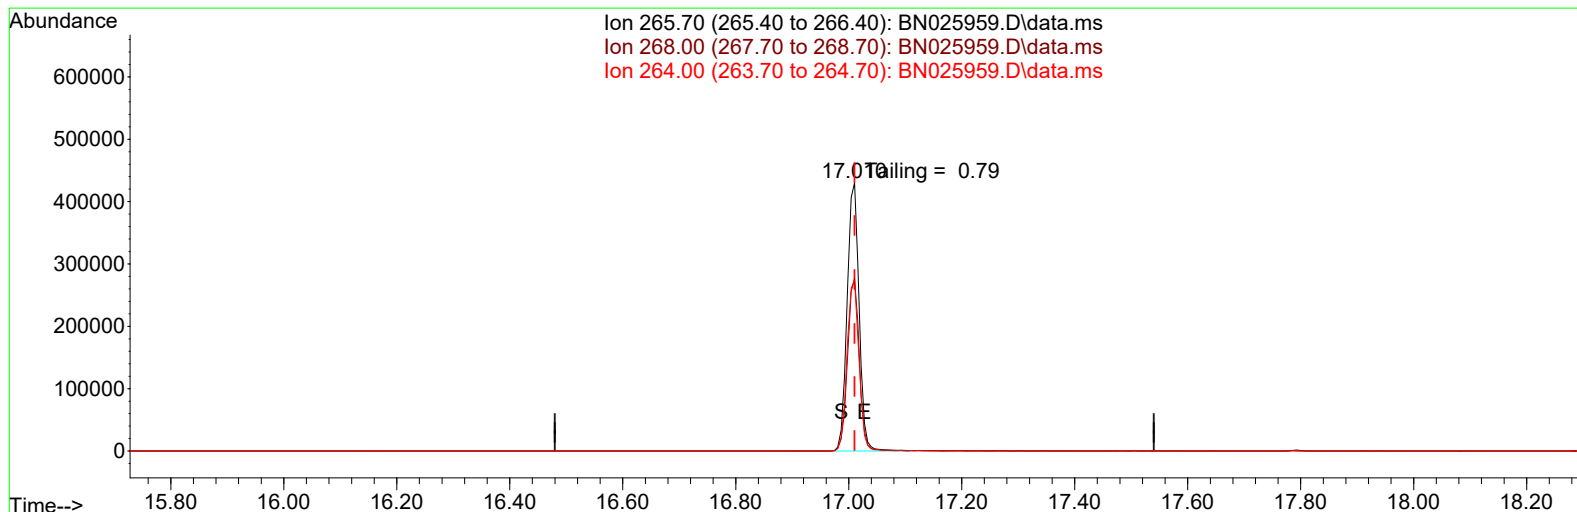

TIC: BN025959.D\data.ms

(70) Pentachlorophenol (C)

17.010min (0.000) 23744.44 ng




response 633371

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.20
264.00	61.60	63.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062323\
Data File : BN025959.D
Acq On : 23 Jun 2023 09:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 24 07:09:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 24 07:09:34 2023
Response via : Initial Calibration

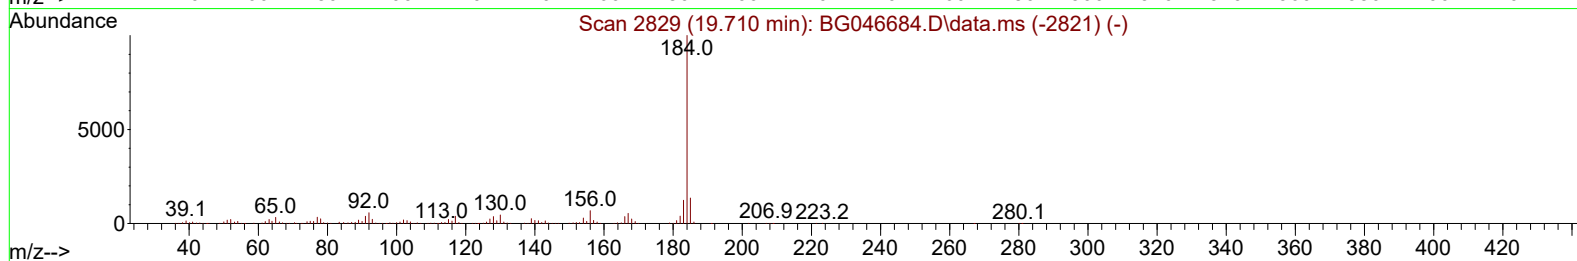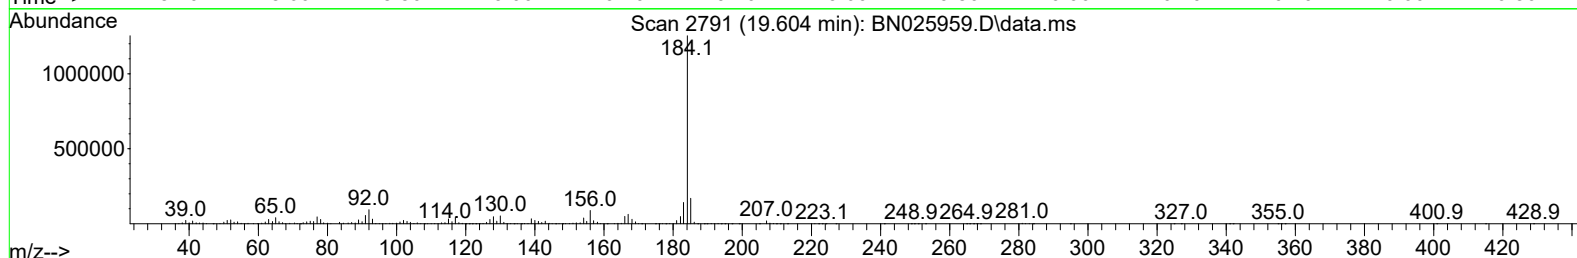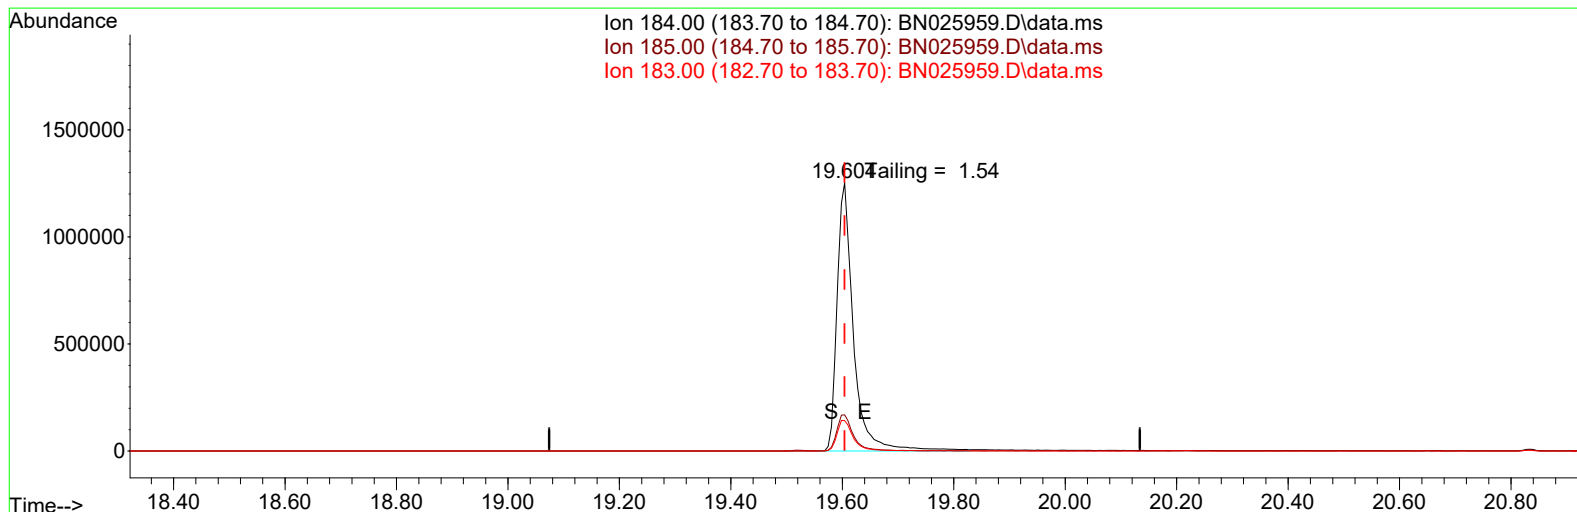

TIC: BN025959.D\data.ms

(77) Benzidine

19.604min (0.000) 1316165.19 ng

response 2596562

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.52
183.00	13.20	11.34
0.00	0.00	0.00