




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006541.D
Acq On : 24 Jun 2019 21:04
Operator : HP/JU
Sample : K3362-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41Z5

Manual Integrations
APPROVED

mohammad
6/25/2019 10:20:27 PM

Quant Time: Jun 25 00:44:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

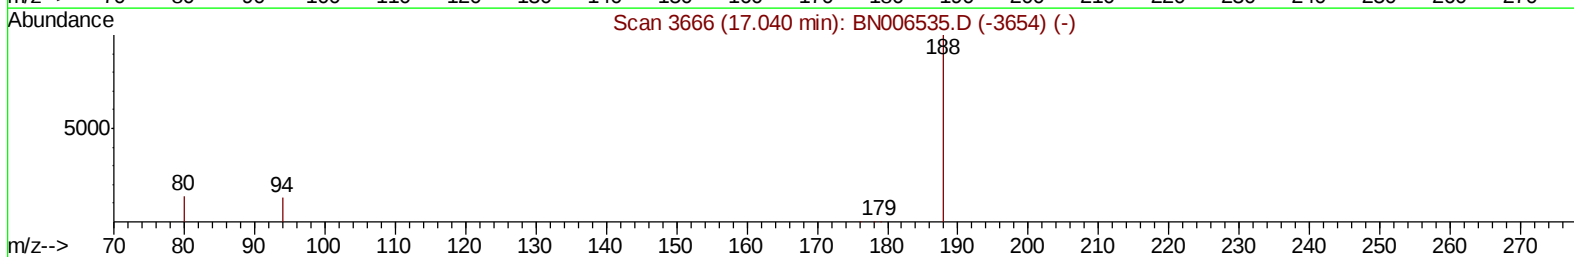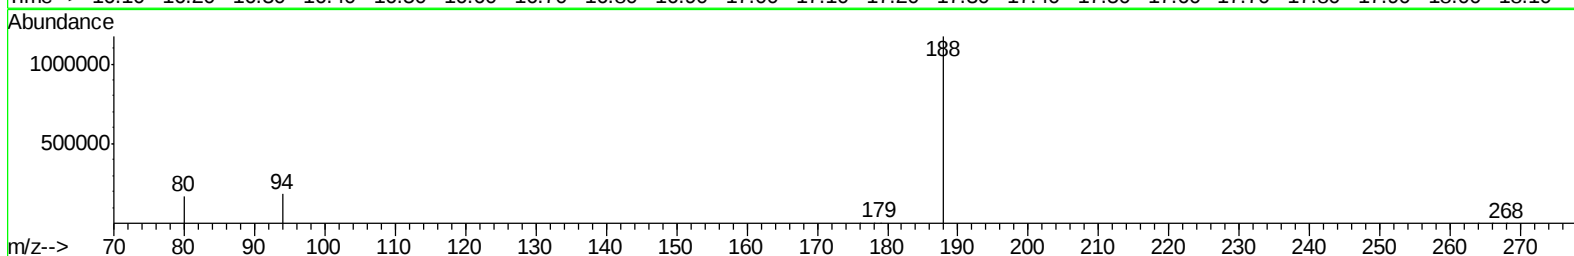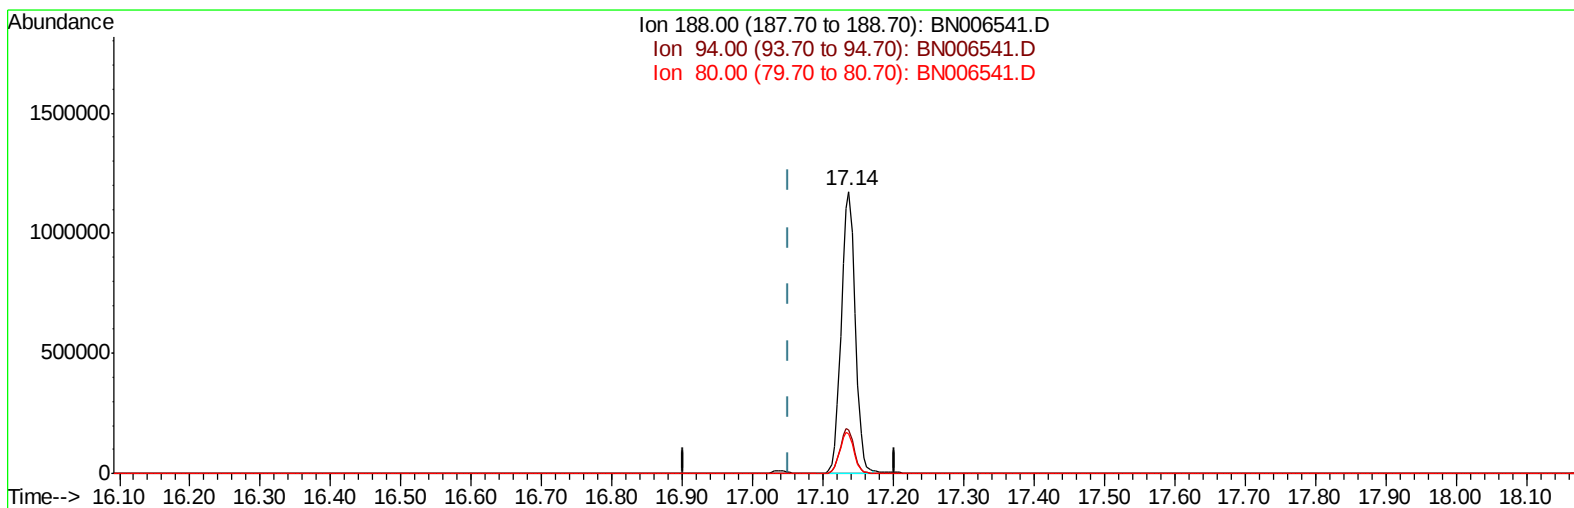

TIC: BN006541.D

(10) Phenanthrene-d10 (I)

17.137min (+0.085) 0.40ng/ul

response 1644594

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	15.58
80.00	13.60	14.18
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006541.D
Acq On : 24 Jun 2019 21:04
Operator : HP/JU
Sample : K3362-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41Z5

Manual Integrations
APPROVED

mohammad
6/25/2019 10:20:27 PM

Quant Time: Jun 25 00:44:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

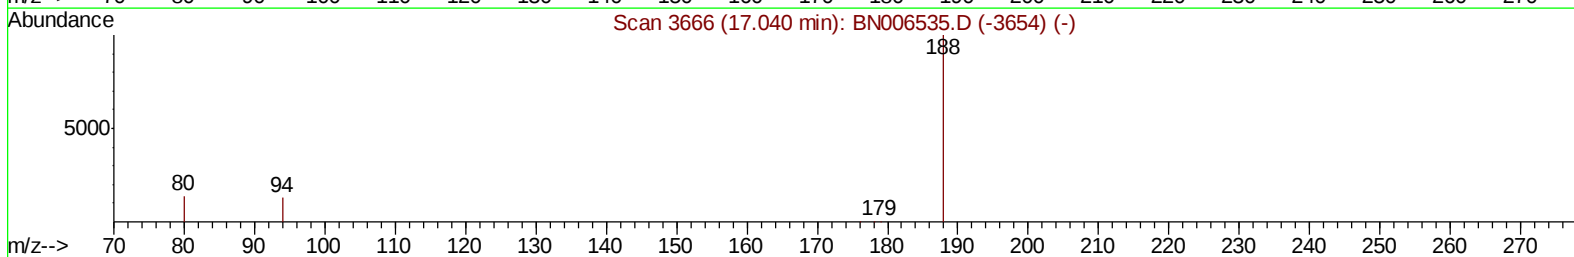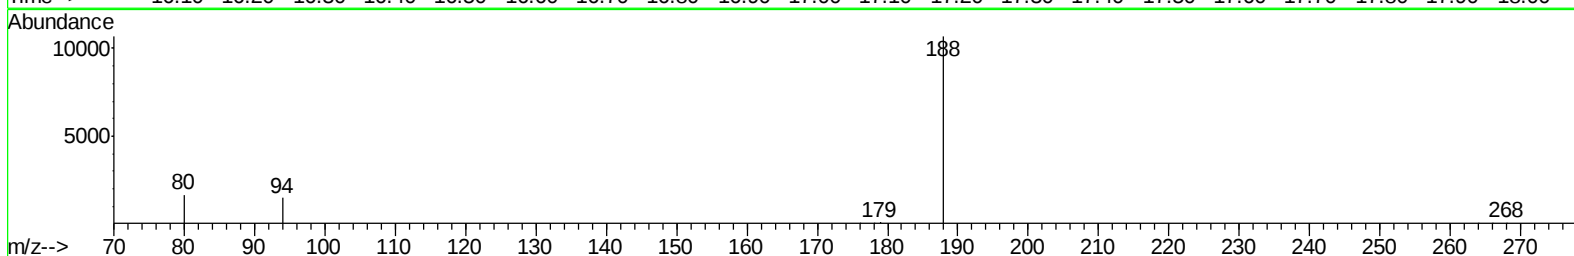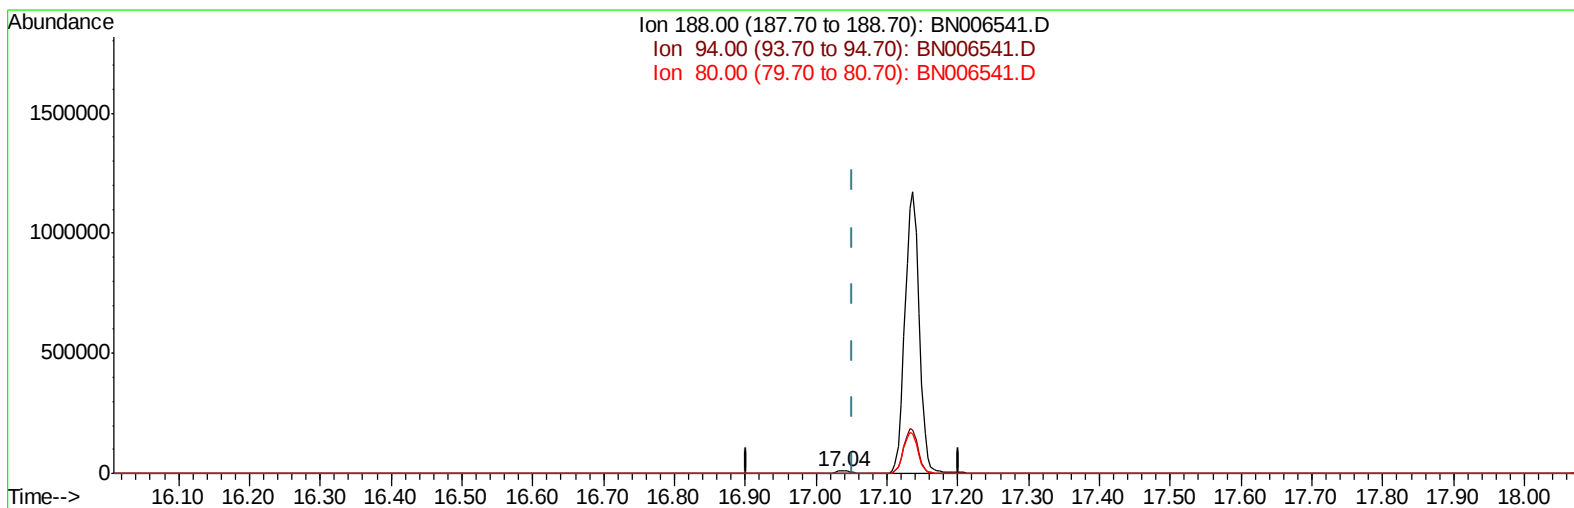

TIC: BN006541.D

(10) Phenanthrene-d10 (I)

17.036min (-0.017) 0.40ng/ul m

response 15440

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	13.92
80.00	13.60	15.46
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006541.D
Acq On : 24 Jun 2019 21:04
Operator : HP/JU
Sample : K3362-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41Z5

Manual Integrations
APPROVED

mohammad
6/25/2019 10:20:27 PM

Quant Time: Jun 25 03:22:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

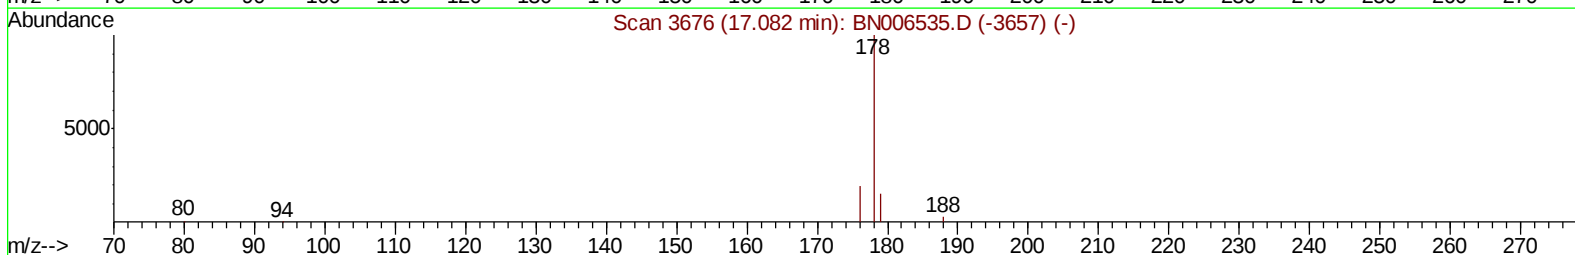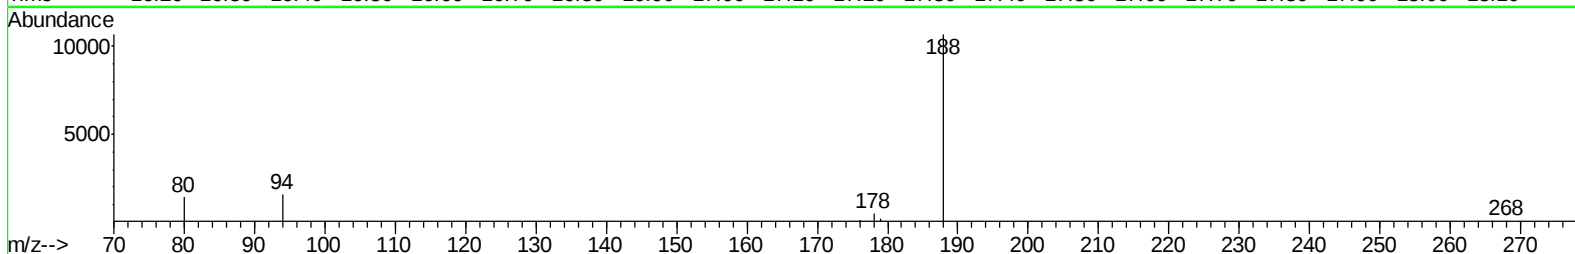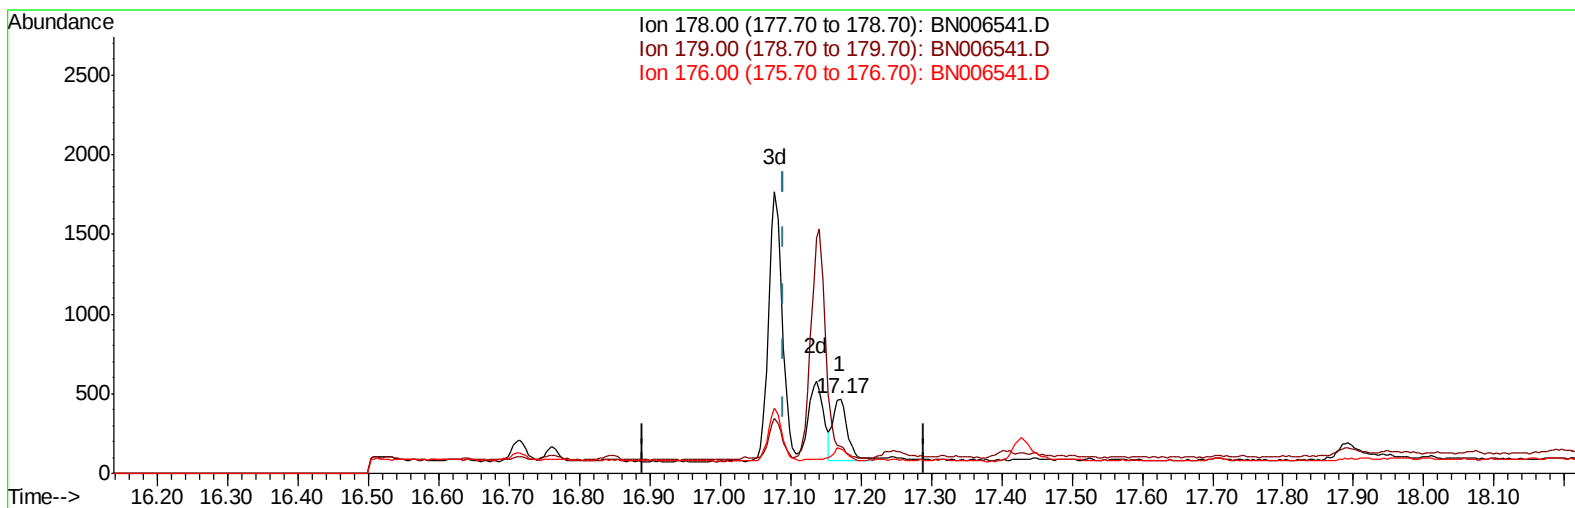

TIC: BN006541.D

(12) Phenanthrene

17.171min (+0.080) 0.01ng/ul

response 565

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	35.47#
176.00	19.10	32.69#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006541.D
Acq On : 24 Jun 2019 21:04
Operator : HP/JU
Sample : K3362-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41Z5

Manual Integrations
APPROVED

mohammad
6/25/2019 10:20:27 PM

Quant Time: Jun 25 03:22:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

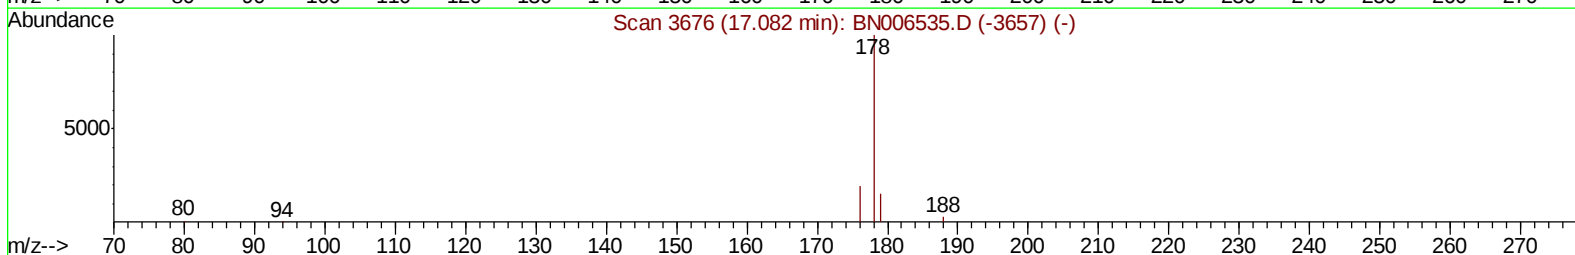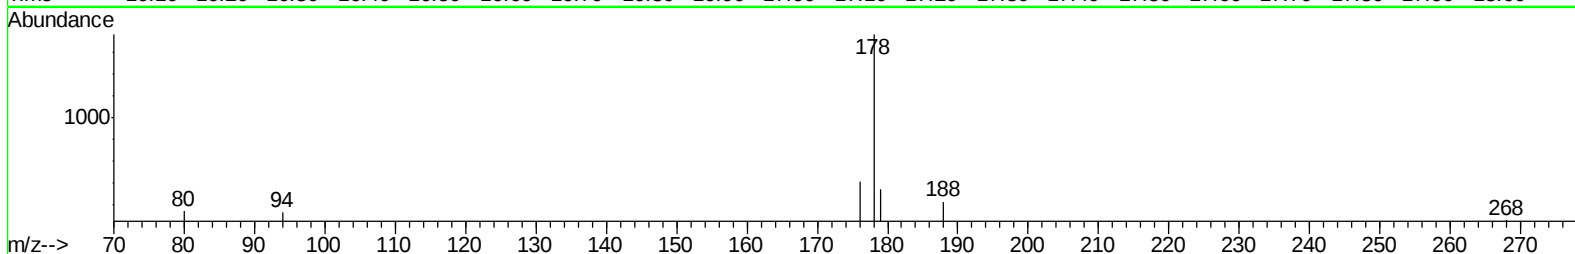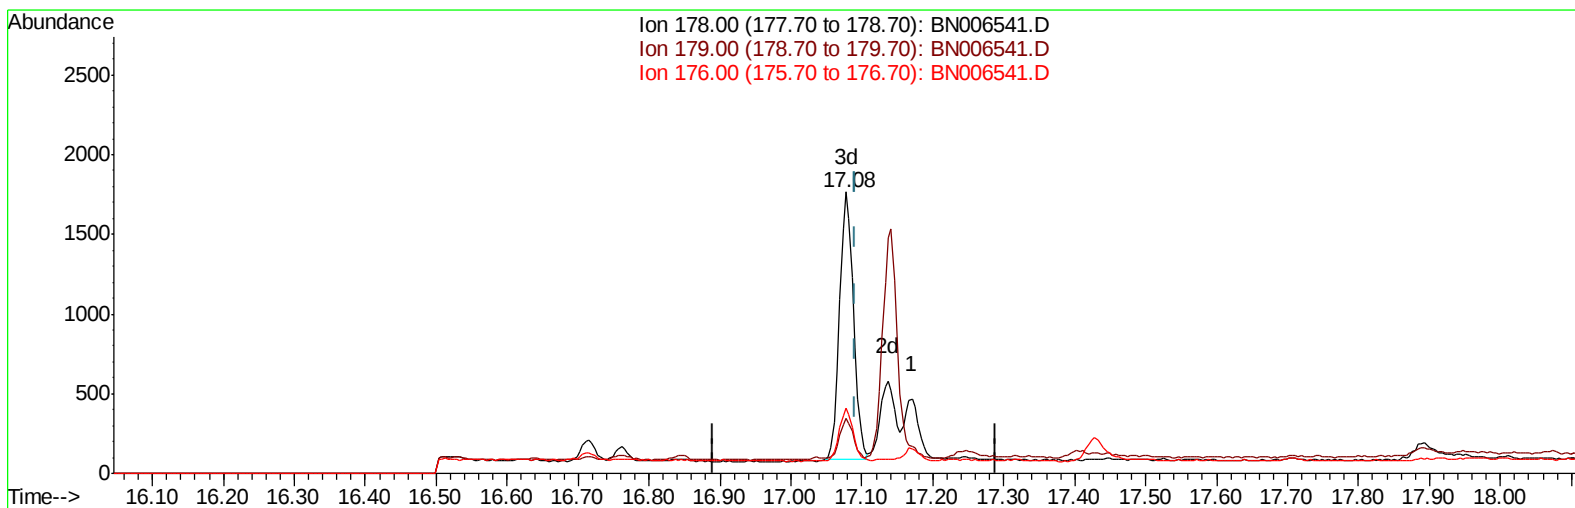

TIC: BN006541.D

(12) Phenanthrene

17.078min (-0.013) 0.05ng/ul m

response 2288

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	19.41#
176.00	19.10	22.98#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006541.D
Acq On : 24 Jun 2019 21:04
Operator : HP/JU
Sample : K3362-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41Z5

Manual Integrations
APPROVED

mohammad
6/25/2019 10:20:27 PM

Quant Time: Jun 25 03:22:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

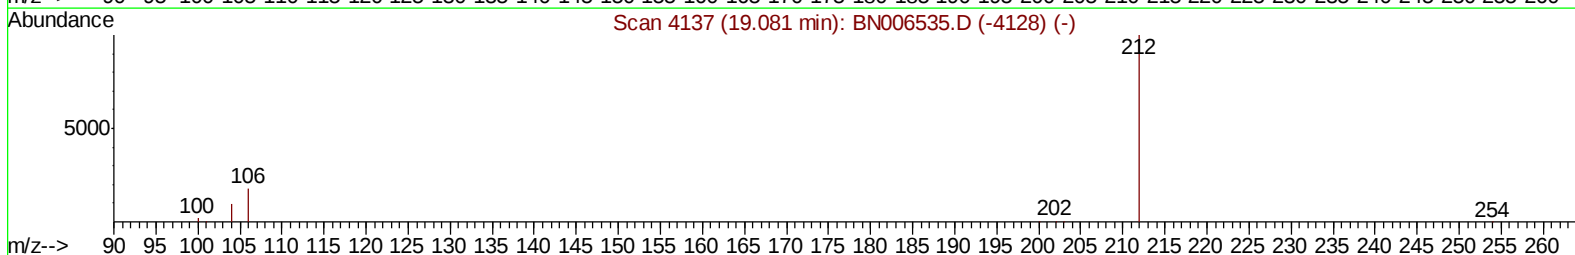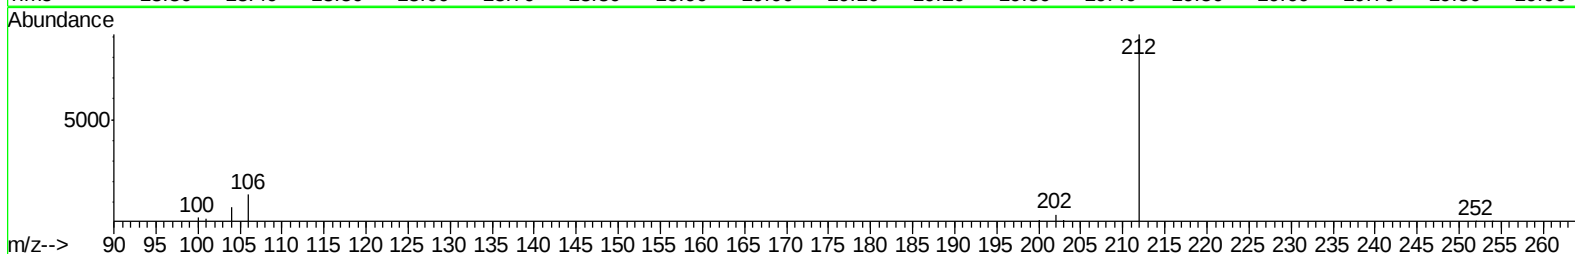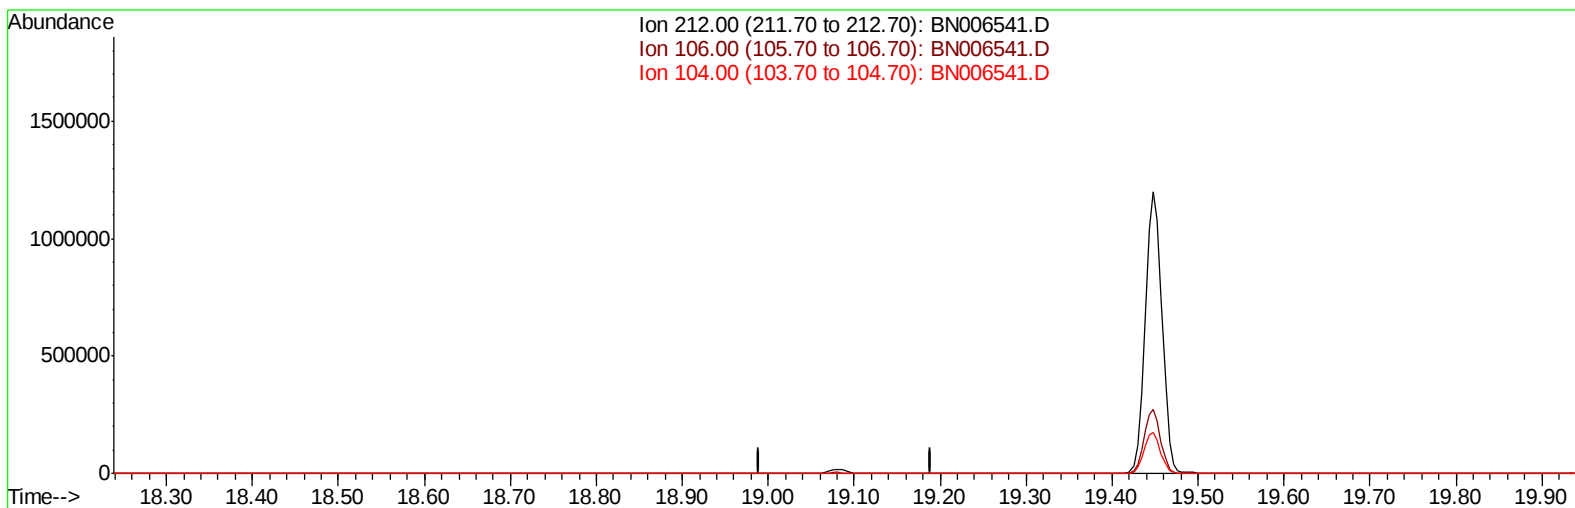

TIC: BN006541.D

(14) Fluoranthene-d10 (SURR)

19.090min (-19.090) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006541.D
Acq On : 24 Jun 2019 21:04
Operator : HP/JU
Sample : K3362-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41Z5

Manual Integrations
APPROVED

mohammad
6/25/2019 10:20:27 PM

Quant Time: Jun 25 03:22:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

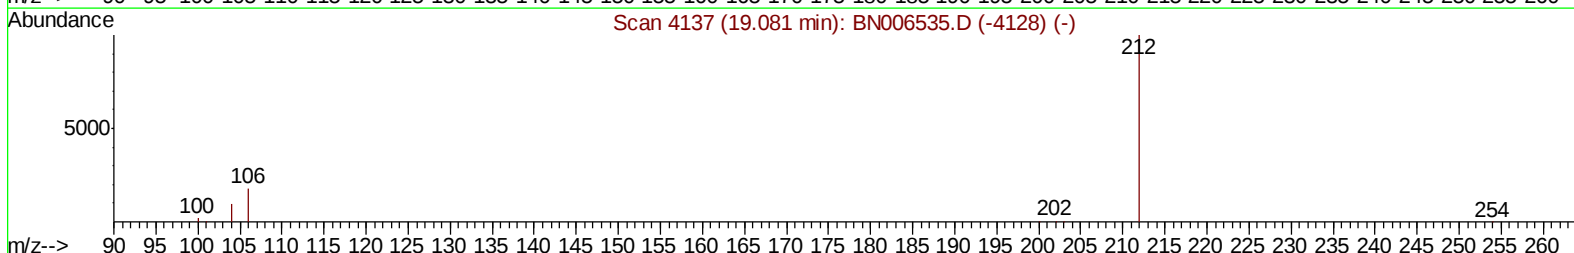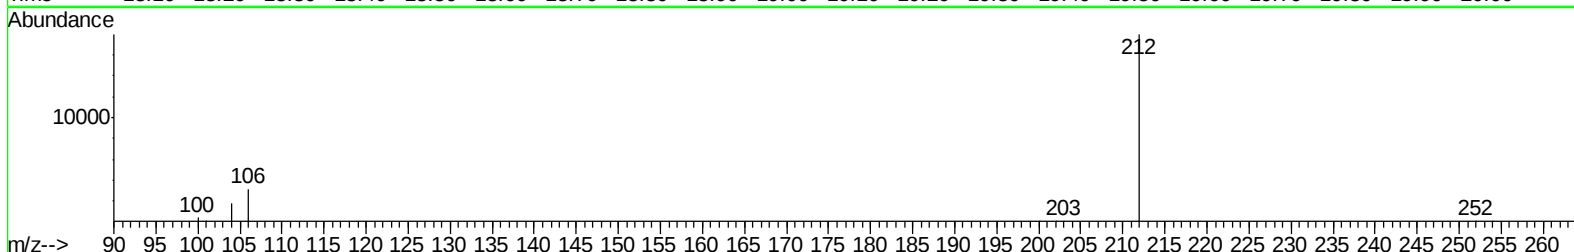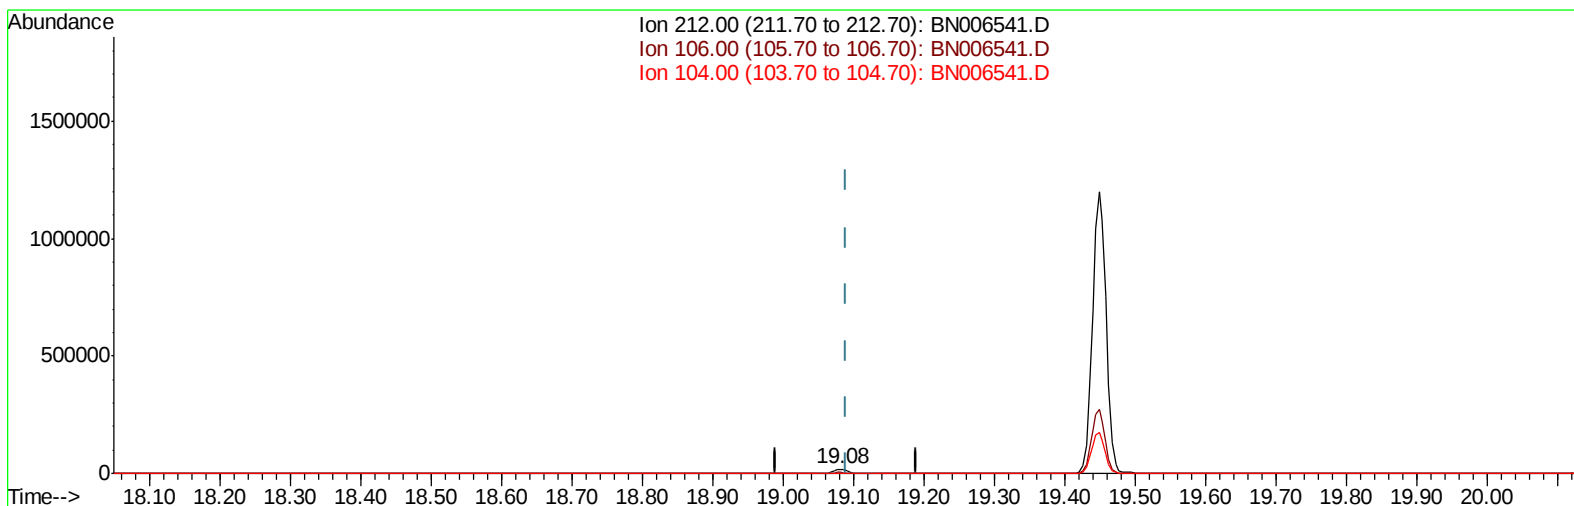

TIC: BN006541.D

(14) Fluoranthene-d10 (SURR)

19.081min (-0.009) 0.58ng/ul m

response 24253

Ion	Exp%	Act%
212.00	100	100
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006541.D
Acq On : 24 Jun 2019 21:04
Operator : HP/JU
Sample : K3362-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41Z5

Manual Integrations
APPROVED

mohammad
6/25/2019 10:20:27 PM

Quant Time: Jun 25 03:22:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

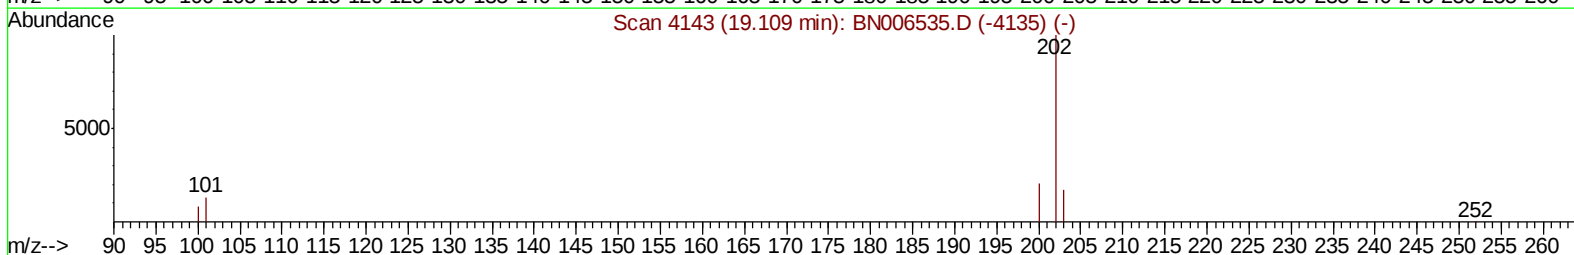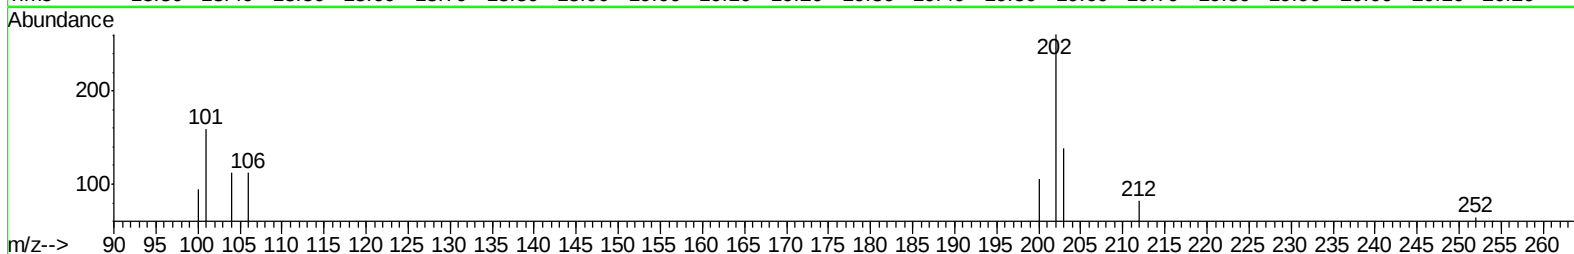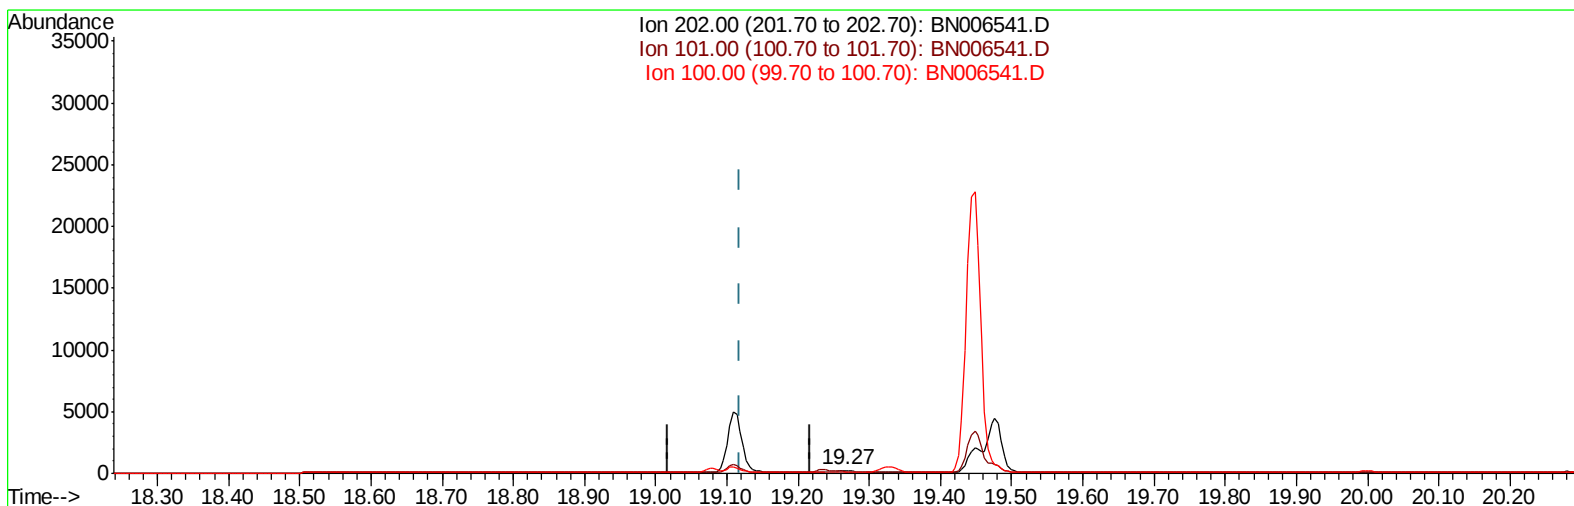

TIC: BN006541.D

(15) Fluoranthene (C)

19.267min (+0.149) 0.00ng/ul

response 229

Ion	Exp%	Act%
202.00	100	100
101.00	12.10	60.92#
100.00	8.70	36.40#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006541.D
Acq On : 24 Jun 2019 21:04
Operator : HP/JU
Sample : K3362-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41Z5

Manual Integrations
APPROVED

mohammad
6/25/2019 10:20:27 PM

Quant Time: Jun 25 03:22:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

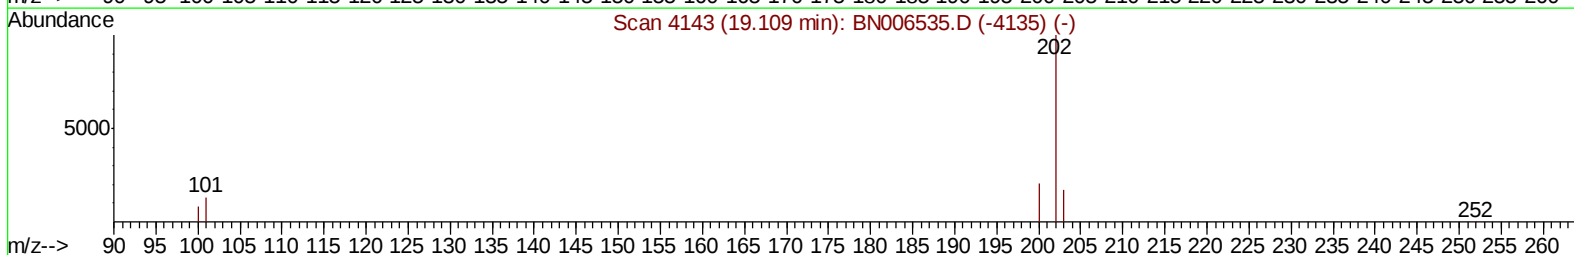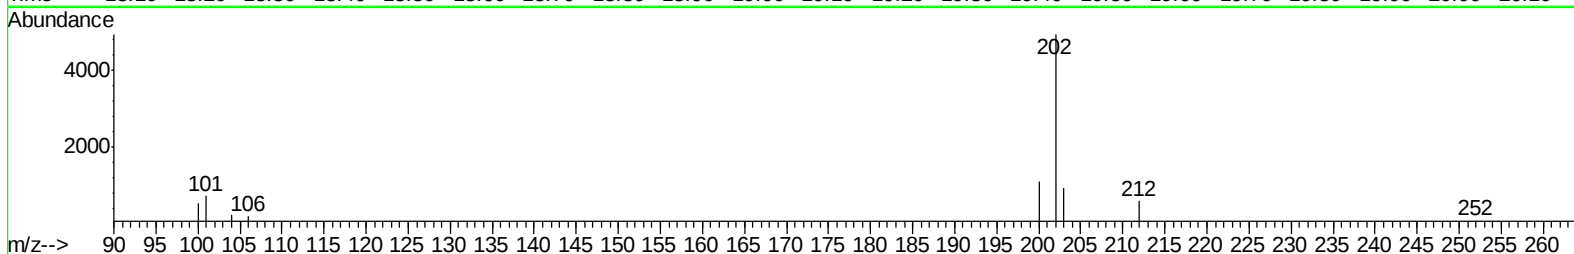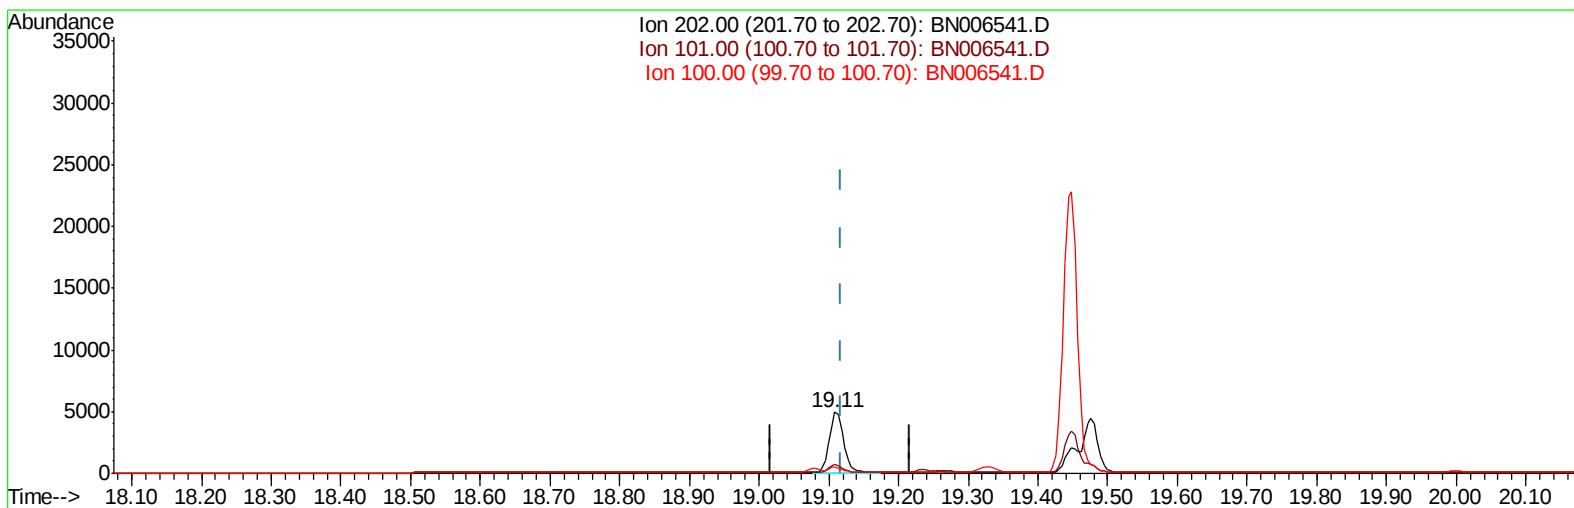

TIC: BN006541.D

(15) Fluoranthene (C)

19.109min (-0.009) 0.13ng/ul m

response 7272

Ion	Exp%	Act%
202.00	100	100
101.00	12.10	14.64
100.00	8.70	10.81
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006541.D
Acq On : 24 Jun 2019 21:04
Operator : HP/JU
Sample : K3362-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41Z5

Manual Integrations
APPROVED

mohammad
6/25/2019 10:20:27 PM

Quant Time: Jun 25 03:22:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

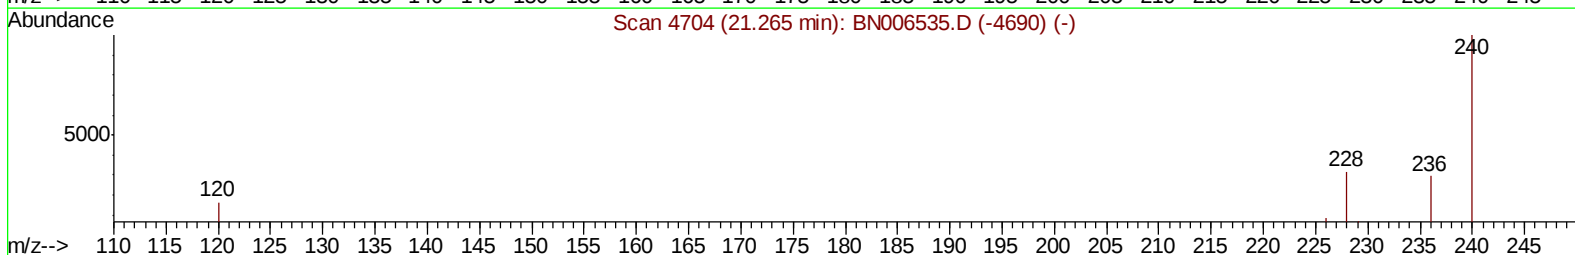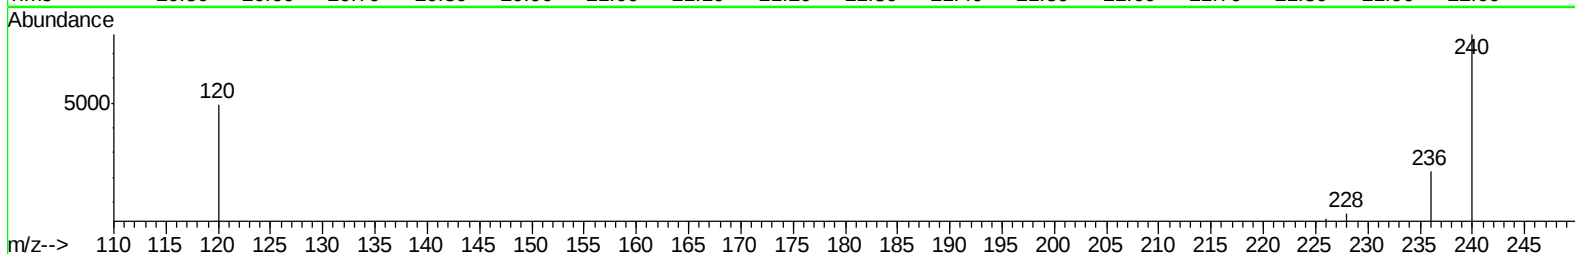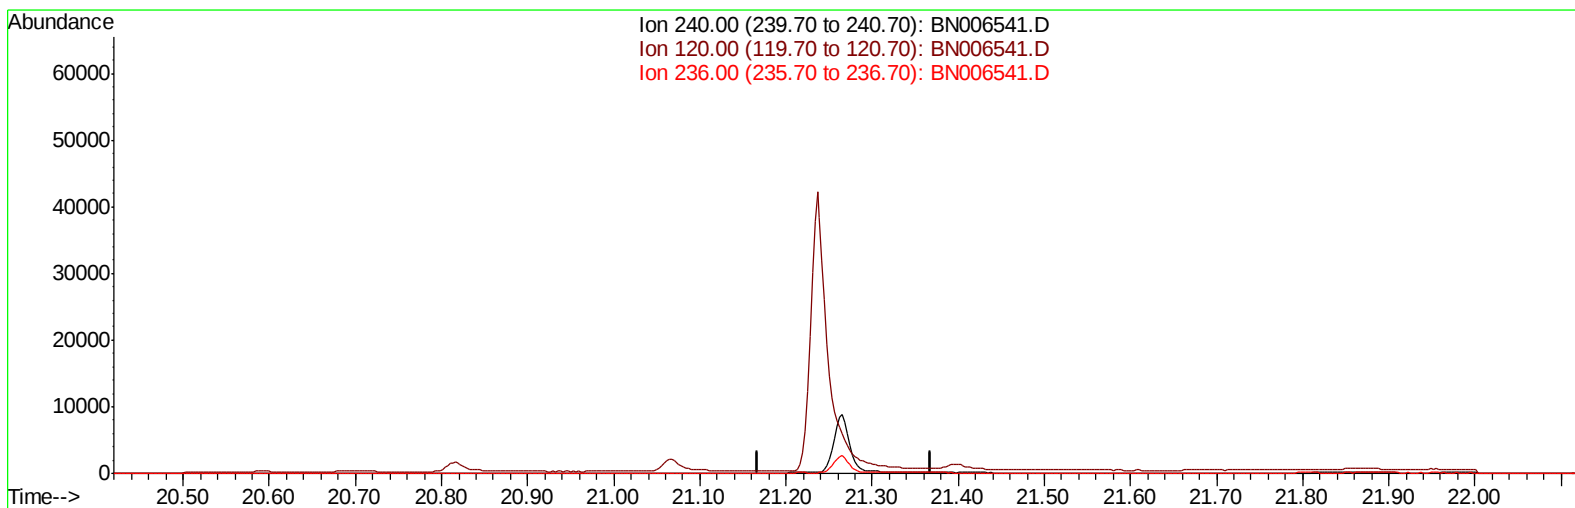

TIC: BN006541.D

(16) Chrysene-d12 (I)

21.268min (-21.268) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	20.10	0.00#
236.00	30.10	0.00#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006541.D
Acq On : 24 Jun 2019 21:04
Operator : HP/JU
Sample : K3362-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41Z5

Manual Integrations
APPROVED

mohammad
6/25/2019 10:20:27 PM

Quant Time: Jun 25 03:22:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

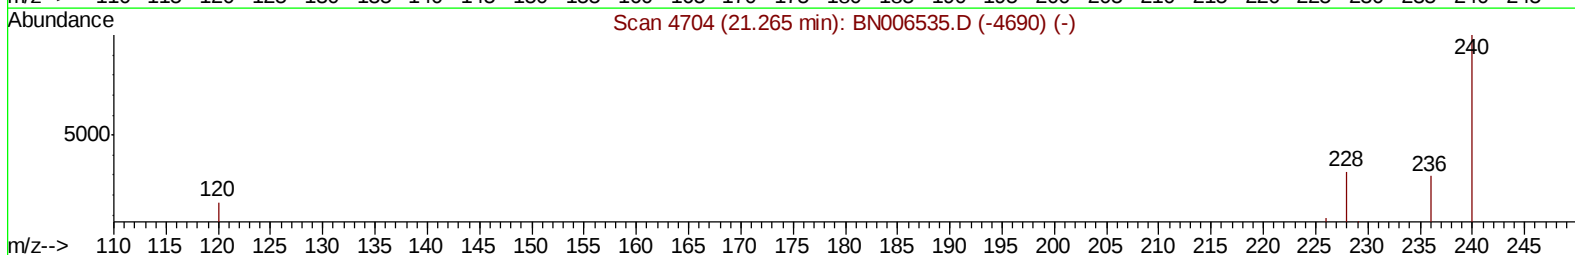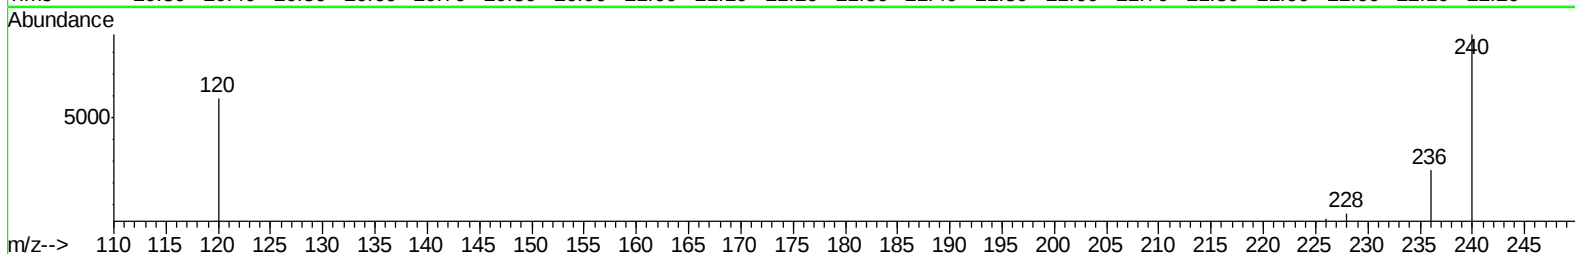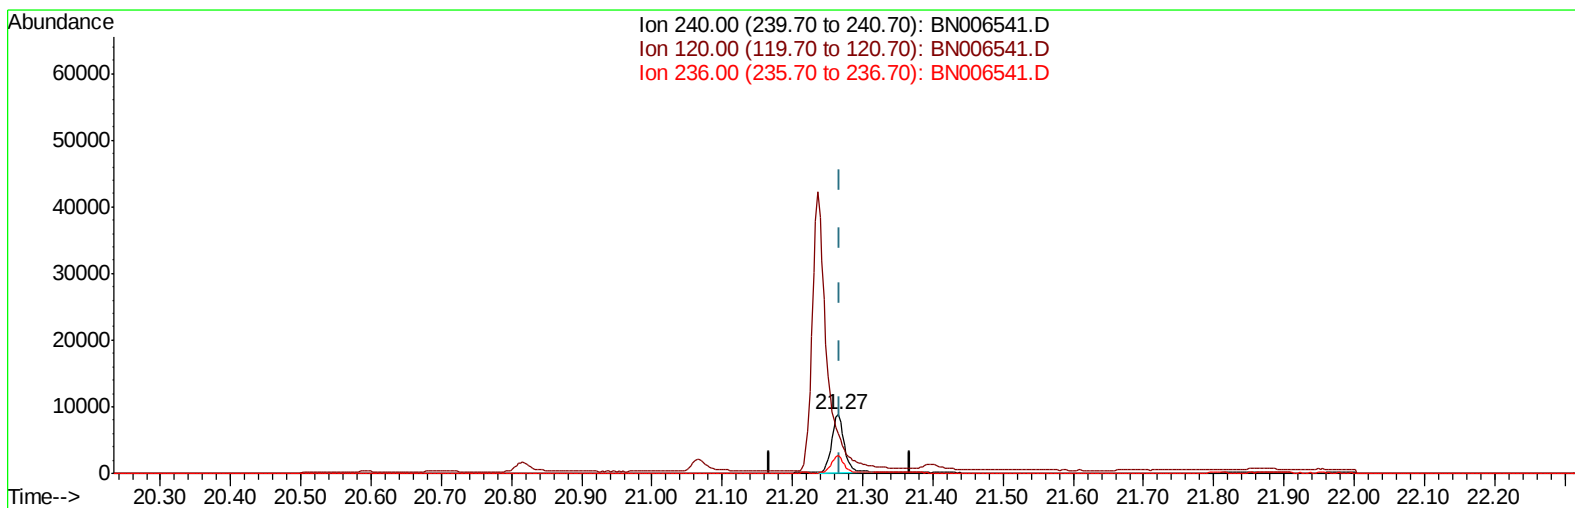

TIC: BN006541.D

(16) Chrysene-d12 (I)

21.265min (-0.003) 0.40ng/ul m

response 10825

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	66.79#
236.00	30.10	29.64
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006541.D
Acq On : 24 Jun 2019 21:04
Operator : HP/JU
Sample : K3362-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41Z5

Manual Integrations
APPROVED

mohammad
6/25/2019 10:20:27 PM

Quant Time: Jun 25 03:24:39 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

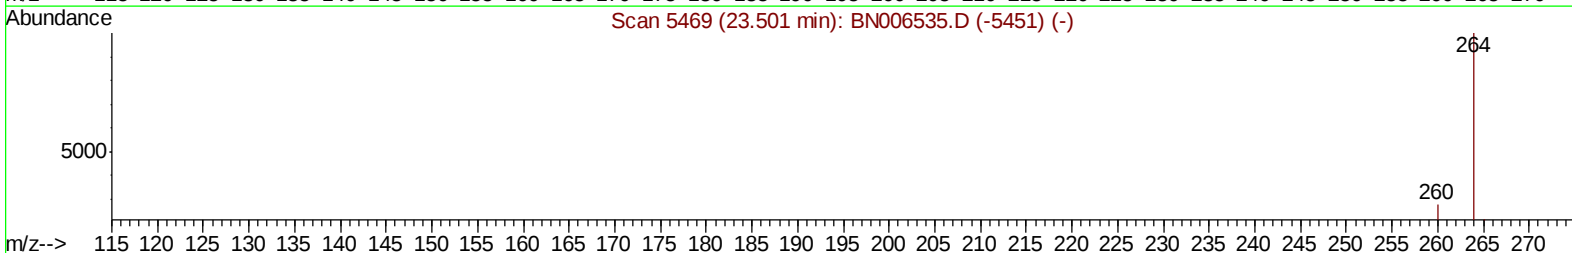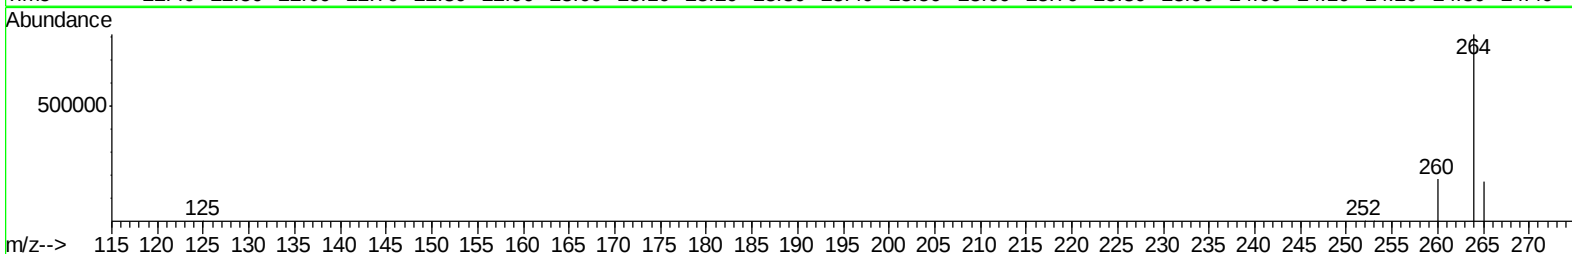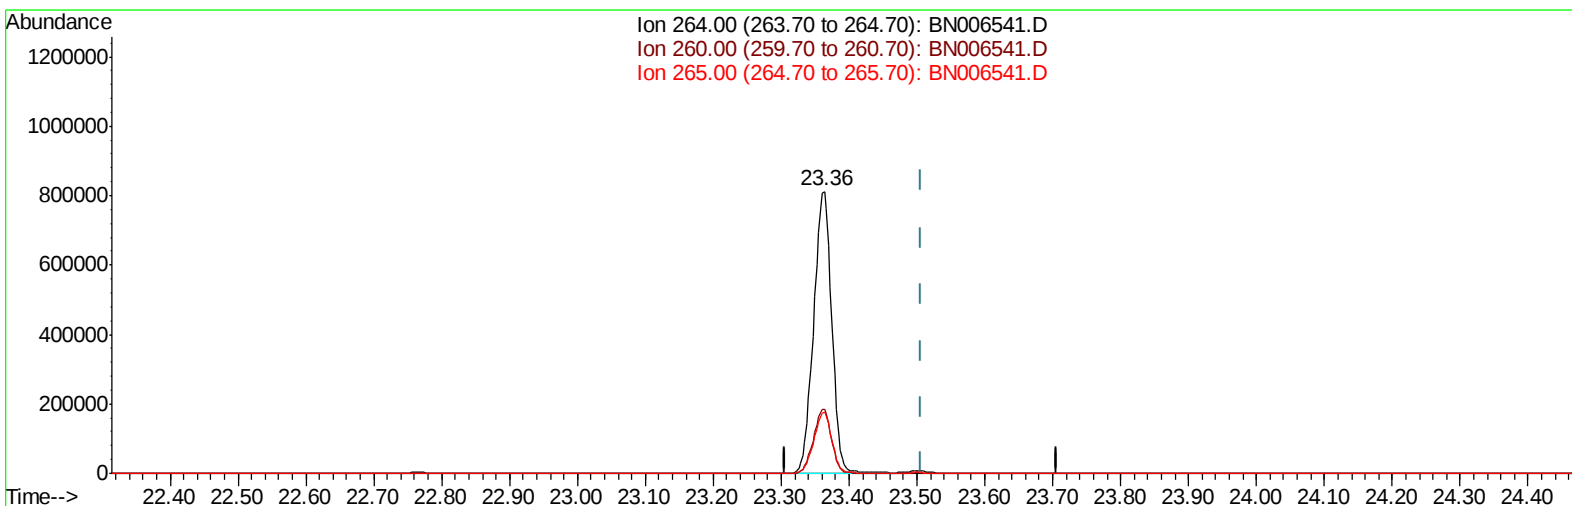

TIC: BN006541.D

(20) Perylene-d12 (I)

23.364min (-0.143) 0.40ng/ul

response 1510502

Ion	Exp%	Act%
264.00	100	100
260.00	29.20	22.63#
265.00	44.70	21.69#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006541.D
Acq On : 24 Jun 2019 21:04
Operator : HP/JU
Sample : K3362-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41Z5

Manual Integrations
APPROVED

mohammad
6/25/2019 10:20:27 PM

Quant Time: Jun 25 03:24:39 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

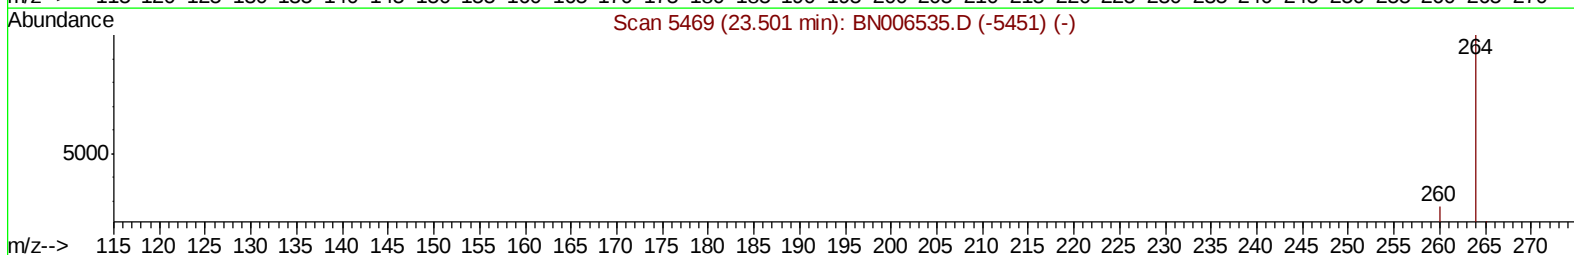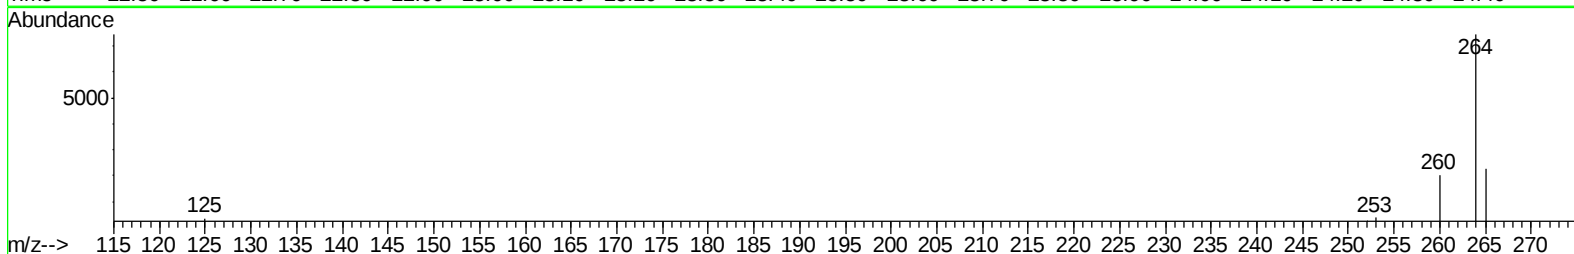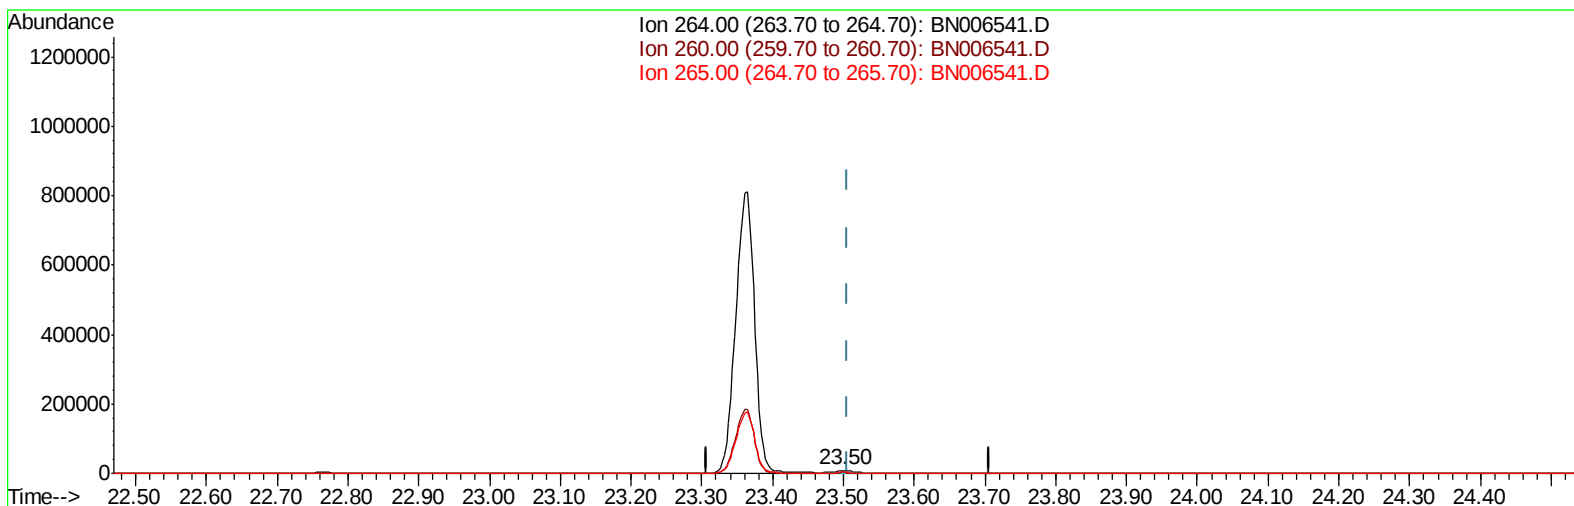

TIC: BN006541.D

(20) Perylene-d12 (I)

23.498min (-0.009) 0.40ng/ul m

response 10537

Ion	Exp%	Act%
264.00	100	100
260.00	29.20	27.04
265.00	44.70	30.61#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006541.D
Acq On : 24 Jun 2019 21:04
Operator : HP/JU
Sample : K3362-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41Z5

Manual Integrations
APPROVED

mohammad
6/25/2019 10:20:27 PM

Quant Time: Jun 25 03:25:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

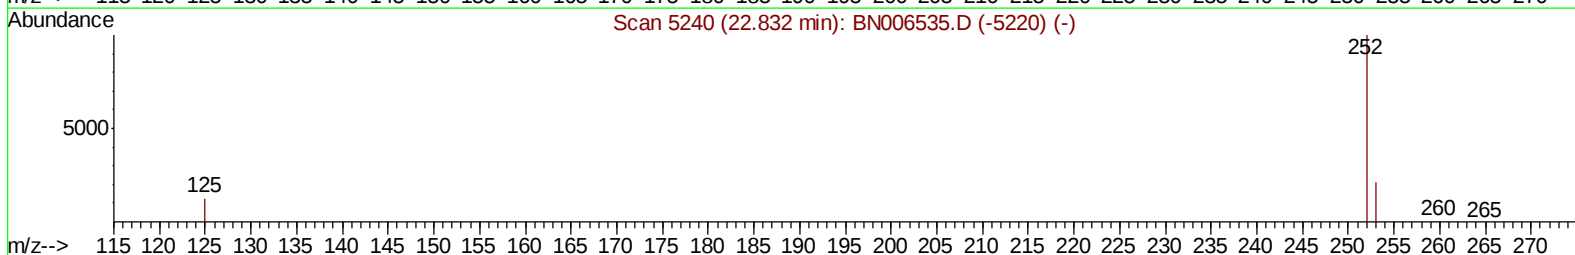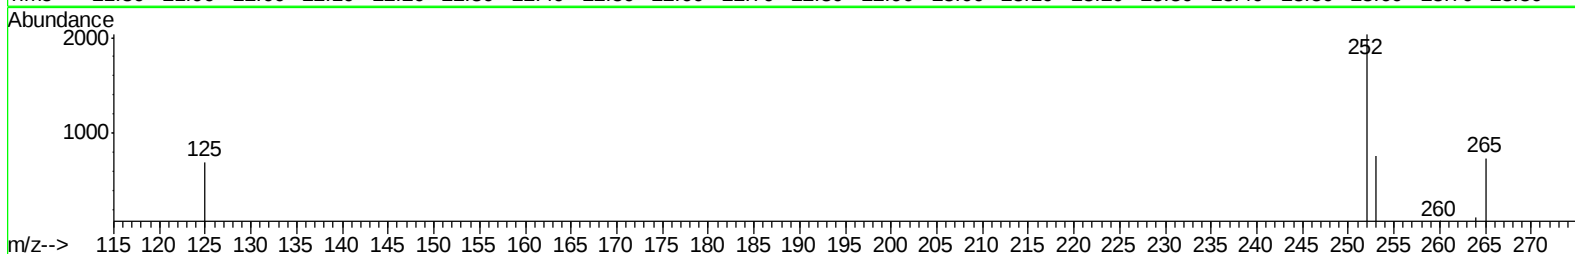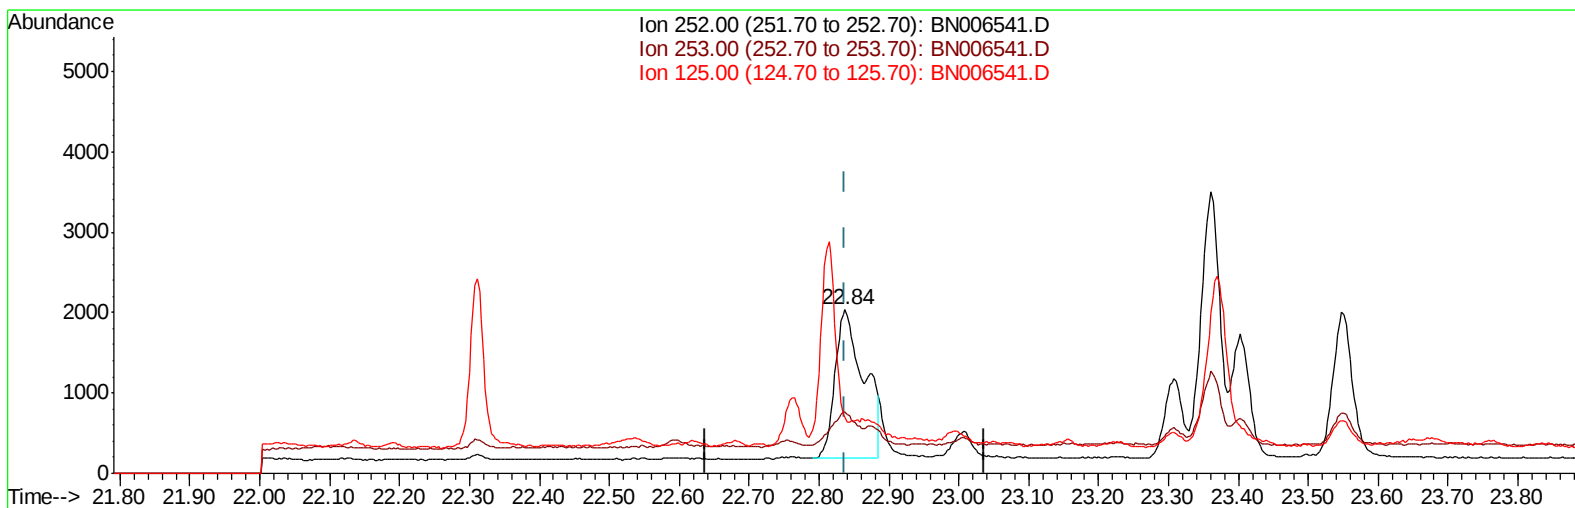

TIC: BN006541.D

(21) Benzo(b)fluoranthene

22.838min (+0.000) 0.12ng/ul

response 5250

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	37.53
125.00	20.50	34.63
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006541.D
Acq On : 24 Jun 2019 21:04
Operator : HP/JU
Sample : K3362-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41Z5

Manual Integrations
APPROVED

mohammad
6/25/2019 10:20:27 PM

Quant Time: Jun 25 03:25:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

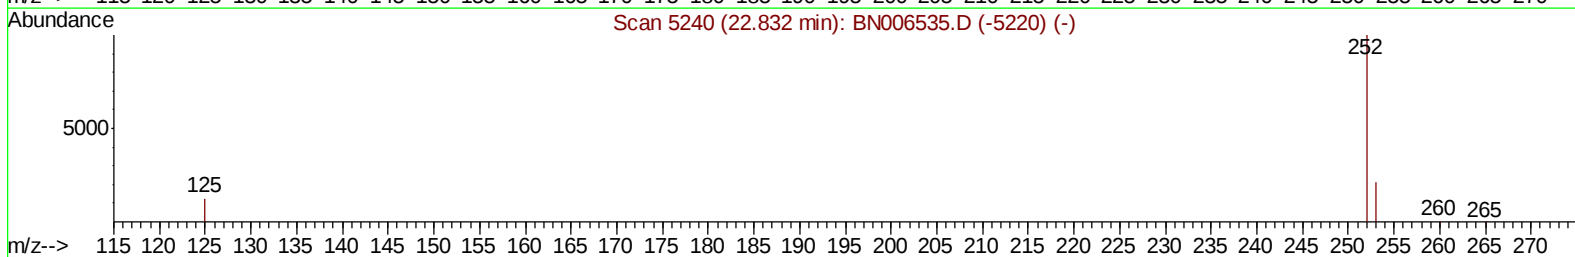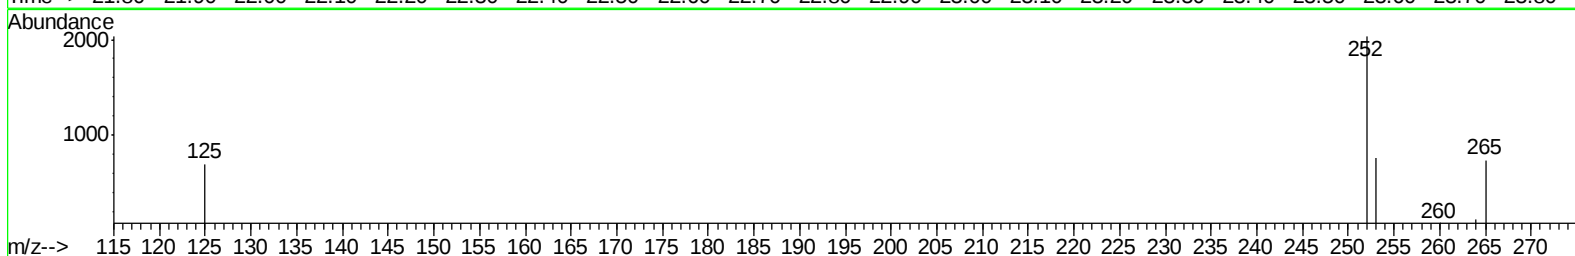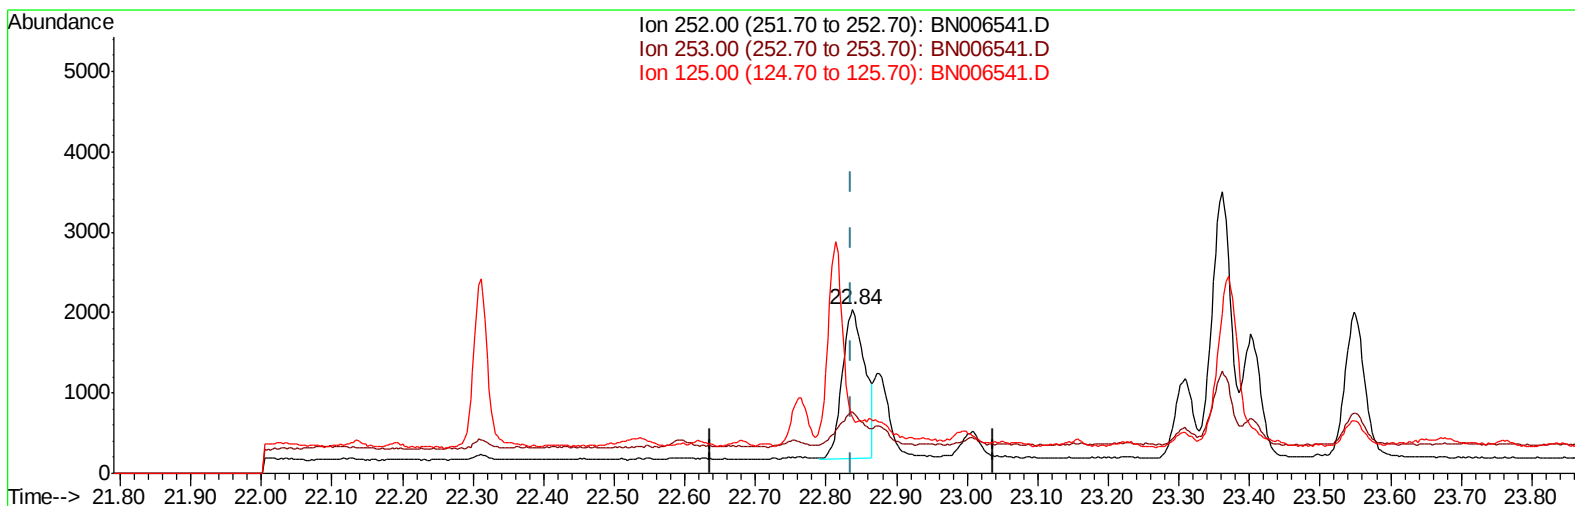

TIC: BN006541.D

(21) Benzo(b)fluoranthene

22.838min (+0.000) 0.09ng/ul m

response 4052

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	37.53
125.00	20.50	34.63
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006541.D
Acq On : 24 Jun 2019 21:04
Operator : HP/JU
Sample : K3362-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41Z5

Manual Integrations
APPROVED

mohammad
6/25/2019 10:20:27 PM

Quant Time: Jun 25 03:25:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

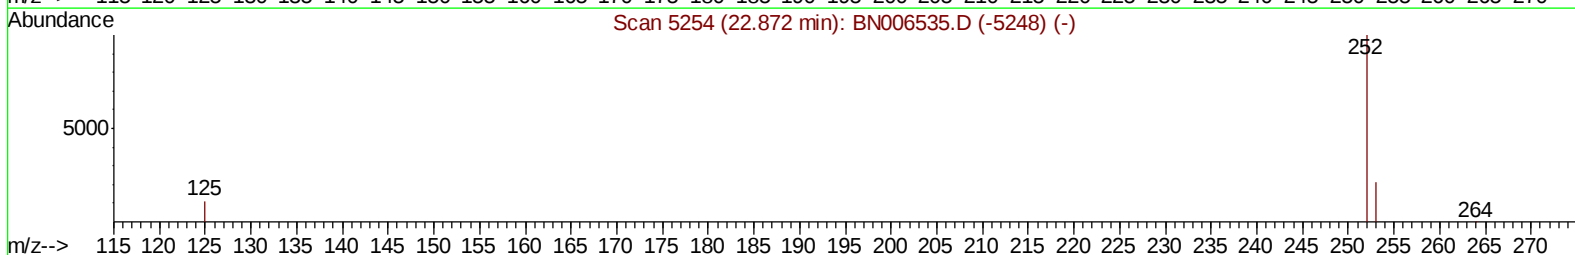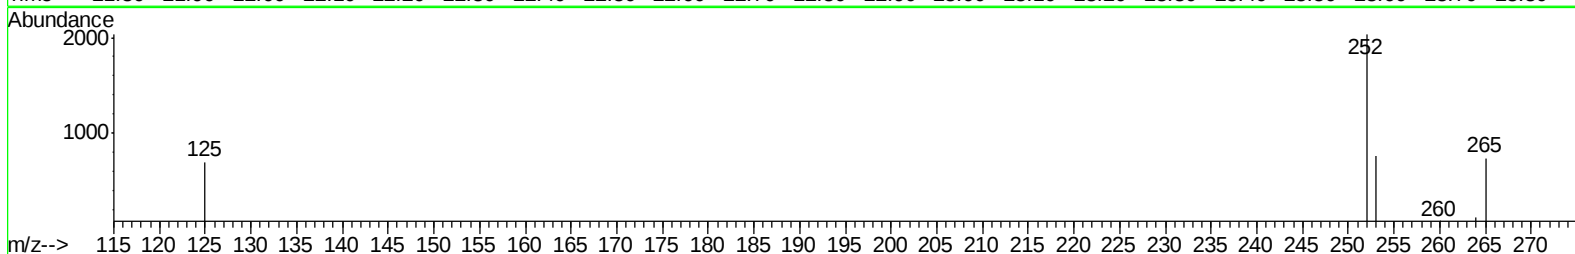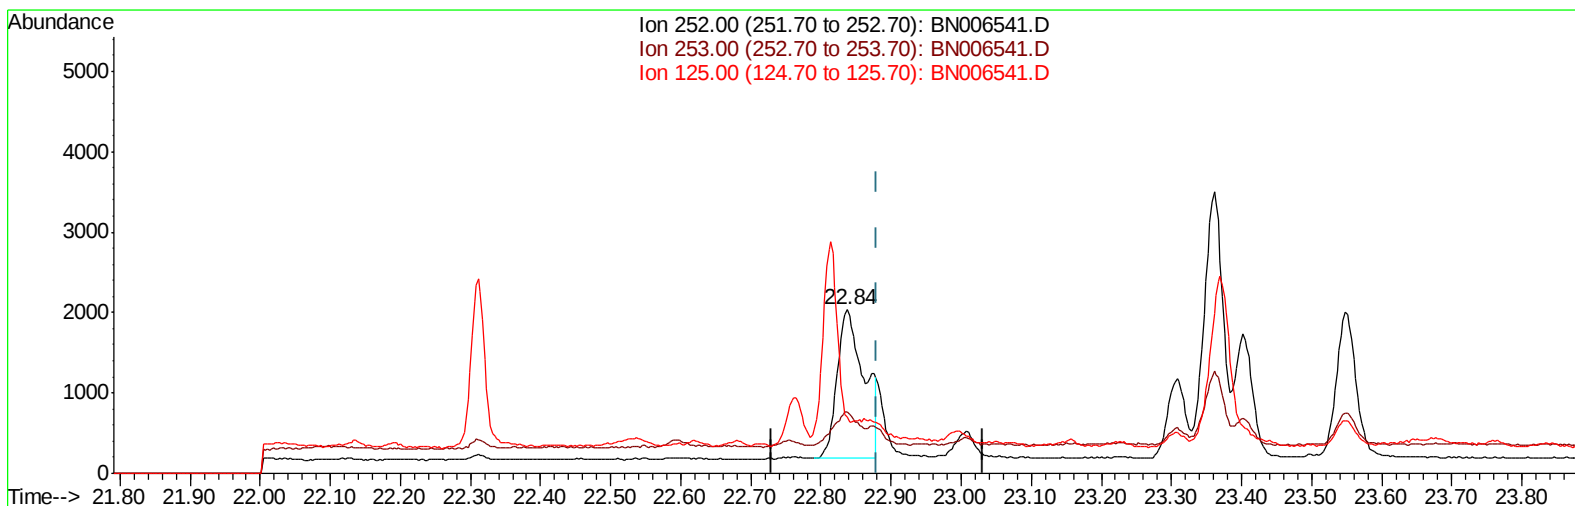

TIC: BN006541.D

(22) Benzo(k)fluoranthene

22.838min (-0.044) 0.12ng/ul

response 4949

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	37.53#
125.00	17.90	34.63#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006541.D
Acq On : 24 Jun 2019 21:04
Operator : HP/JU
Sample : K3362-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41Z5

Manual Integrations
APPROVED

mohammad
6/25/2019 10:20:27 PM

Quant Time: Jun 25 03:25:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

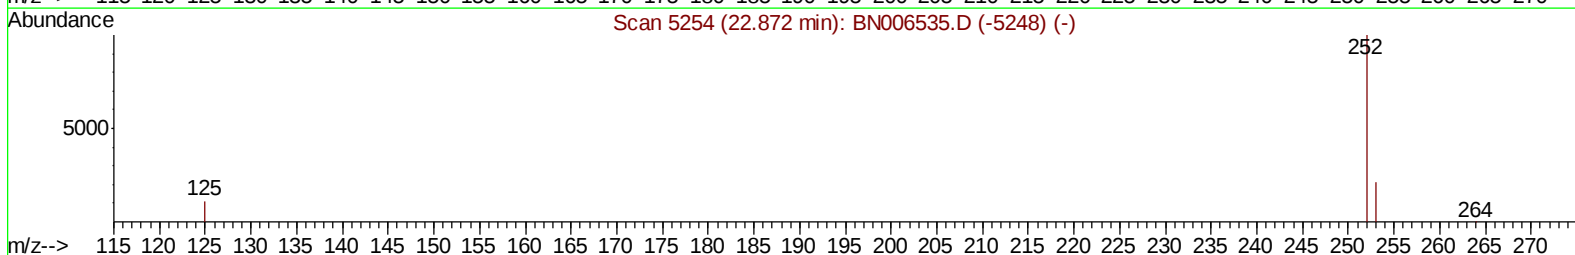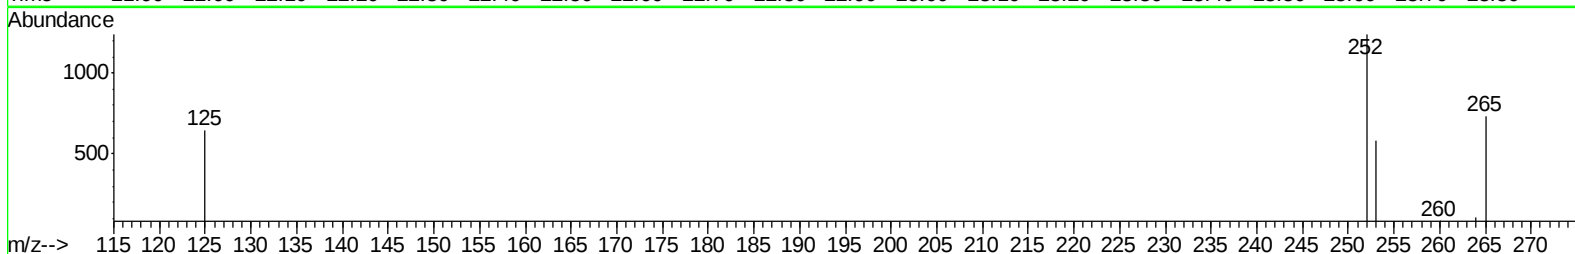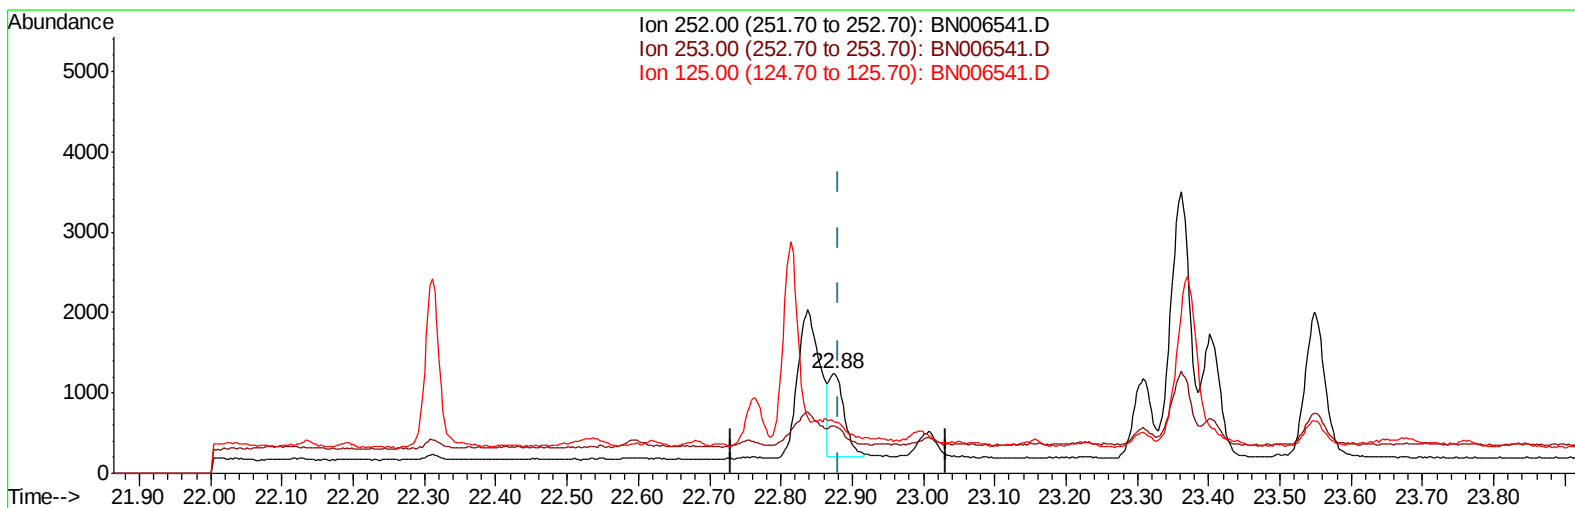

TIC: BN006541.D

(22) Benzo(k)fluoranthene

22.876min (-0.006) 0.04ng/ul m

response 1559

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	46.97#
125.00	17.90	51.74#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006541.D
Acq On : 24 Jun 2019 21:04
Operator : HP/JU
Sample : K3362-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41Z5

Manual Integrations
APPROVED

mohammad
6/25/2019 10:20:27 PM

Quant Time: Jun 25 03:25:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

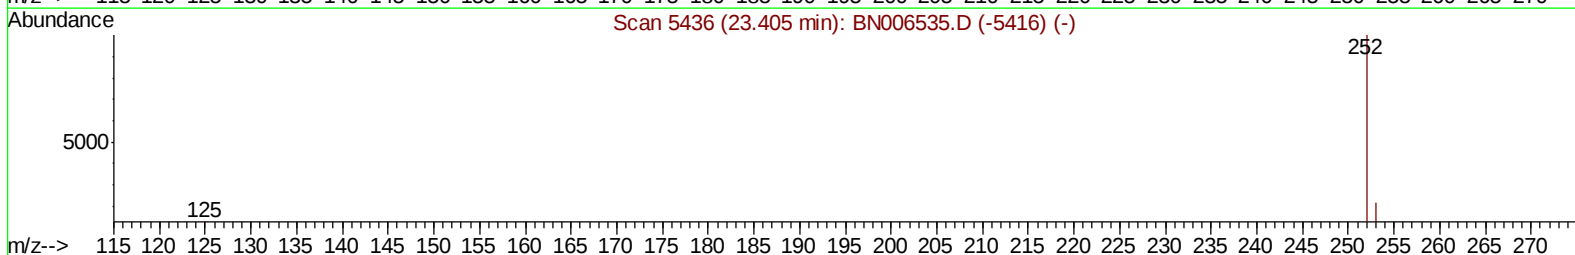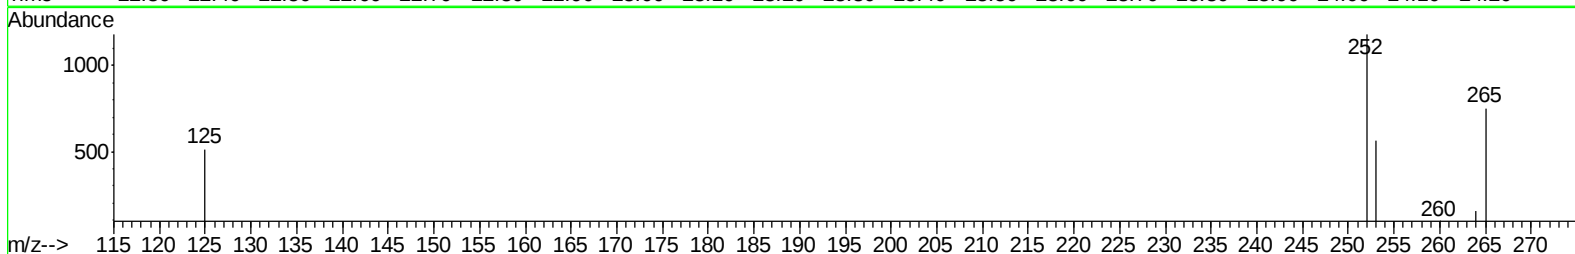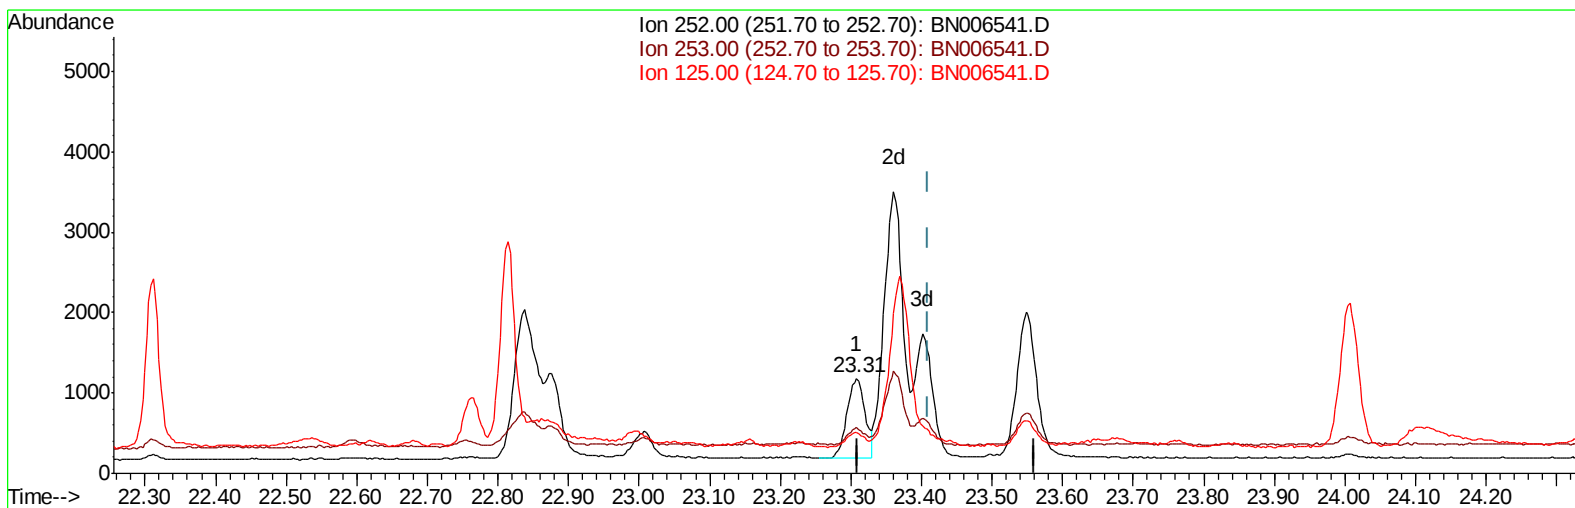

TIC: BN006541.D

(23) Benzo(a)pyrene (C)

23.308min (-0.102) 0.04ng/ul

response 1784

Ion	Exp%	Act%
252.00	100	100
253.00	26.40	48.05#
125.00	25.40	43.49#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006541.D
Acq On : 24 Jun 2019 21:04
Operator : HP/JU
Sample : K3362-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41Z5

Manual Integrations
APPROVED

mohammad
6/25/2019 10:20:27 PM

Quant Time: Jun 25 03:25:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

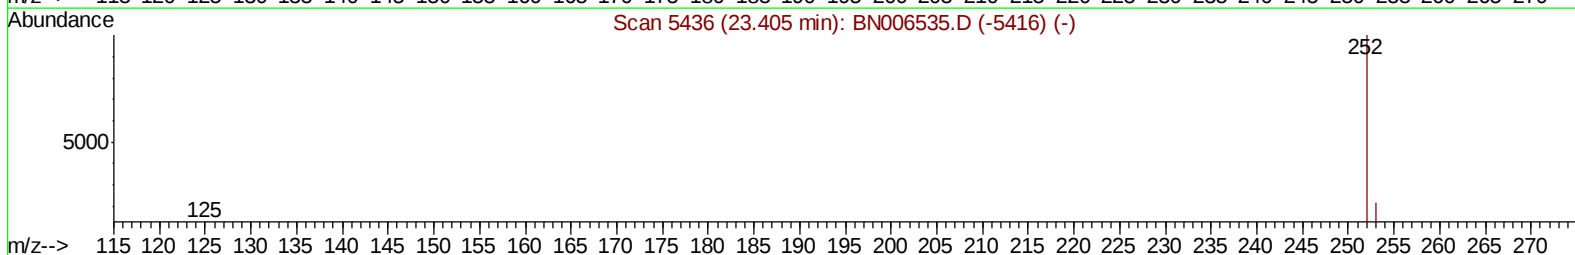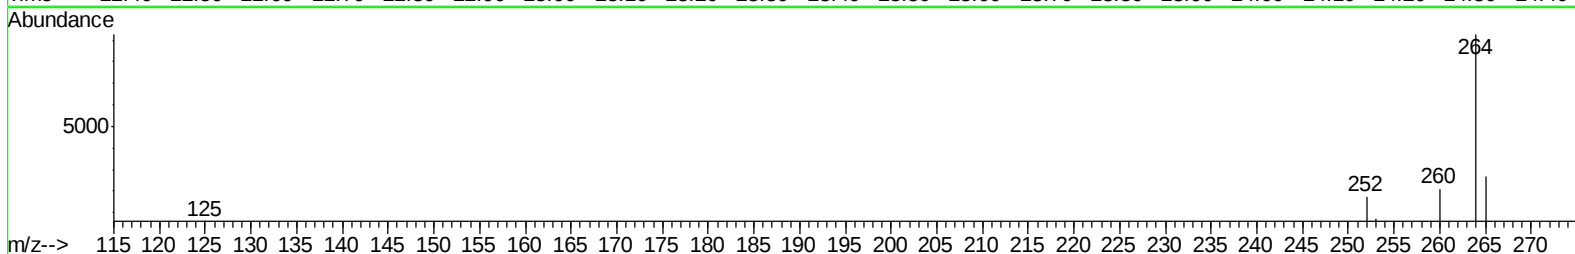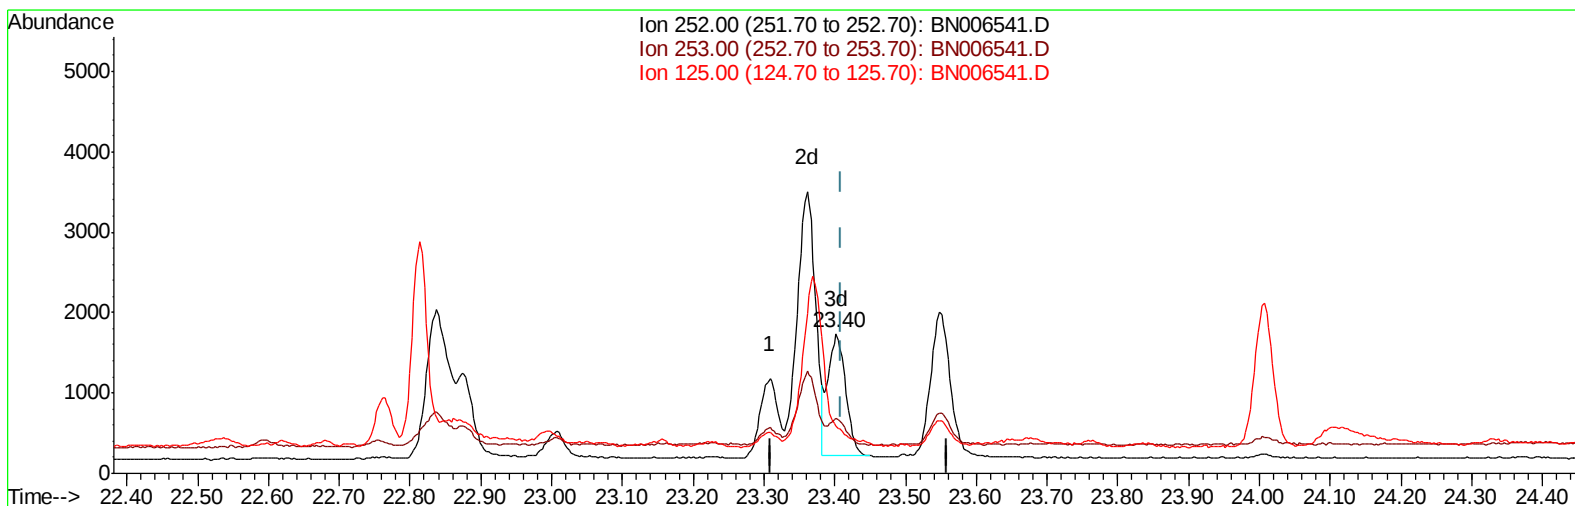

TIC: BN006541.D

(23) Benzo(a)pyrene (C)

23.402min (-0.009) 0.07ng/ul m

response 2673

Ion	Exp%	Act%
252.00	100	100
253.00	26.40	39.51#
125.00	25.40	34.16#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006541.D
Acq On : 24 Jun 2019 21:04
Operator : HP/JU
Sample : K3362-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41Z5

Manual Integrations
APPROVED

mohammad
6/25/2019 10:20:27 PM

Quant Time: Jun 25 03:25:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

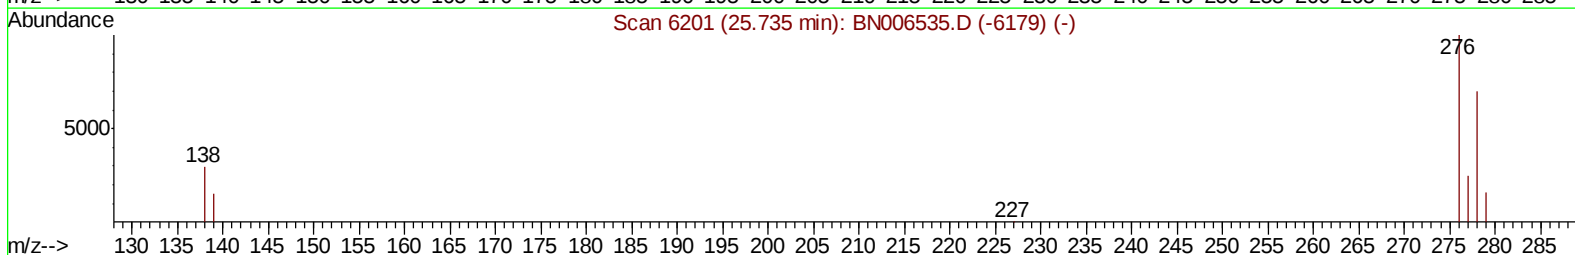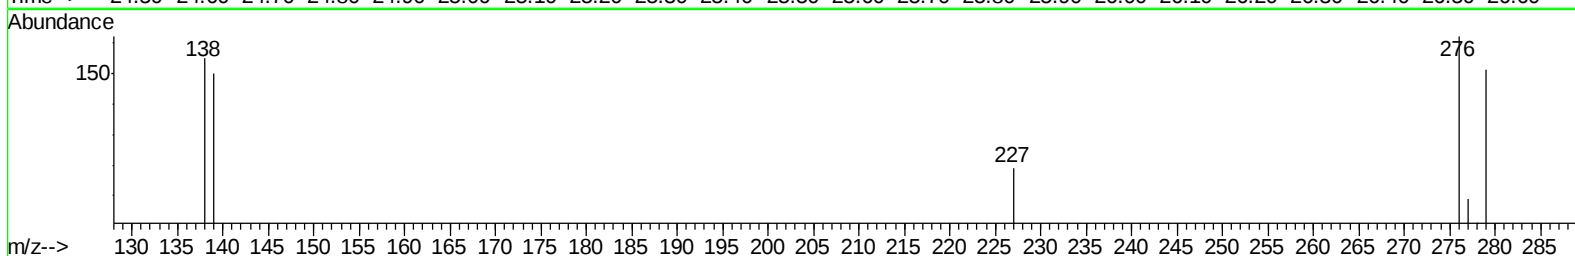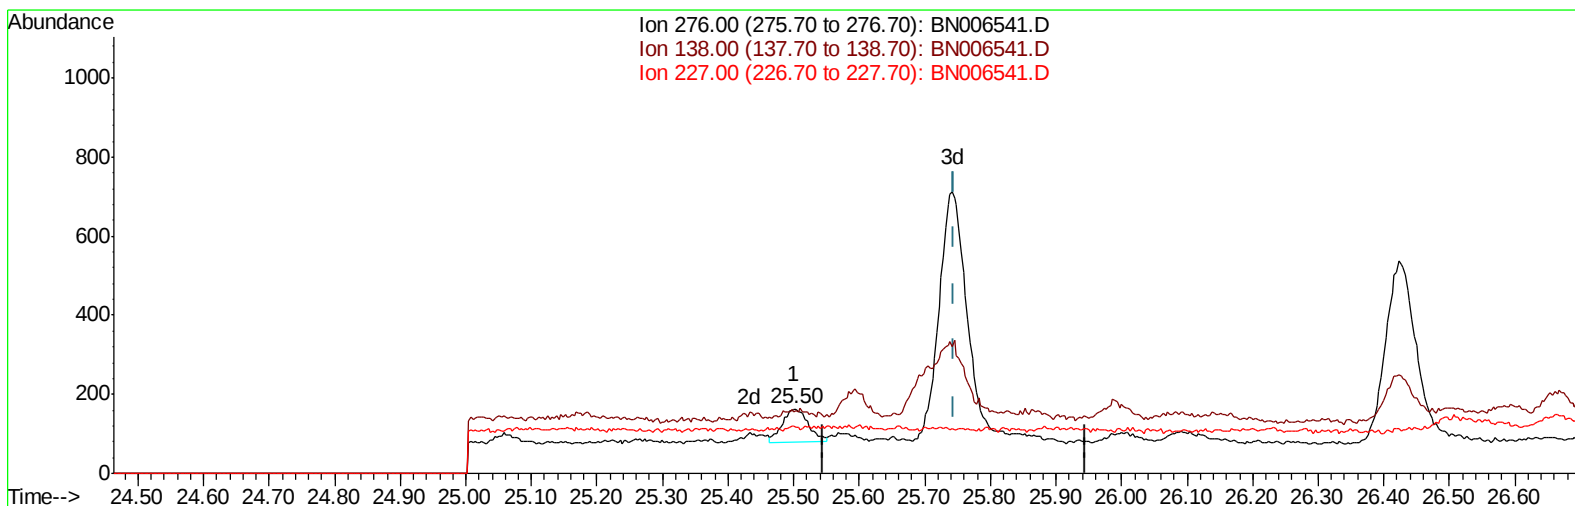

TIC: BN006541.D

(24) Indeno(1,2,3-cd)pyrene

25.500min (-0.245) 0.01ng/ul

response 226

Ion	Exp%	Act%
276.00	100	100
138.00	32.00	26.99
227.00	0.40	5.75#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006541.D
Acq On : 24 Jun 2019 21:04
Operator : HP/JU
Sample : K3362-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41Z5

Manual Integrations
APPROVED

mohammad
6/25/2019 10:20:27 PM

Quant Time: Jun 25 03:25:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

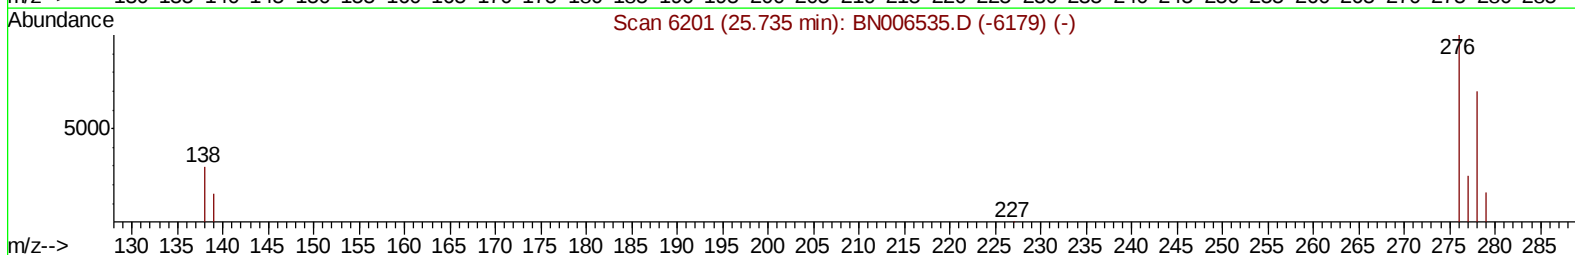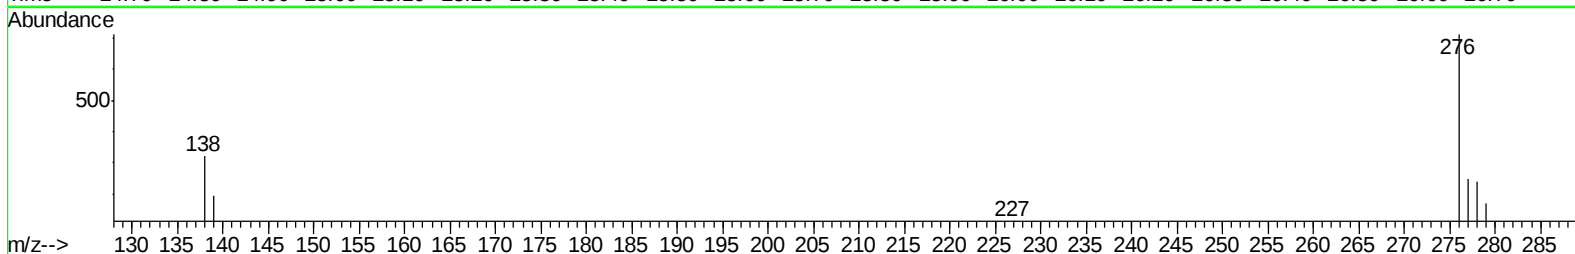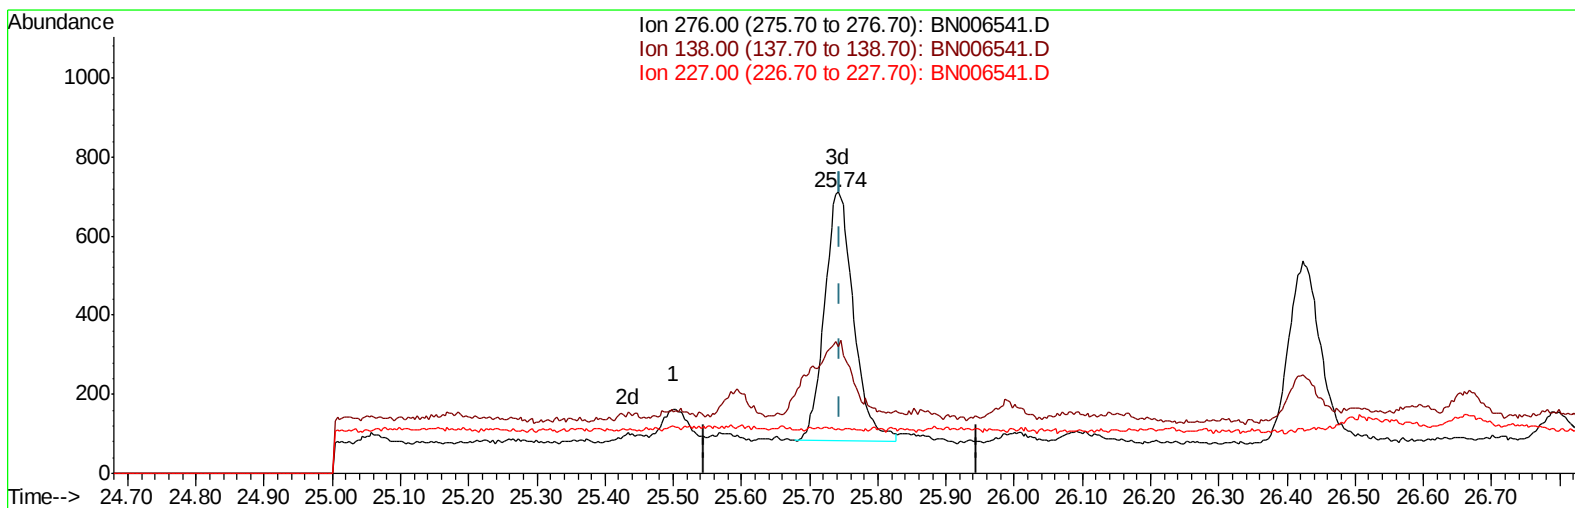

TIC: BN006541.D

(24) Indeno(1,2,3-cd)pyrene
25.742min (-0.003) 0.04ng/ul m
response 1857

Ion	Exp%	Act%
276.00	100	100
138.00	32.00	3.28#
227.00	0.40	0.70#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006541.D
Acq On : 24 Jun 2019 21:04
Operator : HP/JU
Sample : K3362-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A41Z5

Manual Integrations
APPROVED

mohammad
6/25/2019 10:20:27 PM

Quant Time: Jun 25 03:25:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

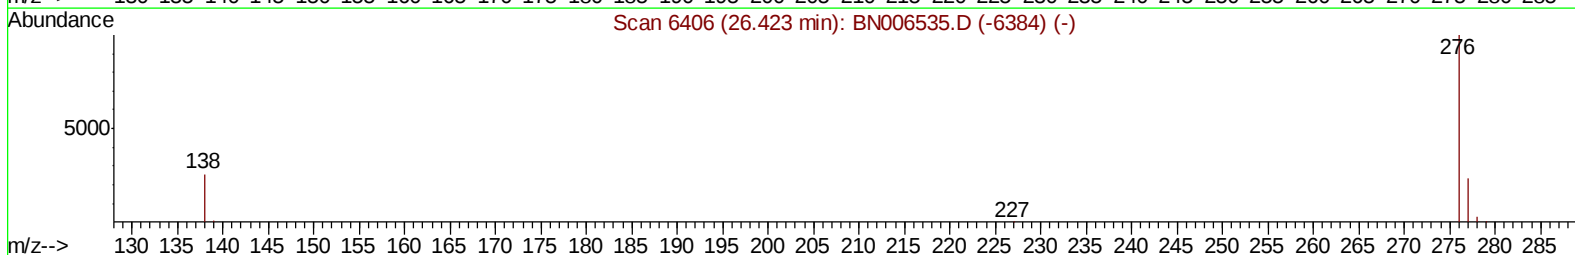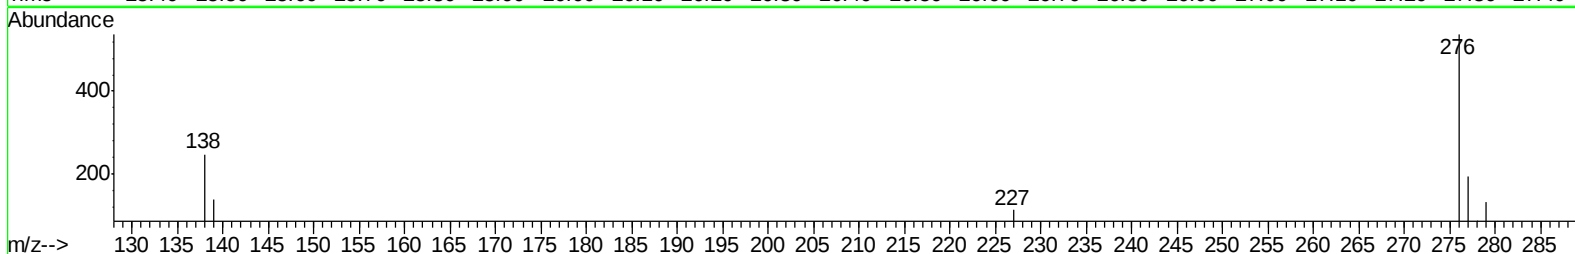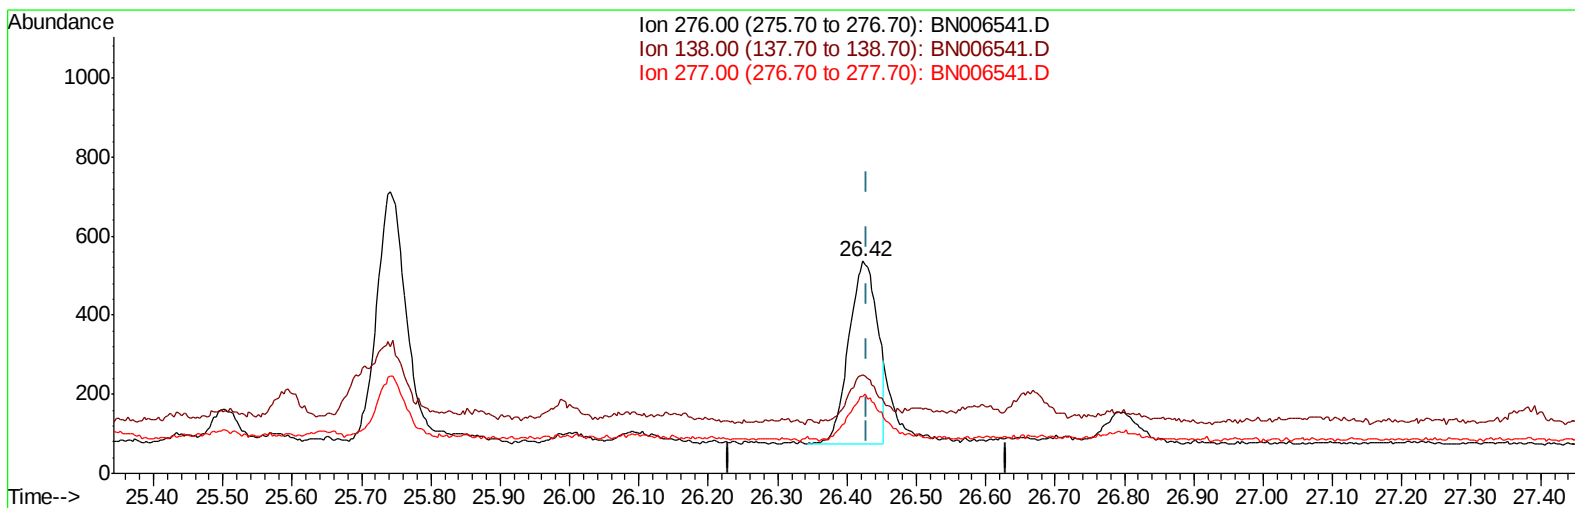

TIC: BN006541.D

(26) Benzo(g,h,i)perylene

26.423min (-0.007) 0.04ng/ul

response 1324

Ion	Exp%	Act%
276.00	100	100
138.00	30.30	46.18#
277.00	26.90	36.13#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006541.D
Acq On : 24 Jun 2019 21:04
Operator : HP/JU
Sample : K3362-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41Z5

Manual Integrations
APPROVED

mohammad
6/25/2019 10:20:27 PM

Quant Time: Jun 25 03:25:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

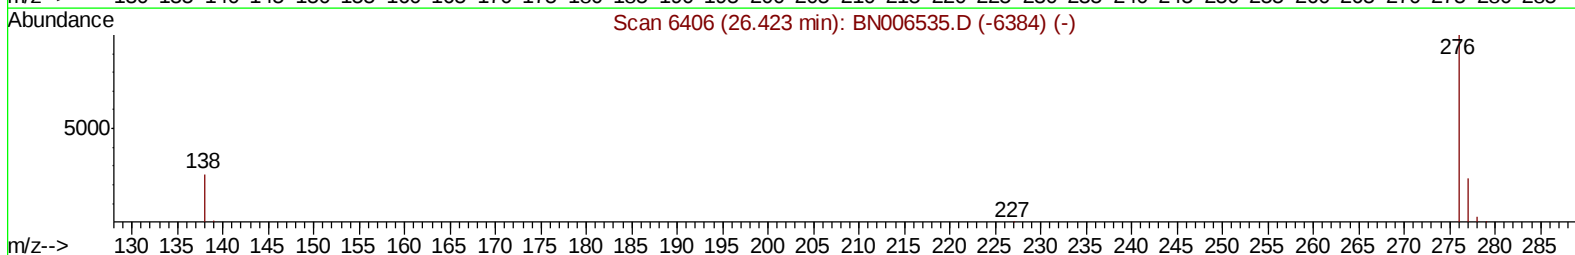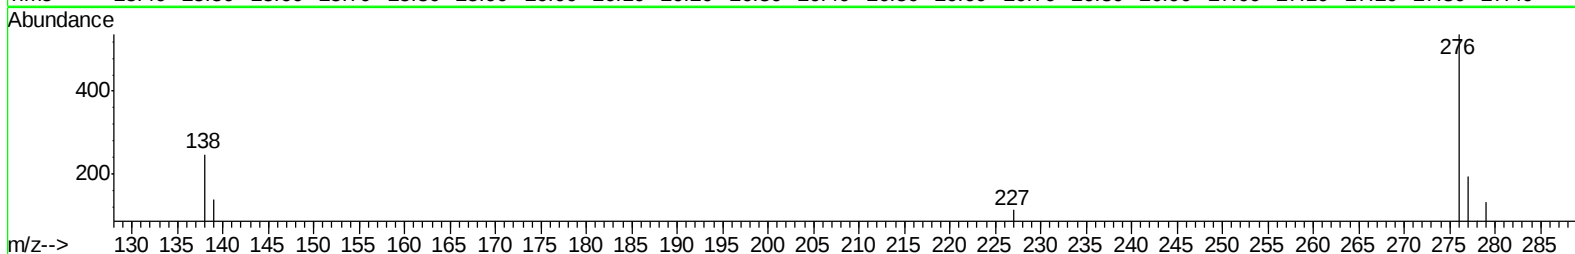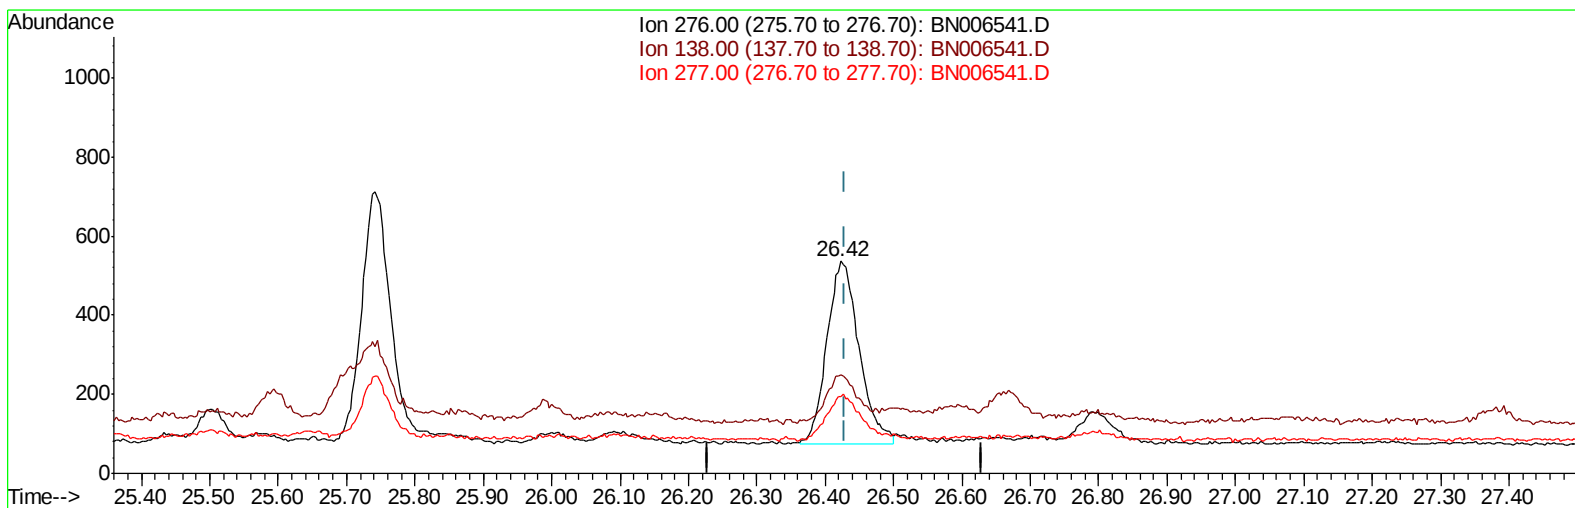

TIC: BN006541.D

(26) Benzo(g,h,i)perylene

26.423min (-0.007) 0.04ng/ul m

response 1504

Ion	Exp%	Act%
276.00	100	100
138.00	30.30	46.18#
277.00	26.90	36.13#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
 Data File : BN006541.D
 Acq On : 24 Jun 2019 21:04
 Operator : HP/JU
 Sample : K3362-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A41Z5

Manual Integrations
 APPROVED

mohammad
 6/25/2019 10:20:27 PM

Quant Time: Jun 25 03:27:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	5055	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.41	136	18184	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.28	164	8820	0.40	ng/ul	-0.01
10) Phenanthrene-d10	17.04	188	15440m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.27	240	10825m	0.40	ng/ul	0.00
20) Perylene-d12	23.50	264	10537m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.01	152	14173	0.51	ng/ul	-0.02
14) Fluoranthene-d10	19.08	212	24253m	0.58	ng/ul	0.00
Target Compounds					Qvalue	
12) Phenanthrene	17.08	178	2288m	0.046	ng/ul	
15) Fluoranthene	19.11	202	7272m	0.133	ng/ul	
17) Pyrene	19.48	202	6007	0.105	ng/ul#	93
18) Benzo(a)anthracene	21.25	228	2960	0.062	ng/ul#	92
19) Chrysene	21.30	228	2818	0.063	ng/ul#	91
21) Benzo(b)fluoranthene	22.84	252	4052m	0.092	ng/ul	
22) Benzo(k)fluoranthene	22.88	252	1559m	0.036	ng/ul	
23) Benzo(a)pyrene	23.40	252	2673m	0.065	ng/ul	
24) Indeno(1,2,3-cd)pyrene	25.74	276	1857m	0.042	ng/ul	
26) Benzo(g,h,i)perylene	26.42	276	1504m	0.041	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006541.D
Acq On : 24 Jun 2019 21:04
Operator : HP/JU
Sample : K3362-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A41Z5

Manual Integrations
APPROVED

mohammad
6/25/2019 10:20:27 PM

Quant Time: Jun 25 03:27:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

