

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006545.D

Acq On : 24 Jun 2019 23:22

Operator : HP/JU

Sample : K3362-06

Misc :

ALS Vial : 23 Sample Multiplier: 1

Quant Time: Jun 25 03:54:01 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :


A41X5

Manual Integrations

APPROVED

mohammad

6/25/2019 10:20:47 PM

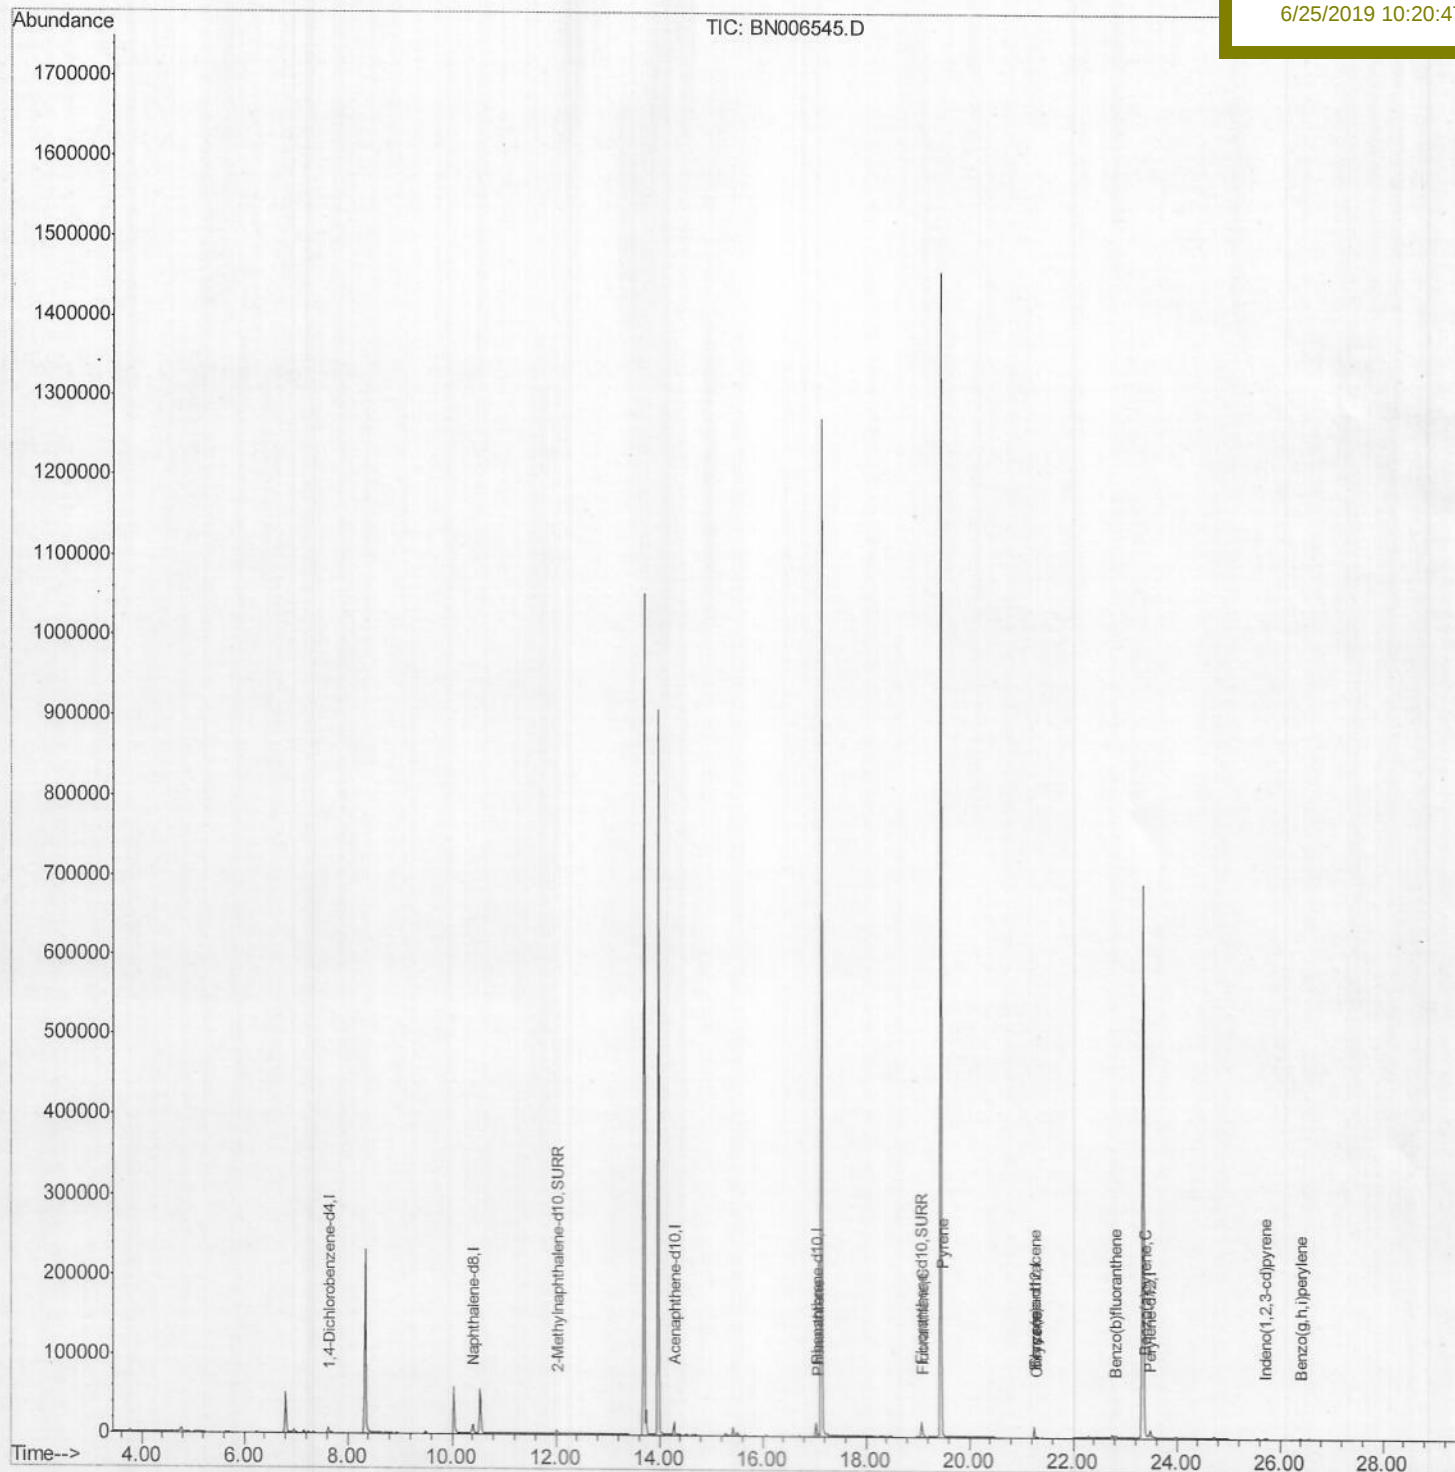

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006545.D

Acq On : 24 Jun 2019 23:22

Operator : HP/JU

Sample : K3362-06

Misc :

ALS Vial : 23 Sample Multiplier: 1

Quant Time: Jun 25 00:44:59 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N




ClientSampleId :

A41X5

Manual Integrations
APPROVED

mohammad

6/25/2019 10:20:47 PM

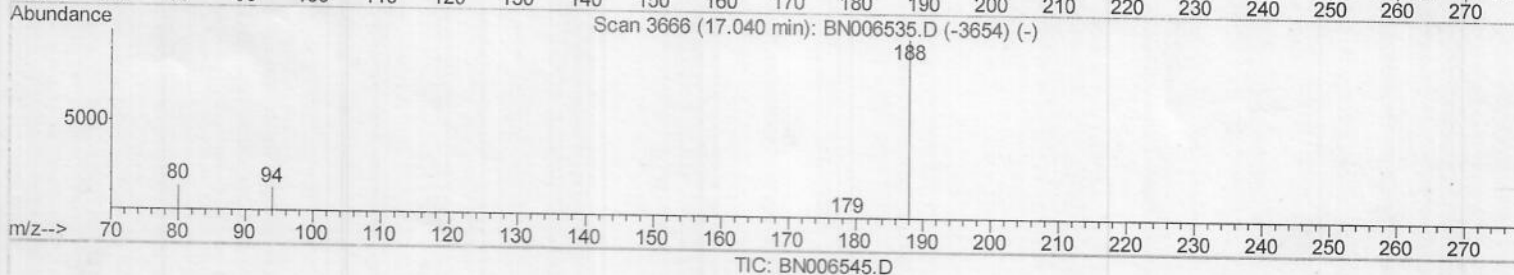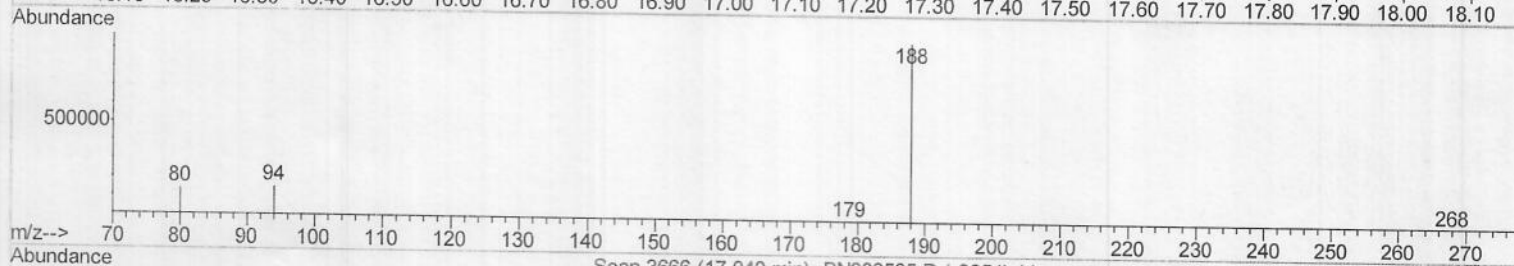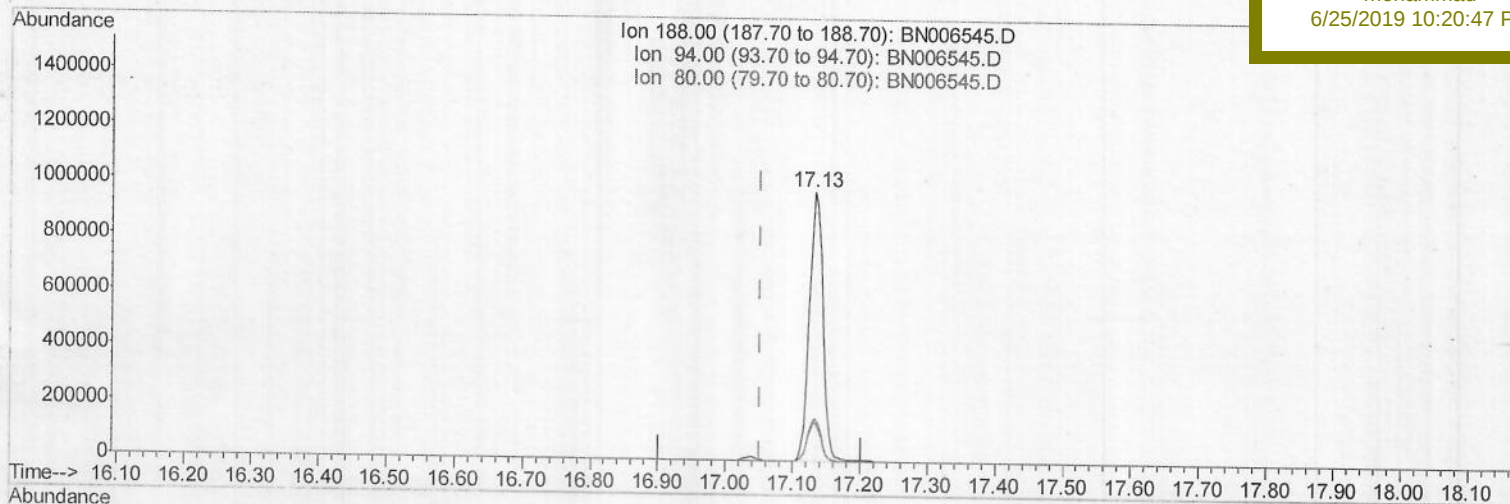

(10) Phenanthrene-d10 (I)

17.133min (+0.080) 0.40ng/ul

response 1350248

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	15.99#
80.00	13.60	14.58
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006545.D

Acq On : 24 Jun 2019 23:22

Operator : HP/JU

Sample : K3362-06

Misc :

ALS Vial : 23 Sample Multiplier: 1

Quant Time: Jun 25 00:44:59 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N




ClientSampleId :

A41X5

Manual Integrations
APPROVED

mohammad

6/25/2019 10:20:47 PM

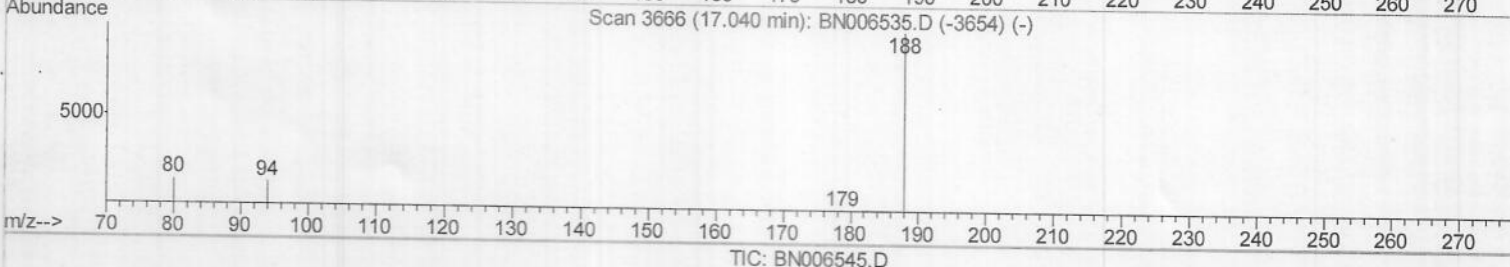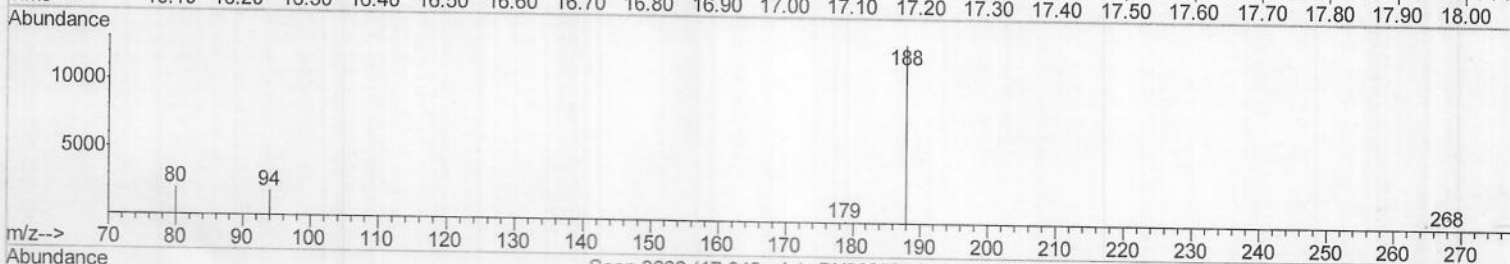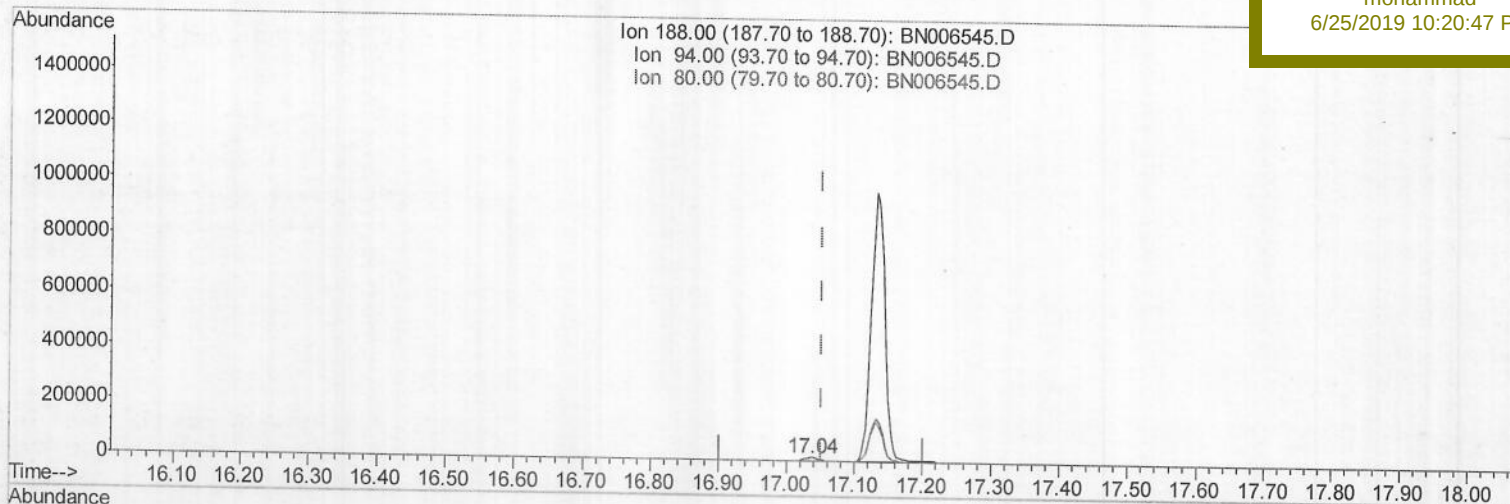

(10) Phenanthrene-d10 (I)

17.036min (-0.017) 0.40ng/ul m

JU
> 06/26/19

response 18899

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	13.72
80.00	13.60	15.17
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006545.D

Acq On : 24 Jun 2019 23:22

Operator : HP/JU

Sample : K3362-06

Misc :

ALS Vial : 23 Sample Multiplier: 1

Quant Time: Jun 25 03:49:18 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019




Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A41X5

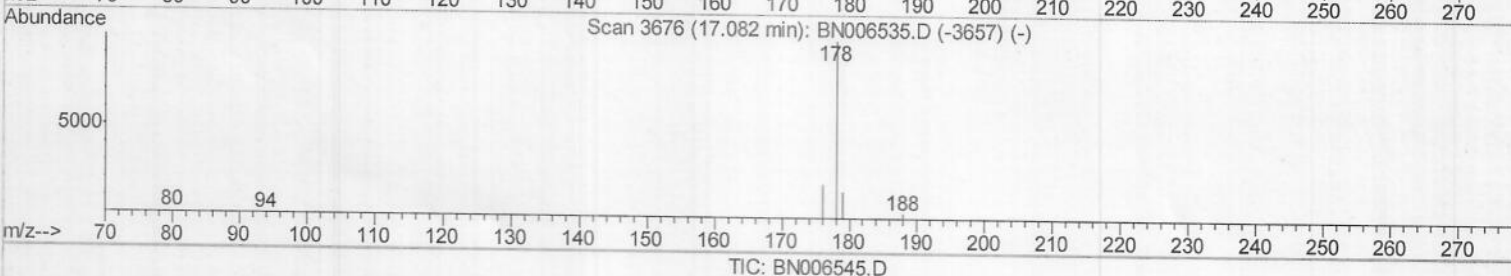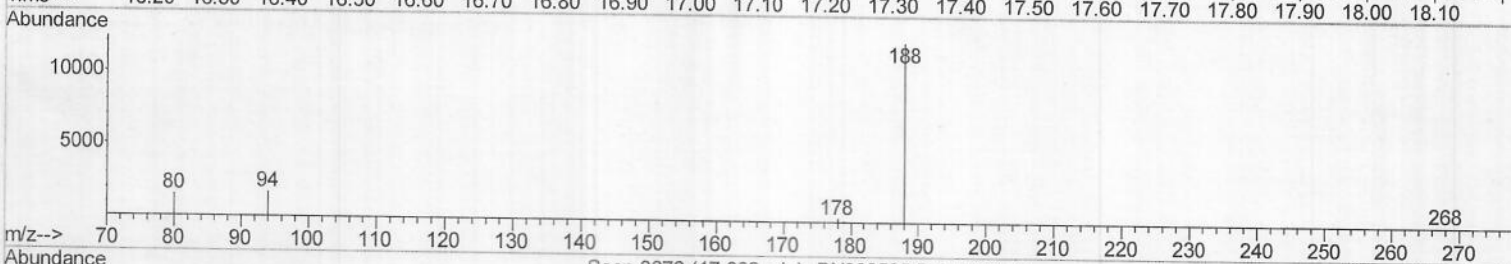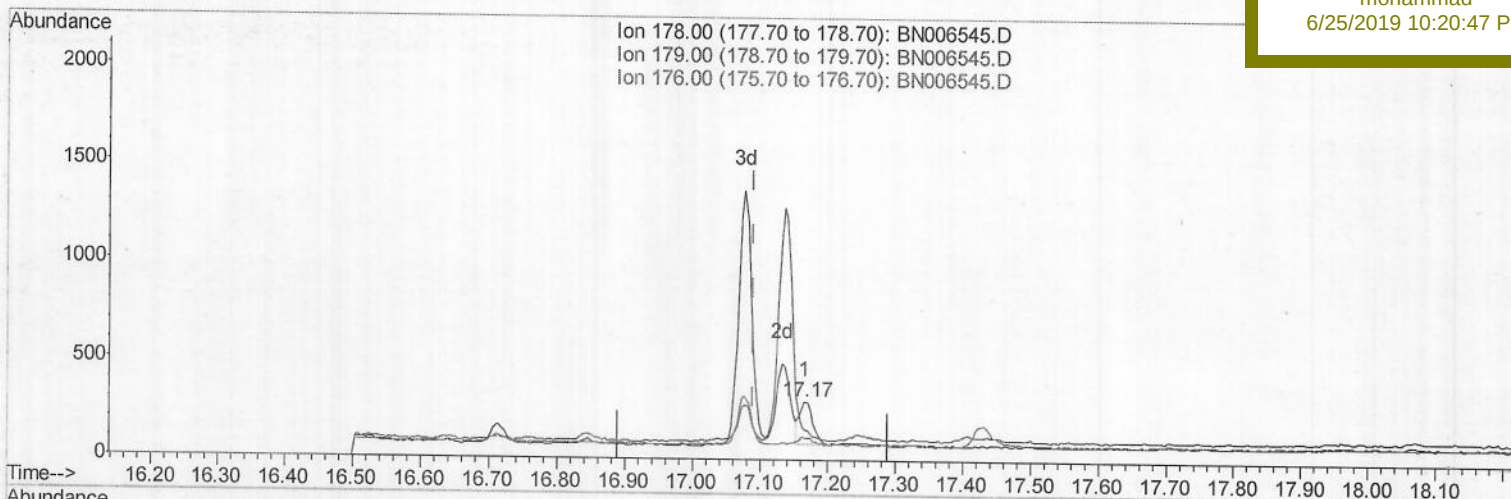Manual Integrations
APPROVEDmohammad
6/25/2019 10:20:47 PM

(12) Phenanthrene

17.166min (+0.076) 0.00ng/ul

response 295

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	51.84#
176.00	19.10	36.79#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006545.D

Acq On : 24 Jun 2019 23:22

Operator : HP/JU

Sample : K3362-06

Misc :

ALS Vial : 23 Sample Multiplier: 1

Quant Time: Jun 25 03:49:18 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019




Response via : Initial Calibration

Instrument :

BNA_N

Client Sampled :

A41X5

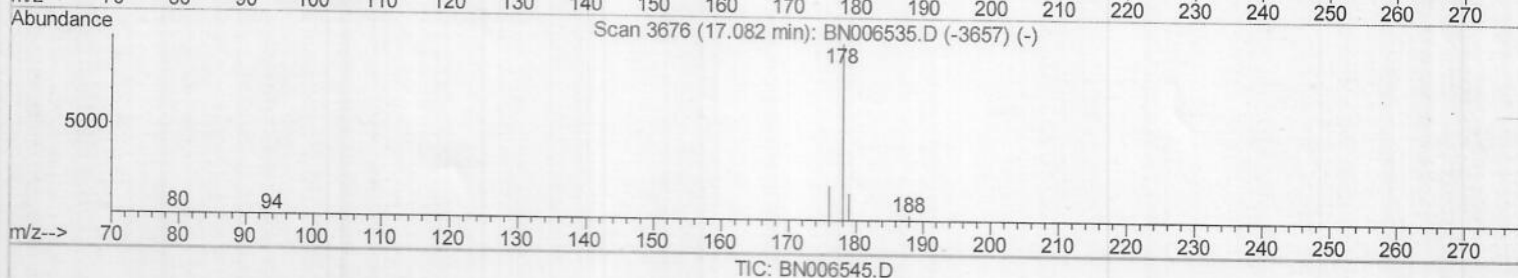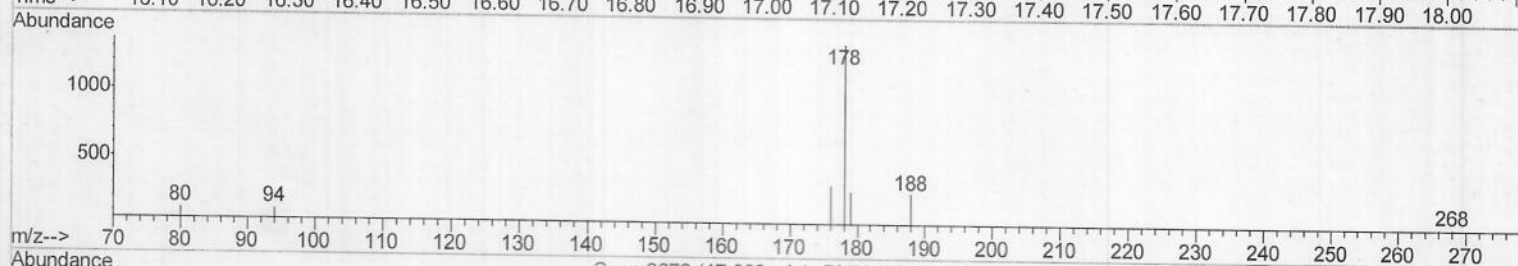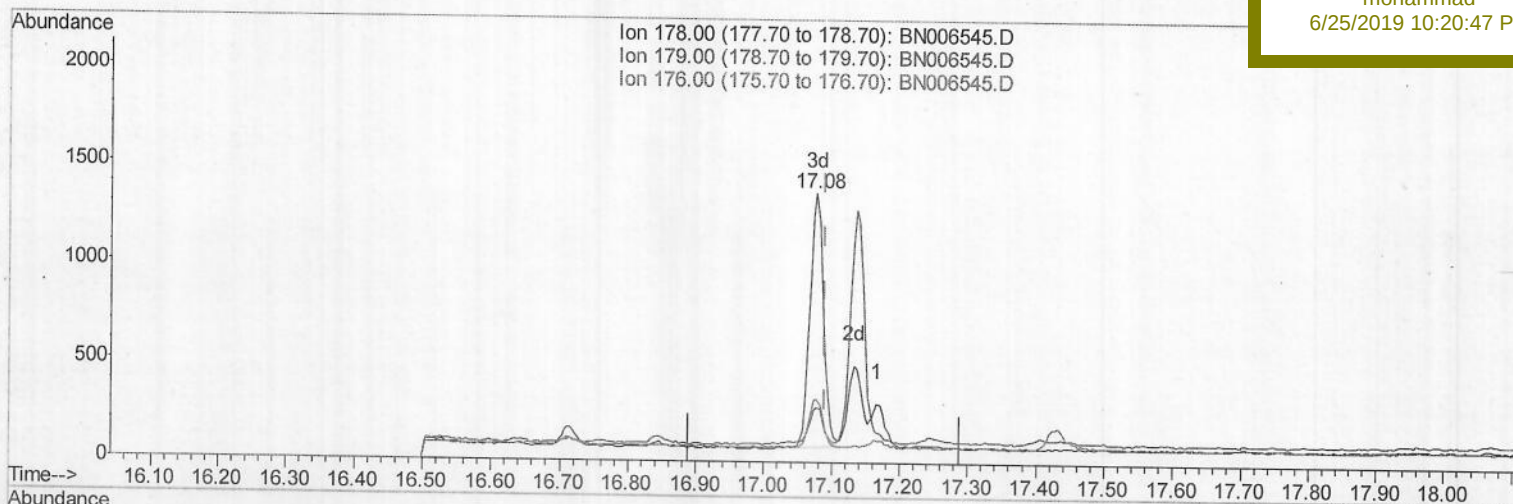Manual Integrations
APPROVEDmohammad
6/25/2019 10:20:47 PM

(12) Phenanthrene

17.078min (-0.013) 0.03ng/ul m

JU
06/26/19

response 1776

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	20.64#
176.00	19.10	23.79#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006545.D

Acq On : 24 Jun 2019 23:22

Operator : HP/JU

Sample : K3362-06

Misc :

ALS Vial : 23 Sample Multiplier: 1

Quant Time: Jun 25 03:49:47 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A41X5

Manual Integrations

APPROVED

mohammad

6/25/2019 10:20:47 PM

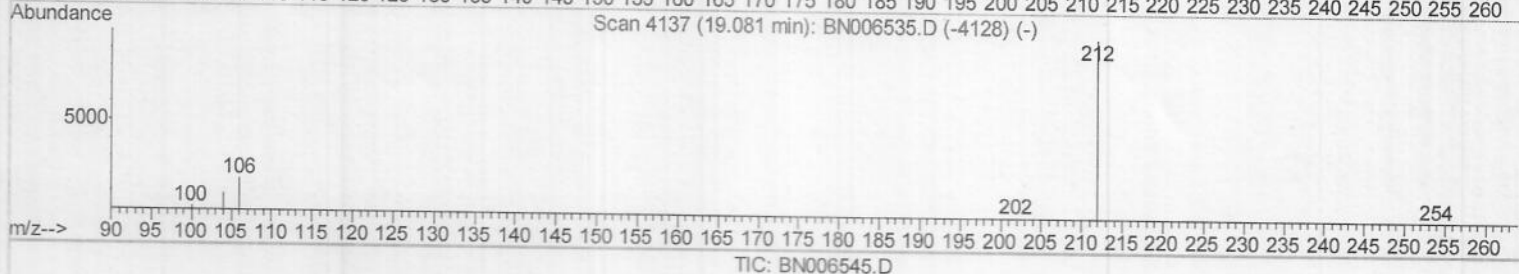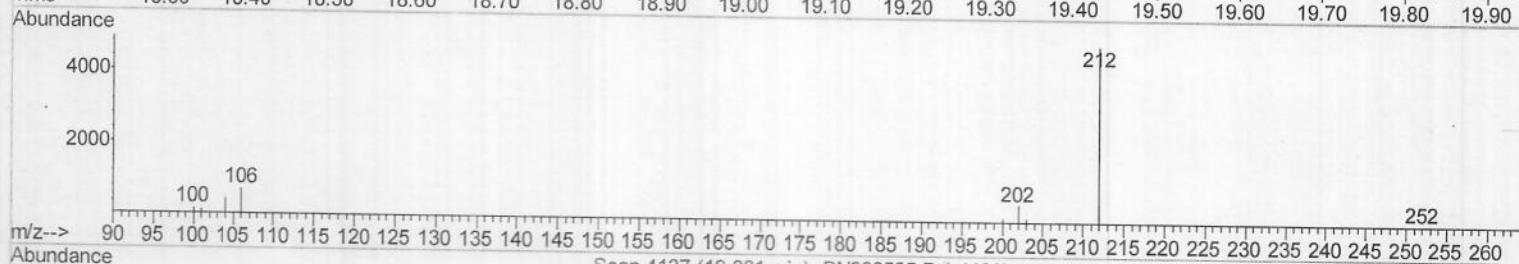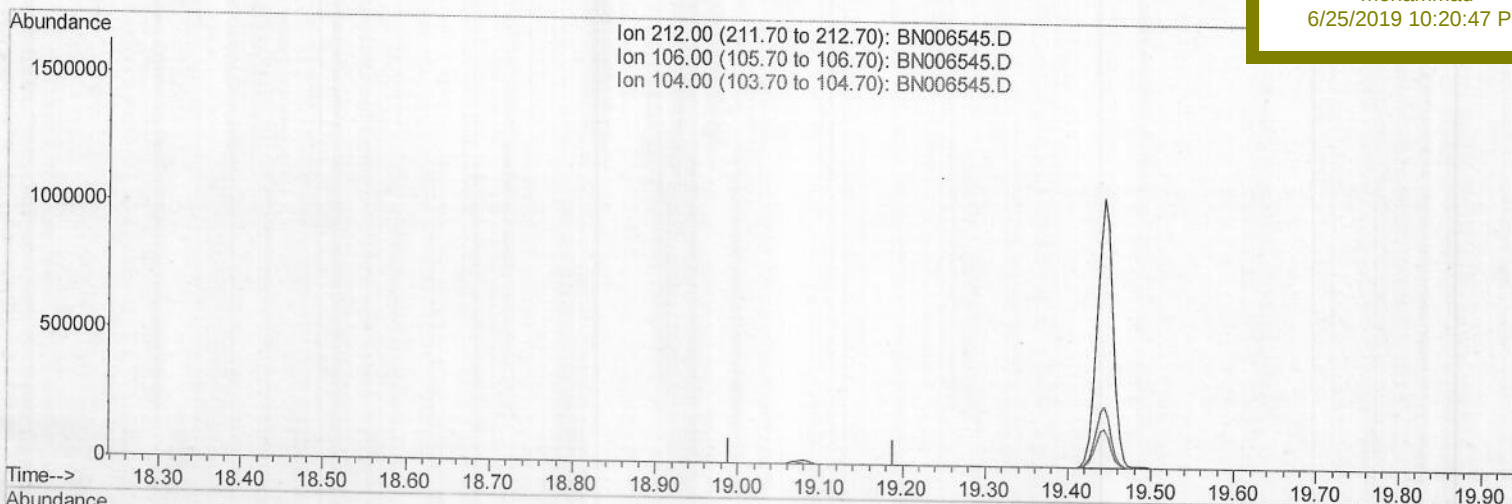

TIC: BN006545.D

(14) Fluoranthene-d10 (SURR)

19.090min (-19.090) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006545.D

Acq On : 24 Jun 2019 23:22

Operator : HP/JU

Sample : K3362-06

Misc :

ALS Vial : 23 Sample Multiplier: 1

Quant Time: Jun 25 03:49:47 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A41X5

Manual Integrations

APPROVED

mohammad

6/25/2019 10:20:47 PM

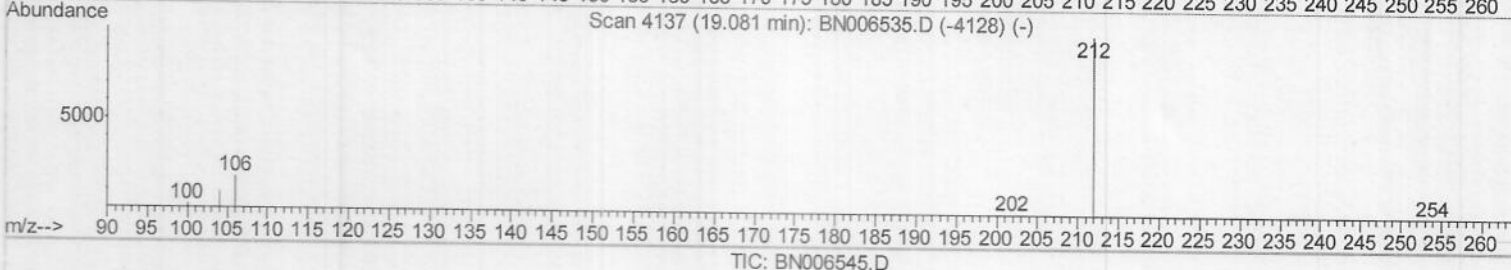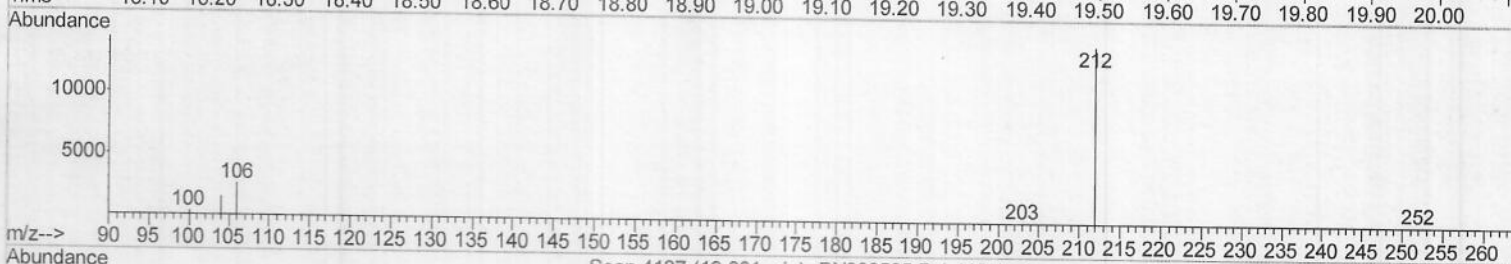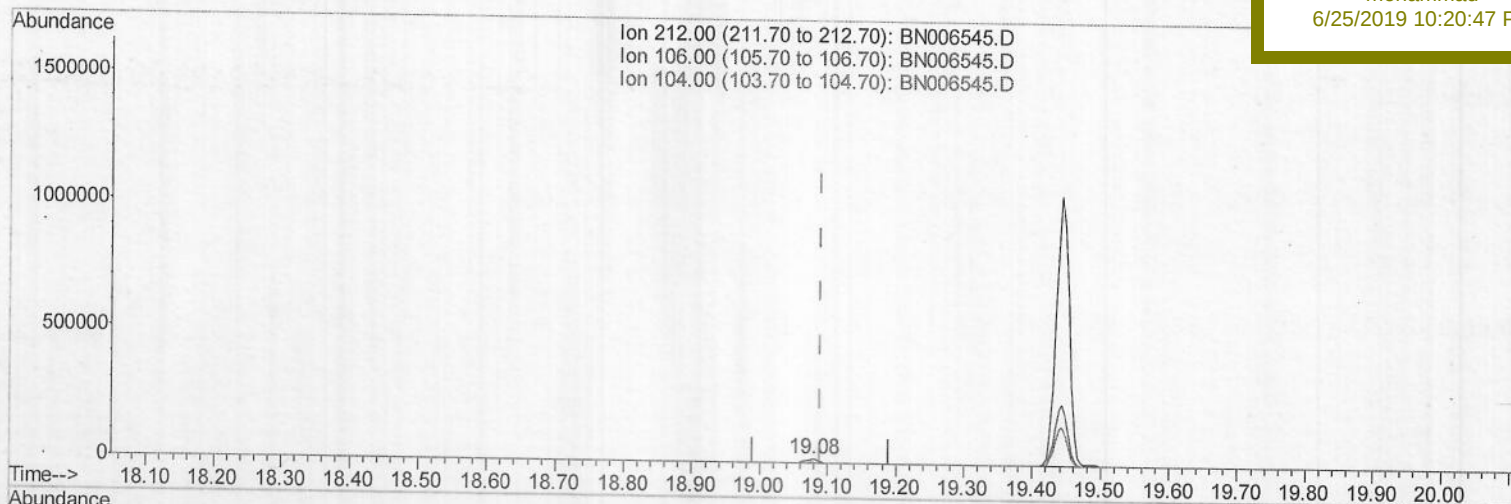

(14) Fluoranthene-d10 (SURR)

19.076min (-0.014) 0.39ng/ul m

response 19918

Ion	Exp%	Act%
212.00	100	100
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00

JU
06/26/19

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006545.D

Acq On : 24 Jun 2019 23:22

Operator : HP/JU

Sample : K3362-06

Misc :

ALS Vial : 23 Sample Multiplier: 1

Quant Time: Jun 25 03:49:47 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A41X5

Manual Integrations

APPROVED

mohammad

6/25/2019 10:20:47 PM

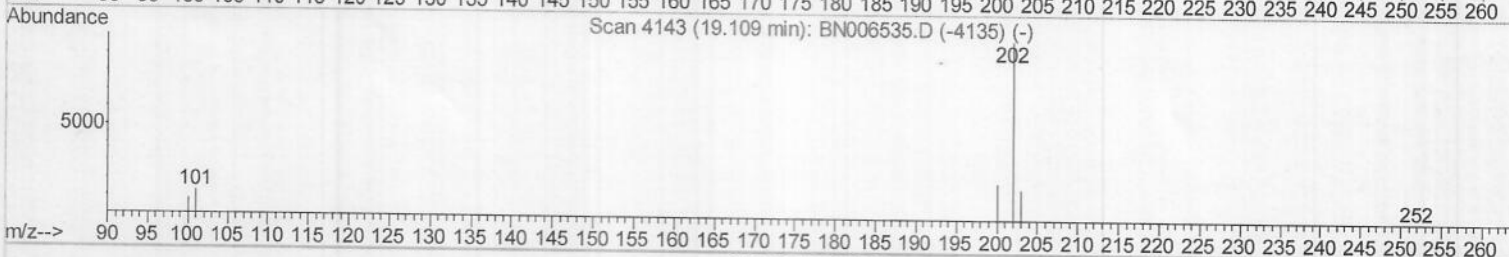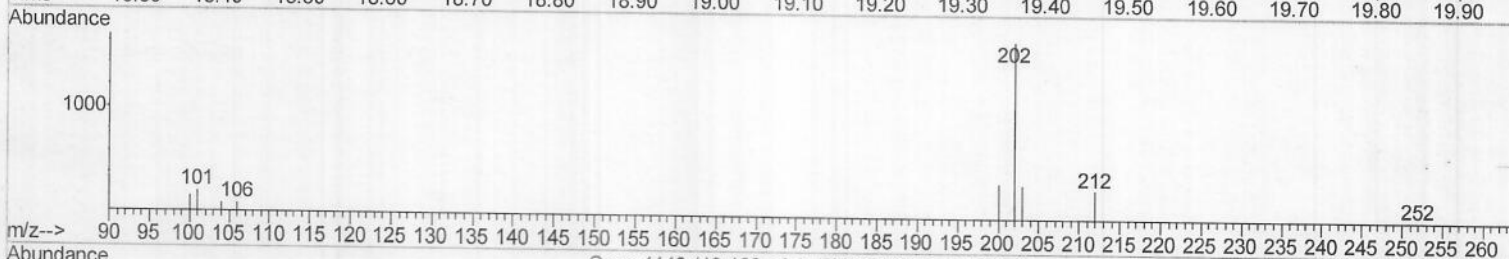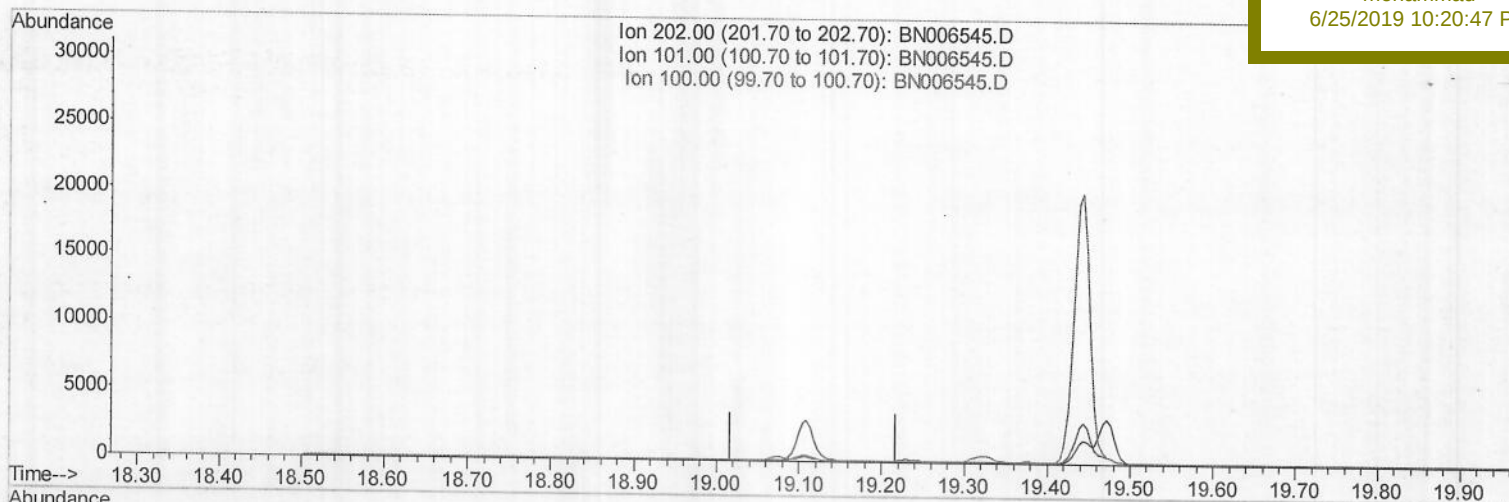

TIC: BN006545.D

(15) Fluoranthene (C)

19.118min (-19.118) 0.00ng/ul

response 0

Ion	Exp%	Act%
202.00	100	0.00
101.00	12.10	0.00
100.00	8.70	0.00
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006545.D
Acq On : 24 Jun 2019 23:22
Operator : HP/JU
Sample : K3362-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Jun 25 03:49:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampled :
A41X5

Manual Integrations
APPROVED

mohammad
6/25/2019 10:20:47 PM

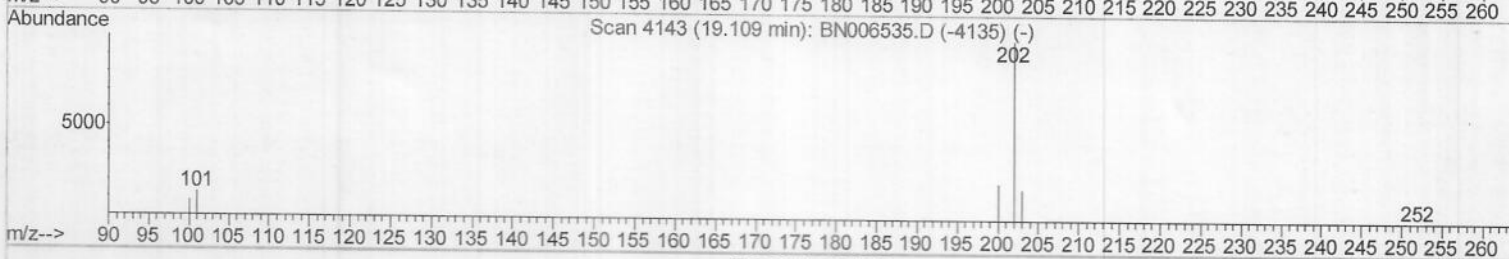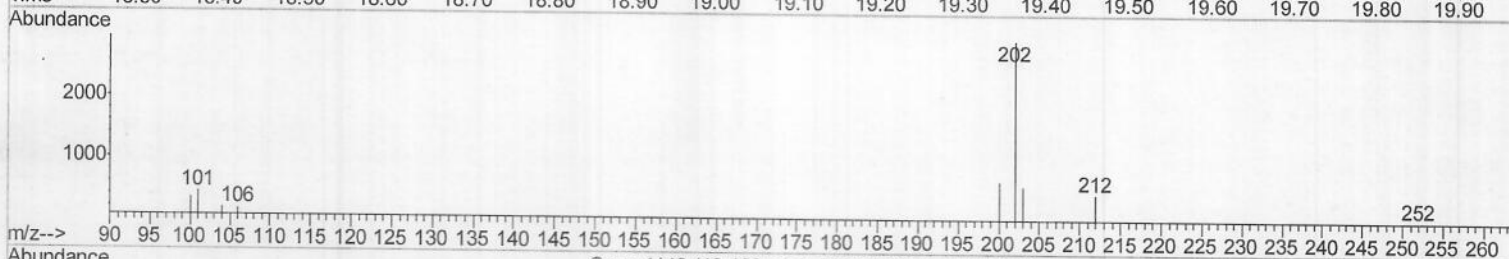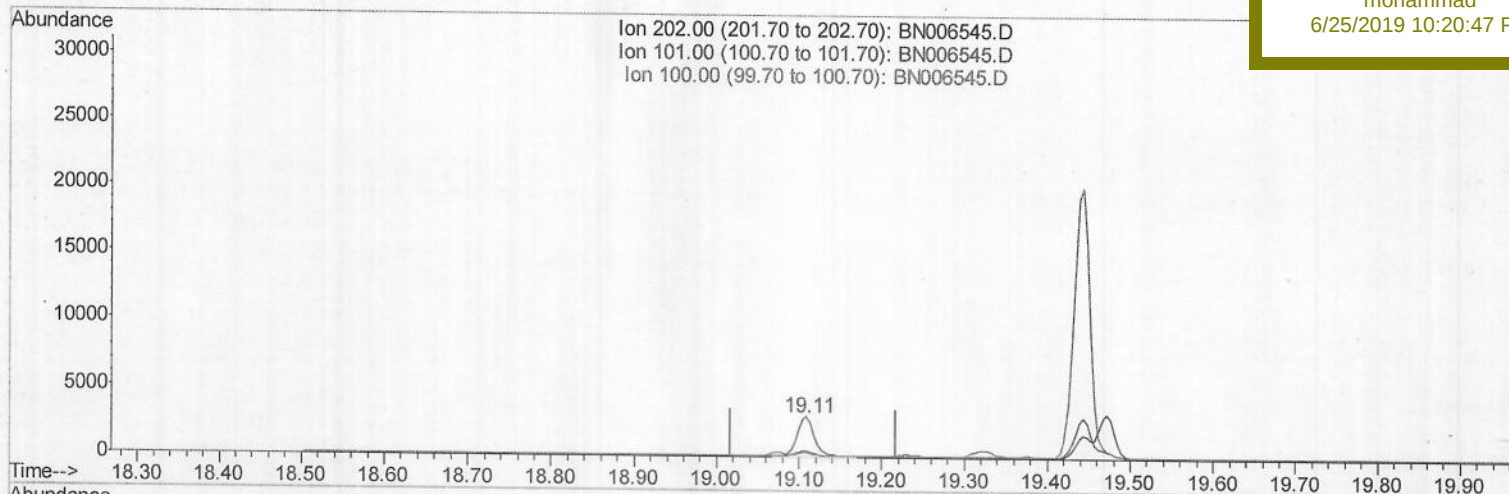

TIC: BN006545.D

(15) Fluoranthene (C)

19.109min (-0.009) 0.07ng/ul m

response 4674

Ion	Exp%	Act%
202.00	100	100
101.00	12.10	14.40
100.00	8.70	11.32
0.00	0.00	0.00

JU
7 06/26/19

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006545.D

Acq On : 24 Jun 2019 23:22

Operator : HP/JU

Sample : K3362-06

Misc :

ALS Vial : 23 Sample Multiplier: 1

Quant Time: Jun 25 03:49:47 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N




Client Sampled :

A41X5

Manual Integrations
APPROVED

mohammad

6/25/2019 10:20:47 PM

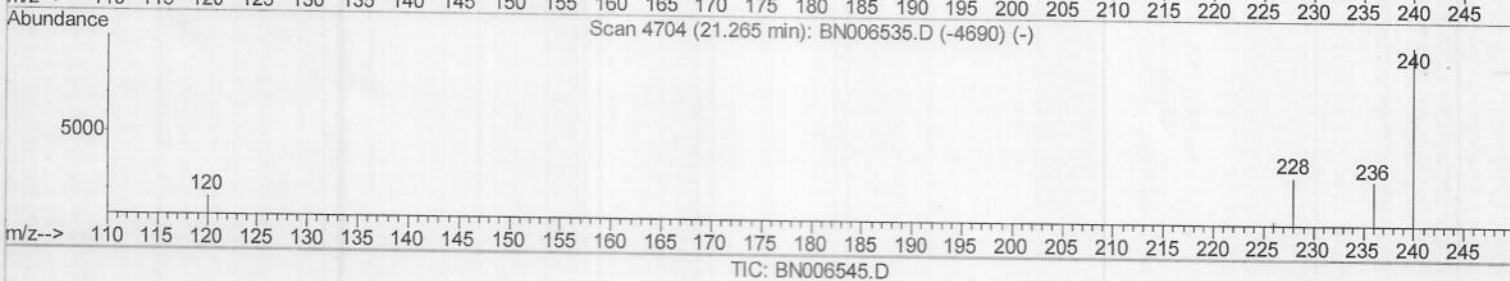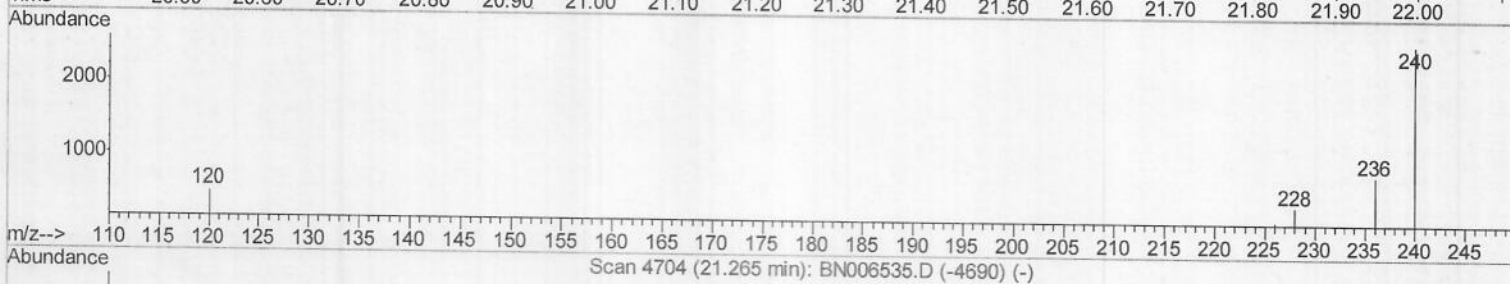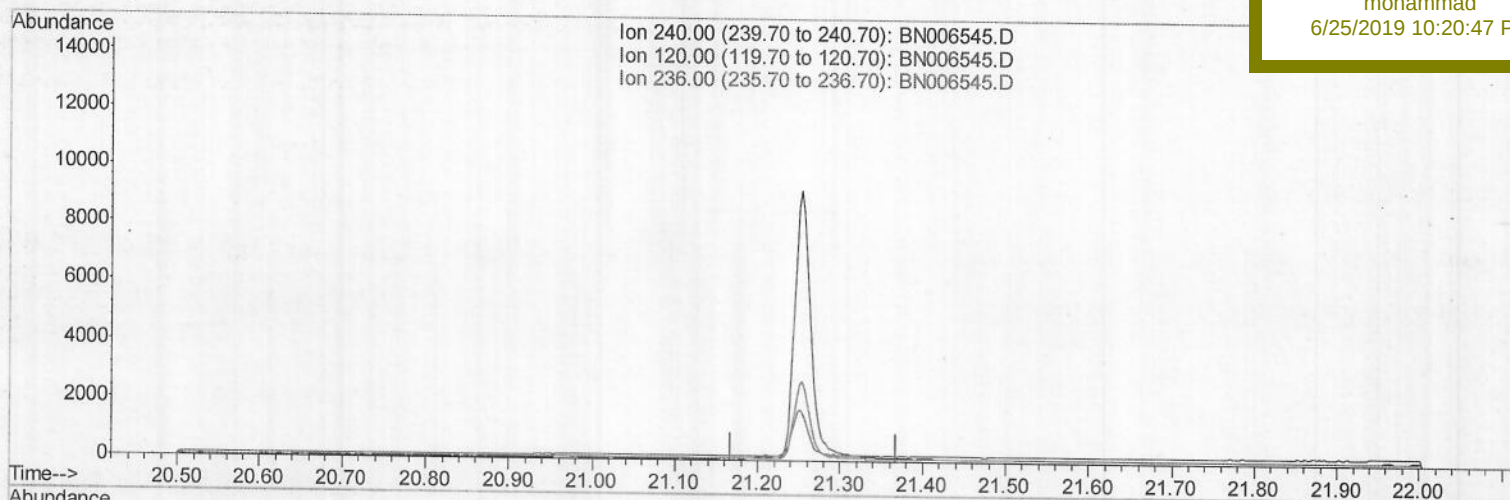

(16) Chrysene-d12 (I)

21.268min (-21.268) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	20.10	0.00#
236.00	30.10	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006545.D

Acq On : 24 Jun 2019 23:22

Operator : HP/JU

Sample : K3362-06

Misc :

ALS Vial : 23 Sample Multiplier: 1

Quant Time: Jun 25 03:49:47 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N




ClientSampleId :

A41X5

Manual Integrations
APPROVED

mohammad

6/25/2019 10:20:47 PM

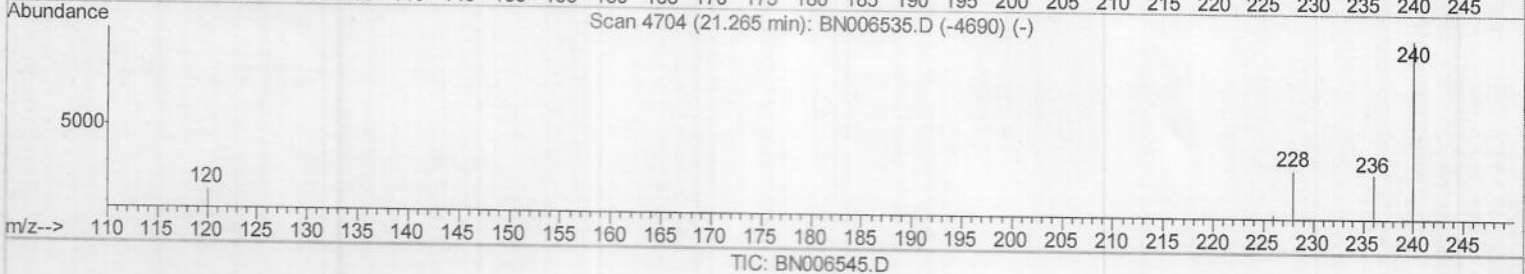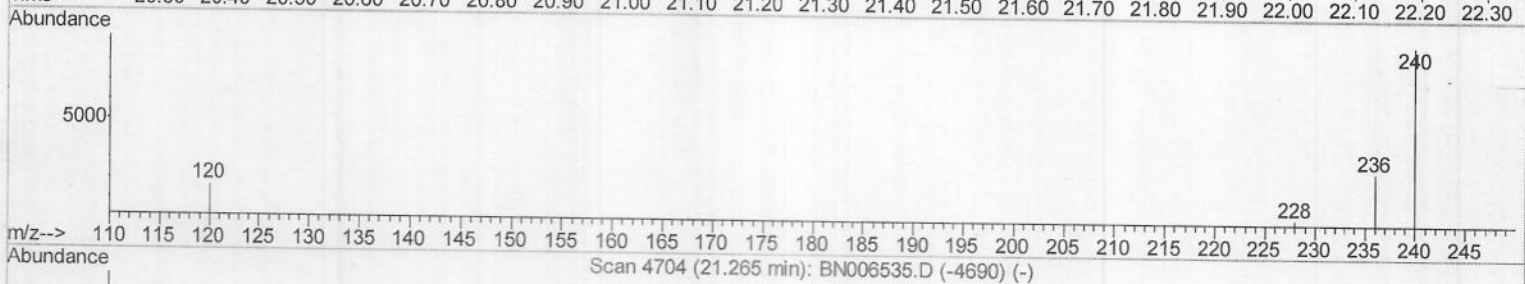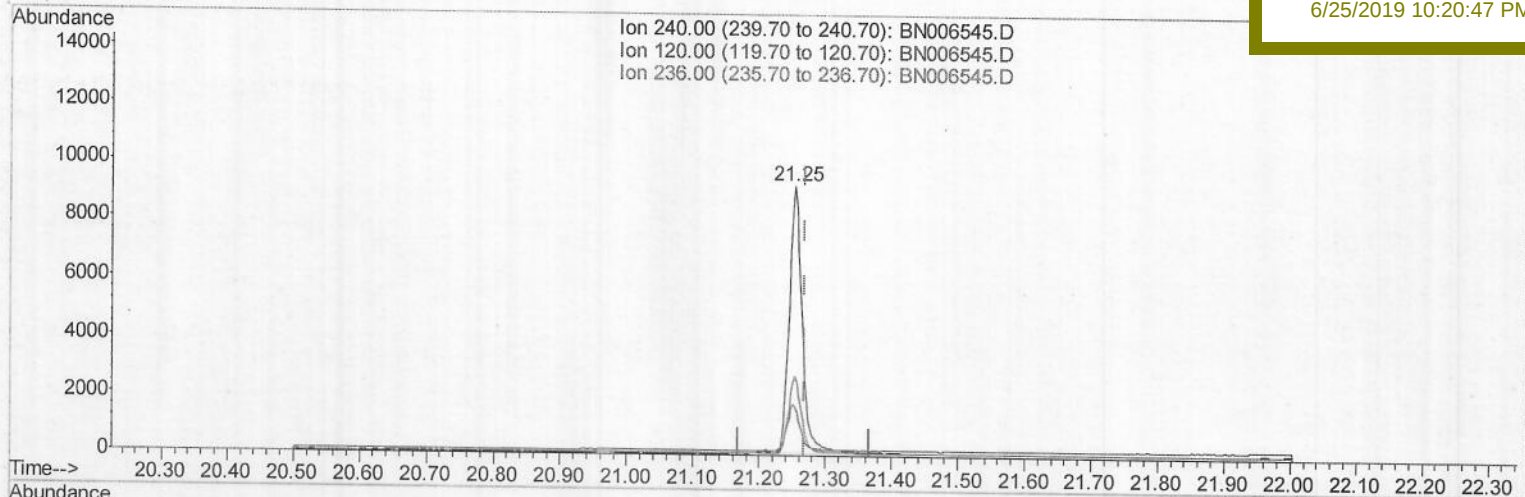

(16) Chrysene-d12 (I)

21.254min (-0.014) 0.40ng/ul m

response 12624

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	18.08
236.00	30.10	29.72
0.00	0.00	0.00

S JU 06/26/19

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006545.D

Acq On : 24 Jun 2019 23:22

Operator : HP/JU

Sample : K3362-06

Misc :

ALS Vial : 23 Sample Multiplier: 1

Quant Time: Jun 25 03:50:53 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A41X5

Manual Integrations

APPROVED

mohammad

6/25/2019 10:20:47 PM

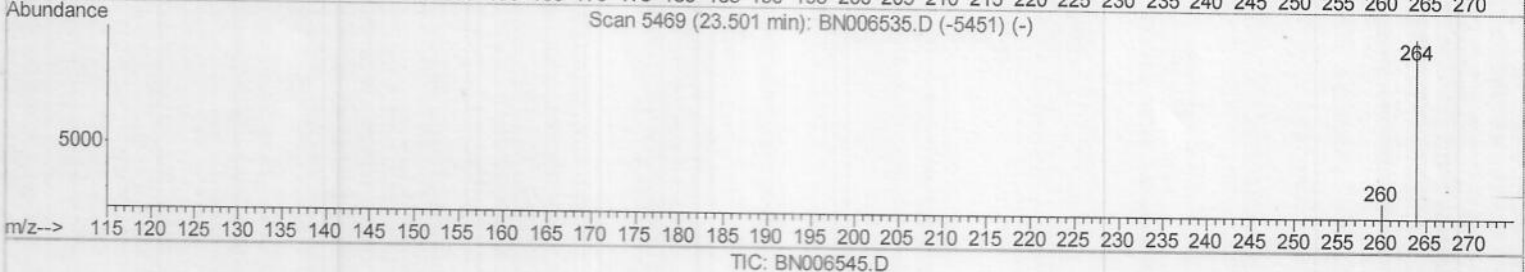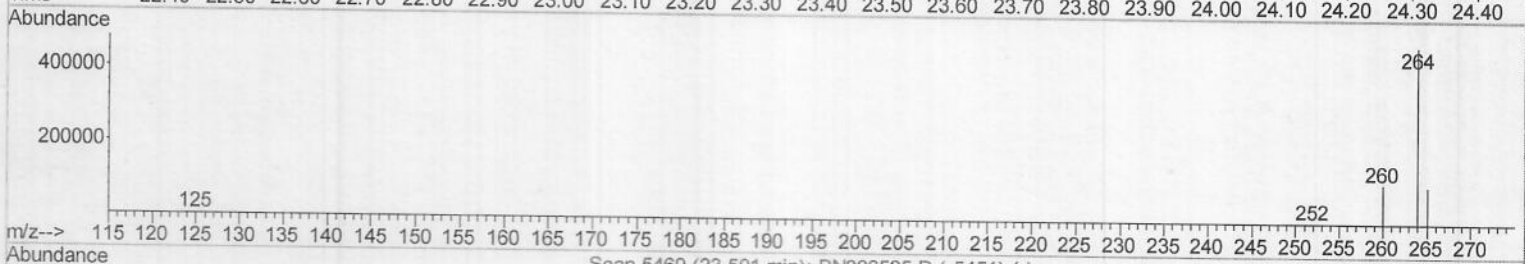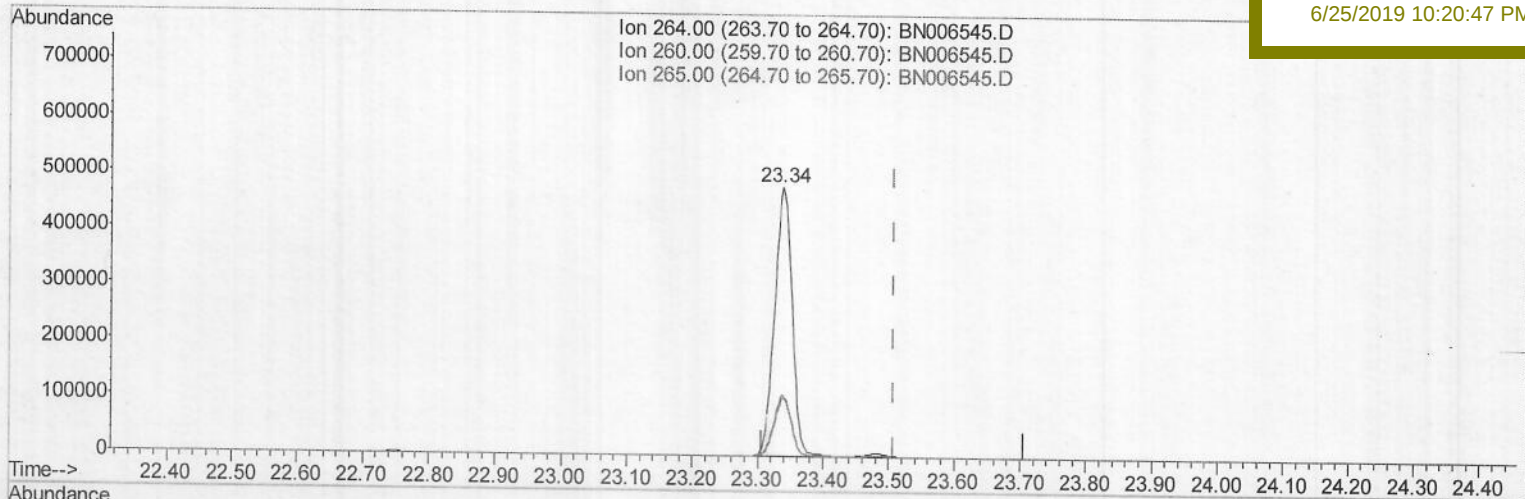

(20) Perylene-d12 (I)

23.338min (-0.169) 0.40ng/ul

response 865309

Ion	Exp%	Act%
264.00	100	100
260.00	29.20	22.67#
265.00	44.70	21.29#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006545.D

Acq On : 24 Jun 2019 23:22

Operator : HP/JU

Sample : K3362-06

Misc :

ALS Vial : 23 Sample Multiplier: 1

Quant Time: Jun 25 03:50:53 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N




ClientSampleId :

A41X5

Manual Integrations
APPROVED

mohammad

6/25/2019 10:20:47 PM

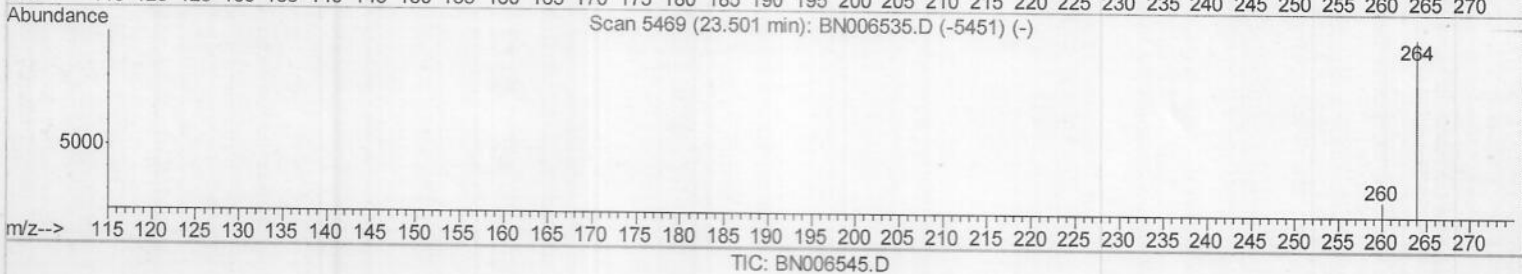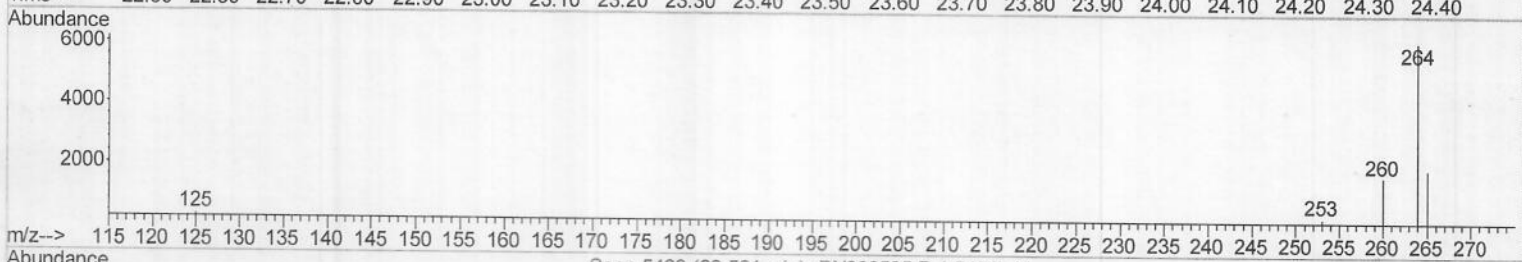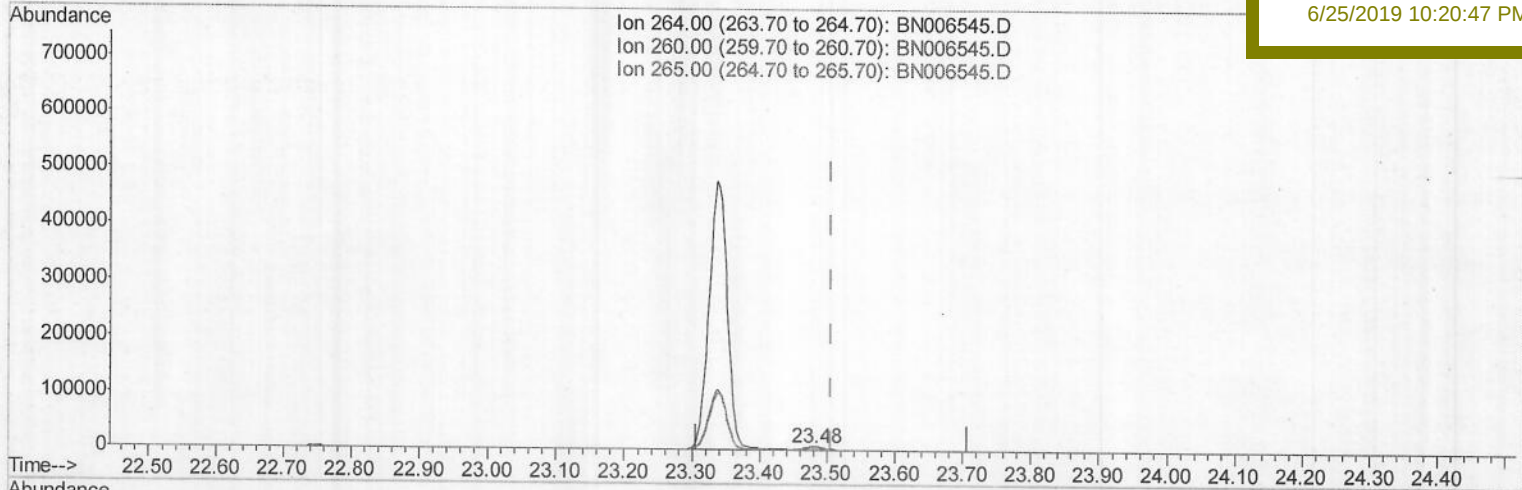

(20) Perylene-d12 (I)

23.481min (-0.026) 0.40ng/ul m

response 9223

Ion	Exp%	Act%
264.00	100	100
260.00	29.20	27.59
265.00	44.70	31.85#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006545.D

Acq On : 24 Jun 2019 23:22

Operator : HP/JU

Sample : K3362-06

Misc :

ALS Vial : 23 Sample Multiplier: 1

Quant Time: Jun 25 03:51:32 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A41X5

Manual Integrations

APPROVED

mohammad

6/25/2019 10:20:47 PM

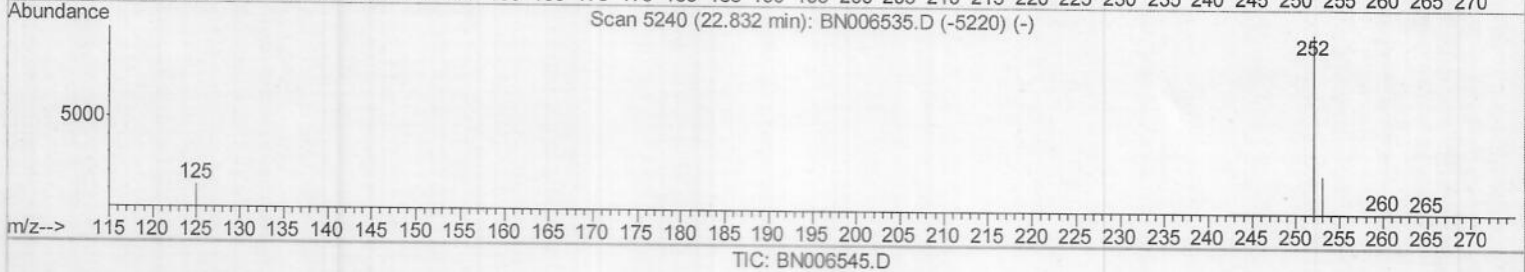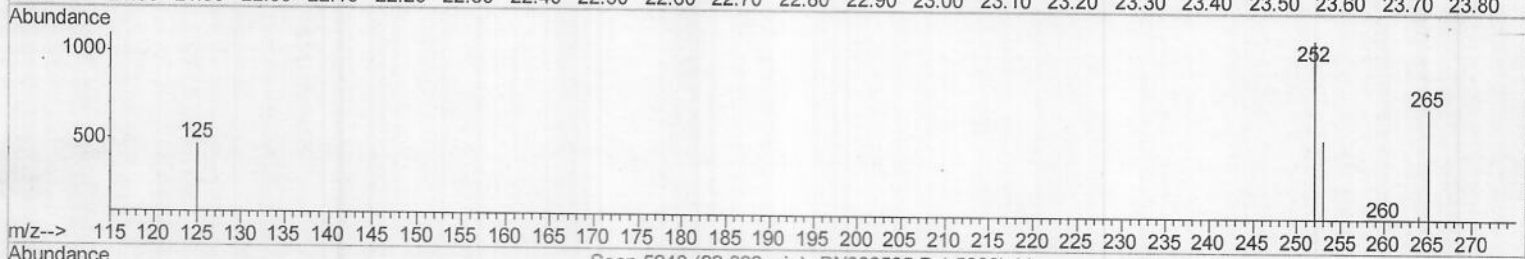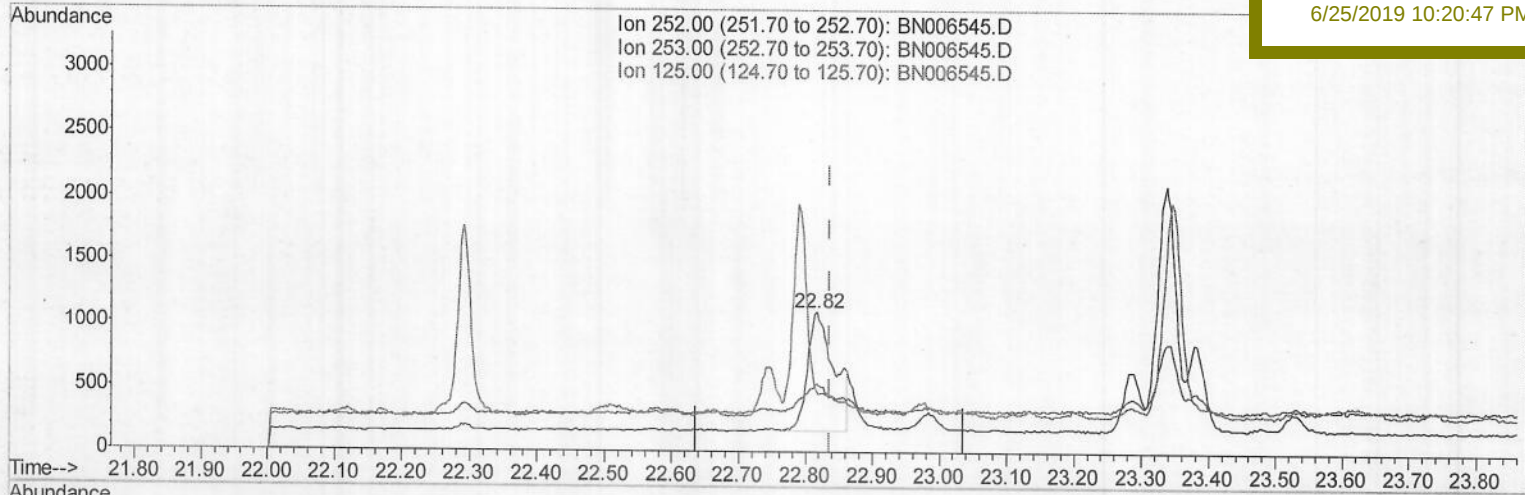

(21) Benzo(b)fluoranthene

22.817min (-0.020) 0.07ng/ul

response 2513

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	48.54
125.00	20.50	42.69#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
 Data File : BN006545.D
 Acq On : 24 Jun 2019 23:22
 Operator : HP/JU
 Sample : K3362-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Quant Time: Jun 25 03:51:32 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 A41X5

Manual Integrations
 APPROVED

mohammad
 6/25/2019 10:20:47 PM

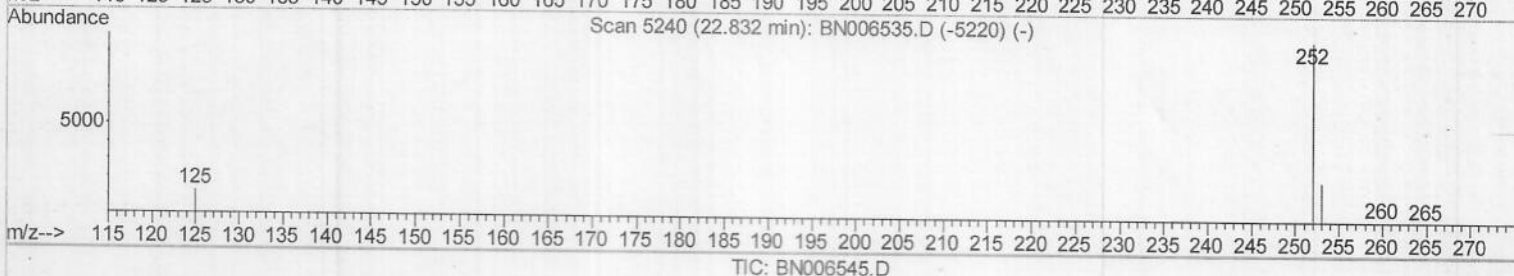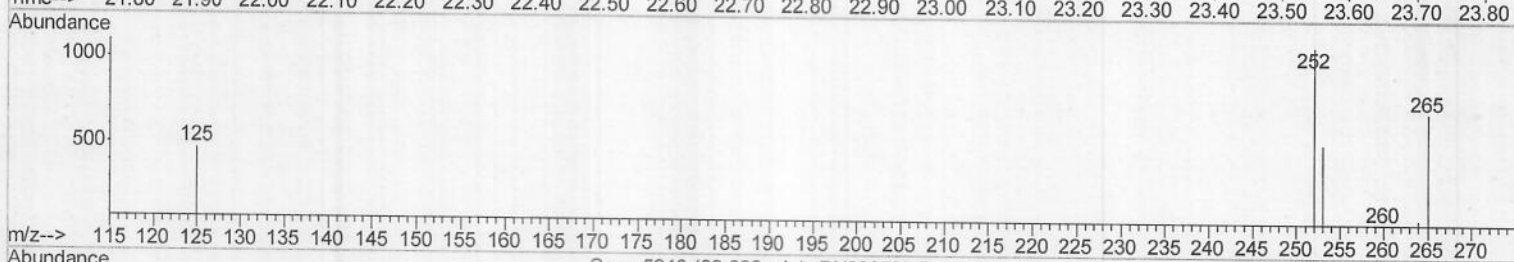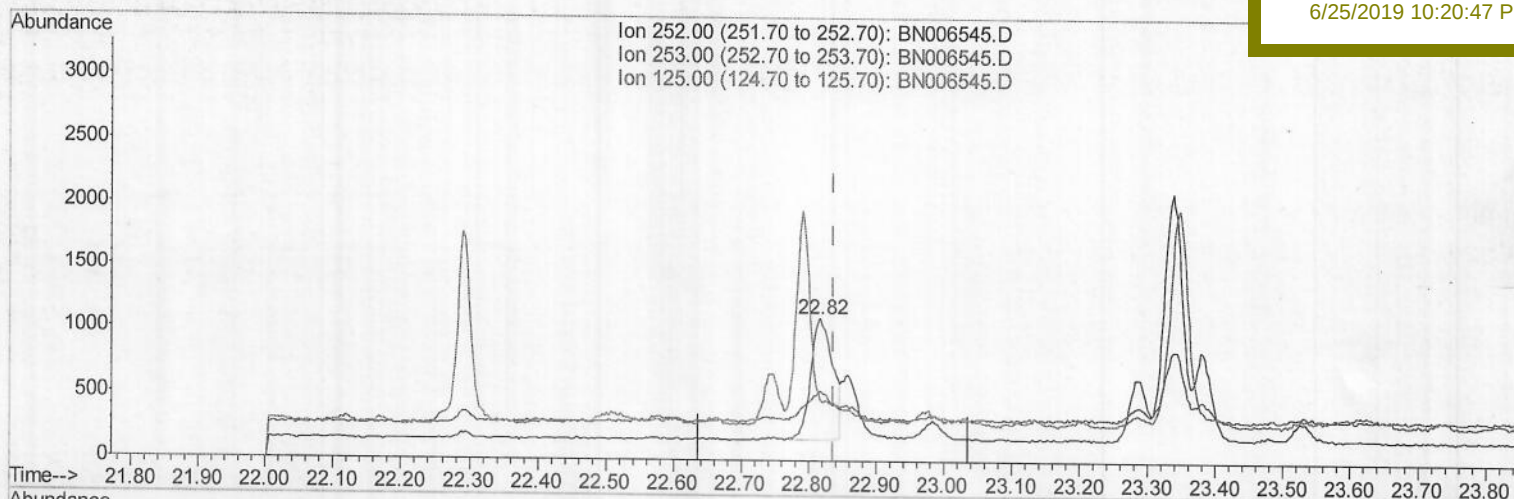

(21) Benzo(b)fluoranthene

22.817min (-0.020) 0.05ng/ul m

response 2089

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	48.54
125.00	20.50	42.69#
0.00	0.00	0.00

Y JU 06/26/19

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006545.D

Acq On : 24 Jun 2019 23:22

Operator : HP/JU

Sample : K3362-06

Misc :

ALS Vial : 23 Sample Multiplier: 1

Quant Time: Jun 25 03:52:00 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

Client Sampled :




A41X5

Manual Integrations

APPROVED

mohammad

6/25/2019 10:20:47 PM

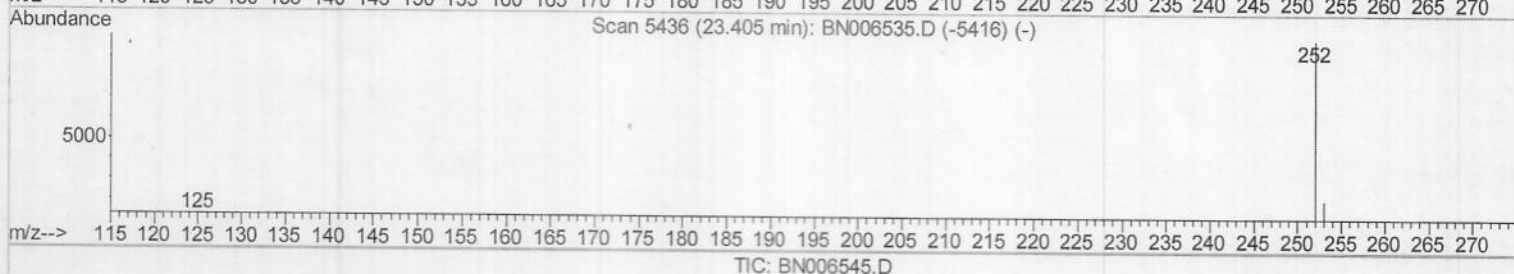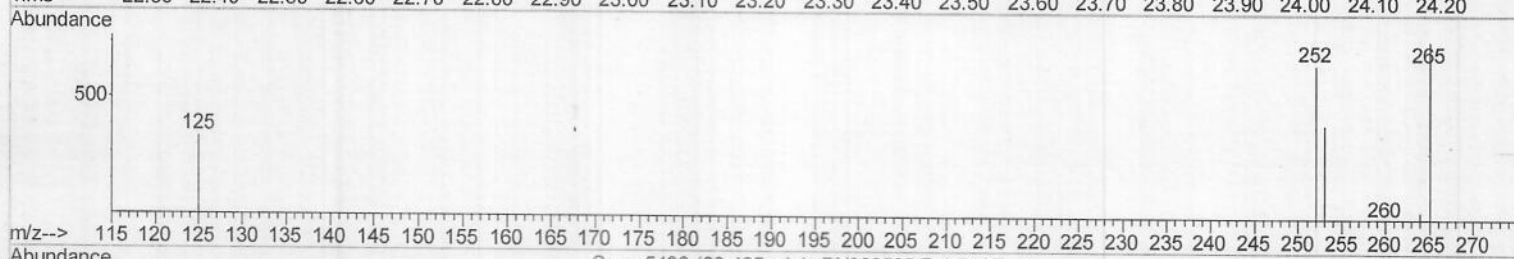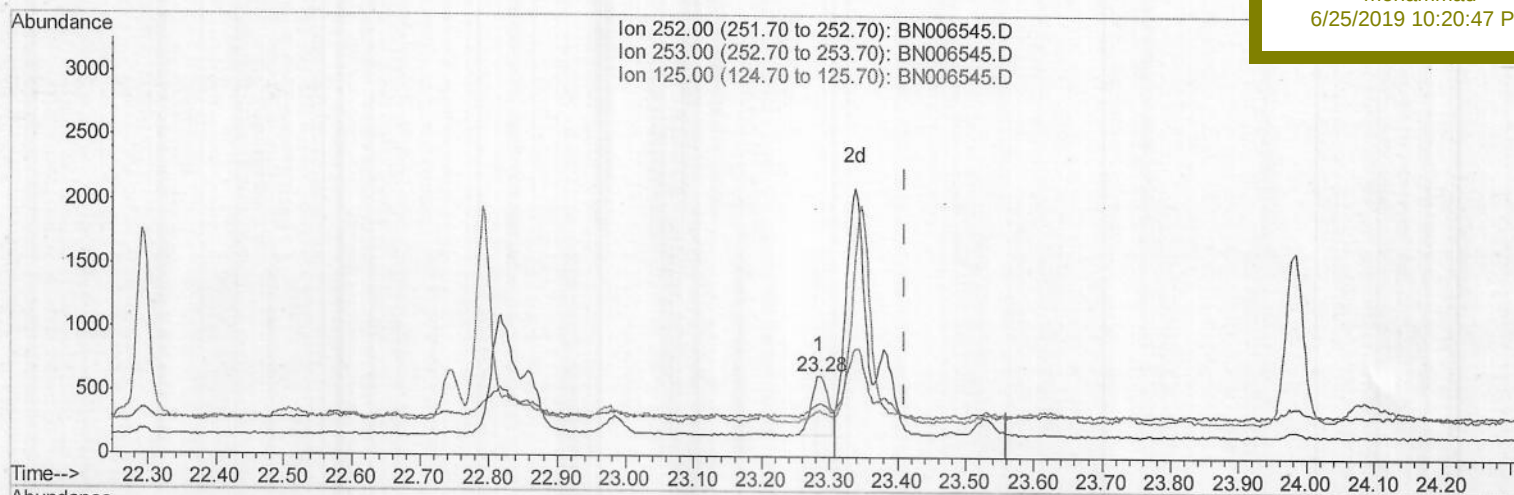

(23) Benzo(a)pyrene (C)

23.285min (-0.126) 0.02ng/ul

response 820

Ion	Exp%	Act%
252.00	100	100
253.00	26.40	65.62#
125.00	25.40	56.62#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006545.D

Acq On : 24 Jun 2019 23:22

Operator : HP/JU

Sample : K3362-06

Misc :

ALS Vial : 23 Sample Multiplier: 1

Quant Time: Jun 25 03:52:00 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

Client Sampled :




A41X5

Manual Integrations

APPROVED

mohammad

6/25/2019 10:20:47 PM

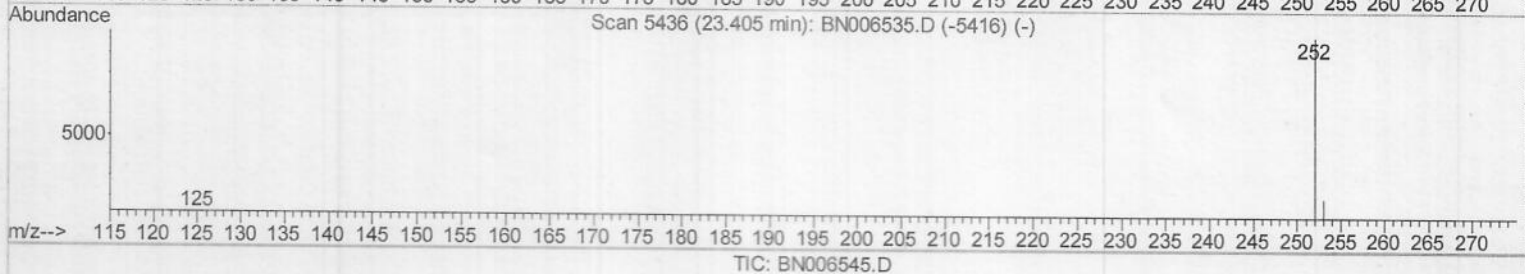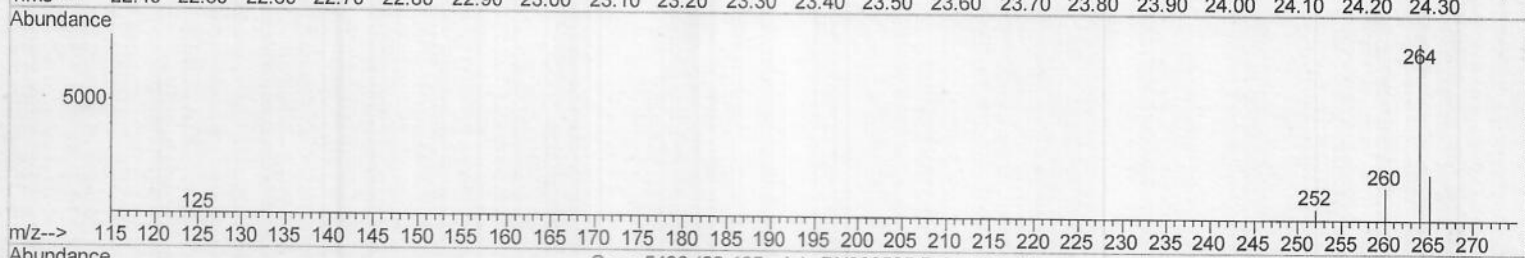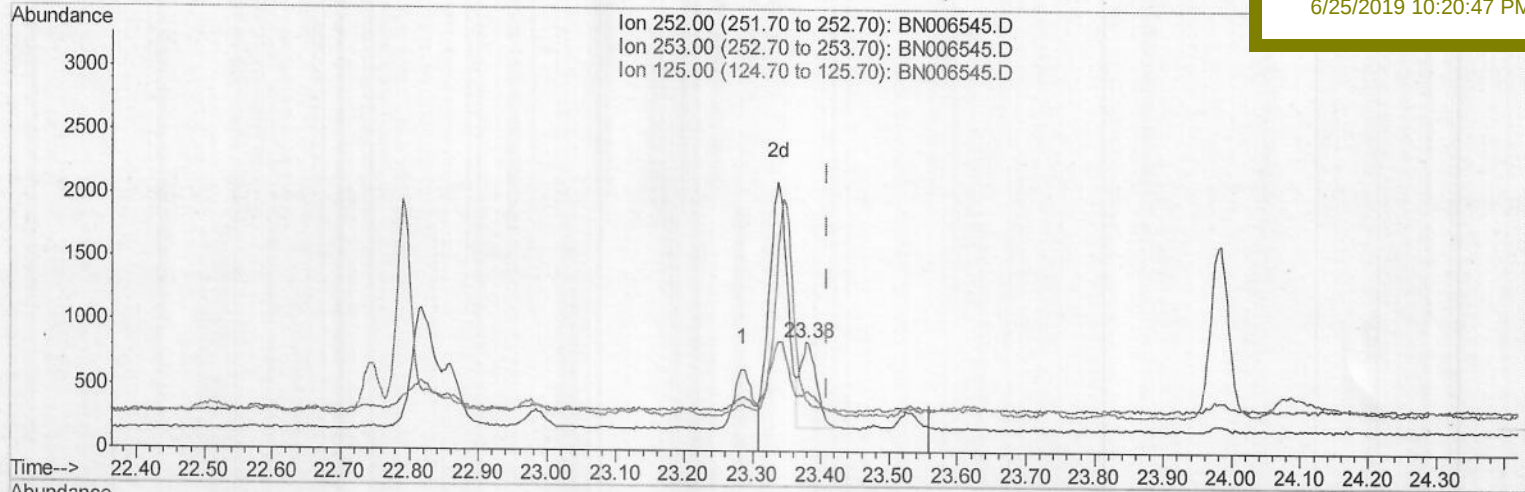

TIC: BN006545.D

(23) Benzo(a)pyrene (C)

23.378min (-0.032) 0.03ng/ul m

response 1104

Ion	Exp%	Act%
252.00	100	100
253.00	26.40	55.73#
125.00	25.40	47.34#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006545.D

Acq On : 24 Jun 2019 23:22

Operator : HP/JU

Sample : K3362-06

Misc :

ALS Vial : 23 Sample Multiplier: 1

Quant Time: Jun 25 03:52:00 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A41X5

Manual Integrations

APPROVED

mohammad

6/25/2019 10:20:47 PM

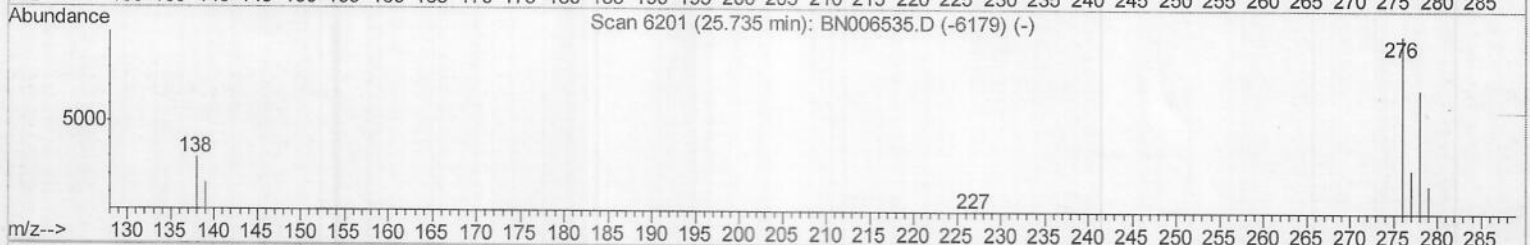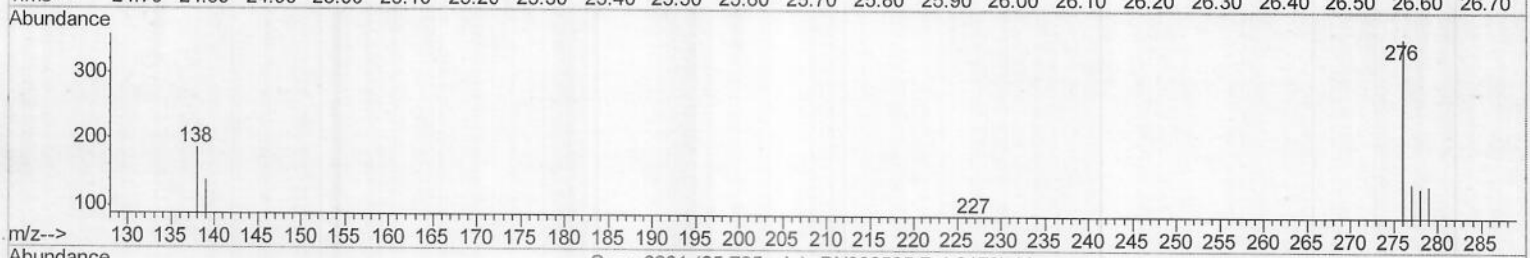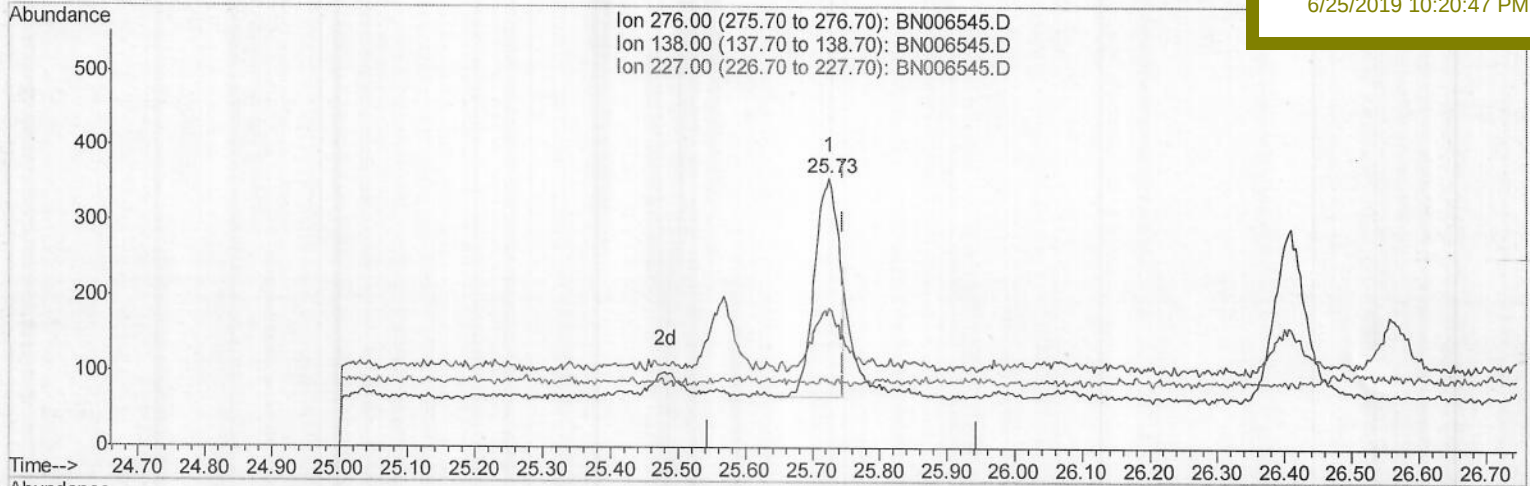

(24) Indeno(1,2,3-cd)pyrene

25.725min (-0.020) 0.02ng/ul

response 722

Ion	Exp%	Act%
276.00	100	100
138.00	32.00	28.39
227.00	0.40	0.42
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006545.D

Acq On : 24 Jun 2019 23:22

Operator : HP/JU

Sample : K3362-06

Misc :

ALS Vial : 23 Sample Multiplier: 1

Quant Time: Jun 25 03:52:00 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A41X5

Manual Integrations

APPROVED

mohammad

6/25/2019 10:20:47 PM

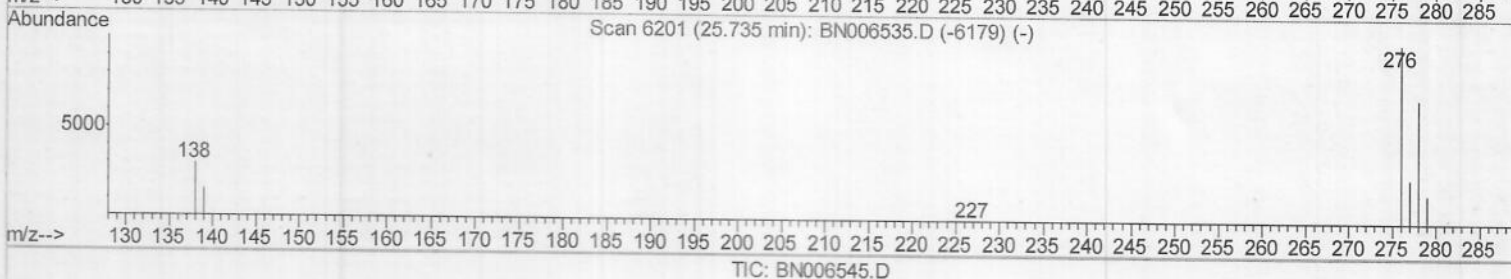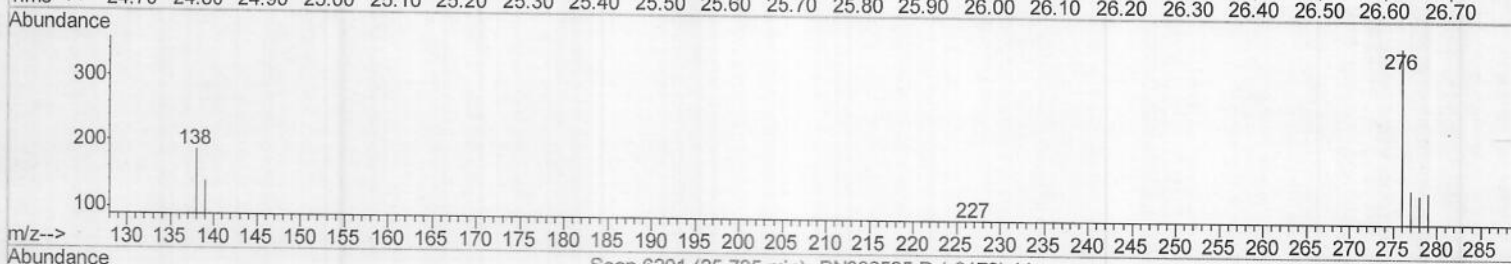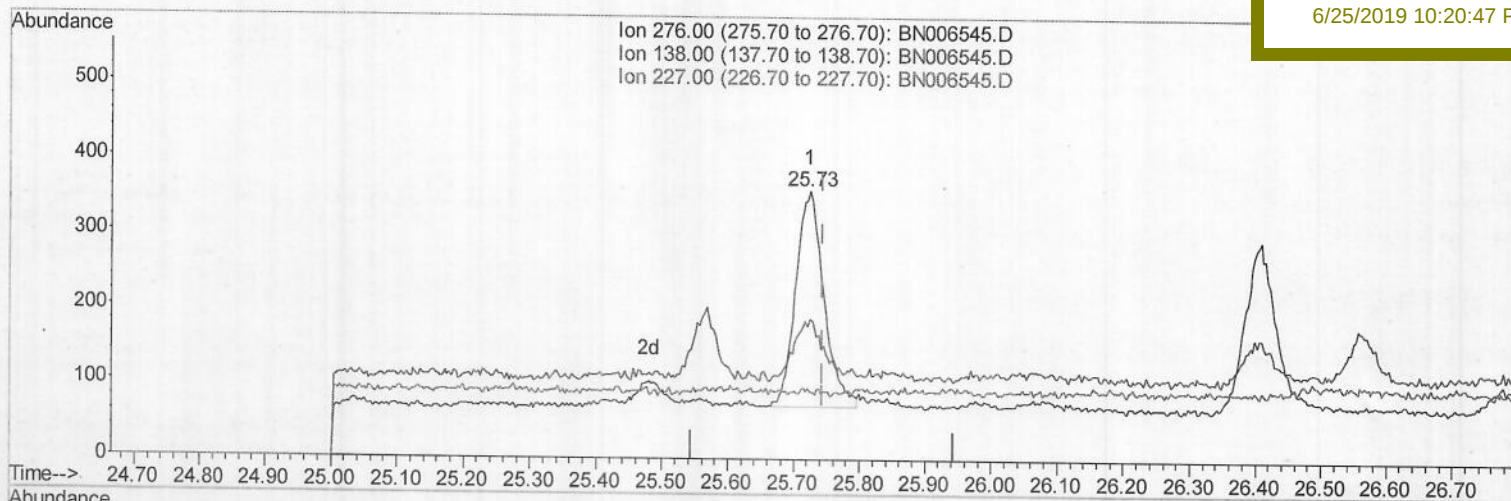

TIC: BN006545.D

(24) Indeno(1,2,3-cd)pyrene

25.725min (-0.020) 0.02ng/ui m

response 860

Ion	Exp%	Act%
276.00	100	100
138.00	32.00	23.84#
227.00	0.40	0.35
0.00	0.00	0.00

JU 06/26/19

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006545.D

Acq On : 24 Jun 2019 23:22

Operator : HP/JU

Sample : K3362-06

Misc :

ALS Vial : 23 Sample Multiplier: 1

Quant Time: Jun 25 03:52:00 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019




Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A41X5

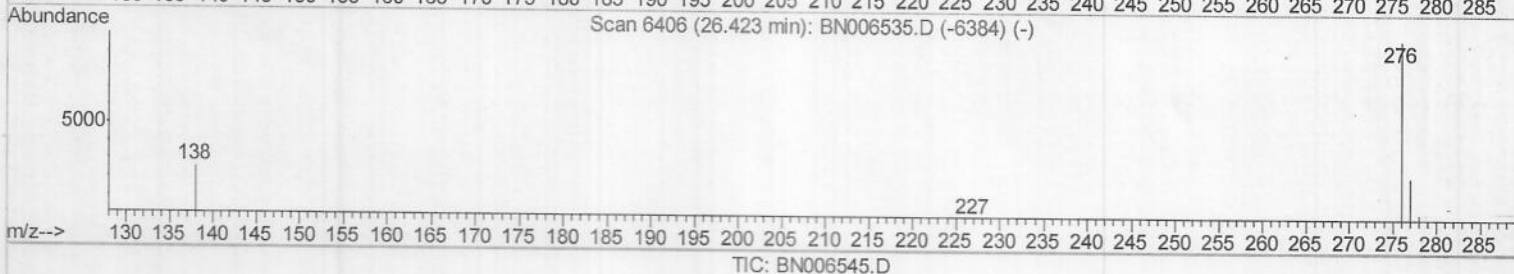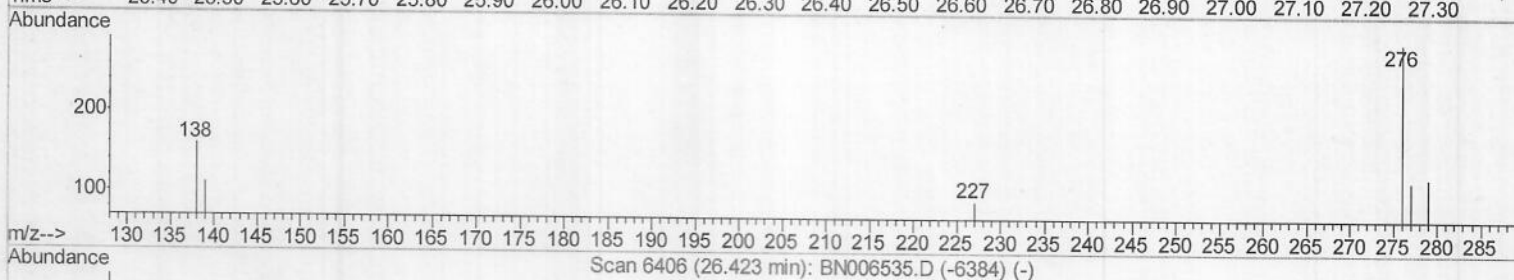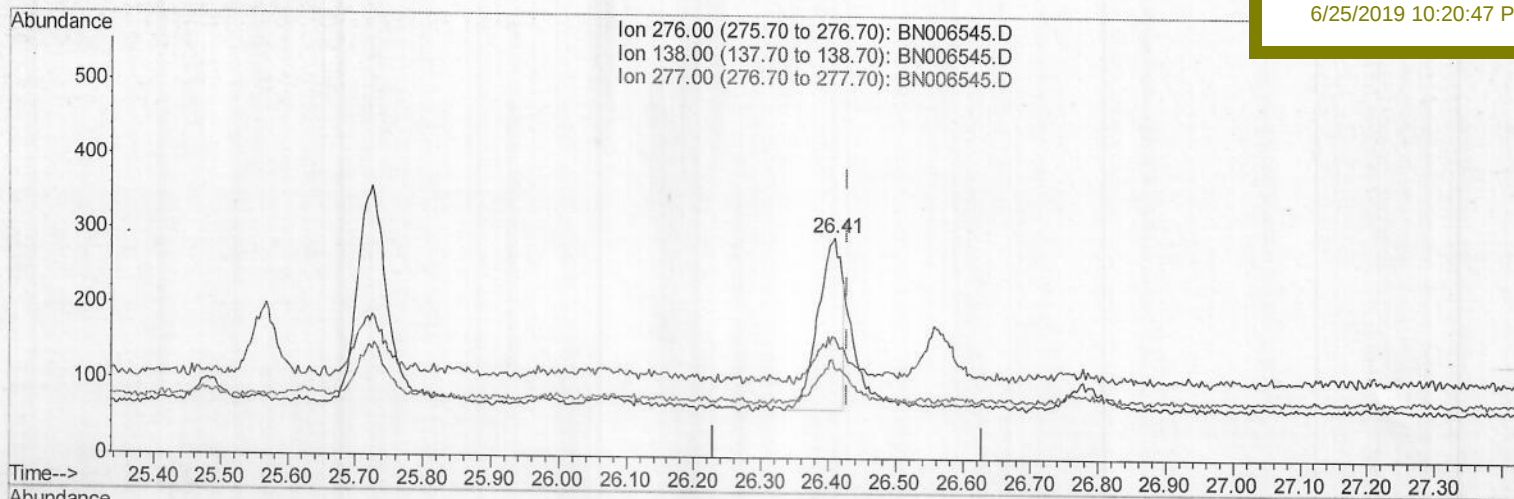Manual Integrations
APPROVEDmohammad
6/25/2019 10:20:47 PM

(26) Benzo(g,h,i)perylene

26.409min (-0.020) 0.02ng/ul

response 560

Ion	Exp%	Act%
276.00	100	100
138.00	30.30	54.45#
277.00	26.90	40.41#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006545.D

Acq On : 24 Jun 2019 23:22

Operator : HP/JU

Sample : K3362-06

Misc :

ALS Vial : 23 Sample Multiplier: 1

Quant Time: Jun 25 03:52:00 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019




Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A41X5

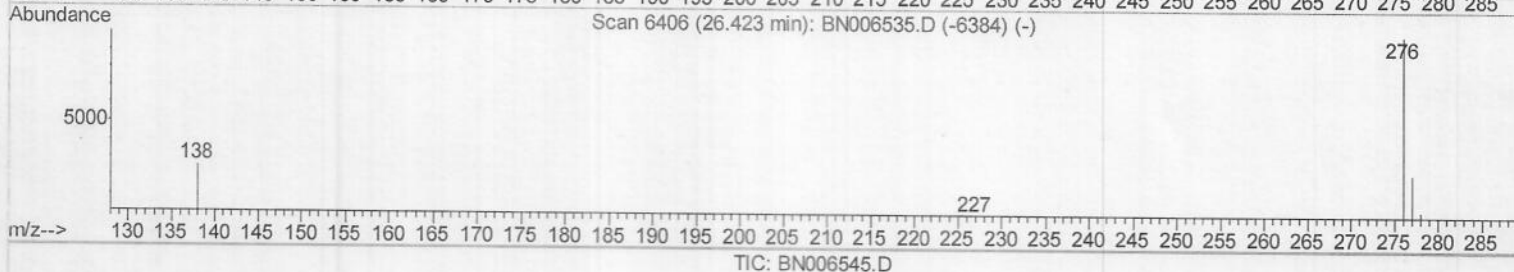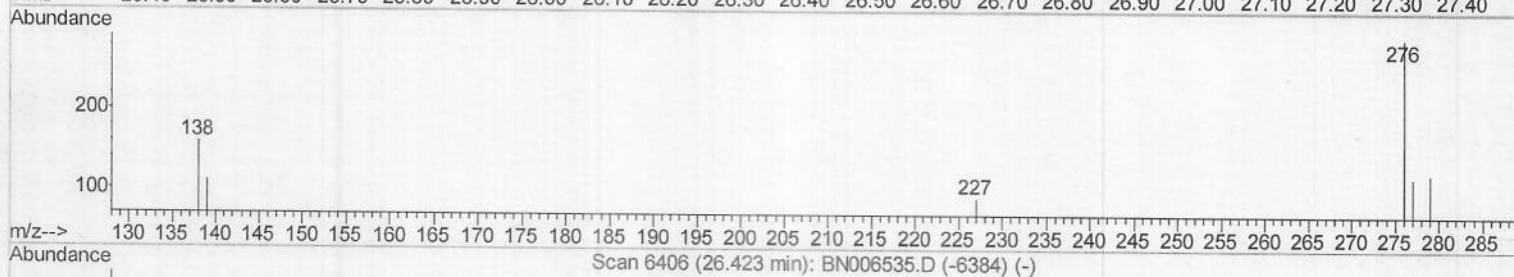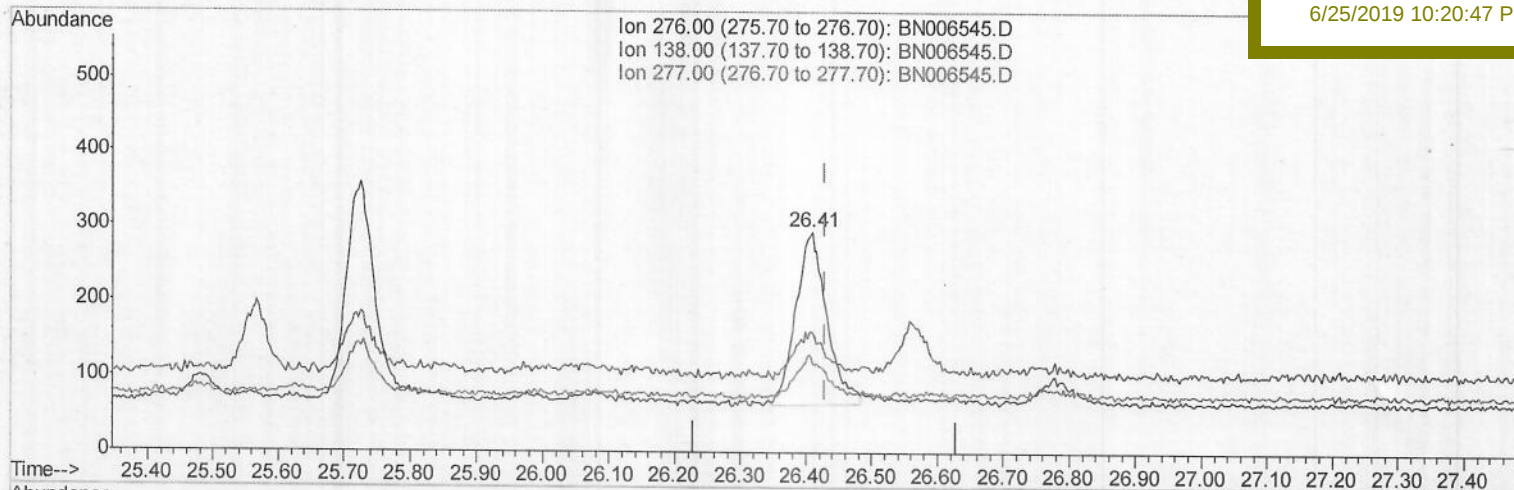Manual Integrations
APPROVEDmohammad
6/25/2019 10:20:47 PM

(26) Benzo(g,h,i)perylene

26.409min (-0.020) 0.02ng/ul m

response 748

Ion	Exp%	Act%
276.00	100	100
138.00	30.30	54.45#
277.00	26.90	40.41#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
 Data File : BN006545.D
 Acq On : 24 Jun 2019 23:22
 Operator : HP/JU
 Sample : K3362-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A41X5

Quant. Time: Jun 25 03:54:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 6/25/2019 10:20:47 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	4215	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.41	136	16055	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.28	164	8916	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	18899m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.25	240	12624m	0.40	ng/ul	-0.01
20) Perylene-d12	23.48	264	9223m	0.40	ng/ul	-0.03
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.01	152	8147	0.33	ng/ul	-0.01
14) Fluoranthene-d10	19.08	212	19918m	0.39	ng/ul	-0.01
Target Compounds						
12) Phenanthrene	17.08	178	1776m	0.029	ng/ul	
15) Fluoranthene	19.11	202	4674m	0.070	ng/ul	
17) Pyrene	19.47	202	4012	0.060	ng/ul#	91
18) Benzo (a) anthracene	21.24	228	1424	0.026	ng/ul#	88
19) Chrysene	21.29	228	1669	0.032	ng/ul#	89
21) Benzo (b) fluoranthene	22.82	252	2089m	0.054	ng/ul	
23) Benzo (a) pyrene	23.38	252	1104m	0.031	ng/ul	
24) Indeno (1,2,3-cd) pyrene	25.73	276	860m	0.022	ng/ul	
26) Benzo (g,h,i) perylene	26.41	276	748m	0.023	ng/ul	

JU
 06/26/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed