

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006546.D

Acq On : 24 Jun 2019 23:57

Operator : HP/JU

Sample : K3362-08

Misc :

ALS Vial : 24 Sample Multiplier: 1

Quant Time: Jun 25 04:08:36 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampled :

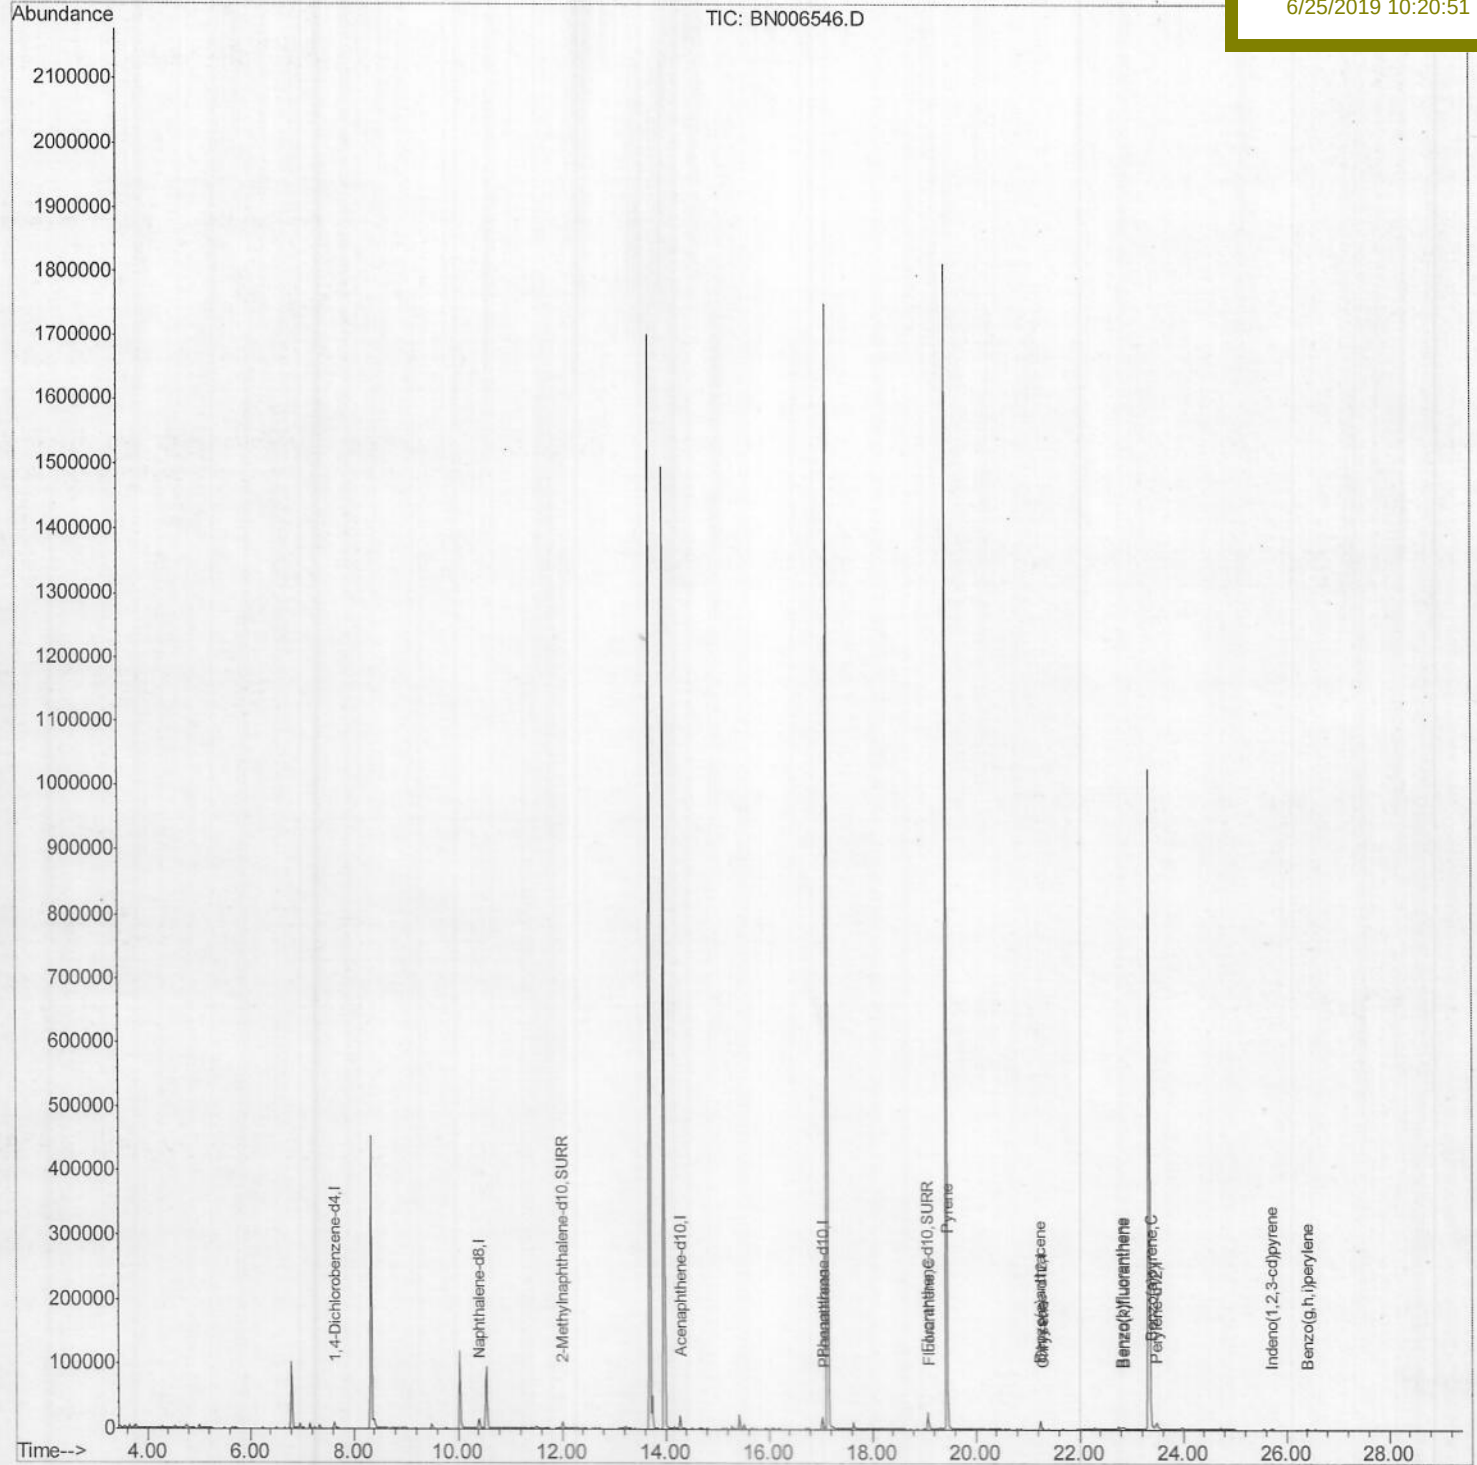
A41X7

Manual Integrations

APPROVED

mohammad

6/25/2019 10:20:51 PM



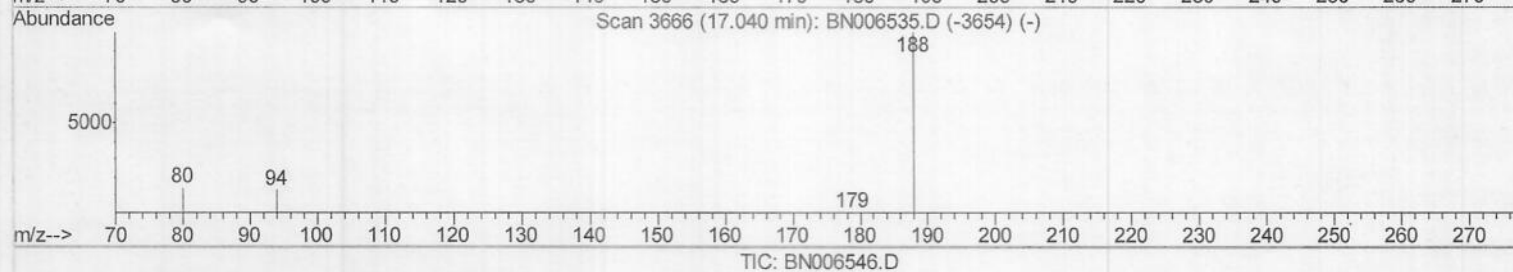
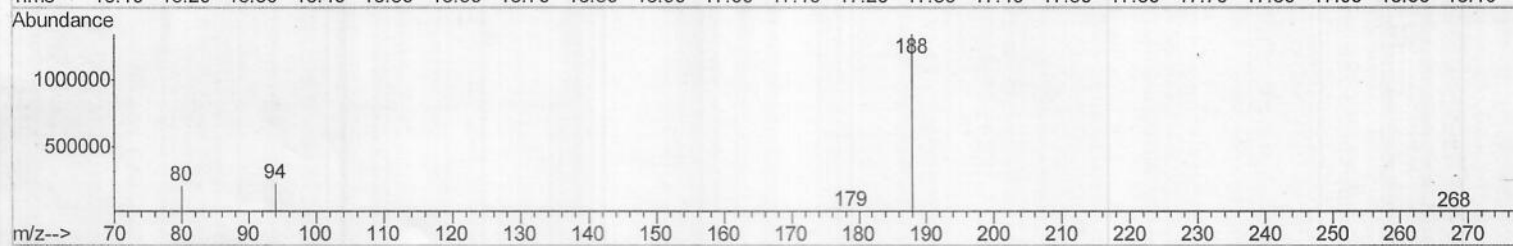
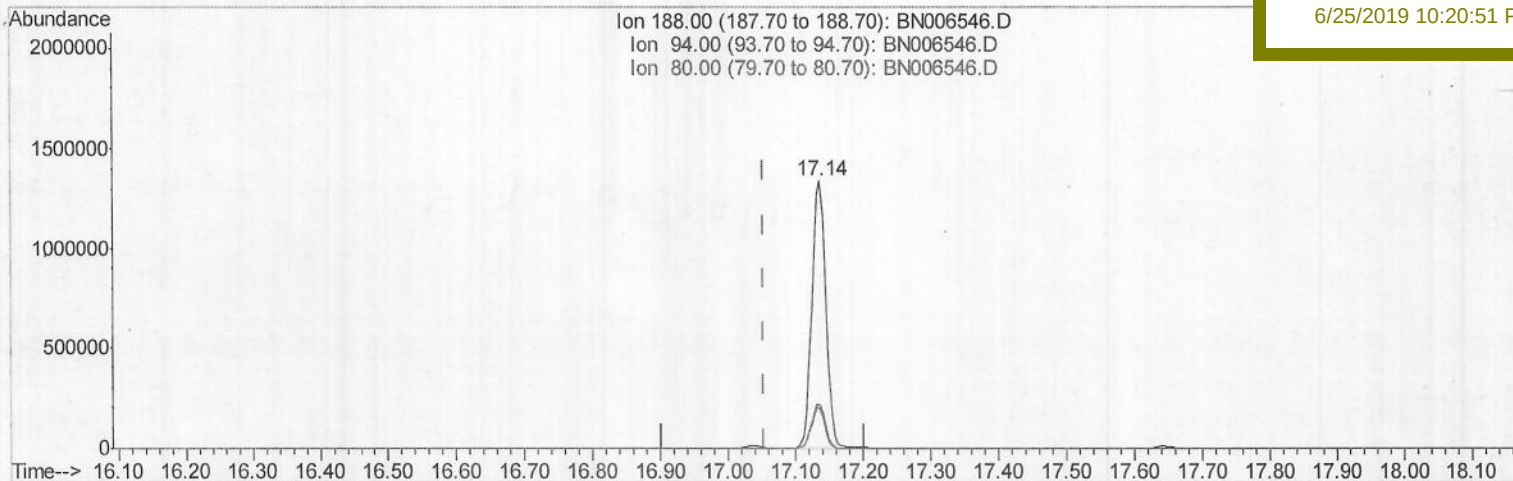
Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006546.D
Acq On : 24 Jun 2019 23:57
Operator : HP/JU
Sample : K3362-08
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Jun 25 00:45:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A41X7

Manual Integrations
APPROVED

mohammad
6/25/2019 10:20:51 PM



(10) Phenanthrene-d10 (I)

17.137min (+0.084) 0.40ng/ul

response 1946306

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	15.95#
80.00	13.60	14.57
0.00	0.00	0.00

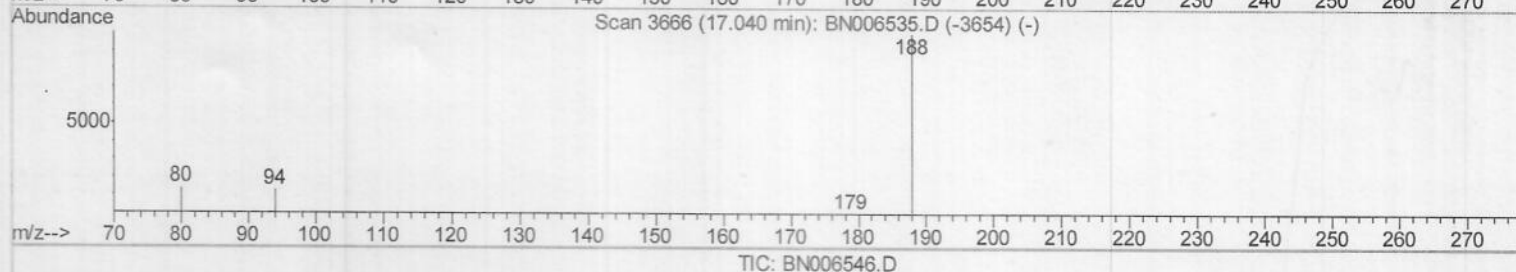
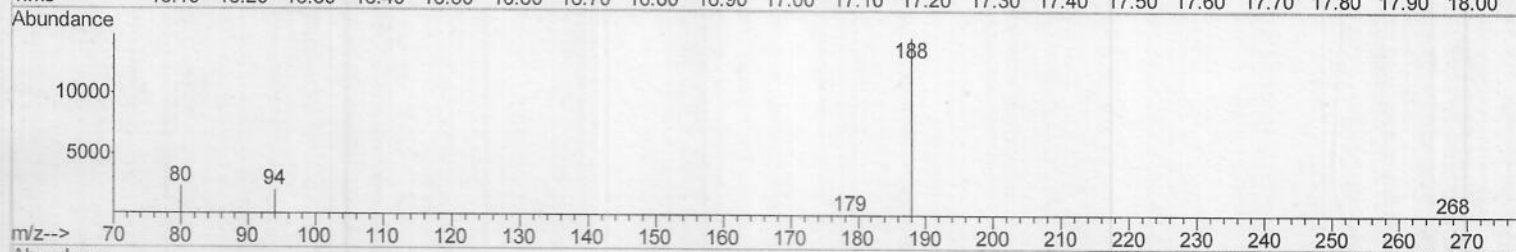
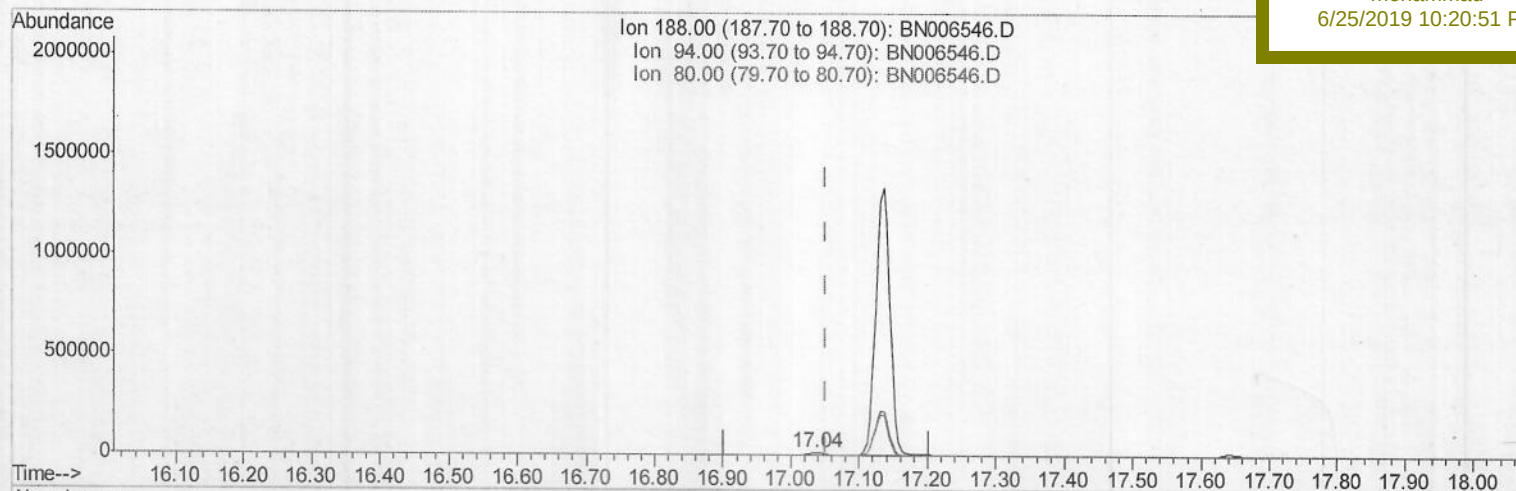
Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006546.D
Acq On : 24 Jun 2019 23:57
Operator : HP/JU
Sample : K3362-08
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Jun 25 00:45:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A41X7

Manual Integrations
APPROVED

mohammad
6/25/2019 10:20:51 PM



TIC: BN006546.D

(10) Phenanthrene-d10 (I)

17.035min (-0.017) 0.40ng/ul m

> JU 06/26/19

response 20881

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	13.63
80.00	13.60	15.12
0.00	0.00	0.00

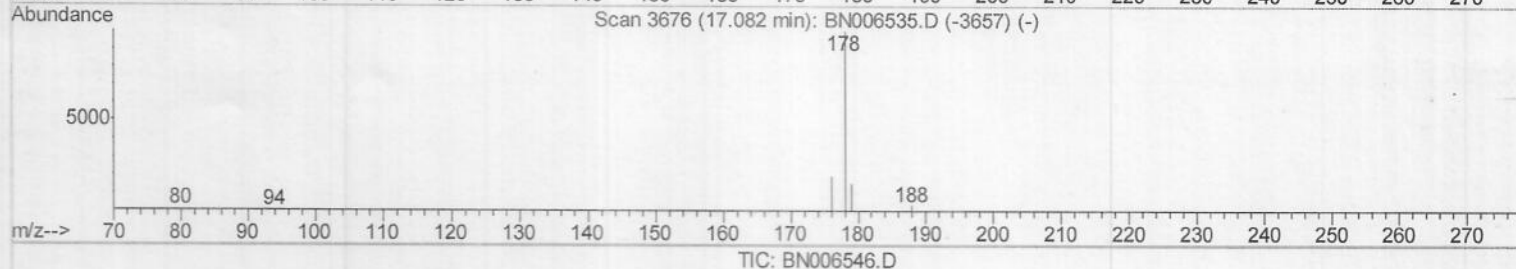
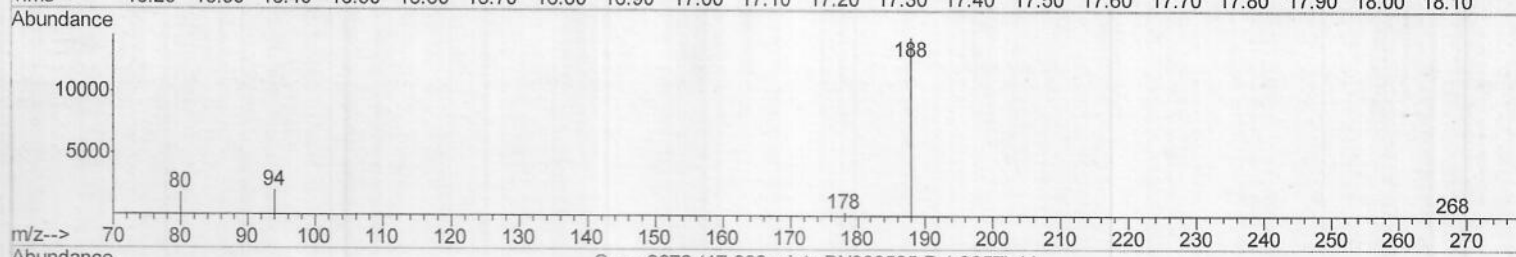
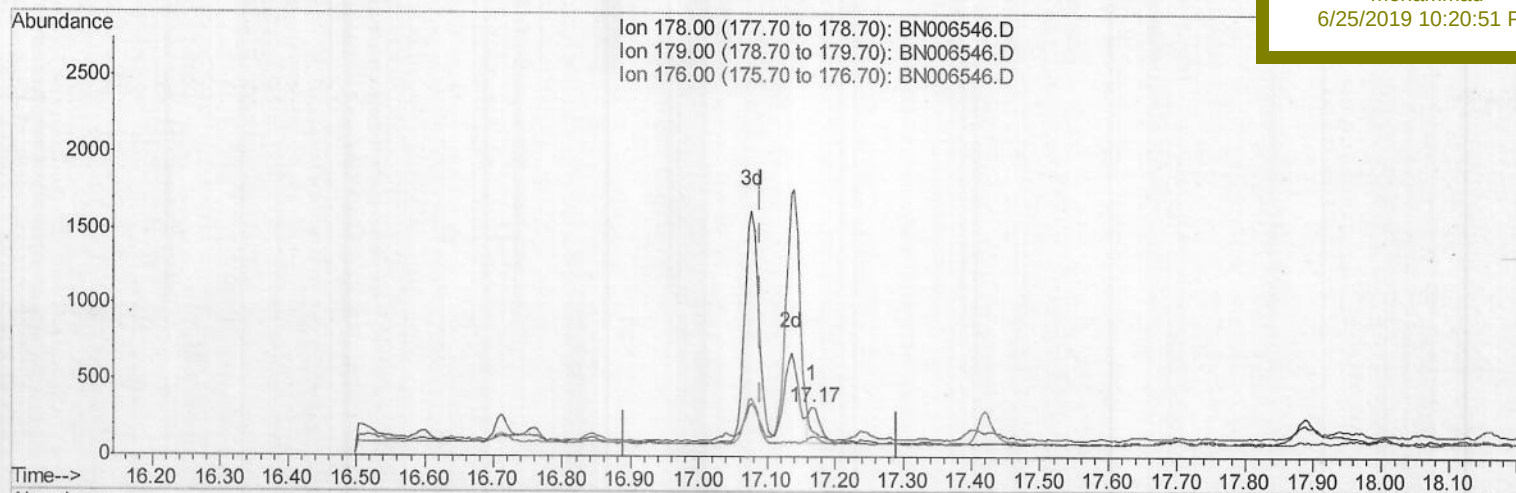
Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006546.D
Acq On : 24 Jun 2019 23:57
Operator : HP/JU
Sample : K3362-08
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Jun 25 04:04:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A41X7

Manual Integrations
APPROVED

mohammad
6/25/2019 10:20:51 PM



(12) Phenanthrene

17.166min (+0.076) 0.00ng/ul

response 277

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	52.62#
176.00	19.10	39.69#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006546.D

Acq On : 24 Jun 2019 23:57

Operator : HP/JU

Sample : K3362-08

Misc :

ALS Vial : 24 Sample Multiplier: 1

Quant Time: Jun 25 04:04:41 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

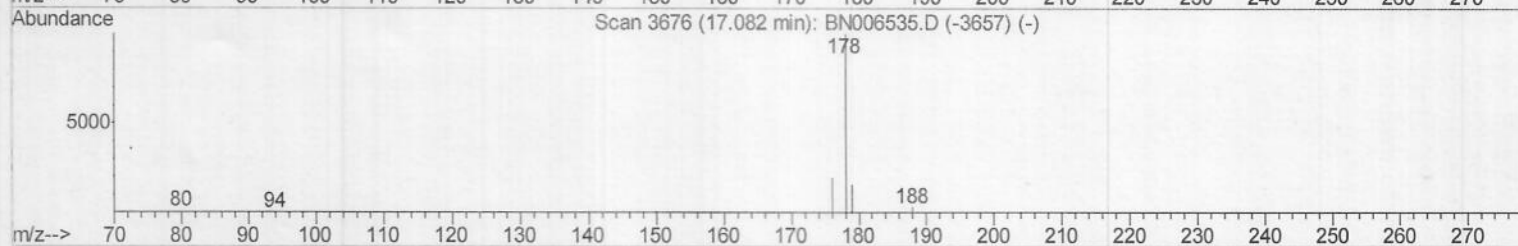
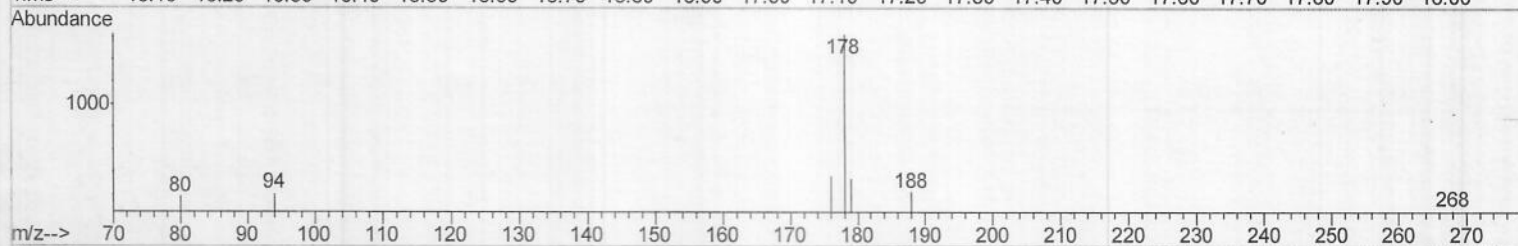
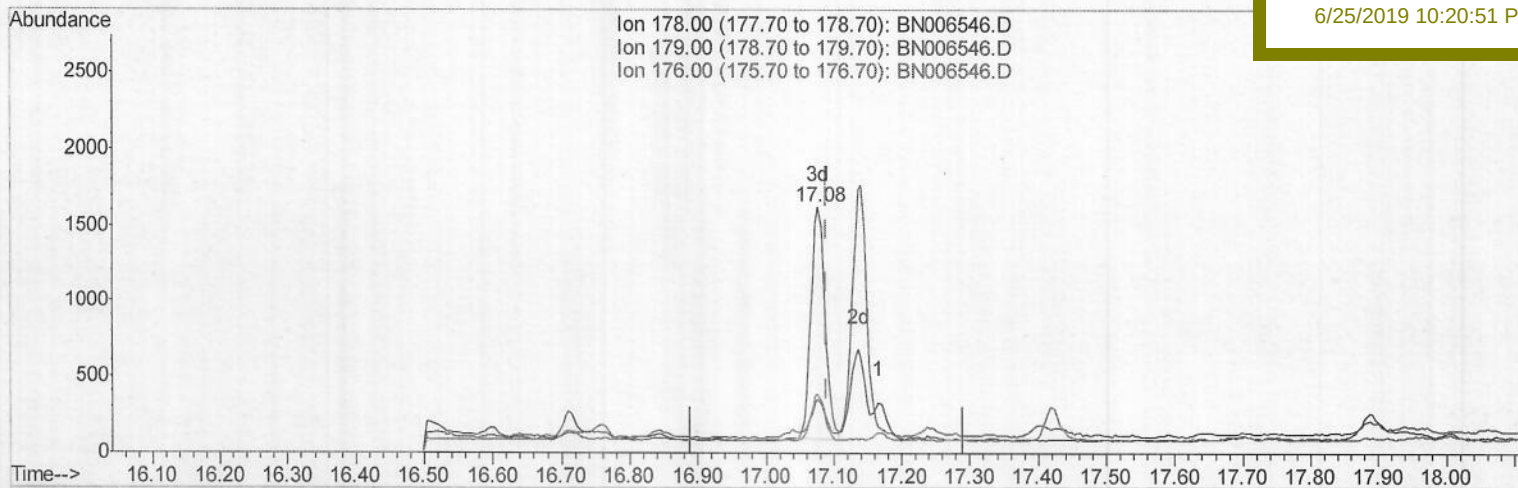
Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A41X7

Manual Integrations
APPROVEDmohammad
6/25/2019 10:20:51 PM

TIC: BN006546.D

(12) Phenanthrene

17.078min (-0.013) 0.03ng/ul m > JU 06/26/19

response 2197

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	21.20#
176.00	19.10	23.17#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006546.D

Acq On : 24 Jun 2019 23:57

Operator : HP/JU

Sample : K3362-08

Misc :

ALS Vial : 24 Sample Multiplier: 1

Quant Time: Jun 25 04:04:41 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

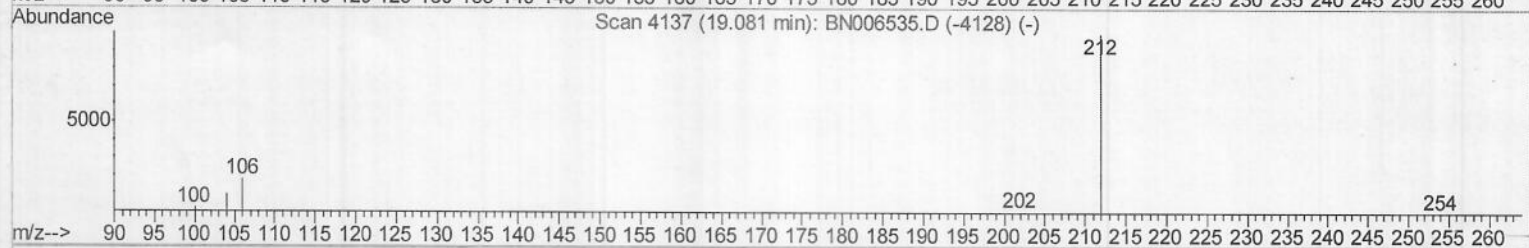
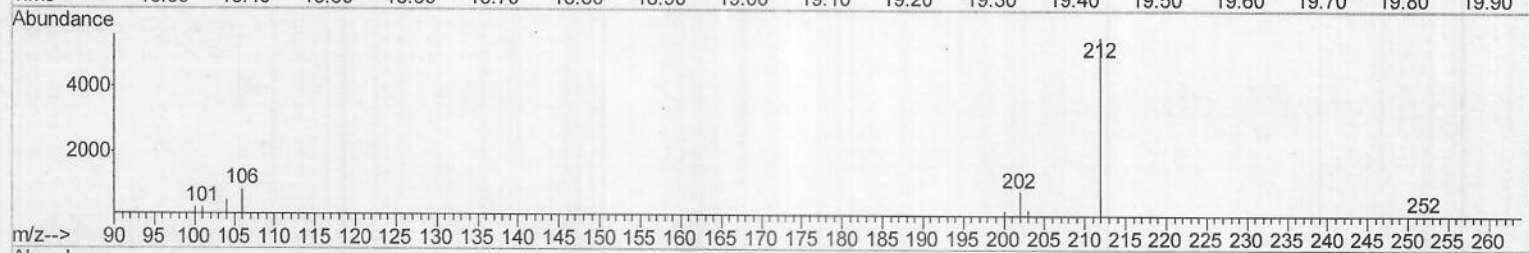
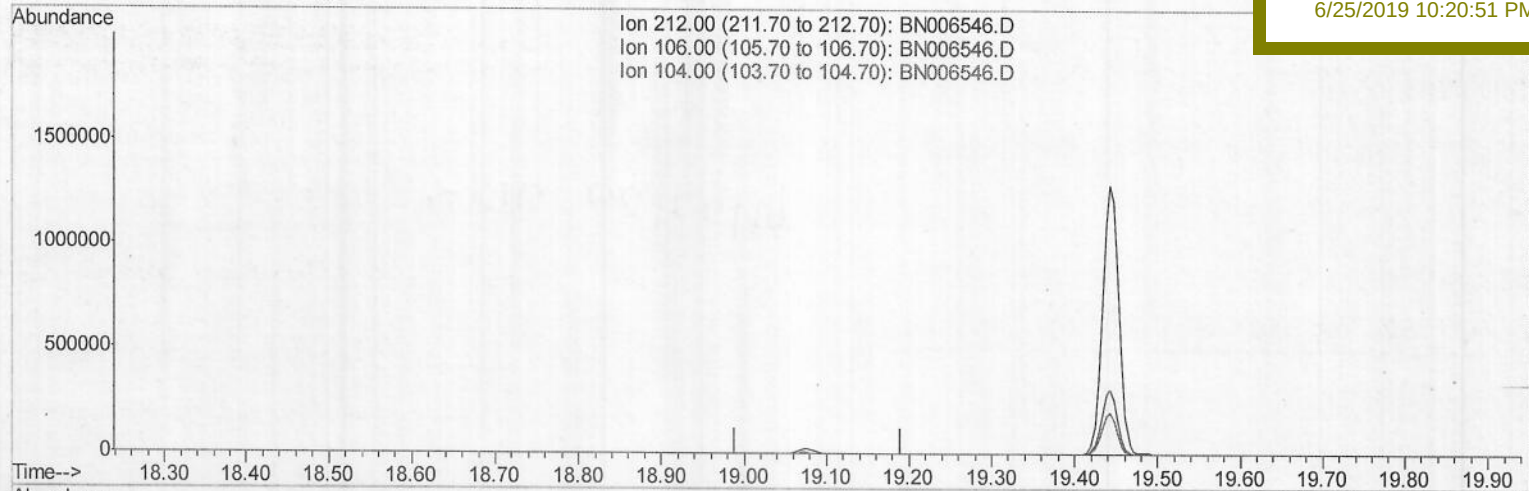
Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A41X7

Manual Integrations
APPROVEDmohammad
6/25/2019 10:20:51 PM

(14) Fluoranthene-d10 (SURR)

19.090min (-19.090) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006546.D

Acq On : 24 Jun 2019 23:57

Operator : HP/JU

Sample : K3362-08

Misc :

ALS Vial : 24 Sample Multiplier: 1

Quant Time: Jun 25 04:04:41 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

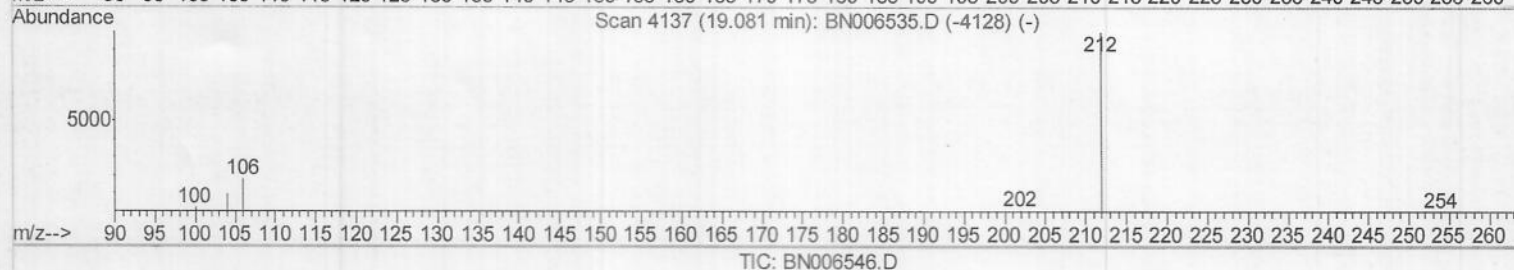
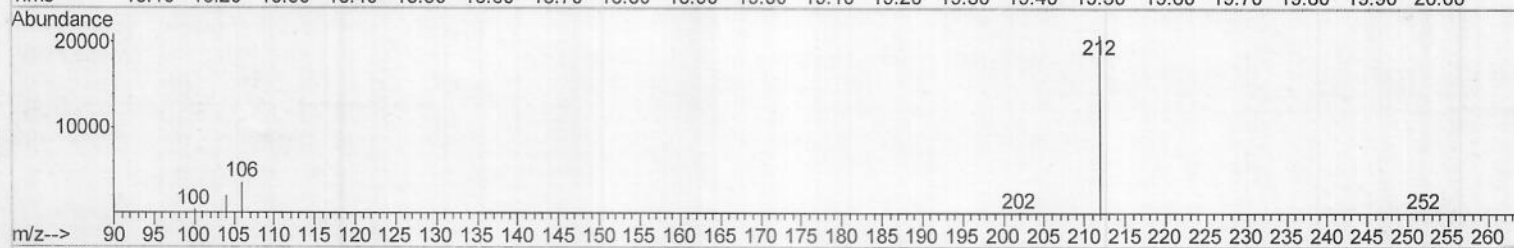
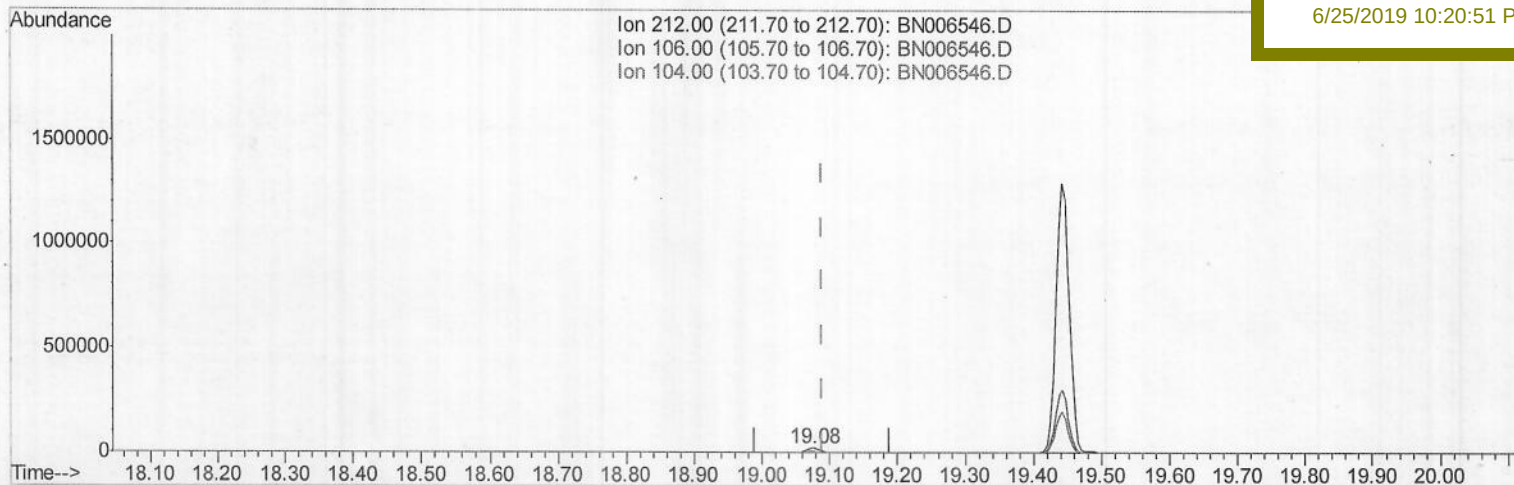
Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A41X7

Manual Integrations
APPROVEDmohammad
6/25/2019 10:20:51 PM

(14) Fluoranthene-d10 (SURR)

19.076min (-0.014) 0.50ng/ul m

response 27882

Ion	Exp%	Act%
212.00	100	100
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006546.D

Acq On : 24 Jun 2019 23:57

Operator : HP/JU

Sample : K3362-08

Misc :

ALS Vial : 24 Sample Multiplier: 1

Quant Time: Jun 25 04:04:41 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

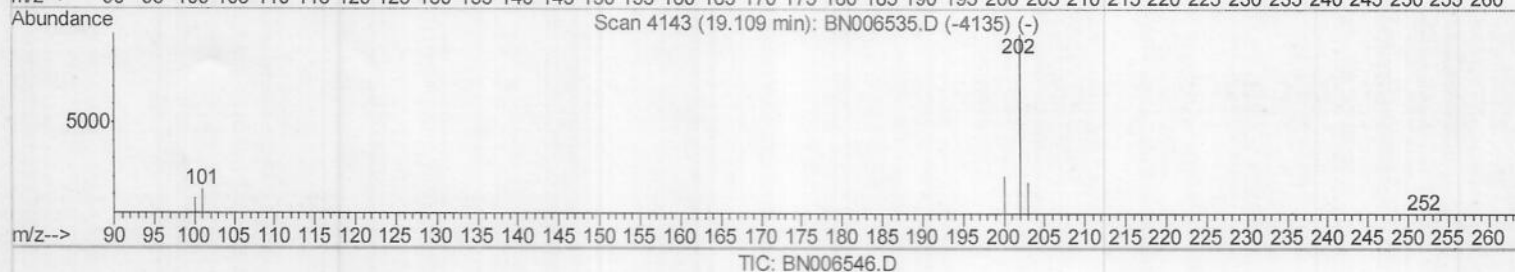
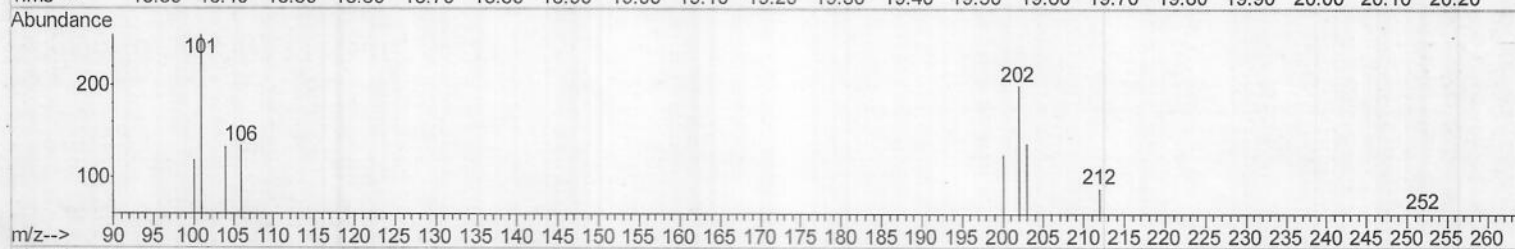
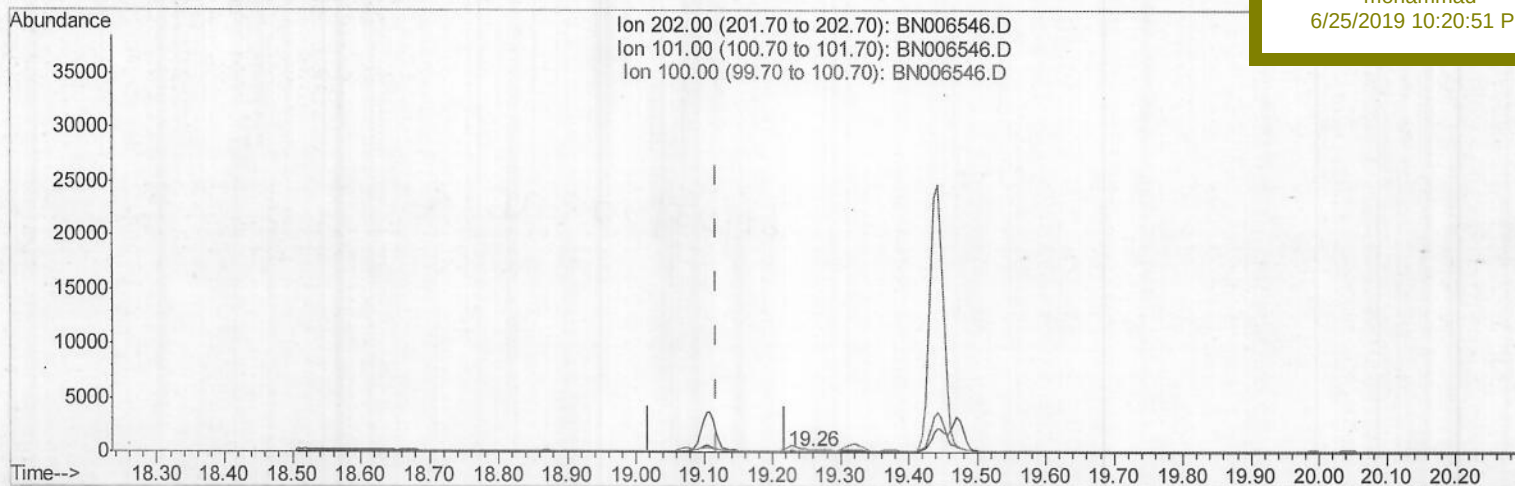
Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A41X7

Manual Integrations
APPROVEDmohammad
6/25/2019 10:20:51 PM

(15) Fluoranthene (C)

19.257min (+0.139) 0.00ng/ul

response 108

Ion	Exp%	Act%
202.00	100	100
101.00	12.10	127.64#
100.00	8.70	59.80#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006546.D

Acq On : 24 Jun 2019 23:57

Operator : HP/JU

Sample : K3362-08

Misc :

ALS Vial : 24 Sample Multiplier: 1

Quant Time: Jun 25 04:04:41 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

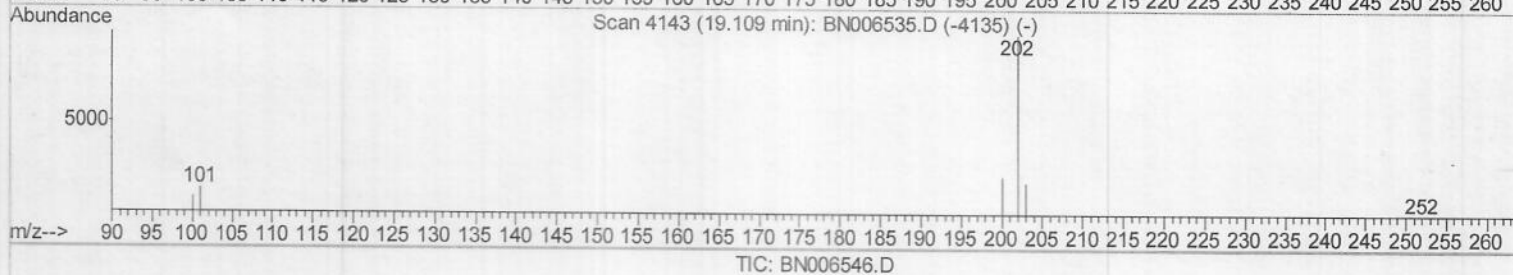
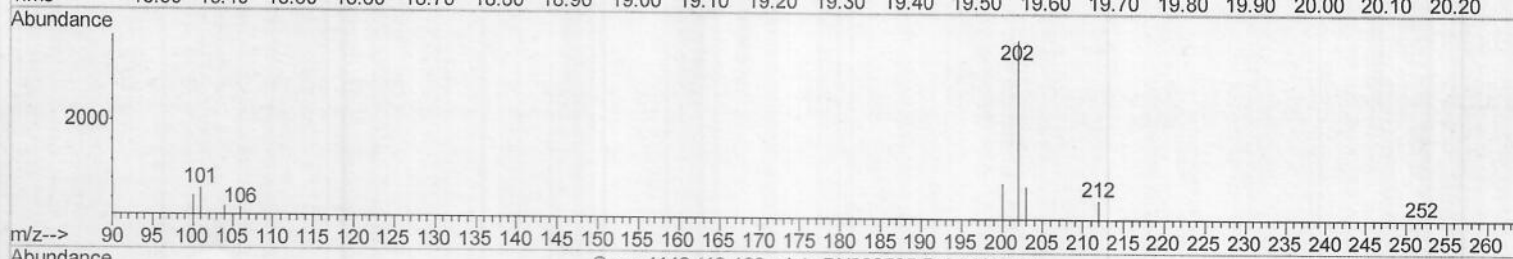
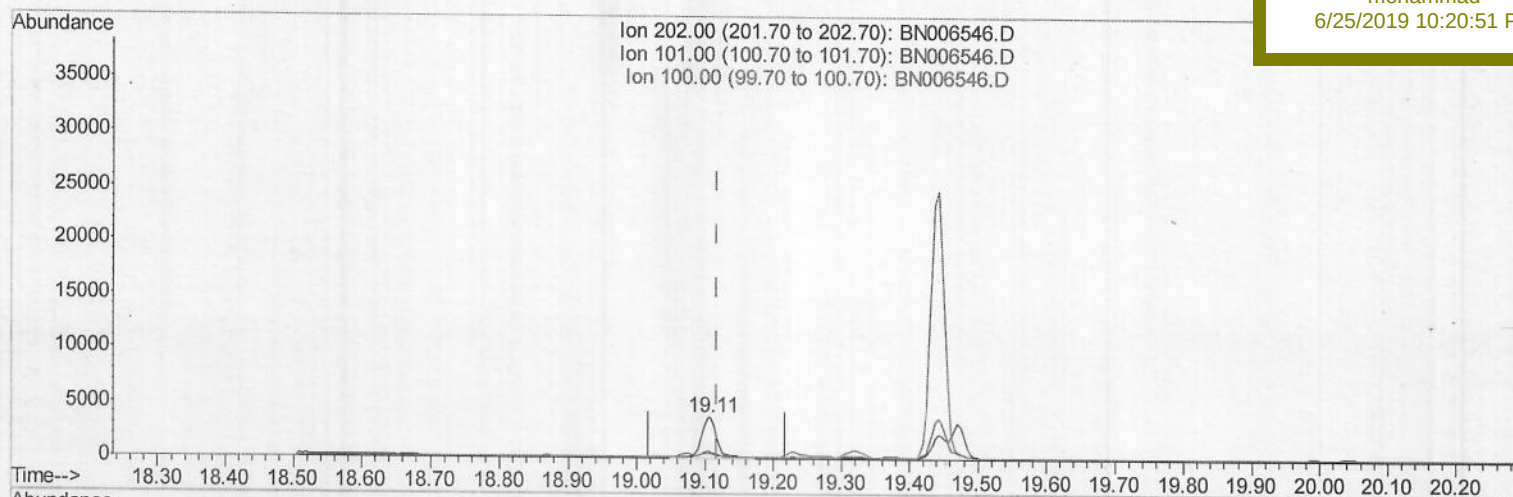
Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A41X7

Manual Integrations
APPROVEDmohammad
6/25/2019 10:20:51 PM

(15) Fluoranthene (C)

19.108min (-0.010) 0.08ng/ul m

response 6170

Ion	Exp%	Act%
202.00	100	100
101.00	12.10	16.08
100.00	8.70	12.08
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006546.D

Acq On : 24 Jun 2019 23:57

Operator : HP/JU

Sample : K3362-08

Misc :

ALS Vial : 24 Sample Multiplier: 1

Quant Time: Jun 25 04:04:41 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

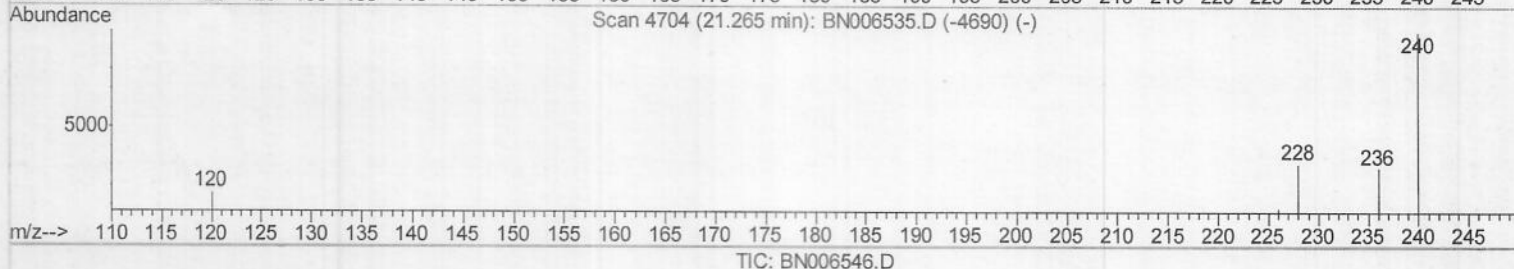
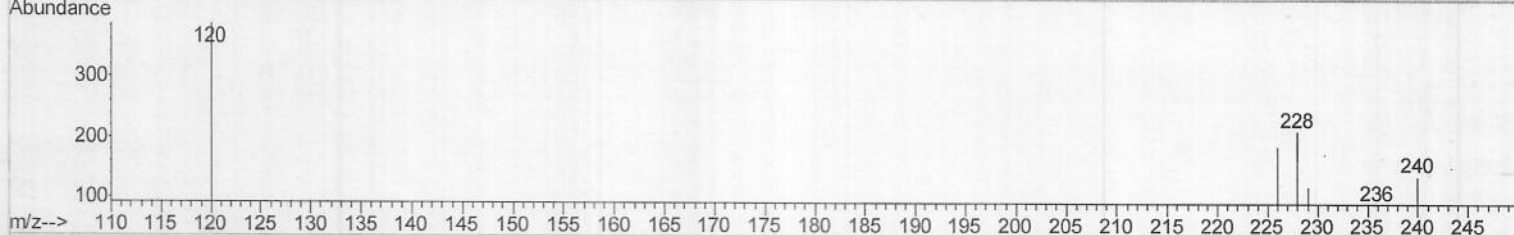
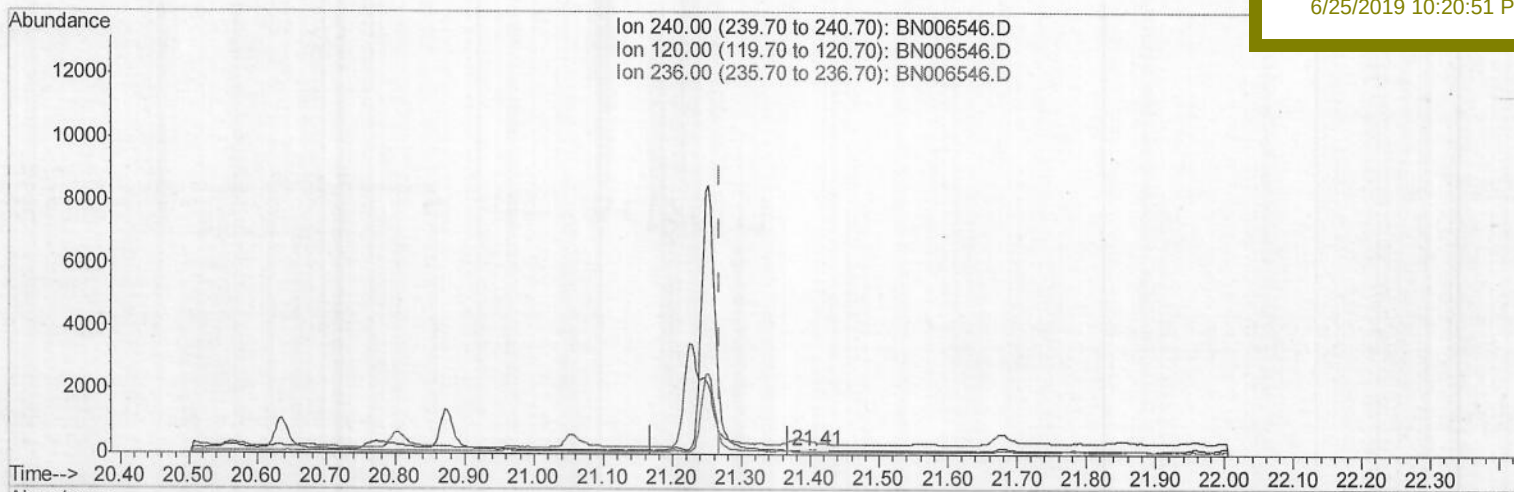
A41X7

Manual Integrations

APPROVED

mohammad

6/25/2019 10:20:51 PM



(16) Chrysene-d12 (I)

21.407min (+0.139) 0.40ng/ul

response 38

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	278.26#
236.00	30.10	65.94#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006546.D

Acq On : 24 Jun 2019 23:57

Operator : HP/JU

Sample : K3362-08

Misc :

ALS Vial : 24 Sample Multiplier: 1

Quant Time: Jun 25 04:04:41 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

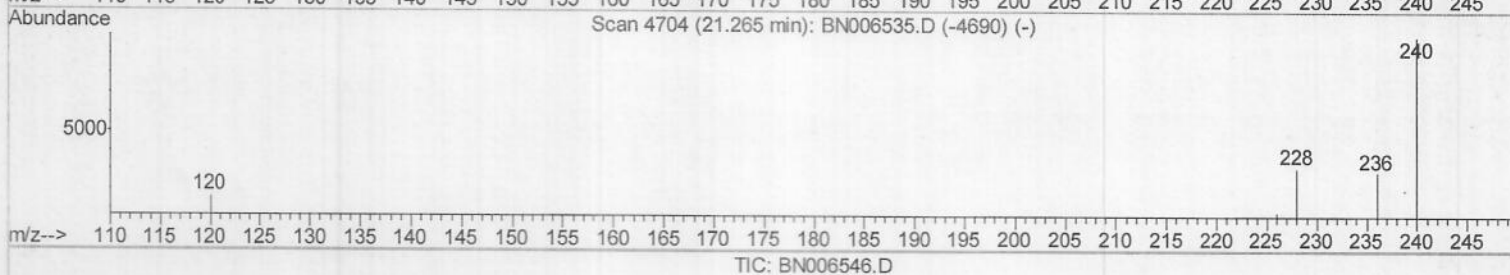
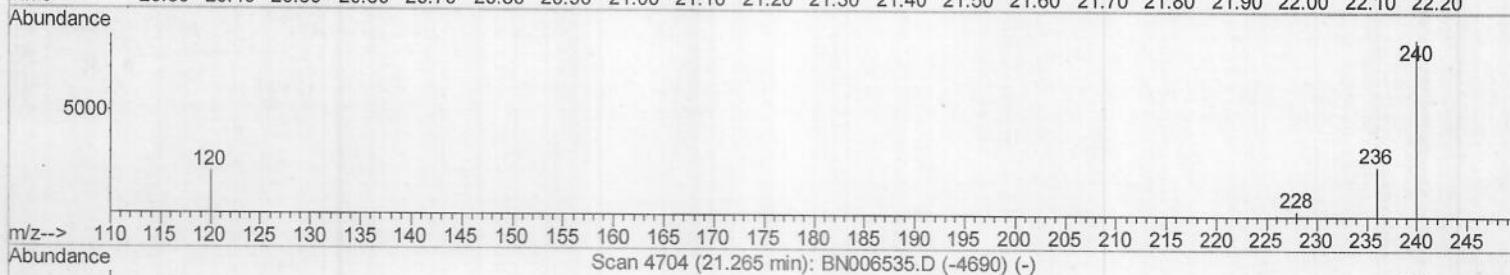
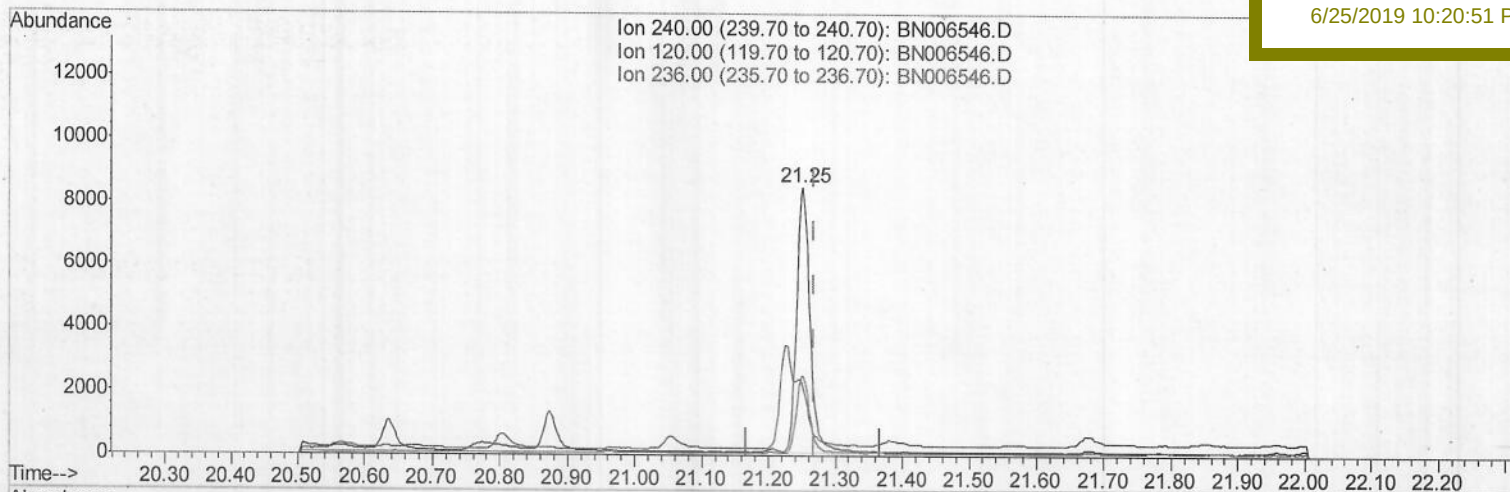
Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A41X7

Manual Integrations
APPROVEDmohammad
6/25/2019 10:20:51 PM

(16) Chrysene-d12 (I)

21.252min (-0.016) 0.40ng/ul m

response 11657

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	25.48#
236.00	30.10	29.55
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006546.D

Acq On : 24 Jun 2019 23:57

Operator : HP/JU

Sample : K3362-08

Misc :

ALS Vial : 24 Sample Multiplier: 1

Quant Time: Jun 25 04:05:57 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

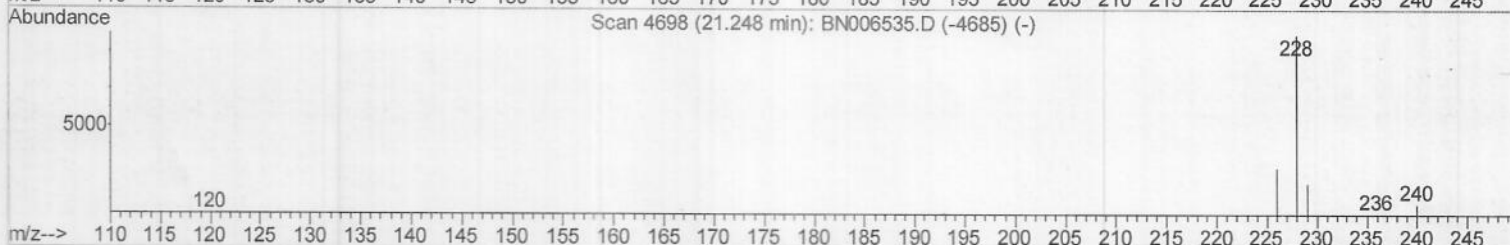
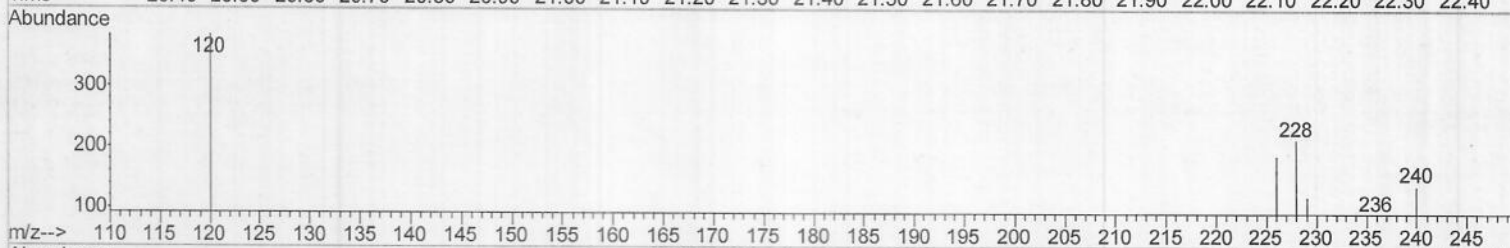
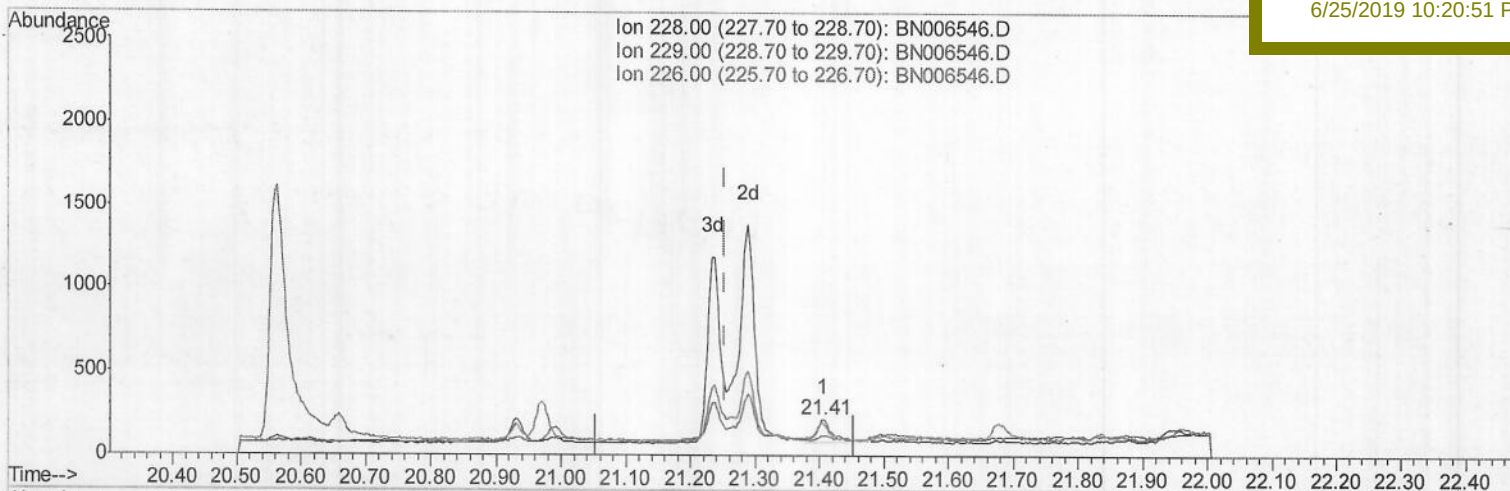
A41X7

Manual Integrations

APPROVED

mohammad

6/25/2019 10:20:51 PM



(18) Benzo(a)anthracene

21.407min (+0.153) 0.00ng/ui

response 214

Ion	Exp%	Act%
228.00	100	100
229.00	20.60	55.87#
226.00	28.50	87.79#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006546.D

Acq On : 24 Jun 2019 23:57

Operator : HP/JU

Sample : K3362-08

Misc :

ALS Vial : 24 Sample Multiplier: 1

Quant Time: Jun 25 04:05:57 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

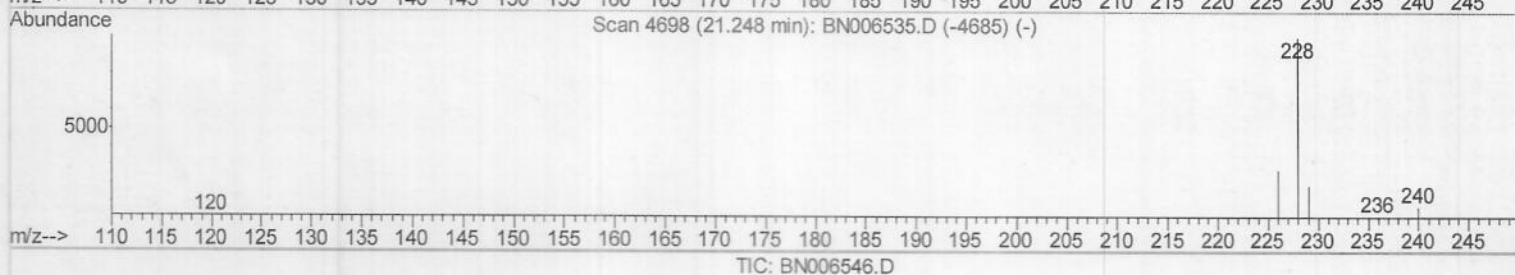
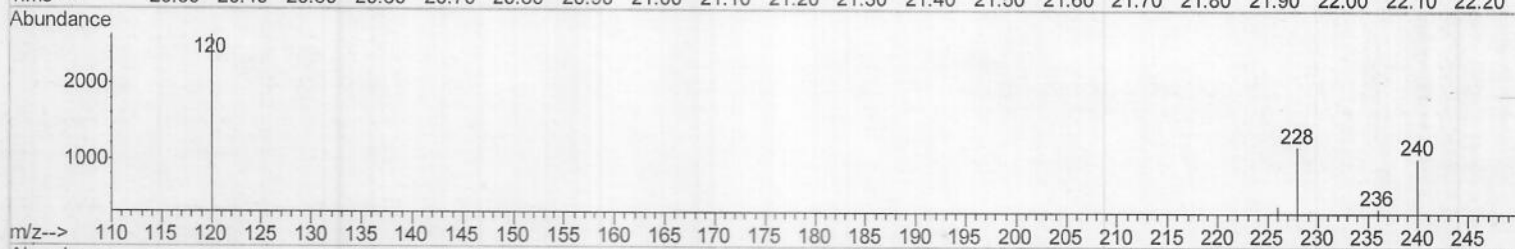
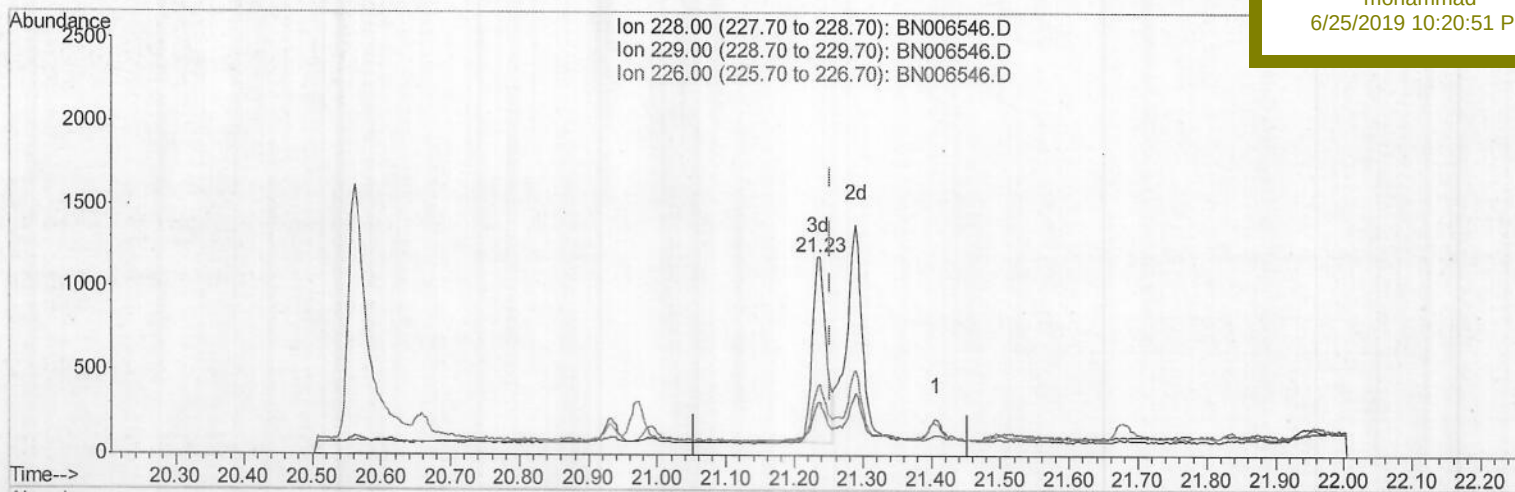
Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A41X7

Manual Integrations
APPROVEDmohammad
6/25/2019 10:20:51 PM

(18) Benzo(a)anthracene

21.234min (-0.019) 0.03ng/ul m

response 1527

Ion	Exp%	Act%
228.00	100	100
229.00	20.60	26.27#
226.00	28.50	33.95
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006546.D

Acq On : 24 Jun 2019 23:57

Operator : HP/JU

Sample : K3362-08

Misc :

ALS Vial : 24 Sample Multiplier: 1

Quant Time: Jun 25 04:05:57 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

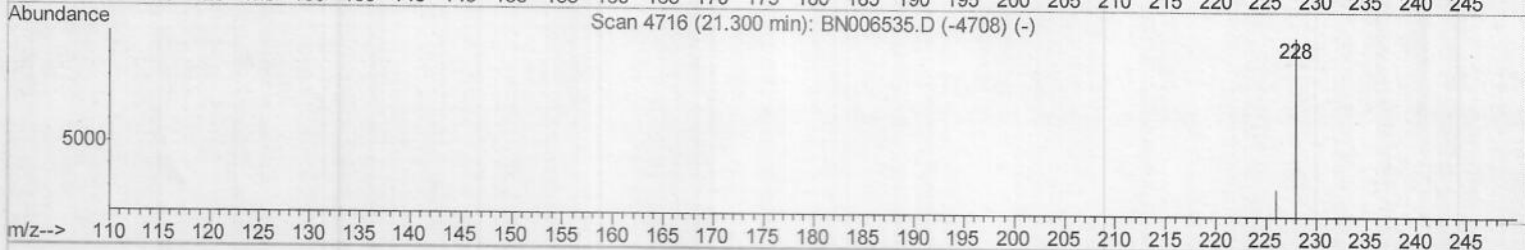
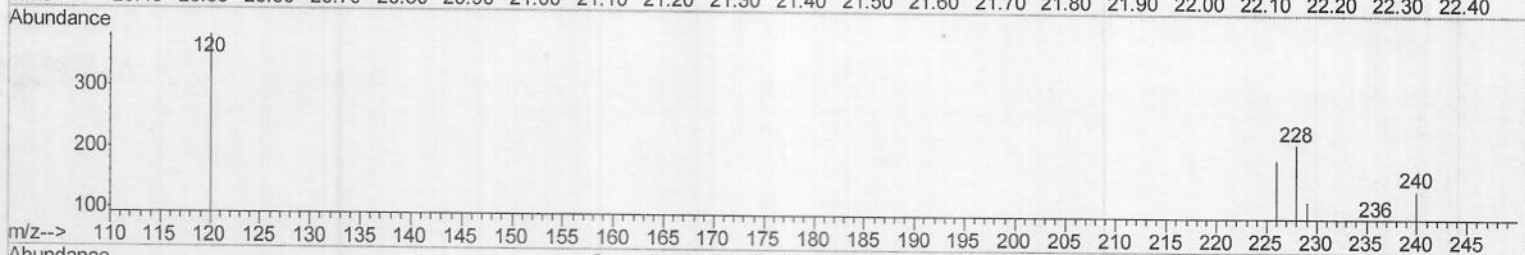
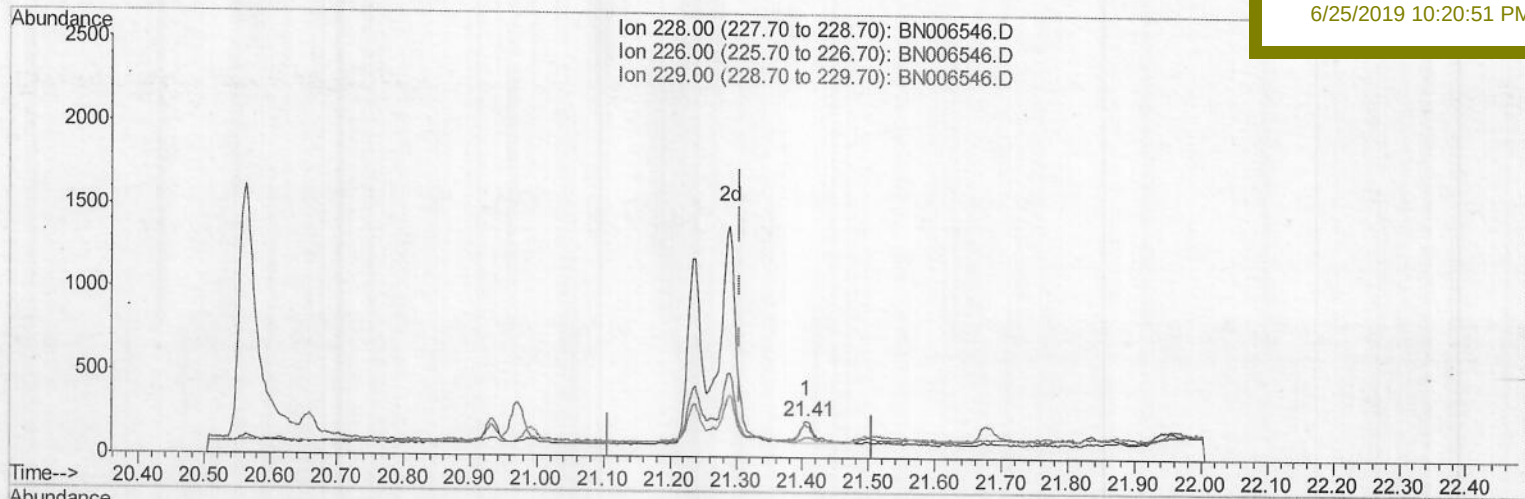
A41X7

Manual Integrations

APPROVED

mohammad

6/25/2019 10:20:51 PM



(19) Chrysene

21.407min (+0.101) 0.00ng/ul

response 204

Ion	Exp%	Act%
228.00	100	100
226.00	31.30	87.79#
229.00	20.40	55.87#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006546.D

Acq On : 24 Jun 2019 23:57

Operator : HP/JU

Sample : K3362-08

Misc :

ALS Vial : 24 Sample Multiplier: 1

Quant Time: Jun 25 04:05:57 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

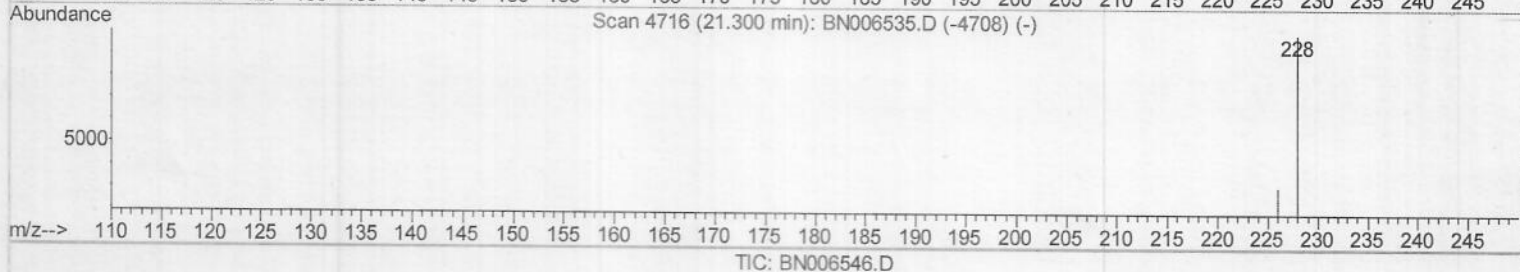
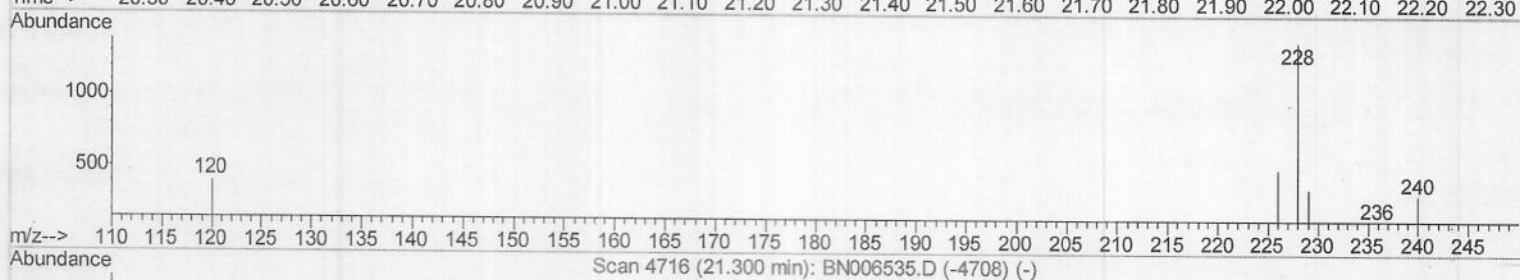
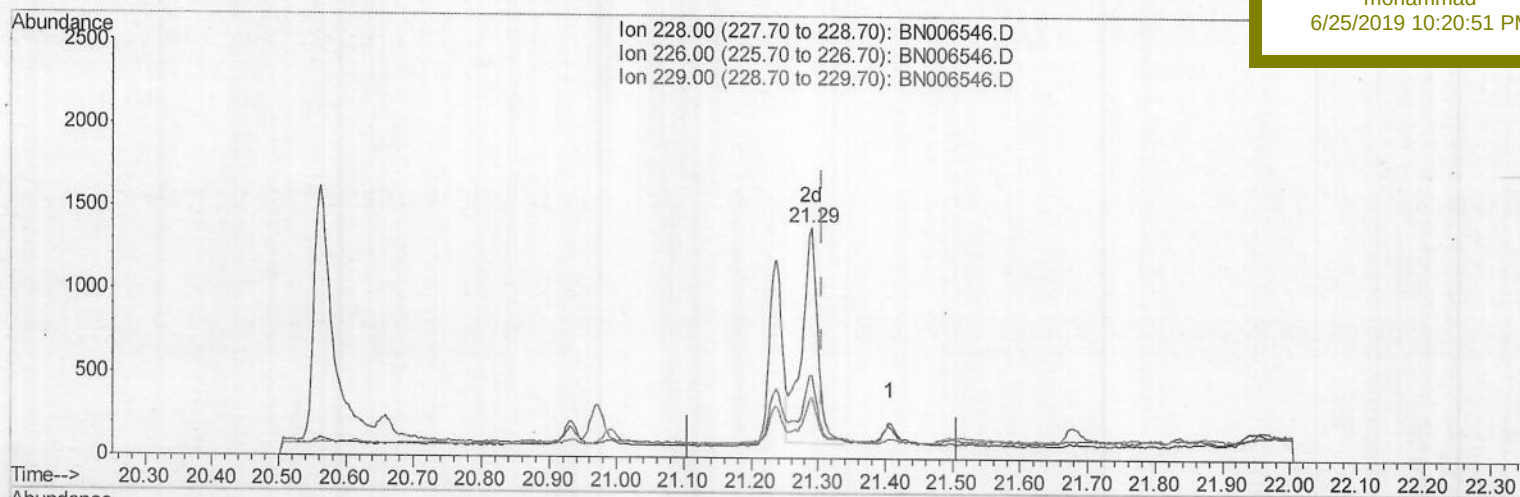
Response via : Initial Calibration

Instrument :

BNA_N

ClientSampled :

A41X7

Manual Integrations
APPROVEDmohammad
6/25/2019 10:20:51 PM

(19) Chrysene

21.290min (-0.016) 0.04ng/ul m

response 2176

Ion	Exp%	Act%
228.00	100	100
226.00	31.30	36.03
229.00	20.40	26.34#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006546.D

Acq On : 24 Jun 2019 23:57

Operator : HP/JU

Sample : K3362-08

Misc :

ALS Vial : 24 Sample Multiplier: 1

Quant Time: Jun 25 04:05:57 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

Response via : Initial Calibration

Instrument :

BNA_N

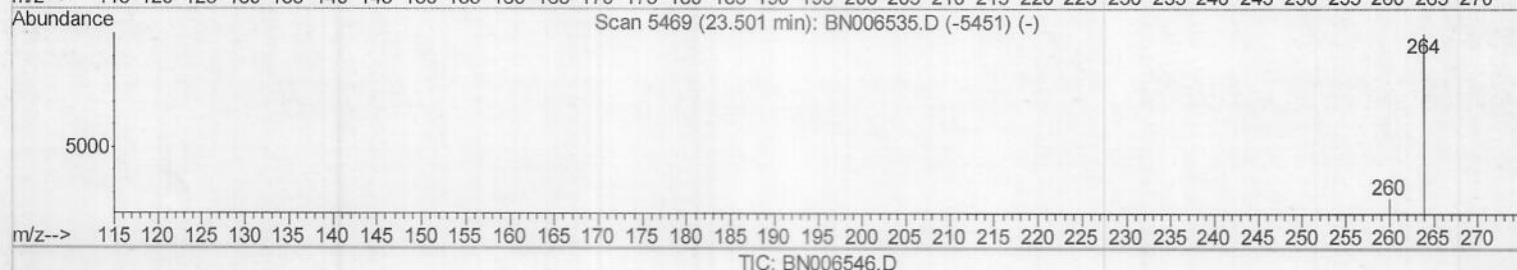
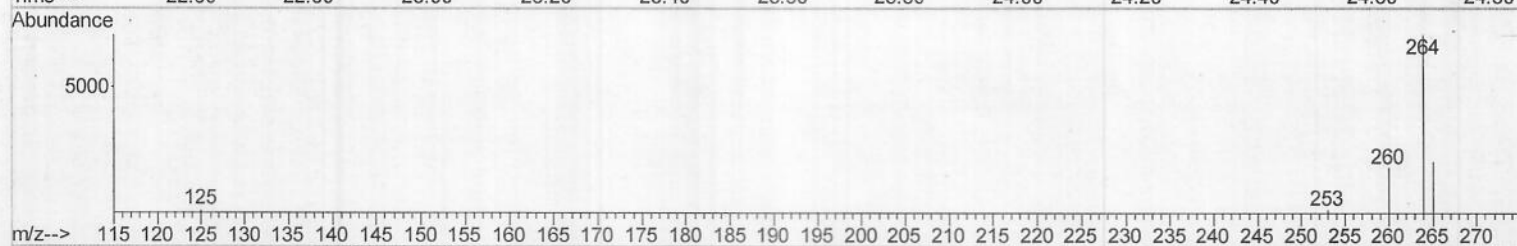
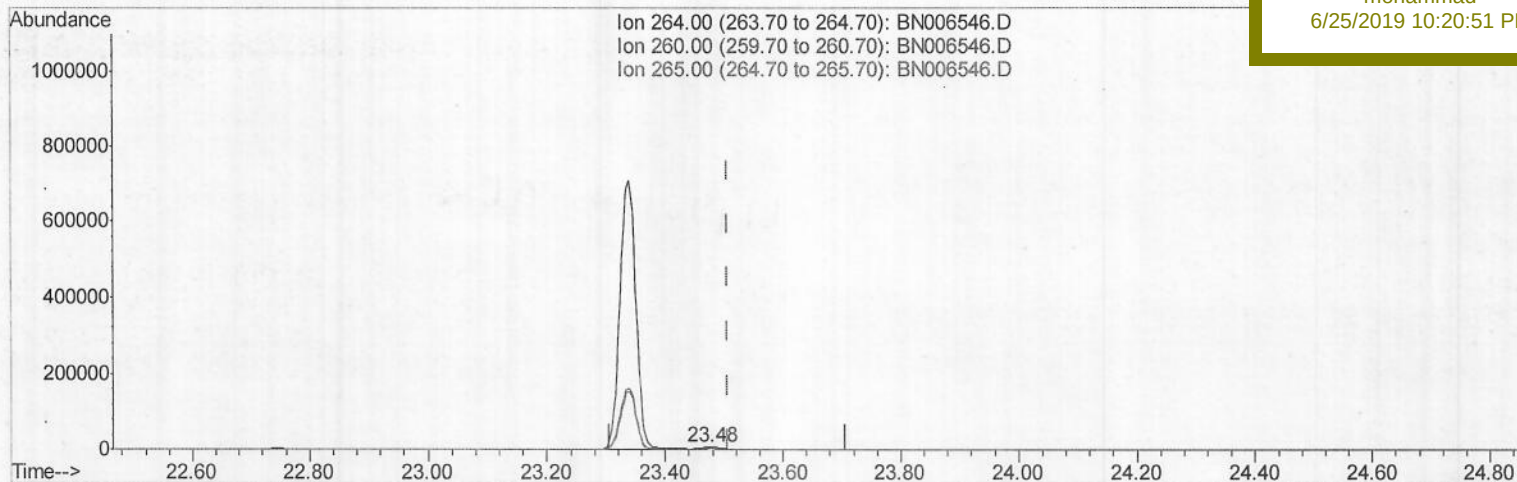
ClientSampleId :

A41X7

Manual Integrations
APPROVED

mohammad

6/25/2019 10:20:51 PM



(20) Perylene-d12 (I)

23.476min (-0.031) 0.40ng/ul

response 15583

Ion	Exp%	Act%
264.00	100	100
260.00	29.20	27.50
265.00	44.70	30.83#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006546.D

Acq On : 24 Jun 2019 23:57

Operator : HP/JU

Sample : K3362-08

Misc :

ALS Vial : 24 Sample Multiplier: 1

Quant Time: Jun 25 04:05:57 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

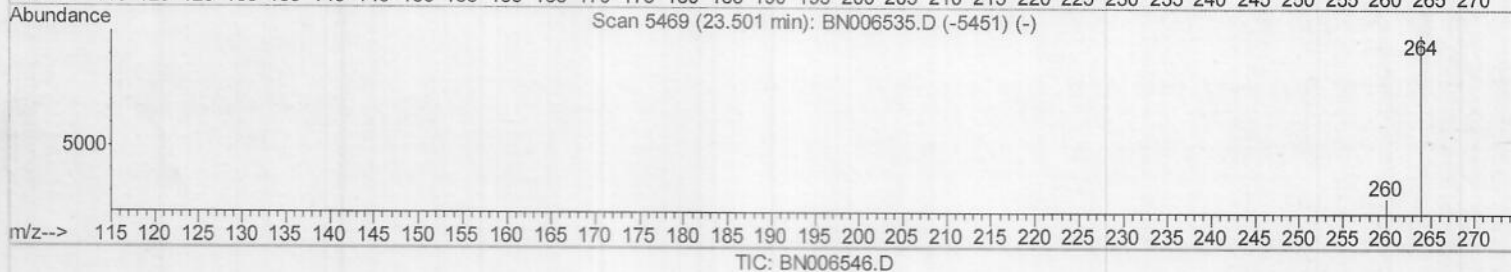
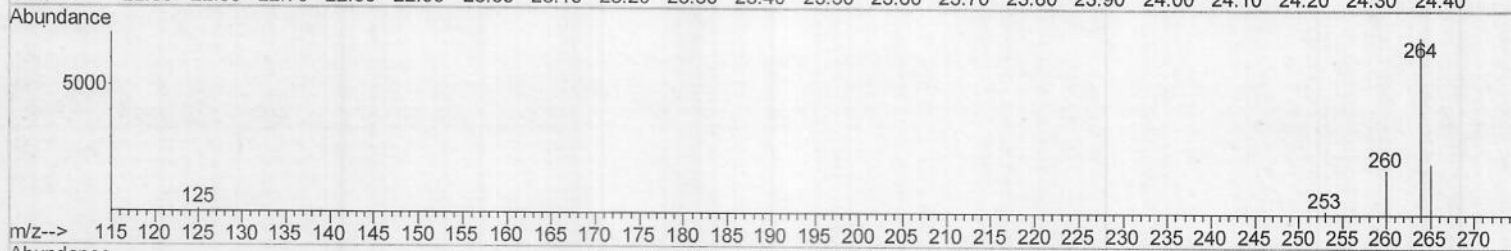
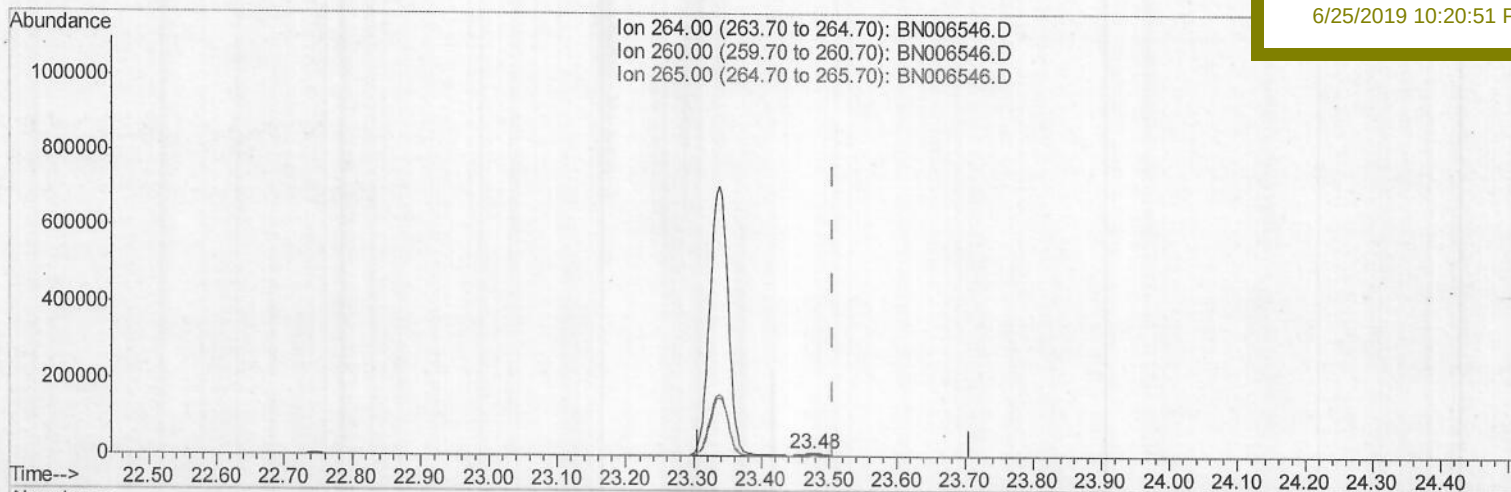
Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A41X7

Manual Integrations
APPROVEDmohammad
6/25/2019 10:20:51 PM

(20) Perylene-d12 (I)

23.476min (-0.031) 0.40ng/ul m

response 10185

Ion	Exp%	Act%
264.00	100	100
260.00	29.20	27.50
265.00	44.70	30.83#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006546.D

Acq On : 24 Jun 2019 23:57

Operator : HP/JU

Sample : K3362-08

Misc :

ALS Vial : 24 Sample Multiplier: 1

Quant Time: Jun 25 04:07:52 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

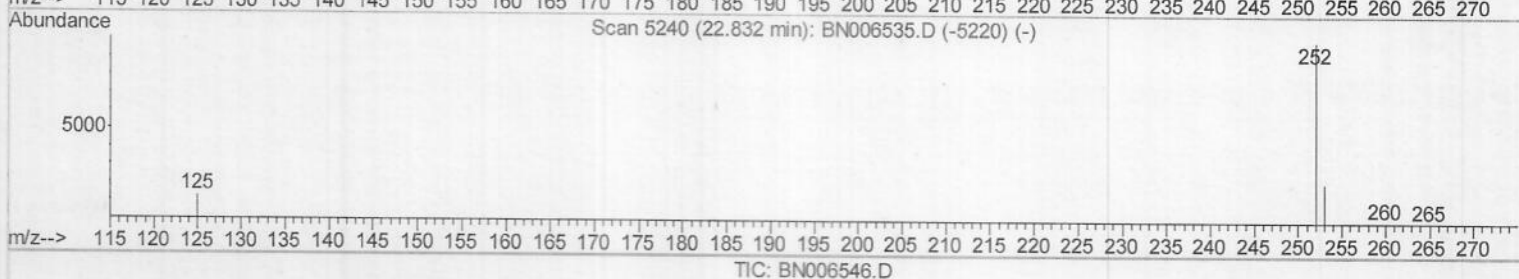
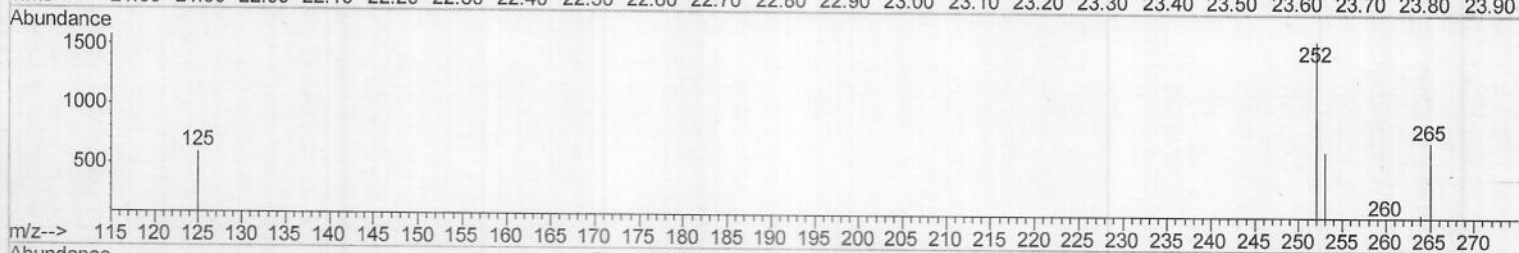
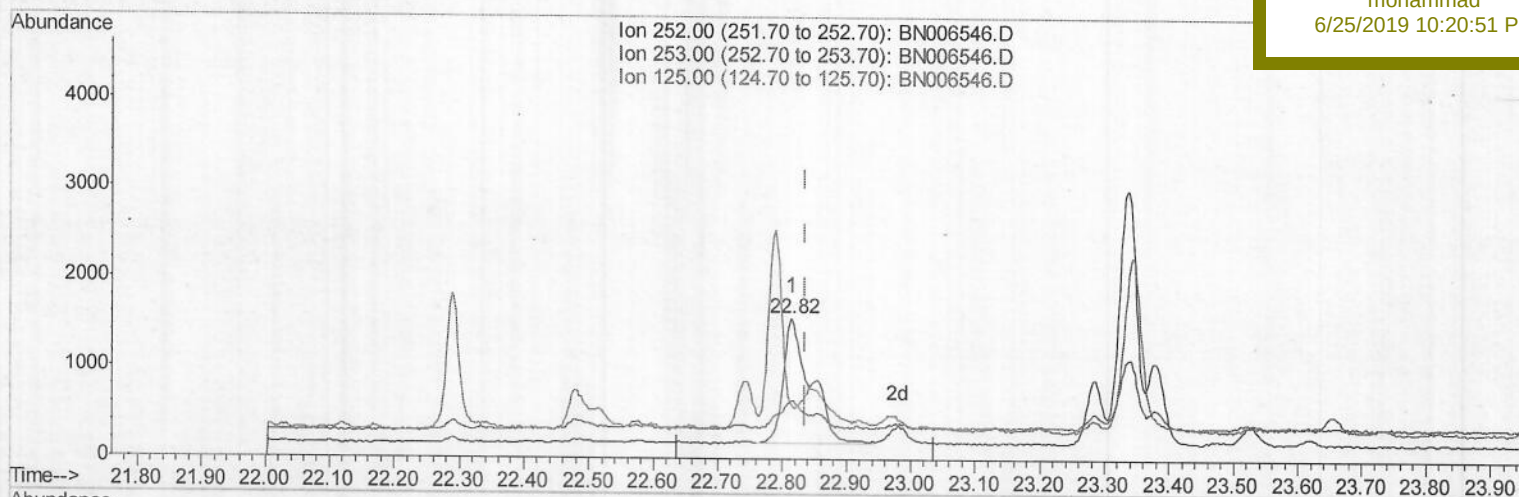
Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A41X7

Manual Integrations
APPROVEDmohammad
6/25/2019 10:20:51 PM

(21) Benzo(b)fluoranthene

22.815min (-0.022) 0.10ng/ul

response 4127

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	41.07
125.00	20.50	37.76
0.00	0.00	0.00

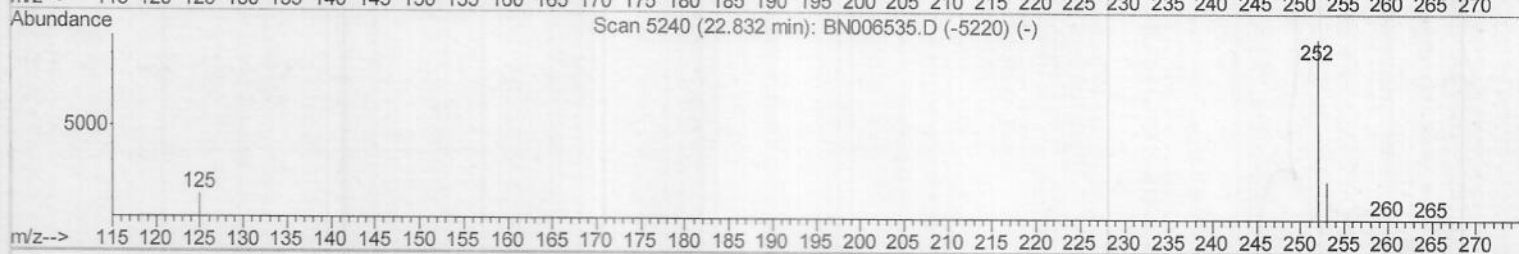
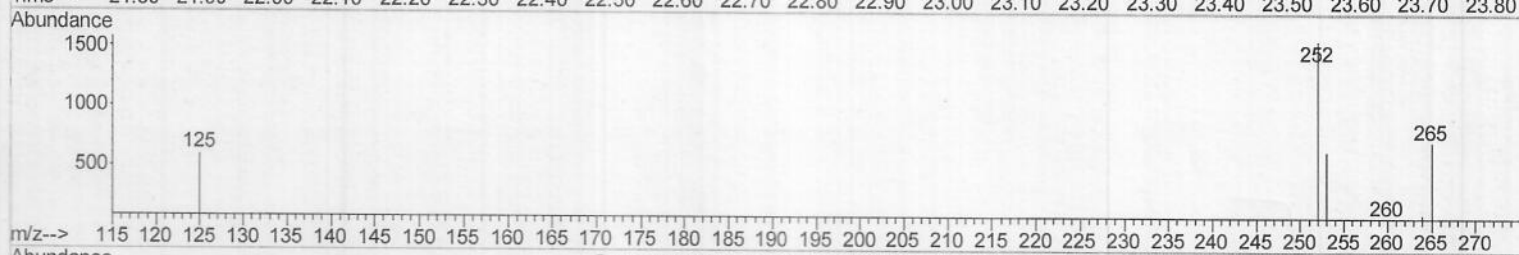
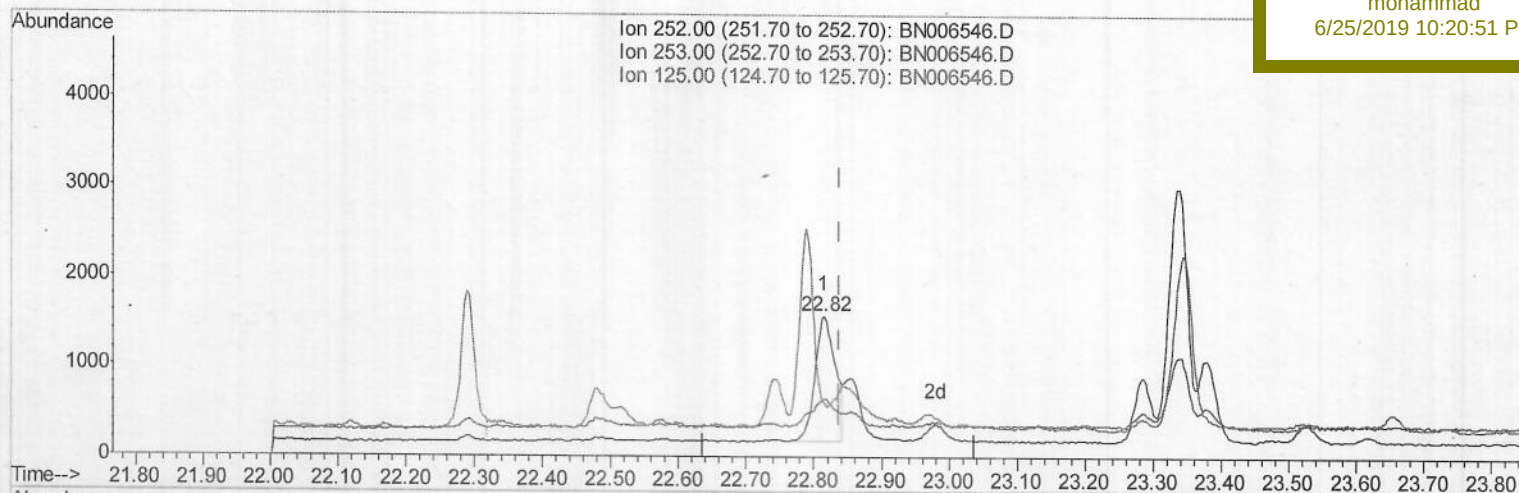
Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006546.D
Acq On : 24 Jun 2019 23:57
Operator : HP/JU
Sample : K3362-08
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Jun 25 04:07:52 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 17 11:13:07 2019
Response via : Initial Calibration

Instrument :
BNA_N
Client Sampled :
A41X7

Manual Integrations
APPROVED

mohammad
6/25/2019 10:20:51 PM



(21) Benzo(b)fluoranthene

22.815min (-0.022) 0.07ng/ul m

response 2888

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	41.07
125.00	20.50	37.76
0.00	0.00	0.00

7 JU 06/26/19

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006546.D

Acq On : 24 Jun 2019 23:57

Operator : HP/JU

Sample : K3362-08

Misc :

ALS Vial : 24 Sample Multiplier: 1

Quant Time: Jun 25 04:07:52 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

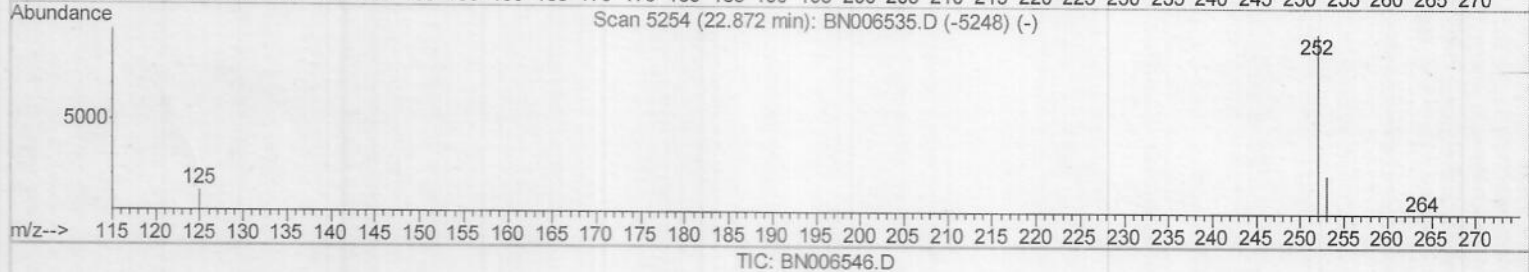
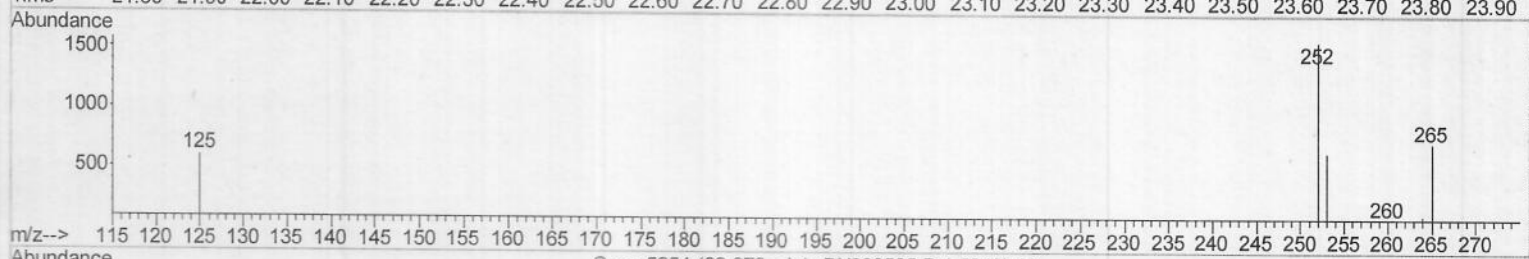
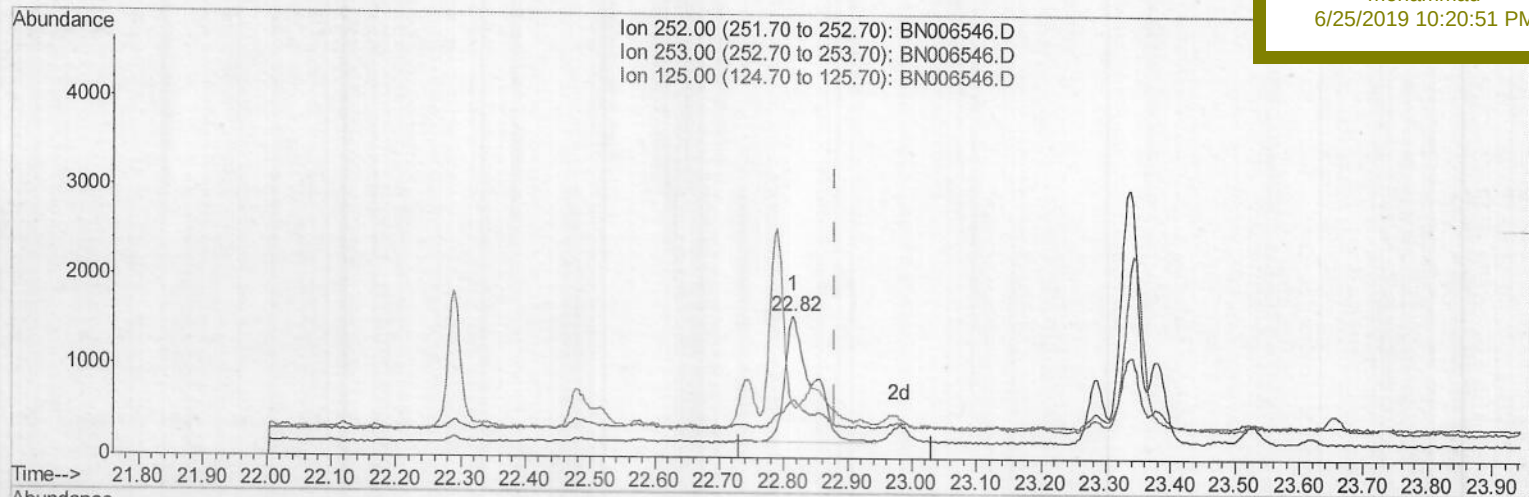
Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A41X7

Manual Integrations
APPROVEDmohammad
6/25/2019 10:20:51 PM

(22) Benzo(k)fluoranthene

22.815min (-0.066) 0.10ng/ul

response 4127

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	41.07#
125.00	17.90	37.76#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006546.D

Acq On : 24 Jun 2019 23:57

Operator : HP/JU

Sample : K3362-08

Misc :

ALS Vial : 24 Sample Multiplier: 1

Quant Time: Jun 25 04:07:52 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 17 11:13:07 2019

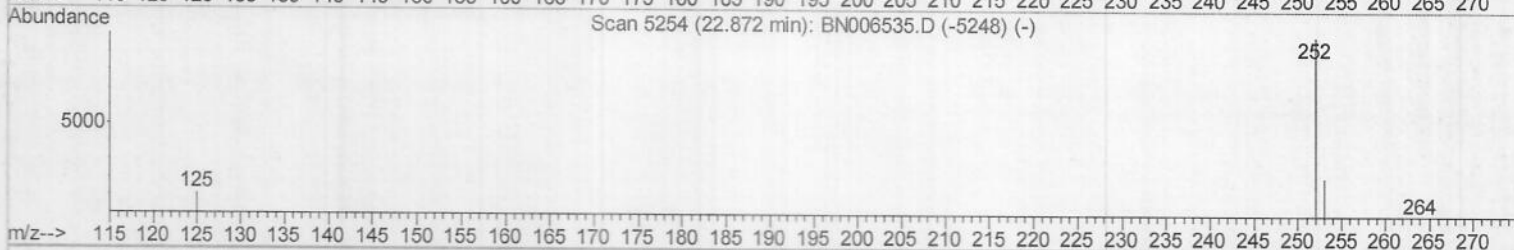
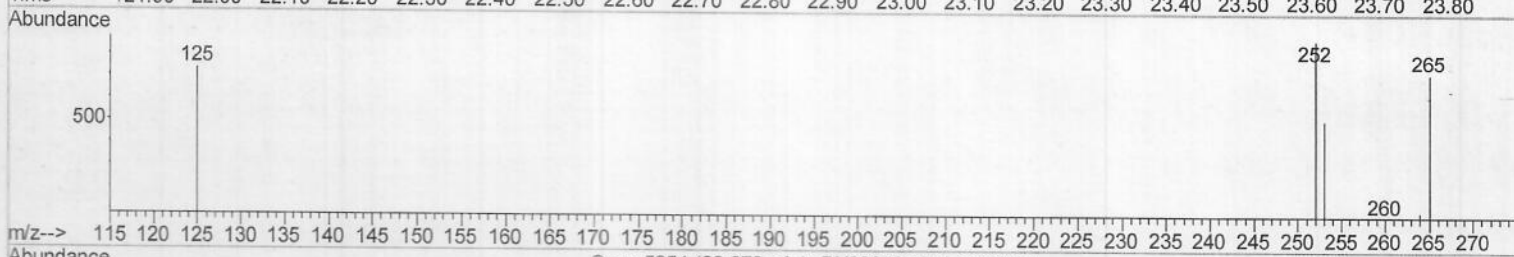
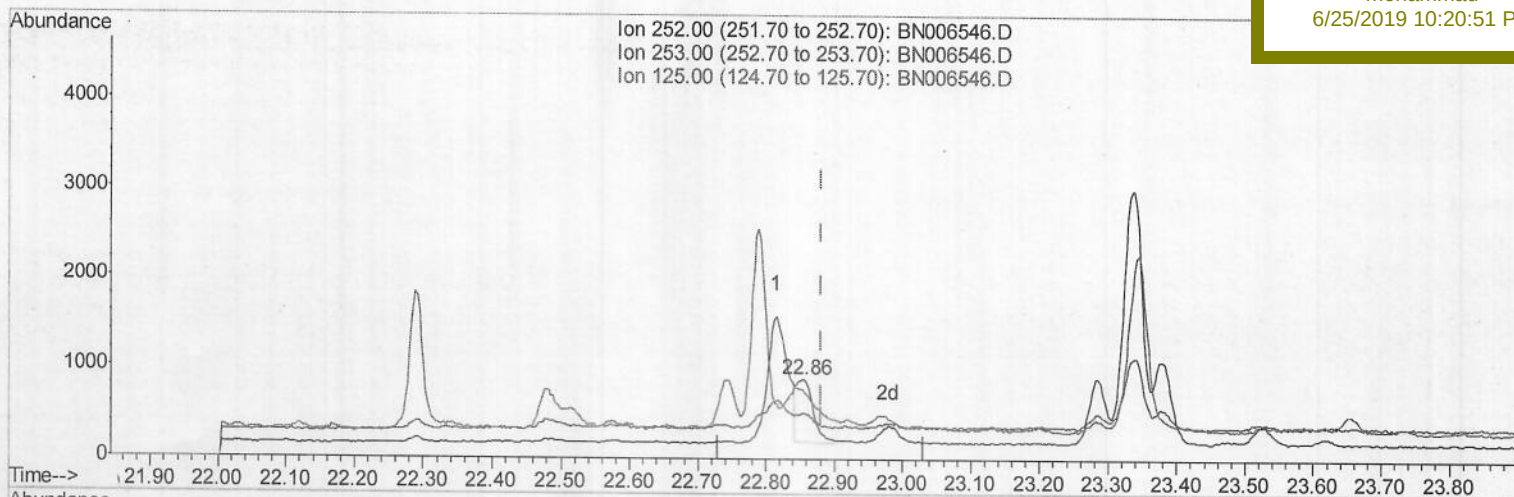
Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A41X7

Manual Integrations
APPROVEDmohammad
6/25/2019 10:20:51 PM

TIC: BN006546.D

(22) Benzo(k)fluoranthene

22.856min (-0.025) 0.03ng/ul m

response 1182

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	58.04#
125.00	17.90	83.92#
0.00	0.00	0.00

> JU 06/26/19

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
 Data File : BN006546.D
 Acq On : 24 Jun 2019 23:57
 Operator : HP/JU
 Sample : K3362-08
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Quant Time: Jun 25 04:08:36 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 17 11:13:07 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 A41X7

Manual Integrations
 APPROVED

mohammad
 6/25/2019 10:20:51 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	5551	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.41	136	20882	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.28	164	11029	0.40	ng/ul	-0.01
10) Phenanthrene-d10	17.04	188	20881m7	0.40	ng/ul	-0.02
16) Chrysene-d12	21.25	240	11657m7	0.40	ng/ul	-0.02
20) Perylene-d12	23.48	264	10185m7	0.40	ng/ul	-0.03
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.01	152	15800	0.49	ng/ul	-0.02
14) Fluoranthene-d10	19.08	212	27882m7	0.50	ng/ul	-0.01
Target Compounds						
12) Phenanthrene	17.08	178	2197m7	0.033	ng/ul	Qvalue
15) Fluoranthene	19.11	202	6170m7	0.083	ng/ul	
17) Pyrene	19.47	202	3914	0.064	ng/ul#	87
18) Benzo(a)anthracene	21.23	228	1527m7	0.030	ng/ul	
19) Chrysene	21.29	228	2176m7	0.045	ng/ul	
21) Benzo(b)fluoranthene	22.82	252	2888m7	0.068	ng/ul	
22) Benzo(k)fluoranthene	22.86	252	1182m7	0.029	ng/ul	
23) Benzo(a)pyrene	23.38	252	1484	0.038	ng/ul#	57
24) Indeno(1,2,3-cd)pyrene	25.72	276	1378	0.032	ng/ul#	62
26) Benzo(g,h,i)perylene	26.40	276	1205	0.034	ng/ul#	73

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU
 06/26/19