


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006553.D
Acq On : 25 Jun 2019 04:07
Operator : HP/JU
Sample : K3388-08
Misc :
ALS Vial : 30 Sample Multiplier: 1

Quant Time: Jun 25 07:21:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 25 01:51:13 2019
Response via : Initial Calibration

Instrument :
BNA_N
Client Sampled :
A4219

Manual Integrations
APPROVED

mohammad
6/25/2019 10:21:13 PM

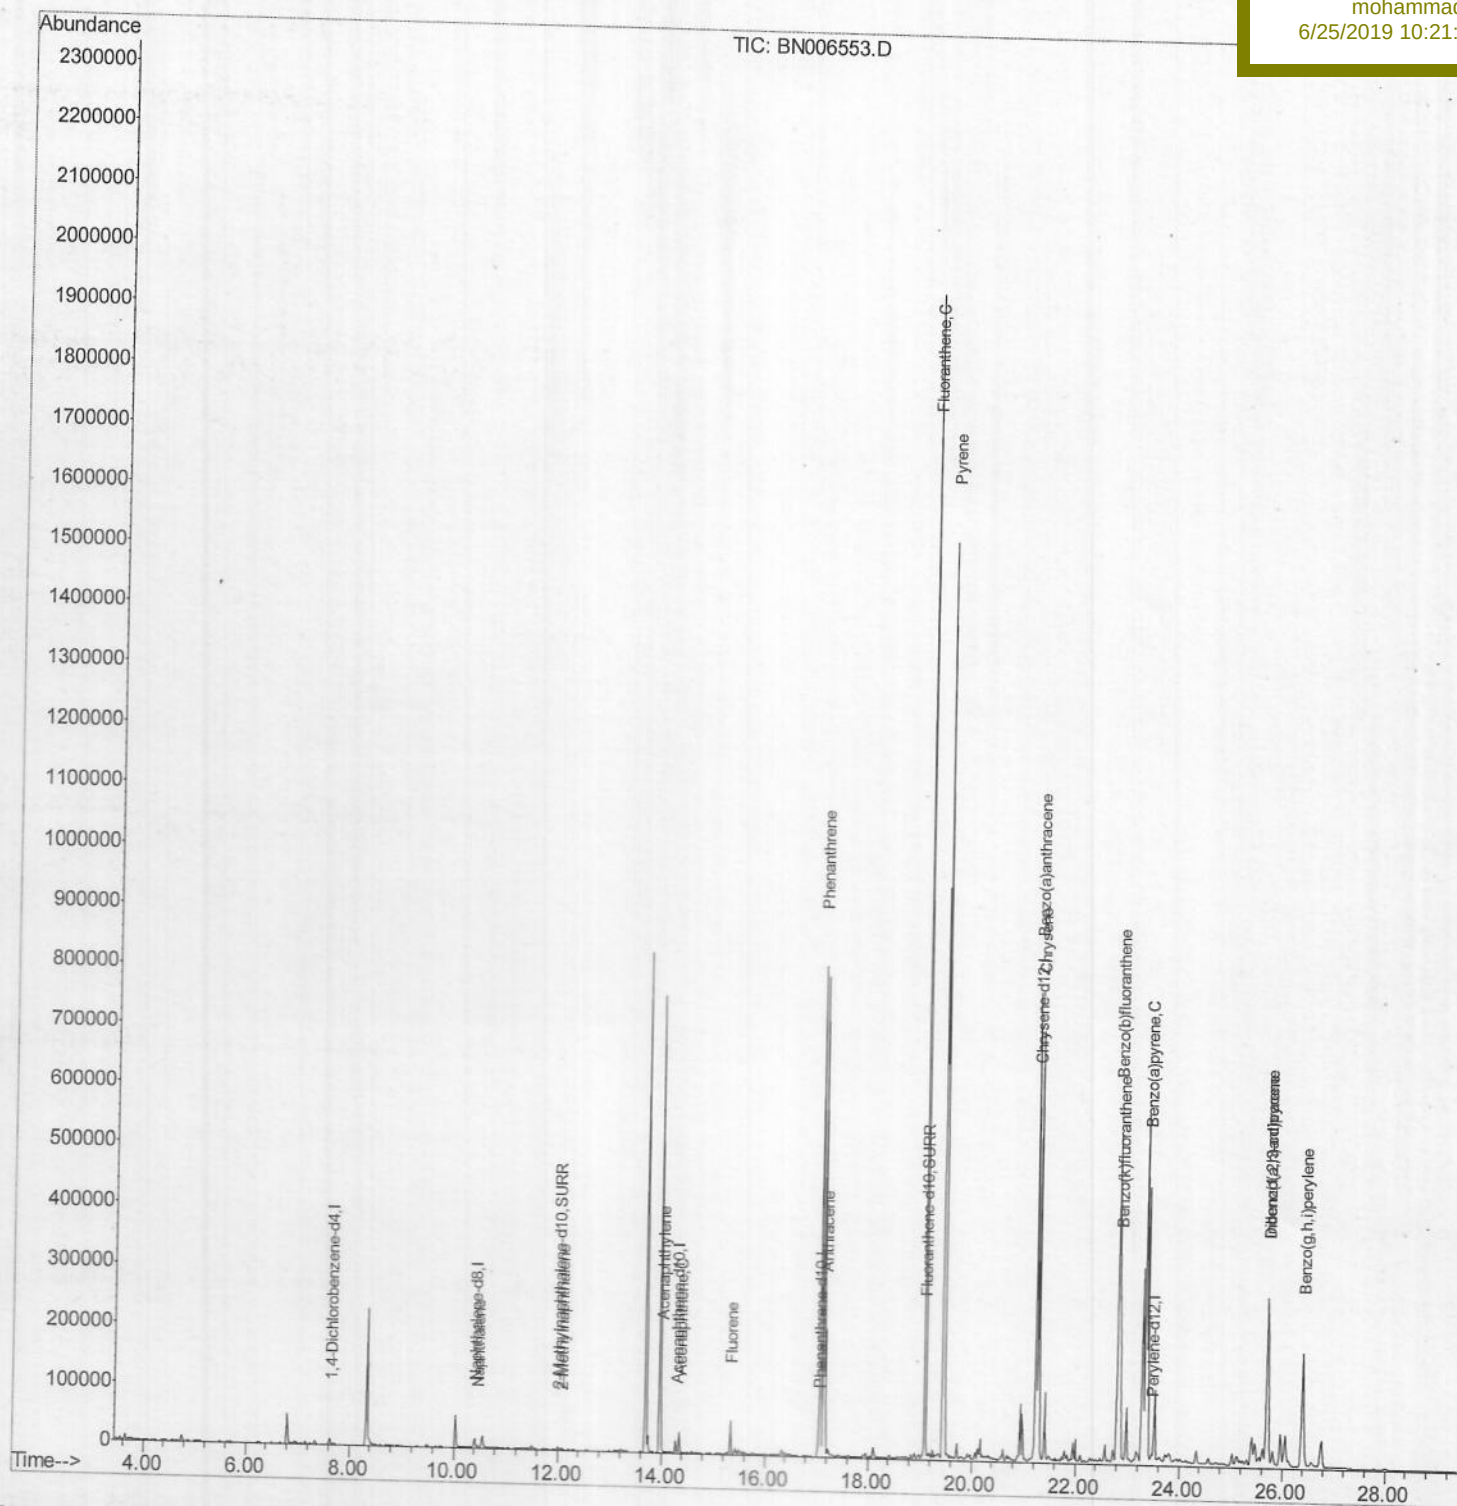

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
 Data File : BN006553.D
 Acq On : 25 Jun 2019 04:07
 Operator : HP/JU
 Sample : K3388-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4219

Manual Integrations
 APPROVED

mohammad
 6/25/2019 10:21:13 PM

Quant Time: Jun 25 07:11:38 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 25 01:51:13 2019
 Response via : Initial Calibration

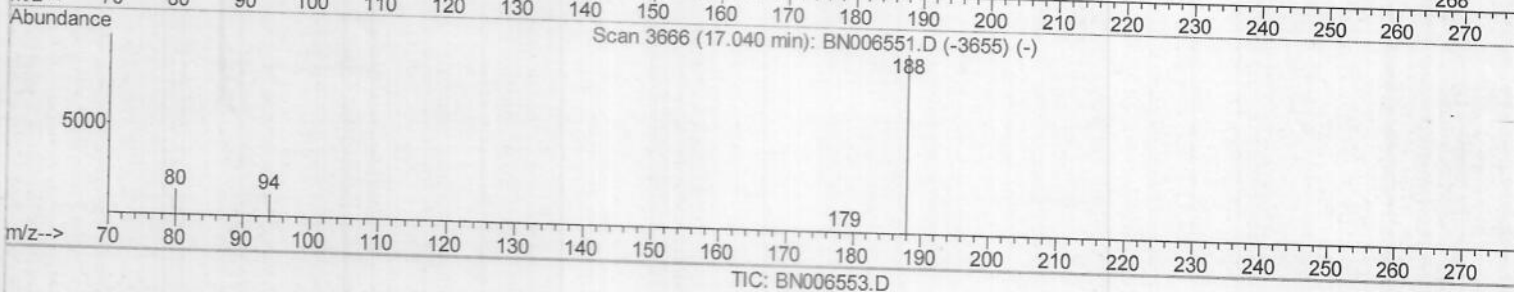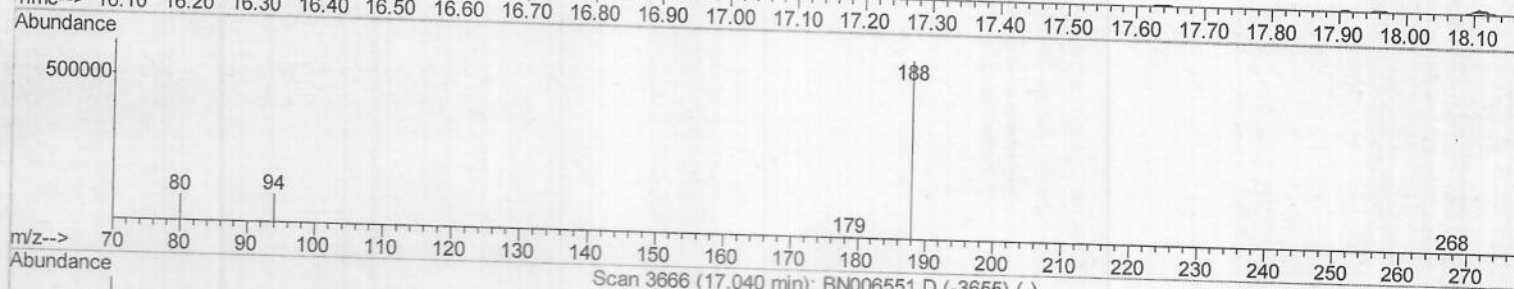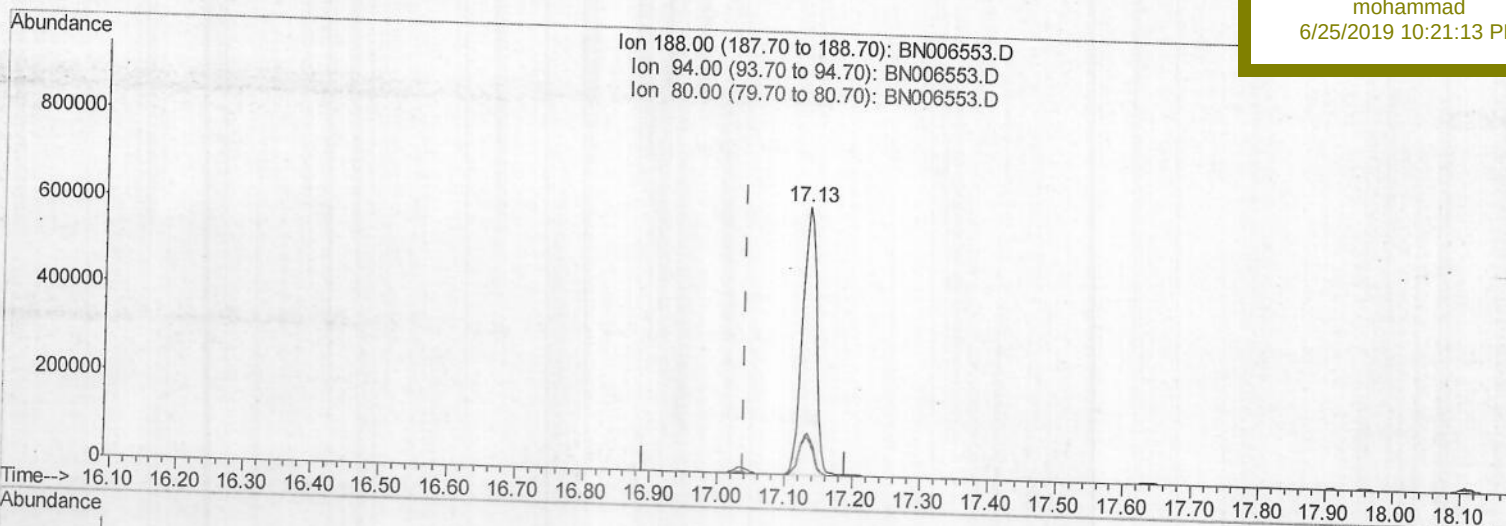

(10) Phenanthrene-d10 (I)
 17.133min (+0.093) 0.40ng/ul
 response 876990

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	15.67#
80.00	13.60	14.32
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
 Data File : BN006553.D
 Acq On : 25 Jun 2019 04:07
 Operator : HP/JU
 Sample : K3388-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4219

Manual Integrations
 APPROVED

mohammad
 6/25/2019 10:21:13 PM

Quant Time: Jun 25 07:11:38 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 25 01:51:13 2019
 Response via : Initial Calibration

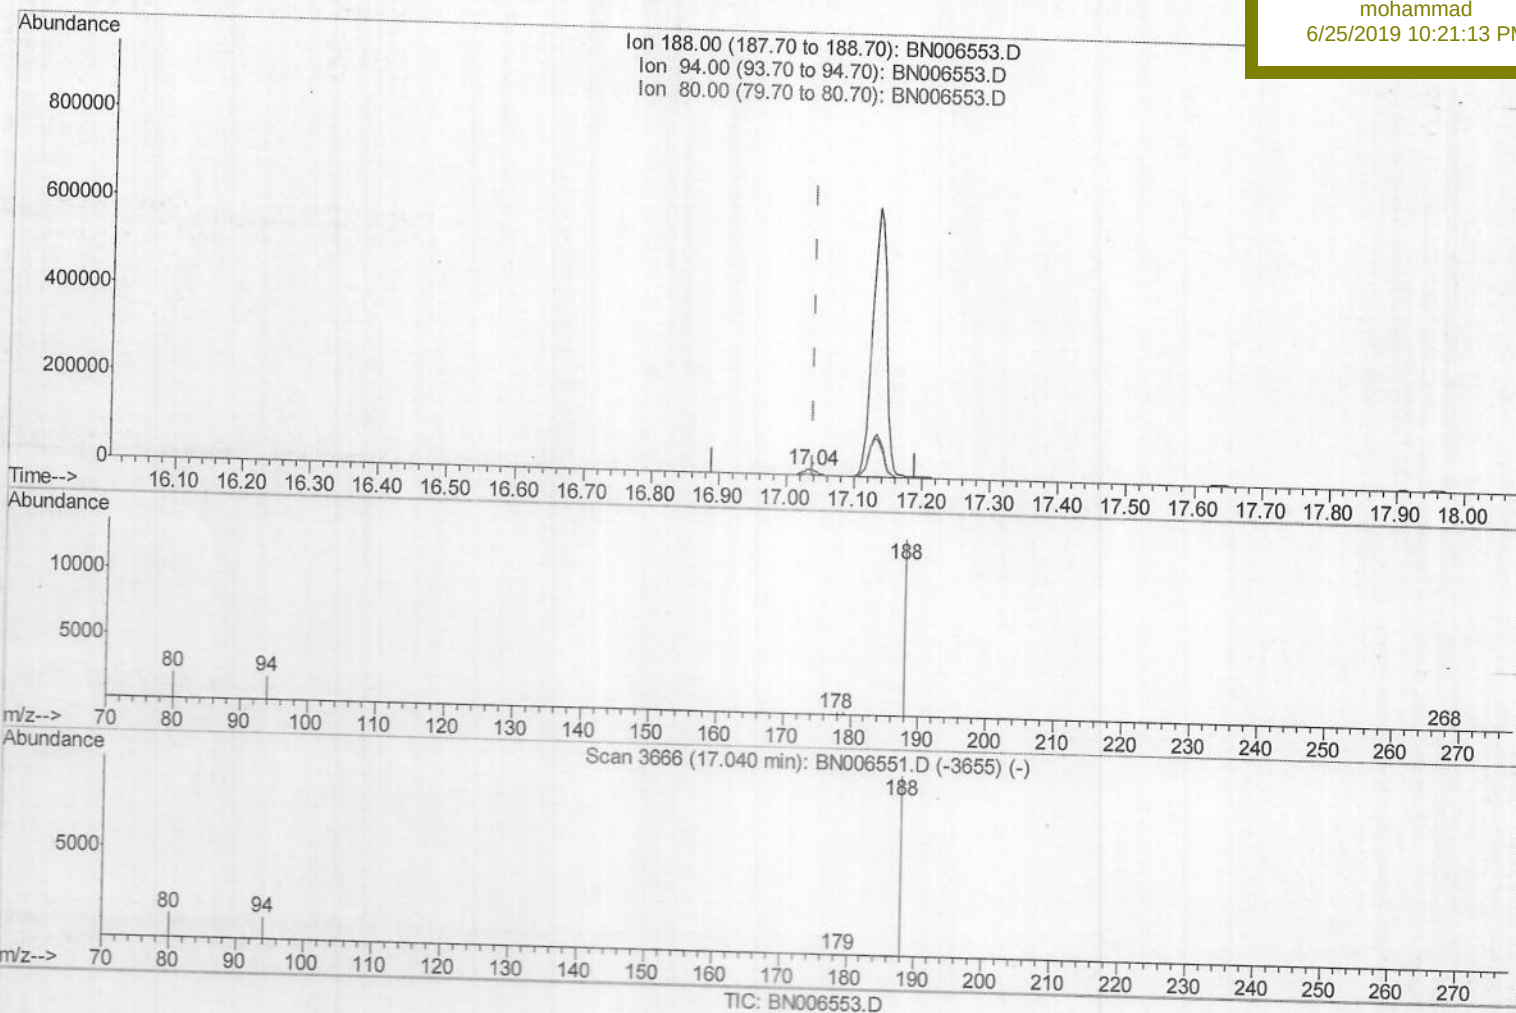

(10) Phenanthrene-d10 (I)

17.035min (-0.004) 0.40ng/ul m

response 18631

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	13.53
80.00	13.60	15.03
0.00	0.00	0.00

> JU 06/27/19

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
 Data File : BN006553.D
 Acq On : 25 Jun 2019 04:07
 Operator : HP/JU
 Sample : K3388-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Quant Time: Jun 25 07:18:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 25 01:51:13 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 A4219

Manual Integrations
 APPROVED

mohammad
 6/25/2019 10:21:13 PM

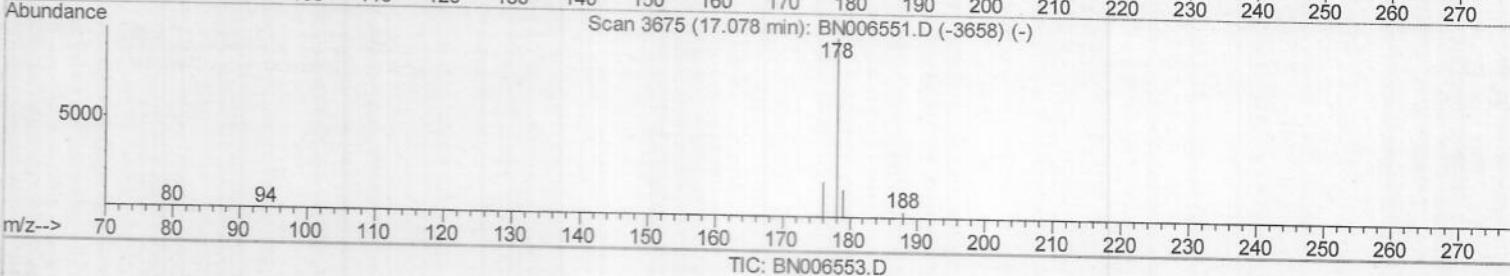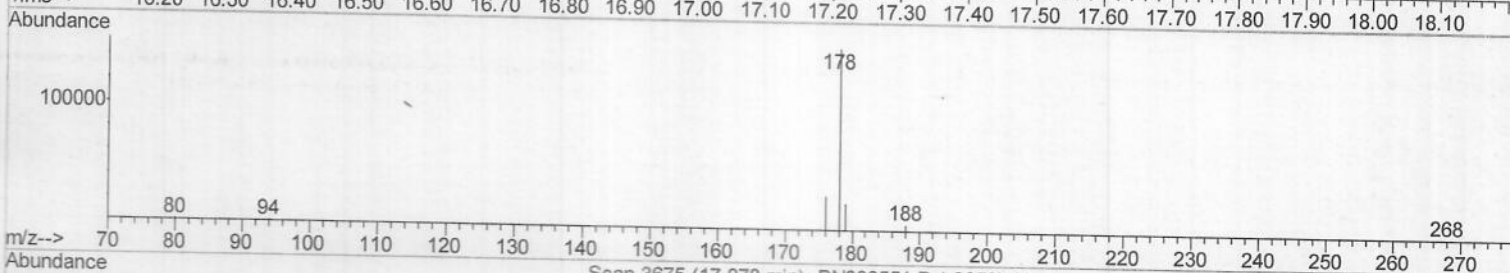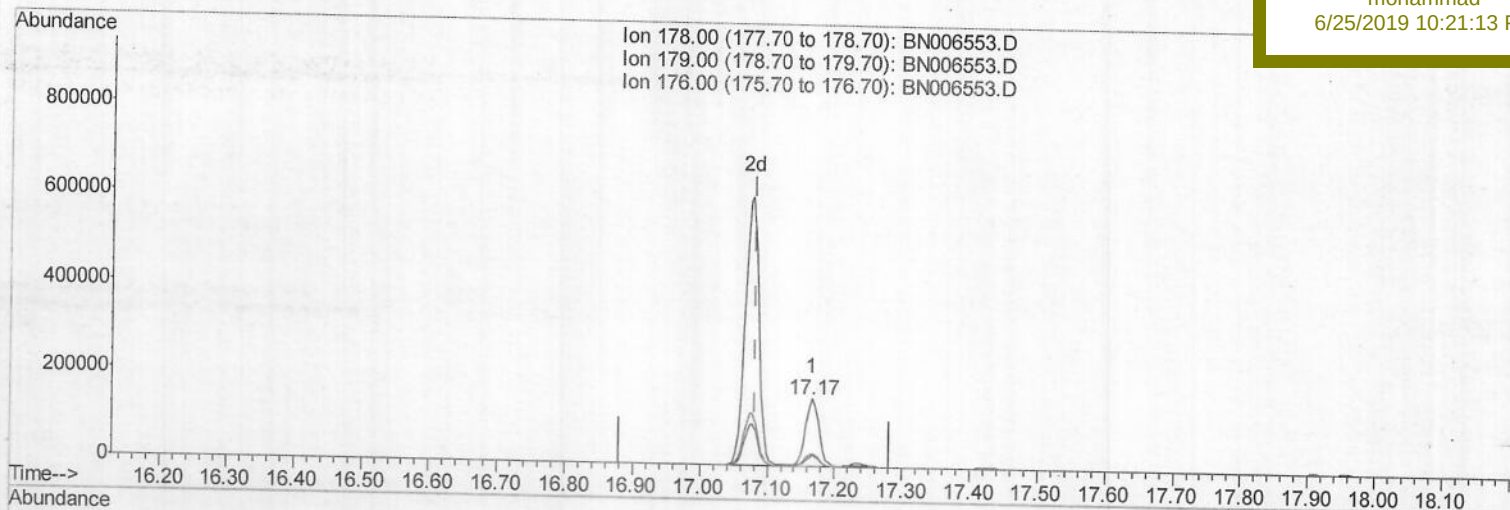

(12) Phenanthrene

17.166min (+0.084) 3.50ng/ul

response 209299

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	15.45
176.00	19.10	18.92
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
 Data File : BN006553.D
 Acq On : 25 Jun 2019 04:07
 Operator : HP/JU
 Sample : K3388-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4219

Manual Integrations
 APPROVED

mohammad
 6/25/2019 10:21:13 PM

Quant Time: Jun 25 07:18:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 25 01:51:13 2019
 Response via : Initial Calibration

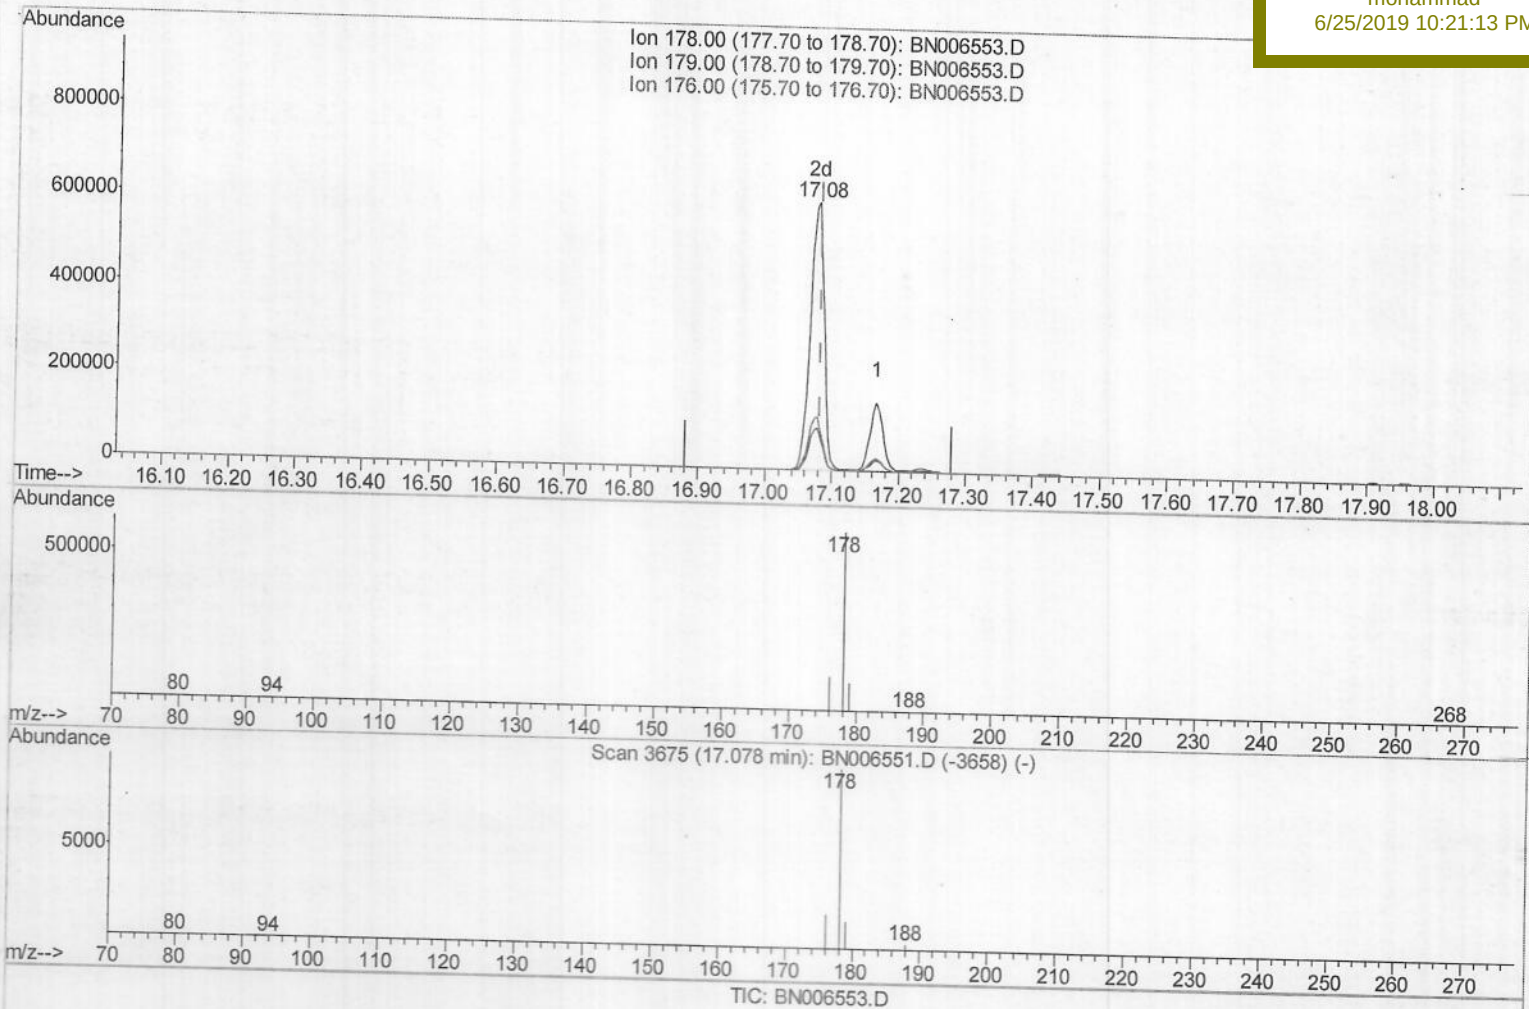

(12) Phenanthrene

17.078min (-0.004) 14.28ng/ul m

> JU 06/27/19

response 854028

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	15.58
176.00	19.10	19.41
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006553.D

Acq On : 25 Jun 2019 04:07

Operator : HP/JU

Sample : K3388-08

Misc :

ALS Vial : 30 Sample Multiplier: 1

Quant Time: Jun 25 07:18:40 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Jun 25 01:51:13 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A4219

Manual Integrations

APPROVED

mohammad

6/25/2019 10:21:13 PM

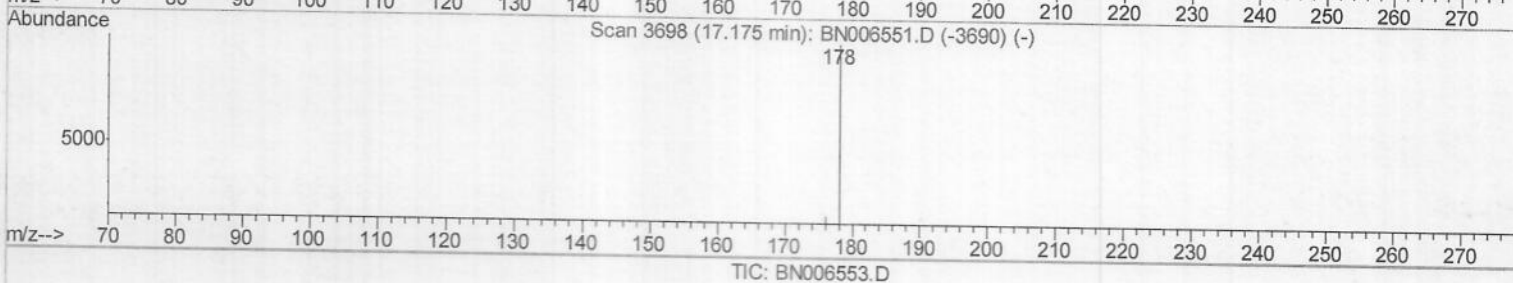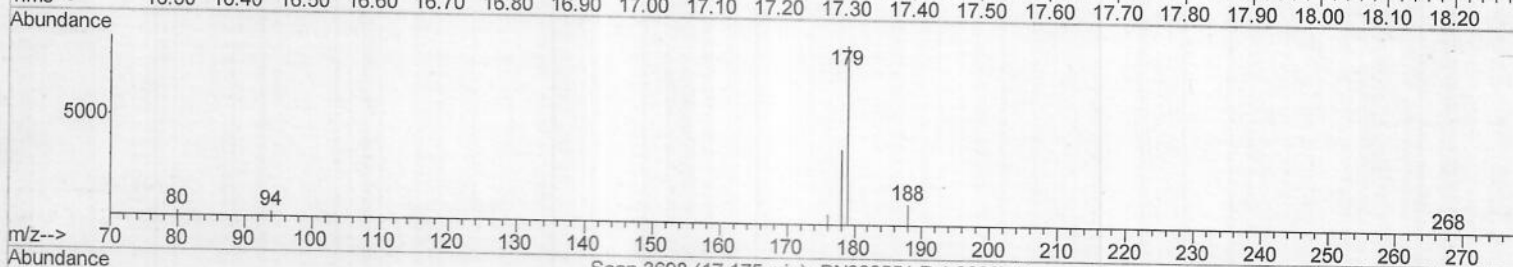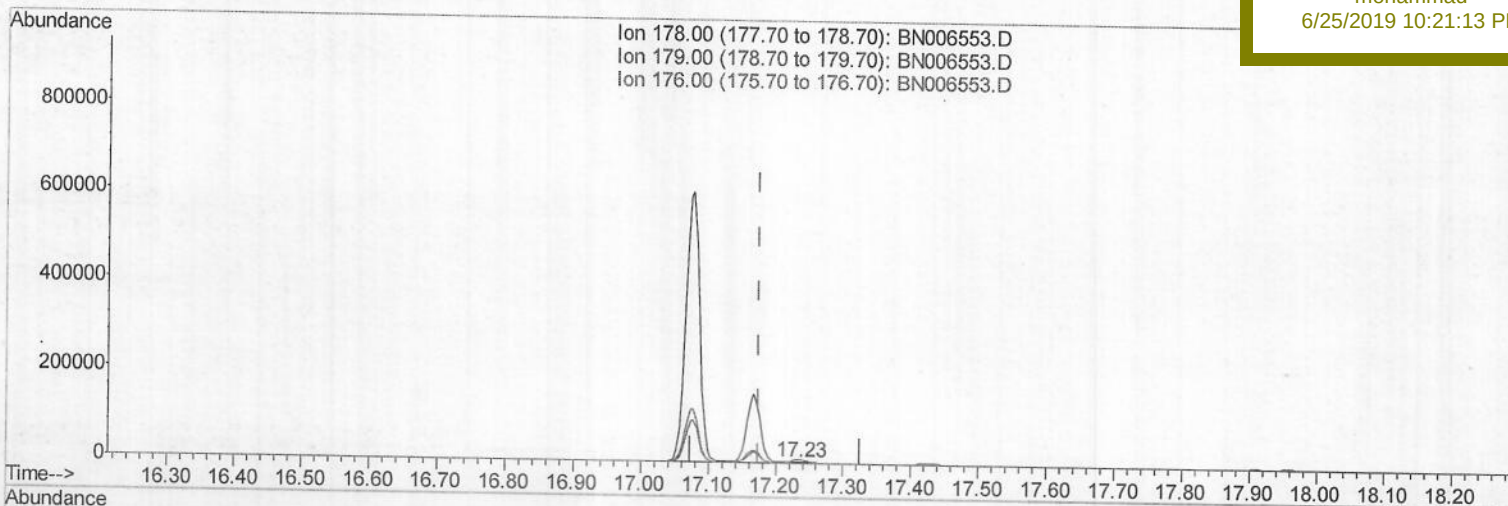

TIC: BN006553.D

(13) Anthracene

17.234min (+0.059) 0.09ng/ul

response 5144

Ion Exp% Act%

178.00 100 100

179.00 15.30 237.10#

176.00 18.90 13.87#

0.00 0.00 0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006553.D

Acq On : 25 Jun 2019 04:07

Operator : HP/JU

Sample : K3388-08

Misc :

ALS Vial : 30 Sample Multiplier: 1

Quant Time: Jun 25 07:18:40 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Jun 25 01:51:13 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




A4219

Manual Integrations

APPROVED

mohammad

6/25/2019 10:21:13 PM

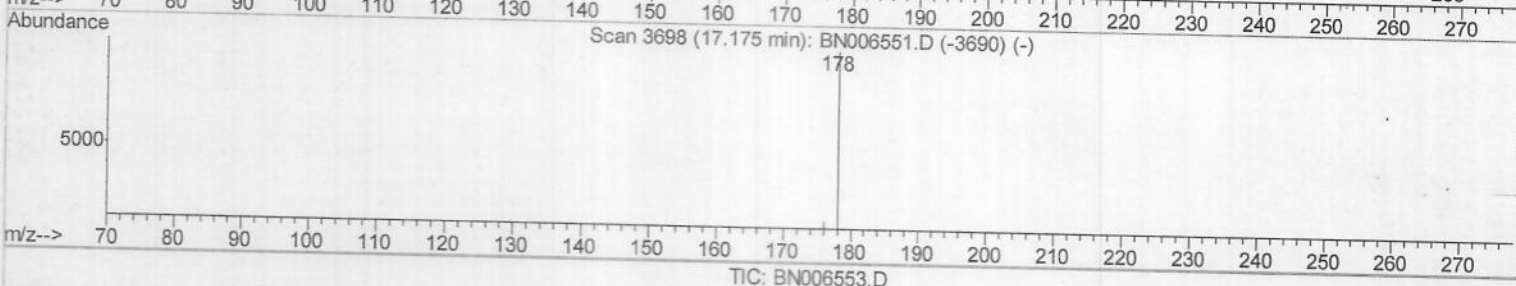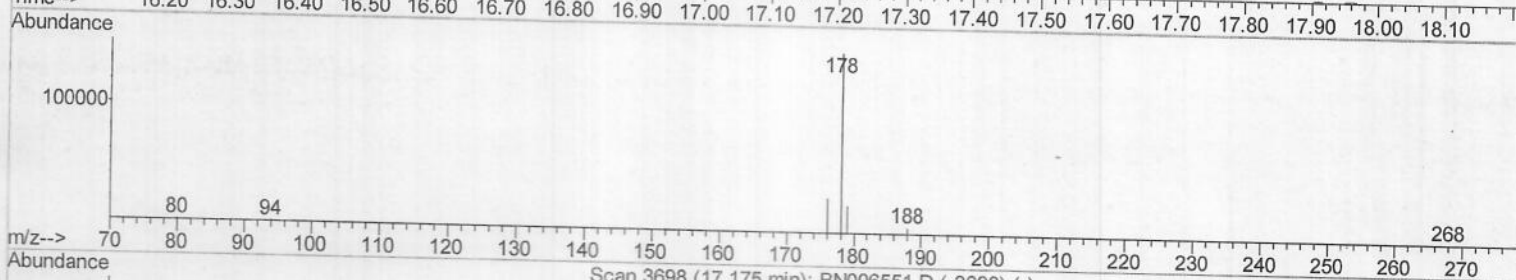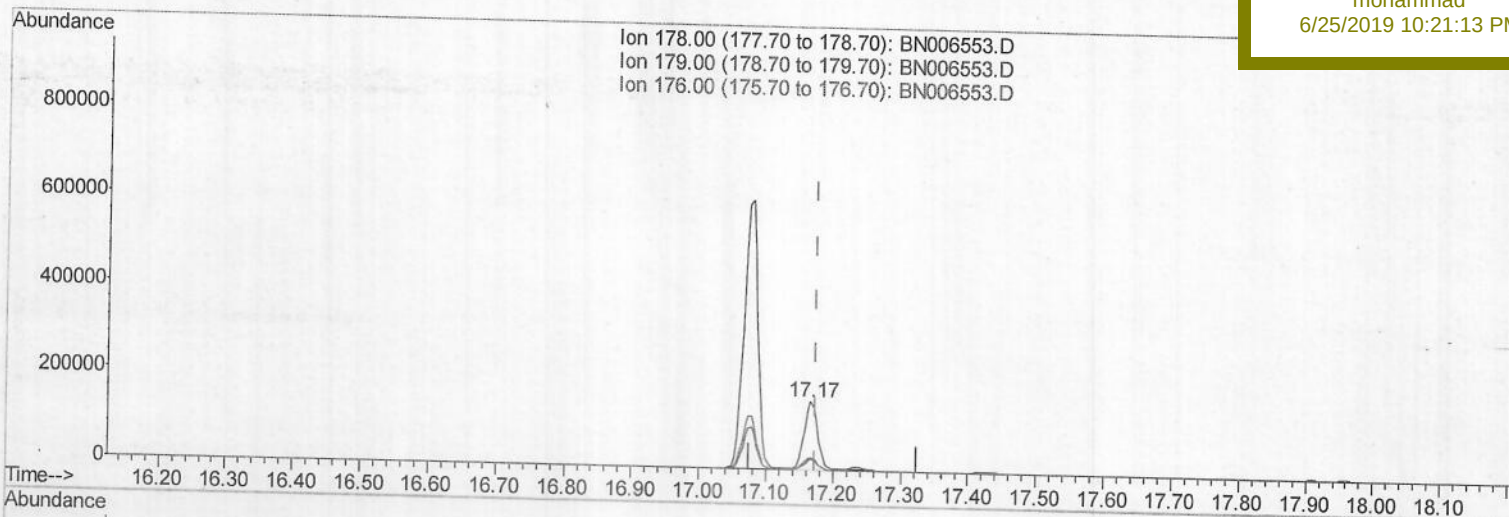

TIC: BN006553.D

(13) Anthracene

17.166min (-0.008) 3.81ng/ul m 7 JU 06/27/19

response 217465

Ion	Exp%	Act%
178.00	100	100
179.00	15.30	15.45
176.00	18.90	18.92
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
 Data File : BN006553.D
 Acq On : 25 Jun 2019 04:07
 Operator : HP/JU
 Sample : K3388-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4219

Manual Integrations
 APPROVED

mohammad
 6/25/2019 10:21:13 PM

Quant Time: Jun 25 07:18:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 25 01:51:13 2019
 Response via : Initial Calibration

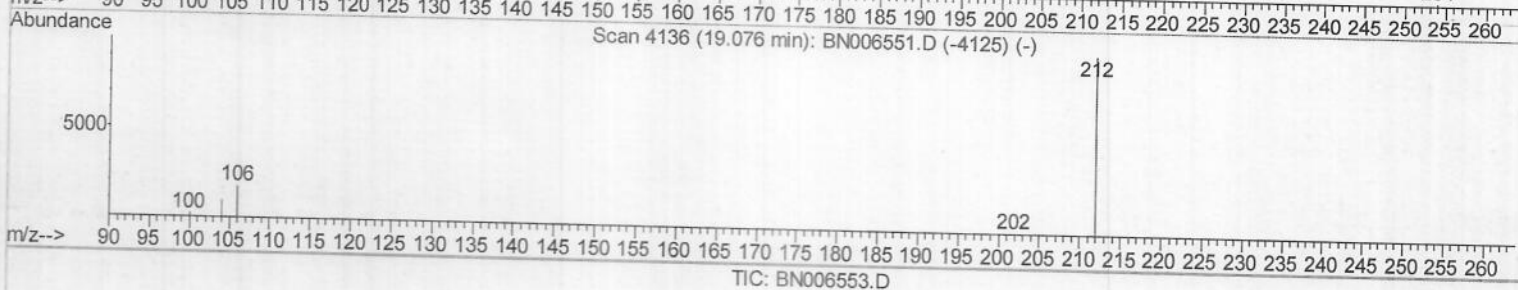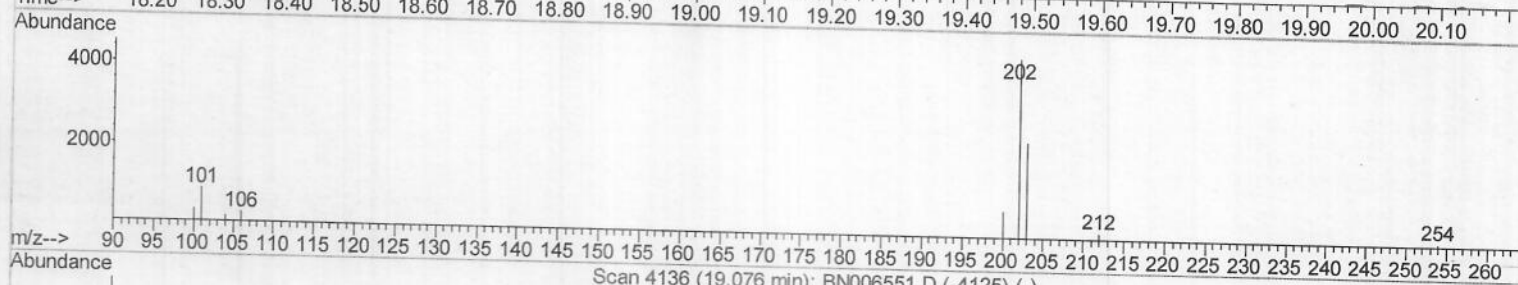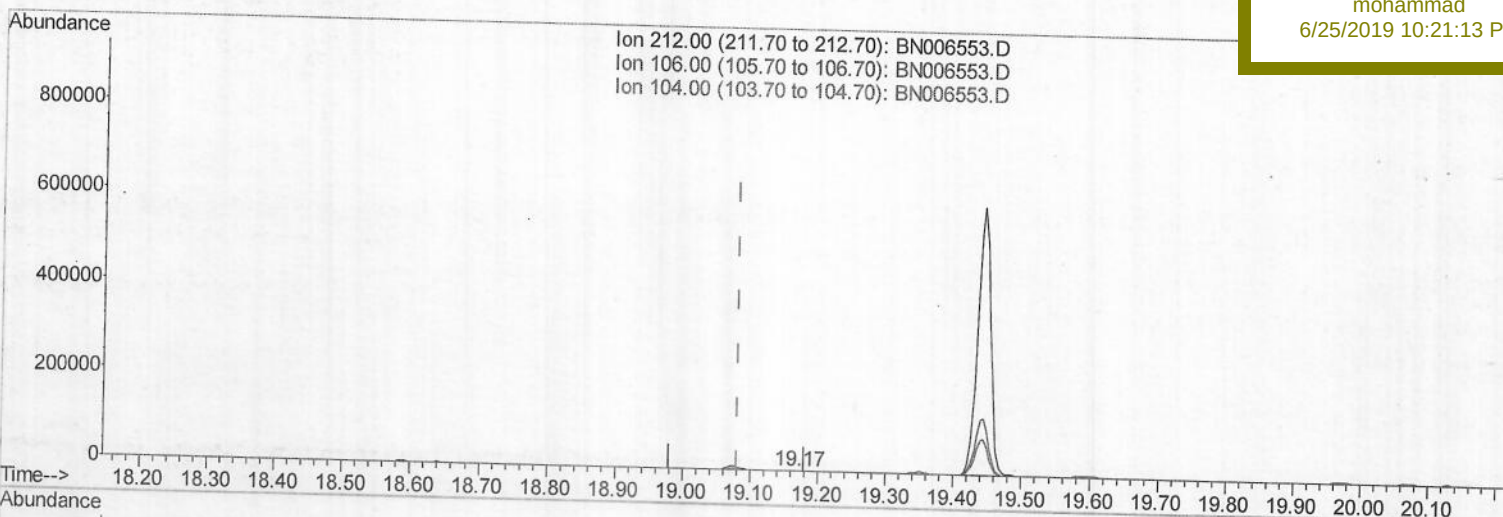

(14) Fluoranthene-d10 (SURR)

19.169min (+0.088) 0.00ng/ul

response 241

Ion	Exp%	Act%
212.00	100	100
106.00	18.10	0.00#
104.00	9.90	67.22#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
 Data File : BN006553.D
 Acq On : 25 Jun 2019 04:07
 Operator : HP/JU
 Sample : K3388-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4219

Quant Time: Jun 25 07:18:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 25 01:51:13 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 6/25/2019 10:21:13 PM

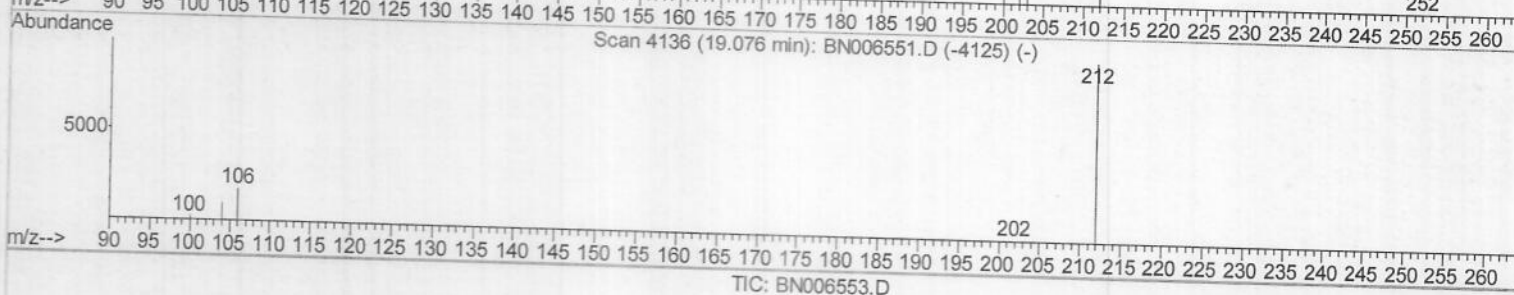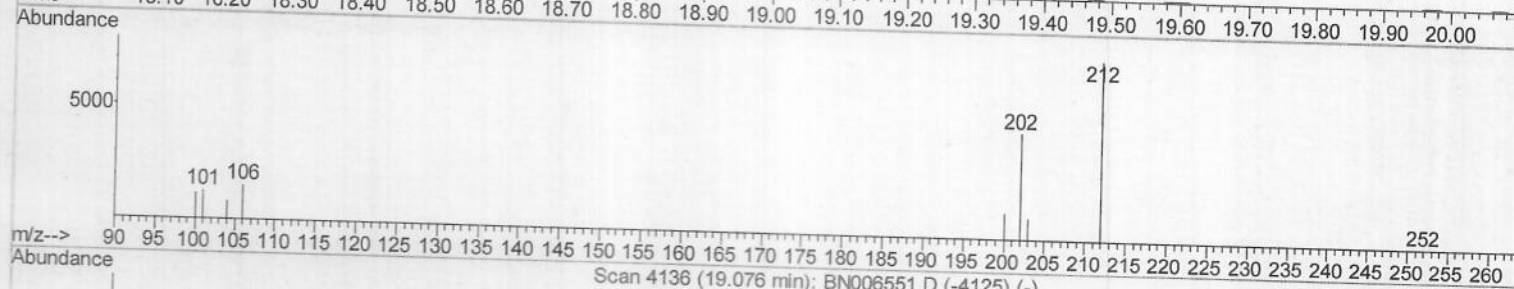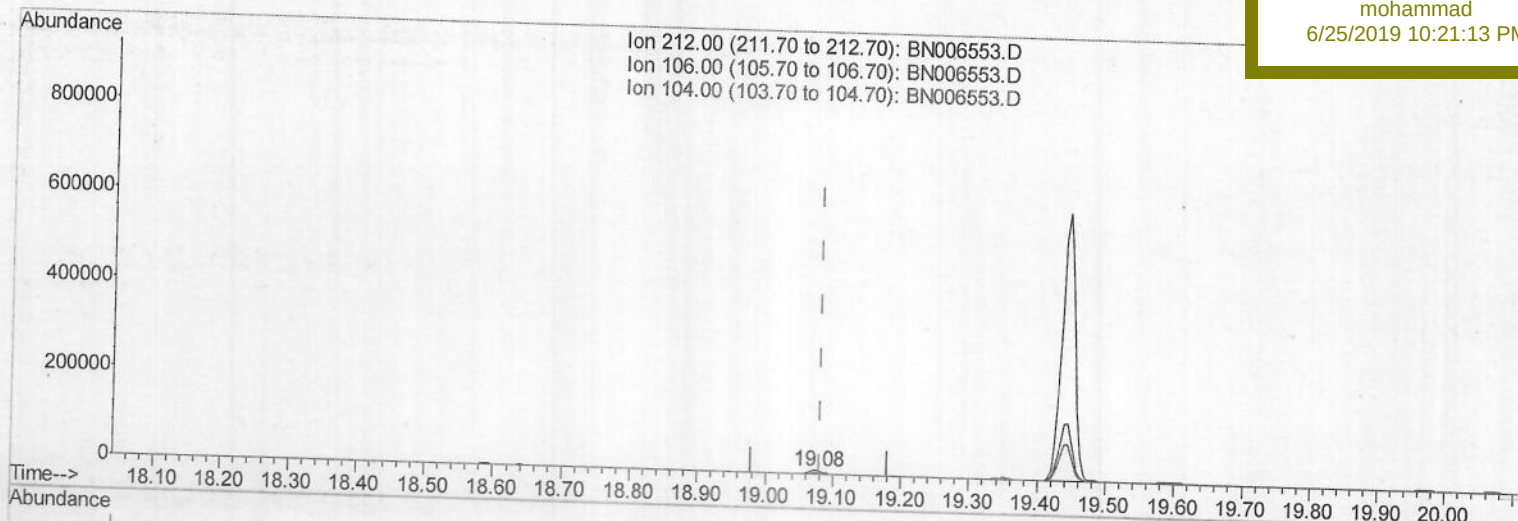

(14) Fluoranthene-d10 (SURR)

19.076min (-0.005) 0.22ng/ul m

response 11030

Ion	Exp%	Act%
212.00	100	100
106.00	18.10	0.00#
104.00	9.90	1.47#
0.00	0.00	0.00

> JU 06/24/19

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
 Data File : BN006553.D
 Acq On : 25 Jun 2019 04:07
 Operator : HP/JU
 Sample : K3388-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4219

Manual Integrations
 APPROVED

mohammad
 6/25/2019 10:21:13 PM

Quant Time: Jun 25 07:18:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 25 01:51:13 2019
 Response via : Initial Calibration

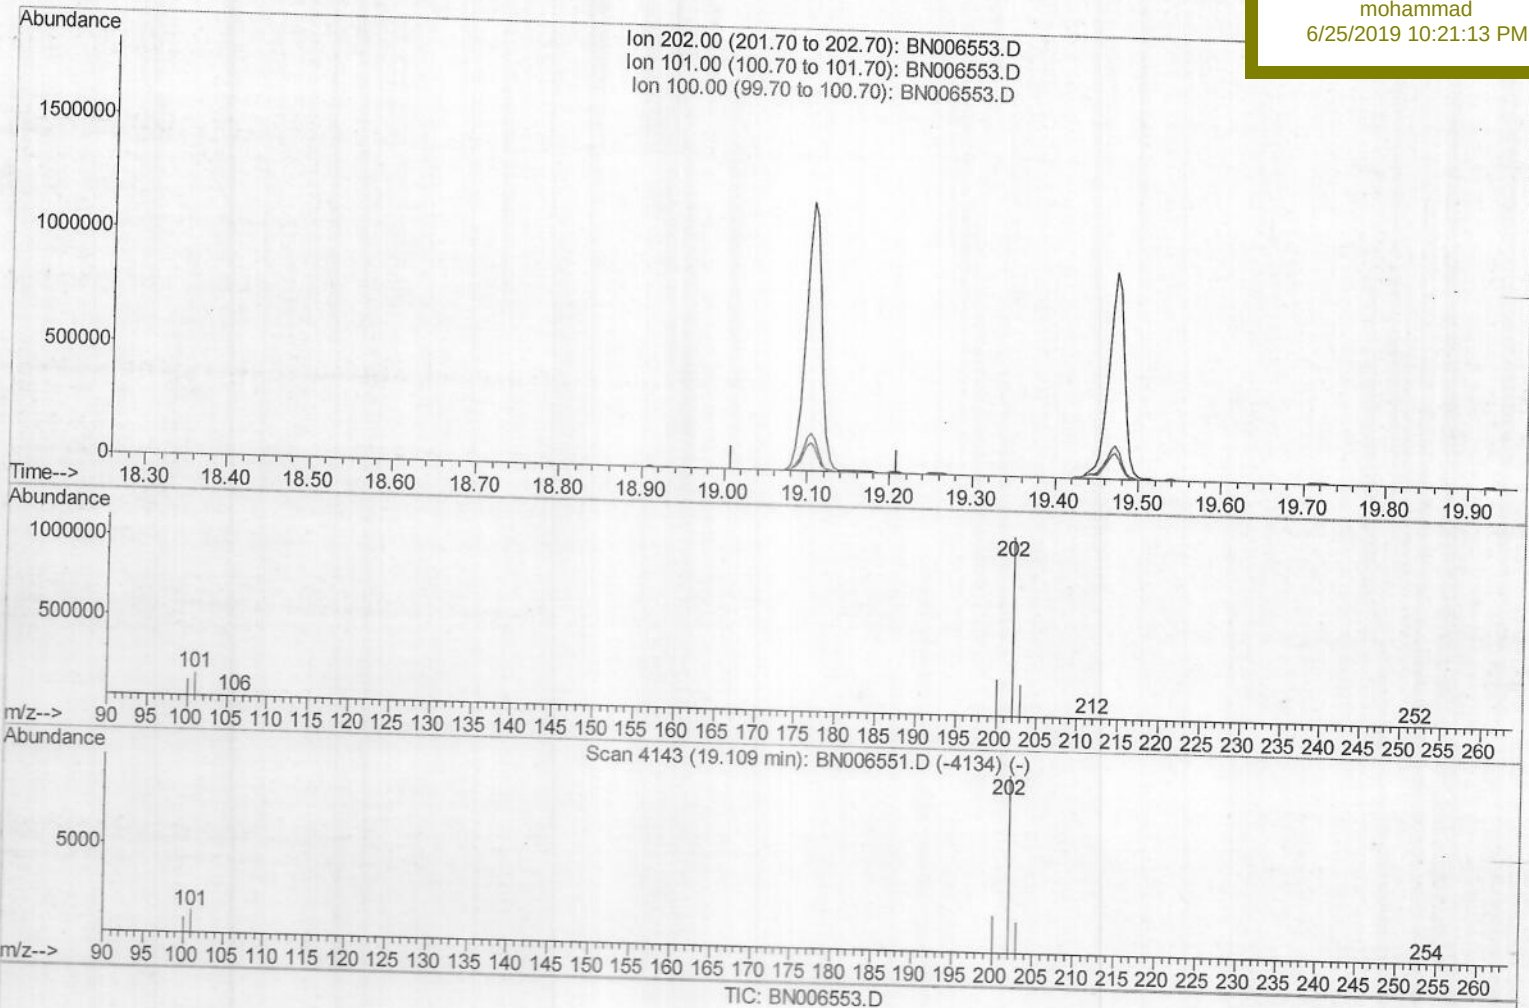

(15) Fluoranthene (C)

19.109min (-19.109) 0.00ng/ul

response 0

Ion	Exp%	Act%
202.00	100	0.00
101.00	12.10	0.00
100.00	8.70	0.00
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006553.D
Acq On : 25 Jun 2019 04:07
Operator : HP/JU
Sample : K3388-08
Misc :
ALS Vial : 30 Sample Multiplier: 1

Quant Time: Jun 25 07:18:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 25 01:51:13 2019
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A4219

Manual Integrations
APPROVED

mohammad
6/25/2019 10:21:13 PM

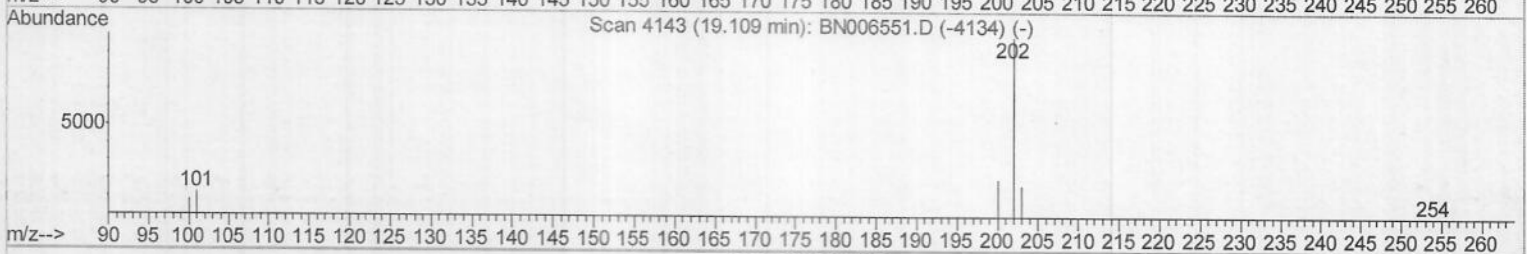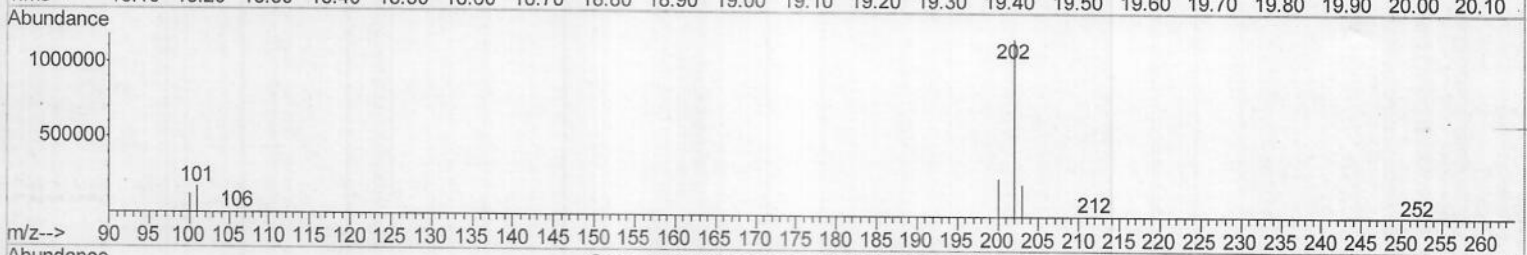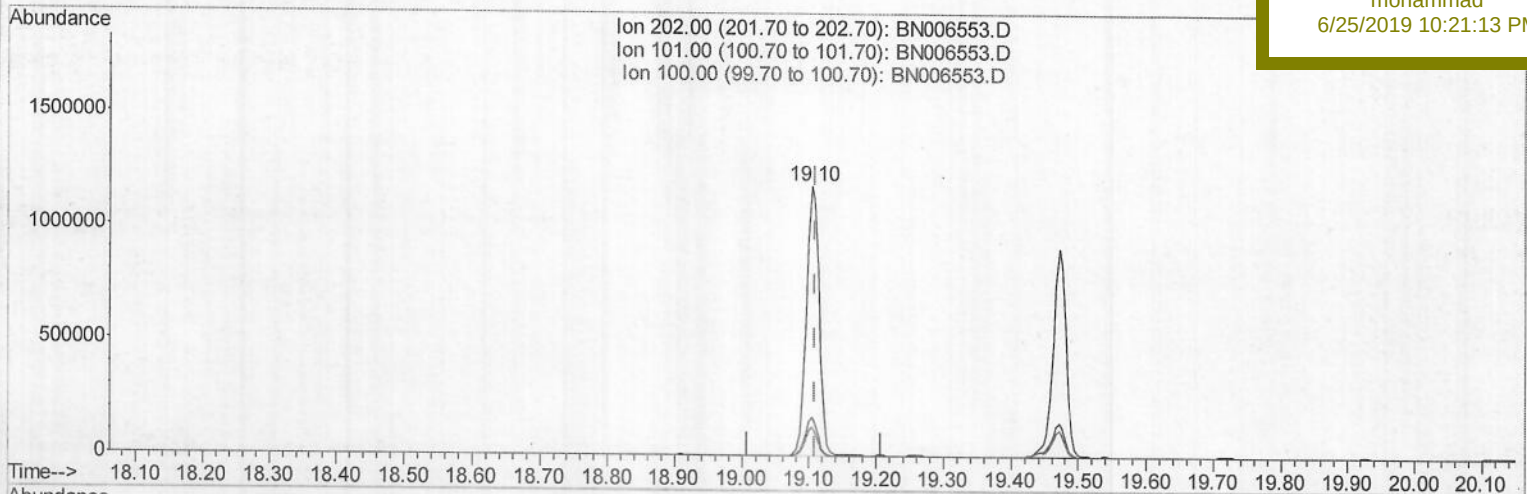

TIC: BN006553.D

(15) Fluoranthene (C)

19.104min (-0.005) 24.11ng/ul m

response 1591967

Ion	Exp%	Act%
202.00	100	100
101.00	12.10	14.10
100.00	8.70	10.28
0.00	0.00	0.00

7 JU 06/27/19

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
 Data File : BN006553.D
 Acq On : 25 Jun 2019 04:07
 Operator : HP/JU
 Sample : K3388-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Quant Time: Jun 25 07:18:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 25 01:51:13 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
ClientSampleId :
 A4219

Manual Integrations
APPROVED

mohammad
 6/25/2019 10:21:13 PM

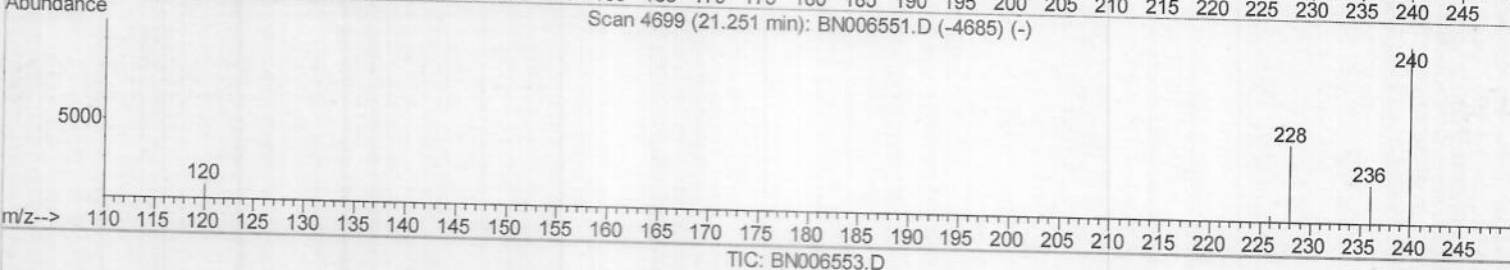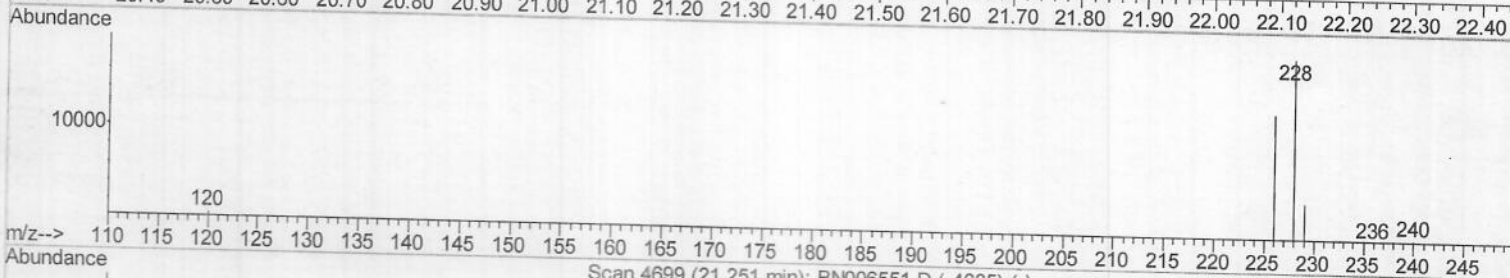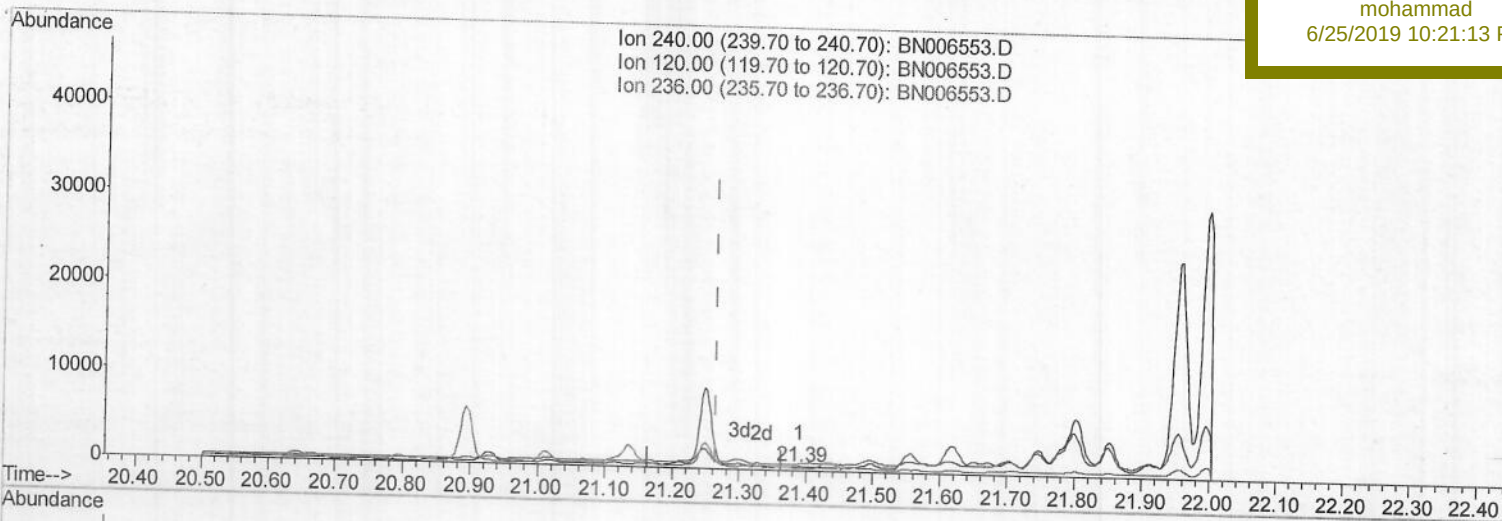

(16) Chrysene-d12 (I)

21.391min (+0.126) 0.40ng/ul

response 560

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	154.44#
236.00	30.10	62.30#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
 Data File : BN006553.D
 Acq On : 25 Jun 2019 04:07
 Operator : HP/JU
 Sample : K3388-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 Client Sampled :
 A4219

Manual Integrations
 APPROVED

mohammad
 6/25/2019 10:21:13 PM

Quant Time: Jun 25 07:18:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 25 01:51:13 2019
 Response via : Initial Calibration

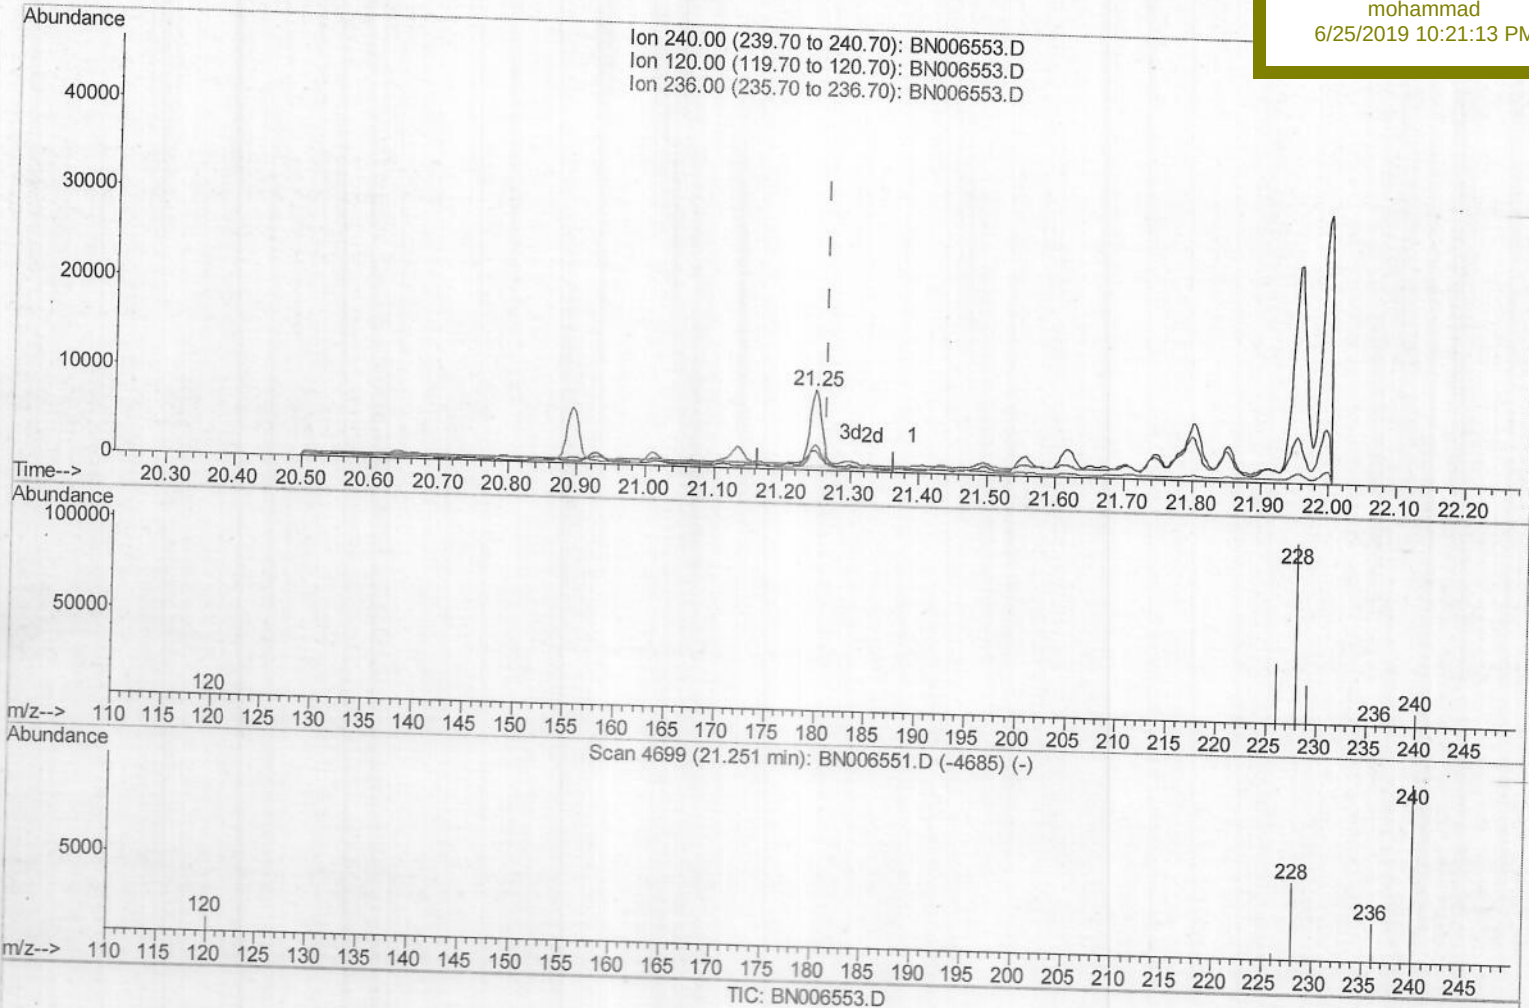

(16) Chrysene-d12 (I)

21.248min (-0.017) 0.40ng/ul m

response 10411

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	24.73#
236.00	30.10	31.40
0.00	0.00	0.00

7 JU 06/27/19

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
 Data File : BN006553.D
 Acq On : 25 Jun 2019 04:07
 Operator : HP/JU
 Sample : K3388-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 Client Sampled :
 A4219

Quant Time: Jun 25 07:20:00 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 25 01:51:13 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 6/25/2019 10:21:13 PM

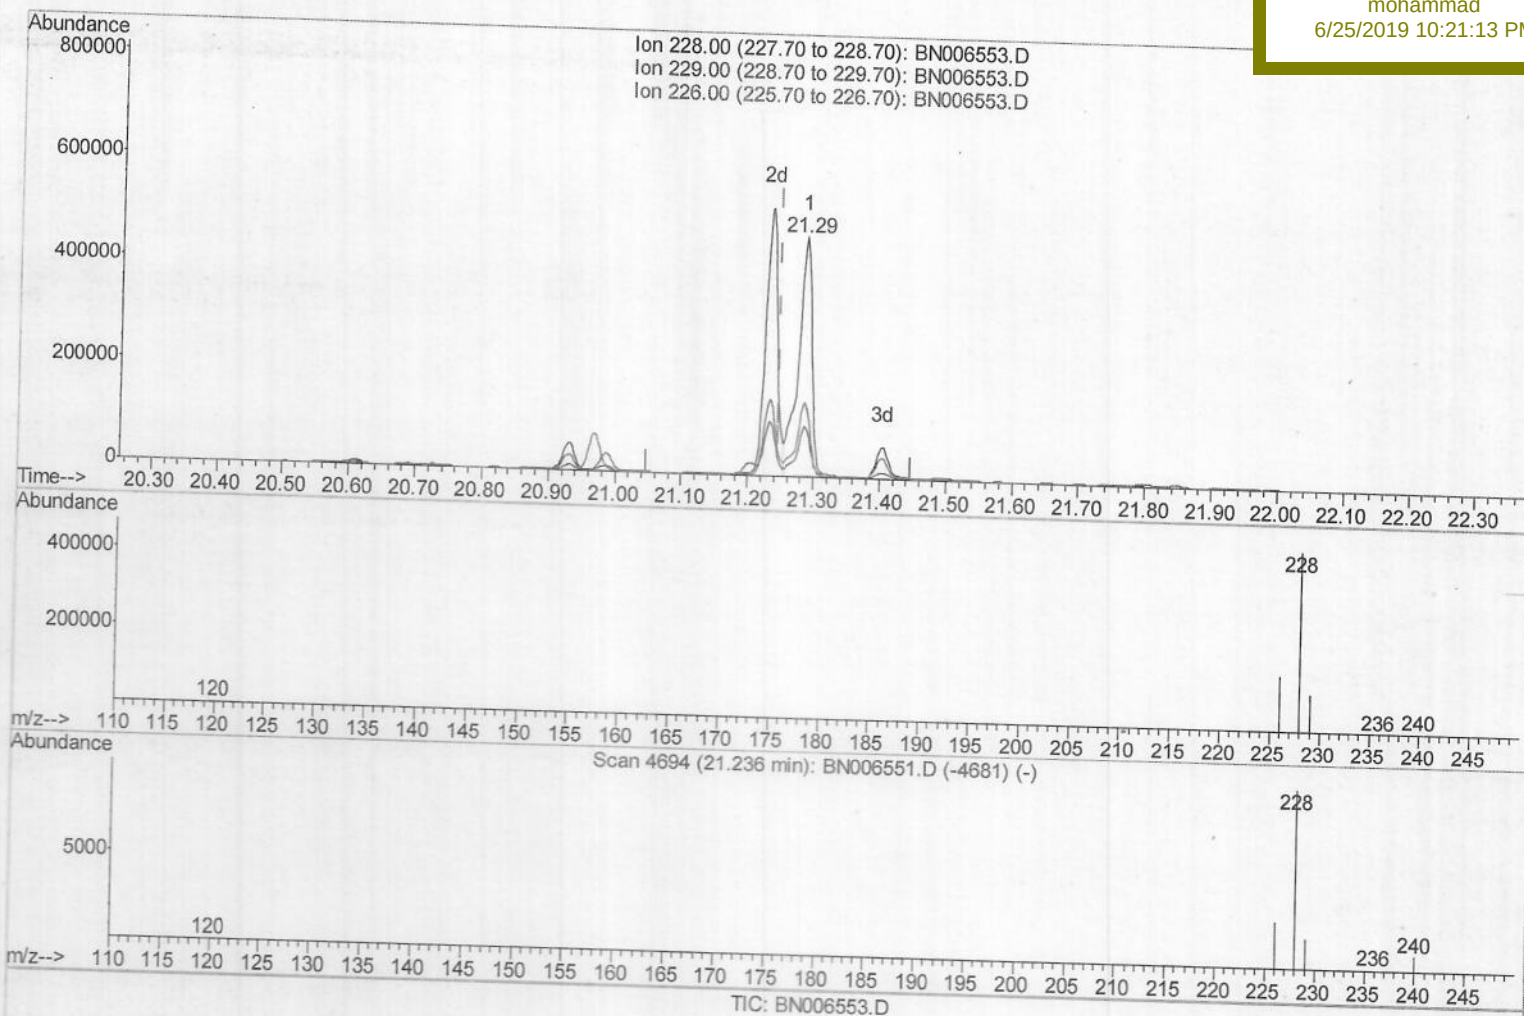

(18) Benzo(a)anthracene

21.286min (+0.038) 14.58ng/ul

response 671312

Ion	Exp%	Act%
228.00	100	100
229.00	20.60	21.44
226.00	28.50	30.99
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
Data File : BN006553.D
Acq On : 25 Jun 2019 04:07
Operator : HP/JU
Sample : K3388-08
Misc :
ALS Vial : 30 Sample Multiplier: 1




Quant Time: Jun 25 07:20:00 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 25 01:51:13 2019
Response via : Initial Calibration

Instrument :

BNA_N

Client Sampled :

A4219

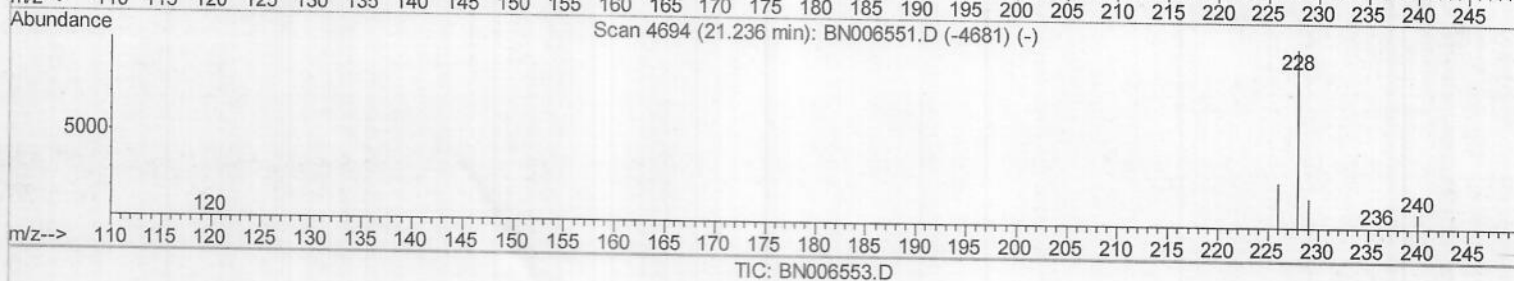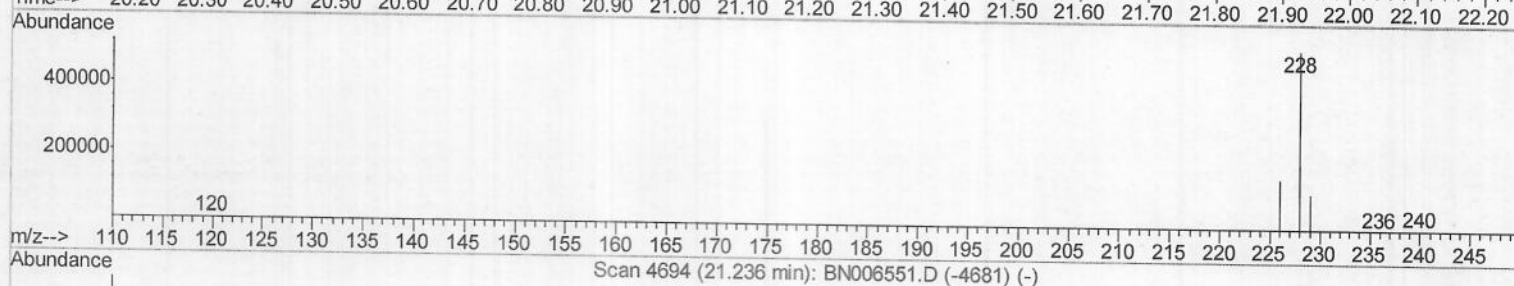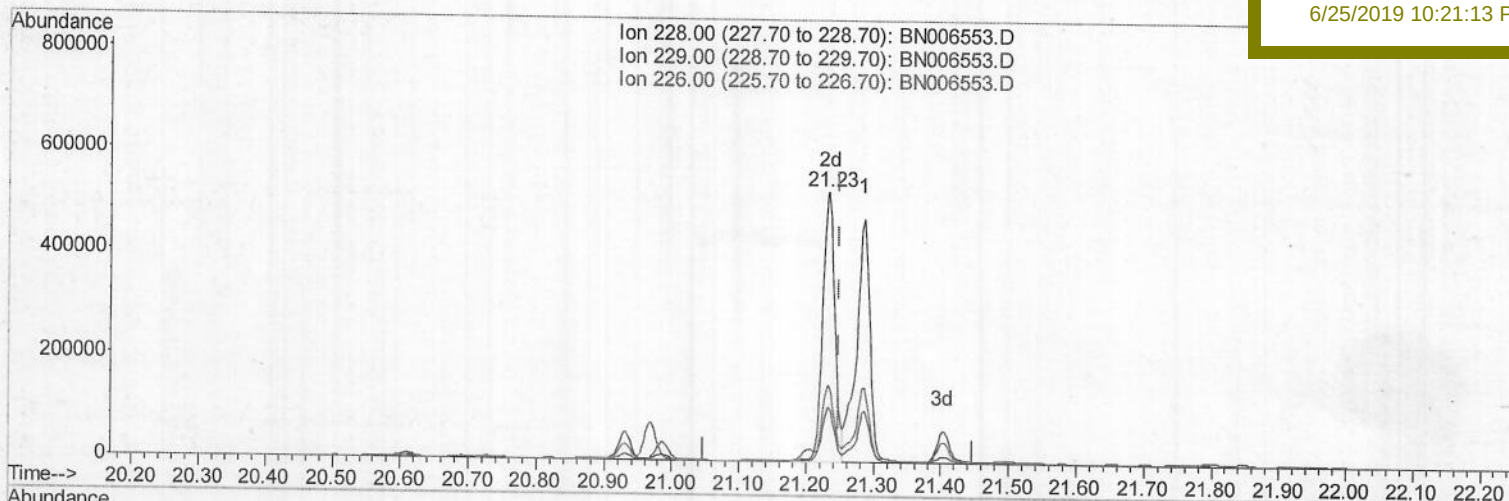Manual Integrations
APPROVEDmohammad
6/25/2019 10:21:13 PM

(18) Benzo(a)anthracene

21.233min (-0.015) 14.38ng/ul m

7 JU 06/27/19

response 662335

Ion	Exp%	Act%
228.00	100	100
229.00	20.60	20.28
226.00	28.50	28.51
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006553.D

Acq On : 25 Jun 2019 04:07

Operator : HP/JU

Sample : K3388-08

Misc :

ALS Vial : 30 Sample Multiplier: 1

Quant Time: Jun 25 07:20:00 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Jun 25 01:51:13 2019

Response via : Initial Calibration

Instrument :

BNA_N




ClientSampleId :

A4219

Manual Integrations
APPROVED

mohammad

6/25/2019 10:21:13 PM

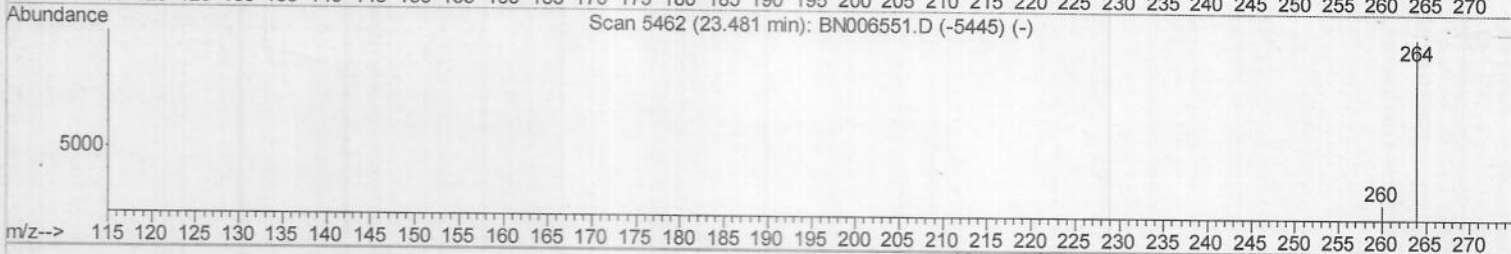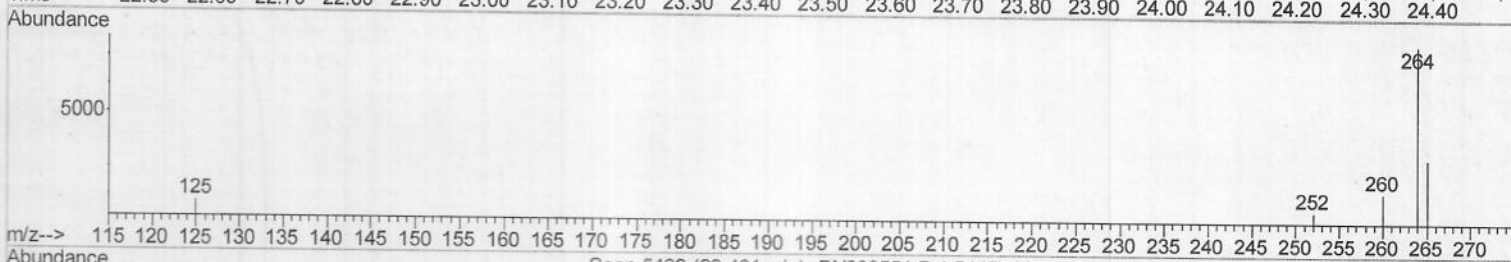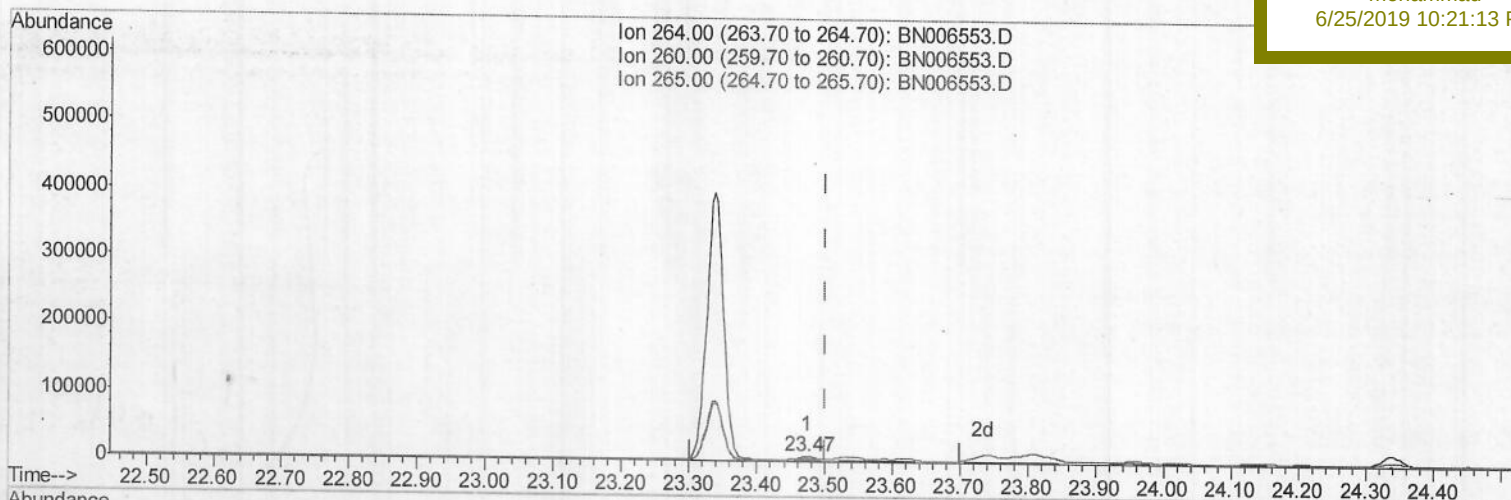

(20) Perylene-d12 (I)

23.475min (-0.026) 0.40ng/ul

response 11004

Ion	Exp%	Act%
264.00	100	100
260.00	29.20	29.88
265.00	44.70	46.57
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
 Data File : BN006553.D
 Acq On : 25 Jun 2019 04:07
 Operator : HP/JU
 Sample : K3388-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1




Instrument :
 BNA_N
ClientSampleId :
 A4219

Manual Integrations
APPROVED

mohammad
 6/25/2019 10:21:13 PM

Quant Time: Jun 25 07:20:00 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 25 01:51:13 2019
 Response via : Initial Calibration

Ion 264.00 (263.70 to 264.70): BN006553.D
 Ion 260.00 (259.70 to 260.70): BN006553.D
 Ion 265.00 (264.70 to 265.70): BN006553.D

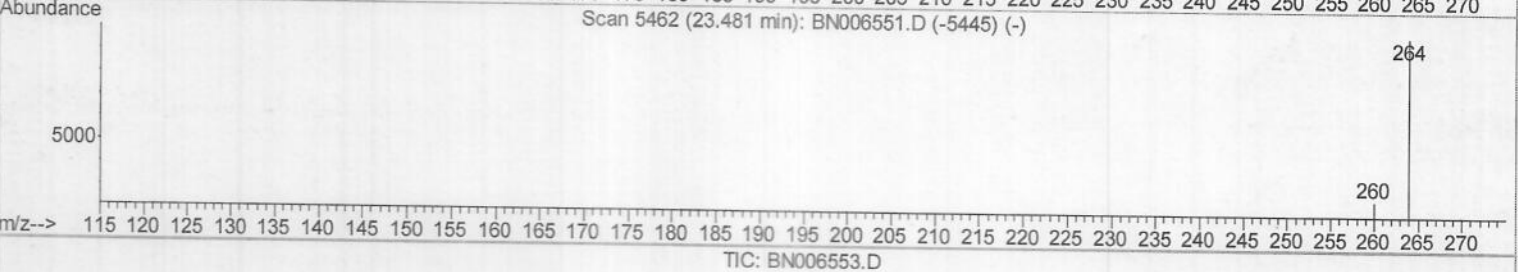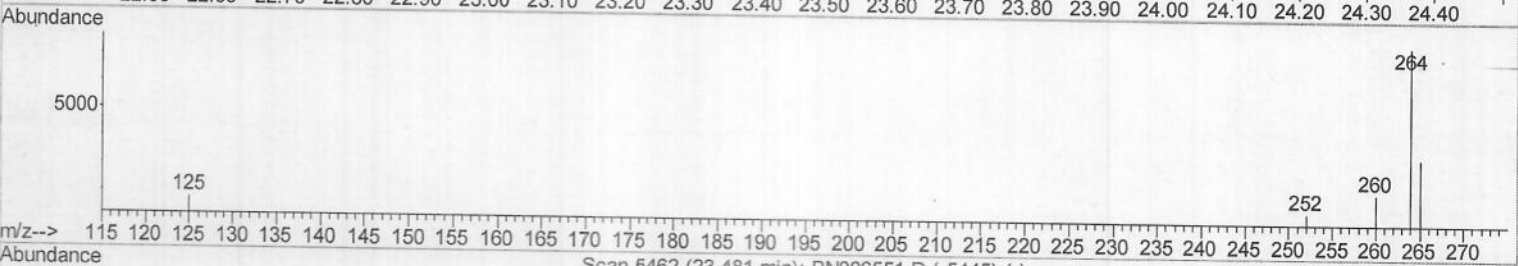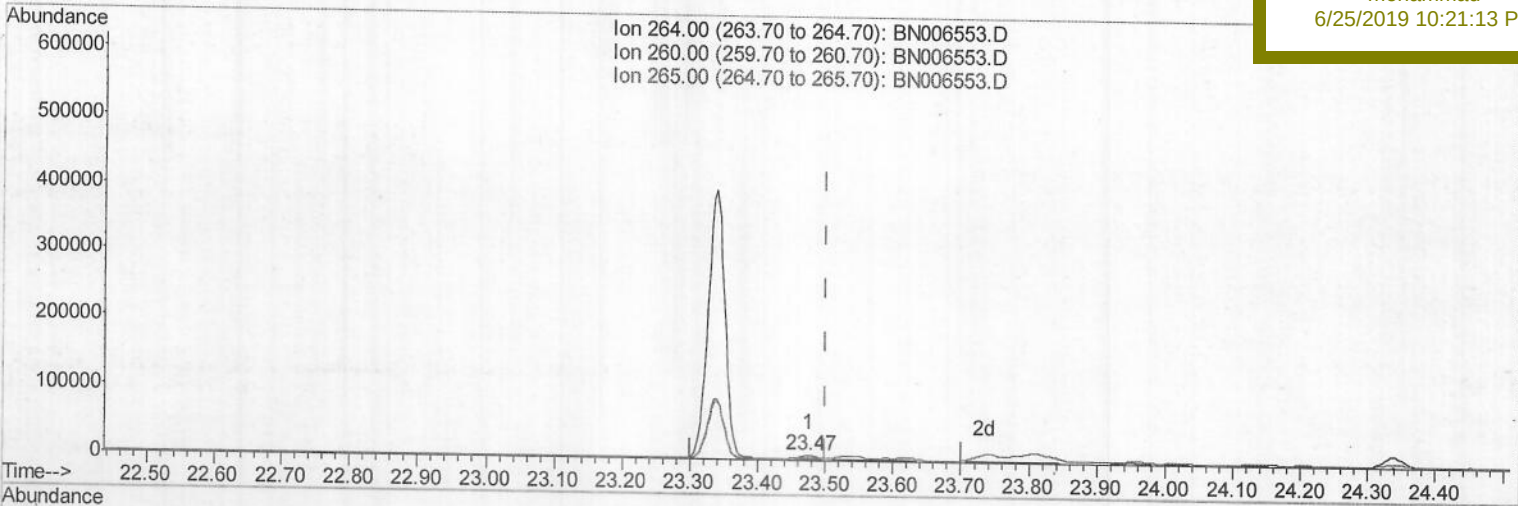

(20) Perylene-d12 (I)

23.475min (-0.026) 0.40ng/ul m

response 11812

Ion	Exp%	Act%
264.00	100	100
260.00	29.20	29.88
265.00	44.70	46.57
0.00	0.00	0.00

7 JU 06/27/19

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
 Data File : BN006553.D
 Acq On : 25 Jun 2019 04:07
 Operator : HP/JU
 Sample : K3388-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4219

Manual Integrations
 APPROVED

mohammad
 6/25/2019 10:21:13 PM

Quant Time: Jun 25 07:20:49 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 25 01:51:13 2019
 Response via : Initial Calibration

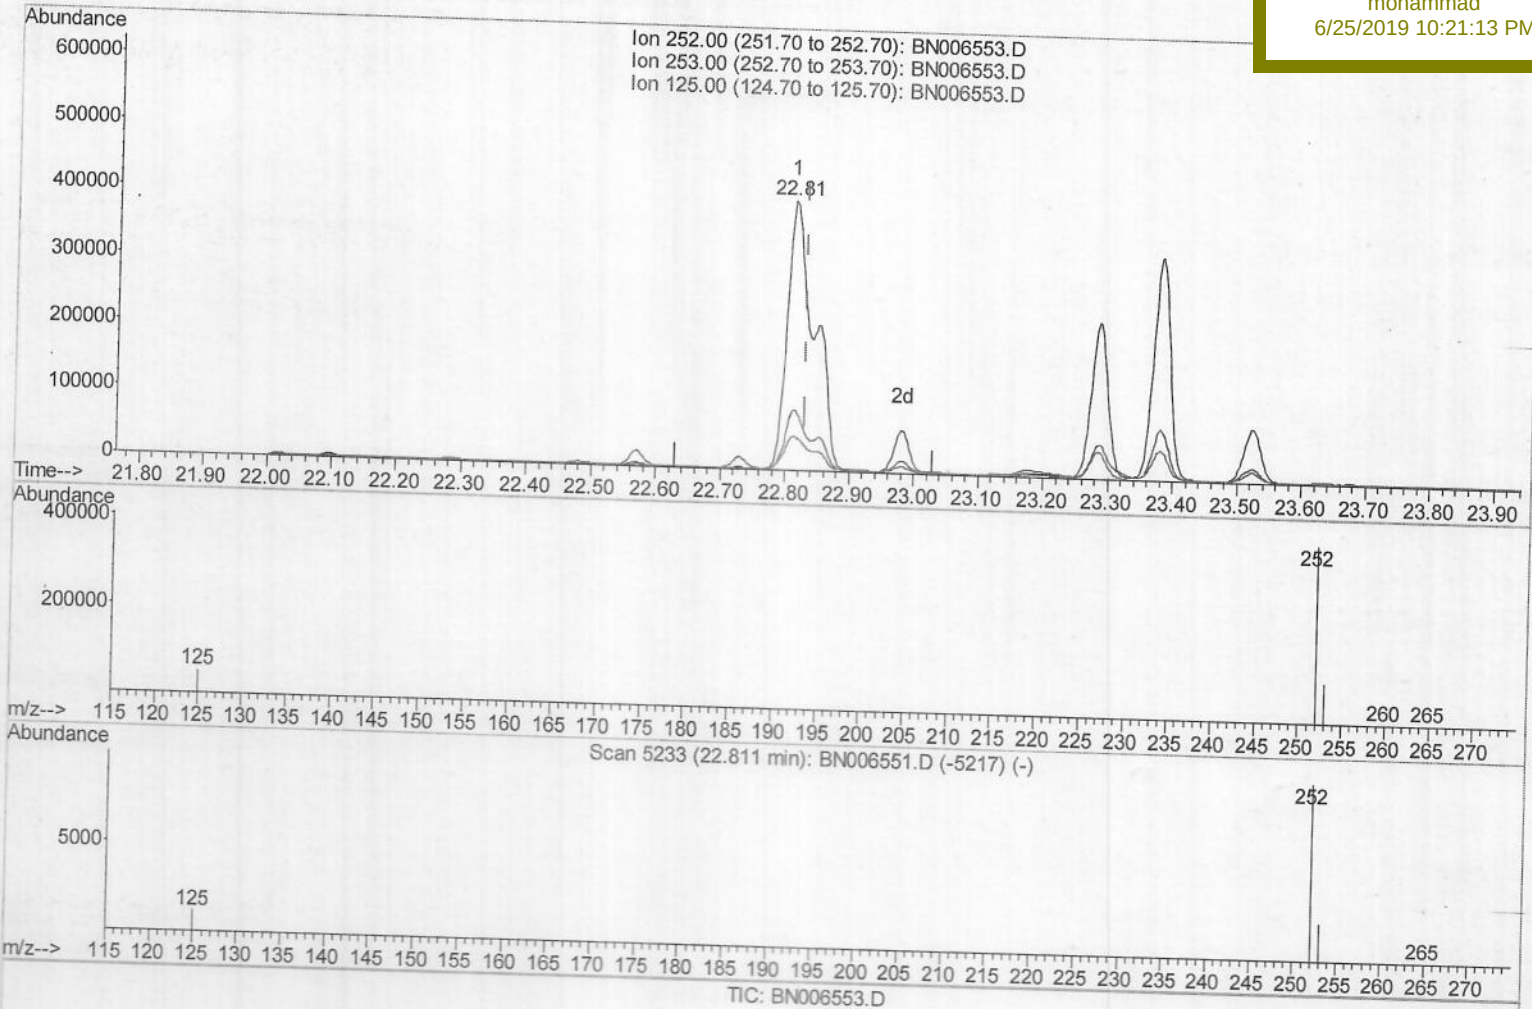

(21) Benzo(b)fluoranthene
 22.811min (-0.020) 24.12ng/ul
 response 1187764

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	22.51
125.00	20.50	12.72
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
 Data File : BN006553.D
 Acq On : 25 Jun 2019 04:07
 Operator : HP/JU
 Sample : K3388-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Quant Time: Jun 25 07:20:49 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 25 01:51:13 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 Client Sampled :
 A4219

Manual Integrations
 APPROVED

mohammad
 6/25/2019 10:21:13 PM

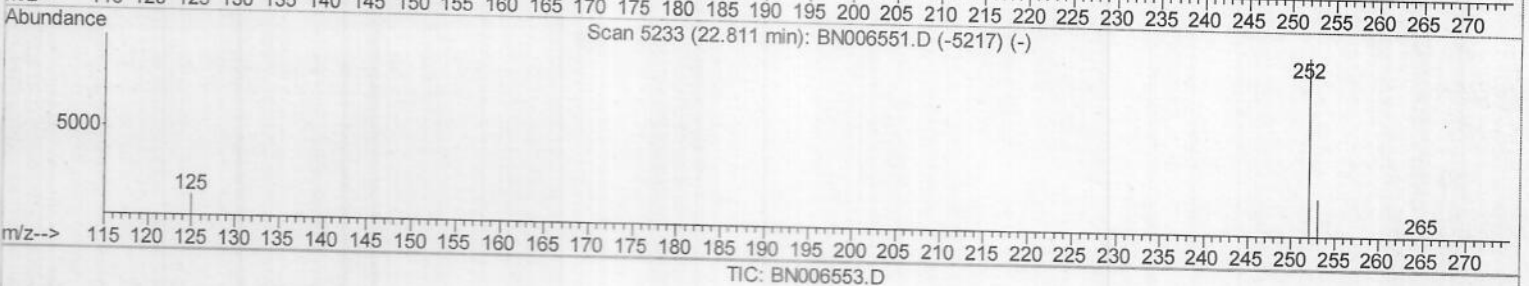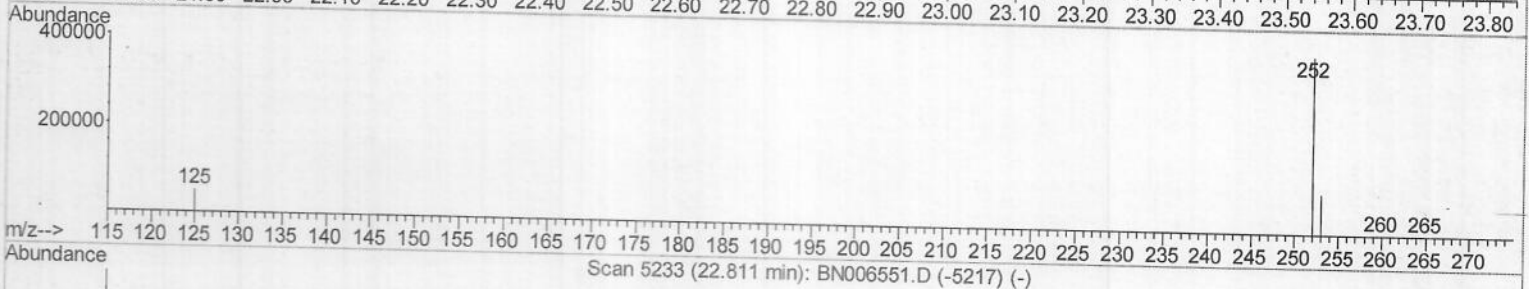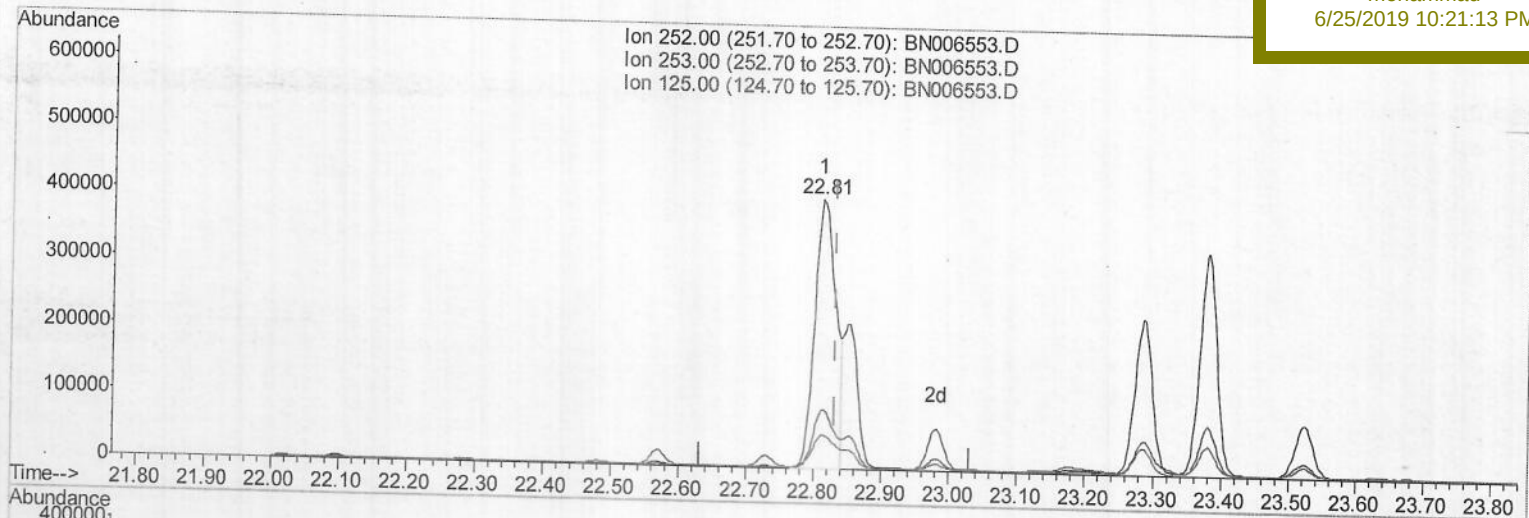

(21) Benzo(b)fluoranthene

22.811min (-0.020) 17.68ng/ul m > JU 06/27/19

response 870613

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	22.51
125.00	20.50	12.72
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
 Data File : BN006553.D
 Acq On : 25 Jun 2019 04:07
 Operator : HP/JU
 Sample : K3388-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Quant Time: Jun 25 07:20:49 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 25 01:51:13 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 A4219

Manual Integrations
 APPROVED

mohammad
 6/25/2019 10:21:13 PM

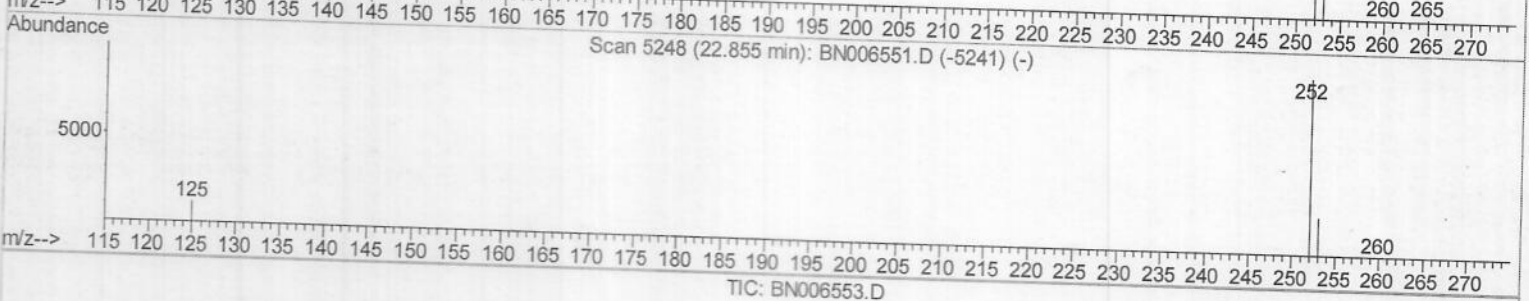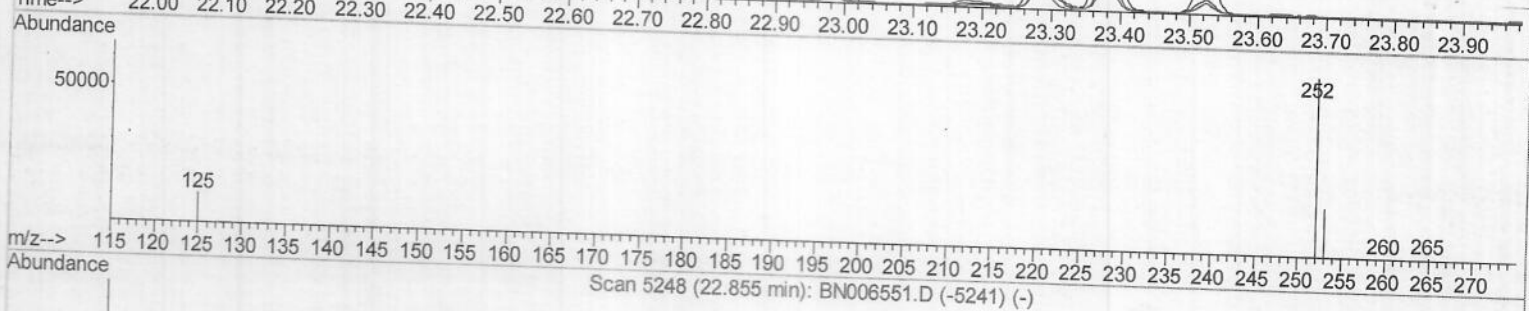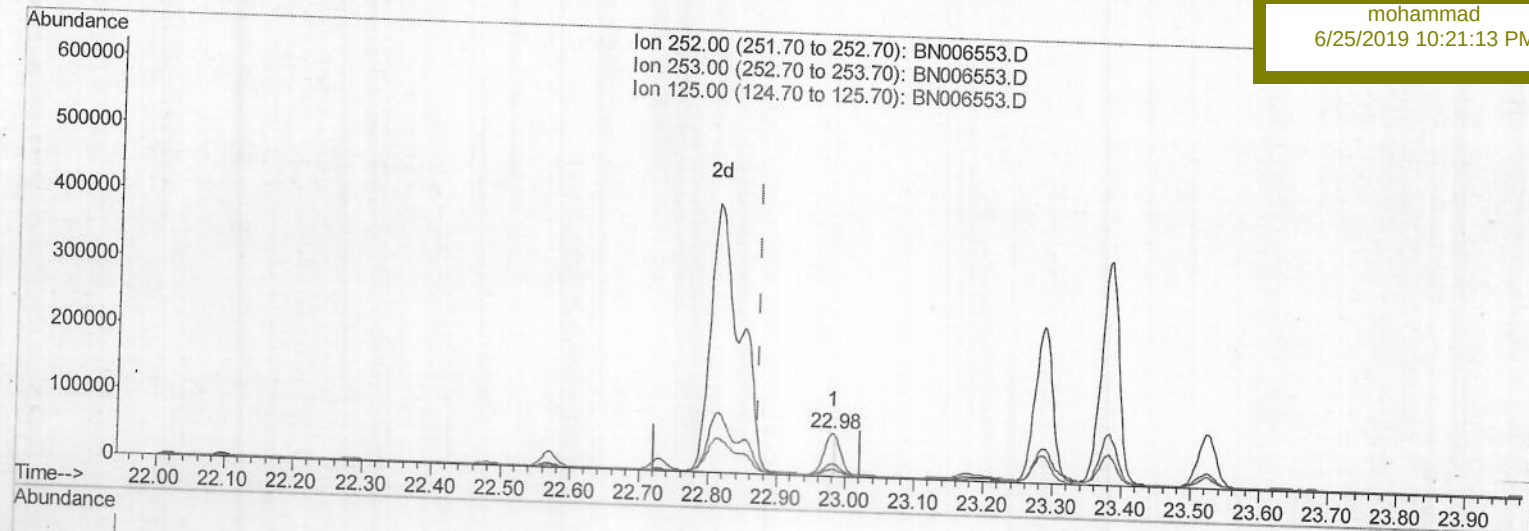

(22) Benzo(k)fluoranthene
 22.981min (+0.108) 1.37ng/ul
 response 65851

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	27.76
125.00	17.90	16.76
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\

Data File : BN006553.D

Acq On : 25 Jun 2019 04:07

Operator : HP/JU

Sample : K3388-08

Misc :

ALS Vial : 30 Sample Multiplier: 1

Quant Time: Jun 25 07:20:49 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Jun 25 01:51:13 2019




Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

A4219

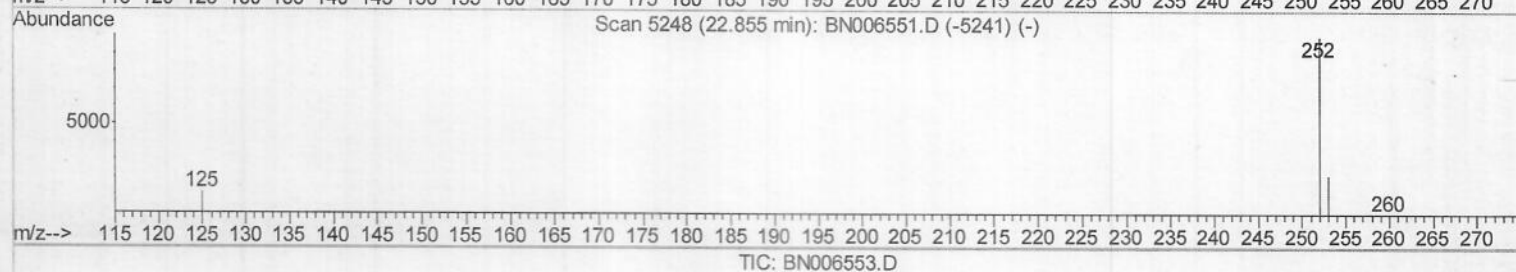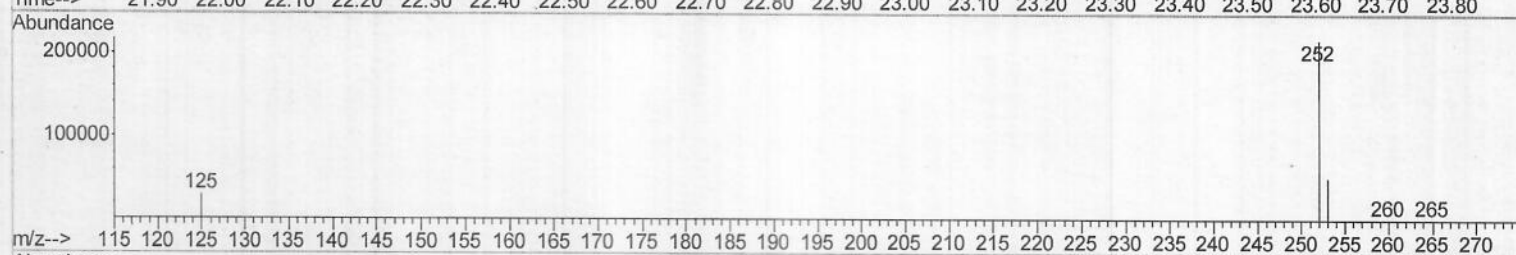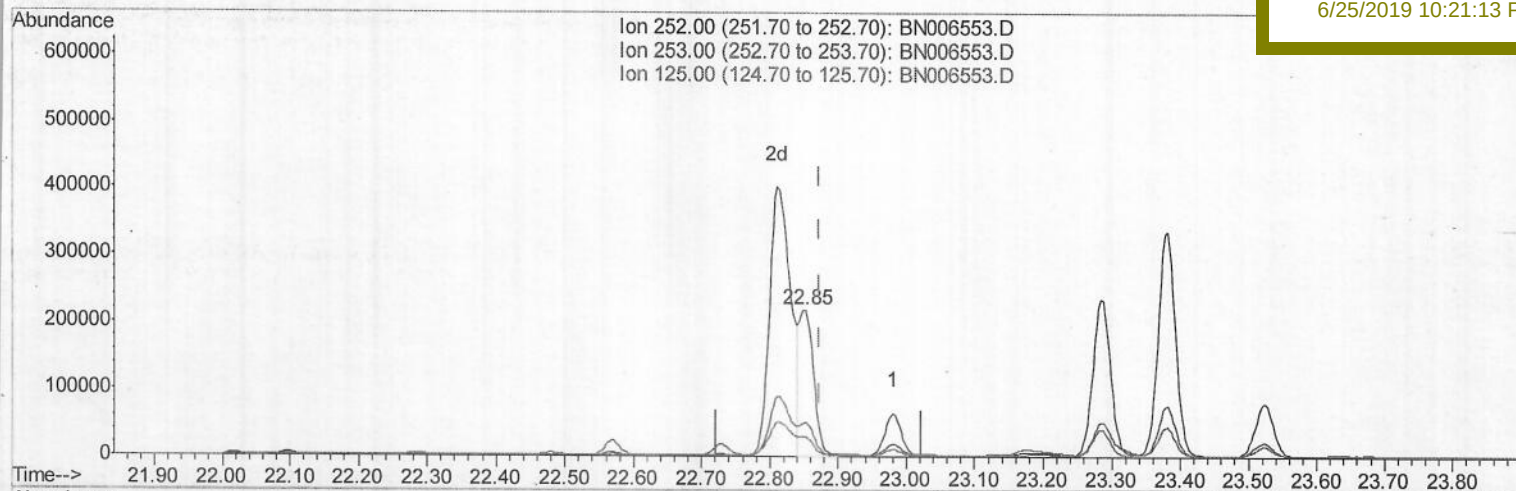Manual Integrations
APPROVEDmohammad
6/25/2019 10:21:13 PM

(22) Benzo(k)fluoranthene

22.852min (-0.020) 6.70ng/ul m

response 321443

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	23.13
125.00	17.90	13.42#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062419\
 Data File : BN006553.D
 Acq On : 25 Jun 2019 04:07
 Operator : HP/JU
 Sample : K3388-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 Client Sampled :
 A4219

Quant Time: Jun 25 07:21:26 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 25 01:51:13 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 6/25/2019 10:21:13 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	5649	0.40	ng/ul	0.00
2) Naphthalene-d8	10.41	136	20541	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.28	164	9958	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	18631m	0.40	ng/ul	0.00
16) Chrysene-d12	21.25	240	10411m	0.40	ng/ul	-0.02
20) Perylene-d12	23.47	264	11812m	0.40	ng/ul	-0.03
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.01	152	6251	0.20	ng/ul	0.00
14) Fluoranthene-d10	19.08	212	11030m	0.22	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.46	128	5142	0.091	ng/ul#	95
5) 2-Methylnaphthalene	12.08	142	1715	0.043	ng/ul	99
7) Acenaphthylene	14.00	152	9035	0.163	ng/ul	97
8) Acenaphthene	14.34	153	18308	0.477	ng/ul	100
9) Fluorene	15.33	166	34370	0.765	ng/ul	97
12) Phenanthrene	17.08	178	854028m	14.280	ng/ul	
13) Anthracene	17.17	178	217465m	3.808	ng/ul	
15) Fluoranthene	19.10	202	1591967m	24.106	ng/ul	
17) Pyrene	19.47	202	1229723	22.424	ng/ul	99
18) Benzo(a)anthracene	21.23	228	662335m	14.384	ng/ul	
19) Chrysene	21.29	228	671312	15.530	ng/ul	99
21) Benzo(b)fluoranthene	22.81	252	870613m	17.676	ng/ul	
22) Benzo(k)fluoranthene	22.85	252	321443m	6.700	ng/ul	
23) Benzo(a)pyrene	23.38	252	589960	12.861	ng/ul#	85
24) Indeno(1,2,3-cd)pyrene	25.71	276	420379	8.467	ng/ul#	89
25) Dibenzo(a,h)anthracene	25.71	278	106727	2.689	ng/ul	95
26) Benzo(g,h,i)perylene	26.39	276	368071	8.851	ng/ul	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU
 06/27/19