

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062423\
 Data File : BN025975.D
 Acq On : 23 Jun 2023 19:38
 Operator : MA/JU
 Sample : PB153403BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK403

Quant Time: Jun 24 01:00:58 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 22 01:27:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.976	152	7129	0.400	ng/ul	0.00
4) Naphthalene-d8	10.791	136	22469	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.616	164	14032	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.359	188	30243	0.400	ng/ul	0.00
17) Chrysene-d12	21.548	240	20799	0.400	ng/ul	0.00
23) Perylene-d12	23.998	264	19692	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.326	96	46341	5.772	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.380	152	11786	0.341	ng/ul	0.00
18) Fluoranthene-d10	19.386	212	27232	0.344	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.606	166	4526	0.073	ng/ul#	12
20) Pyrene	19.748	202	4137	0.036	ng/ul#	1
26) Benzo(a)pyrene	23.840	252	6382	0.087	ng/ul#	49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062423\
Data File : BN025975.D
Acq On : 23 Jun 2023 19:38
Operator : MA/JU
Sample : PB153403BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK403

Quant Time: Jun 24 01:00:58 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 22 01:27:41 2023
Response via : Initial Calibration




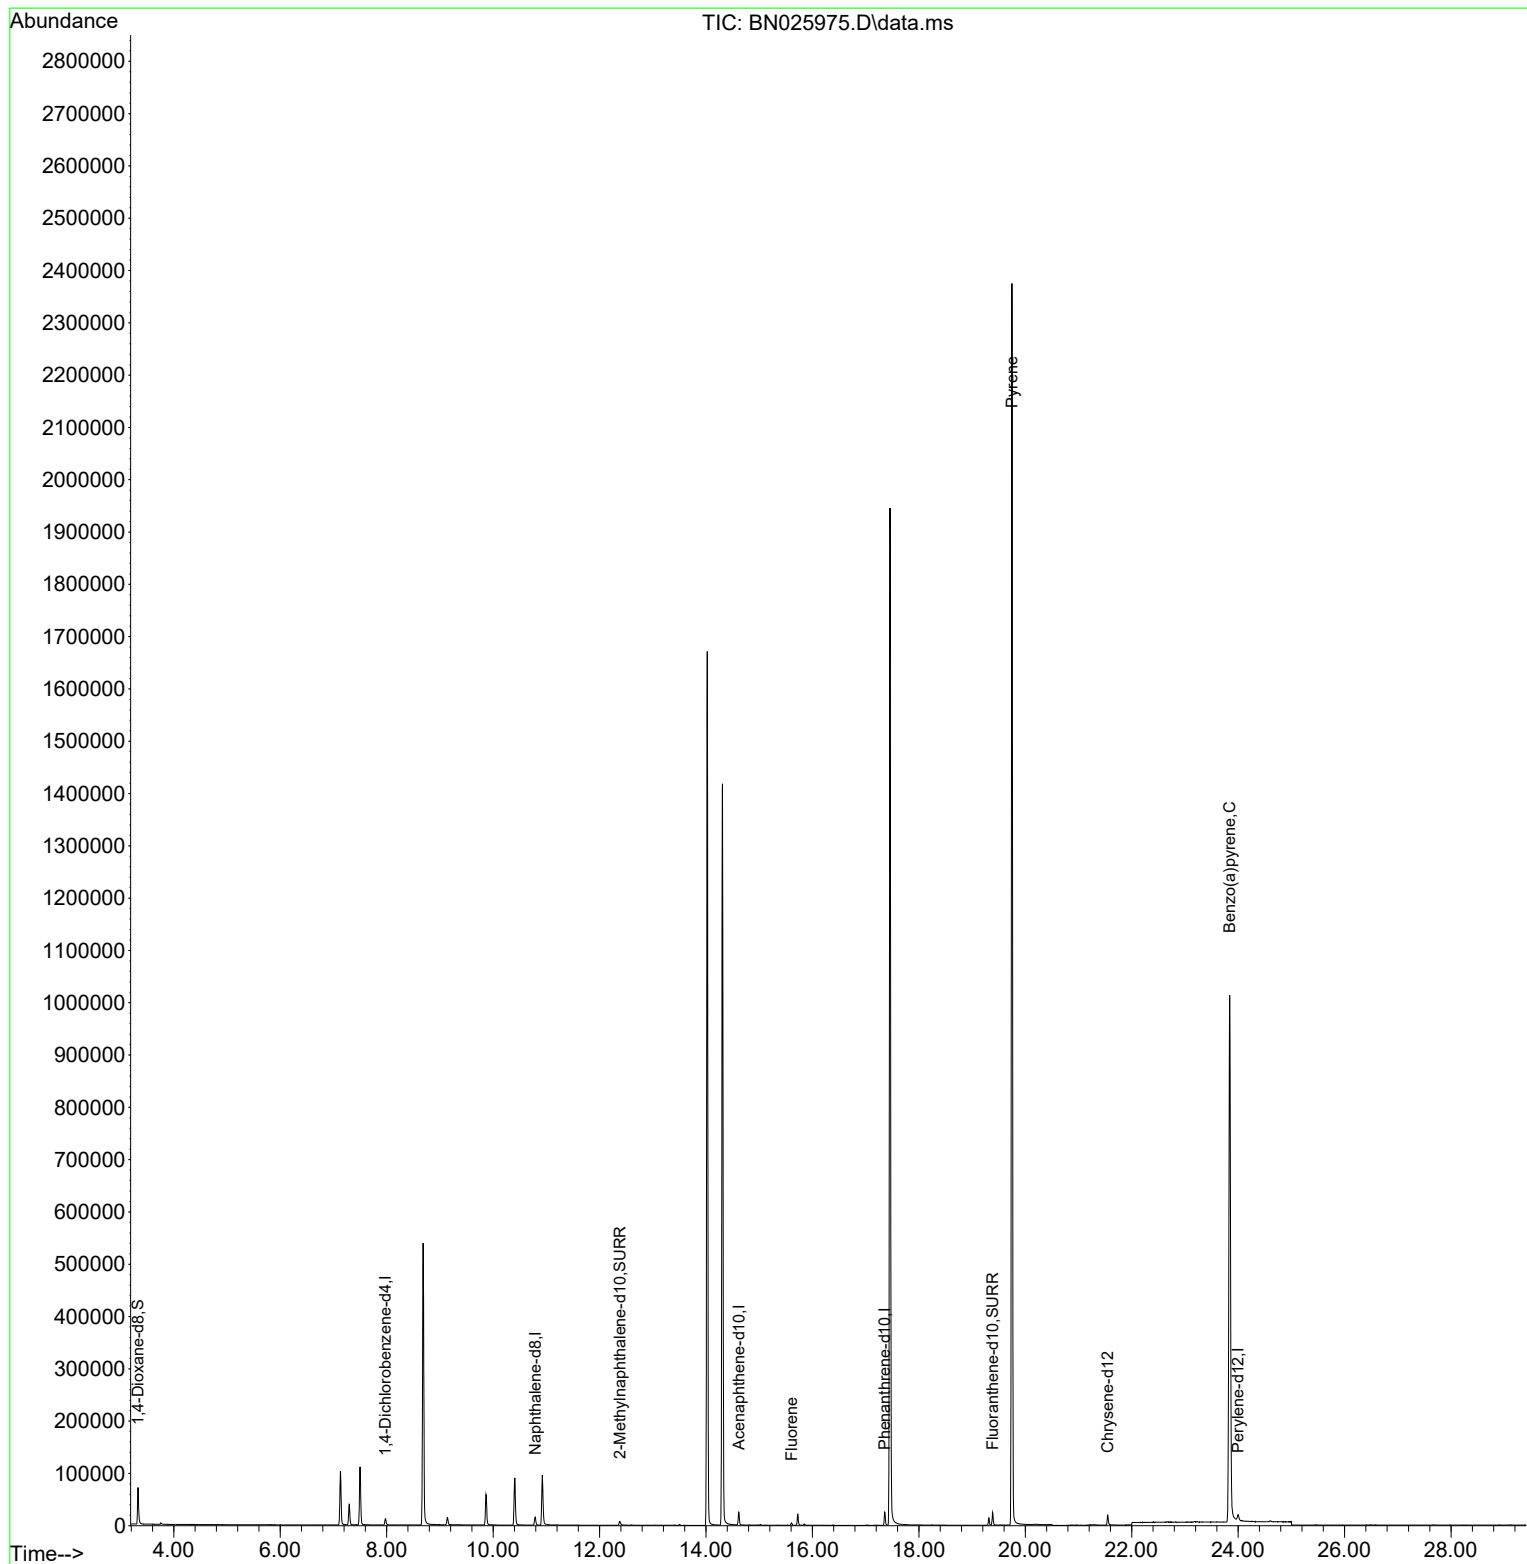


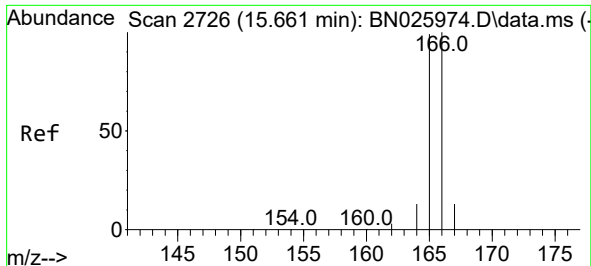

#12
Fluorene
Concen: 0.073 ng/ul
RT: 15.606 min Scan# 21
Delta R.T. -0.061 min
Lab File: BN025975.D
Acq: 23 Jun 2023 19:38




Instrument :
BNA_N
ClientSampleId :
SBLK403


Tgt Ion:166 Resp: 4526
Ion Ratio Lower Upper
166 100
165 6.6 79.9 119.9#
167 32.2 10.8 16.2#

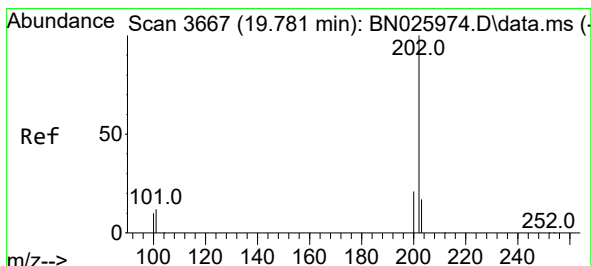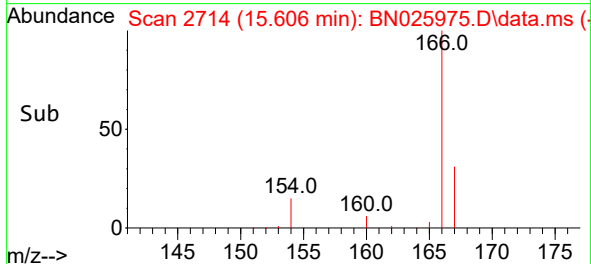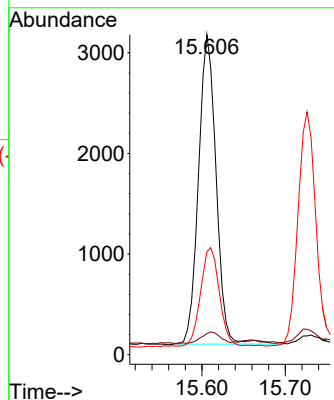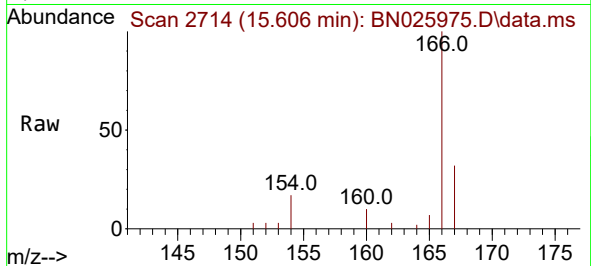

#20
Pyrene
Concen: 0.036 ng/ul
RT: 19.748 min Scan# 3660
Delta R.T. -0.034 min
Lab File: BN025975.D
Acq: 23 Jun 2023 19:38


Tgt Ion:202 Resp: 4137
Ion Ratio Lower Upper
202 100
101 178.6 11.4 17.0#
100 1396.5 9.1 13.7#

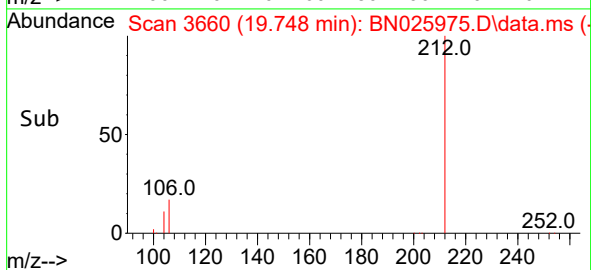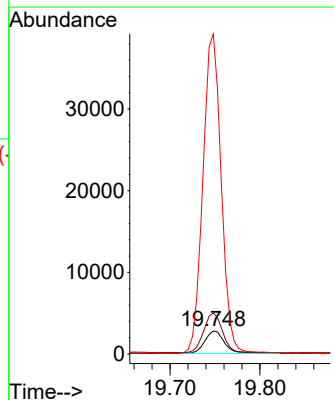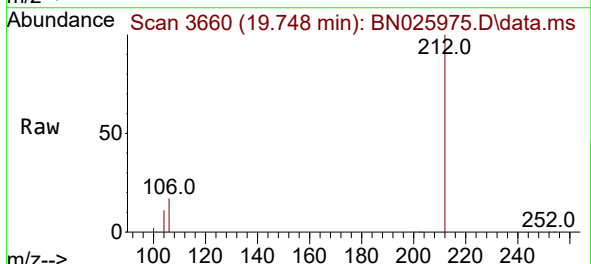

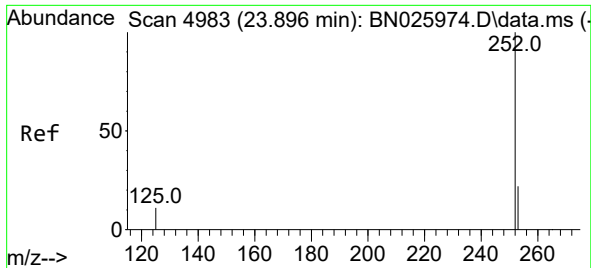

#26
 Benzo(a)pyrene
 Concen: 0.087 ng/ul
 RT: 23.840 min Scan# 4983
 Delta R.T. -0.068 min
 Lab File: BN025975.D
 Acq: 23 Jun 2023 19:38

Instrument :
 BNA_N
 ClientSampleId :
 SBLK403

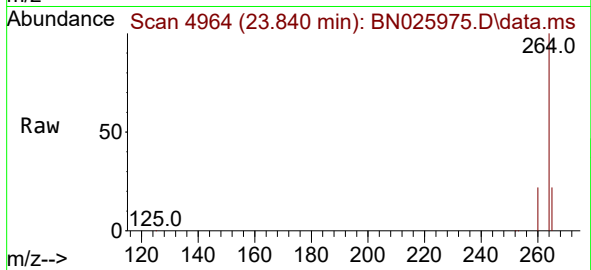

Tgt Ion:252 Resp: 6382
 Ion Ratio Lower Upper
 252 100
 253 55.5 26.0 39.0#
 125 52.5 17.3 25.9#

