

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062423\
 Data File : BN026008.D
 Acq On : 24 Jun 2023 16:48
 Operator : MA/JU
 Sample : PB153447BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK447

Quant Time: Jun 24 23:50:13 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 22 01:27:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.976	152	6722	0.400	ng/ul	0.00
4) Naphthalene-d8	10.787	136	22164	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.616	164	14094	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.359	188	30401	0.400	ng/ul	0.00
17) Chrysene-d12	21.543	240	17824	0.400	ng/ul	0.00
23) Perylene-d12	24.002	264	19225	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.327	96	43166	5.702	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.376	152	11713	0.344	ng/ul	0.00
18) Fluoranthene-d10	19.387	212	27090	0.399	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.606	166	4555	0.074	ng/ul#	12
20) Pyrene	19.749	202	4211	0.043	ng/ul#	1
26) Benzo(a)pyrene	23.850	252	6074	0.085	ng/ul#	53


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062423\
Data File : BN026008.D
Acq On : 24 Jun 2023 16:48
Operator : MA/JU
Sample : PB153447BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK447

Quant Time: Jun 24 23:50:13 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 22 01:27:41 2023
Response via : Initial Calibration

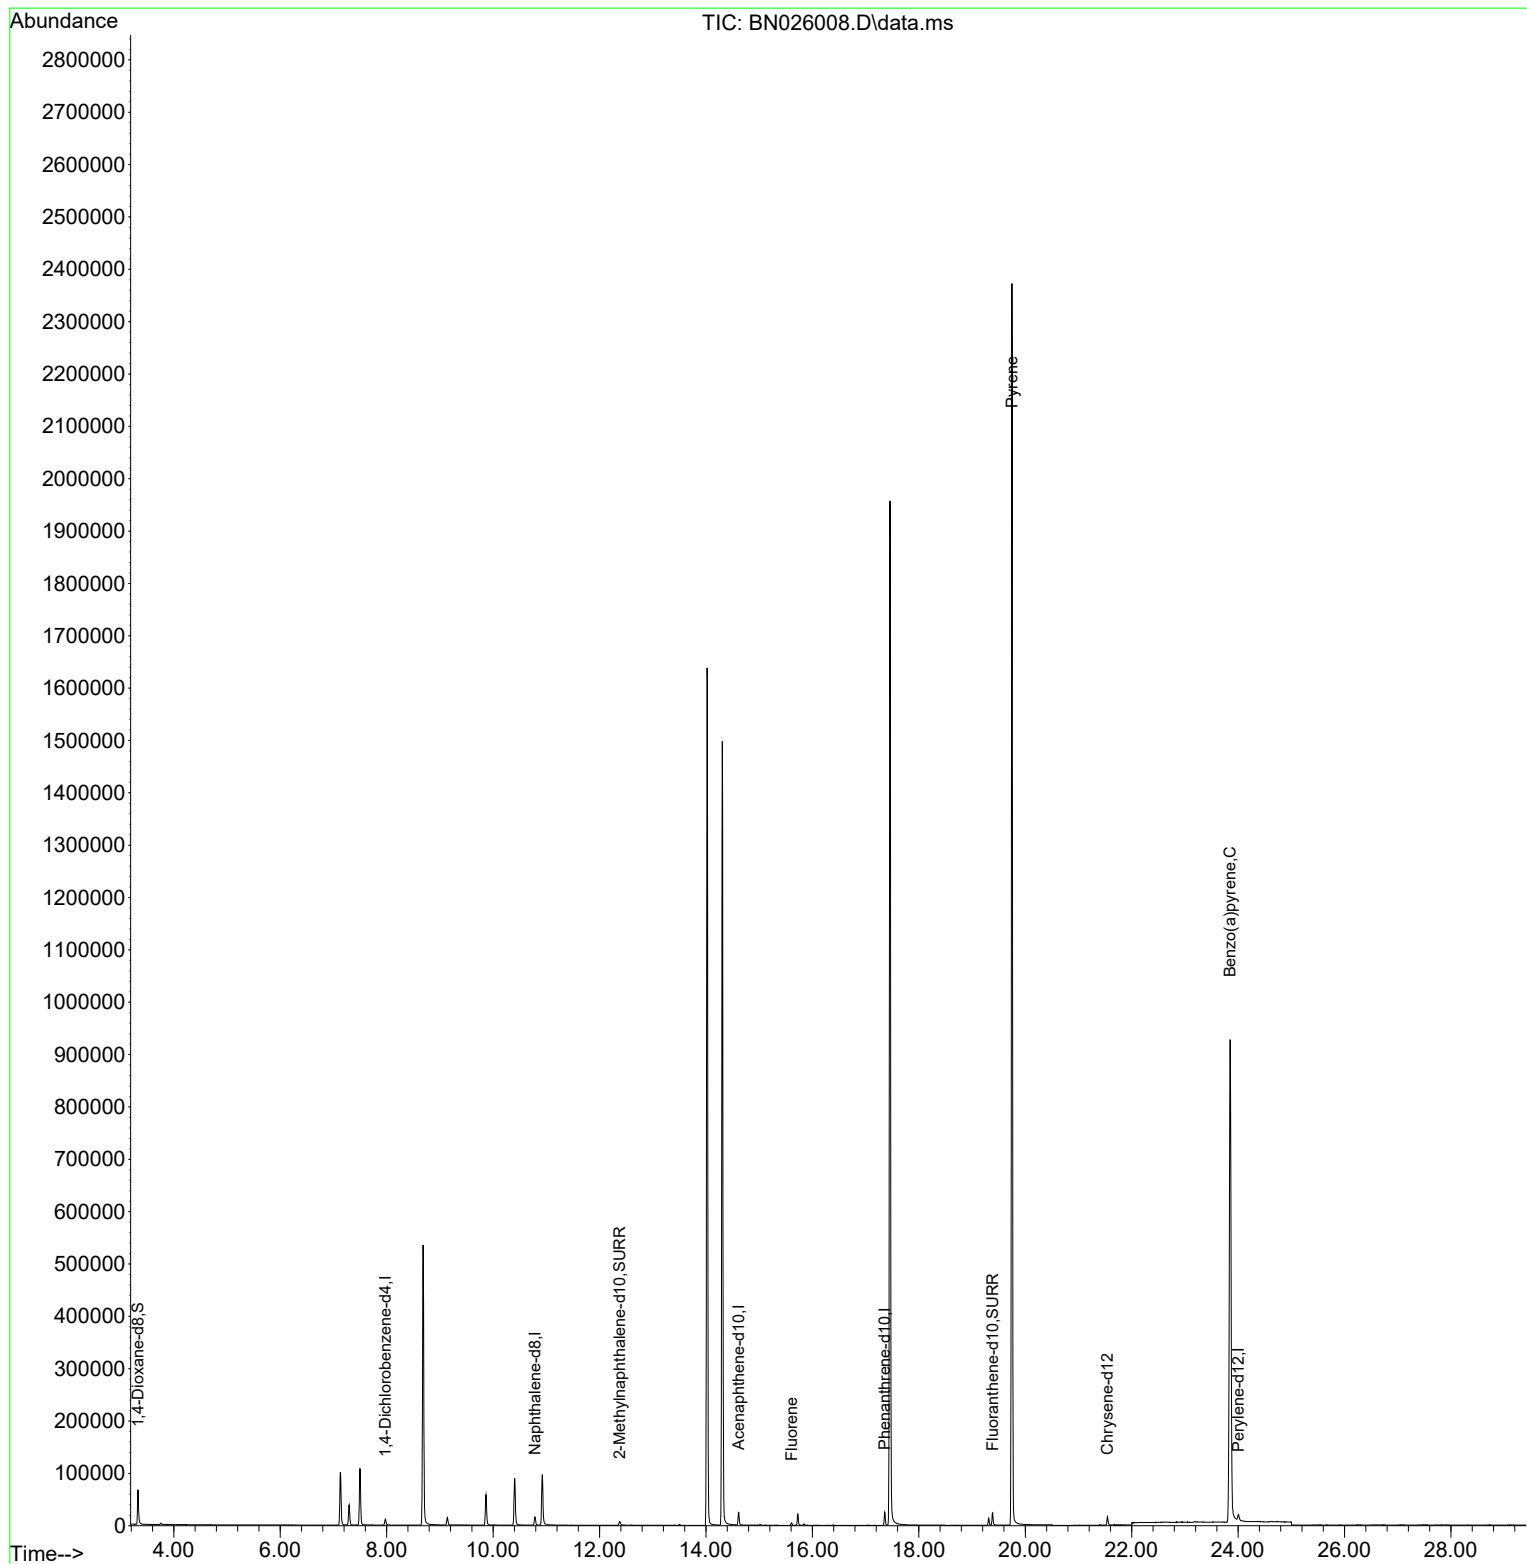

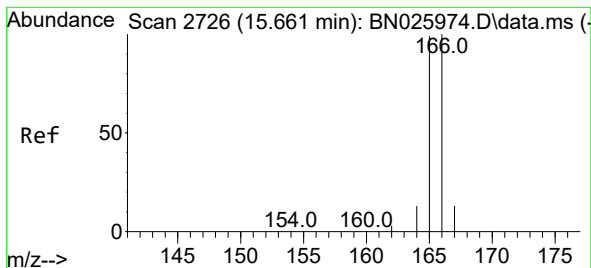

#12

Fluorene

Concen: 0.074 ng/ul

RT: 15.606 min Scan# 21

Delta R.T. -0.060 min

Lab File: BN026008.D

Acq: 24 Jun 2023 16:48

Instrument :

BNA_N

ClientSampleId :

SBLK447





Tgt Ion:166 Resp: 4555

Ion Ratio Lower Upper

166 100

165 6.7 79.9 119.9#

167 33.2 10.8 16.2#

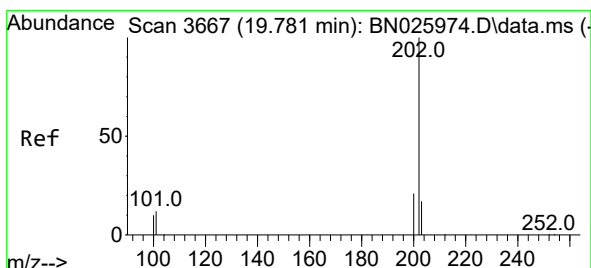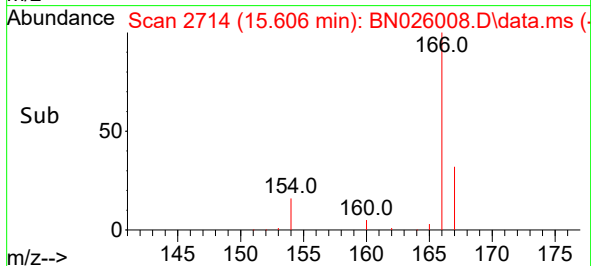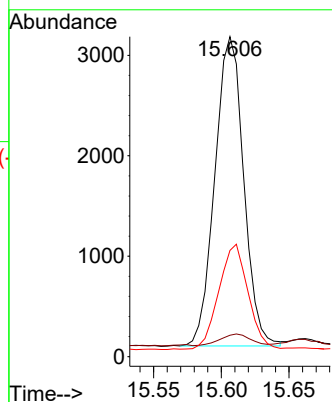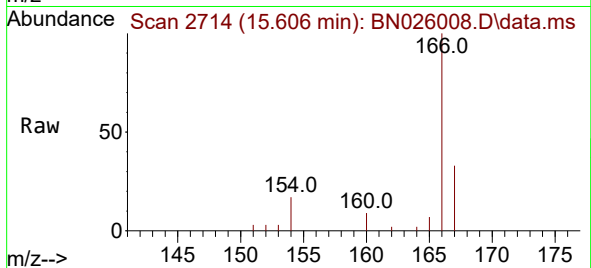

#20

Pyrene

Concen: 0.043 ng/ul

RT: 19.749 min Scan# 3660

Delta R.T. -0.033 min

Lab File: BN026008.D

Acq: 24 Jun 2023 16:48




Tgt Ion:202 Resp: 4211


Ion Ratio Lower Upper

202 100

101 176.2 11.4 17.0#


100 1363.3 9.1 13.7#

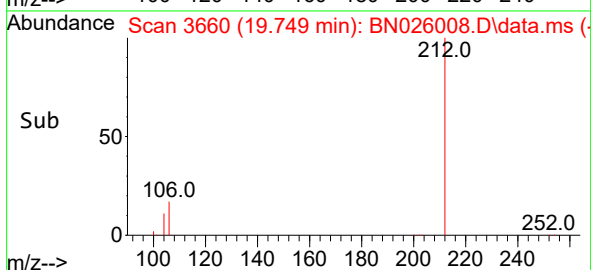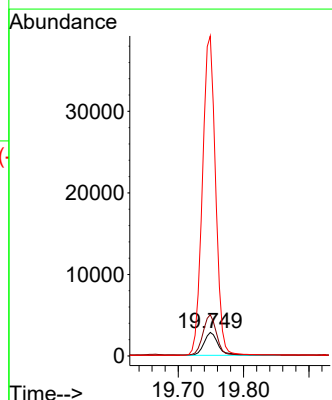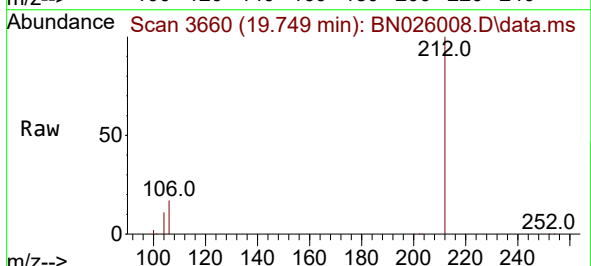

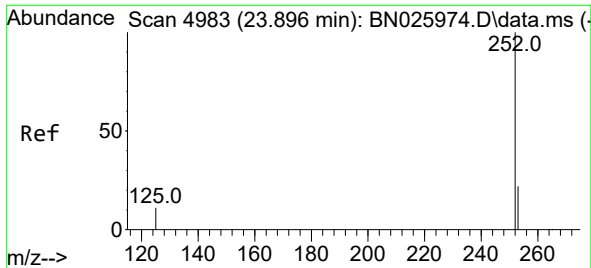

#26
Benzo(a)pyrene
Concen: 0.085 ng/ul
RT: 23.850 min Scan# 4983
Delta R.T. -0.059 min
Lab File: BN026008.D
Acq: 24 Jun 2023 16:48

Instrument :
BNA_N
ClientSampleId :
SBLK447

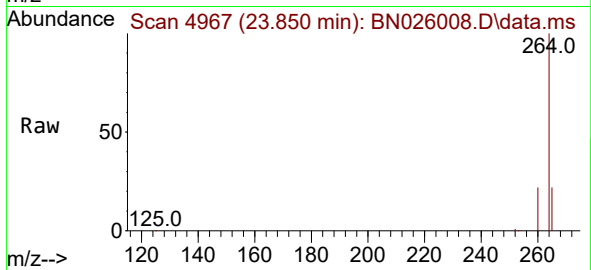

Tgt Ion:252 Resp: 6074
Ion Ratio Lower Upper
252 100
253 54.8 26.0 39.0#
125 48.6 17.3 25.9#

