

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062518\
 Data File : BN001904.D
 Acq On : 25 Jun 2018 10:34
 Operator : JU/SJ
 Sample : PB110517BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 26 04:48:07 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 26 04:45:44 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	425358	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	1918097	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.34	164	1160244	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.09	188	2744700	20.00	ng/ul	0.00
75) Chrysene-d12	21.29	240	3082960	20.00	ng/ul	0.00
83) Perylene-d12	23.52	264	2968983	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.27	96	63722	6.51	ng/uL	0.00
5) Phenol-d5	6.89	99	1164386	30.25	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	764323	32.18	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	954671	31.28	ng/ul	0.00
13) 4-Methylphenol-d8	8.41	113	934479	30.30	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	477576	33.53	ng/ul	0.00
22) 2-Nitrophenol-d4	9.58	143	511882	34.72	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.10	165	944511	30.01	ng/ul	0.00
29) 4-Chloroaniline-d4	10.62	131	1438528	44.15	ng/ul	0.00
43) Dimethylphthalate-d6	13.76	166	3395504	34.66	ng/ul	0.00
46) Acenaphthylene-d8	14.03	160	3987669	32.97	ng/ul	0.00
51) 4-Nitrophenol-d4	14.54	143	566491	31.39	ng/ul	0.00
57) Fluorene-d10	15.34	176	2866720	33.38	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.45	200	409334	27.38	ng/ul	0.00
70) Anthracene-d10	17.19	188	4635046	34.95	ng/ul	0.00
76) Pyrene-d10	19.49	212	5359991	34.49	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.38	264	5604198	34.71	ng/ul	0.00


Target Compounds				Ovalue	
45) 2,6-Dinitrotoluene	13.76	165	19553	1.075	ng/ul# 44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062518\
Data File : BN001904.D
Acq On : 25 Jun 2018 10:34
Operator : JU/SJ
Sample : PB110517BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 26 04:48:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061918.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 26 04:45:44 2018
Response via : Initial Calibration

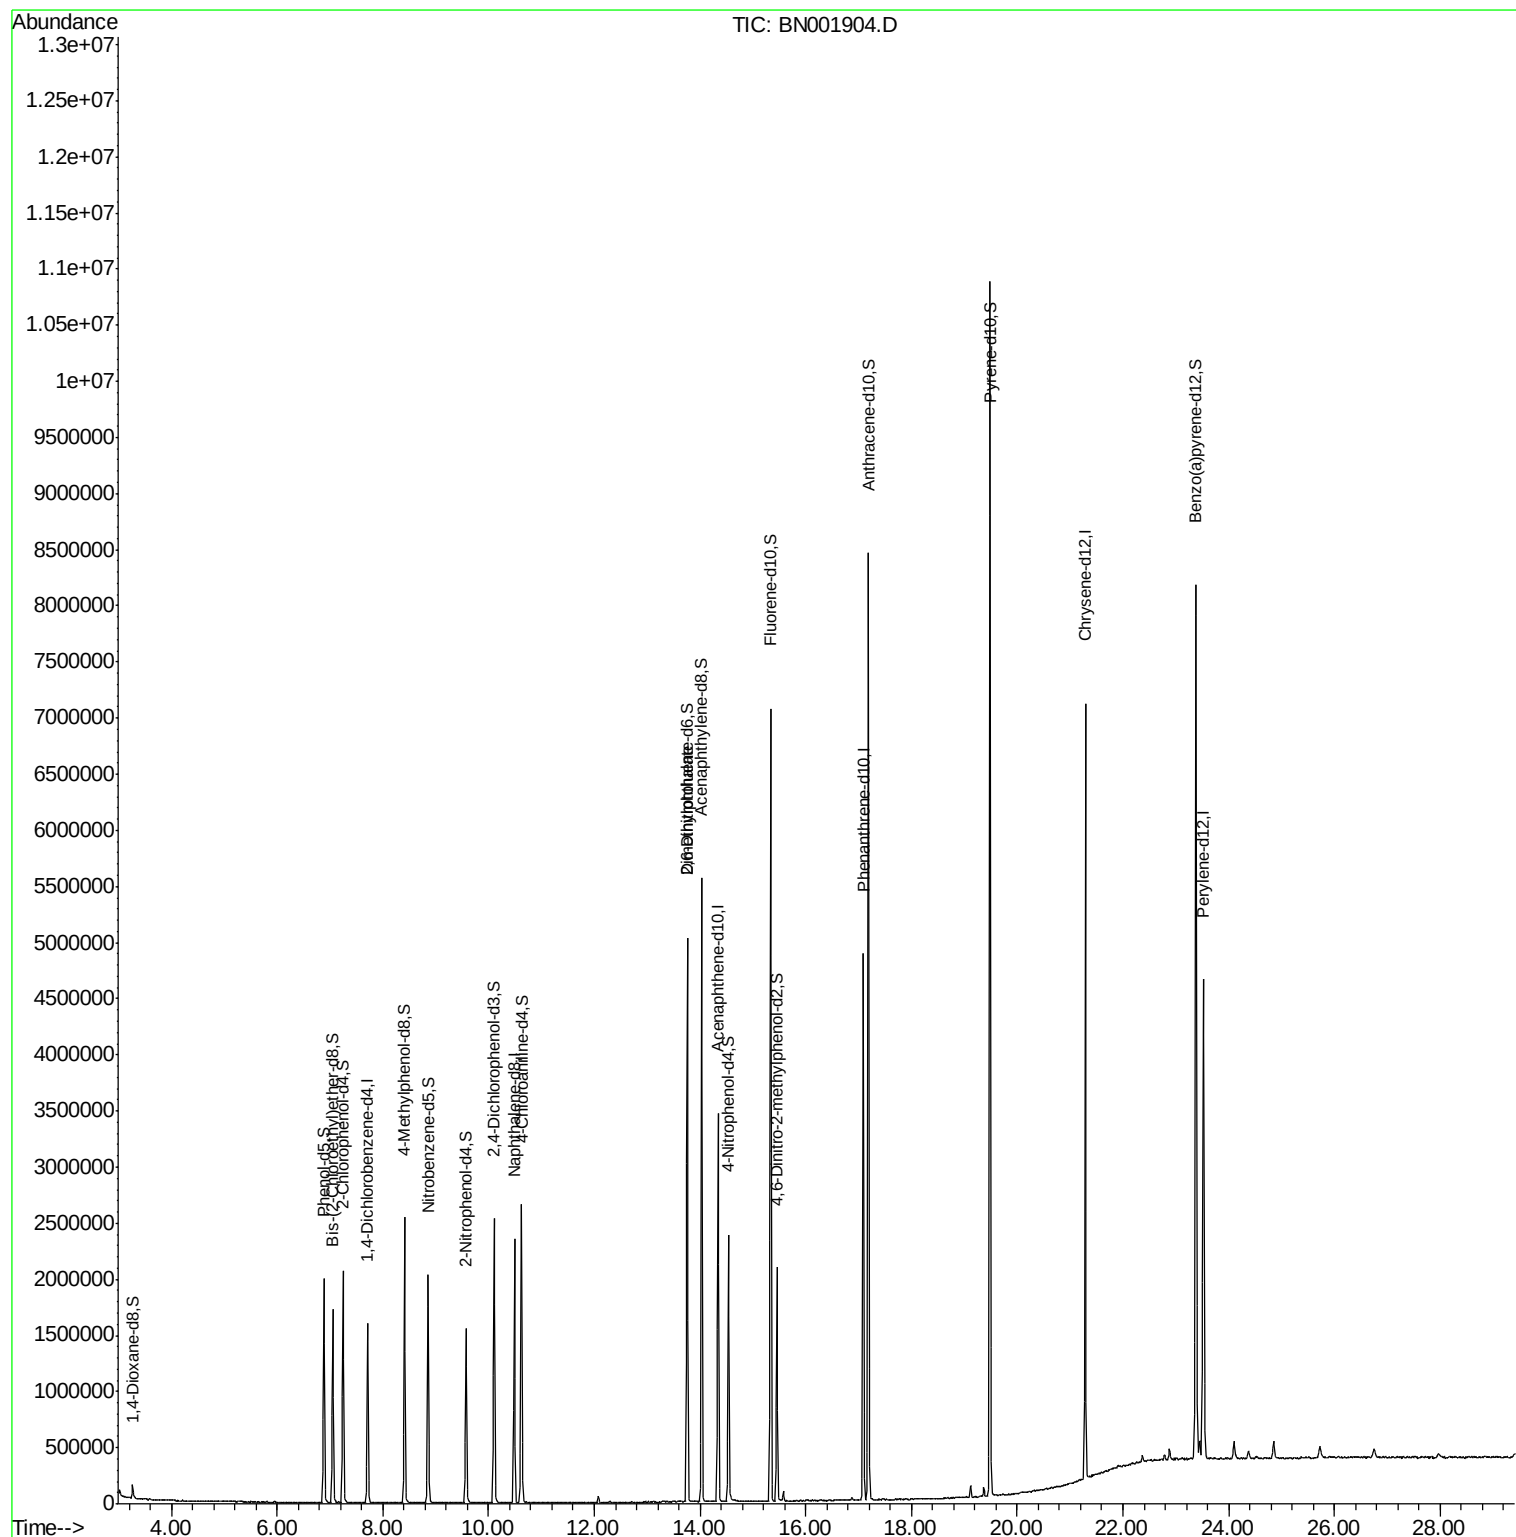

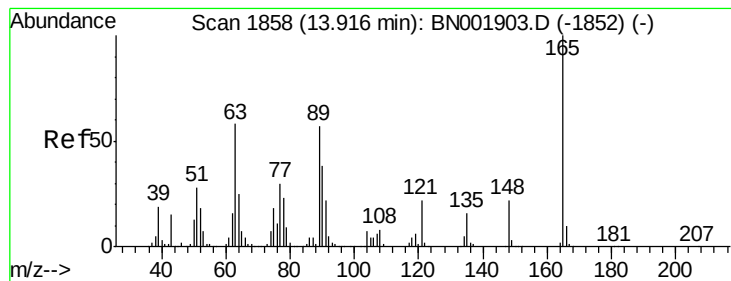

#45

2,6-Dinitrotoluene

Concen: 1.075 ng/ul

RT: 13.76 min Scan# 1832

Delta R.T. -0.15 min


Lab File: BN001904.D

Acq: 25 Jun 2018 10:34

Instrument :

BNA_N

ClientSampleId :

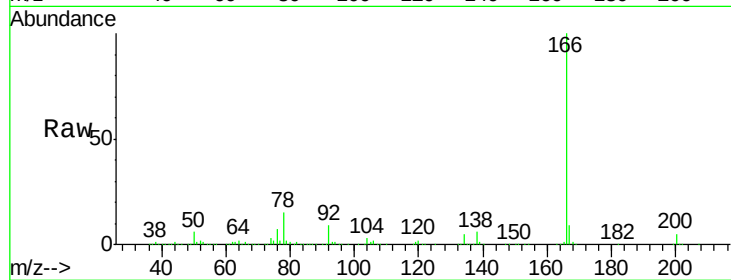

Tot Ion:	165	Resp:	19553
Ion	Ratio	Lower	Upper
165	100		
89	0.0	43.8	65.8#
121	25.5	17.8	26.6

