

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN062518\
 Data File : BN001911.D
 Acq On : 25 Jun 2018 14:50
 Operator : JU/SJ
 Sample : J3569-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 26 04:49:05 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 26 04:45:44 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	592638	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	2718026	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.34	164	1554652	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.09	188	3502785	20.00	ng/ul	0.00
75) Chrysene-d12	21.29	240	2776517	20.00	ng/ul	0.00
83) Perylene-d12	23.52	264	2448471	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.27	96	54952	4.03	ng/uL	0.00
5) Phenol-d5	6.89	99	1224403	22.83	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	789552	23.86	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	1000885	23.54	ng/ul	0.00
13) 4-Methylphenol-d8	8.41	113	923875	21.50	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	503276	24.93	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	556027	26.62	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.11	165	1033064	23.16	ng/ul	0.00
29) 4-Chloroaniline-d4	10.62	131	1246174	26.99	ng/ul	0.00
43) Dimethylphthalate-d6	13.76	166	3285964	25.03	ng/ul	0.00
46) Acenaphthylene-d8	14.03	160	4049561	24.98	ng/ul	0.00
51) 4-Nitrophenol-d4	14.54	143	526078	21.75	ng/ul	0.00
57) Fluorene-d10	15.34	176	2827496	24.57	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.45	200	433891	22.74	ng/ul	0.00
70) Anthracene-d10	17.19	188	4249076	25.11	ng/ul	0.00
76) Pyrene-d10	19.49	212	4342530	31.03	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.38	264	3411058	25.62	ng/ul	0.00

Target Compounds


					Ovalue
6) Phenol	6.91	94	98245	1.816	ng/ul 94
44) Dimethylphthalate	13.80	163	1335122	10.347	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN062518\
Data File : BN001911.D
Acq On : 25 Jun 2018 14:50
Operator : JU/SJ
Sample : J3569-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 26 04:49:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061918.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 26 04:45:44 2018
Response via : Initial Calibration

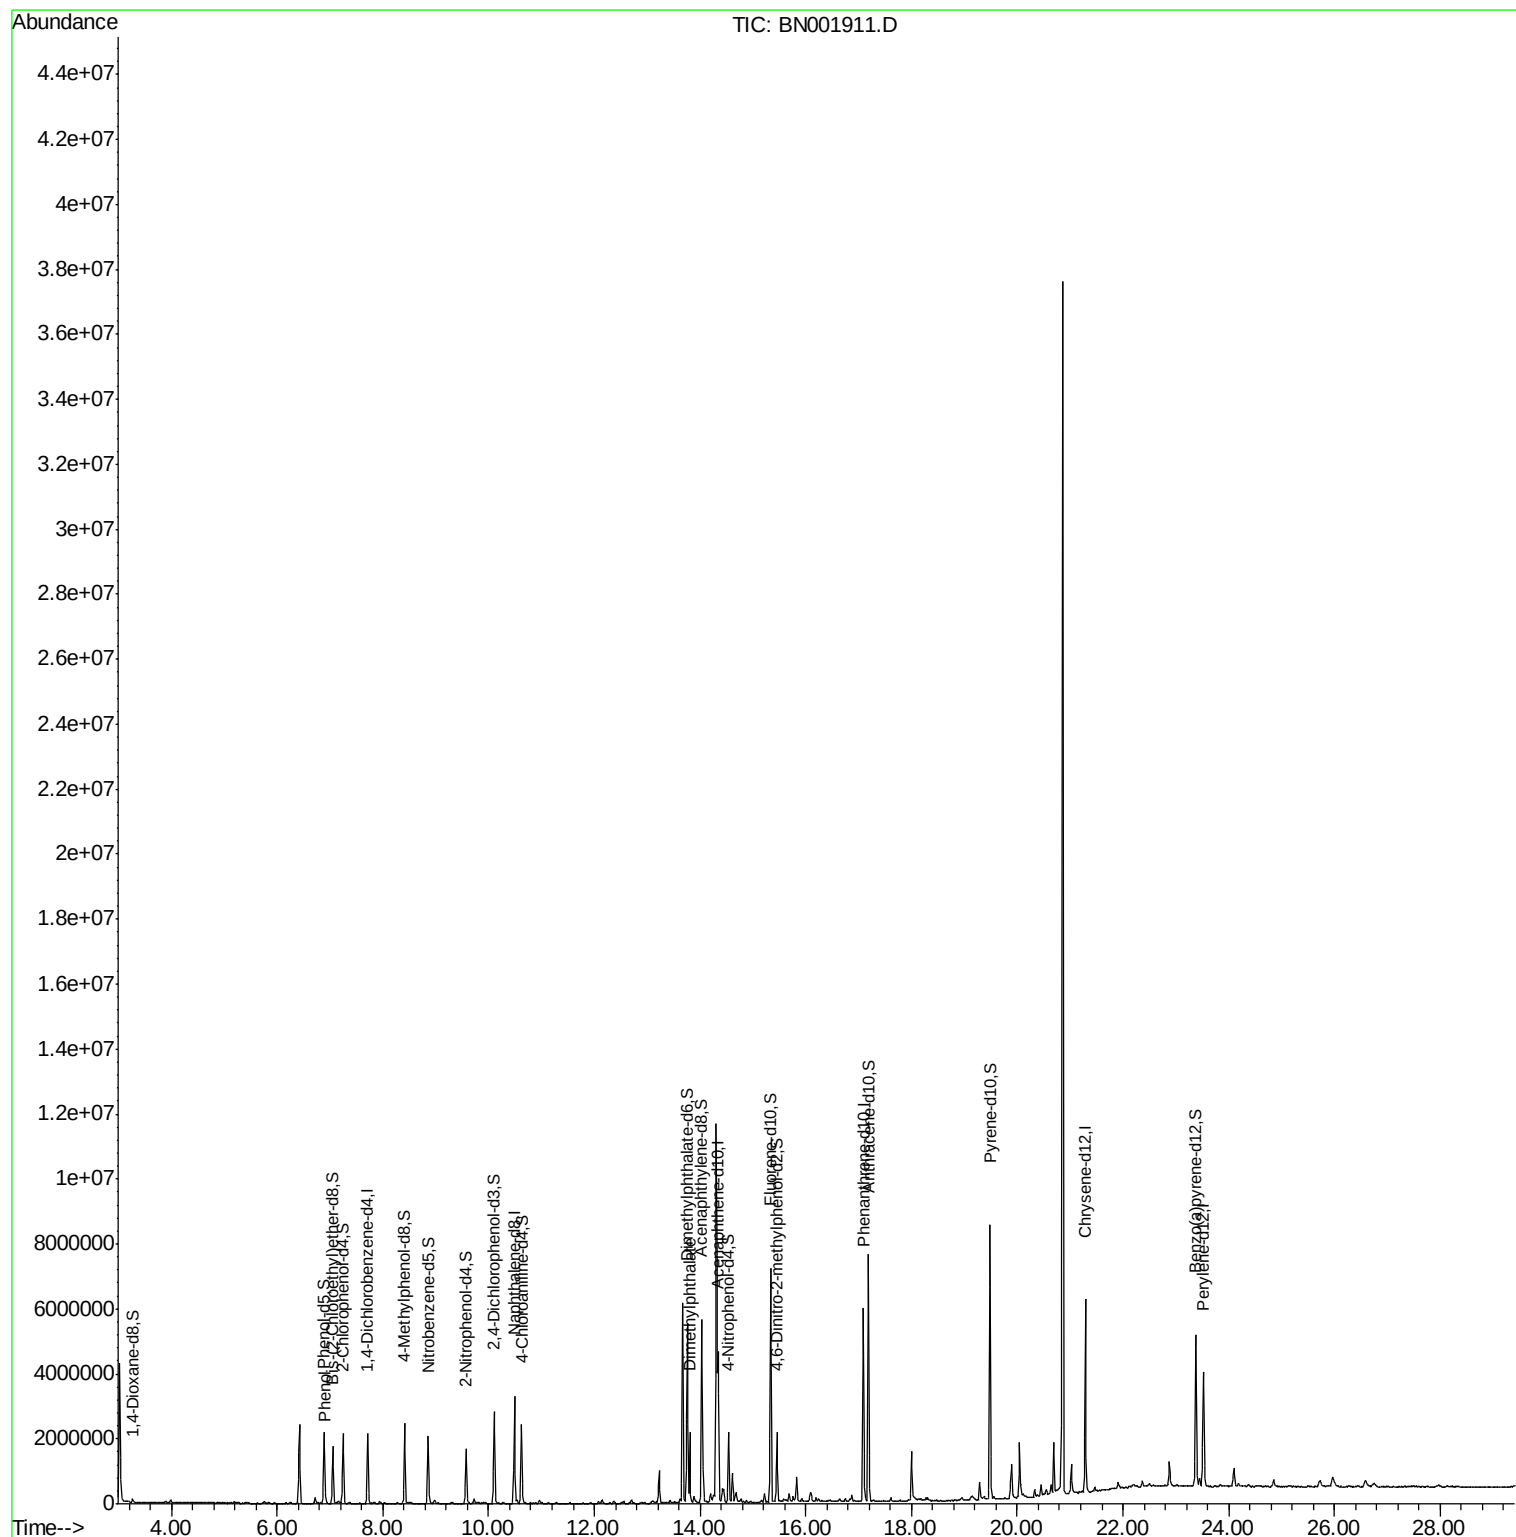

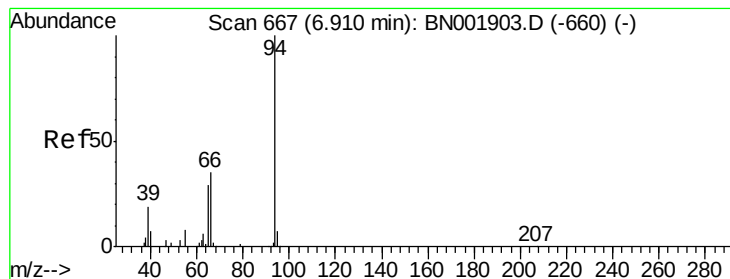





#6

Phenol

Concen: 1.816 ng/ul
 RT: 6.91 min Scan# 667
 Delta R.T. -0.00 min
 Lab File: BN001911.D
 Acq: 25 Jun 2018 14:50

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion: 94 Resp: 98245
 Ion Ratio Lower Upper
 94 100
 65 30.9 23.0 34.6
 66 42.9 30.4 45.6

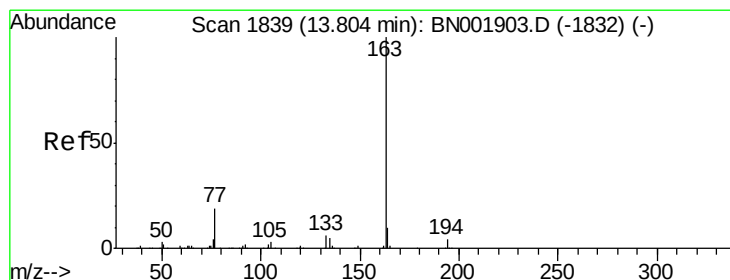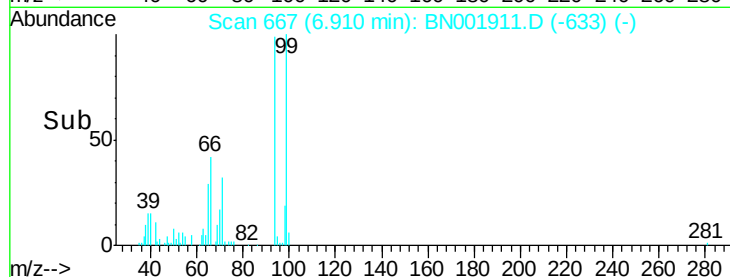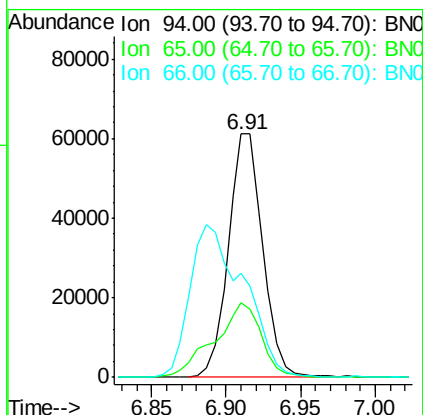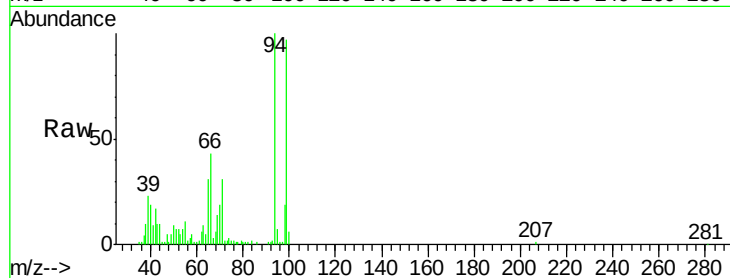

#44

Dimethylphthalate

Concen: 10.347 ng/ul
 RT: 13.80 min Scan# 1839
 Delta R.T. -0.00 min
 Lab File: BN001911.D
 Acq: 25 Jun 2018 14:50

Tgt Ion:163 Resp: 1335122
 Ion Ratio Lower Upper
 163 100
 194 4.2 4.0 6.0
 164 10.3 8.4 12.6

