

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN062518\
 Data File : BN001916.D
 Acq On : 25 Jun 2018 17:47
 Operator : JU/SJ
 Sample : J3569-22
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DAXT7

Quant Time: Jun 26 04:49:38 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 26 04:45:44 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	553934	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	2387078	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.34	164	1330154	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.09	188	2604618	20.00	ng/ul	0.00
75) Chrysene-d12	21.29	240	2199177	20.00	ng/ul	0.00
83) Perylene-d12	23.52	264	2279076	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.27	96	35767	2.80	ng/uL	0.00
5) Phenol-d5	6.89	99	686164	13.69	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	487499	15.76	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	596539	15.01	ng/ul	0.00
13) 4-Methylphenol-d8	8.41	113	573137	14.27	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	281272	15.87	ng/ul	0.00
22) 2-Nitrophenol-d4	9.58	143	301633	16.44	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.10	165	555638	14.18	ng/ul	0.00
29) 4-Chloroaniline-d4	10.62	131	794857	19.60	ng/ul	0.00
43) Dimethylphthalate-d6	13.76	166	1737866	15.47	ng/ul	0.00
46) Acenaphthylene-d8	14.03	160	2085850	15.04	ng/ul	0.00
51) 4-Nitrophenol-d4	14.54	143	89945	4.35	ng/ul	0.00
57) Fluorene-d10	15.33	176	1456559	14.79	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.45	200	77901	5.49	ng/ul	0.00
70) Anthracene-d10	17.19	188	2067205	16.43	ng/ul	0.00
76) Pyrene-d10	19.49	212	2083706	18.80	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.38	264	2191922	17.69	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.80	163	482224	4.368	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN062518\
Data File : BN001916.D
Acq On : 25 Jun 2018 17:47
Operator : JU/SJ
Sample : J3569-22
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DAXT7

Quant Time: Jun 26 04:49:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061918.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 26 04:45:44 2018
Response via : Initial Calibration

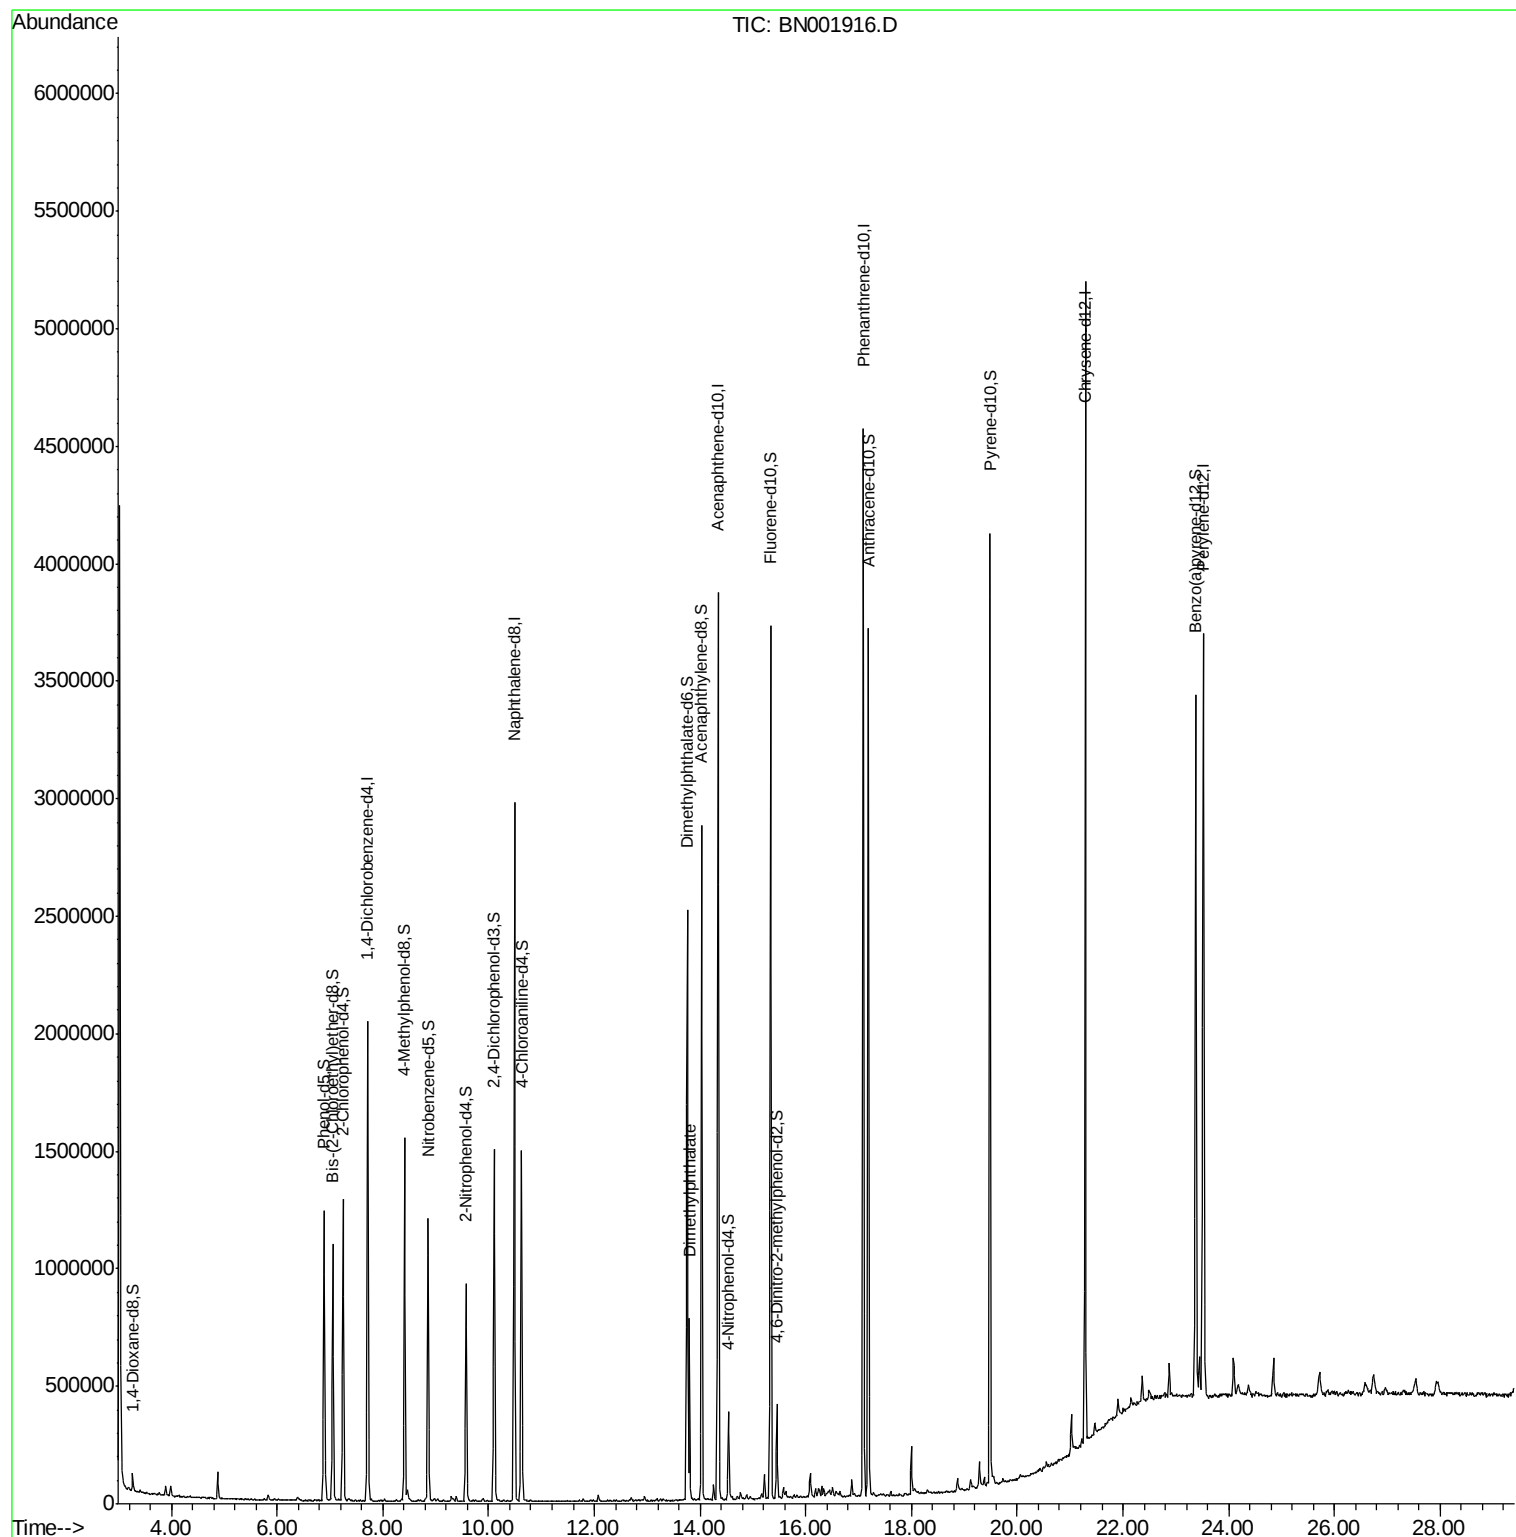

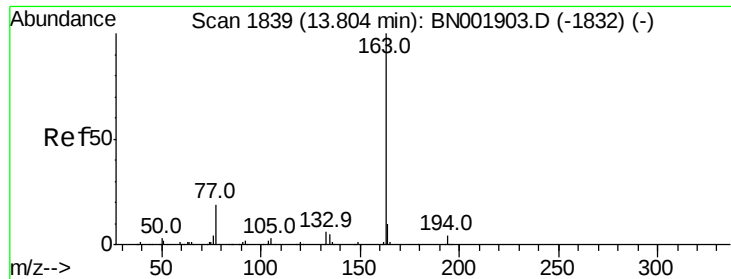

#44

Dimethylphthalate

Concen: 4.368 ng/ul

RT: 13.80 min Scan# 1838

Delta R.T. -0.01 min

Lab File: BN001916.D

Acq: 25 Jun 2018 17:47

Instrument :

BNA_N

ClientSampleId :

DAXT7


Tot Ion:163 Resp: 482224

Ion Ratio Lower Upper

163 100

194 4.1 4.0 6.0

164 10.2 8.4 12.6

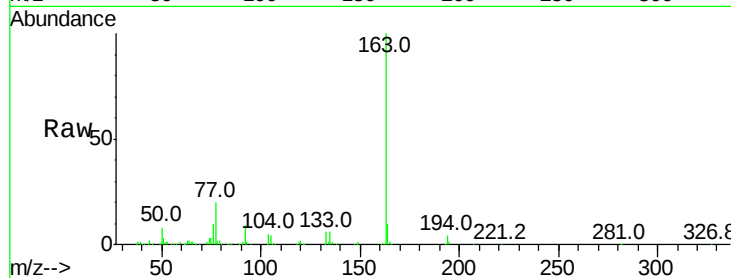

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

