

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN062518\
 Data File : BN001917.D
 Acq On : 25 Jun 2018 18:22
 Operator : JU/SJ
 Sample : J3569-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DAXQ5

Manual Integrations
 APPROVED

Sohil
 6/27/2018 11:06:38 AM

Quant Time: Jun 26 05:56:59 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 26 04:45:44 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	518608	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	2347342	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.34	164	1434224	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.09	188	3099938	20.00	ng/ul	0.00
75) Chrysene-d12	21.29	240	2443046	20.00	ng/ul	0.00
83) Perylene-d12	23.52	264	2189463	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.27	96	27990m	2.34	ng/uL	0.00
5) Phenol-d5	6.89	99	549073	11.70	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	372068	12.85	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	454579	12.22	ng/ul	0.00
13) 4-Methylphenol-d8	8.41	113	445521	11.85	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	219550	12.59	ng/ul	0.00
22) 2-Nitrophenol-d4	9.58	143	230240	12.76	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.10	165	448767	11.65	ng/ul	0.00
29) 4-Chloroaniline-d4	10.62	131	618773	15.52	ng/ul	0.00
43) Dimethylphthalate-d6	13.75	166	1518952	12.54	ng/ul	0.00
46) Acenaphthylene-d8	14.03	160	1884296	12.60	ng/ul	0.00
51) 4-Nitrophenol-d4	14.54	143	99312	4.45	ng/ul	0.00
57) Fluorene-d10	15.33	176	1349149	12.71	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.45	200	83632	4.95	ng/ul	0.00
70) Anthracene-d10	17.19	188	1932250	12.90	ng/ul	0.00
76) Pyrene-d10	19.49	212	1980376	16.08	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.37	264	1589704	13.35	ng/ul	-0.01

Target Compounds					Ovalue	
44) Dimethylphthalate	13.80	163	368433	3.095	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN062518\
Data File : BN001917.D
Acq On : 25 Jun 2018 18:22
Operator : JU/SJ
Sample : J3569-04
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
DAXQ5

Manual Integrations
APPROVED

Sohil
6/27/2018 11:06:38 AM

Quant Time: Jun 26 05:56:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061918.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 26 04:45:44 2018
Response via : Initial Calibration

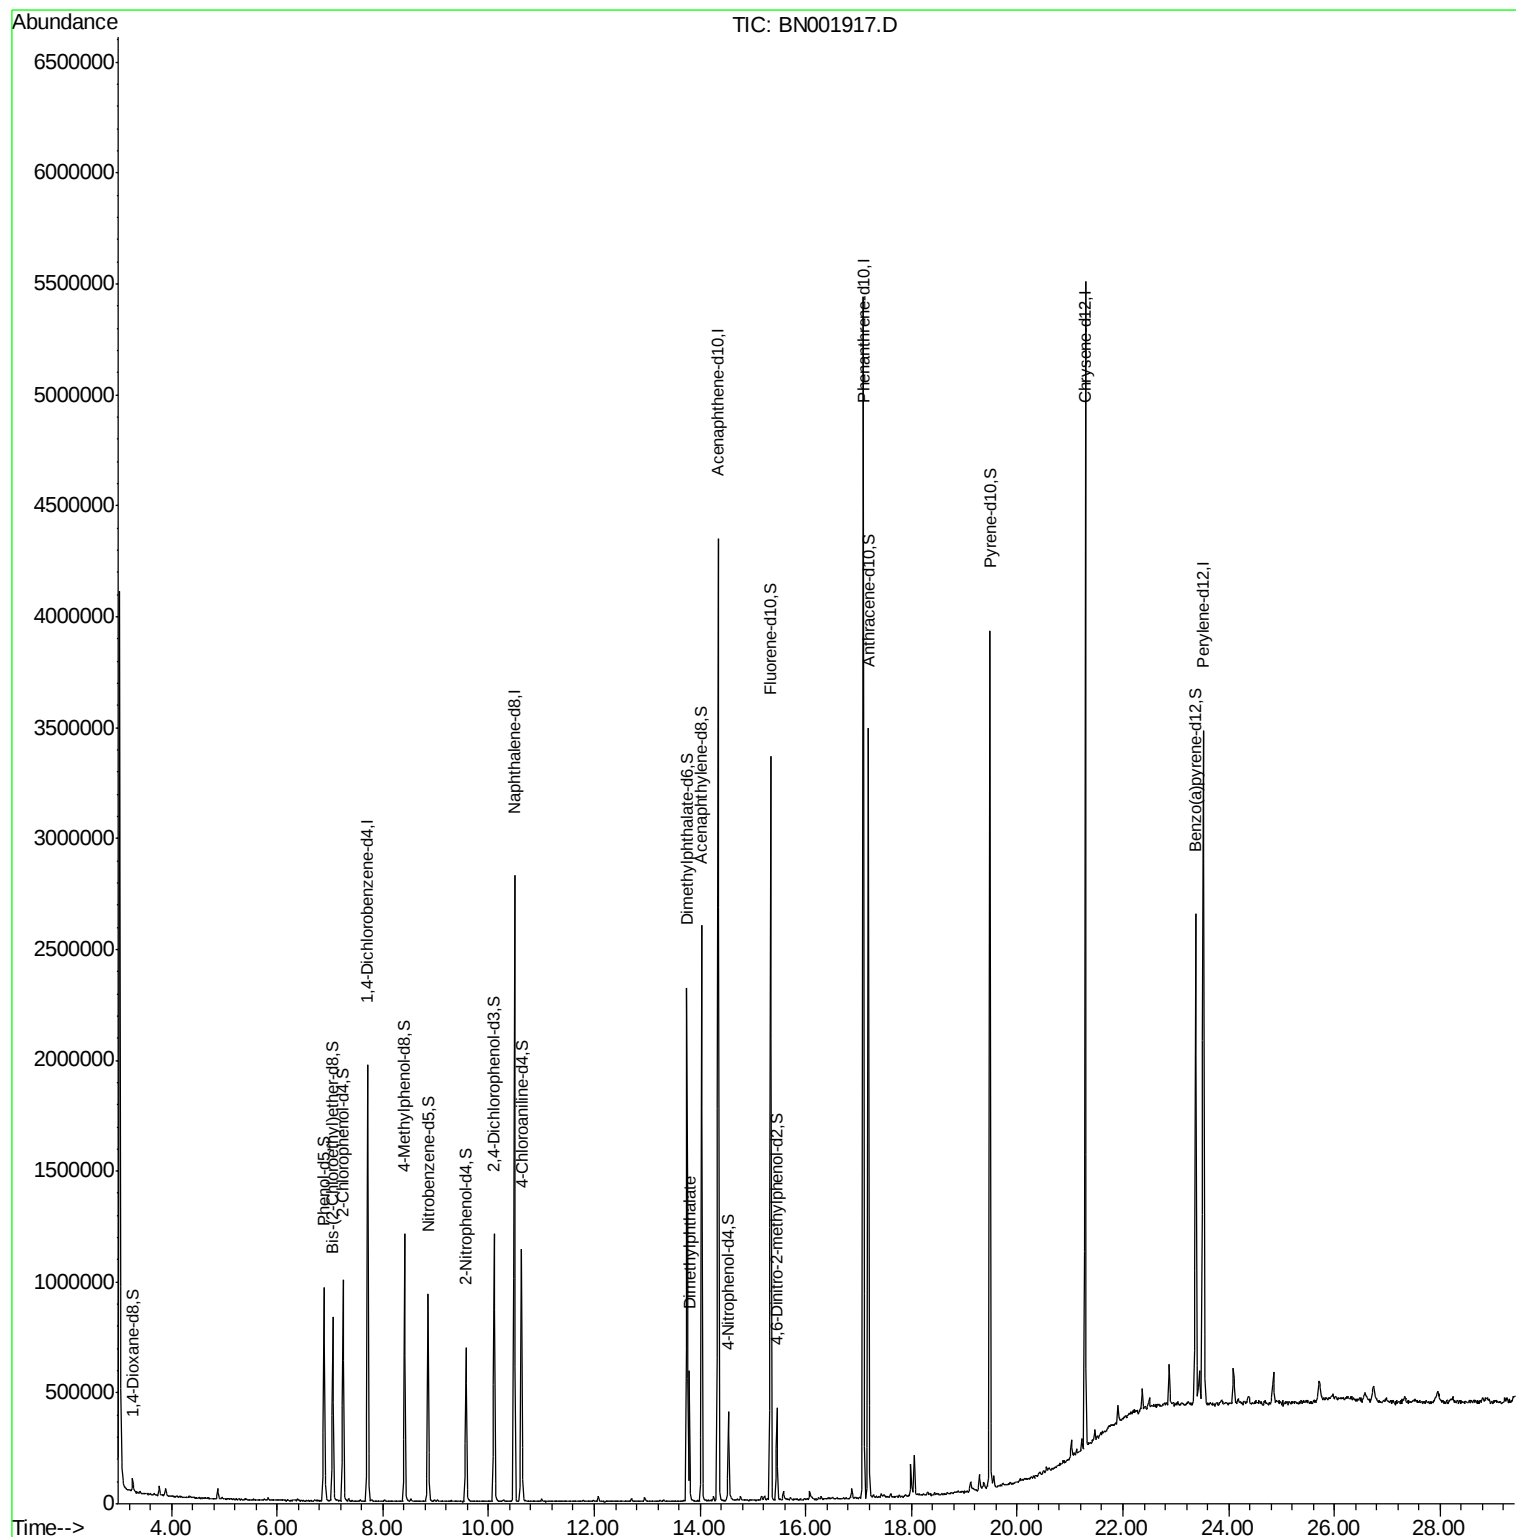

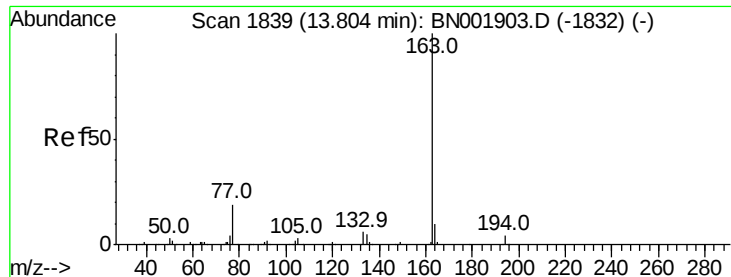

#44

Dimethylphthalate

Concen: 3.095 ng/ul

RT: 13.80 min Scan# 1838

Delta R.T. -0.01 min

Lab File: BN001917.D

Acq: 25 Jun 2018 18:22

Instrument :

BNA_N

ClientSampleId :

DAXQ5

Tot Ion:	163	Resp:	368433
Ion Ratio	Lower	Upper	
163	100		
194	4.2	4.0	6.0
164	10.4	8.4	12.6

Manual Integrations
APPROVED

Sohil
6/27/2018 11:06:38 AM

