
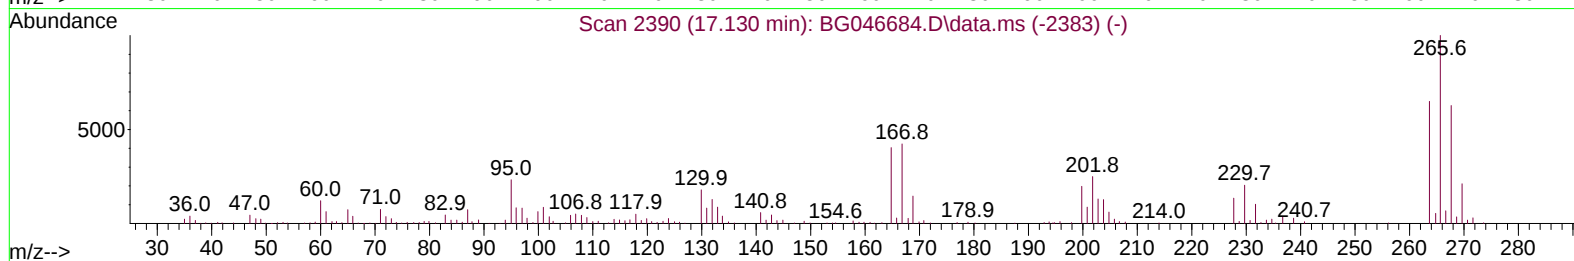
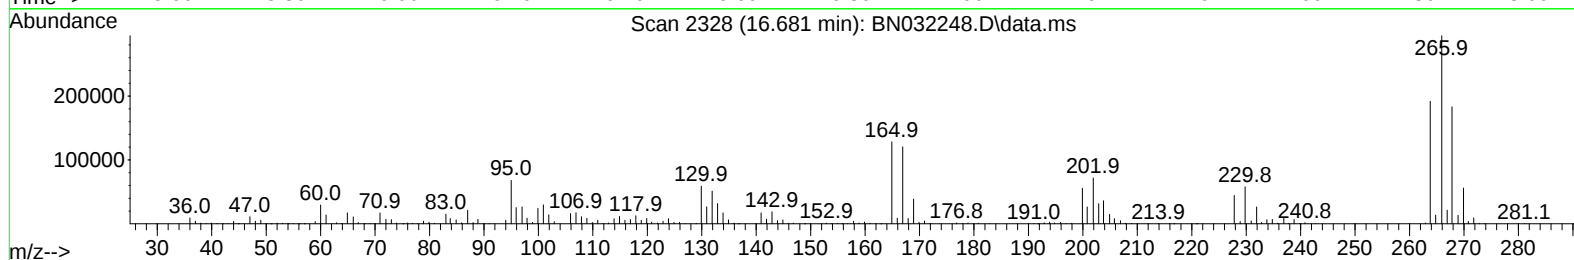


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062524\
Data File : BN032248.D
Acq On : 25 Jun 2024 20:14
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 51 Sample Multiplier: 1

Quant Time: Jun 26 02:35:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration

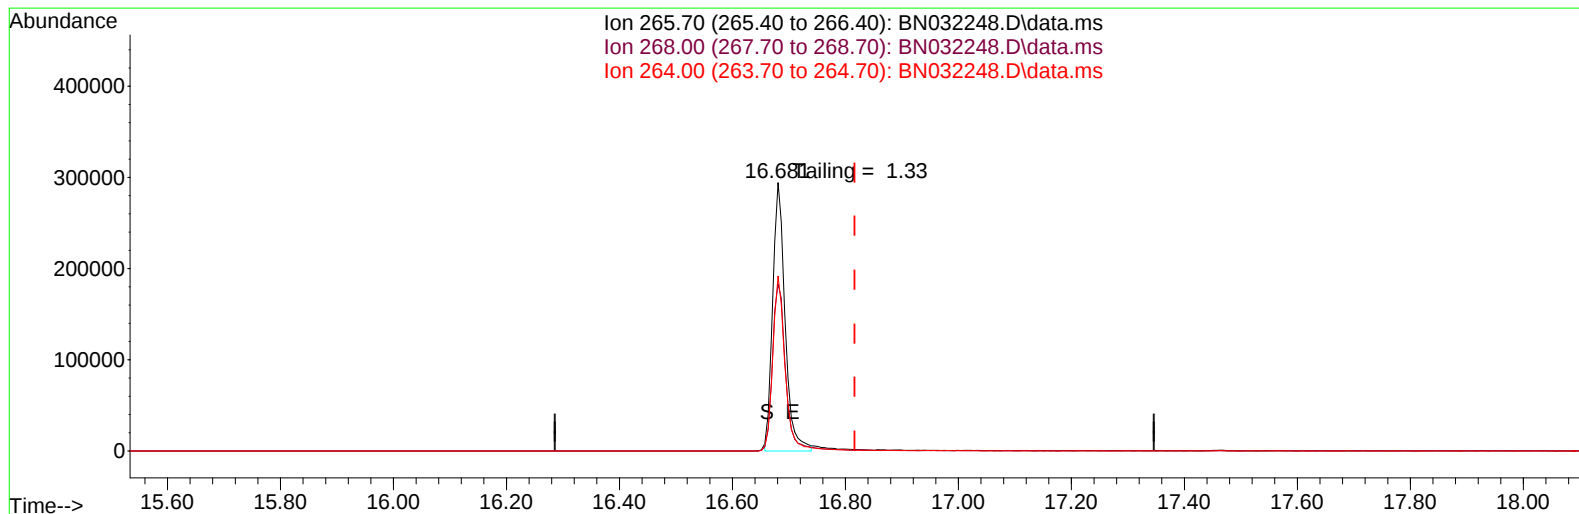

TIC: BN032248.D\data.ms

(70) Pentachlorophenol (C)




16.681min (-0.135) 26527.00 ng

response 469856

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.23
264.00	61.60	65.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062524\
Data File : BN032248.D
Acq On : 25 Jun 2024 20:14
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 51 Sample Multiplier: 1

Quant Time: Jun 26 02:35:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration

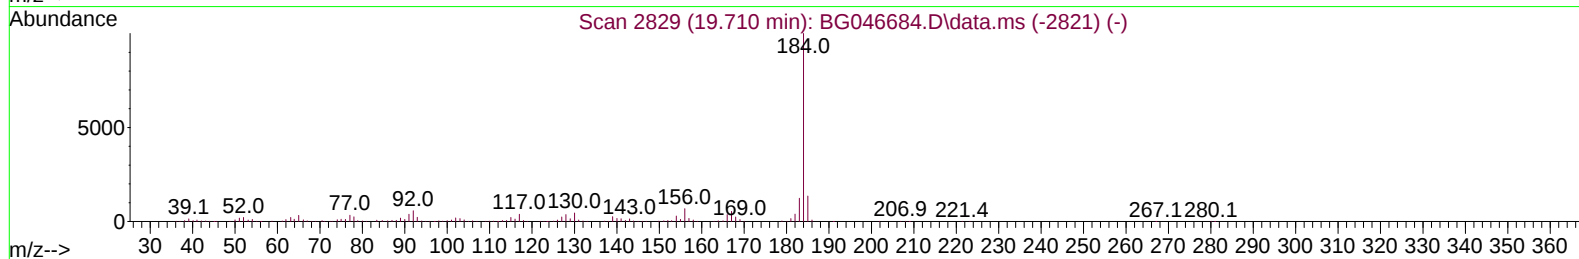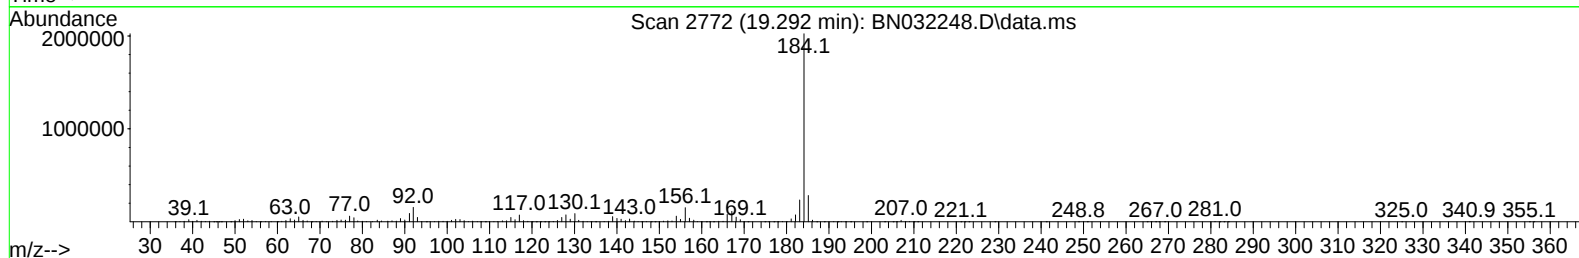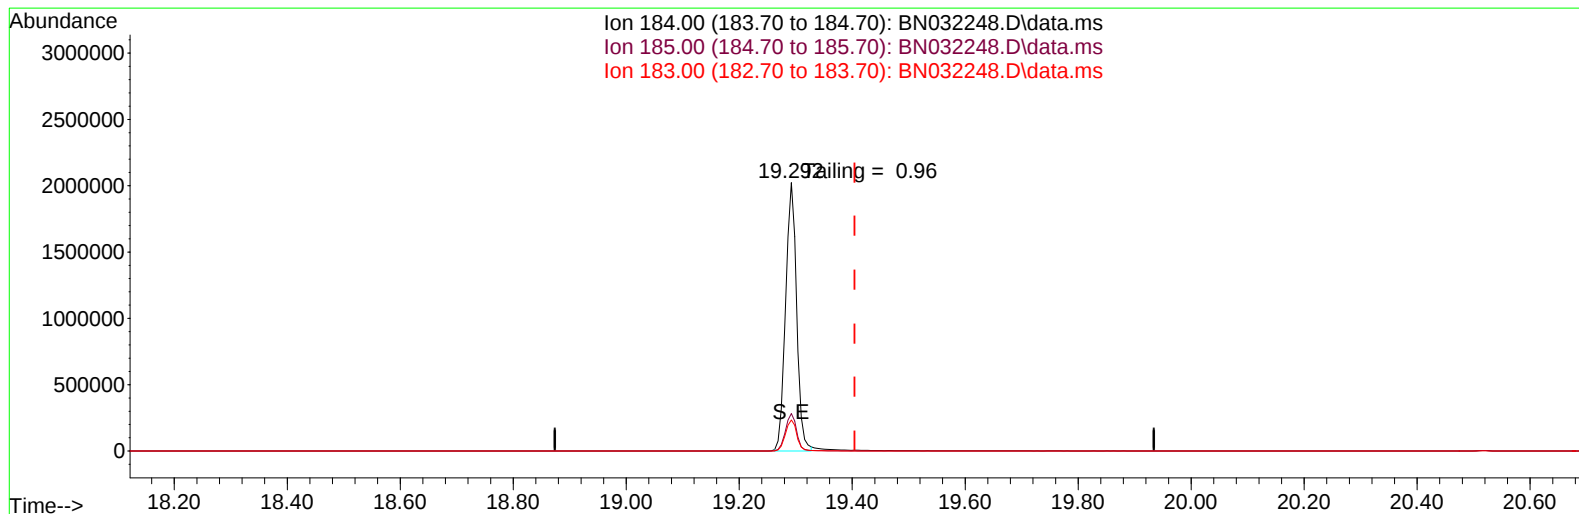

TIC: BN032248.D\data.ms

(77) Benzidine**19.292min (-0.112) 291038.87 ng****response 2799071**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.94
183.00	13.20	11.55
0.00	0.00	0.00