
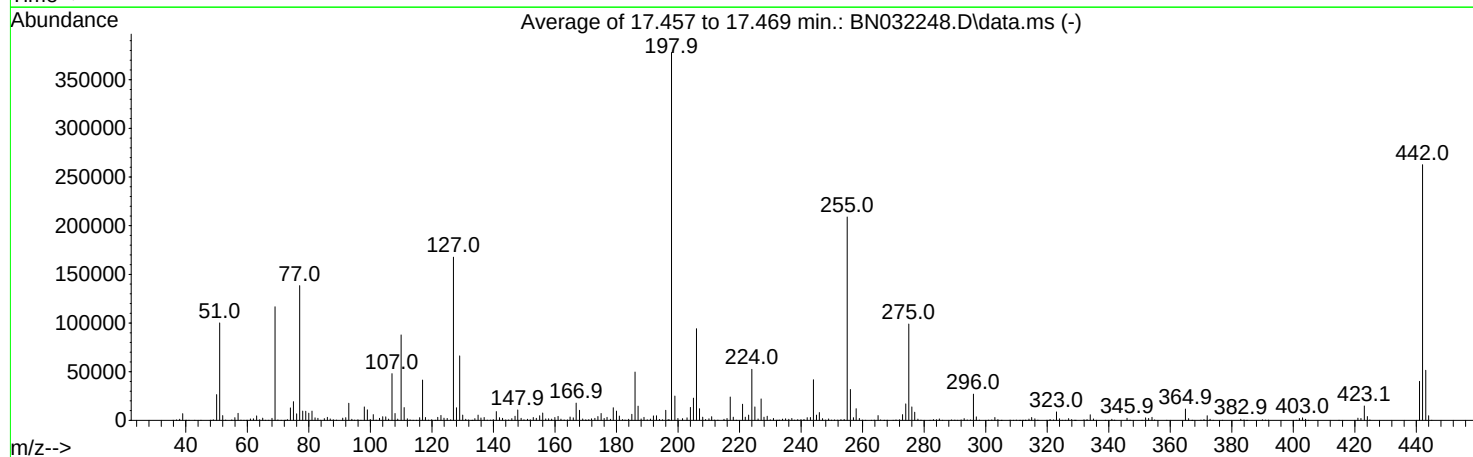


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062524\
Data File : BN032248.D
Acq On : 25 Jun 2024 20:14
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN061024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 19 11:30:34 2024

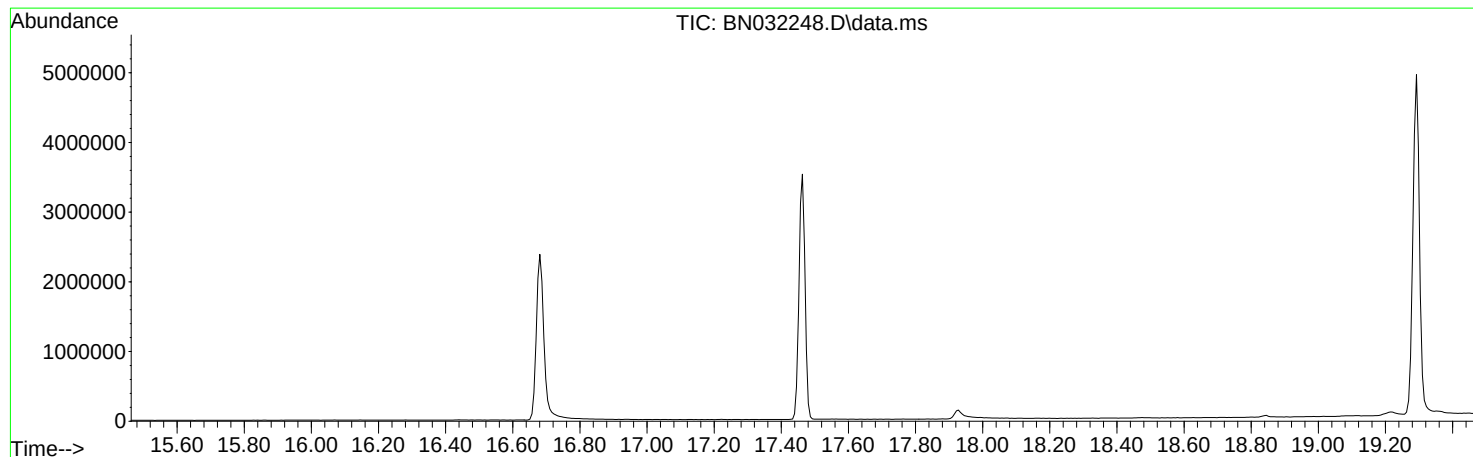




AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.5	100175	PASS
68	69	0.00	2	1.9	2237	PASS
69	198	0.00	100	30.9	116794	PASS
70	69	0.00	2	0.4	505	PASS
127	198	10	80	44.4	167699	PASS
197	198	0.00	2	0.2	783	PASS
198	198	100	100	100.0	377920	PASS
199	198	5	9	6.6	25067	PASS
275	198	10	60	26.2	98899	PASS
365	198	1	100	3.1	11742	PASS
441	198	0.01	100	10.6	40075	PASS
442	442	50	100	100.0	262635	PASS
443	442	15	24	19.6	51515	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062524\
Data File : BN032248.D
Acq On : 25 Jun 2024 20:14
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 26 02:35:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration

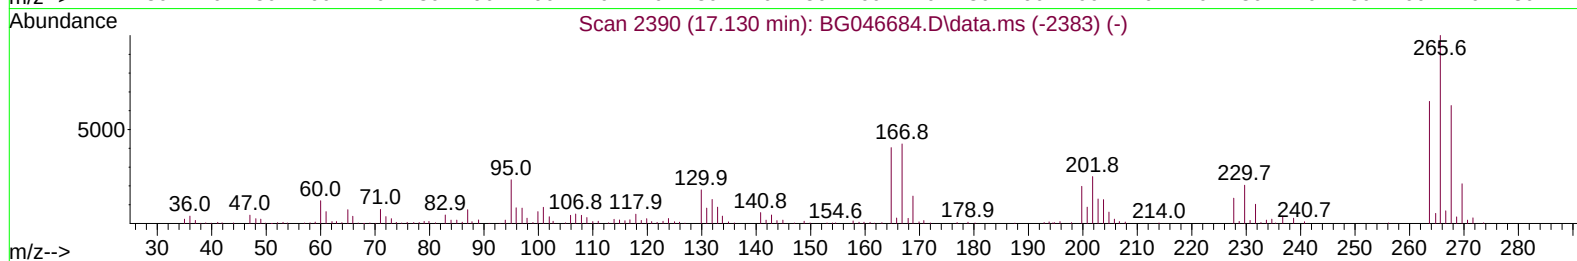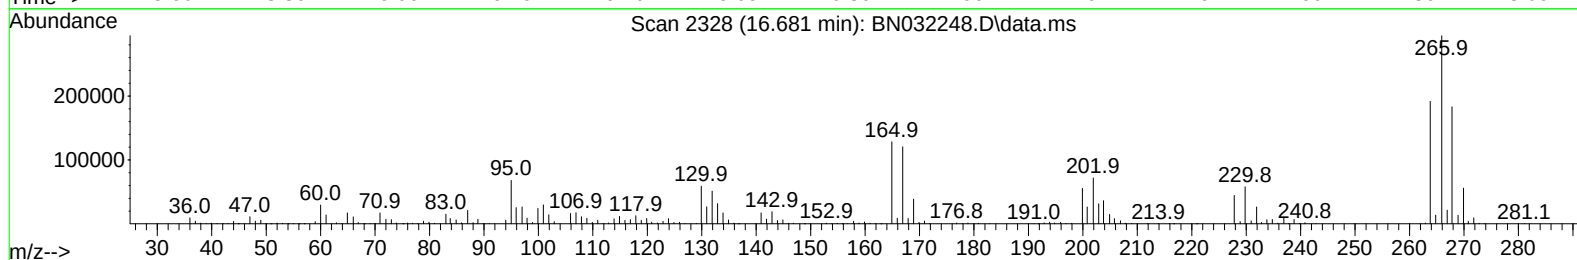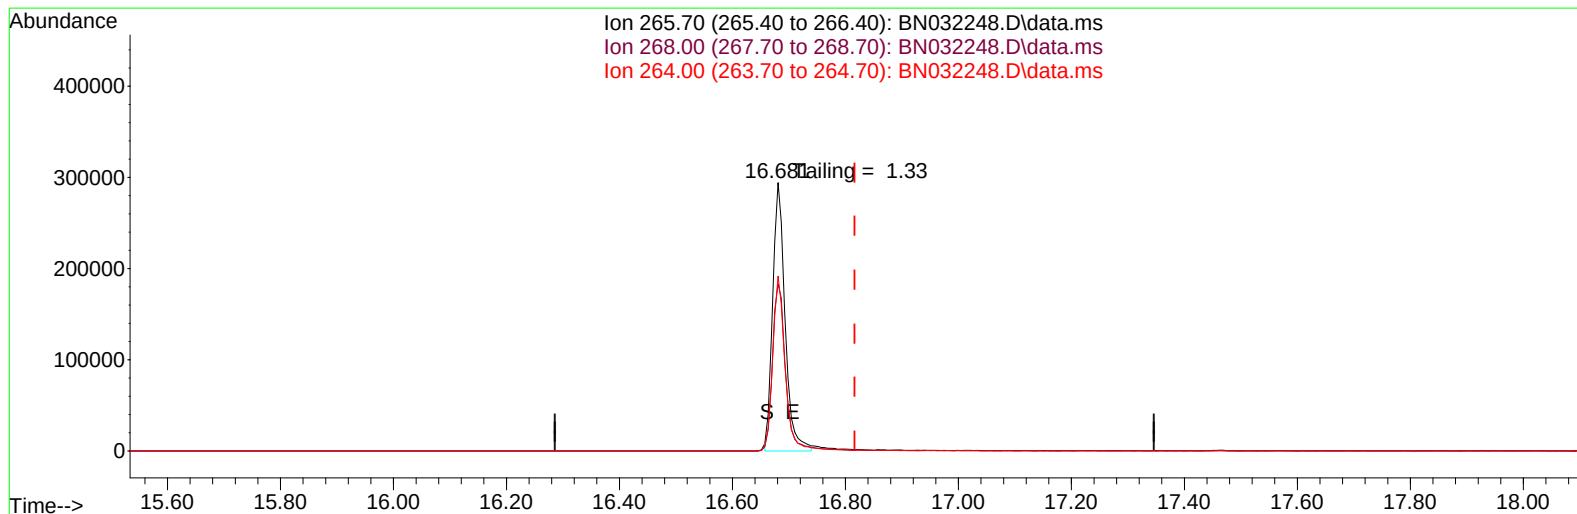

TIC: BN032248.D\data.ms

(70) Pentachlorophenol (C)

16.681min (-0.135) 26527.00 ng




response 469856

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.23
264.00	61.60	65.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062524\
Data File : BN032248.D
Acq On : 25 Jun 2024 20:14
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 26 02:35:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration

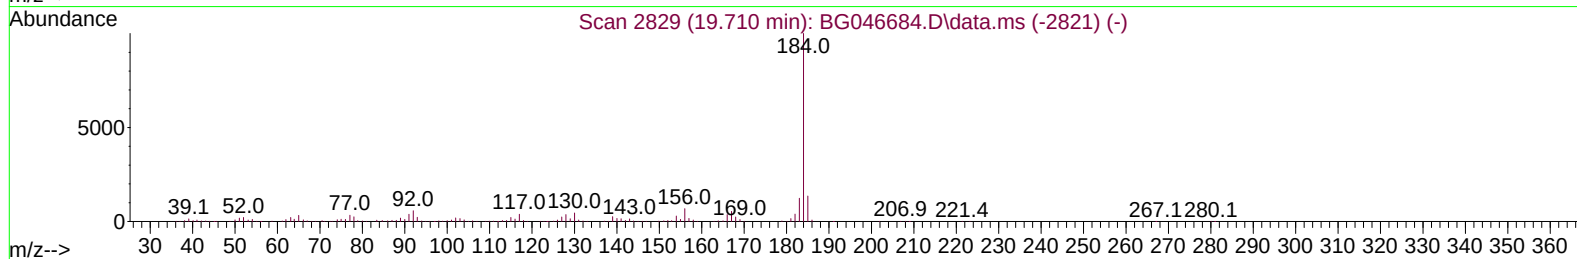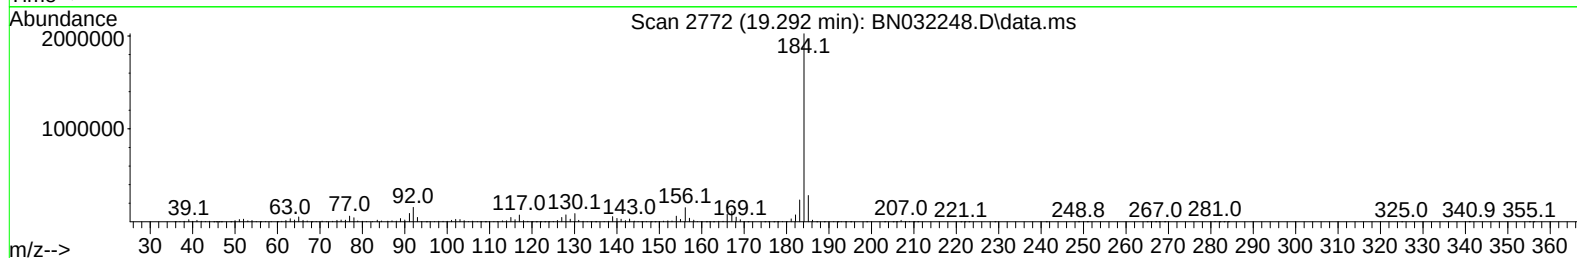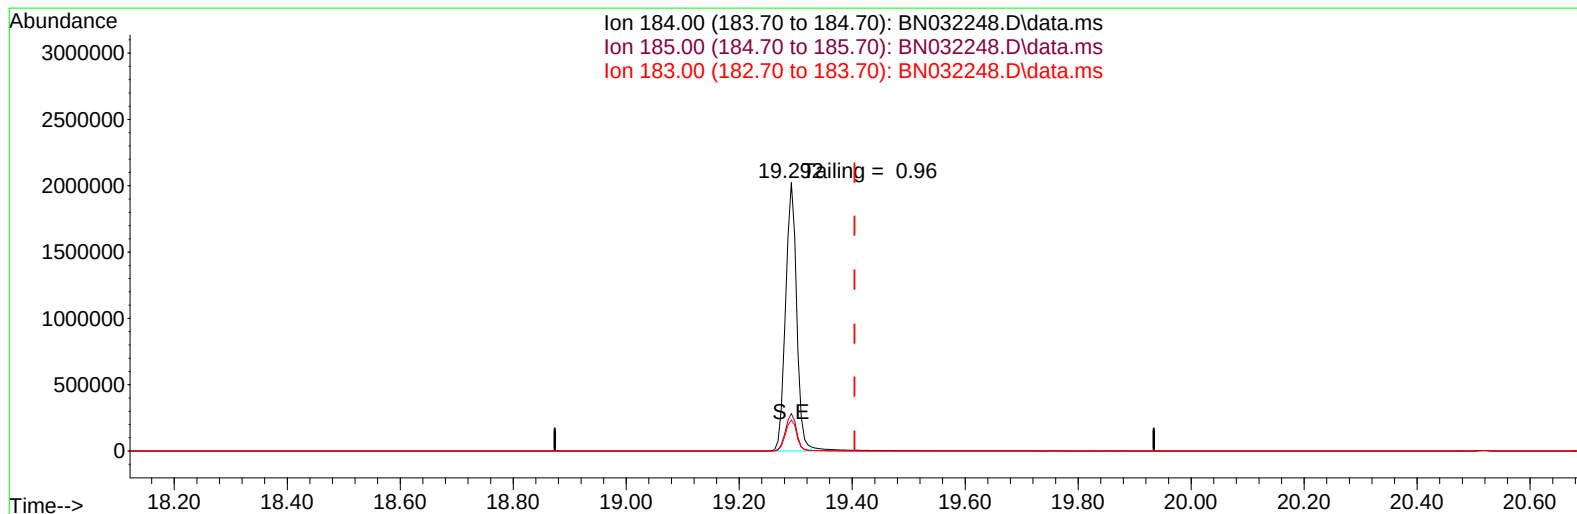

TIC: BN032248.D\data.ms

(77) Benzidine

19.292min (-0.112) 291038.87 ng

response 2799071

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.94
183.00	13.20	11.55
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/25/2024	BNA_N	<u>BN032248.D</u>
Compound Name	Response	Retention Time
DDT	1280521	20.516
DDD	60749	20.08
DDE	1176	19.569
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
61925	1342446	4.61

Instrument :
BNA_N
ClientSampleId :
DFTPP