


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062524\
Data File : BN032266.D
Acq On : 26 Jun 2024 08:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN061024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 19 11:30:34 2024

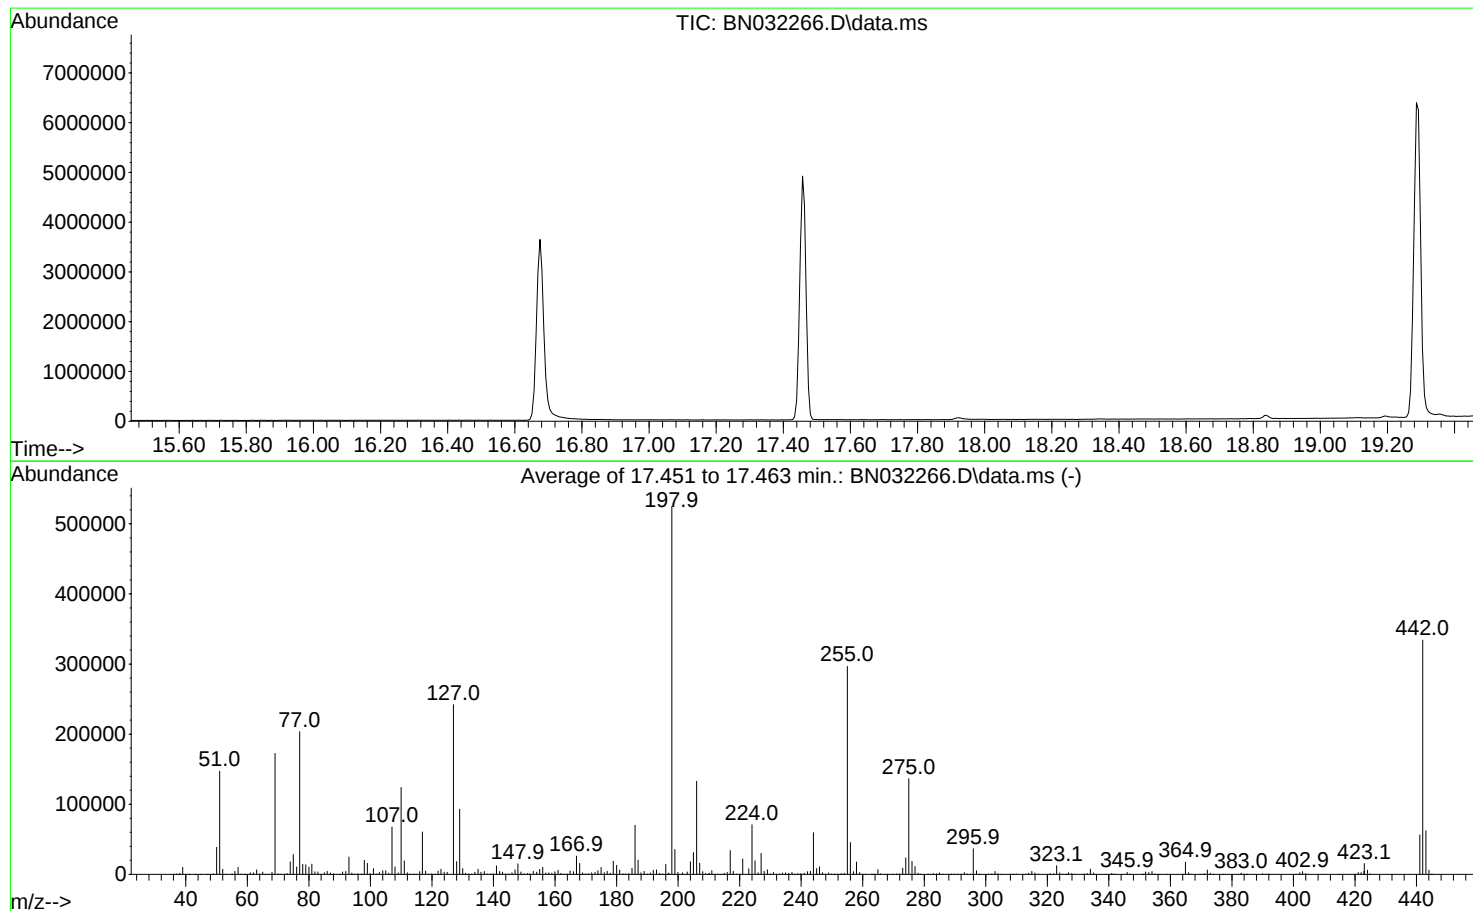




AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	147251	PASS
68	69	0.00	2	1.7	2880	PASS
69	198	0.00	100	32.9	172652	PASS
70	69	0.00	2	0.5	844	PASS
127	198	10	80	46.1	242112	PASS
197	198	0.00	2	0.4	1895	PASS
198	198	100	100	100.0	524736	PASS
199	198	5	9	6.8	35443	PASS
275	198	10	60	26.0	136603	PASS
365	198	1	100	3.3	17309	PASS
441	198	0.01	100	10.8	56456	PASS
442	442	50	100	100.0	334144	PASS
443	442	15	24	18.7	62339	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062524\
Data File : BN032266.D
Acq On : 26 Jun 2024 08:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 26 09:36:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration

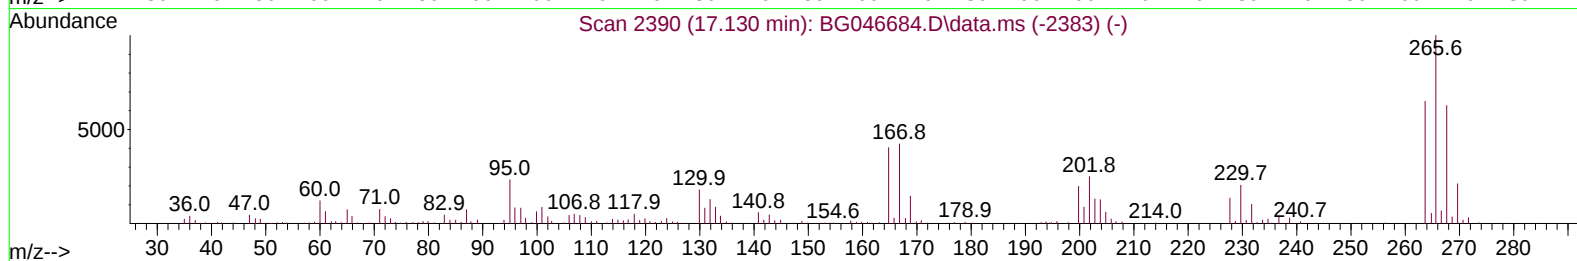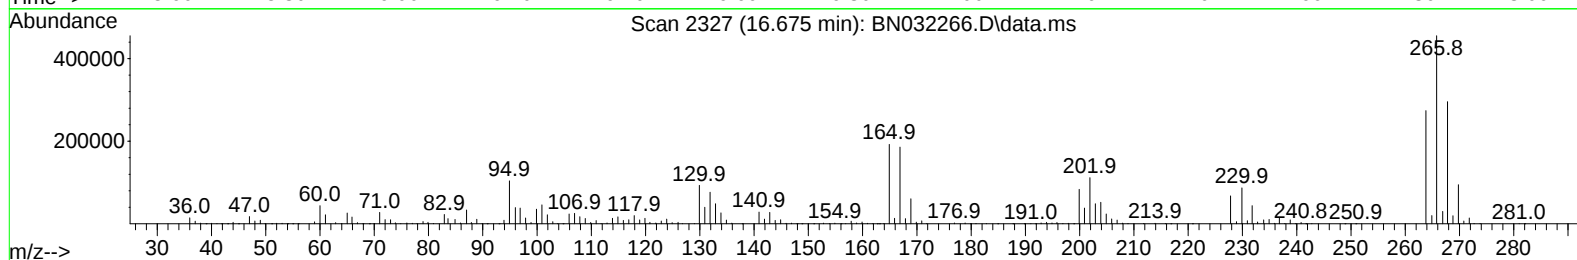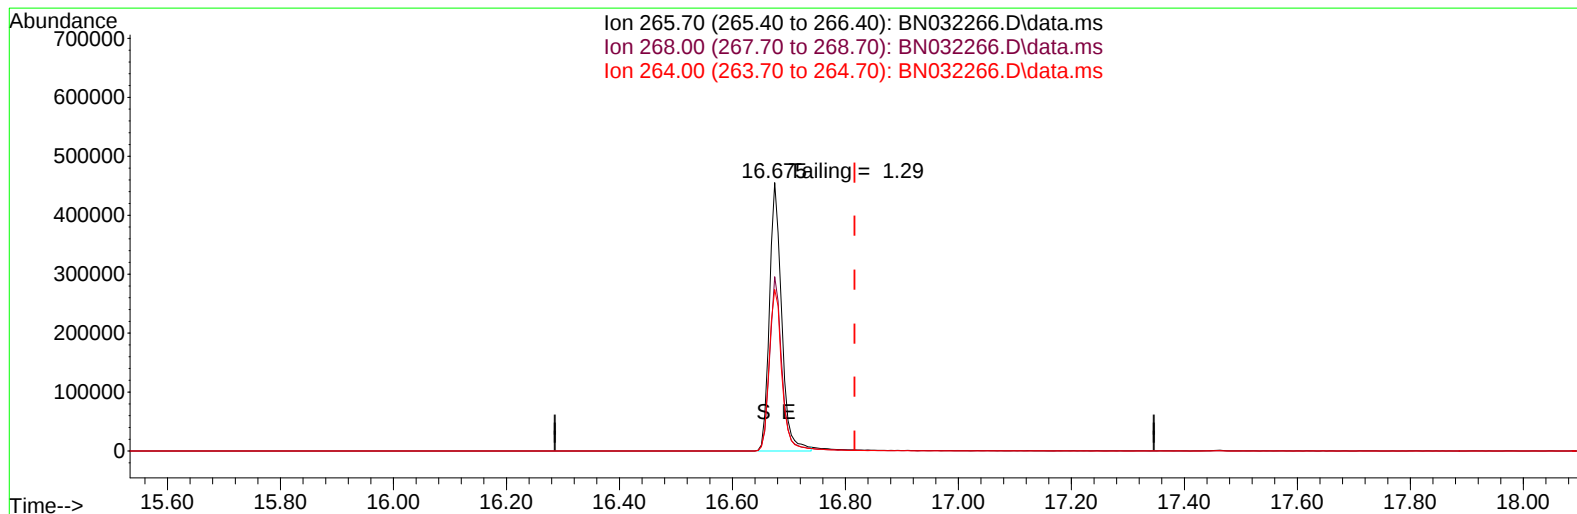

TIC: BN032266.D\data.ms

(70) Pentachlorophenol (C)

16.675min (-0.141) 27688.51 ng




response 705114

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.93
264.00	61.60	60.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062524\
 Data File : BN032266.D
 Acq On : 26 Jun 2024 08:23
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jun 26 09:36:50 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 20 01:44:29 2024
 Response via : Initial Calibration

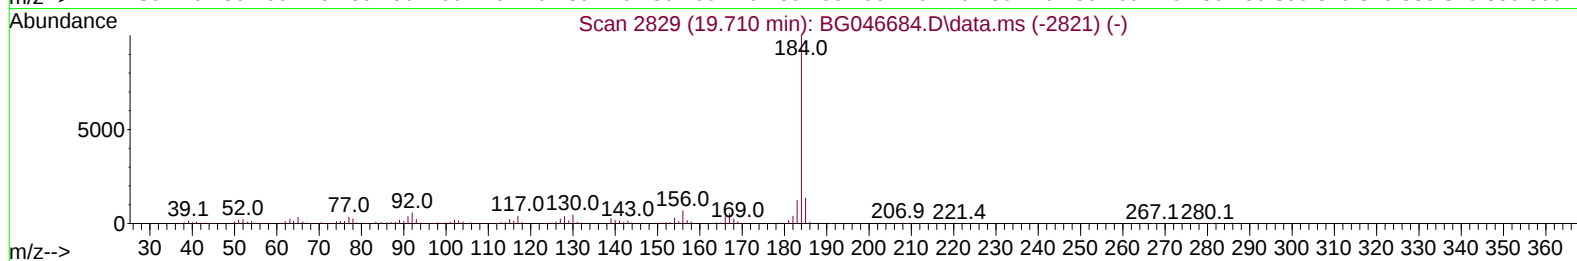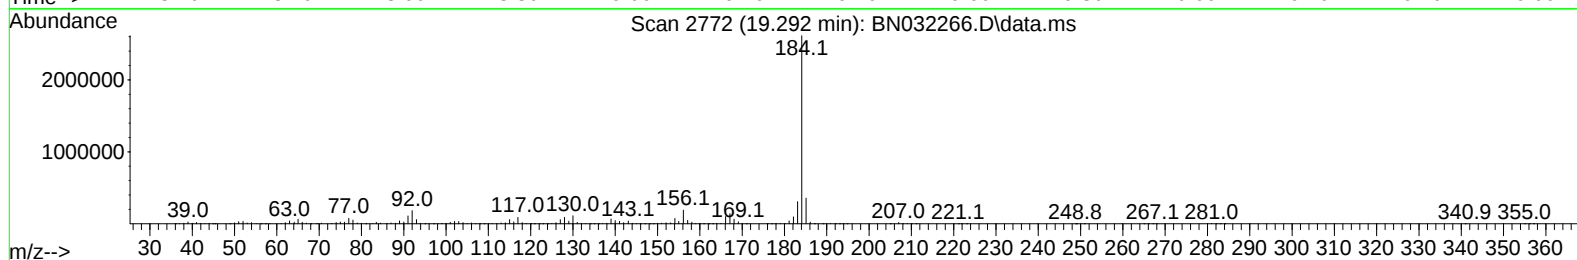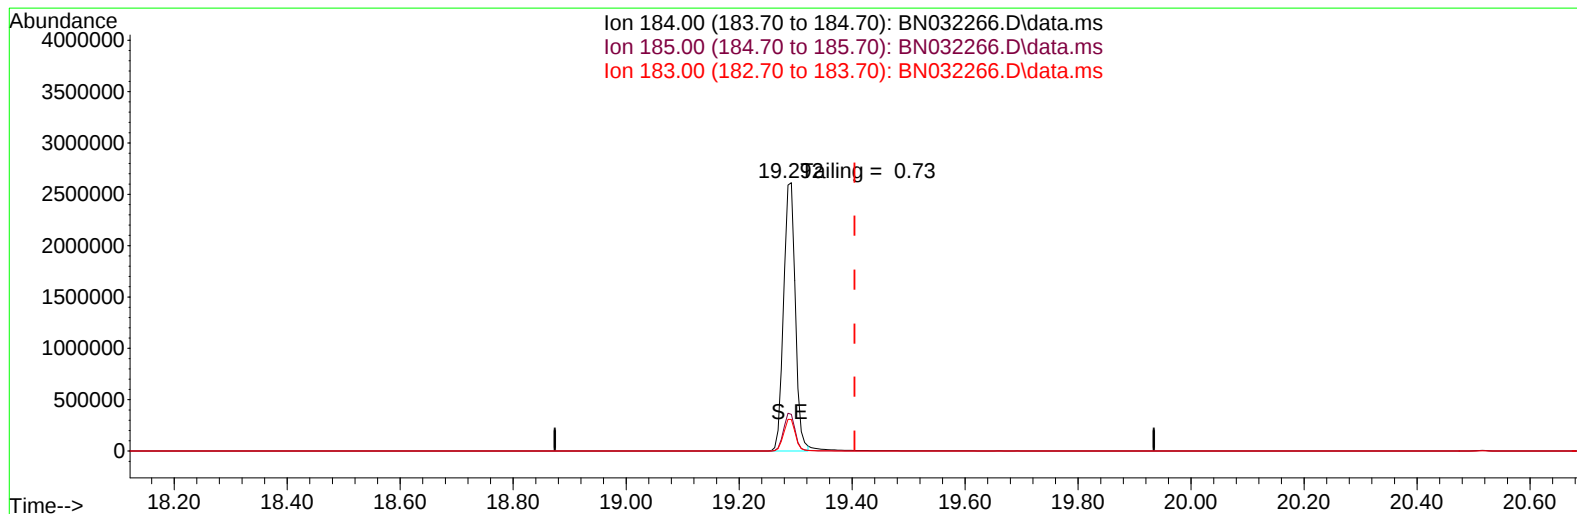

TIC: BN032266.D\data.ms

(77) Benzidine

19.292min (-0.112) 0.00 ng

response 3837896

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.65
183.00	13.20	11.77
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/25/2024	BNA_N	<u>BN032266.D</u>
Compound Name	Response	Retention Time
DDT	1825859	20.516
DDD	64771	20.075
DDE	2040	19.563
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
66811	1892670	3.53

Instrument :
BNA_N
ClientSampleId :
DFTPP