

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062621\
 Data File : BN015089.D
 Acq On : 25 Jun 2021 21:55
 Operator : CG/JU
 Sample : M2680-13
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGD45

Quant Time: Jun 25 23:12:40 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 24 14:43:13 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.728	152	149040	20.000	ng/ul	0.00
20) Naphthalene-d8	10.498	136	608928	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.351	164	358987	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.098	188	716481	20.000	ng/ul	0.00
79) Chrysene-d12	21.292	240	715643	20.000	ng/ul	0.00
88) Perylene-d12	23.545	264	714389	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.287	96	15000	3.916	ng/uL	0.00
4) Pyridine-d5	3.681	84	146053	14.144	ng/ul	0.00
7) Phenol-d5	6.893	99	263731	20.388	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.063	67	158737	20.895	ng/ul	0.00
11) 2-Chlorophenol-d4	7.263	132	213424	21.759	ng/ul	0.00
15) 4-Methylphenol-d8	8.416	113	164881	16.515	ng/ul	0.00
21) Nitrobenzene-d5	8.869	128	100595	24.150	ng/ul	0.00
24) 2-Nitrophenol-d4	9.587	143	95738	25.803	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.116	165	184701	21.090	ng/ul	0.00
31) 4-Chloroaniline-d4	10.628	131	258858	19.073	ng/ul	0.00
46) Dimethylphthalate-d6	13.763	166	568294	23.054	ng/ul	0.00
49) Acenaphthylene-d8	14.039	160	730354	22.823	ng/ul	0.00
54) 4-Nitrophenol-d4	14.539	143	74884	17.416	ng/ul	0.00
60) Fluorene-d10	15.345	176	498141	23.228	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.457	200	37712	12.744	ng/ul	0.00
73) Anthracene-d10	17.198	188	774398	23.614	ng/ul	0.00
81) Pyrene-d10	19.498	212	896764	23.907	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.398	264	919400	26.070	ng/ul	0.00


Target Compounds					Qvalue	
86) Bis(2-ethylhexyl)phtha...	21.221	149	89134	3.309	ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062621\
Data File : BN015089.D
Acq On : 25 Jun 2021 21:55
Operator : CG/JU
Sample : M2680-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGD45

Quant Time: Jun 25 23:12:40 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 24 14:43:13 2021
Response via : Initial Calibration

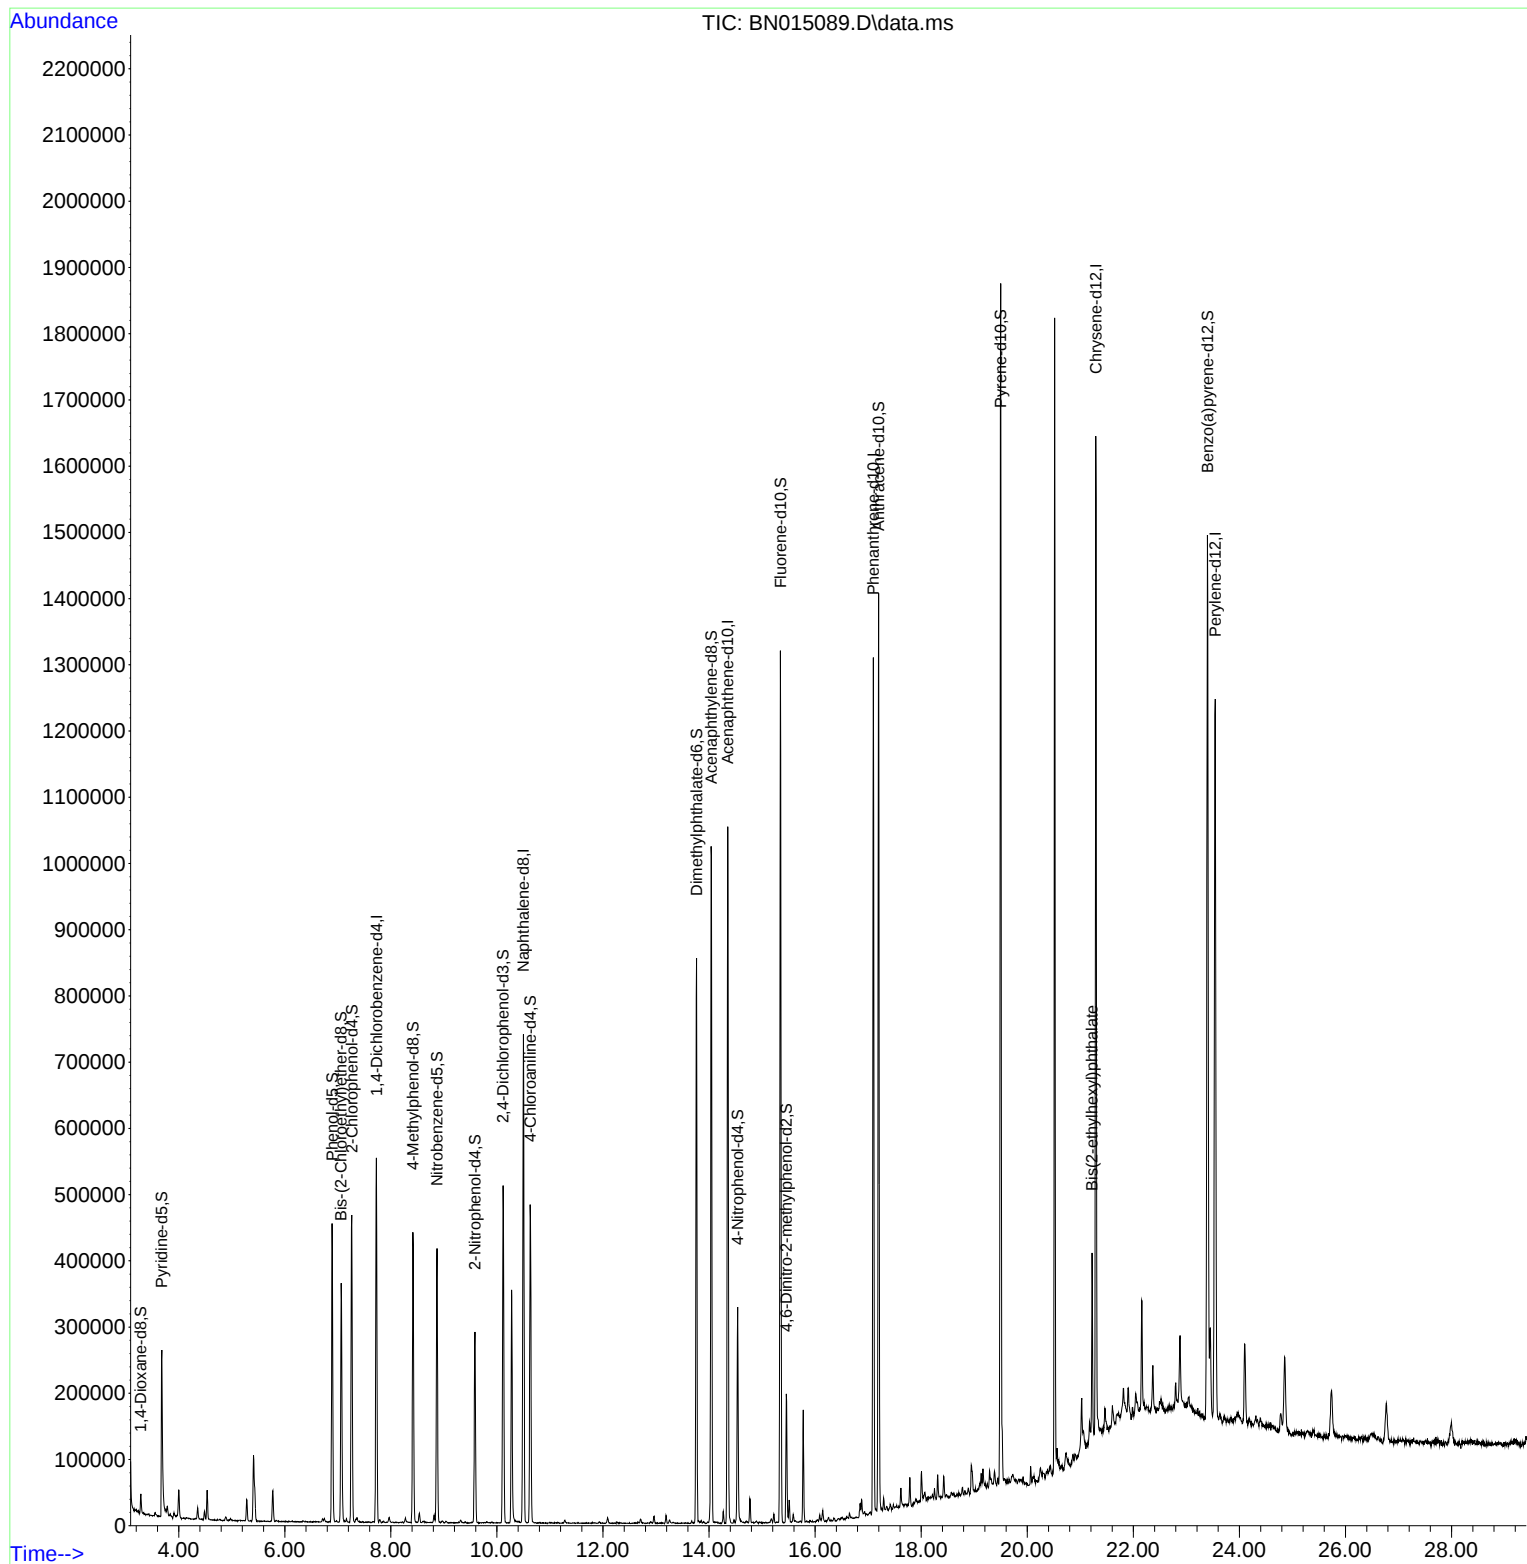

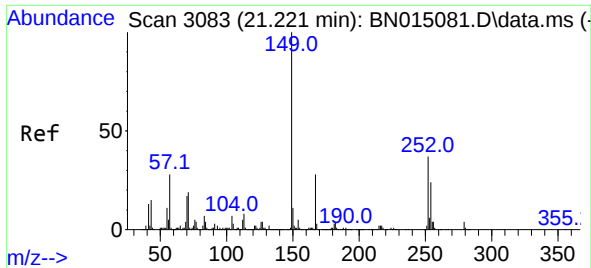

#86
Bis(2-ethylhexyl)phthalate
Concen: 3.309 ng/ul
RT: 21.221 min Scan# 3083
Delta R.T. -0.006 min
Lab File: BN015089.D
Acq: 25 Jun 2021 21:55

Instrument :
BNA_N
ClientSampleId :
BGD45

Tgt Ion:149 Resp: 89134
Ion Ratio Lower Upper
149 100
167 27.8 23.4 35.0
279 3.2 3.4 5.2#

