

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062621\
 Data File : BN015093.D
 Acq On : 26 Jun 2021 00:18
 Operator : CG/JU
 Sample : M2680-11
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGD37

Quant Time: Jun 26 00:52:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 24 14:43:13 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.728	152	165677	20.000	ng/u1	0.00
20) Naphthalene-d8	10.498	136	688417	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.351	164	410756	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.098	188	813438	20.000	ng/u1	0.00
79) Chrysene-d12	21.292	240	774595	20.000	ng/u1	0.00
88) Perylene-d12	23.539	264	791785	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.287	96	13715	3.221	ng/uL	0.00
4) Pyridine-d5	3.675	84	138924	12.102	ng/u1	0.00
7) Phenol-d5	6.893	99	258977	18.010	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.063	67	147603	17.478	ng/u1	0.00
11) 2-Chlorophenol-d4	7.263	132	197583	18.121	ng/u1	0.00
15) 4-Methylphenol-d8	8.416	113	190021	17.122	ng/u1	0.00
21) Nitrobenzene-d5	8.869	128	96513	20.495	ng/u1	0.00
24) 2-Nitrophenol-d4	9.586	143	88951	21.205	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.116	165	186035	18.790	ng/u1	0.00
31) 4-Chloroaniline-d4	10.628	131	268939	17.527	ng/u1	0.00
46) Dimethylphthalate-d6	13.763	166	604951	21.448	ng/u1	0.00
49) Acenaphthylene-d8	14.039	160	733371	20.029	ng/u1	0.00
54) 4-Nitrophenol-d4	14.539	143	84478	17.171	ng/u1	0.00
60) Fluorene-d10	15.345	176	524659	21.381	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.457	200	34907	10.390	ng/u1	0.00
73) Anthracene-d10	17.198	188	862821	23.175	ng/u1	0.00
81) Pyrene-d10	19.498	212	1057954	26.058	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.398	264	1107430	28.332	ng/u1	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.221	149	76391	2.620	ng/u1	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062621\
Data File : BN015093.D
Acq On : 26 Jun 2021 00:18
Operator : CG/JU
Sample : M2680-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGD37


Quant Time: Jun 26 00:52:46 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 24 14:43:13 2021
Response via : Initial Calibration

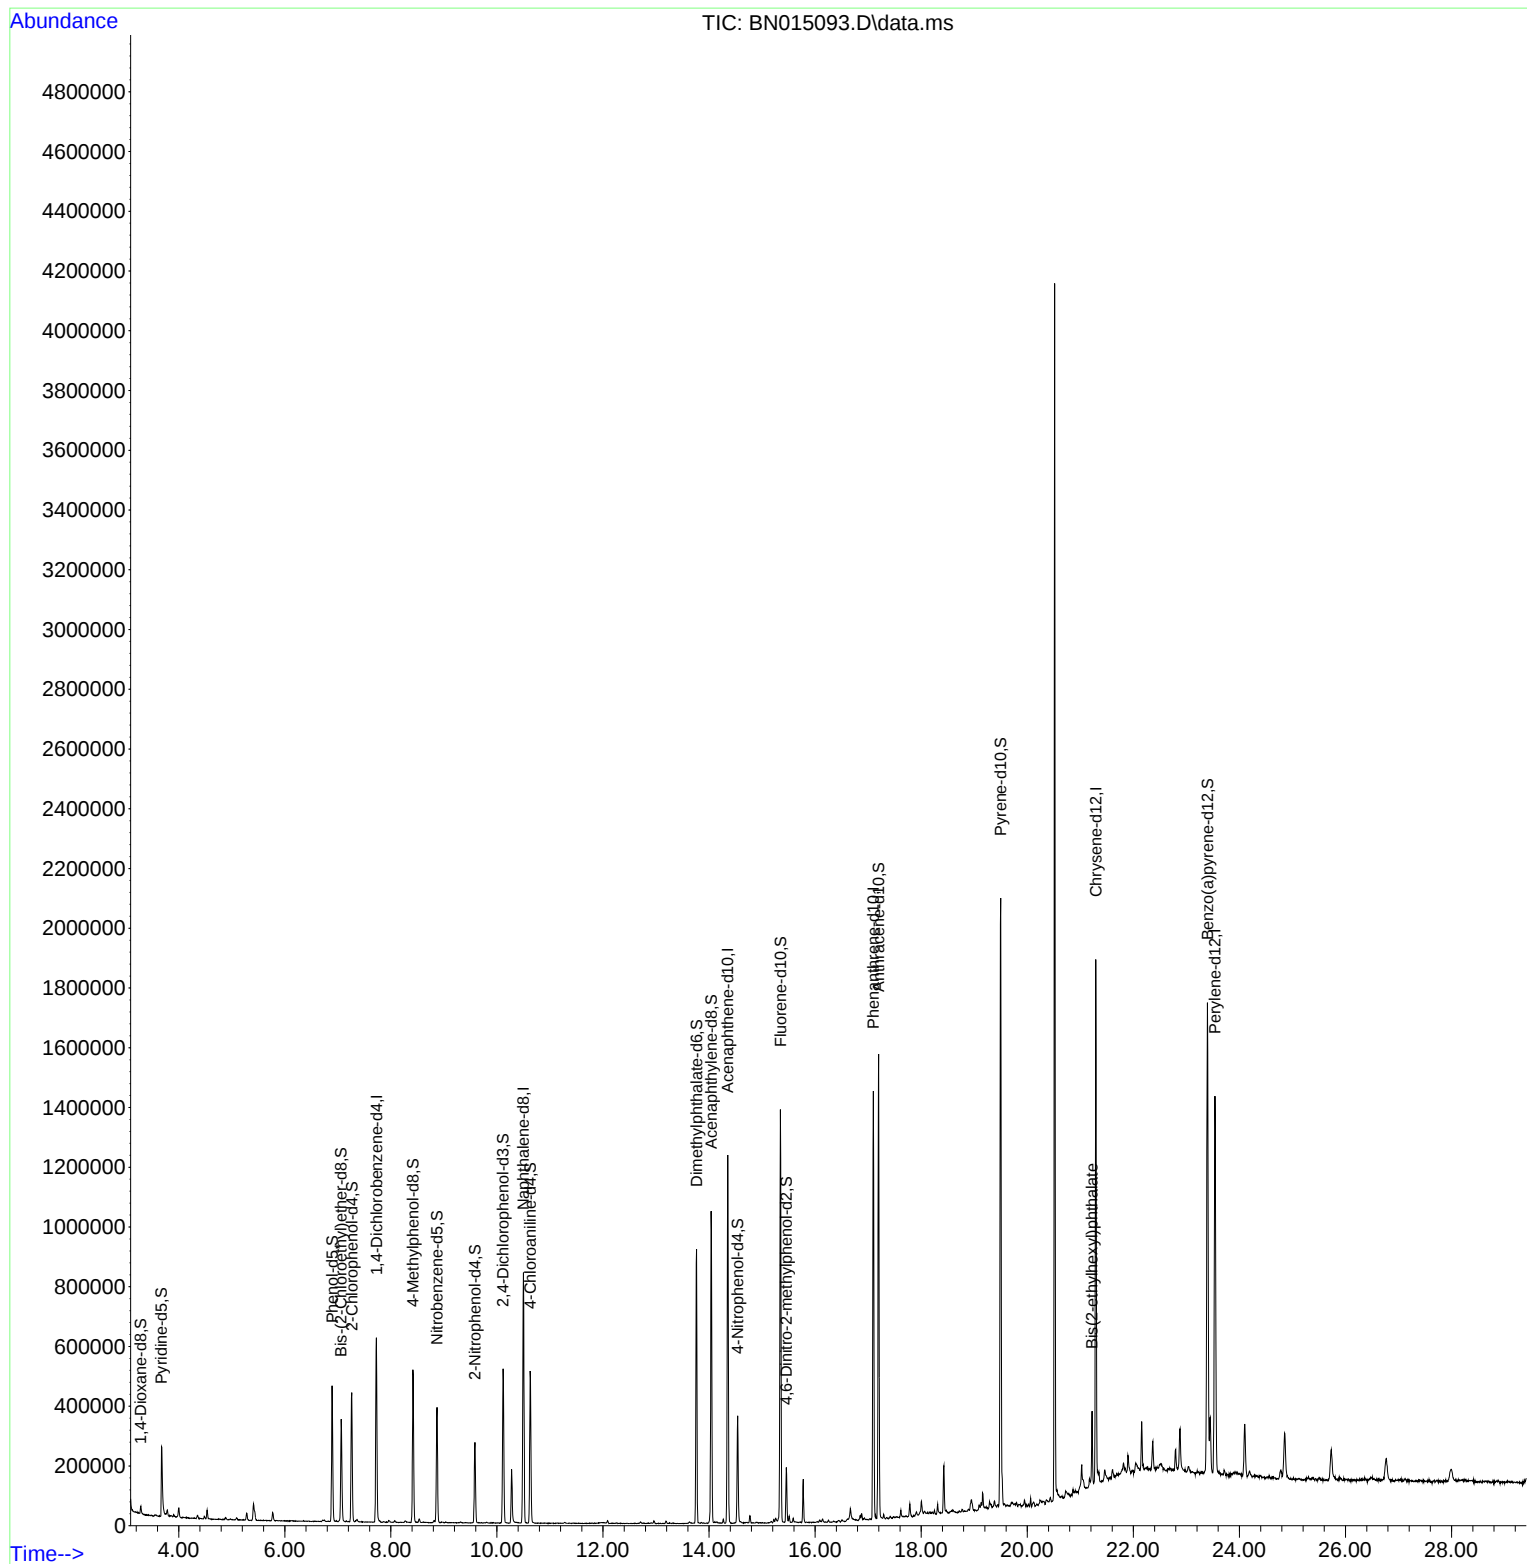

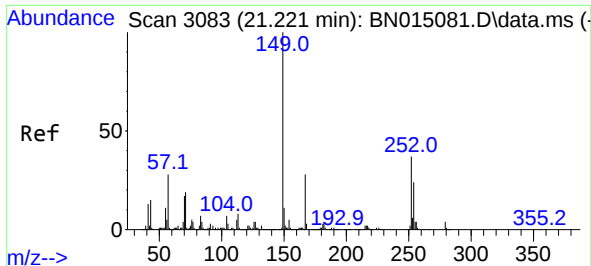

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 2.620 ng/ul
 RT: 21.221 min Scan# 3083
 Delta R.T. -0.006 min
 Lab File: BN015093.D
 Acq: 26 Jun 2021 00:18

Instrument :
 BNA_N
 ClientSampleId :
 BGD37

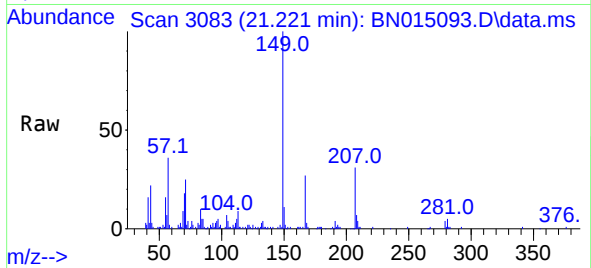

Tgt Ion:149 Resp: 76391

Ion	Ratio	Lower	Upper
149	100		
167	26.5	23.4	35.0
279	3.6	3.4	5.2

